


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100418\
Data File : VN051656.D
Acq On : 4 Oct 2018 9:42
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Title : SW846 8260
Last Update : Fri Oct 05 02:22:33 2018

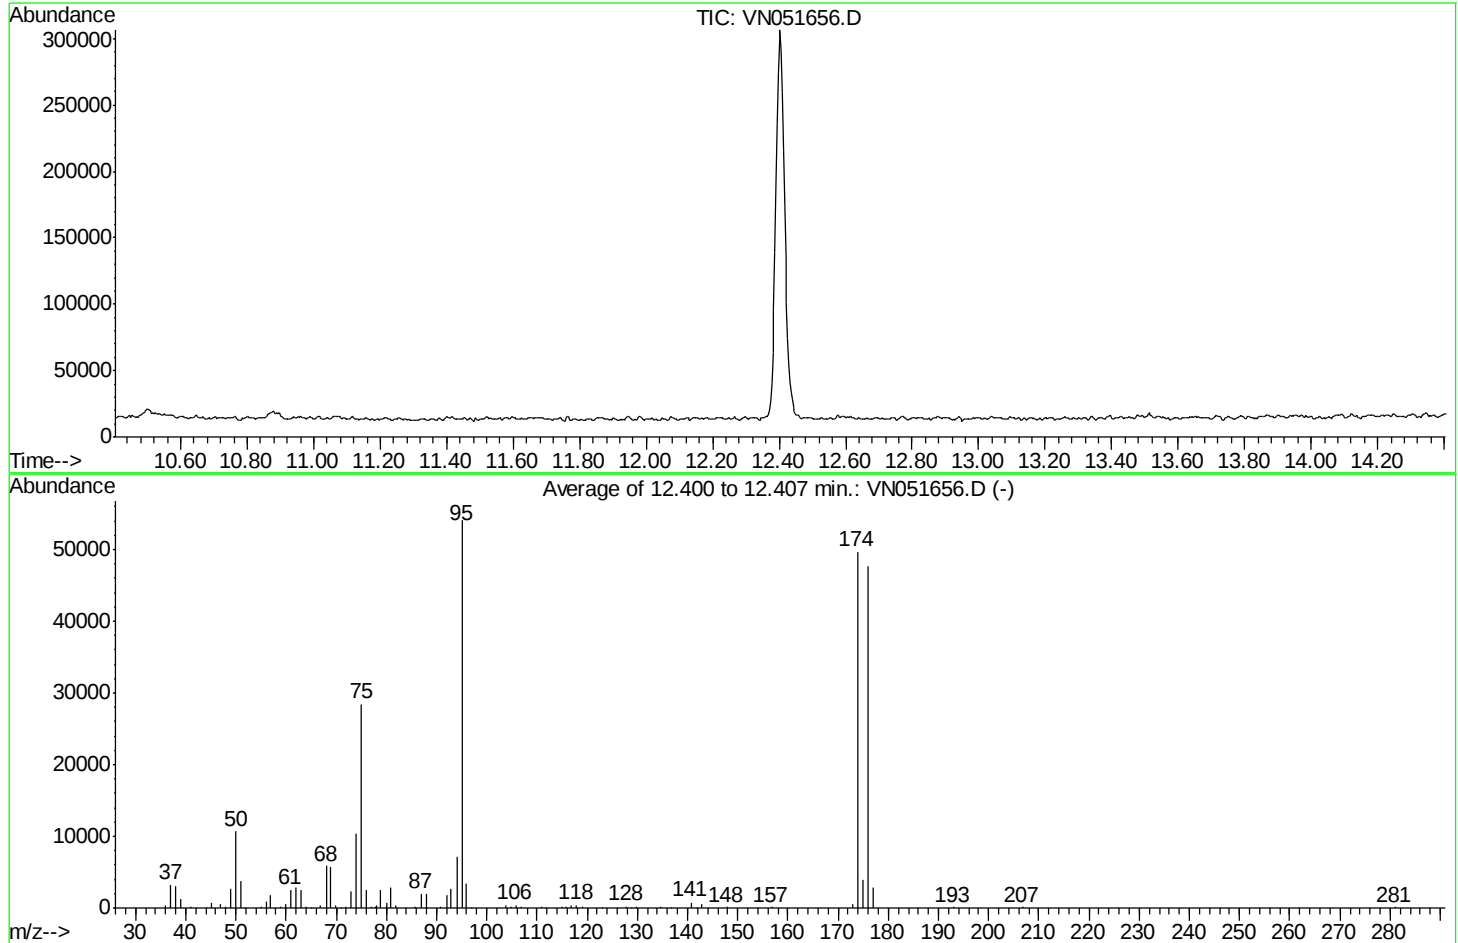

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	10641	PASS
75	95	30	60	52.6	28432	PASS
95	95	100	100	100.0	54077	PASS
96	95	5	9	6.3	3425	PASS
173	174	0.00	2	1.1	545	PASS
174	95	50	100	91.8	49656	PASS
175	174	5	9	8.0	3948	PASS
176	174	95	101	96.1	47744	PASS
177	176	5	9	5.9	2824	PASS