


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100419\  
Data File : VN058526.D  
Acq On : 4 Oct 2019 9:35  
Operator : JC/SP  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N092719W.M  
Title : SW846 8260  
Last Update : Mon Sep 30 08:07:38 2019

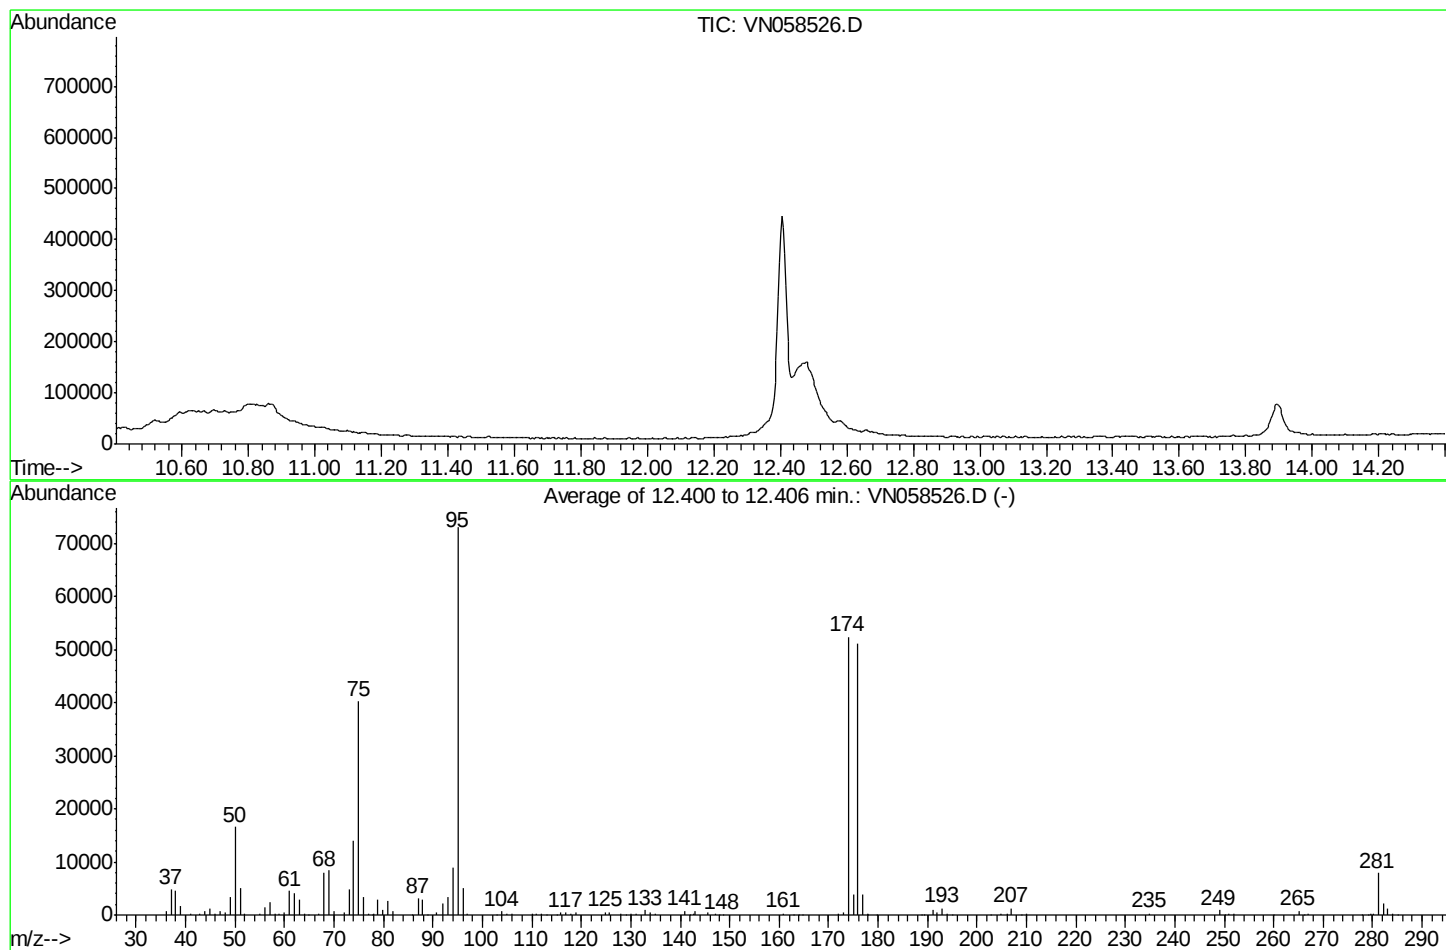

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3293

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 22.7      | 16622   | PASS             |
| 75          | 95           | 30           | 60           | 55.1      | 40259   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 73066   | PASS             |
| 96          | 95           | 5            | 9            | 7.0       | 5118    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.1       | 555     | PASS             |
| 174         | 95           | 50           | 100          | 71.8      | 52426   | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 3951    | PASS             |
| 176         | 174          | 95           | 101          | 97.8      | 51269   | PASS             |
| 177         | 176          | 5            | 9            | 7.4       | 3773    | PASS             |