
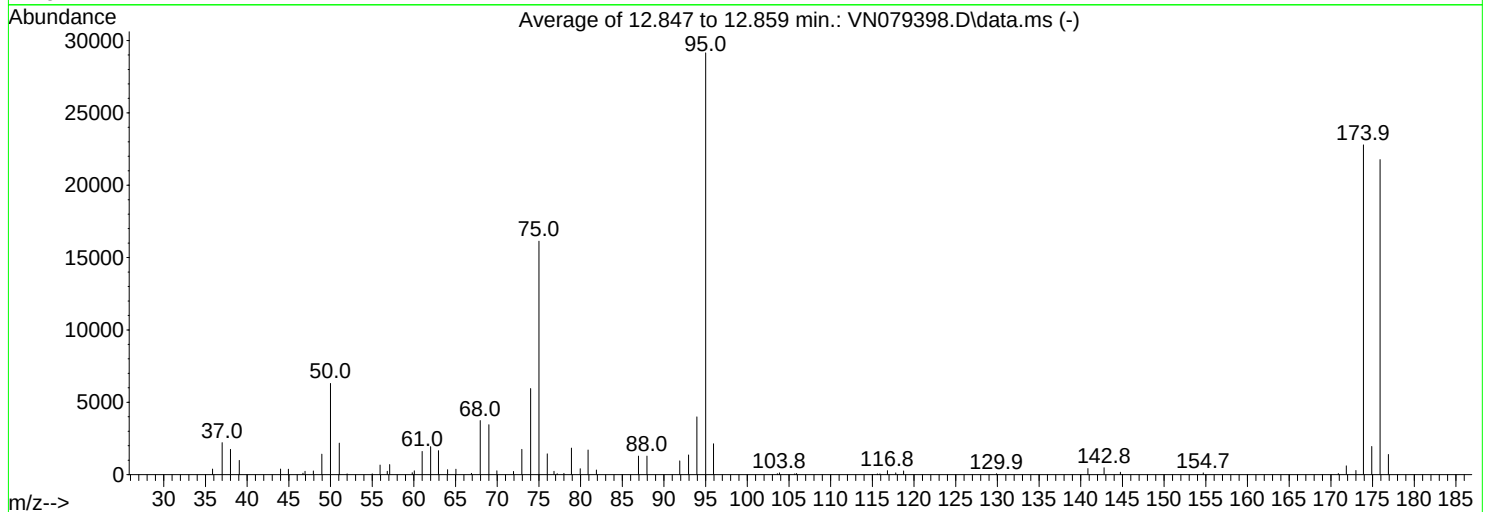


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100423\
Data File : VN079398.D
Acq On : 04 Oct 2023 12:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 05:05:24 2023

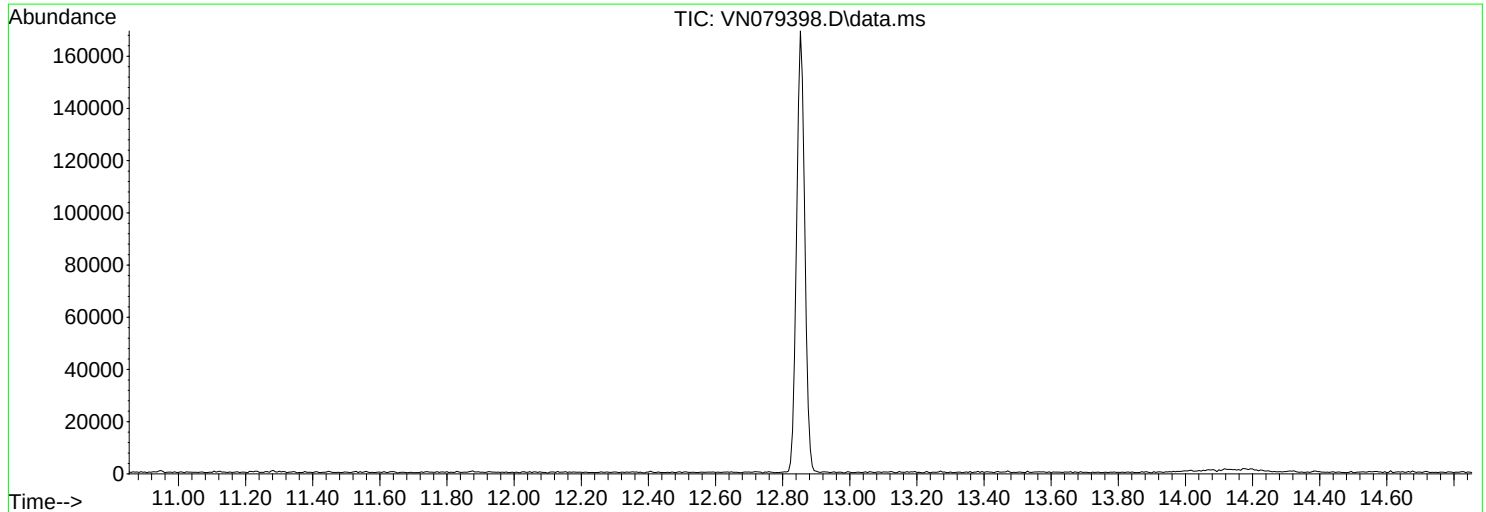

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	6307	PASS
75	95	30	60	55.4	16135	PASS
95	95	100	100	100.0	29147	PASS
96	95	5	9	7.3	2131	PASS
173	174	0.00	2	1.3	287	PASS
174	95	50	100	78.2	22792	PASS
175	174	5	9	8.5	1946	PASS
176	174	95	101	95.5	21773	PASS
177	176	5	9	6.4	1397	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	384	51.05	2182	64.05	347	76.80	231
37.00	2217	52.00	56	65.05	373	77.20	71
38.00	1744	55.00	54	66.90	91	78.00	8
39.05	989	55.95	664	67.95	3742	78.90	184
44.00	383	56.80	229	69.00	3453	79.95	414
44.95	374	57.10	692	69.95	269	80.90	1705
46.70	101	59.80	137	71.95	217	81.90	324
46.95	235	60.05	271	72.95	1747	86.95	1279
47.95	252	61.00	1608	74.00	5954	87.95	1288
48.95	1421	62.00	1939	75.00	16135	91.90	950
50.00	6307	62.95	1654	76.00	1437	92.95	1355

Average of 12.847 to 12.859 min.: VN079398.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.95	3995	118.75	256	175.90	21773		
95.00	29147	129.90	69	176.90	1397		
95.95	2131	140.85	417				
103.60	71	142.80	478				
103.85	123	144.75	164				
105.70	52	154.70	119				
105.90	82	170.90	73				
115.60	58	171.85	607				
115.90	57	173.00	287				
116.80	274	173.90	22792				
117.80	124	174.90	1946				