
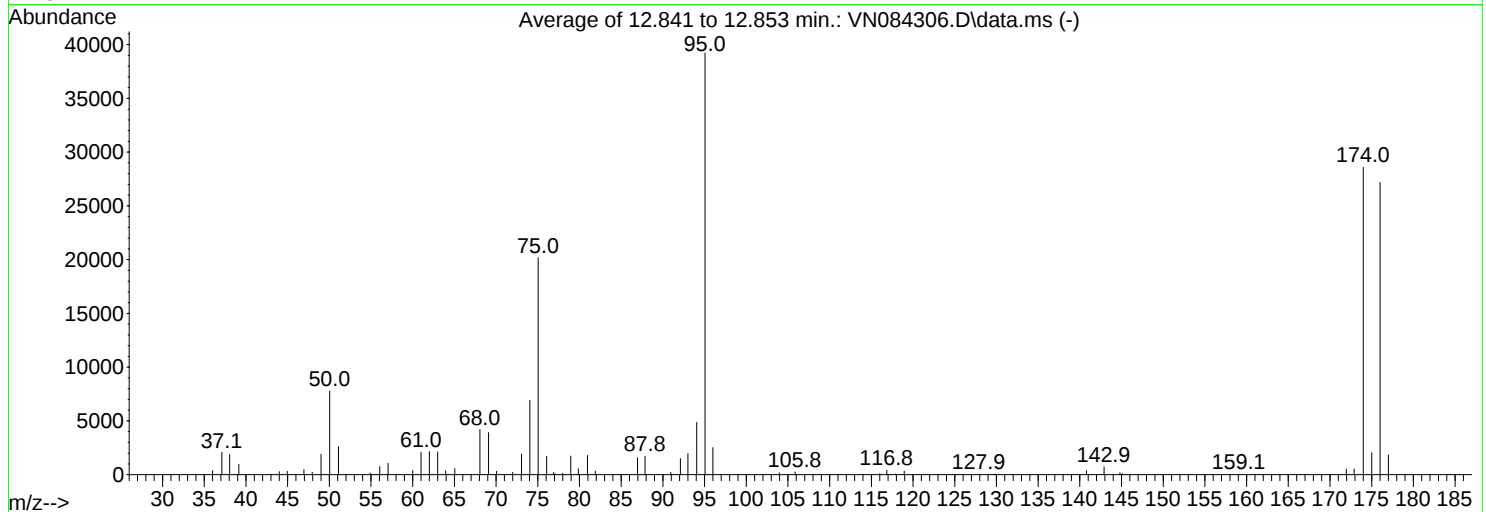


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100424\
Data File : VN084306.D
Acq On : 04 Oct 2024 07:54
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Sep 06 23:42:47 2024

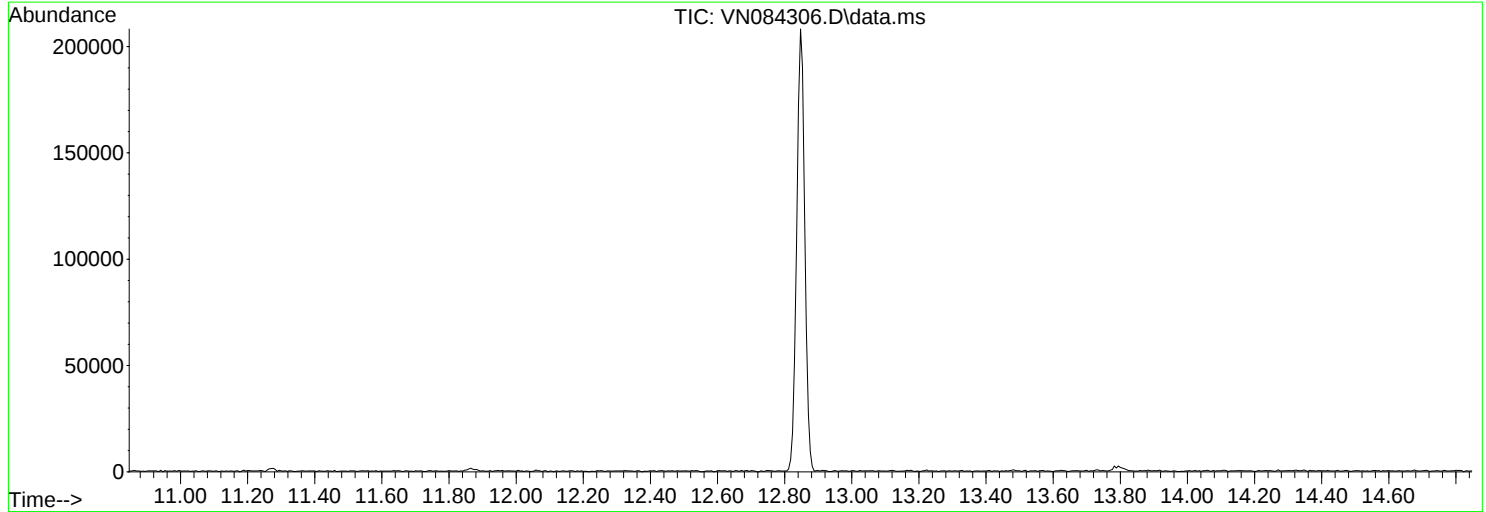

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	7779	PASS
75	95	30	60	51.4	20165	PASS
95	95	100	100	100.0	39235	PASS
96	95	5	9	6.4	2516	PASS
173	174	0.00	2	1.9	540	PASS
174	95	50	100	72.9	28597	PASS
175	174	5	9	7.1	2039	PASS
176	174	95	101	95.0	27181	PASS
177	176	5	9	6.8	1836	PASS