

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100518\
 Data File : VN051688.D
 Acq On : 5 Oct 2018 15:41
 Operator : MD\SY
 Sample : J5239-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 17 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 002M-35TH-AVE(AUG)

Quant Time: Oct 05 16:39:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N100518W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Oct 05 11:11:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.20	128	82519	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.59	114	460915	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.41	117	375059	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	8.03	65	169255	29.55	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	98.50%
60) 4-Bromofluorobenzene	12.40	95	134622	23.52	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	78.40%
63) Toluene-d8	10.09	98	535017	32.13	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	107.10%

Target Compounds


					Ovalue
15) Acetone	3.82	58	194677	656.356 ug/l	82
25) Chloroform	7.37	83	150502	16.902 ug/l	98
41) Bromodichloromethane	9.41	83	14785	2.110 ug/l #	91
62) Toluene	10.16	91	1219939	64.211 ug/l	100
82) p-Isopropyltoluene	13.29	119	49205	2.415 ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN100518\
Data File : VN051688.D
Acq On : 5 Oct 2018 15:41
Operator : MD\SY
Sample : J5239-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 17 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
002M-35TH-AVE(AUG)

Quant Time: Oct 05 16:39:09 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA N\METHODS\624N100518W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Oct 05 11:11:26 2018
Response via : Initial Calibration

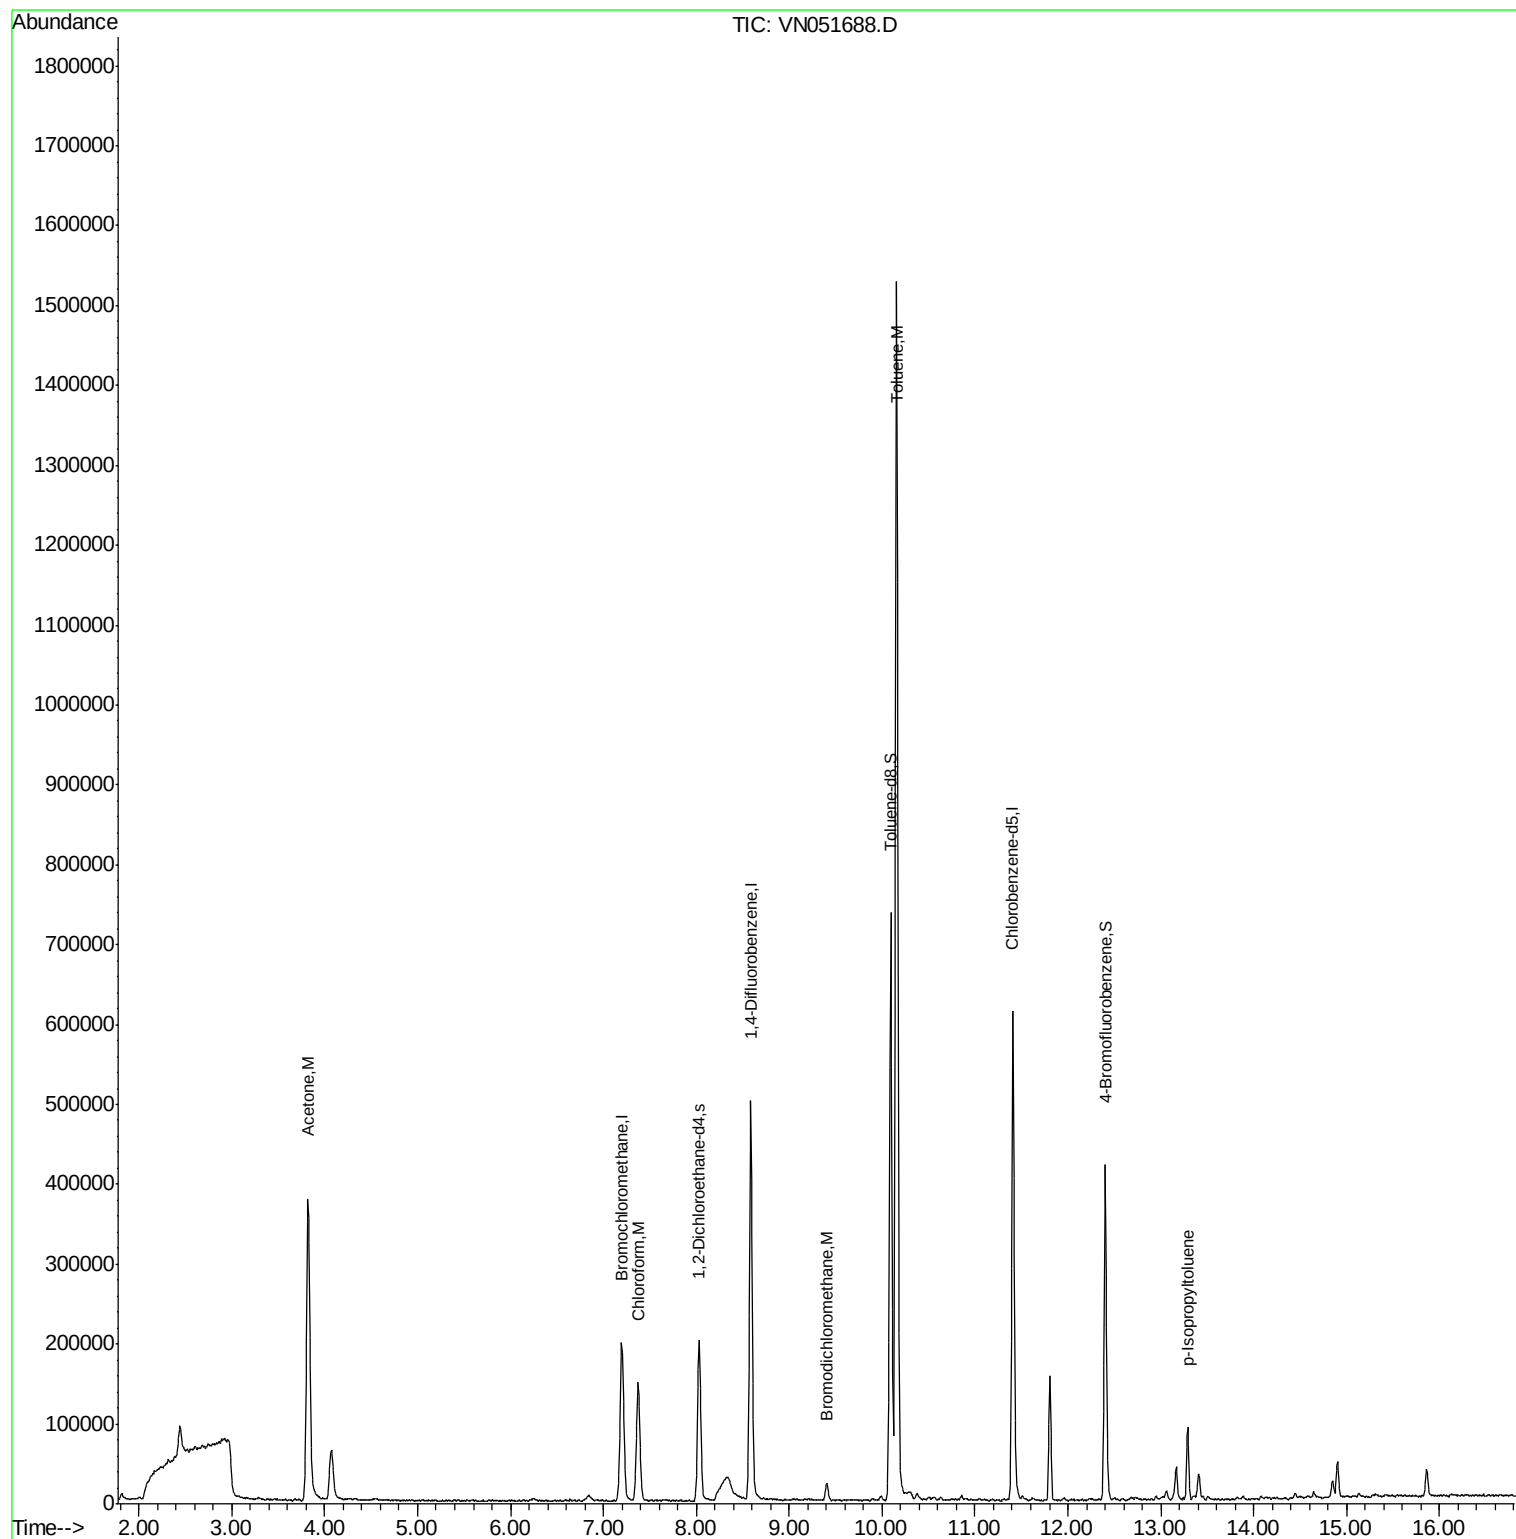


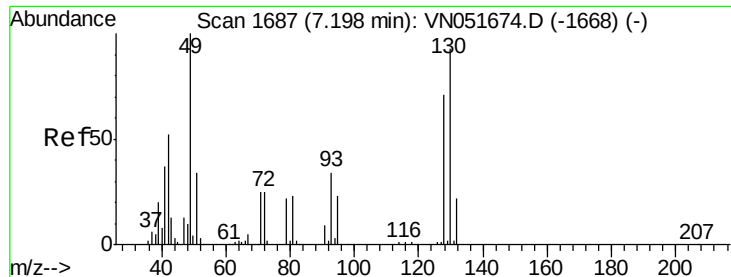




#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.20 min Scan# 1689
Delta R.T. 0.01 min
Lab File: VN051688.D
Acq: 5 Oct 2018 15:41

Instrument :
MSVOA_N
ClientSampleId :
002M-35TH-AVE(AUG)

Tot Ion:128 Resp: 82519
Ion Ratio Lower Upper
128 100
49 138.2 0.0 403.3
130 128.5 0.0 326.0

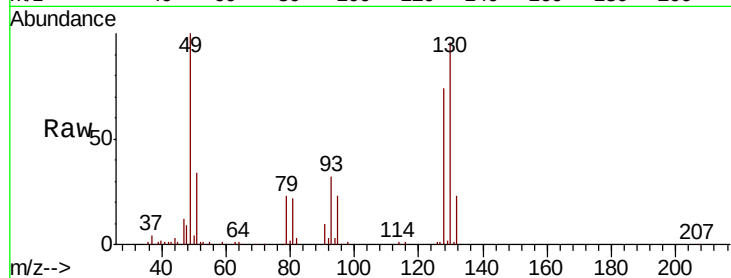


Abundance Ion 128.00 (127.70 to 128.70): V
Ion 49.00 (48.70 to 49.70): VN
Ion 130.00 (129.70 to 130.70): V

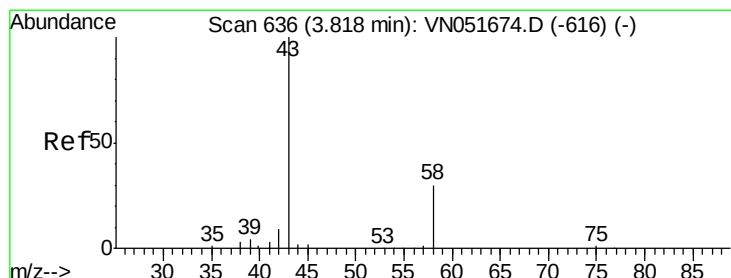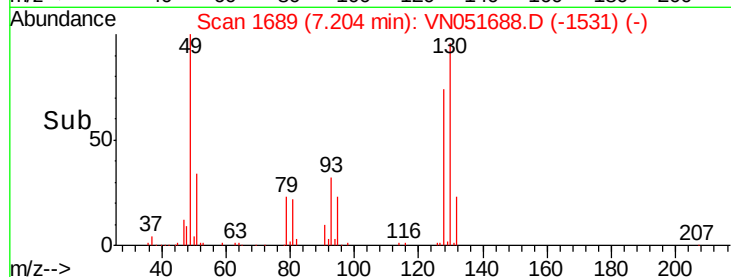
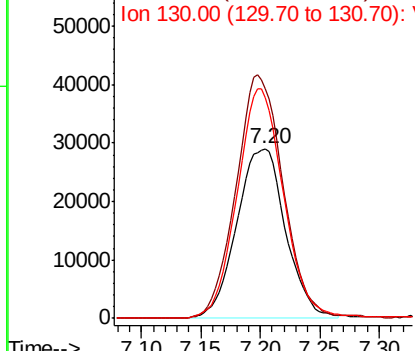



#15
Acetone
Concen: 656.356 ug/l
RT: 3.82 min Scan# 637
Delta R.T. 0.00 min
Lab File: VN051688.D
Acq: 5 Oct 2018 15:41

Tgt Ion: 58 Resp: 194677
Ion Ratio Lower Upper
58 100
43 325.0 232.2 348.2

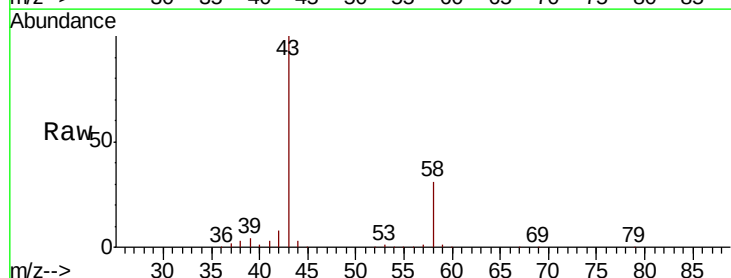

Abundance Ion 58.00 (57.70 to 58.70): VN
Ion 43.00 (42.70 to 43.70): VN



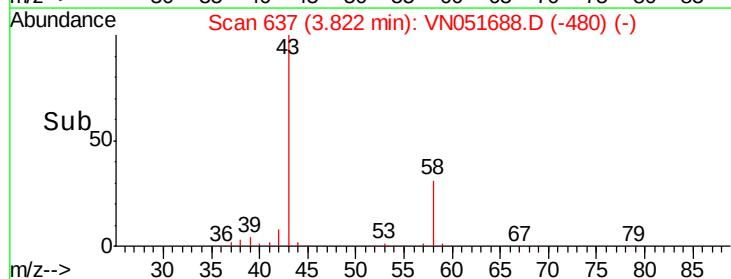
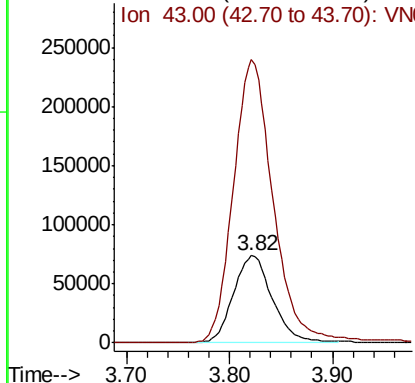


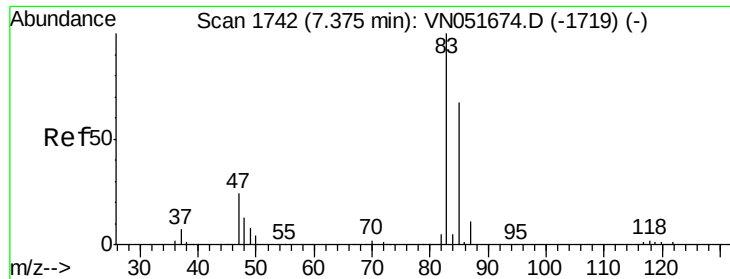

#25
Chloroform
Concen: 16.902 ug/l
RT: 7.37 min Scan# 1742
Delta R.T. -0.00 min
Lab File: VN051688.D
Acq: 5 Oct 2018 15:41




Instrument :
MSVOA_N
ClientSampleId :
002M-35TH-AVE(AUG)


Tot Ion: 83 Resp: 150502
Ion Ratio Lower Upper
83 100
85 66.3 54.6 82.0

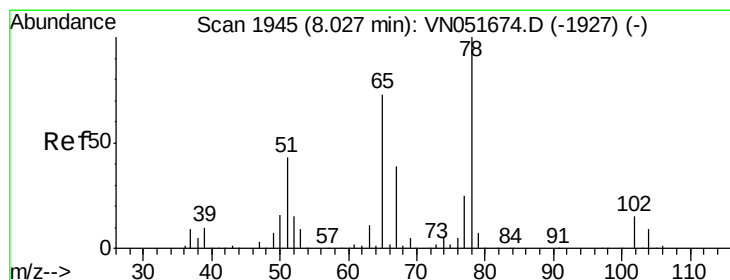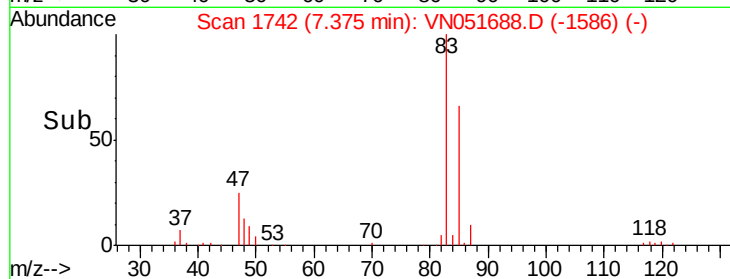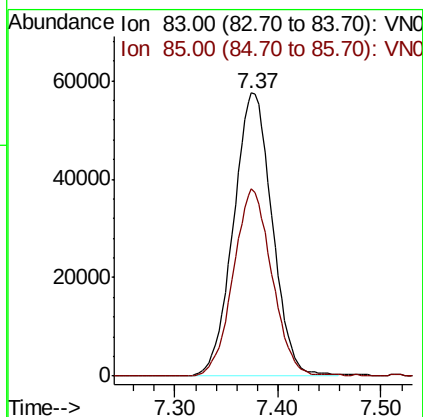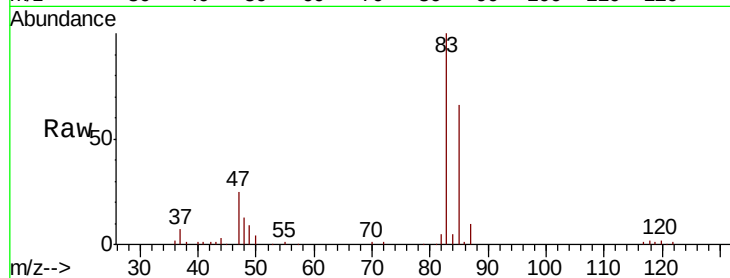

#27
1,2-Dichloroethane-d4
Concen: Below ug/l
RT: 8.03 min Scan# 1946
Delta R.T. 0.00 min
Lab File: VN051688.D
Acq: 5 Oct 2018 15:41

Tgt Ion: 65 Resp: 169255
Ion Ratio Lower Upper
65 100
67 51.3 41.8 62.8


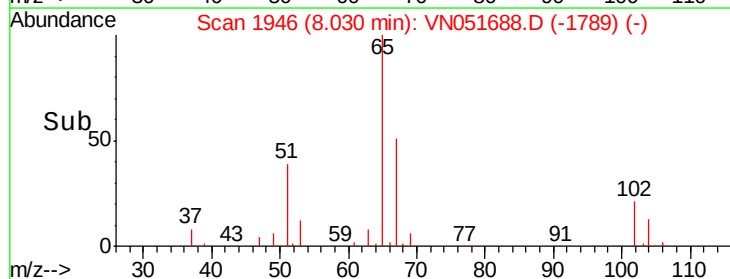
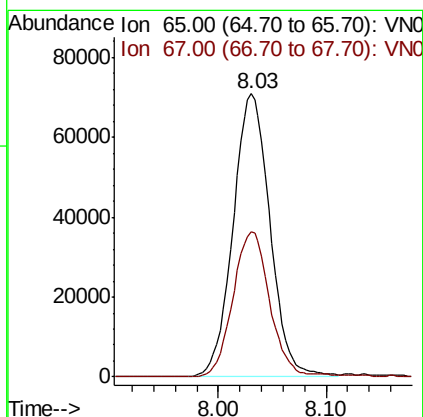
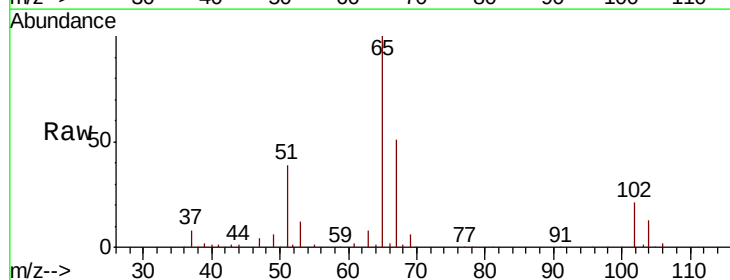


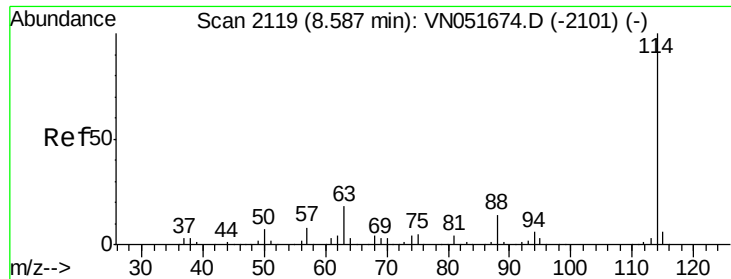

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN051688.D
 Acq: 5 Oct 2018 15:41




Instrument :
 MSVOA_N
 ClientSampleId :
 002M-35TH-AVE(AUG)


Tot Ion	Ratio	Lower	Upper
114	100		
63	18.0	16.2	24.2
88	14.5	12.2	18.4

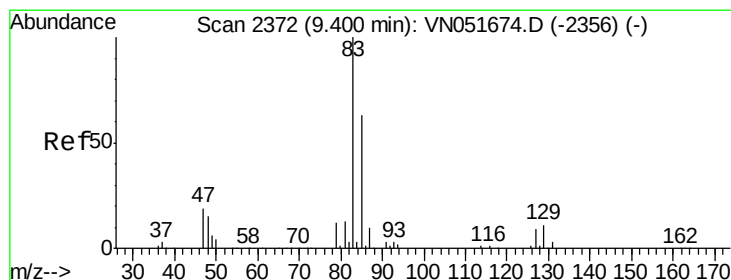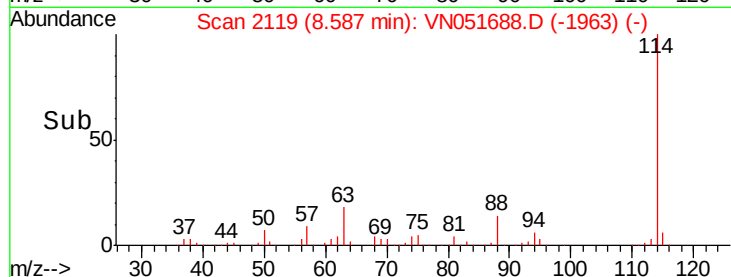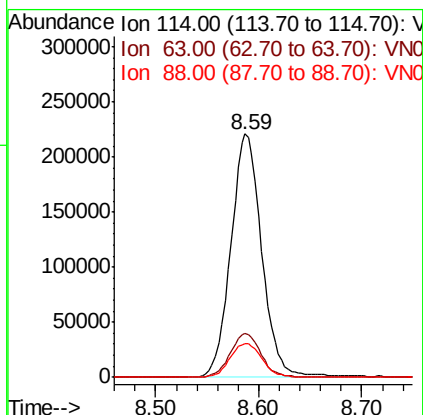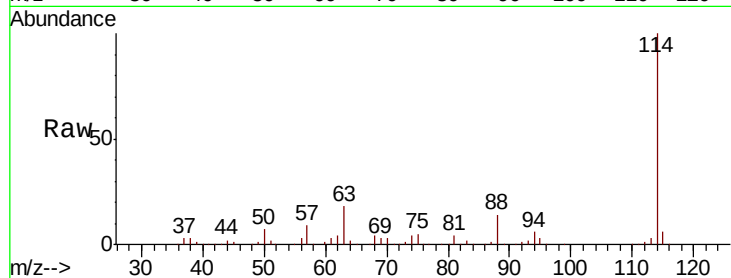

#41
 Bromodichloromethane
 Concen: 2.110 ug/l
 RT: 9.41 min Scan# 2374
 Delta R.T. 0.01 min
 Lab File: VN051688.D
 Acq: 5 Oct 2018 15:41

Tgt Ion	Ratio	Lower	Upper
83	100		
85	61.8	55.7	83.5
127	7.5	8.2	12.4#


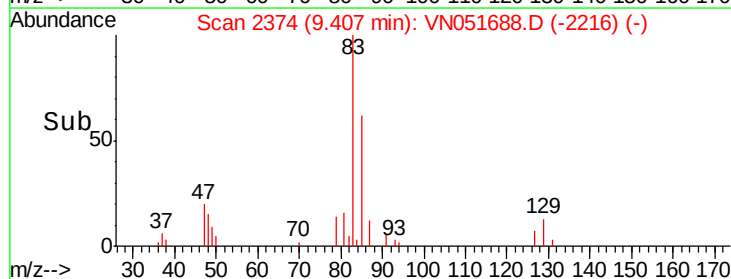
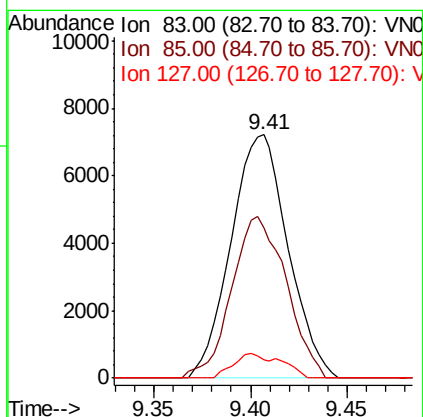
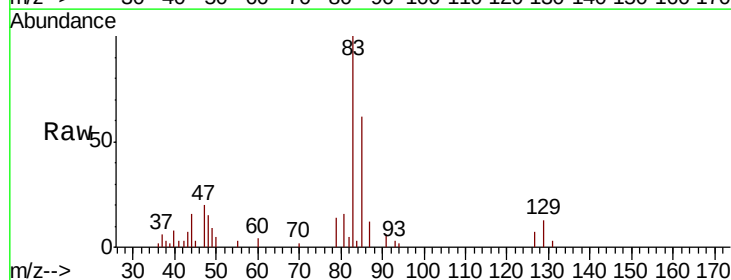


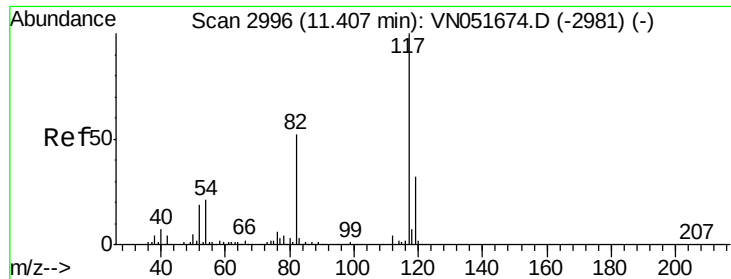

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN051688.D
Acq: 5 Oct 2018 15:41




Instrument :
MSVOA_N
ClientSampleId :
002M-35TH-AVE(AUG)


Tot Ion:117 Resp: 375059
Ion Ratio Lower Upper
117 100
82 52.9 44.1 66.1
119 32.1 25.8 38.8

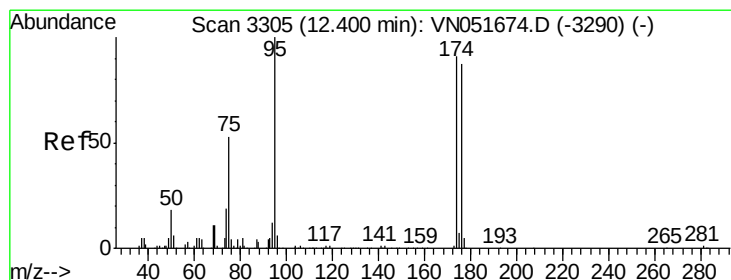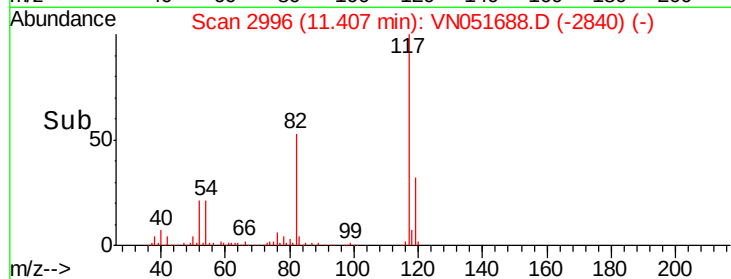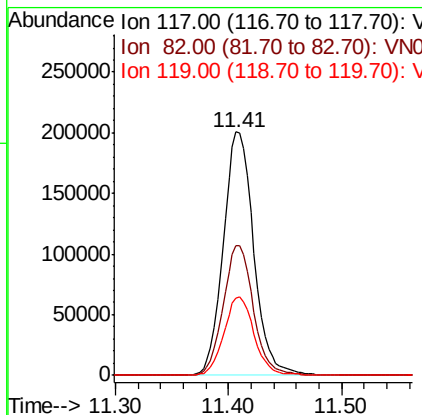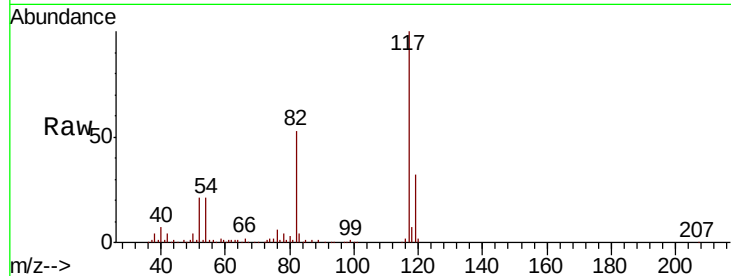

#60
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 12.40 min Scan# 3306
Delta R.T. 0.00 min
Lab File: VN051688.D
Acq: 5 Oct 2018 15:41

Tgt Ion: 95 Resp: 134622
Ion Ratio Lower Upper
95 100
174 95.8 73.5 110.3
176 92.8 70.2 105.2

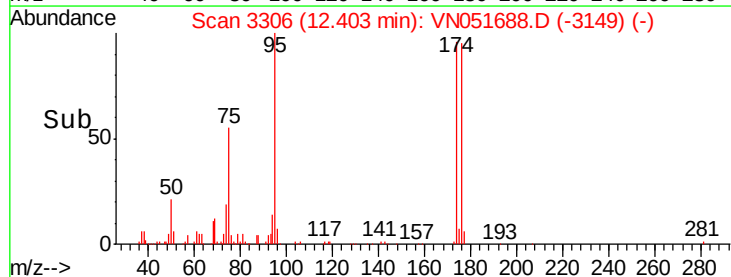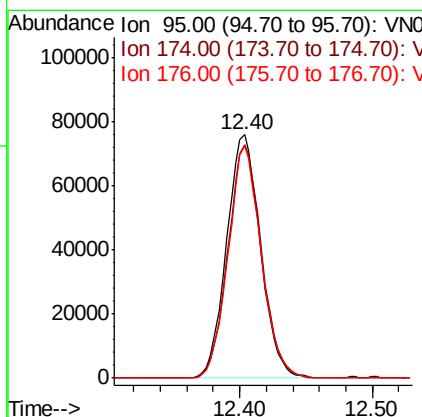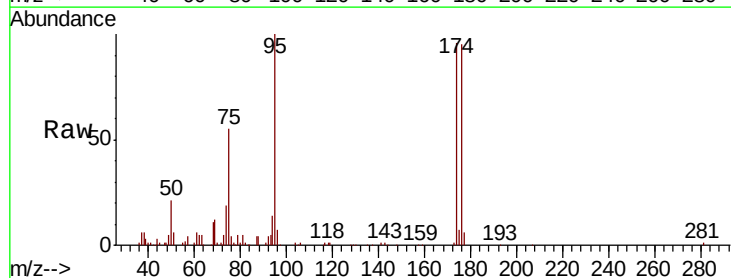

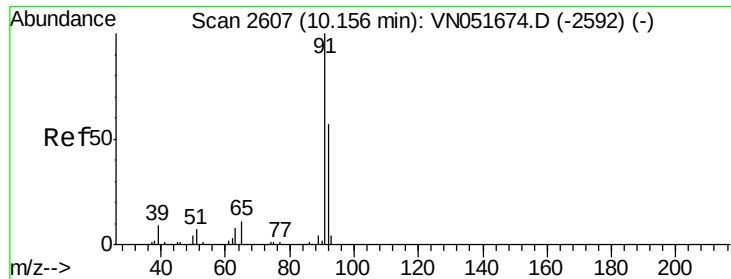

#62

Toluene

Concen: 64.211 ug/l

RT: 10.16 min Scan# 2607

Delta R.T. -0.00 min

Lab File: VN051688.D

Acq: 5 Oct 2018 15:41

Instrument :

MSVOA_N

ClientSampleId :





002M-35TH-AVE(AUG)

Tot Ion: 91 Resp: 1219939

Ion Ratio Lower Upper

91 100

92 55.8 44.6 66.8

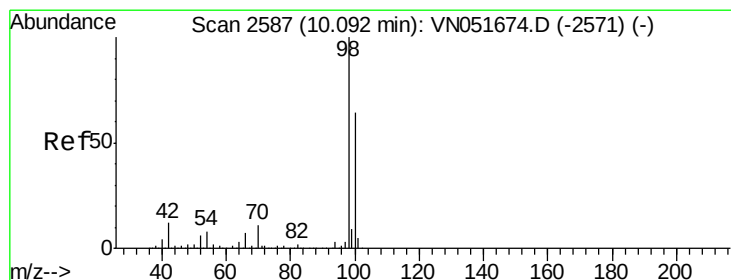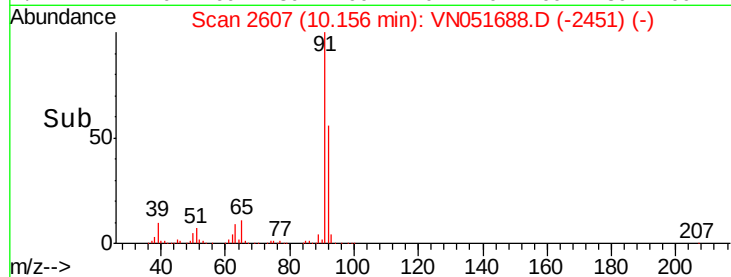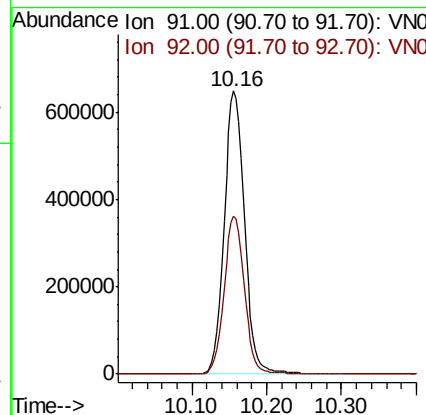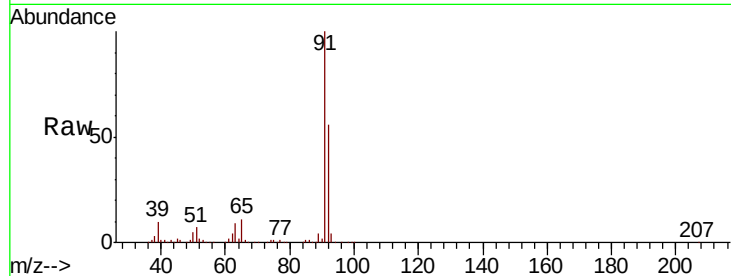

#63

Toluene-d8

Concen: 64.211 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN051688.D




Acq: 5 Oct 2018 15:41


Tgt Ion: 98 Resp: 535017

Ion Ratio Lower Upper

98 100

100 62.9 50.8 76.2

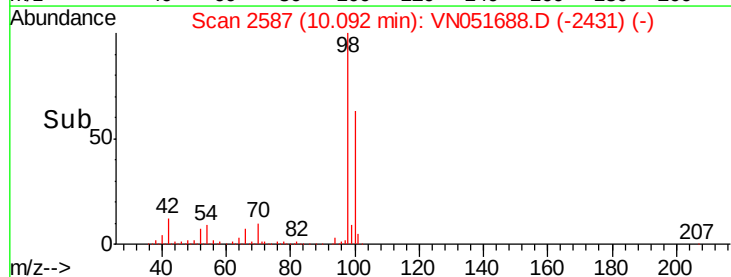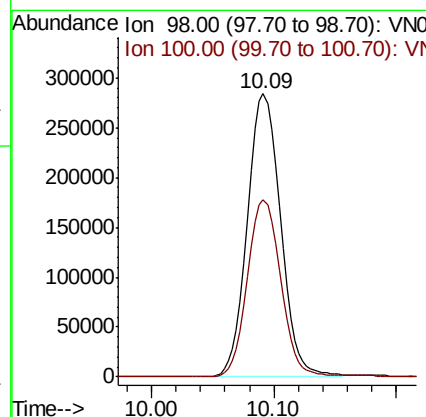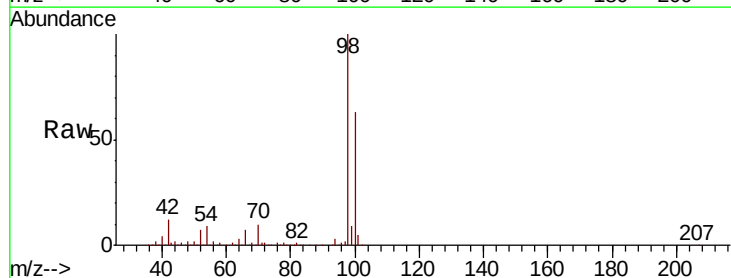

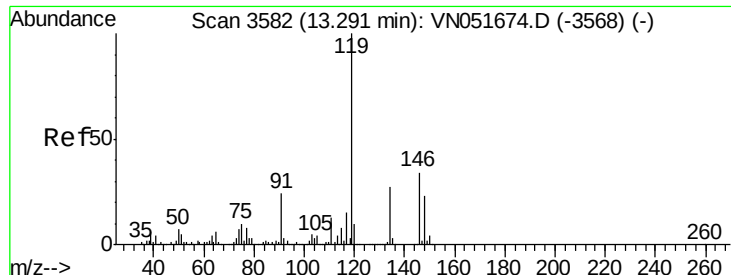

#82
 p-Isopropyltoluene
 Concen: 2.415 ug/l
 RT: 13.29 min Scan# 3582
 Delta R.T. -0.00 min
 Lab File: VN051688.D
 Acq: 5 Oct 2018 15:41

Instrument :
 MSVOA_N
 ClientSampleId :
 002M-35TH-AVE(AUG)

Tot Ion	Ratio	Lower	Upper
119	100		
134	27.7	0.0	53.6
91	24.8	0.0	52.0

