


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100518\
Data File : VN051672.D
Acq On : 5 Oct 2018 7:32
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
Title : SW846 8260
Last Update : Tue Oct 02 06:56:35 2018

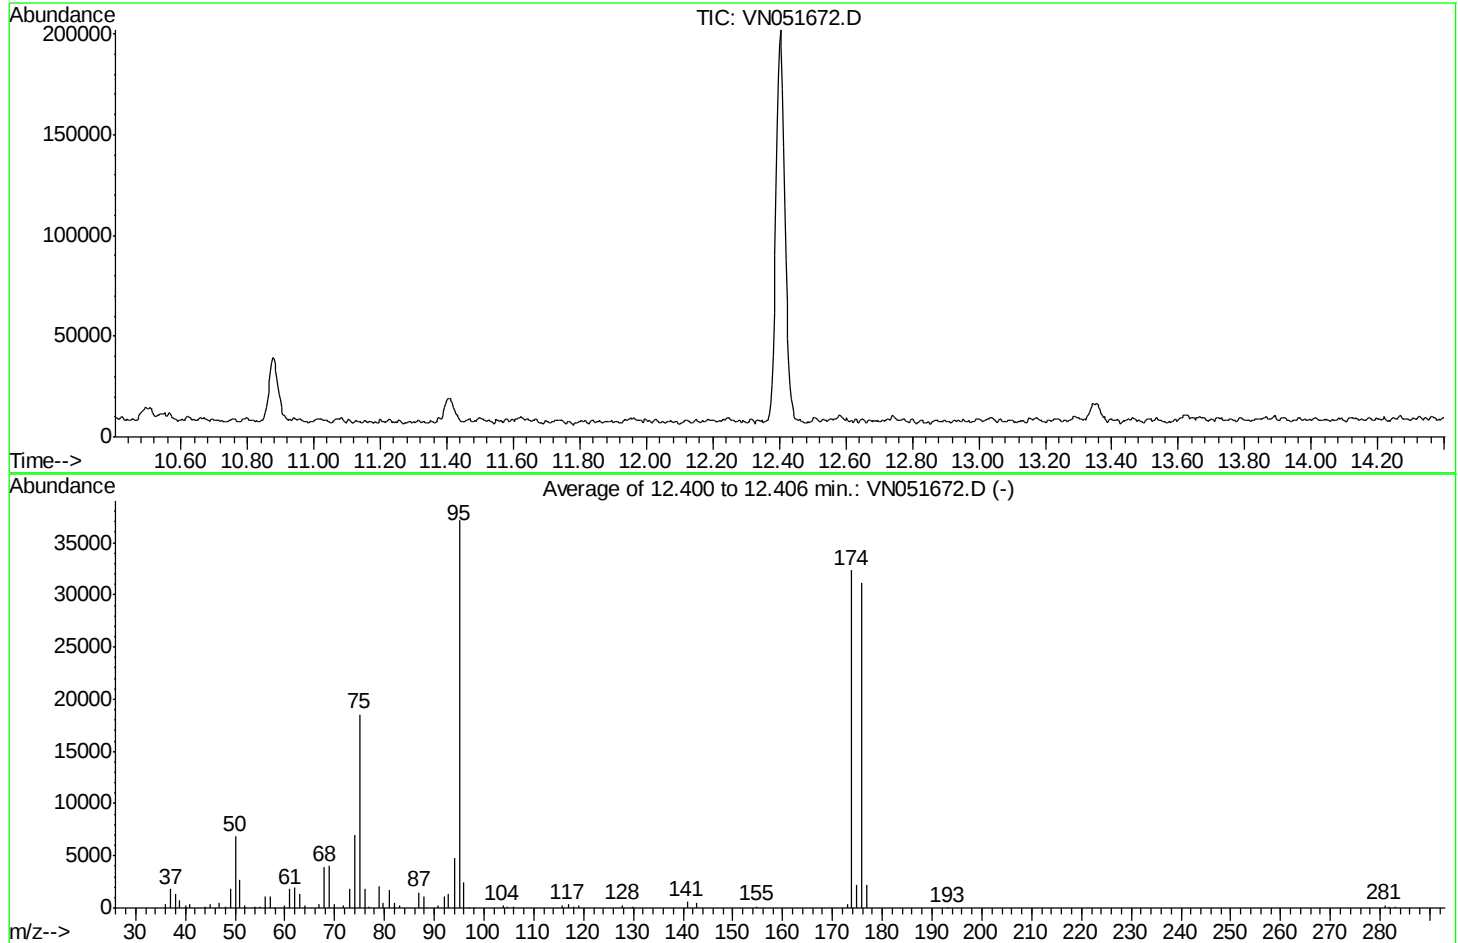

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6847	PASS
75	95	30	60	49.9	18525	PASS
95	95	100	100	100.0	37133	PASS
96	95	5	9	6.5	2396	PASS
173	174	0.00	2	1.2	386	PASS
174	95	50	100	87.0	32314	PASS
175	174	5	9	6.9	2237	PASS
176	174	95	101	96.5	31184	PASS
177	176	5	9	7.0	2195	PASS