

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100520\
 Data File : VN063872.D
 Acq On : 5 Oct 2020 15:45
 Operator : JC/MD
 Sample : PB132063ZHE#04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132063ZHE#04

Manual Integrations
 APPROVED

MMDadoda
 10/6/2020 12:56:52 PM

Quant Time: Oct 06 02:16:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	226649	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	429860	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	444591	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	179634	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	200702	53.60	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.20%	
35) Dibromofluoromethane	7.55	113	142407	47.74	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.48%	
50) Toluene-d8	10.06	98	552248	48.84	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.68%	
62) 4-Bromofluorobenzene	12.38	95	215354	50.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.34%	
Target Compounds						
16) Acetone	3.78	43	11503	9.980	ug/l	100
18) Methyl Acetate	4.29	43	3860m	1.290	ug/l	
20) Methylene Chloride	4.51	84	11671	4.510	ug/l	89
43) Isopropyl Acetate	8.13	43	81893	11.475	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN100520\
Data File : VN063872.D
Acq On : 5 Oct 2020 15:45
Operator : JC/MD
Sample : PB132063ZHE#04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
PB132063ZHE#04

Manual Integrations
APPROVED

MMDadoda
10/6/2020 12:56:52 PM

Quant Time: Oct 06 02:16:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

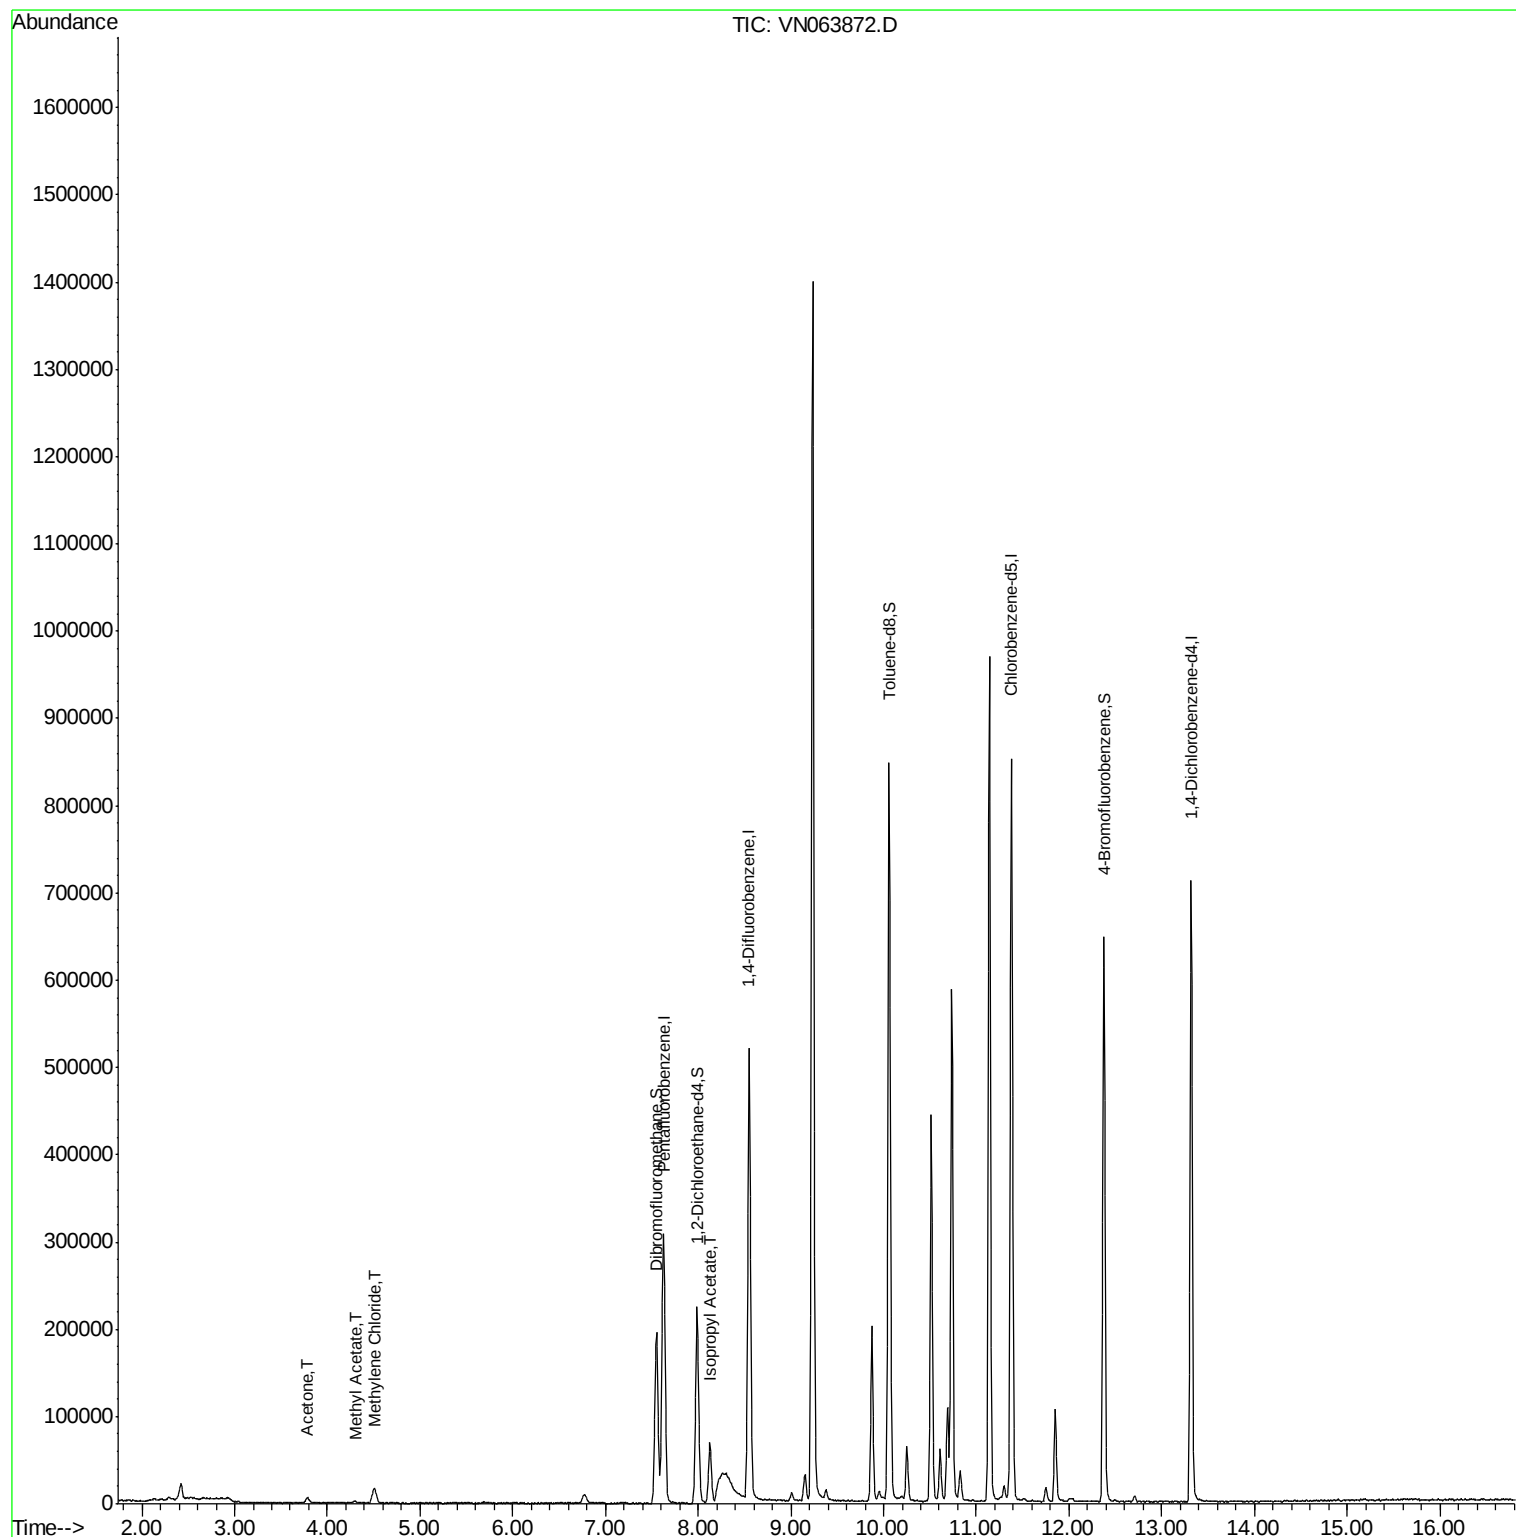

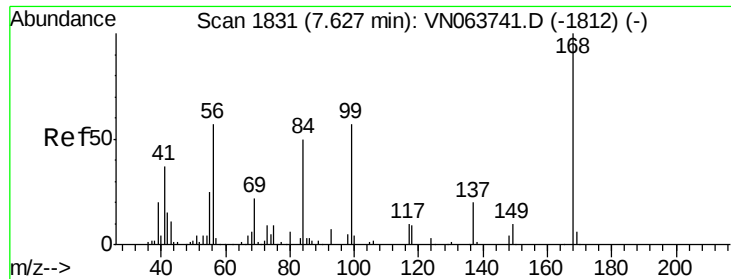

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN063872.D

Acq: 5 Oct 2020 15:45

Instrument :

MSVOA_N

ClientSampleId :

PB132063ZHE#04

Tot Ion:168 Resp: 226649

Ion Ratio Lower Upper

168 100


99 66.5 51.8 77.6

Manual Integrations

APPROVED

MMDadoda

10/6/2020 12:56:52 PM

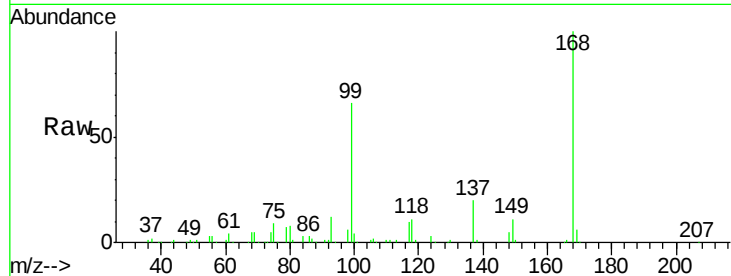

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70

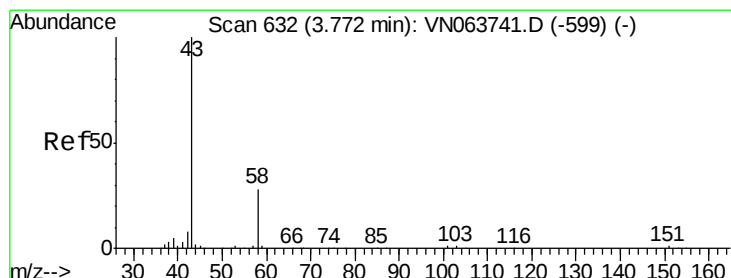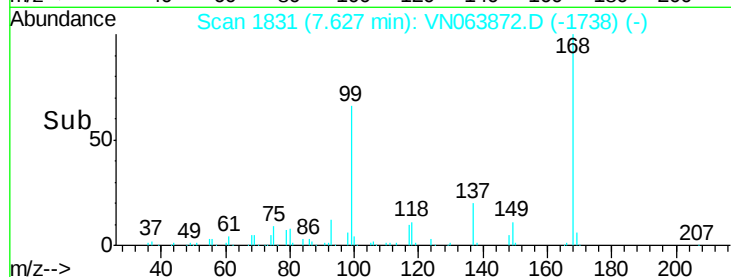

#16

Acetone

Concen: 9.980 ug/l

RT: 3.78 min Scan# 634

Delta R.T. 0.01 min

Lab File: VN063872.D


Acq: 5 Oct 2020 15:45

Tgt Ion: 43 Resp: 11503

Ion Ratio Lower Upper

43 100

58 27.9 22.3 33.5

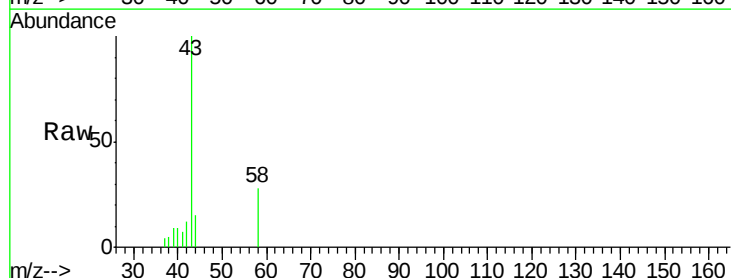

Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO

3.78

4000


3000

2000

1000

0

Time--> 3.70 3.75 3.80 3.85

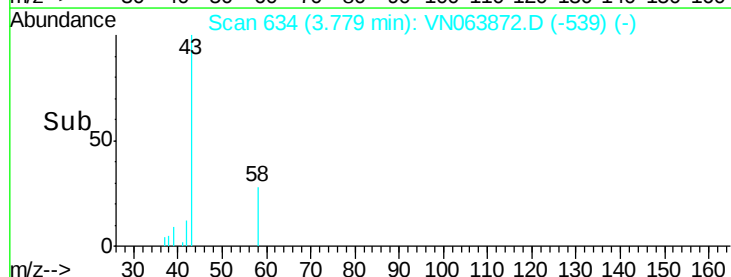







#18
Methyl Acetate
Concen: 1.290 ug/l m
RT: 4.29 min Scan# 794
Delta R.T. 0.02 min
Lab File: VN063872.D
Acq: 5 Oct 2020 15:45

Instrument :
MSVOA_N
ClientSampleId :
PB132063ZHE#04

Tot Ion: 43 Resp: 3860
Ion Ratio Lower Upper
43 100
74 5.7 17.4 26.2#




Manual Integrations
APPROVED


MMDadoda
10/6/2020 12:56:52 PM

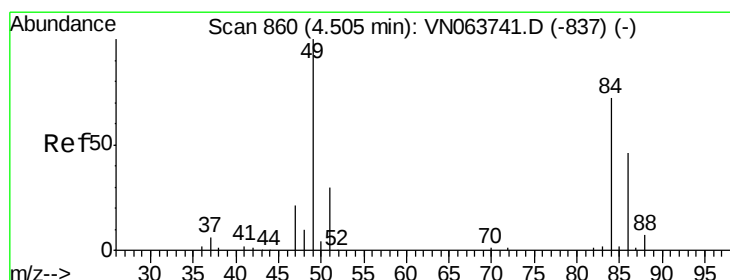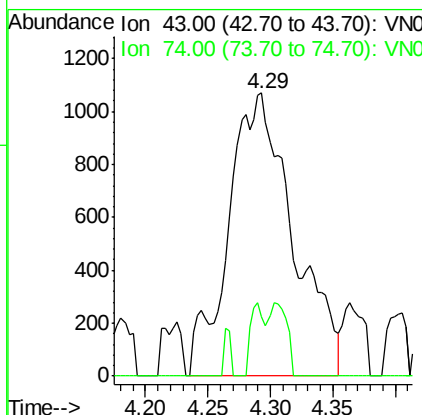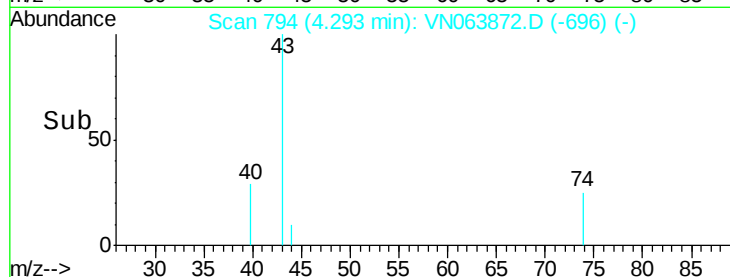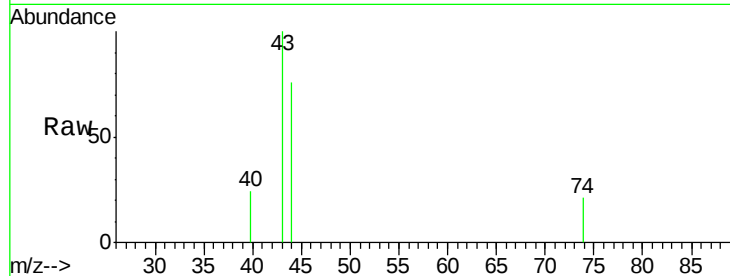

#20
Methylene Chloride
Concen: 4.510 ug/l
RT: 4.51 min Scan# 862
Delta R.T. 0.01 min
Lab File: VN063872.D
Acq: 5 Oct 2020 15:45

Tgt Ion: 84 Resp: 11671
Ion Ratio Lower Upper
84 100
49 120.5 110.4 165.6
51 39.2 33.3 49.9
86 56.9 50.7 76.1

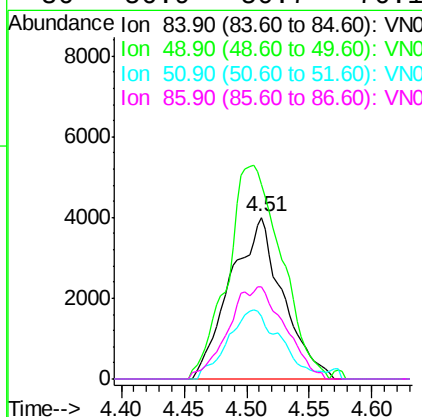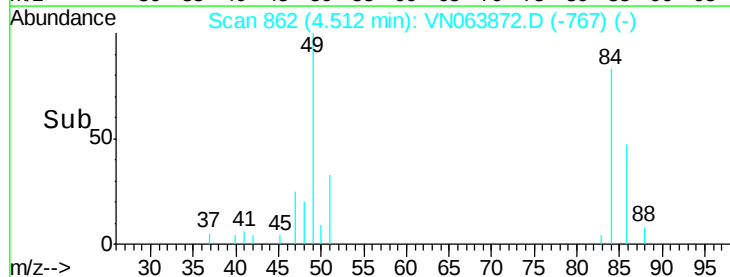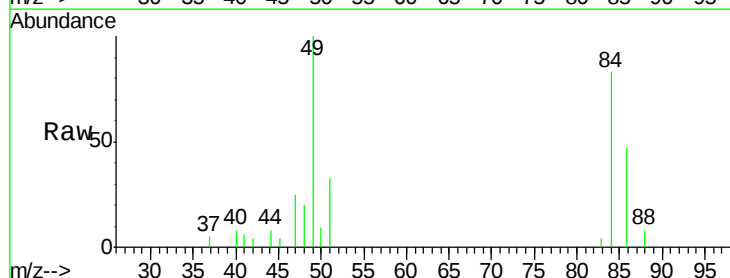

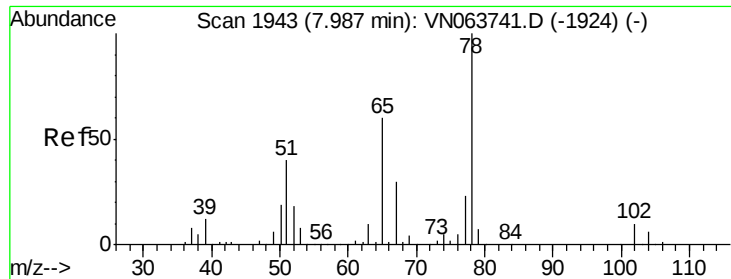





#33
 1,2-Dichloroethane-d4
 Concen: 53.601 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN063872.D
 Acq: 5 Oct 2020 15:45

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132063ZHE#04

Tot Ion	Ratio	Resp	Lower	Upper
65	100	200702		
67	48.8	0.0	99.6	




Manual Integrations
 APPROVED


MMDadoda
 10/6/2020 12:56:52 PM

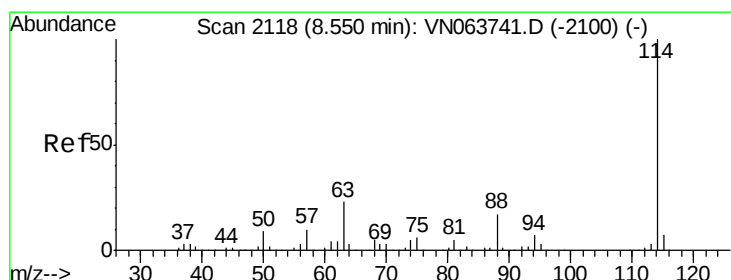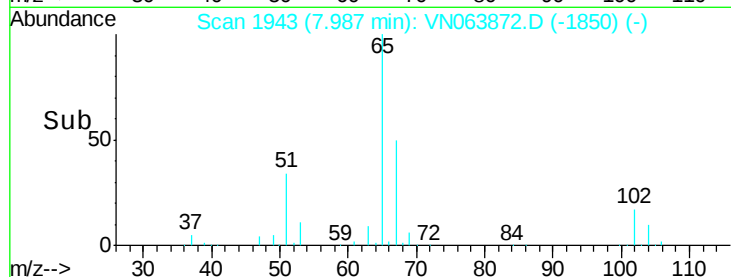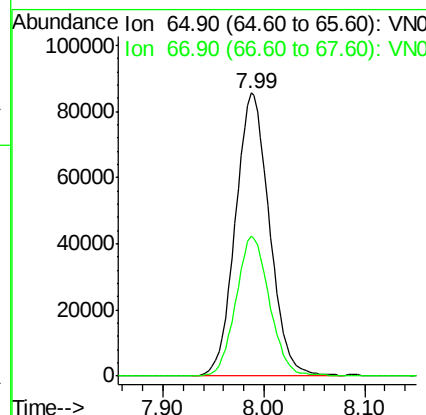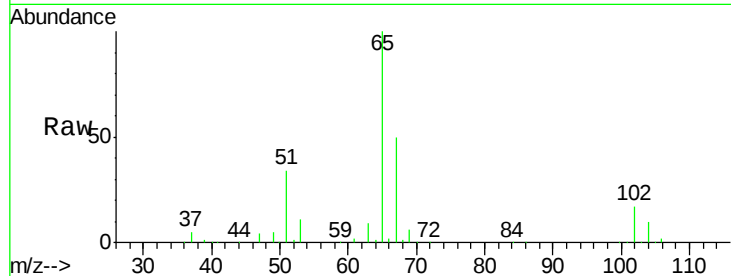

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN063872.D
 Acq: 5 Oct 2020 15:45

Tgt Ion	Ratio	Resp	Lower	Upper
114	100	429860		
63	22.7	0.0	45.0	
88	16.9	0.0	34.0	

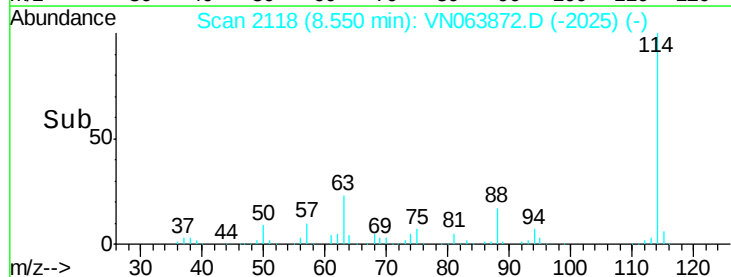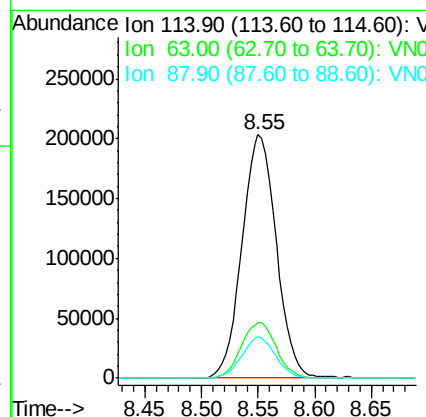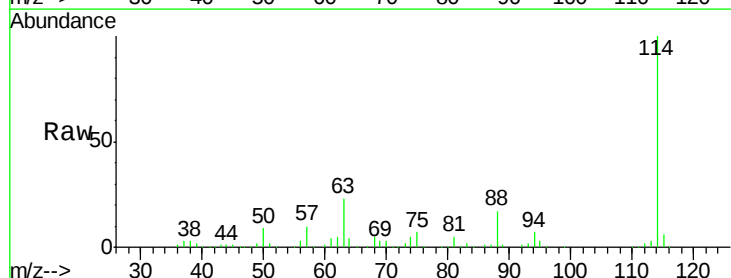

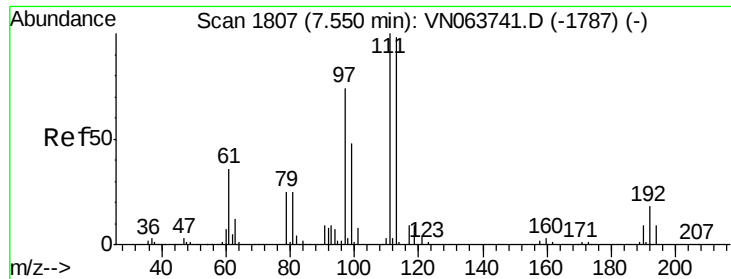





#35
 Dibromofluoromethane
 Concen: 47.744 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN063872.D
 Acq: 5 Oct 2020 15:45

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132063ZHE#04

Tot Ion	Ratio	Resp	Lower	Upper
113	100	142407		
111	101.9	81.8	122.8	
192	19.1	14.2	21.2	




Manual Integrations
 APPROVED


MMDadoda
 10/6/2020 12:56:52 PM

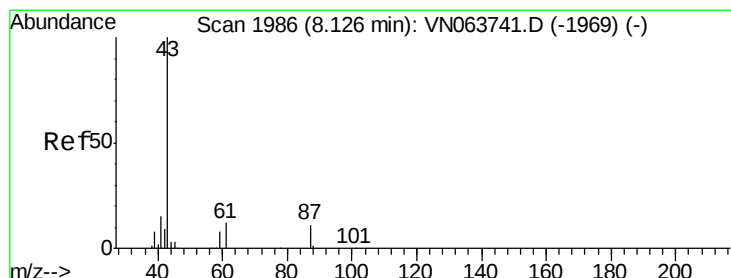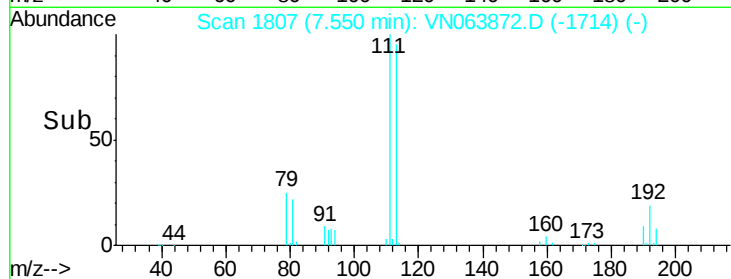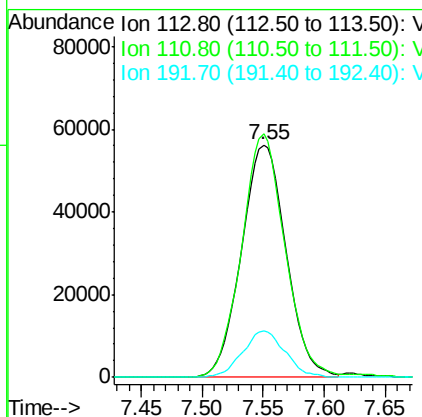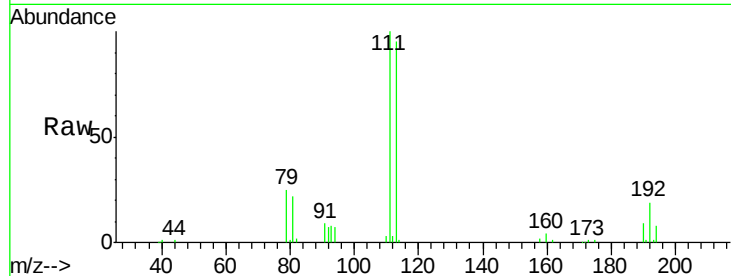

#43
 Isopropyl Acetate
 Concen: 11.475 ug/l
 RT: 8.13 min Scan# 1986
 Delta R.T. 0.00 min
 Lab File: VN063872.D
 Acq: 5 Oct 2020 15:45

Tgt Ion	Ratio	Resp	Lower	Upper
43	100	81893		
61	16.6	14.2	21.4	
87	12.3	9.0	13.6	

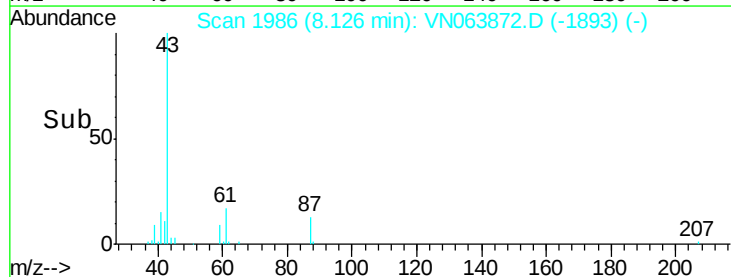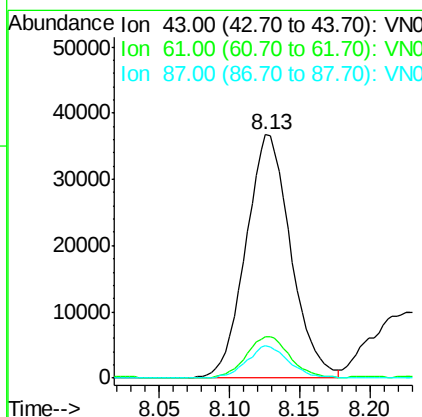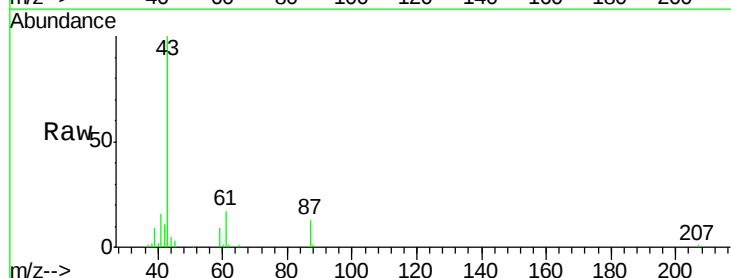

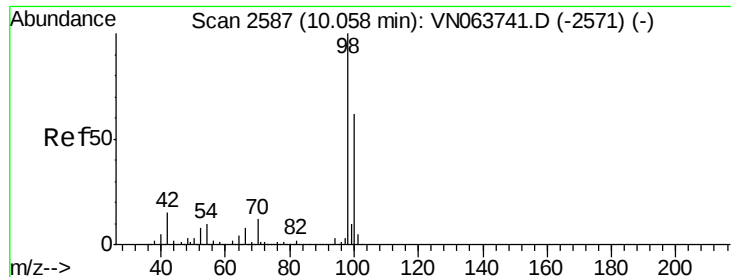





#50
Toluene-d8
Concen: 48.841 ug/l
RT: 10.06 min Scan# 2587
Delta R.T. 0.00 min
Lab File: VN063872.D
Acq: 5 Oct 2020 15:45

Instrument :
MSVOA_N
ClientSampleId :
PB132063ZHE#04

Tot Ion	Ion	Ratio	Resp	Lower	Upper
98	100		552248		
100	63.7		49.8		74.6




Manual Integrations
APPROVED


MMDadoda
10/6/2020 12:56:52 PM

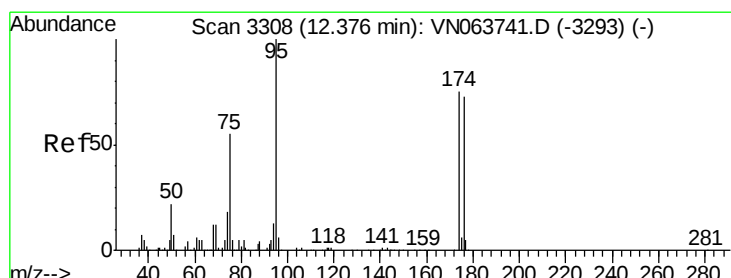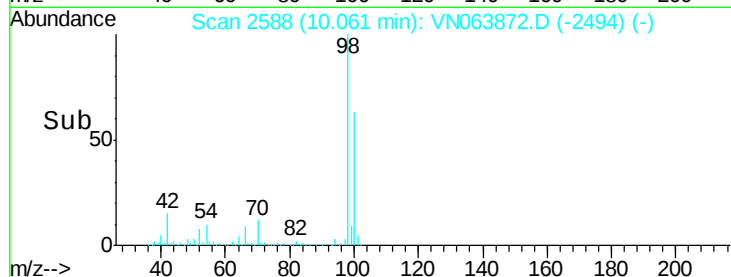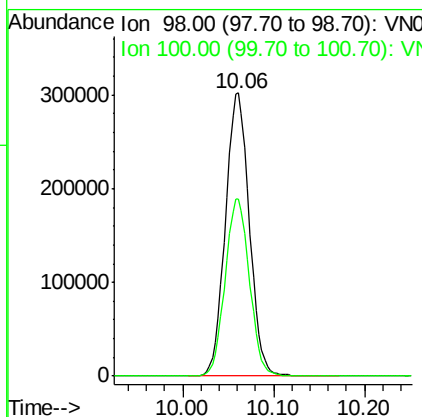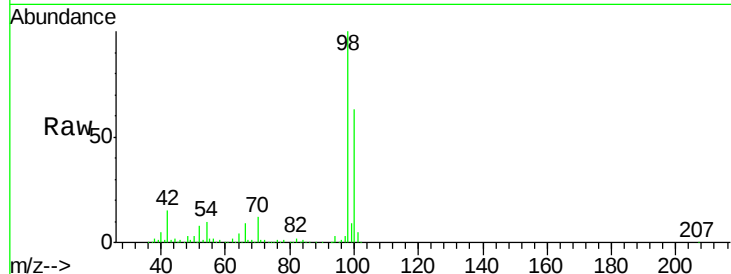

#62
4-Bromofluorobenzene
Concen: 50.666 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN063872.D
Acq: 5 Oct 2020 15:45

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
95	100		215354		
174	75.7		0.0		150.6
176	71.0		0.0		145.4

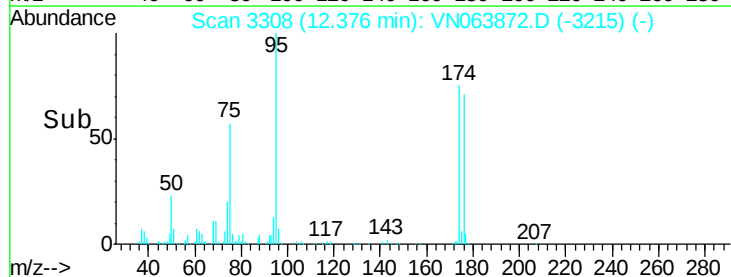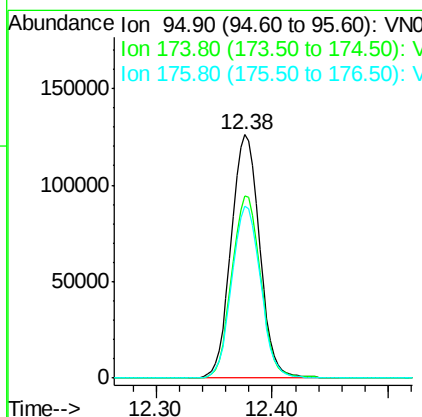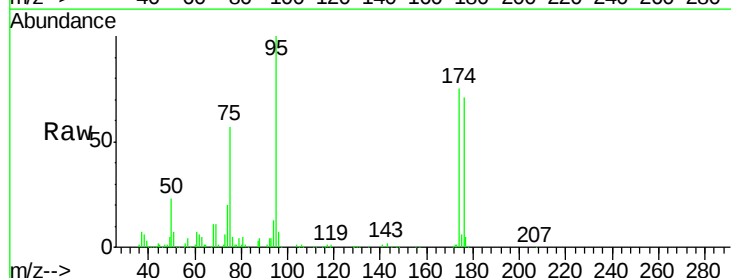

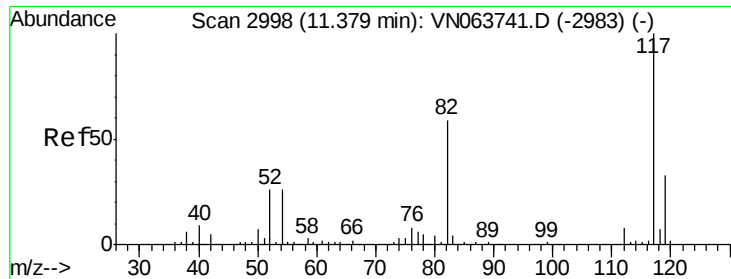





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063872.D
Acq: 5 Oct 2020 15:45

Instrument :
MSVOA_N
ClientSampleId :
PB132063ZHE#04

Tot Ion	Ratio	Lower	Upper
117	100		
82	60.5	47.4	71.2
119	31.4	26.4	39.6

Manual Integrations
APPROVED

MMDadoda
10/6/2020 12:56:52 PM

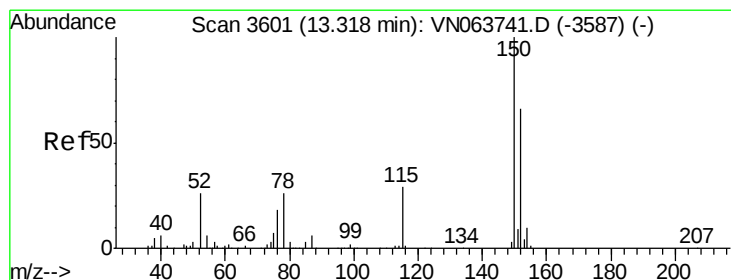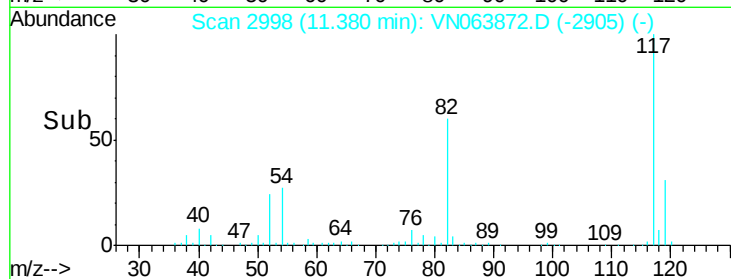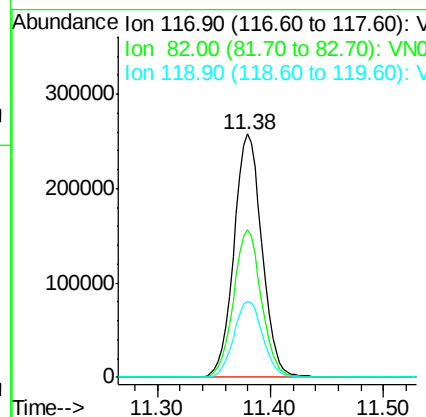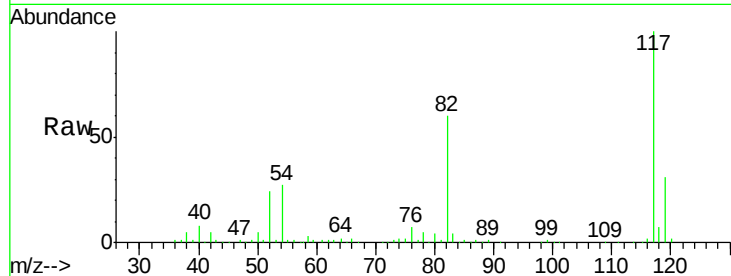

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN063872.D
Acq: 5 Oct 2020 15:45

Tgt Ion	Ratio	Lower	Upper
152	100		
115	60.1	31.3	93.8
150	154.8	0.0	341.8

