

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100520\
 Data File : VN063885.D
 Acq On : 5 Oct 2020 20:56
 Operator : JC/MD
 Sample : L4273-21
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TRIP

Quant Time: Oct 06 03:57:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	222213	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	416093	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	426325	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	168786	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	198452	54.06	ug/l	0.00
Spiked Amount 50.000			Recovery	=	108.12%	
35) Dibromofluoromethane	7.55	113	143655	49.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.52%	
50) Toluene-d8	10.06	98	531650	48.57	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.14%	
62) 4-Bromofluorobenzene	12.38	95	202962	49.33	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.66%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN100520\
Data File : VN063885.D
Acq On : 5 Oct 2020 20:56
Operator : JC/MD
Sample : L4273-21
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TRIP

Quant Time: Oct 06 03:57:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

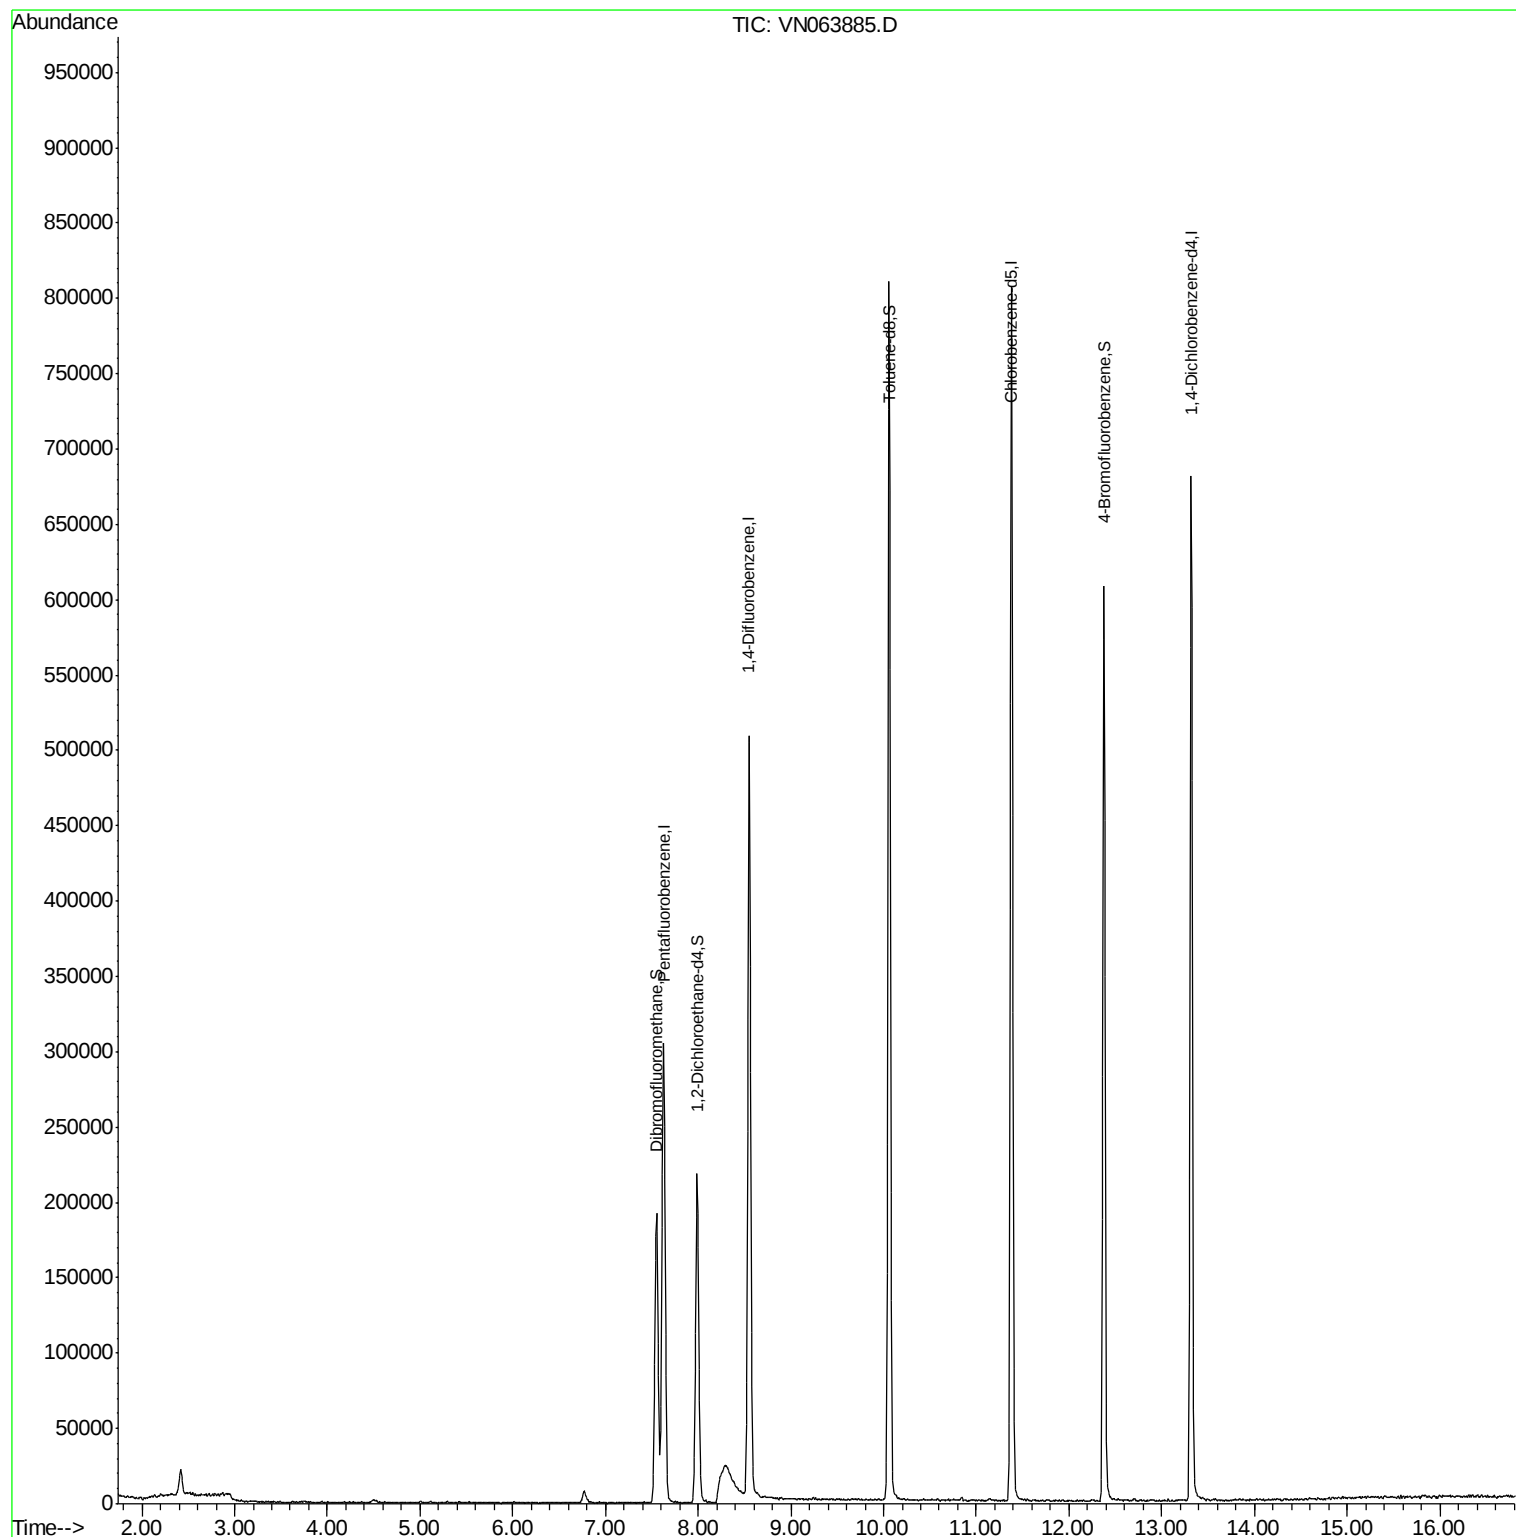

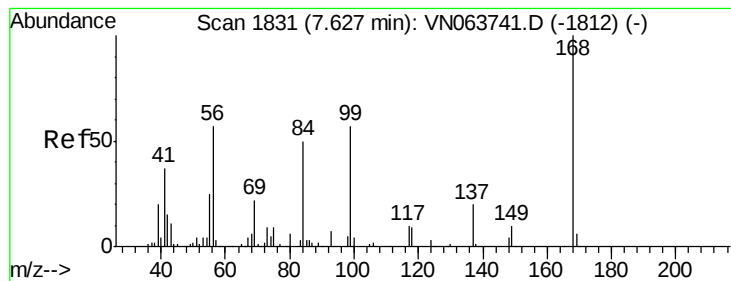

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN063885.D

Acq: 5 Oct 2020 20:56

Instrument :

MSVOA_N

ClientSampled :


TRIP

Tot Ion:168 Resp: 222213

Ion Ratio Lower Upper

168 100

99 64.3 51.8 77.6

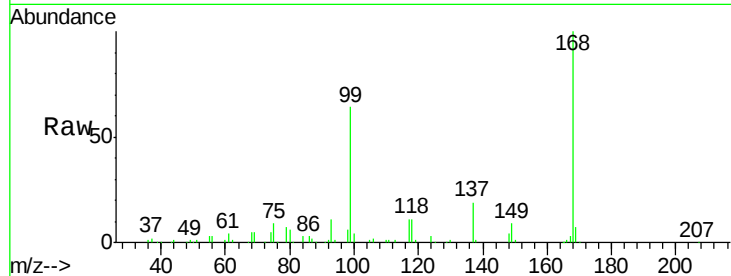

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.63

100000

80000



60000

40000

20000

0

Time-->

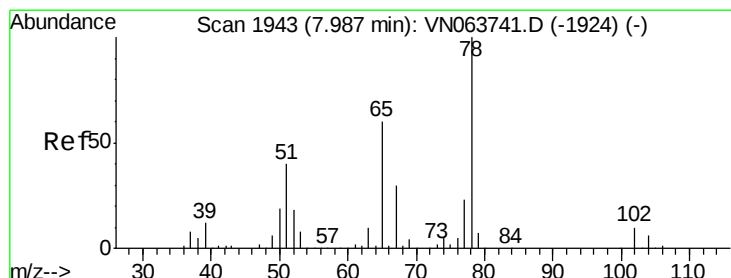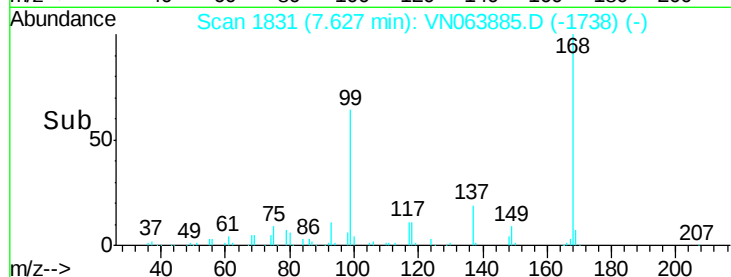

#33

1,2-Dichloroethane-d4

Concen: 54.058 ug/l

RT: 7.99 min Scan# 1944

Delta R.T. 0.00 min

Lab File: VN063885.D


Acq: 5 Oct 2020 20:56

Tgt Ion: 65 Resp: 198452

Ion Ratio Lower Upper

65 100

67 48.0 0.0 99.6

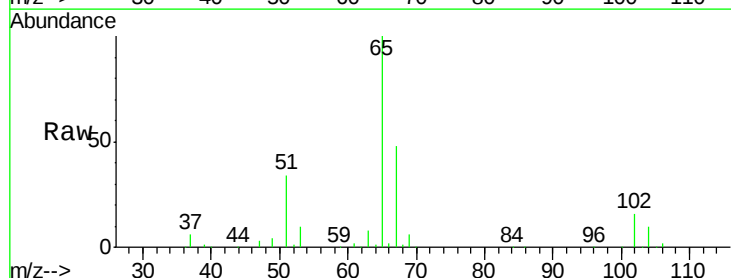

Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

7.99

100000

80000


60000


40000

20000

0

Time-->

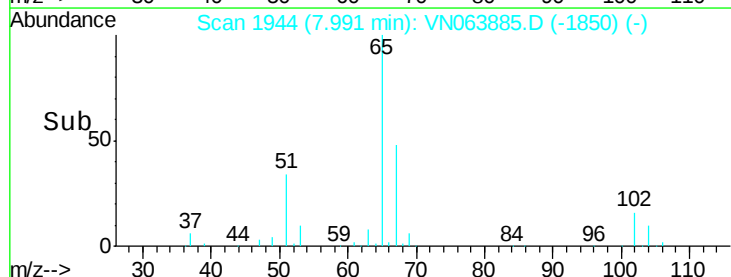

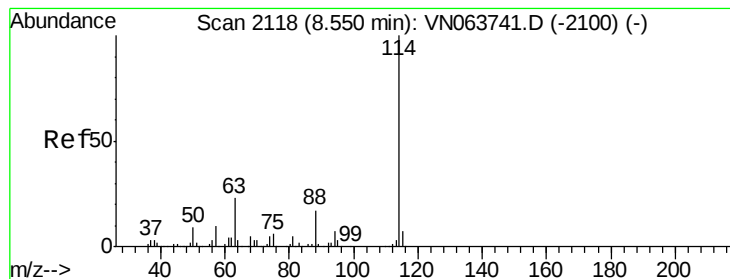

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. 0.00 min

Lab File: VN063885.D

Acq: 5 Oct 2020 20:56

Instrument :

MSVOA_N

ClientSampled :

TRIP


Tot Ion:114 Resp: 416093

Ion Ratio Lower Upper

114 100

63 24.1 0.0 45.0




88 17.0 0.0 34.0

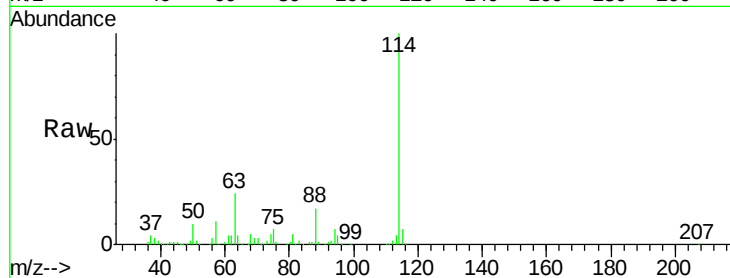

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

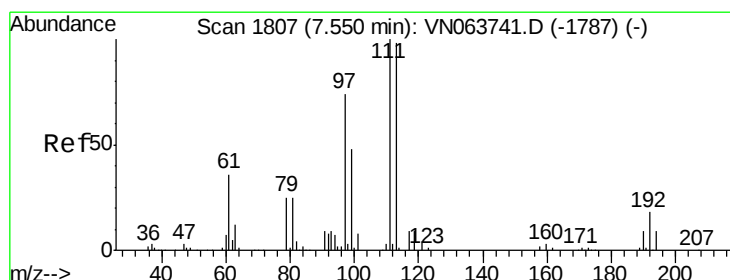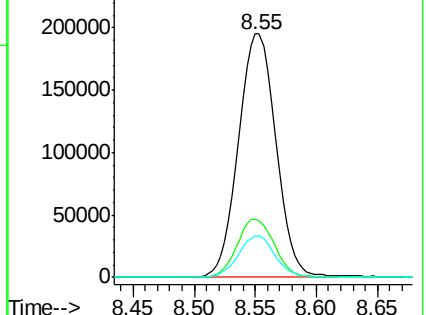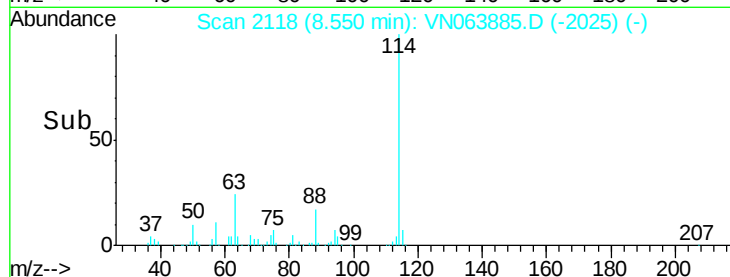

#35

Dibromofluoromethane

Concen: 49.756 ug/l

RT: 7.55 min Scan# 1807

Delta R.T. 0.00 min

Lab File: VN063885.D

Acq: 5 Oct 2020 20:56


Tgt Ion:113 Resp: 143655

Ion Ratio Lower Upper

113 100

111 103.6 81.8 122.8



192 17.7 14.2 21.2

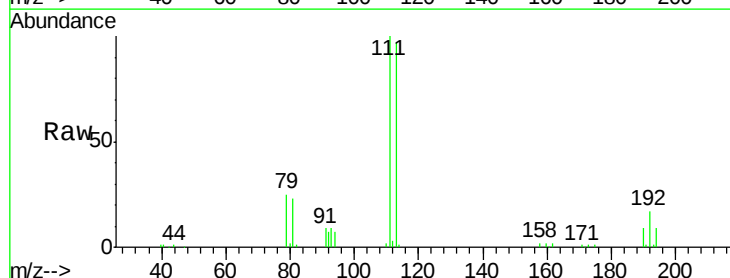


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



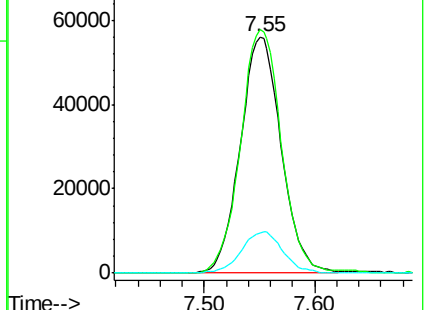
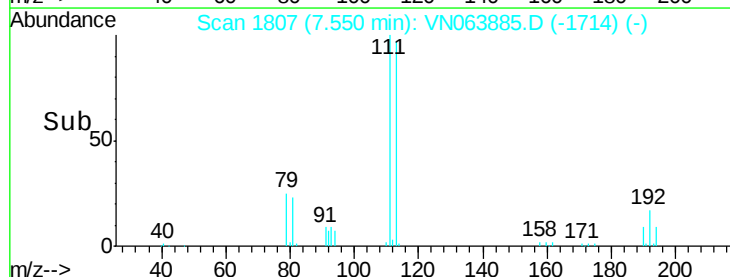


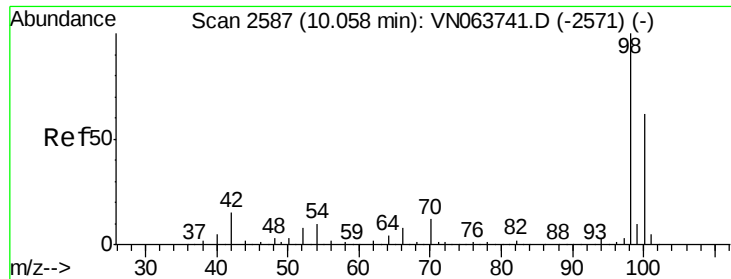

#50
Toluene-d8
Concen: 48.575 ug/l
RT: 10.06 min Scan# 2588
Delta R.T. 0.00 min
Lab File: VN063885.D
Acq: 5 Oct 2020 20:56




Instrument :
MSVOA_N
ClientSampleId :
TRIP


Tot Ion: 98 Resp: 531650
Ion Ratio Lower Upper
98 100
100 62.5 49.8 74.6

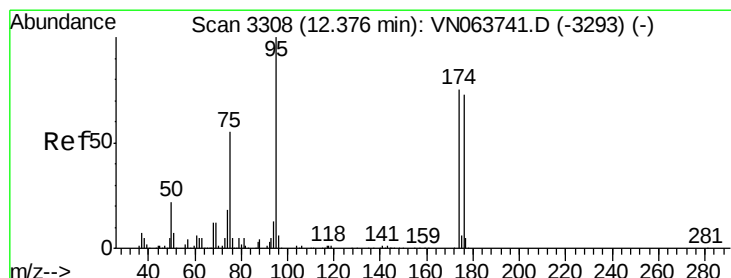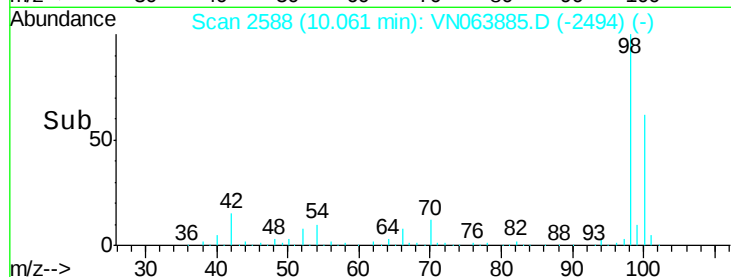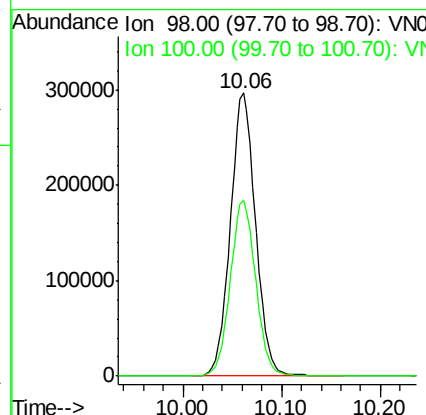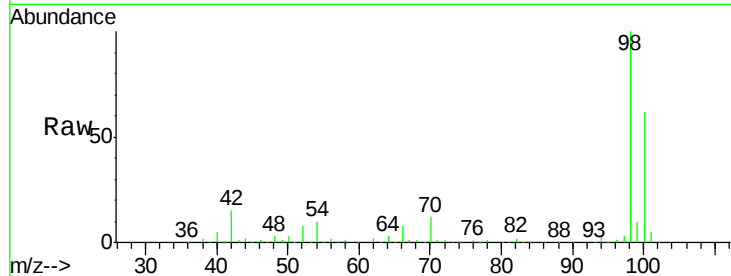

#62
4-Bromofluorobenzene
Concen: 49.331 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN063885.D
Acq: 5 Oct 2020 20:56

Tgt Ion: 95 Resp: 202962
Ion Ratio Lower Upper
95 100
174 74.1 0.0 150.6
176 72.9 0.0 145.4


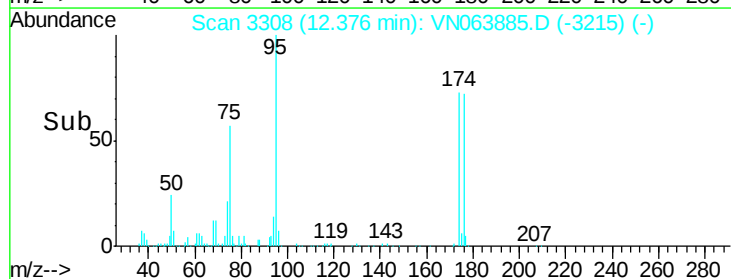
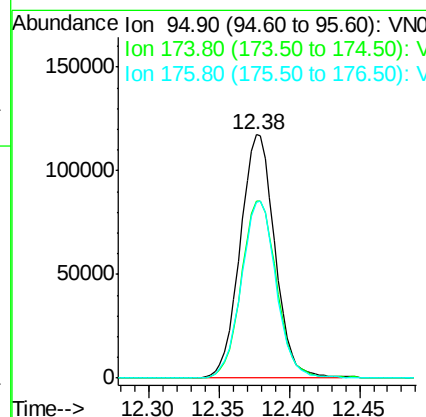
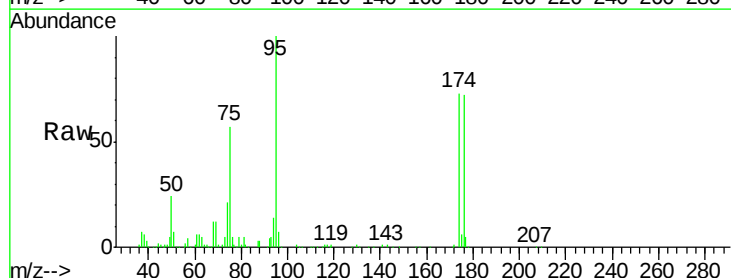


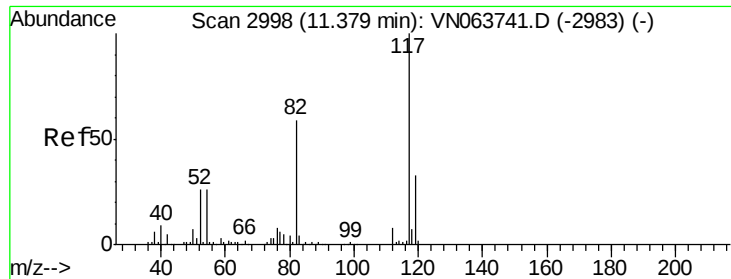

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063885.D
Acq: 5 Oct 2020 20:56

Instrument :
MSVOA_N
ClientSampleId :
TRIP

Tot Ion:117 Resp: 426325
Ion Ratio Lower Upper
117 100
82 60.9 47.4 71.2
119 31.3 26.4 39.6

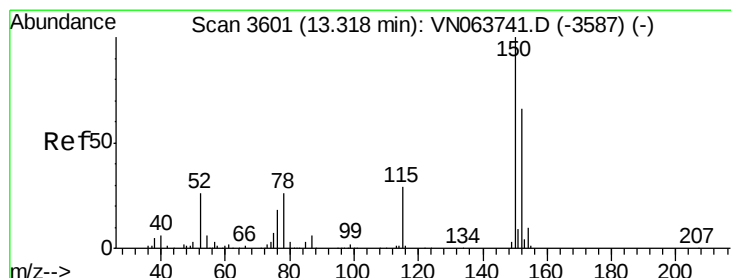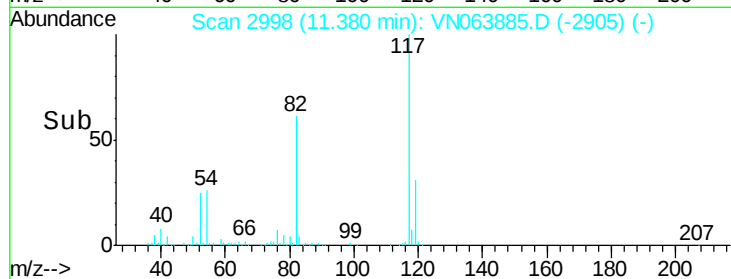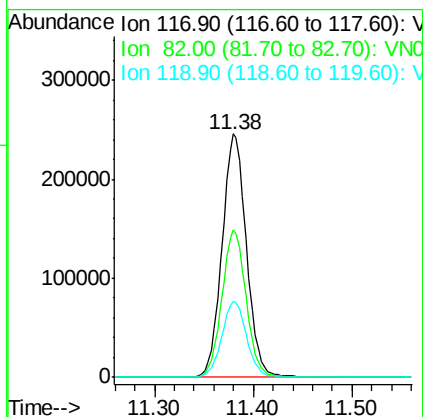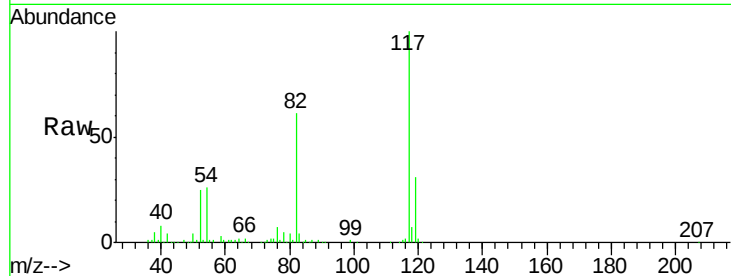

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN063885.D
Acq: 5 Oct 2020 20:56

Tgt Ion:152 Resp: 168786
Ion Ratio Lower Upper
152 100
115 62.2 31.3 93.8
150 157.9 0.0 341.8

