


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100521\
 Data File : VN068799.D
 Acq On : 5 Oct 2021 11:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N092821W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Sep 29 08:56:32 2021

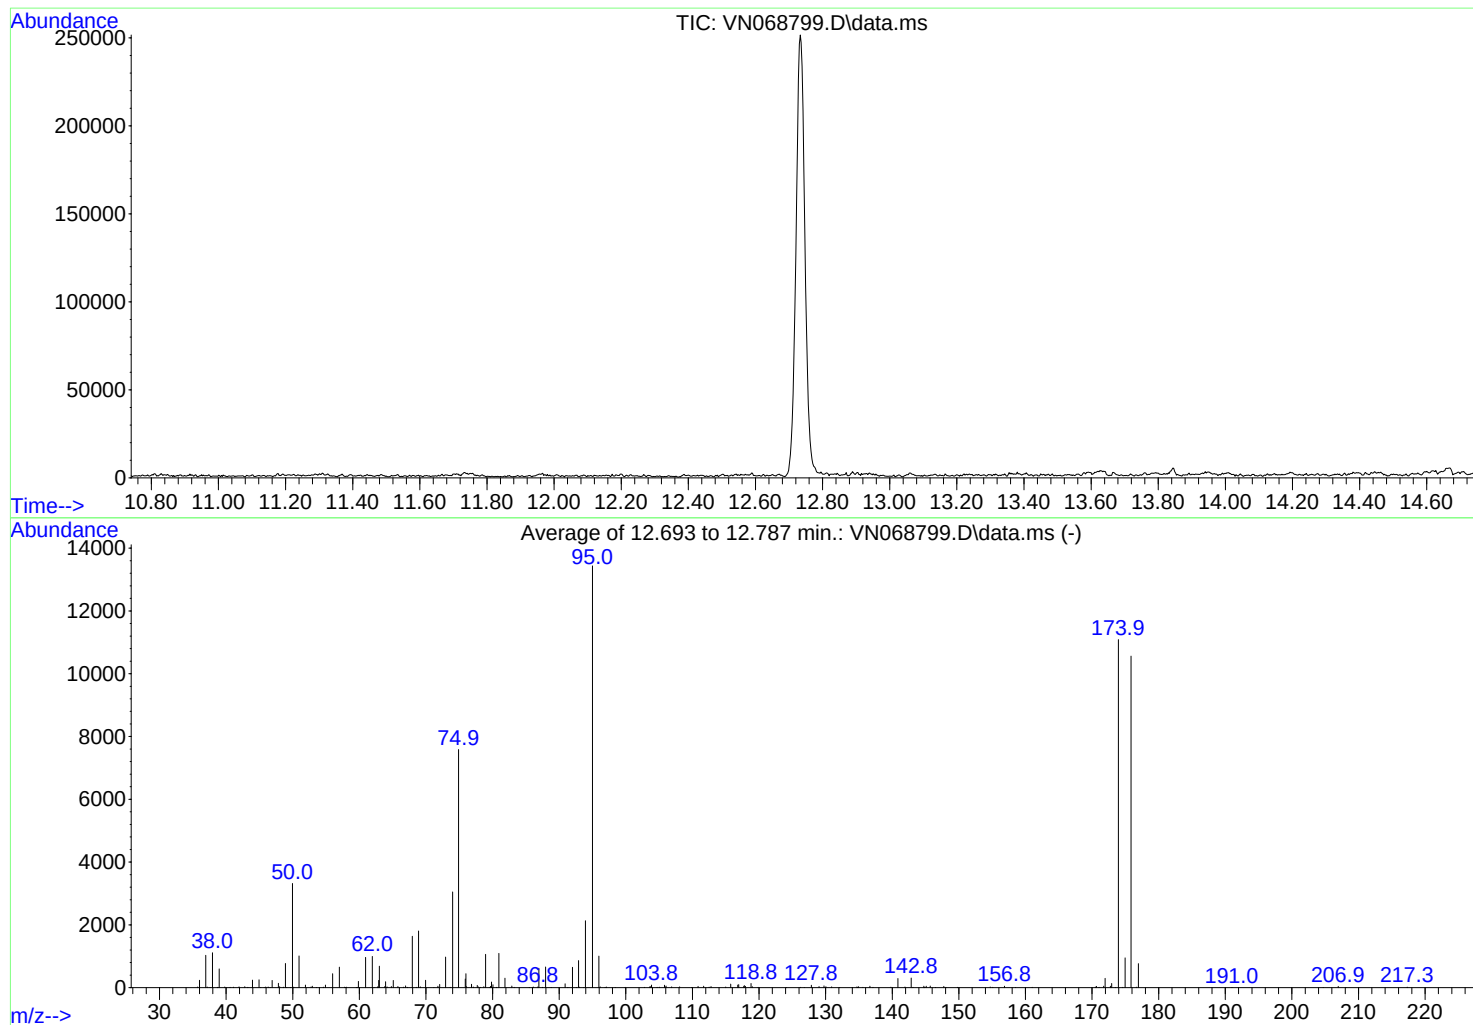

AutoFind: Averaged scan 3991 to 4026; Bkg corrected with scan 3990

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	3320	PASS
75	95	30	60	56.4	7584	PASS
95	95	100	100	100.0	13436	PASS
96	95	5	9	7.5	1005	PASS
173	174	0.00	2	1.2	131	PASS
174	95	50	100	82.5	11088	PASS
175	174	5	9	8.5	947	PASS
176	174	95	101	95.3	10563	PASS
177	176	5	9	7.2	764	PASS