

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100522\
 Data File : VN074753.D
 Acq On : 05 Oct 2022 21:37
 Operator : JC\MD
 Sample : N4957-05
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-21

Quant Time: Oct 06 07:43:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 05:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	281204	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	537823	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	565341	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	266808	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	373778	56.098	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	112.200%
35) Dibromofluoromethane	8.177	113	288160	53.030	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	106.060%
50) Toluene-d8	10.571	98	1190212	51.046	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.100%
62) 4-Bromofluorobenzene	12.853	95	319857	45.128	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.260%
Target Compounds						
					Qvalue	
6) Chloroethane	2.836	64	244223	31.085	ug/l #	51
11) Tert butyl alcohol	5.530	59	2686	1.204	ug/l #	76
13) Acrolein	4.189	56	367	Below Cal	#	14
16) Acetone	4.465	43	133008	35.226	ug/l	100
18) Methyl Acetate	5.059	43	26309	1.882	ug/l	93
20) Methylene Chloride	5.289	84	29691	2.849	ug/l	90
25) 2-Butanone	7.518	43	17973	2.623	ug/l	98
29) Tetrahydrofuran	7.859	42	8418	1.763	ug/l	94
31) Cyclohexane	8.235	56	8132	0.706	ug/l #	60
36) 1,1-Dichloropropene	8.230	75	23908	2.718	ug/l #	43
37) Ethyl Acetate	7.518	43	17973	0.509	ug/l #	86
38) Carbon Tetrachloride	8.235	117	31214	3.763	ug/l #	14
40) Benzene	8.618	78	8159	0.287	ug/l #	72
42) 1,2-Dichloroethane	8.694	62	3608	0.404	ug/l	98
43) Isopropyl Acetate	8.700	43	564895	25.911	ug/l #	92
48) Methyl methacrylate	9.677	41	16335	1.825	ug/l #	85
49) 1,4-Dioxane	9.700	88	61	0.314	ug/l #	24
51) 4-Methyl-2-Pentanone	10.447	43	33325	2.374	ug/l	100
52) Toluene	10.629	92	7506	0.439	ug/l	92
54) cis-1,3-Dichloropropene	10.365	75	175423	14.754	ug/l #	62
57) 1,3-Dichloropropane	11.206	76	24259	1.957	ug/l #	42
59) 2-Hexanone	11.206	43	290777	27.382	ug/l #	56
68) m/p-Xylenes	12.070	106	3590	0.296	ug/l	88
74) N-amyl acetate	12.482	43	3751	0.242	ug/l #	59
75) 1,1,2,2-Tetrachloroethane	12.935	83	70	Below Cal	#	24
76) 1,2,3-Trichloropropane	12.853	75	183792	23.079	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	183792	44.967	ug/l #	15
95) Naphthalene	15.647	128	23209	1.252	ug/l #	95
96) 1,2,3-Trichlorobenzene	15.835	180	463	Below Cal	#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100522\
Data File : VN074753.D
Acq On : 05 Oct 2022 21:37
Operator : JC\MD
Sample : N4957-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-21

Quant Time: Oct 06 07:43:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 05:37:50 2022
Response via : Initial Calibration




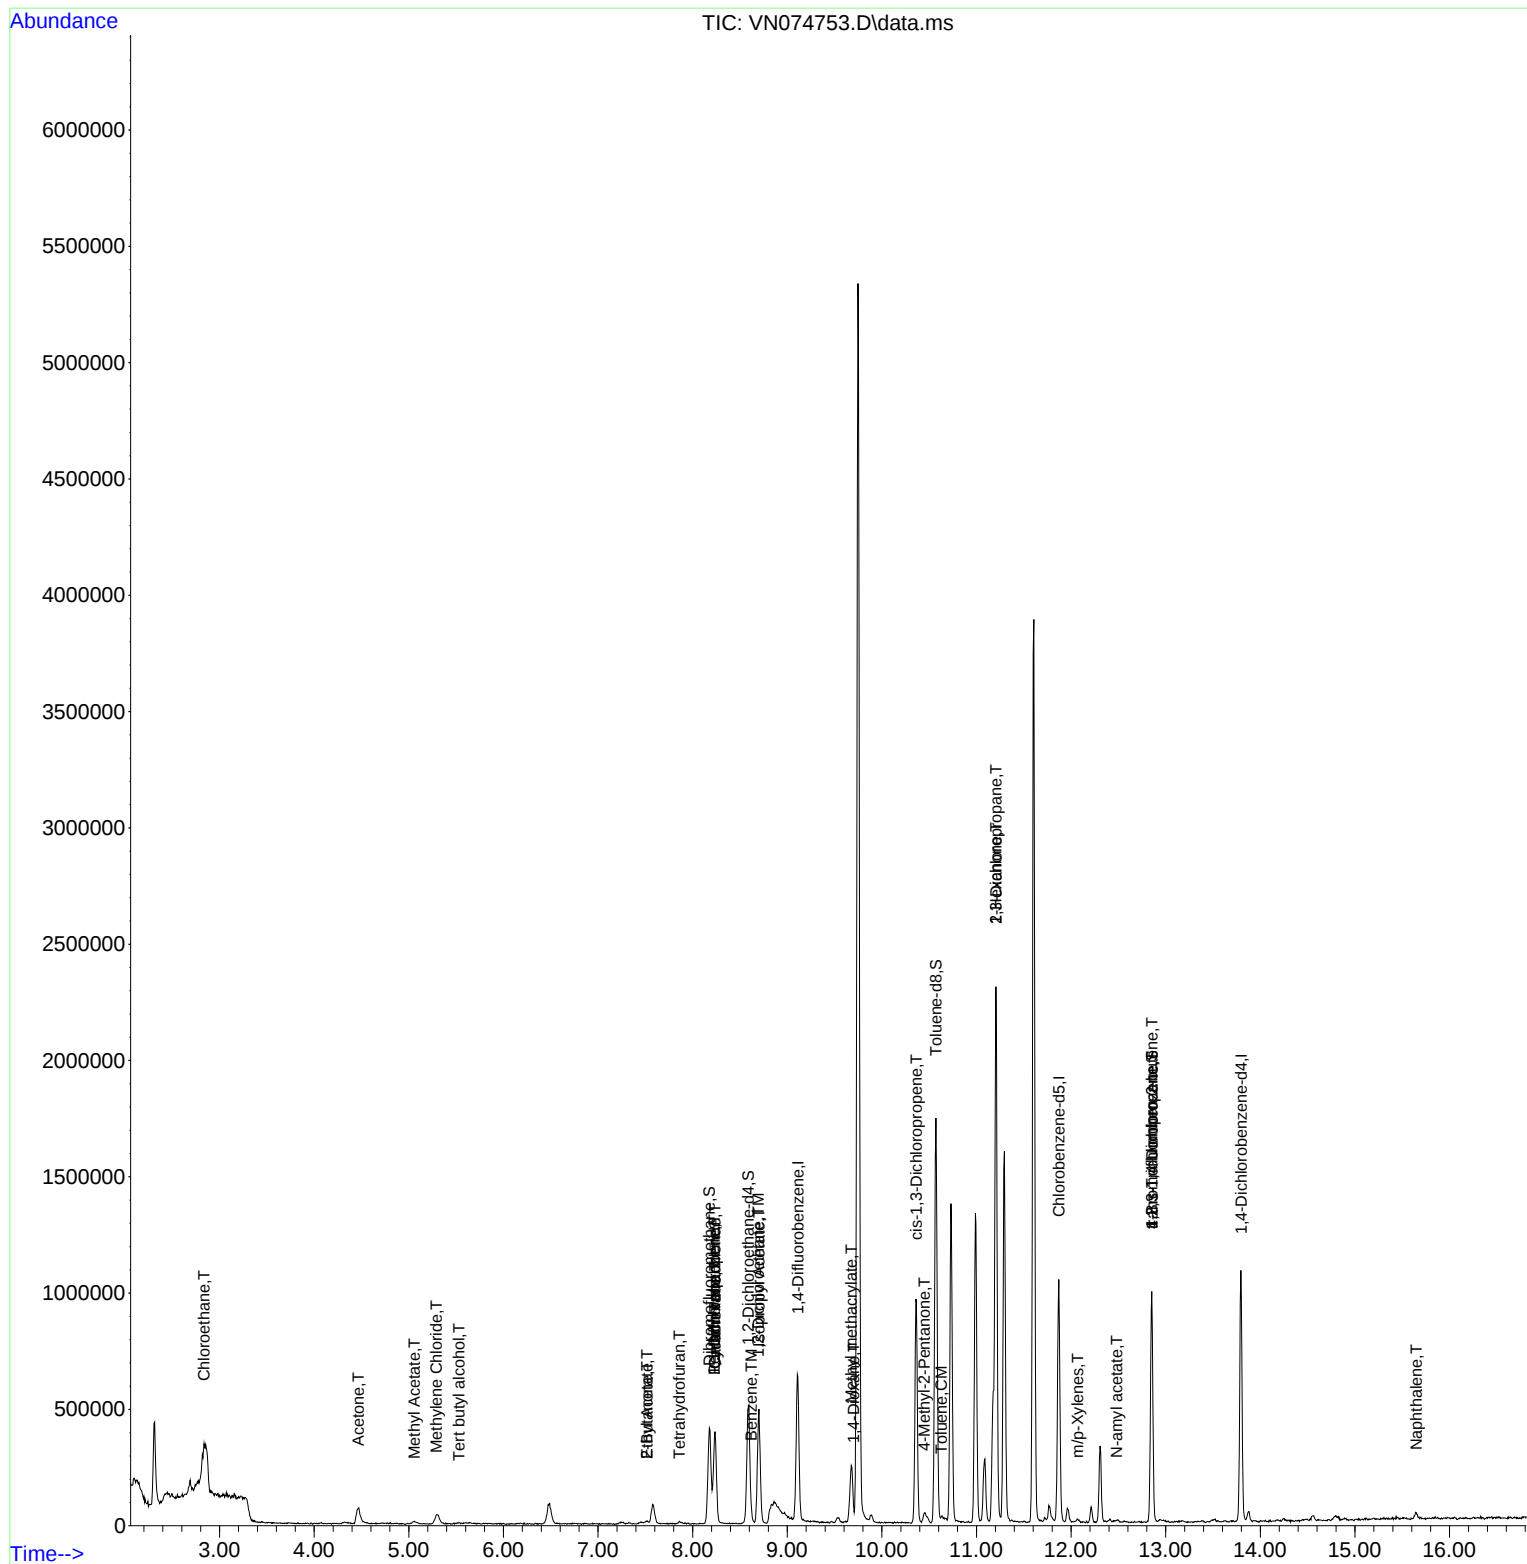




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1051
Delta R.T. -0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion:168 Resp: 281204
Ion Ratio Lower Upper
168 100
99 58.3 42.8 64.2

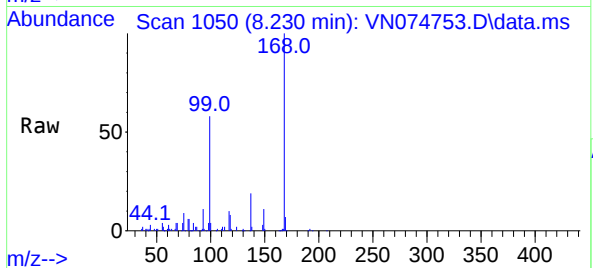

#6
Chloroethane
Concen: 31.085 ug/l
RT: 2.836 min Scan# 133
Delta R.T. -0.277 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 64 Resp: 244223
Ion Ratio Lower Upper
64 100
66 4.5 25.1 37.7#


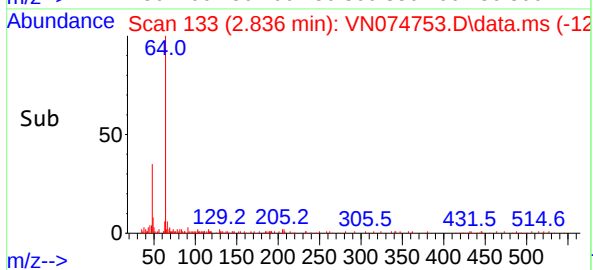






#11
Tert butyl alcohol
Concen: 1.204 ug/l
RT: 5.530 min Scan# 59
Delta R.T. -0.030 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion: 59 Resp: 2686
Ion Ratio Lower Upper
59 100
57 18.5 7.7 11.5#

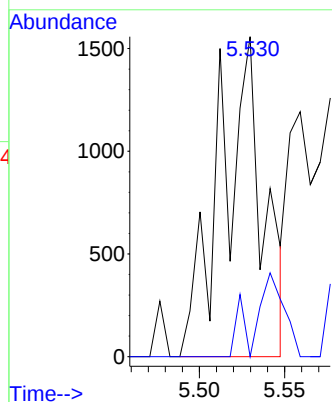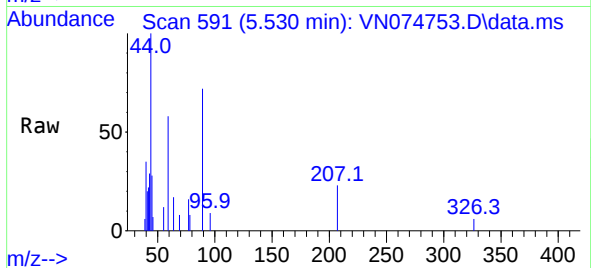

#13
Acrolein
Concen: Below Cal
RT: 4.189 min Scan# 363
Delta R.T. -0.012 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 56 Resp: 367
Ion Ratio Lower Upper
56 100
55 138.1 54.9 82.3#


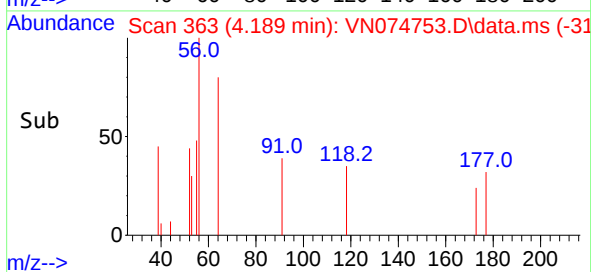
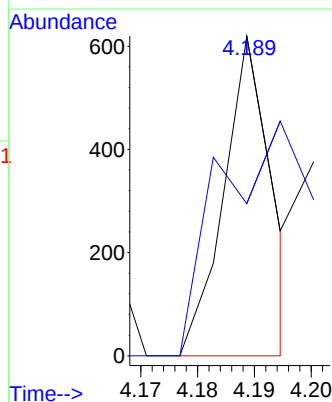





#16
Acetone
Concen: 35.226 ug/l
RT: 4.465 min Scan# 410
Delta R.T. 0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion: 43 Resp: 133008
Ion Ratio Lower Upper
43 100
58 31.3 24.9 37.3

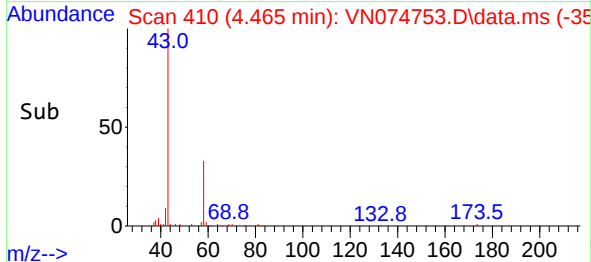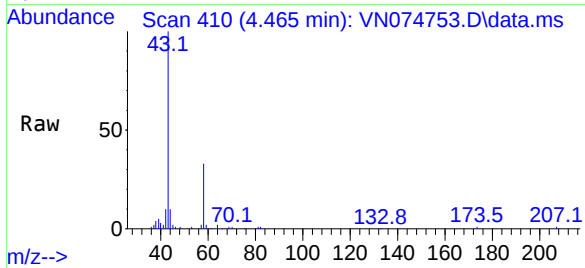

#18
Methyl Acetate
Concen: 1.882 ug/l
RT: 5.059 min Scan# 511
Delta R.T. 0.012 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 43 Resp: 26309
Ion Ratio Lower Upper
43 100
74 19.7 18.5 27.7

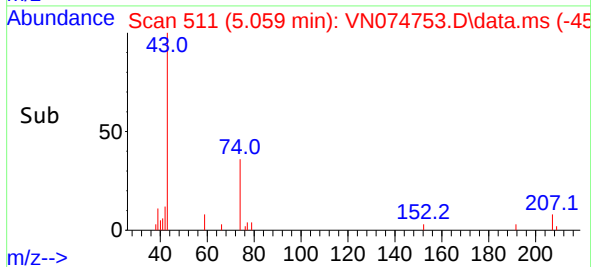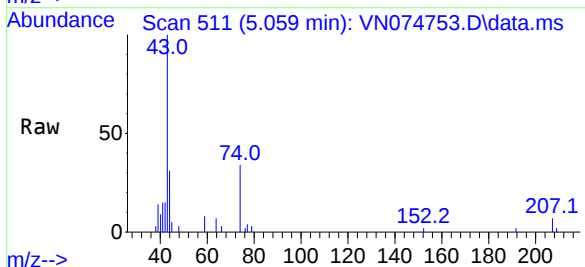







#20
Methylene Chloride
Concen: 2.849 ug/l
RT: 5.289 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Instrument :
MSVOA_N
ClientSampleId :
SB-21

Tgt Ion: 84 Resp: 29691




Ion	Ratio	Lower	Upper
84	100		
49	117.9	107.4	161.0
51	39.1	35.1	52.7
86	60.3	50.4	75.6

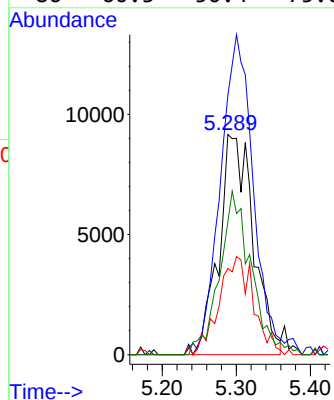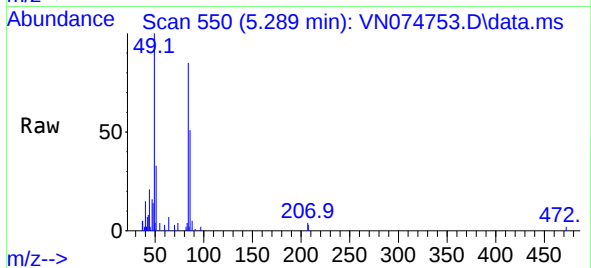


#25
2-Butanone
Concen: 2.623 ug/l
RT: 7.518 min Scan# 929
Delta R.T. 0.017 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 43 Resp: 17973

Ion	Ratio	Lower	Upper
43	100		
72	27.8	21.4	32.0


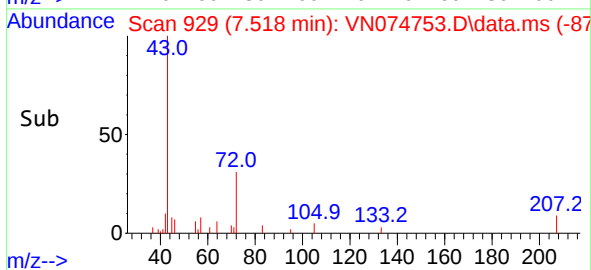
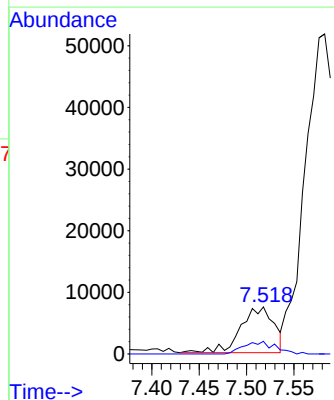





#29
Tetrahydrofuran
Concen: 1.763 ug/l
RT: 7.859 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion:	42	Resp:	8418
Ion	Ratio	Lower	Upper
42	100		
72	34.4	33.0	49.6
71	38.0	30.4	45.6

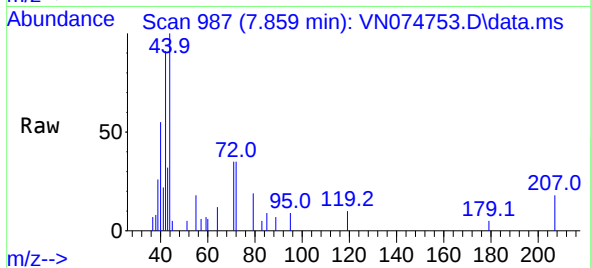

#31
Cyclohexane
Concen: 0.706 ug/l
RT: 8.235 min Scan# 1051
Delta R.T. -0.030 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion:	56	Resp:	8132
Ion	Ratio	Lower	Upper
56	100		
69	82.4	23.1	34.7#
84	66.2	67.1	100.7#


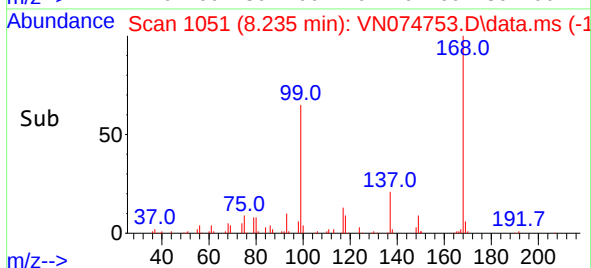
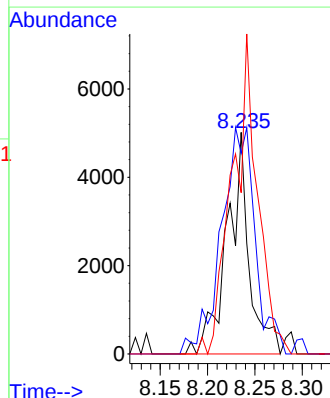





#33
1,2-Dichloroethane-d4
Concen: 56.098 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. -0.000 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion: 65 Resp: 373778
Ion Ratio Lower Upper
65 100
67 54.3 0.0 109.0

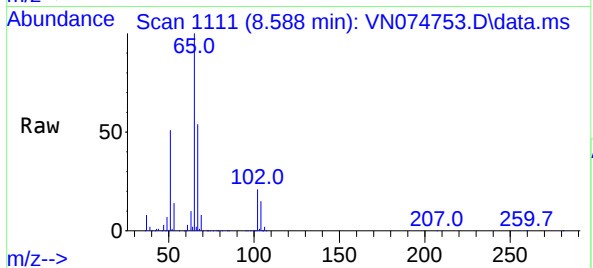

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.112 min Scan# 1200
Delta R.T. 0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 114 Resp: 537823
Ion Ratio Lower Upper
114 100
63 21.4 0.0 41.2
88 15.6 0.0 30.2


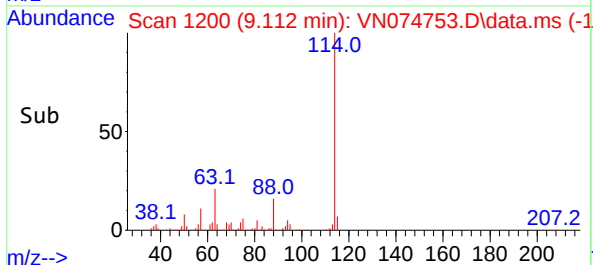
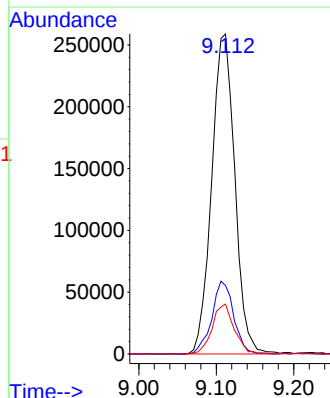
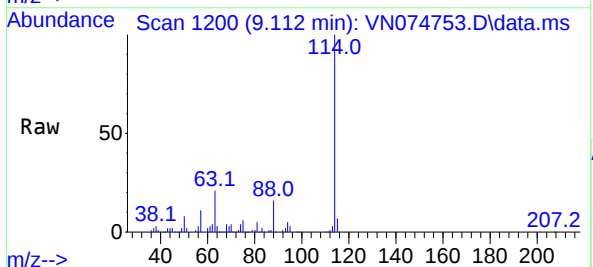




#35
Dibromofluoromethane
Concen: 53.030 ug/l
RT: 8.177 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion:113 Resp: 288160
Ion Ratio Lower Upper
113 100
111 103.1 83.0 124.6
192 16.0 12.6 18.8

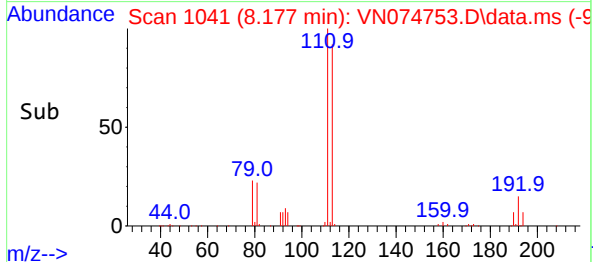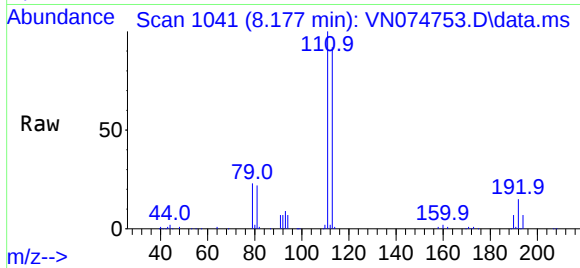

#36
1,1-Dichloropropene
Concen: 2.718 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.147 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 75 Resp: 23908
Ion Ratio Lower Upper
75 100
110 0.0 17.2 51.5#
77 0.8 24.3 36.5#


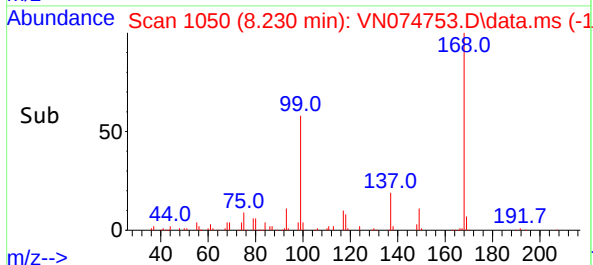
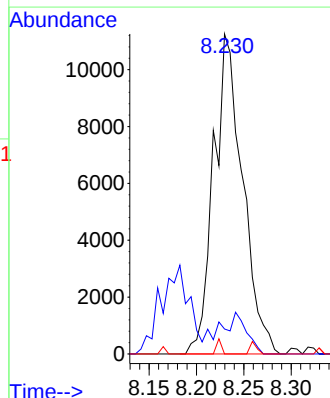
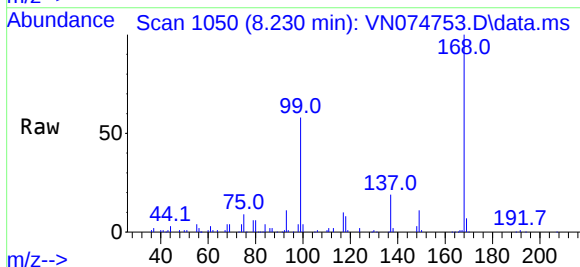




#37
Ethyl Acetate
Concen: 0.509 ug/l
RT: 7.518 min Scan# 91
Delta R.T. 0.017 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion: 43 Resp: 17973
Ion Ratio Lower Upper
43 100
61 0.0 4.3 6.5#
70 0.0 3.0 4.4#



#38
Carbon Tetrachloride
Concen: 3.763 ug/l
RT: 8.235 min Scan# 1051
Delta R.T. -0.135 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 117 Resp: 31214
Ion Ratio Lower Upper
117 100
119 1.1 74.3 111.5#
121 0.0 25.0 37.4#


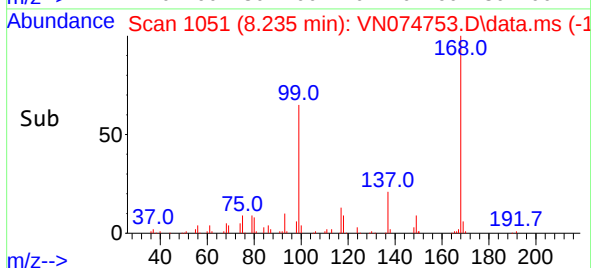
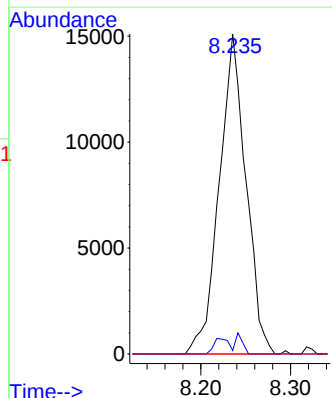





#40
Benzene
Concen: 0.287 ug/l
RT: 8.618 min Scan# 1115
Delta R.T. 0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion: 78 Resp: 8159
Ion Ratio Lower Upper
78 100
77 11.3 20.1 30.1#

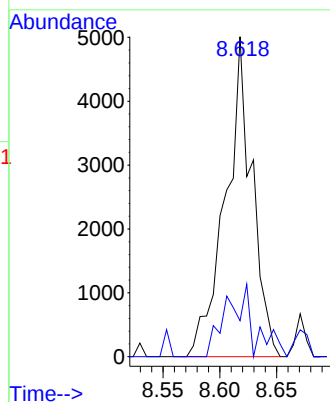

#42
1,2-Dichloroethane
Concen: 0.404 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. 0.017 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 62 Resp: 3608
Ion Ratio Lower Upper
62 100
98 9.0 0.0 19.4


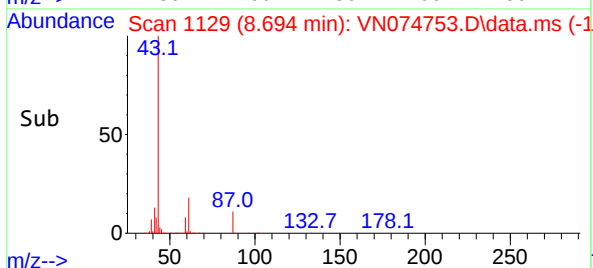






#43
Isopropyl Acetate
Concen: 25.911 ug/l
RT: 8.700 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument : MSVOA_N
ClientSampleId : SB-21


Tgt Ion: 43 Resp: 564895
Ion Ratio Lower Upper
43 100
61 18.7 19.4 29.0#
87 12.1 10.1 15.1

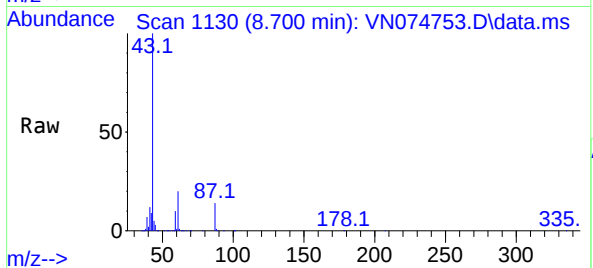

#48
Methyl methacrylate
Concen: 1.825 ug/l
RT: 9.677 min Scan# 1296
Delta R.T. 0.059 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 41 Resp: 16335
Ion Ratio Lower Upper
41 100
69 1.7 0.0 0.0#
39 55.6 54.4 81.6


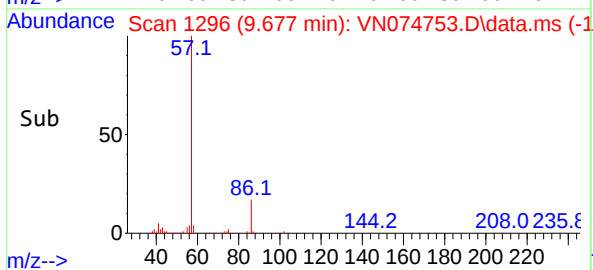






#49
 1,4-Dioxane
 Concen: 0.314 ug/l
 RT: 9.700 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: VN074753.D
 Acq: 05 Oct 2022 21:37




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-21


Tgt Ion:	88	Resp:	61
Ion	Ratio	Lower	Upper
88	100		
43	0.0	23.4	35.2#
58	0.0	54.9	82.3#

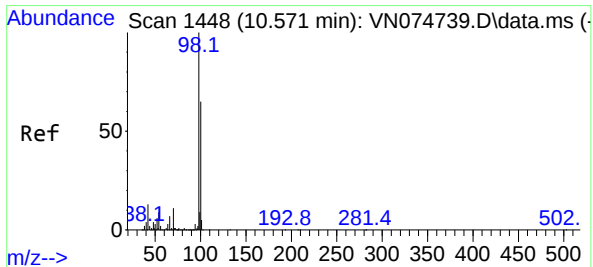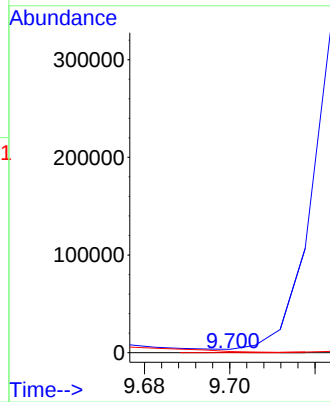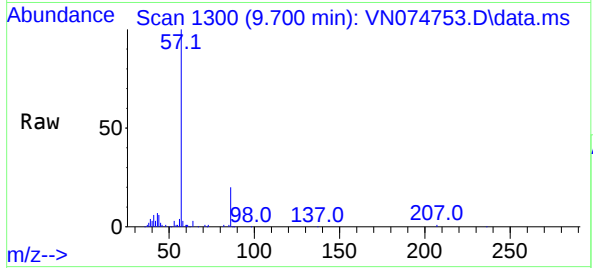

#50
 Toluene-d8
 Concen: 51.046 ug/l
 RT: 10.571 min Scan# 1448
 Delta R.T. -0.000 min
 Lab File: VN074753.D
 Acq: 05 Oct 2022 21:37

Tgt Ion:	98	Resp:	1190212
Ion	Ratio	Lower	Upper
98	100		
100	63.4	50.7	76.1


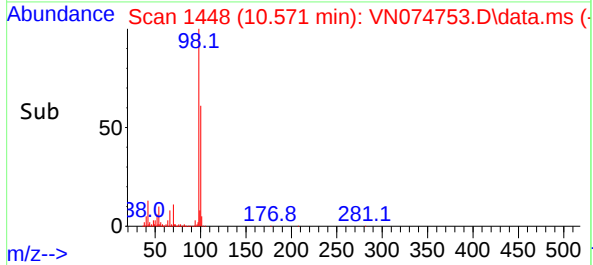

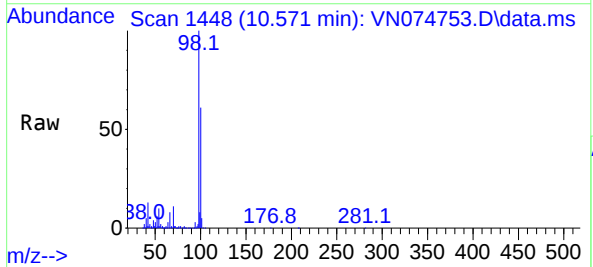




#51
4-Methyl-2-Pentanone
Concen: 2.374 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. -0.000 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion: 43 Resp: 33325
Ion Ratio Lower Upper
43 100
58 38.1 30.6 45.8

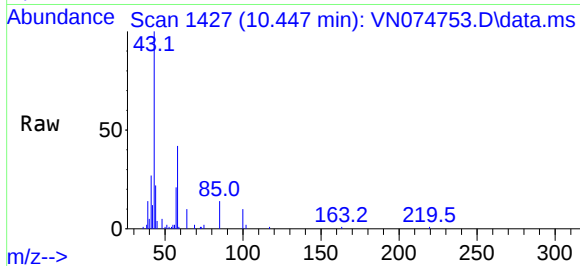

#52
Toluene
Concen: 0.439 ug/l
RT: 10.629 min Scan# 1458
Delta R.T. -0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 92 Resp: 7506
Ion Ratio Lower Upper
92 100
91 186.7 140.2 210.4


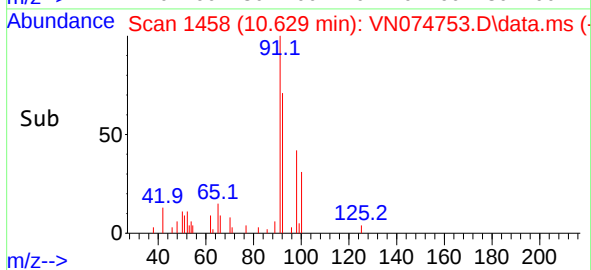

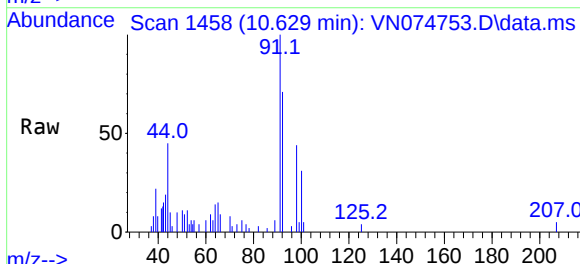


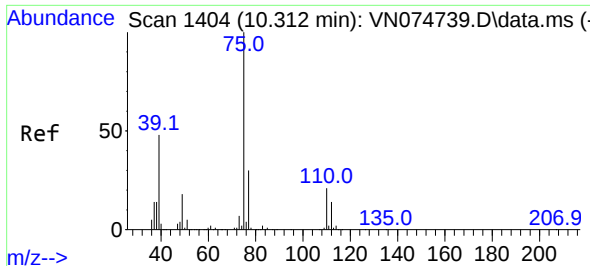

#54
 cis-1,3-Dichloropropene
 Concen: 14.754 ug/l
 RT: 10.365 min Scan# 1413
 Delta R.T. 0.053 min
 Lab File: VN074753.D
 Acq: 05 Oct 2022 21:37




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-21


Tgt Ion: 75 Resp: 175423
 Ion Ratio Lower Upper
 75 100
 77 0.7 24.4 36.6#
 39 29.7 38.6 57.8#

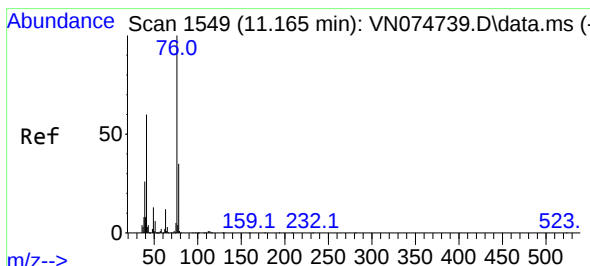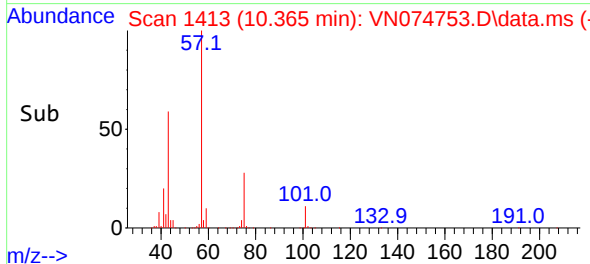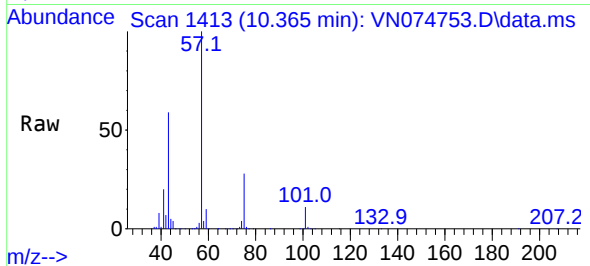

#57
 1,3-Dichloropropane
 Concen: 1.957 ug/l
 RT: 11.206 min Scan# 1556
 Delta R.T. 0.041 min
 Lab File: VN074753.D
 Acq: 05 Oct 2022 21:37

Tgt Ion: 76 Resp: 24259
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.2 39.2#


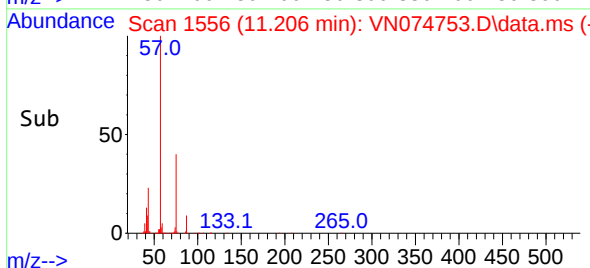
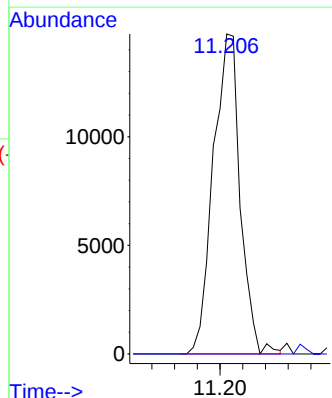
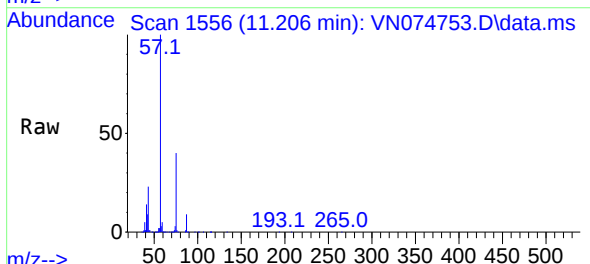




#59
2-Hexanone
Concen: 27.382 ug/l
RT: 11.206 min Scan# 1555
Delta R.T. 0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion: 43 Resp: 290777
Ion Ratio Lower Upper
43 100
58 22.6 27.3 81.9#

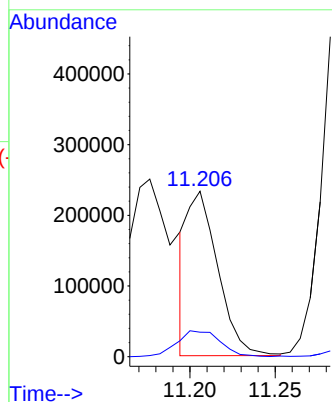

#62
4-Bromofluorobenzene
Concen: 45.128 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 95 Resp: 319857
Ion Ratio Lower Upper
95 100
174 76.1 0.0 149.4
176 71.7 0.0 142.0


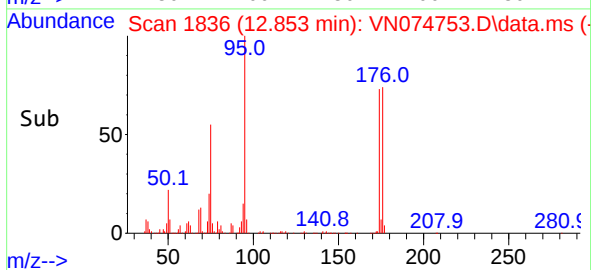






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion:117 Resp: 565341
Ion Ratio Lower Upper
117 100
82 57.8 45.4 68.2
119 28.9 25.1 37.7

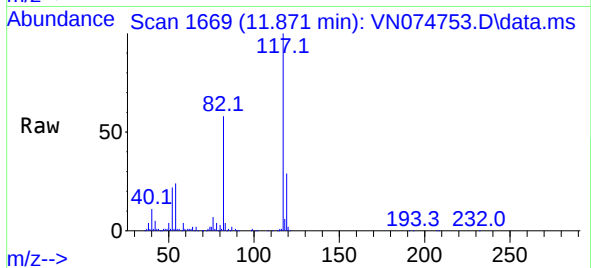

#68
m/p-Xylenes
Concen: 0.296 ug/l
RT: 12.070 min Scan# 1703
Delta R.T. -0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion:106 Resp: 3590
Ion Ratio Lower Upper
106 100
91 224.0 164.2 246.4


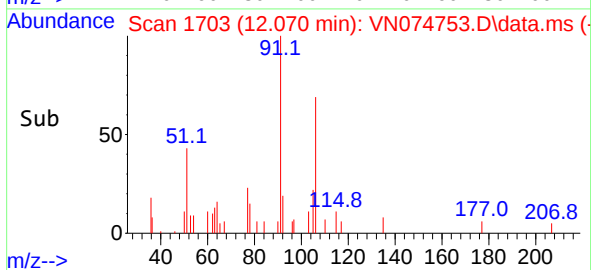






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 1996
Delta R.T. 0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion:152 Resp: 266808
Ion Ratio Lower Upper
152 100
115 60.1 30.0 90.0
150 159.7 0.0 356.4



#74
N-ethyl acetate
Concen: 0.242 ug/l
RT: 12.482 min Scan# 1773
Delta R.T. -0.012 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 43 Resp: 3751
Ion Ratio Lower Upper
43 100
70 7.3 32.9 49.3#
55 17.4 17.8 26.6#
61 0.0 18.9 28.3#


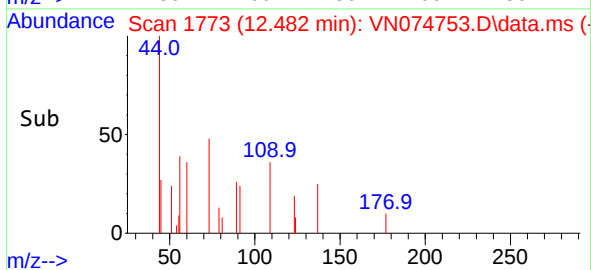






#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.935 min Scan# 1835
Delta R.T. -0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion: 83 Resp: 70
Ion Ratio Lower Upper
83 100
131 0.0 4.3 12.8#
85 0.0 32.9 98.6#

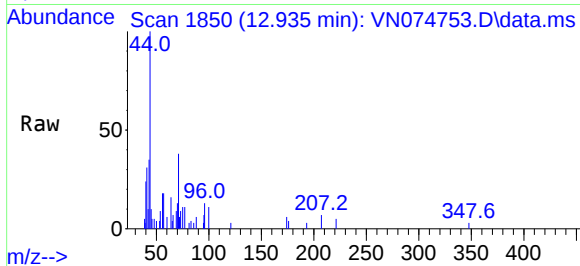

#76
1,2,3-Trichloropropane
Concen: 23.079 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion: 75 Resp: 183792
Ion Ratio Lower Upper
75 100
77 1.3 76.9 230.7#


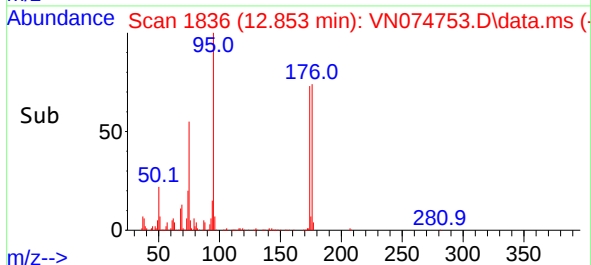
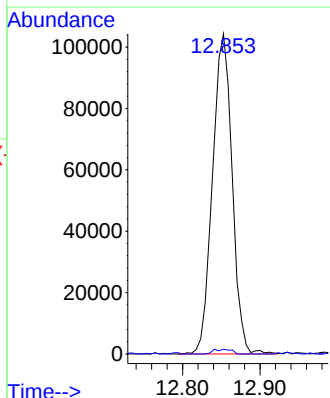
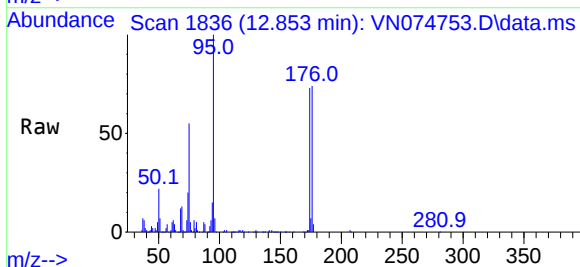




#81
trans-1,4-Dichloro-2-butene
Concen: 44.967 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.117 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37




Instrument :
MSVOA_N
ClientSampleId :
SB-21


Tgt Ion: 75 Resp: 183792
Ion Ratio Lower Upper
75 100
53 0.4 71.4 107.0#
89 0.2 32.1 48.1#



#95
Naphthalene
Concen: 1.252 ug/l
RT: 15.647 min Scan# 2311
Delta R.T. 0.006 min
Lab File: VN074753.D
Acq: 05 Oct 2022 21:37

Tgt Ion:128 Resp: 23209
Ion Ratio Lower Upper
128 100
127 12.6 10.2 15.2
129 6.9 9.0 13.4#

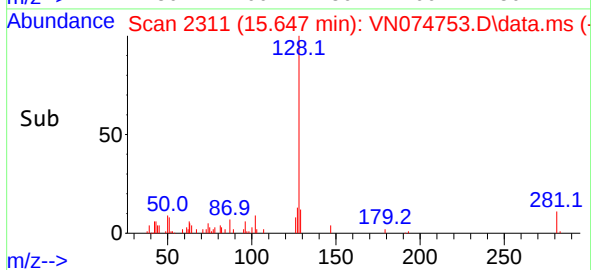



#96
 1,2,3-Trichlorobenzene
 Concen: Below Cal
 RT: 15.835 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN074753.D
 Acq: 05 Oct 2022 21:37

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-21

Tgt Ion:180 Resp: 463
 Ion Ratio Lower Upper
 180 100
 182 83.2 47.3 142.0
 145 13.2 17.1 51.2#

