

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100522\
 Data File : VN074755.D
 Acq On : 05 Oct 2022 22:25
 Operator : JC\MD
 Sample : N4957-07
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-23

Quant Time: Oct 06 07:44:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 05:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	274363	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	522727	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	558112	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	269872	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	352840	54.276	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 108.560%			
35) Dibromofluoromethane	8.177	113	268201	50.782	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.560%			
50) Toluene-d8	10.571	98	1176061	51.896	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 103.800%			
62) 4-Bromofluorobenzene	12.853	95	313890	45.565	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 91.120%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.512	59	4304	1.977	ug/l #	86
13) Acrolein	4.200	56	893	Below Cal		84
16) Acetone	4.465	43	133903	36.347	ug/l	93
18) Methyl Acetate	5.065	43	29667	2.175	ug/l	93
20) Methylene Chloride	5.306	84	28833	2.825	ug/l #	87
25) 2-Butanone	7.506	43	18657	2.790	ug/l #	89
29) Tetrahydrofuran	7.871	42	7586	1.628	ug/l #	62
31) Cyclohexane	8.235	56	8071	0.718	ug/l #	54
36) 1,1-Dichloropropene	8.235	75	25374	2.968	ug/l #	51
37) Ethyl Acetate	7.506	43	18657	0.544	ug/l #	86
38) Carbon Tetrachloride	8.241	117	30167	3.742	ug/l #	15
40) Benzene	8.618	78	8320	0.301	ug/l #	69
43) Isopropyl Acetate	8.700	43	557408	26.306	ug/l #	93
48) Methyl methacrylate	9.676	41	15502	1.782	ug/l #	89
49) 1,4-Dioxane	9.735	88	380	2.015	ug/l #	24
51) 4-Methyl-2-Pentanone	10.453	43	50769	3.721	ug/l #	80
52) Toluene	10.629	92	6003	0.361	ug/l	97
54) cis-1,3-Dichloropropene	10.359	75	167602	14.503	ug/l #	62
57) 1,3-Dichloropropane	11.206	76	19618	1.628	ug/l #	42
59) 2-Hexanone	11.170	43	465842	45.135	ug/l #	24
68) m/p-Xylenes	12.070	106	3326	0.278	ug/l	84
71) Bromoform	12.847	173	2928	0.615	ug/l #	1
74) N-amyl acetate	12.488	43	7833	0.499	ug/l #	58
75) 1,1,2,2-Tetrachloroethane	12.912	83	195	Below Cal	#	24
76) 1,2,3-Trichloropropane	12.853	75	182293	22.631	ug/l #	1
77) Bromobenzene	12.917	156	64	Below Cal	#	58
81) trans-1,4-Dichloro-2-b...	12.853	75	182293	44.094	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	14.706	75	935	0.434	ug/l #	7
95) Naphthalene	15.653	128	22429	1.196	ug/l #	91
96) 1,2,3-Trichlorobenzene	15.835	180	238	Below Cal	#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100522\
Data File : VN074755.D
Acq On : 05 Oct 2022 22:25
Operator : JC\MD
Sample : N4957-07
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-23

Quant Time: Oct 06 07:44:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 05:37:50 2022
Response via : Initial Calibration




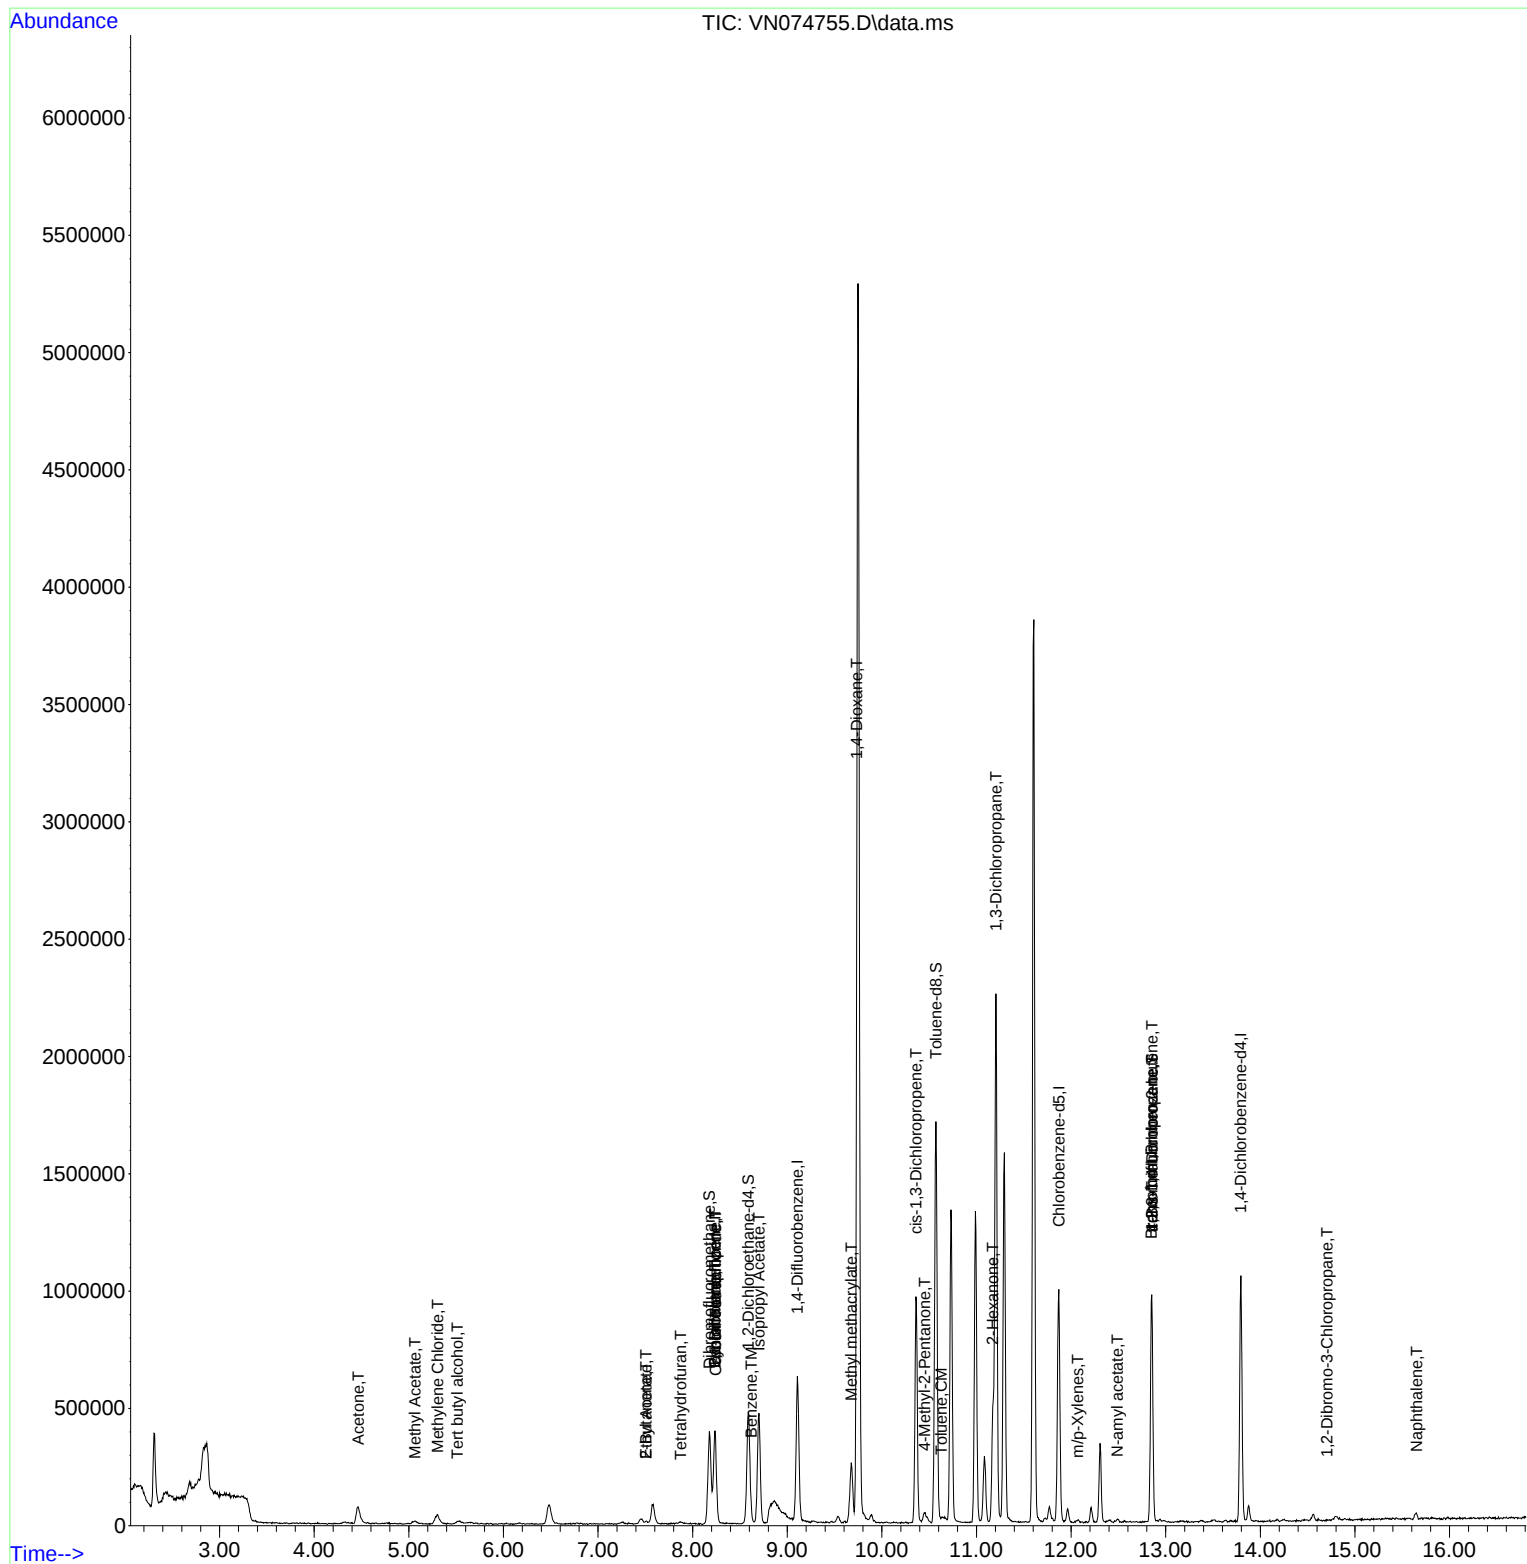




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1
Delta R.T. -0.001 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion:168 Resp: 274363
Ion Ratio Lower Upper
168 100
99 55.6 42.8 64.2

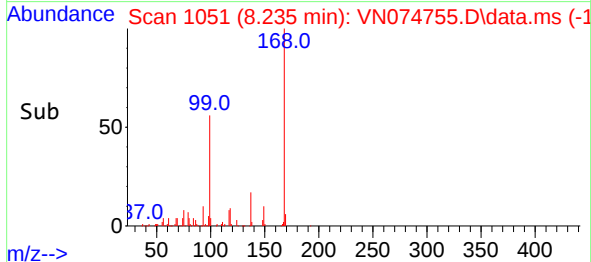

#11
Tert butyl alcohol
Concen: 1.977 ug/l
RT: 5.512 min Scan# 588
Delta R.T. -0.047 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 59 Resp: 4304
Ion Ratio Lower Upper
59 100
57 4.6 7.7 11.5#


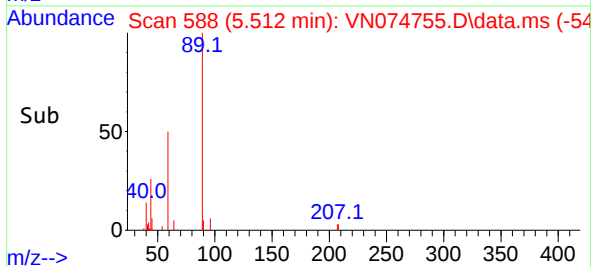

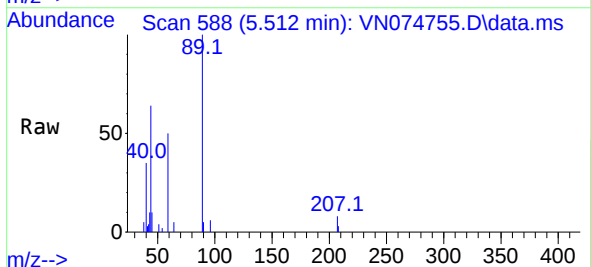




#13
Acrolein
Concen: Below Cal
RT: 4.200 min Scan# 301
Delta R.T. -0.001 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 56 Resp: 893
Ion Ratio Lower Upper
56 100
55 55.8 54.9 82.3

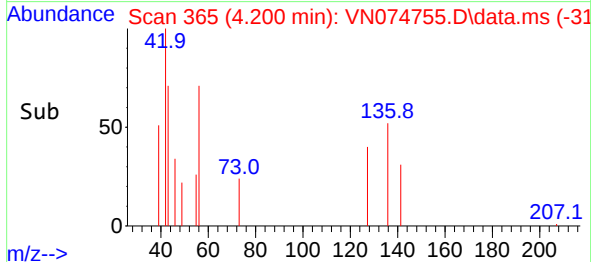

#16
Acetone
Concen: 36.347 ug/l
RT: 4.465 min Scan# 410
Delta R.T. 0.006 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 43 Resp: 133903
Ion Ratio Lower Upper
43 100
58 35.1 24.9 37.3


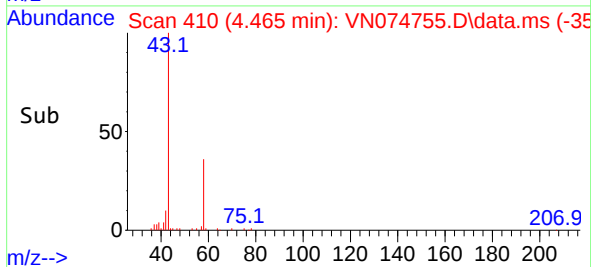

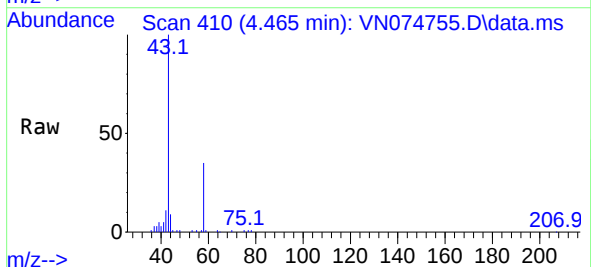




#18
Methyl Acetate
Concen: 2.175 ug/l
RT: 5.065 min Scan# 512
Delta R.T. 0.017 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 43 Resp: 29667
Ion Ratio Lower Upper
43 100
74 19.9 18.5 27.7

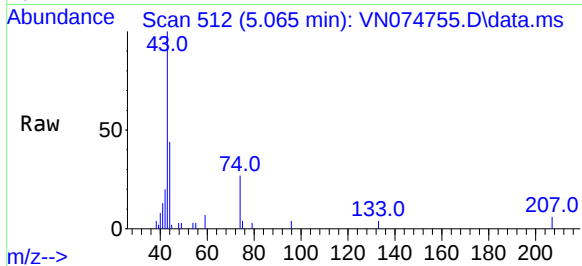

#20
Methylene Chloride
Concen: 2.825 ug/l
RT: 5.306 min Scan# 553
Delta R.T. 0.011 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 84 Resp: 28833
Ion Ratio Lower Upper
84 100
49 120.8 107.4 161.0
51 50.5 35.1 52.7
86 49.0 50.4 75.6#


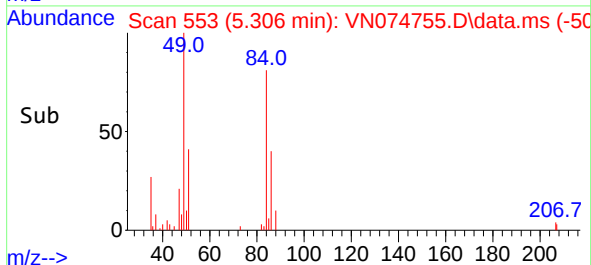
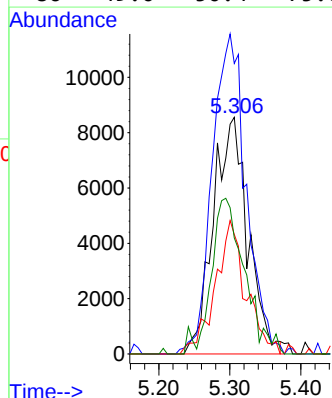
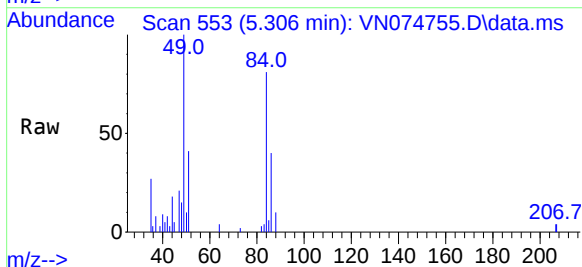




#25
2-Butanone
Concen: 2.790 ug/l
RT: 7.506 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 43 Resp: 18657
Ion Ratio Lower Upper
43 100
72 21.2 21.4 32.0#

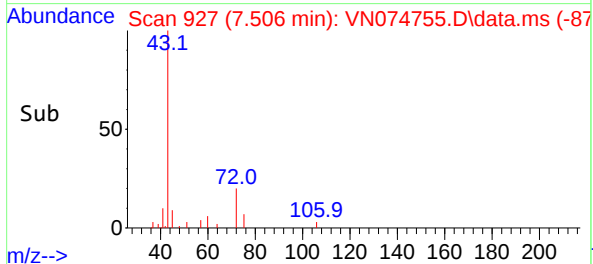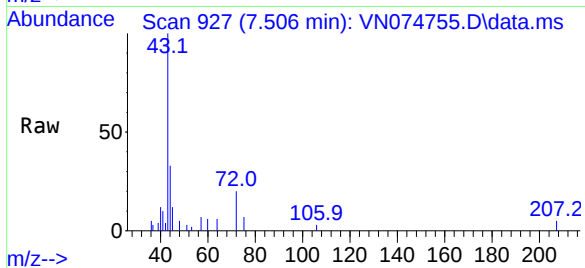

#29
Tetrahydrofuran
Concen: 1.628 ug/l
RT: 7.871 min Scan# 989
Delta R.T. 0.017 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 42 Resp: 7586
Ion Ratio Lower Upper
42 100
72 14.9 33.0 49.6#
71 17.4 30.4 45.6#


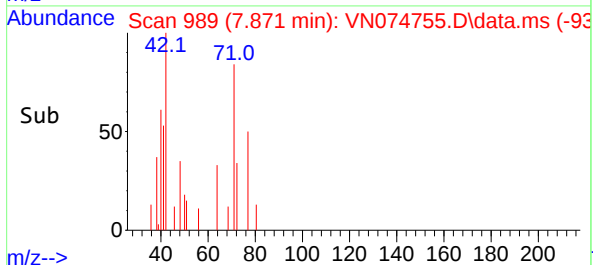
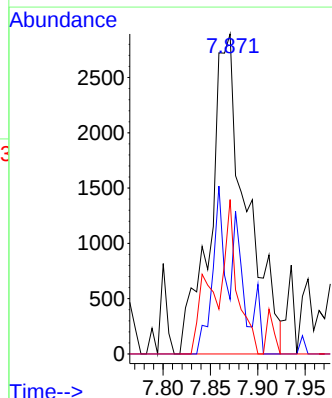
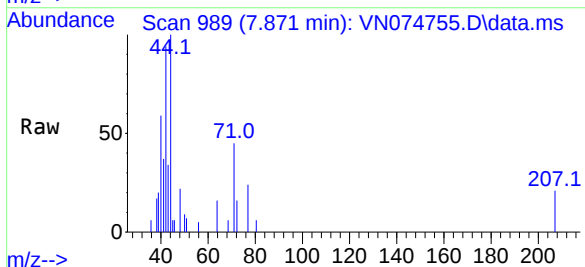




#31
Cyclohexane
Concen: 0.718 ug/l
RT: 8.235 min Scan# 1051
Delta R.T. -0.030 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 56 Resp: 8071
Ion Ratio Lower Upper
56 100
69 100.8 23.1 34.7#
84 97.5 67.1 100.7

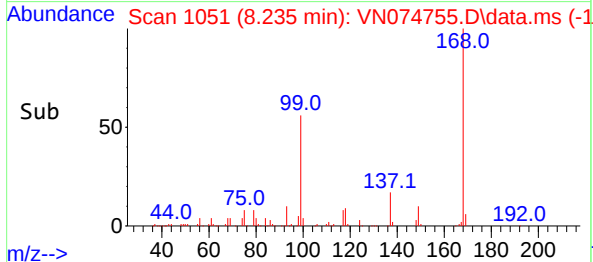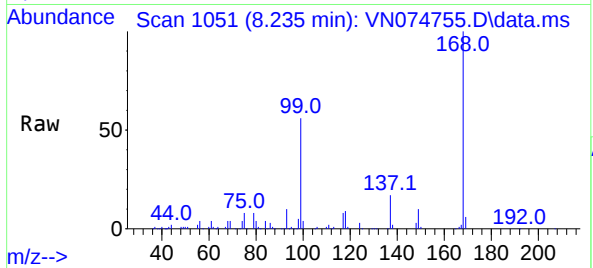

#33
1,2-Dichloroethane-d4
Concen: 54.276 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. -0.000 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 65 Resp: 352840
Ion Ratio Lower Upper
65 100
67 55.1 0.0 109.0

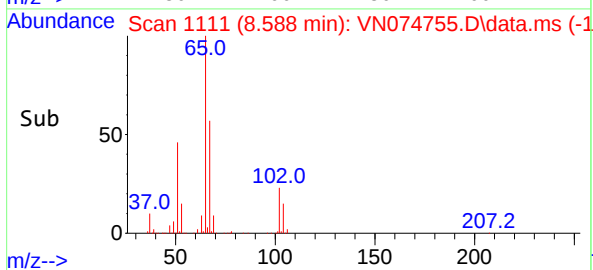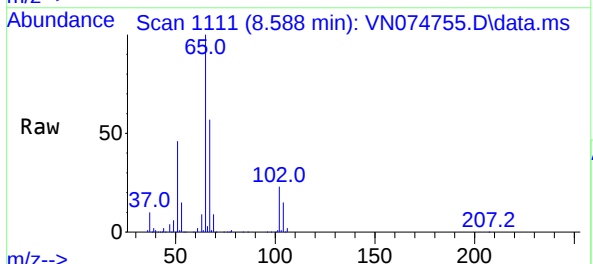



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN074755.D

Acq: 05 Oct 2022 22:25

Instrument :

MSVOA_N

ClientSampleId :

SB-23





Tgt Ion:114 Resp: 522727

Ion Ratio Lower Upper

114 100

63 22.1 0.0 41.2

88 16.2 0.0 30.2

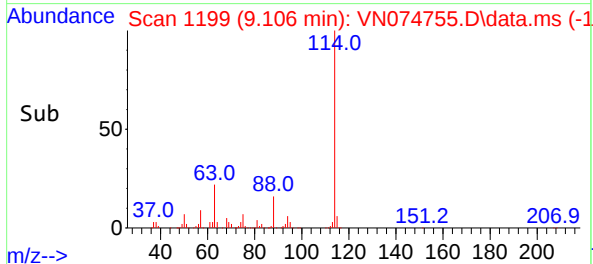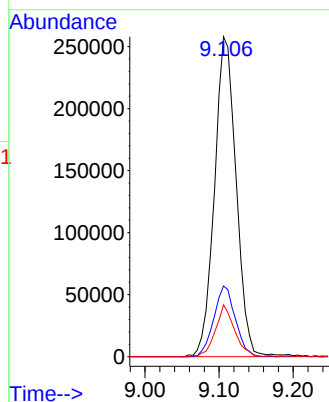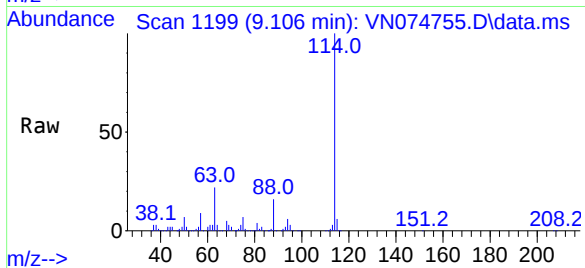

#35

Dibromofluoromethane

Concen: 50.782 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN074755.D

Acq: 05 Oct 2022 22:25




Tgt Ion:113 Resp: 268201


Ion Ratio Lower Upper

113 100

111 104.8 83.0 124.6

192 16.4 12.6 18.8

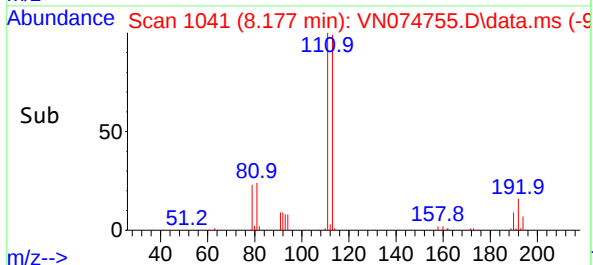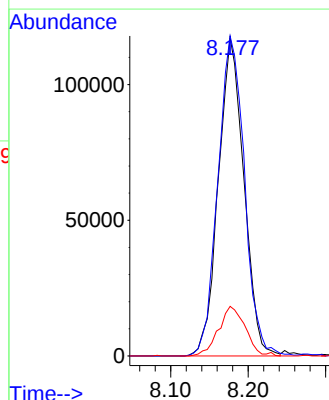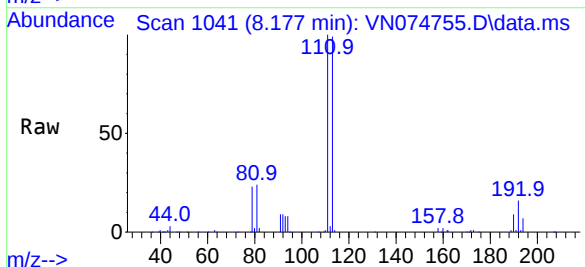



#36

1,1-Dichloropropene

Concen: 2.968 ug/l

RT: 8.235 min Scan# 1

Delta R.T. -0.141 min

Lab File: VN074755.D

Acq: 05 Oct 2022 22:25

Instrument :

MSVOA_N

ClientSampleId :

SB-23





Tgt Ion: 75 Resp: 25374

Ion Ratio Lower Upper

75 100

110 9.8 17.2 51.5#

77 0.0 24.3 36.5#

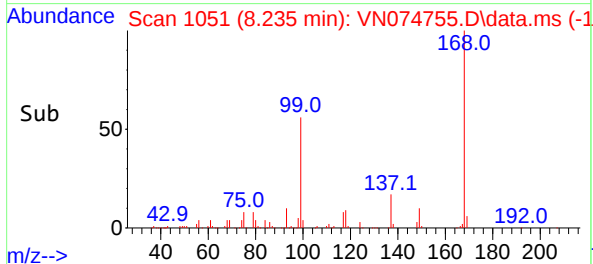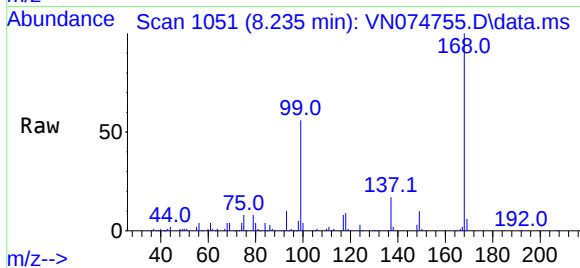

#37

Ethyl Acetate

Concen: 0.544 ug/l

RT: 7.506 min Scan# 927

Delta R.T. 0.006 min

Lab File: VN074755.D

Acq: 05 Oct 2022 22:25




Tgt Ion: 43 Resp: 18657


Ion Ratio Lower Upper

43 100

61 0.0 4.3 6.5#

70 0.0 3.0 4.4#


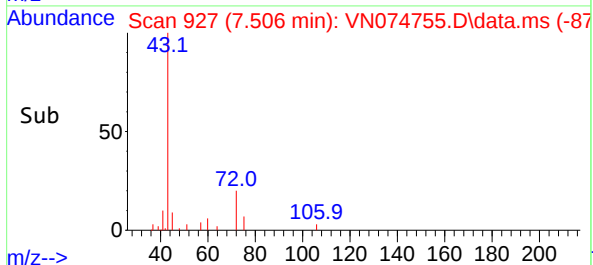
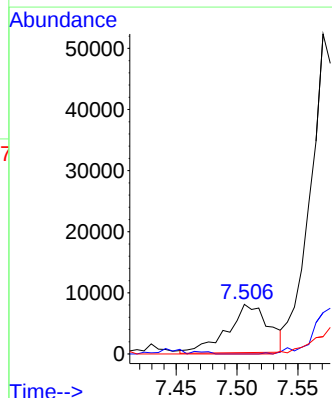
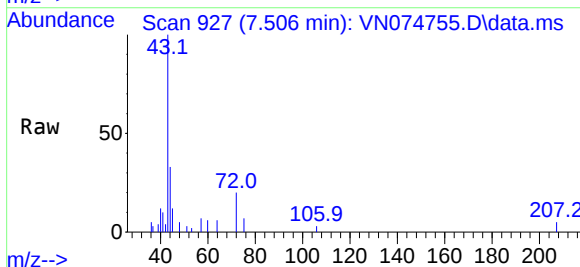




#38
Carbon Tetrachloride
Concen: 3.742 ug/l
RT: 8.241 min Scan# 1105
Delta R.T. -0.130 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion:117 Resp: 30167
Ion Ratio Lower Upper
117 100
119 2.3 74.3 111.5#
121 0.0 25.0 37.4#

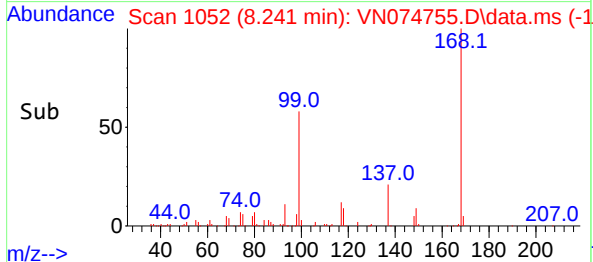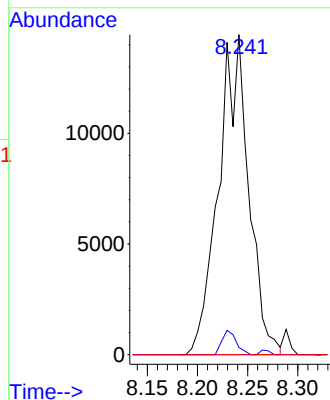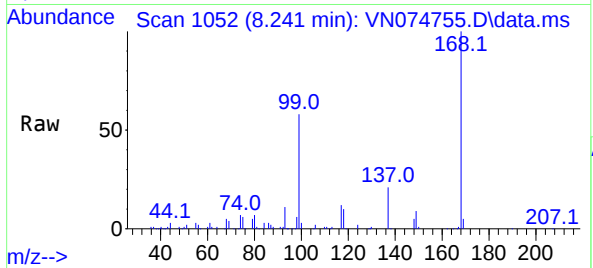

#40
Benzene
Concen: 0.301 ug/l
RT: 8.618 min Scan# 1116
Delta R.T. 0.006 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 78 Resp: 8320
Ion Ratio Lower Upper
78 100
77 9.4 20.1 30.1#


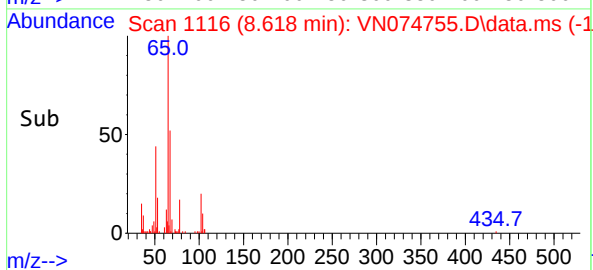
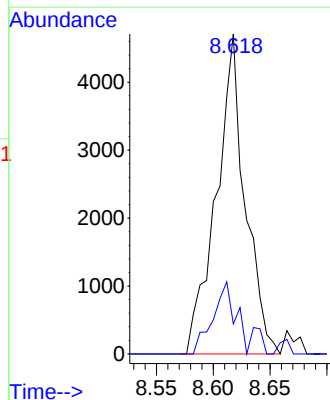
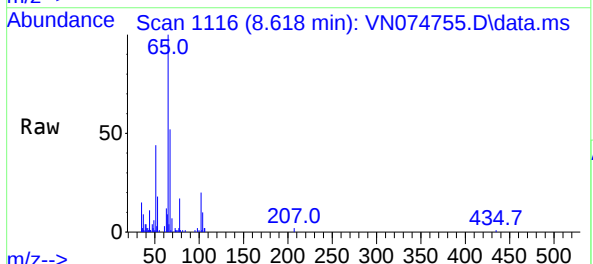




#43
Isopropyl Acetate
Concen: 26.306 ug/l
RT: 8.700 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 43 Resp: 557408
Ion Ratio Lower Upper
43 100
61 19.0 19.4 29.0#
87 12.3 10.1 15.1

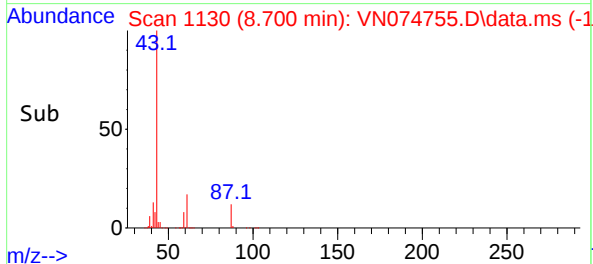

#48
Methyl methacrylate
Concen: 1.782 ug/l
RT: 9.676 min Scan# 1296
Delta R.T. 0.059 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 41 Resp: 15502
Ion Ratio Lower Upper
41 100
69 3.4 0.0 0.0#
39 59.5 54.4 81.6


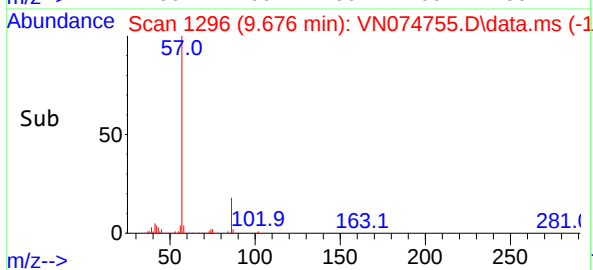

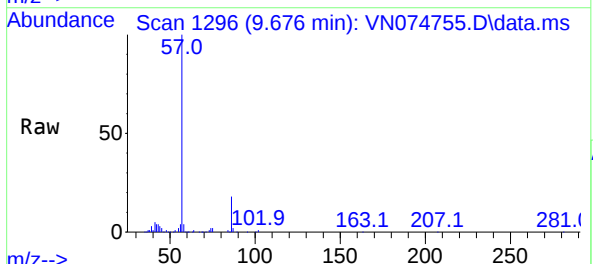


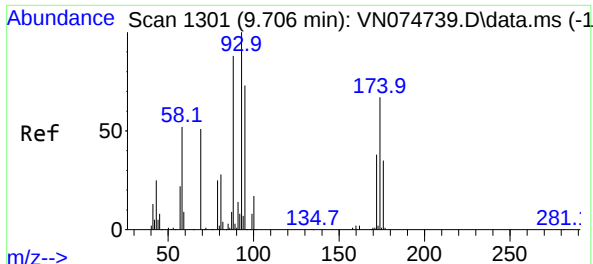

#49
1,4-Dioxane
Concen: 2.015 ug/l
RT: 9.735 min Scan# 11
Delta R.T. 0.029 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 88 Resp: 380
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 0.0 54.9 82.3#

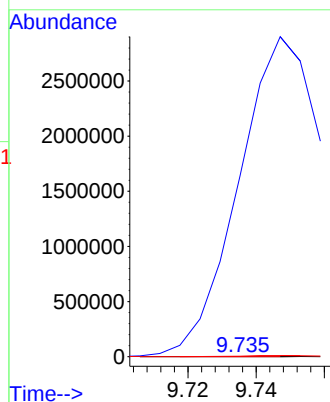

#50
Toluene-d8
Concen: 51.896 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 98 Resp: 1176061
Ion Ratio Lower Upper
98 100
100 63.6 50.7 76.1


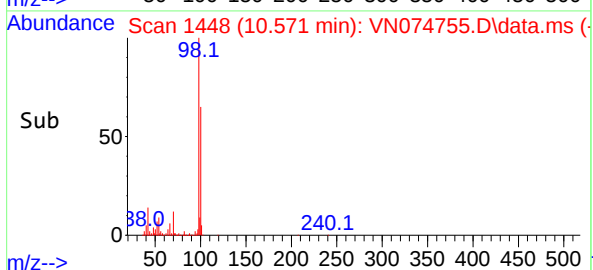
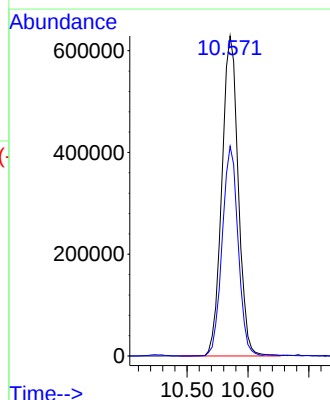
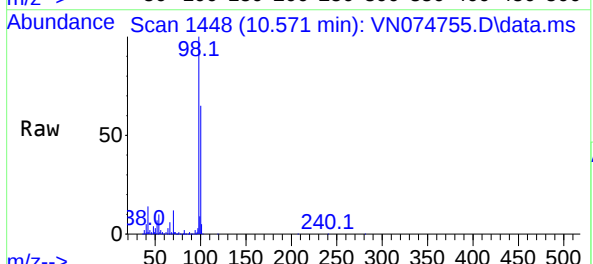




#51
4-Methyl-2-Pentanone
Concen: 3.721 ug/l
RT: 10.453 min Scan# 1427
Delta R.T. 0.006 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 43 Resp: 50769
Ion Ratio Lower Upper
43 100
58 26.0 30.6 45.8#

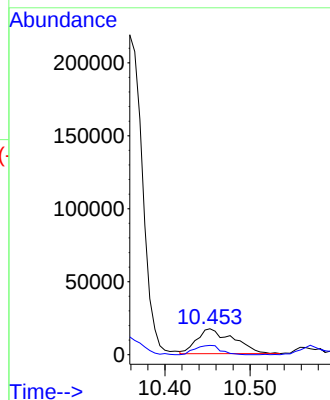

#52
Toluene
Concen: 0.361 ug/l
RT: 10.629 min Scan# 1458
Delta R.T. -0.006 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 92 Resp: 6003
Ion Ratio Lower Upper
92 100
91 170.5 140.2 210.4



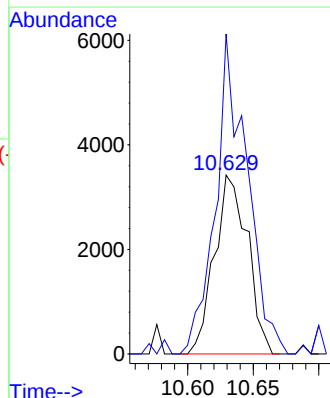





#54
 cis-1,3-Dichloropropene
 Concen: 14.503 ug/l
 RT: 10.359 min Scan# 1412
 Delta R.T. 0.047 min
 Lab File: VN074755.D
 Acq: 05 Oct 2022 22:25




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-23


Tgt Ion: 75 Resp: 167602
 Ion Ratio Lower Upper
 75 100
 77 0.2 24.4 36.6#
 39 29.8 38.6 57.8#



#57
 1,3-Dichloropropane
 Concen: 1.628 ug/l
 RT: 11.206 min Scan# 1556
 Delta R.T. 0.041 min
 Lab File: VN074755.D
 Acq: 05 Oct 2022 22:25

Tgt Ion: 76 Resp: 19618
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.2 39.2#


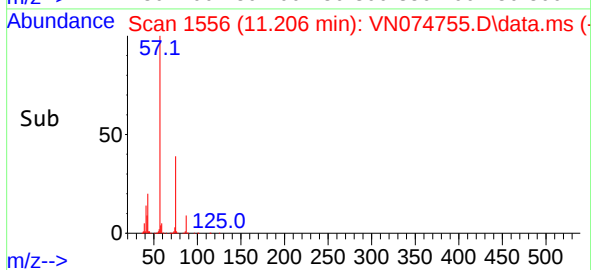






#59
2-Hexanone
Concen: 45.135 ug/l
RT: 11.170 min Scan# 1150
Delta R.T. -0.030 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 43 Resp: 465842
Ion Ratio Lower Upper
43 100
58 0.0 27.3 81.9#



#62
4-Bromofluorobenzene
Concen: 45.565 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 95 Resp: 313890
Ion Ratio Lower Upper
95 100
174 76.4 0.0 149.4
176 73.6 0.0 142.0


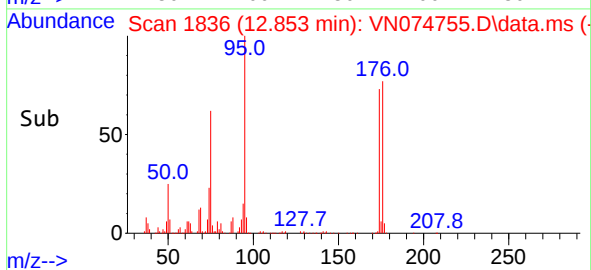






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion:117 Resp: 558112
Ion Ratio Lower Upper
117 100
82 56.1 45.4 68.2
119 31.4 25.1 37.7

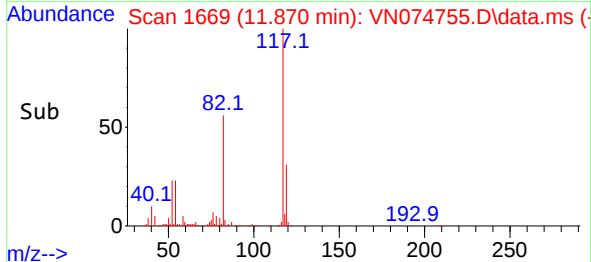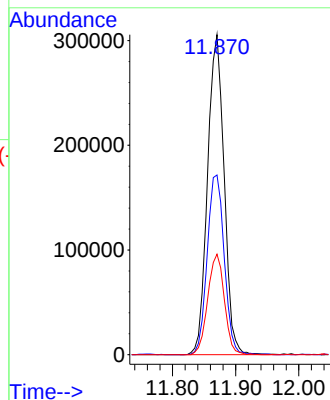

#68
m/p-Xylenes
Concen: 0.278 ug/l
RT: 12.070 min Scan# 1703
Delta R.T. -0.006 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion:106 Resp: 3326
Ion Ratio Lower Upper
106 100
91 180.4 164.2 246.4


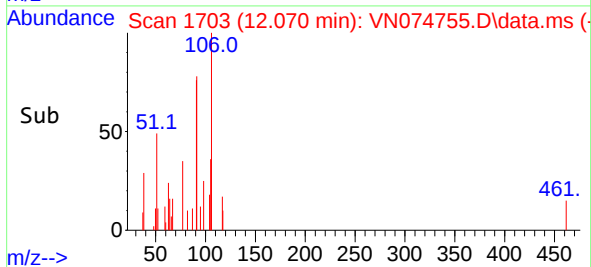
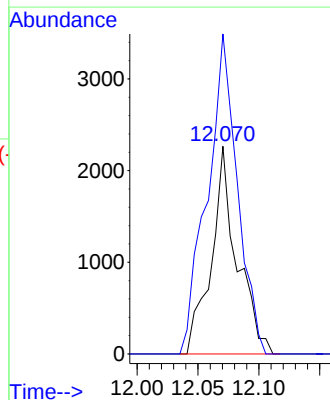
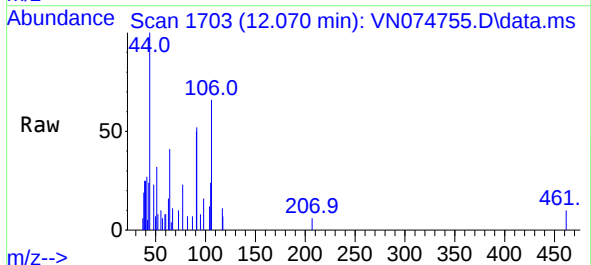




#71
Bromoform
Concen: 0.615 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.264 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion:173 Resp: 2928
Ion Ratio Lower Upper
173 100
175 536.7 23.9 71.7#
254 0.0 0.1 0.1#



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion:152 Resp: 269872
Ion Ratio Lower Upper
152 100
115 60.6 30.0 90.0
150 158.3 0.0 356.4


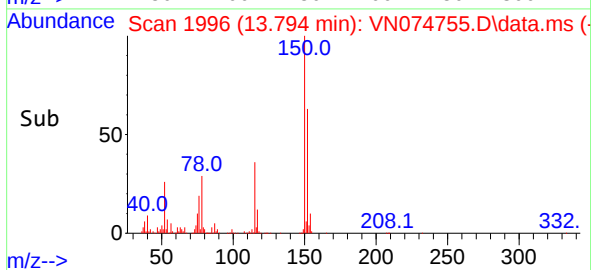






#74
N-amy1 acetate
Concen: 0.499 ug/l
RT: 12.488 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 43 Resp: 7833
Ion Ratio Lower Upper
43 100
70 3.8 32.9 49.3#
55 23.6 17.8 26.6
61 0.0 18.9 28.3#



#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.912 min Scan# 1846
Delta R.T. -0.029 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 83 Resp: 195
Ion Ratio Lower Upper
83 100
131 0.0 4.3 12.8#
85 0.0 32.9 98.6#


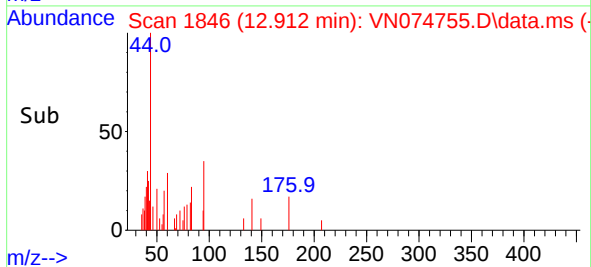

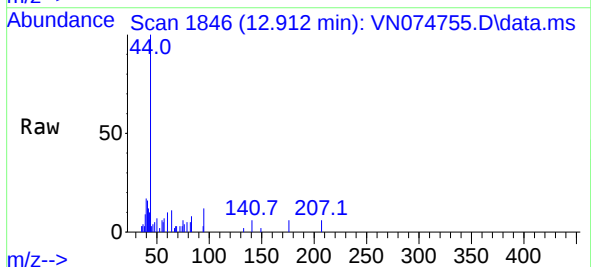




#76
1,2,3-Trichloropropane
Concen: 22.631 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25




Instrument :
MSVOA_N
ClientSampleId :
SB-23


Tgt Ion: 75 Resp: 182293
Ion Ratio Lower Upper
75 100
77 1.6 76.9 230.7#



#77
Bromobenzene
Concen: Below Cal
RT: 12.917 min Scan# 1847
Delta R.T. -0.065 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion: 156 Resp: 64
Ion Ratio Lower Upper
156 100
77 284.4 124.7 374.1
158 0.0 48.3 144.9#


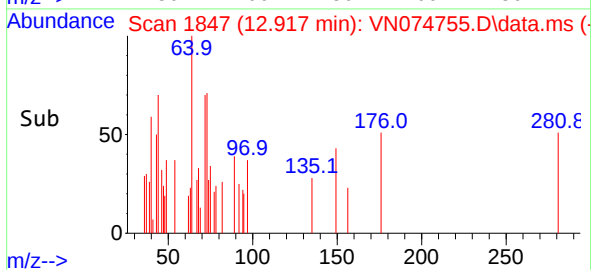






#81
 trans-1,4-Dichloro-2-butene
 Concen: 44.094 ug/l
 RT: 12.853 min Scan# 11
 Delta R.T. 0.117 min
 Lab File: VN074755.D
 Acq: 05 Oct 2022 22:25




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-23


Tgt Ion: 75 Resp: 182293
 Ion Ratio Lower Upper
 75 100
 53 0.1 71.4 107.0#
 89 0.0 32.1 48.1#



#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.434 ug/l
 RT: 14.706 min Scan# 2151
 Delta R.T. -0.017 min
 Lab File: VN074755.D
 Acq: 05 Oct 2022 22:25

Tgt Ion: 75 Resp: 935
 Ion Ratio Lower Upper
 75 100
 155 0.0 40.3 120.8#
 157 6.8 51.3 153.9#



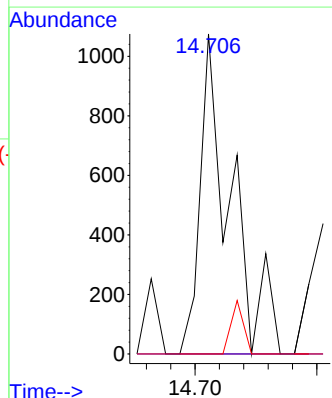





#95
Naphthalene
Concen: 1.196 ug/l
RT: 15.653 min Scan# 21
Delta R.T. 0.012 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Instrument :
MSVOA_N
ClientSampleId :
SB-23

Tgt Ion:128 Resp: 22429
Ion Ratio Lower Upper
128 100
127 16.4 10.2 15.2#
129 14.1 9.0 13.4#

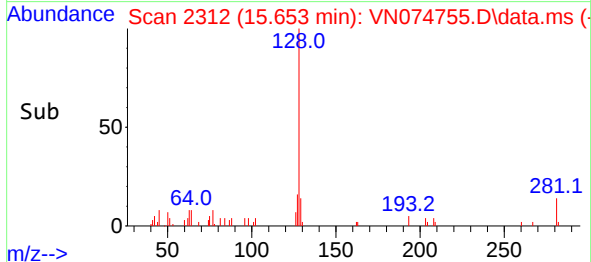

#96
1,2,3-Trichlorobenzene
Concen: Below Cal
RT: 15.835 min Scan# 2343
Delta R.T. -0.006 min
Lab File: VN074755.D
Acq: 05 Oct 2022 22:25

Tgt Ion:180 Resp: 238
Ion Ratio Lower Upper
180 100
182 129.0 47.3 142.0
145 0.0 17.1 51.2#

