

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100522\
 Data File : VN074758.D
 Acq On : 05 Oct 2022 23:38
 Operator : JC\MD
 Sample : N4957-10
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-26

Quant Time: Oct 06 07:45:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 05:37:50 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.236	168	269035	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	513809	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	540821	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	254995	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.589	65	346874	54.415	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 108.840%	
35) Dibromofluoromethane	8.177	113	274460	52.869	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 105.740%	
50) Toluene-d8	10.571	98	1164097	52.260	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 104.520%	
62) 4-Bromofluorobenzene	12.847	95	307053	45.346	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 90.700%	
Target Compounds						
					Qvalue	
6) Chloroethane	3.242	64	69963	9.308	ug/l #	49
11) Tert butyl alcohol	5.536	59	4380	2.052	ug/l #	79
13) Acrolein	4.212	56	436	Below Cal	#	1
16) Acetone	4.465	43	131464	36.392	ug/l	96
18) Methyl Acetate	5.053	43	23809	1.780	ug/l #	90
20) Methylene Chloride	5.289	84	28122	2.797	ug/l #	79
25) 2-Butanone	7.512	43	13682	2.087	ug/l #	70
29) Tetrahydrofuran	7.859	42	8213	1.797	ug/l	93
31) Cyclohexane	8.230	56	7851	0.713	ug/l #	10
36) 1,1-Dichloropropene	8.236	75	26044	3.100	ug/l #	49
37) Ethyl Acetate	7.512	43	13682	0.406	ug/l #	86
38) Carbon Tetrachloride	8.241	117	29003	3.660	ug/l #	15
42) 1,2-Dichloroethane	8.689	62	3567	0.418	ug/l	98
43) Isopropyl Acetate	8.700	43	541775	26.012	ug/l #	92
48) Methyl methacrylate	9.683	41	17631	2.062	ug/l #	16
49) 1,4-Dioxane	9.736	88	414	2.234	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	26978	2.011	ug/l	93
52) Toluene	10.635	92	3786	0.232	ug/l	94
53) t-1,3-Dichloropropene	10.730	75	3913	0.372	ug/l	97
54) cis-1,3-Dichloropropene	10.359	75	172325	15.171	ug/l #	62
57) 1,3-Dichloropropane	11.206	76	24533	2.072	ug/l #	42
59) 2-Hexanone	11.177	43	480209	47.335	ug/l #	24
74) N-amyl acetate	12.477	43	7148	0.482	ug/l #	55
75) 1,1,2,2-Tetrachloroethane	12.859	83	185	Below Cal	#	19
76) 1,2,3-Trichloropropane	12.847	75	177317	23.298	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	177317	45.393	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	14.723	75	419	0.206	ug/l #	3
95) Naphthalene	15.635	128	9623	0.543	ug/l #	78
96) 1,2,3-Trichlorobenzene	15.859	180	191	Below Cal	#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100522\
Data File : VN074758.D
Acq On : 05 Oct 2022 23:38
Operator : JC\MD
Sample : N4957-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-26

Quant Time: Oct 06 07:45:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 05:37:50 2022
Response via : Initial Calibration




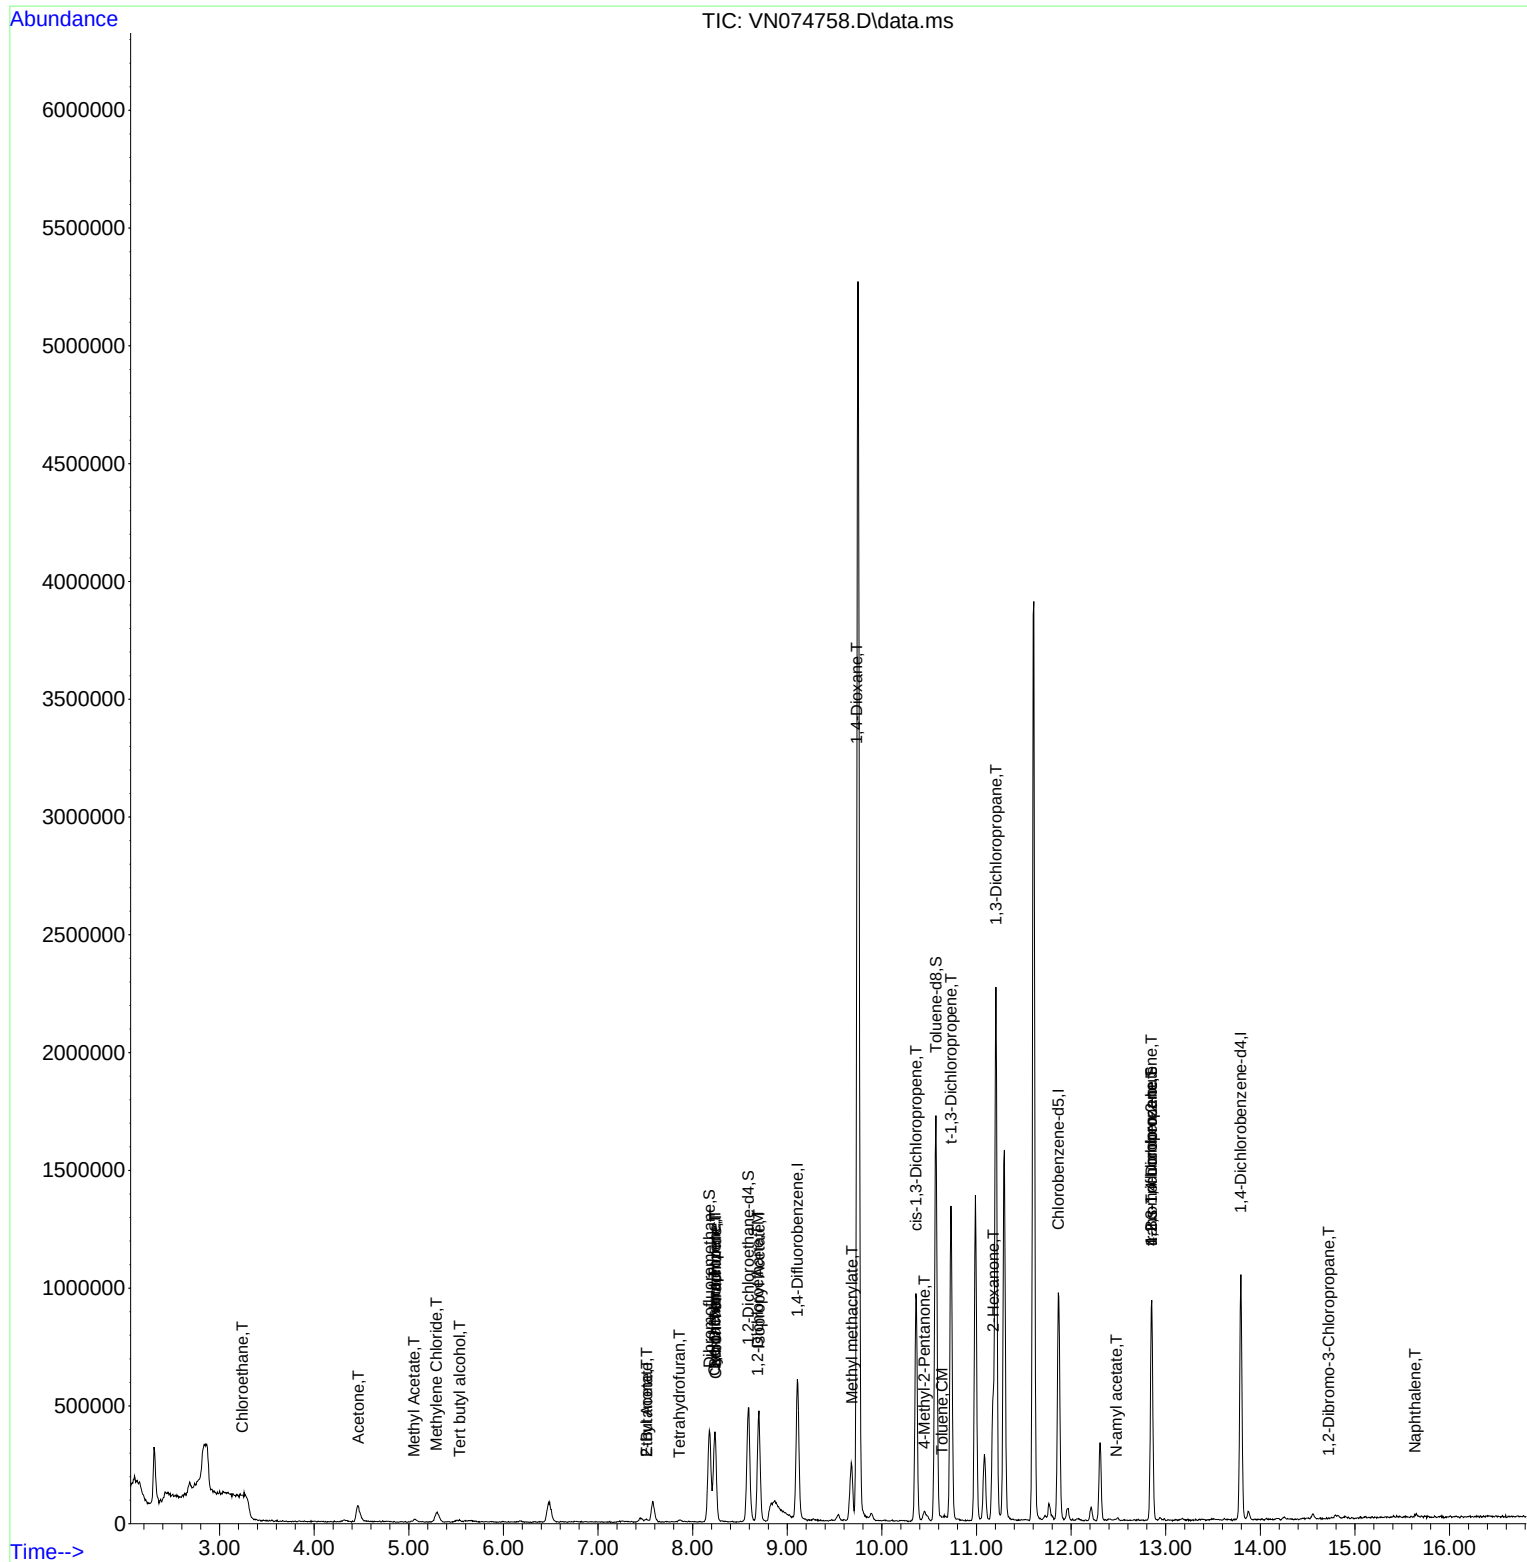


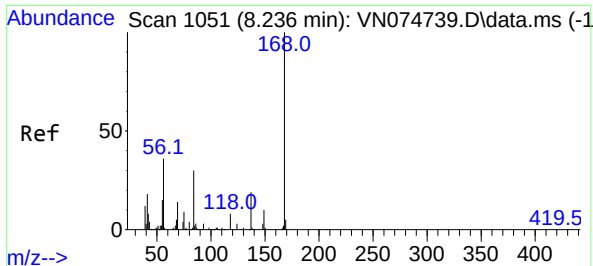

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.236 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion:168 Resp: 269035
Ion Ratio Lower Upper
168 100
99 57.0 42.8 64.2

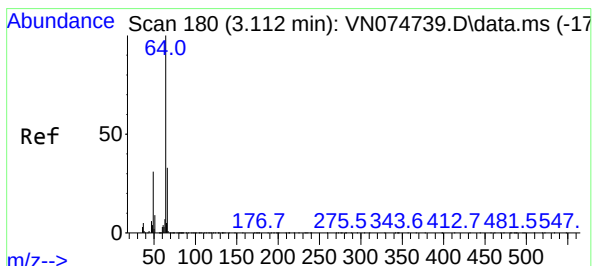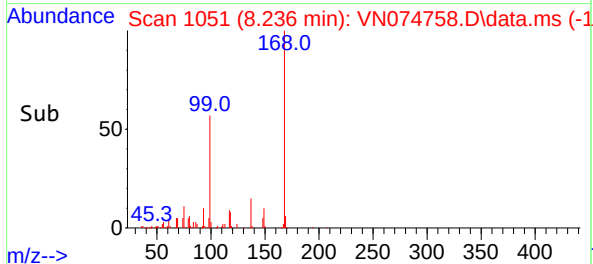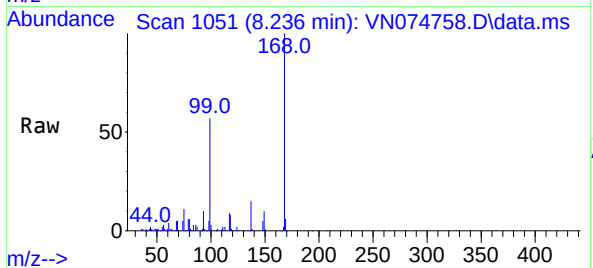

#6
Chloroethane
Concen: 9.308 ug/l
RT: 3.242 min Scan# 202
Delta R.T. 0.129 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 64 Resp: 69963
Ion Ratio Lower Upper
64 100
66 3.2 25.1 37.7#


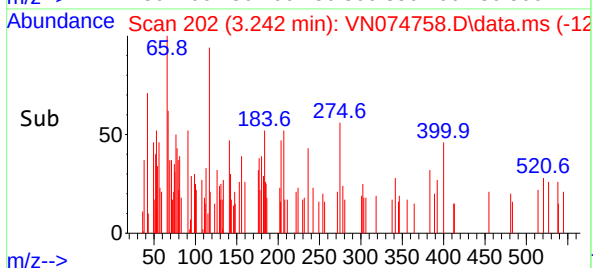
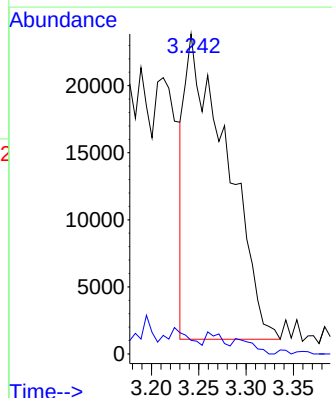
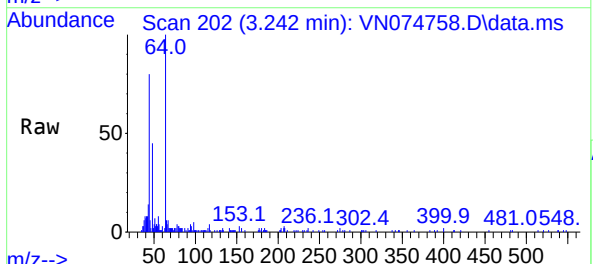




#11
Tert butyl alcohol
Concen: 2.052 ug/l
RT: 5.536 min Scan# 59
Delta R.T. -0.024 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 59 Resp: 4380
Ion Ratio Lower Upper
59 100
57 1.8 7.7 11.5#



#13
Acrolein
Concen: Below Cal
RT: 4.212 min Scan# 367
Delta R.T. 0.011 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 56 Resp: 436
Ion Ratio Lower Upper
56 100
55 220.2 54.9 82.3#


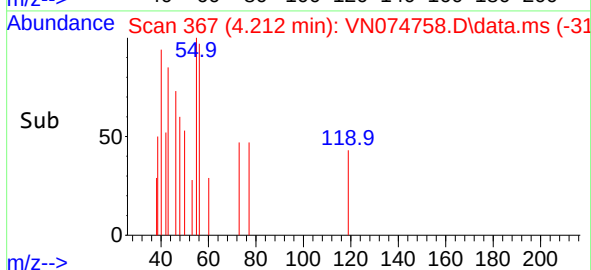






#16
Acetone
Concen: 36.392 ug/l
RT: 4.465 min Scan# 410
Delta R.T. 0.006 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 43 Resp: 131464
Ion Ratio Lower Upper
43 100
58 29.2 24.9 37.3

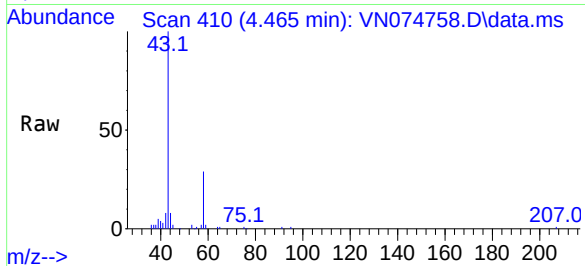

#18
Methyl Acetate
Concen: 1.780 ug/l
RT: 5.053 min Scan# 510
Delta R.T. 0.006 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 43 Resp: 23809
Ion Ratio Lower Upper
43 100
74 18.1 18.5 27.7#


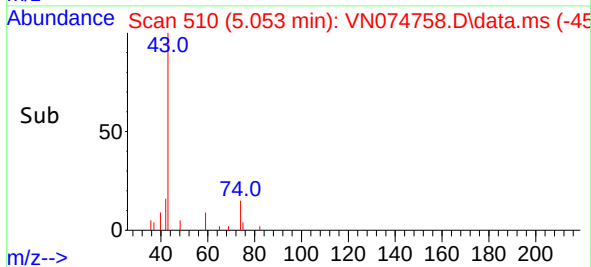

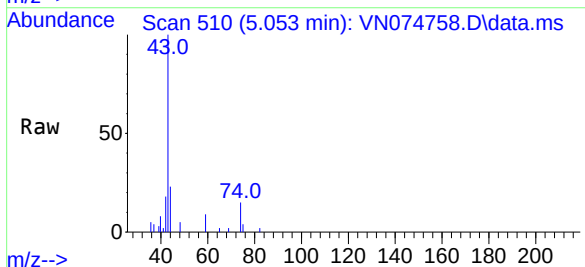




#20
Methylene Chloride
Concen: 2.797 ug/l
RT: 5.289 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 84 Resp: 28122
Ion Ratio Lower Upper
84 100
49 109.2 107.4 161.0
51 27.6 35.1 52.7#
86 48.9 50.4 75.6#

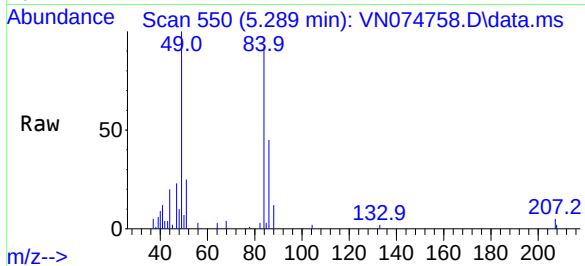

#25
2-Butanone
Concen: 2.087 ug/l
RT: 7.512 min Scan# 928
Delta R.T. 0.012 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 43 Resp: 13682
Ion Ratio Lower Upper
43 100
72 42.1 21.4 32.0#


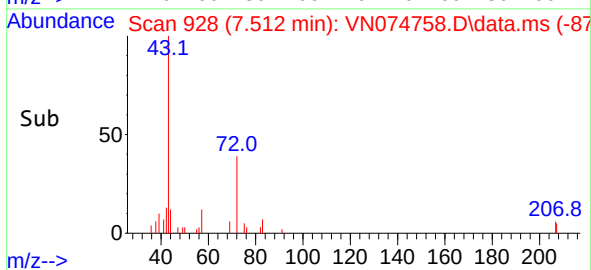

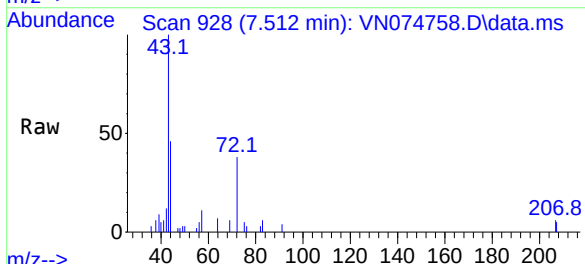




#29
Tetrahydrofuran
Concen: 1.797 ug/l
RT: 7.859 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 42	Resp: 8213
Ion Ratio	Lower Upper
42 100	
72 37.0	33.0 49.6
71 34.1	30.4 45.6

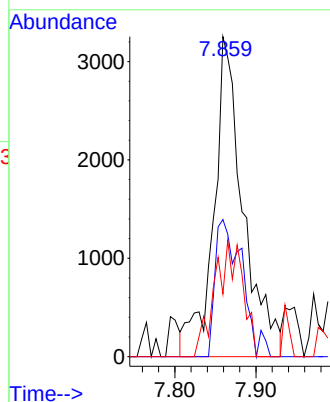

#31
Cyclohexane
Concen: 0.713 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.035 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 56	Resp: 7851		
Ion Ratio	Lower	Upper	
56	100		
69	131.9	23.1	34.7#
84	133.5	67.1	100.7#



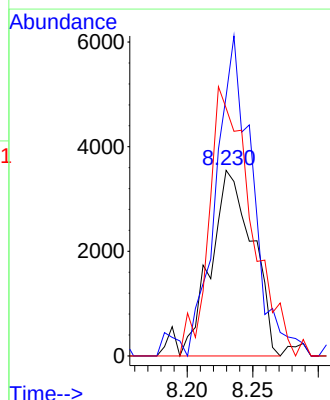



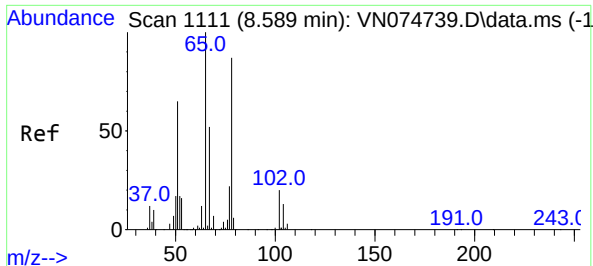

#33
1,2-Dichloroethane-d4
Concen: 54.415 ug/l
RT: 8.589 min Scan# 1111
Delta R.T. -0.000 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 65 Resp: 346874
Ion Ratio Lower Upper
65 100
67 57.6 0.0 109.0

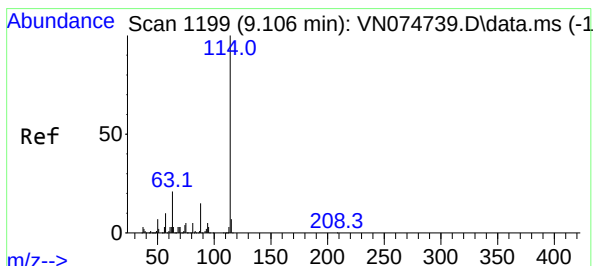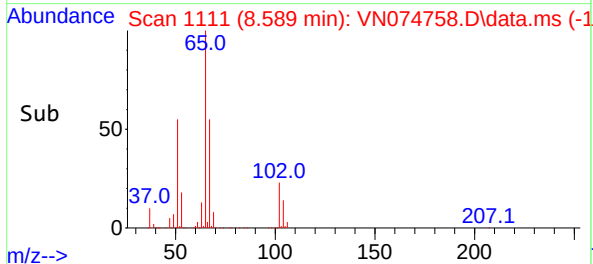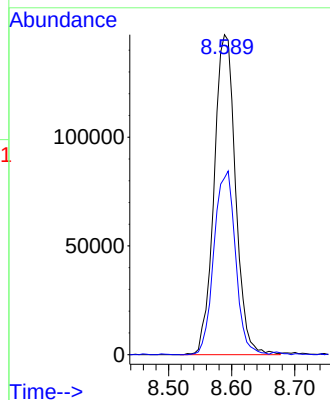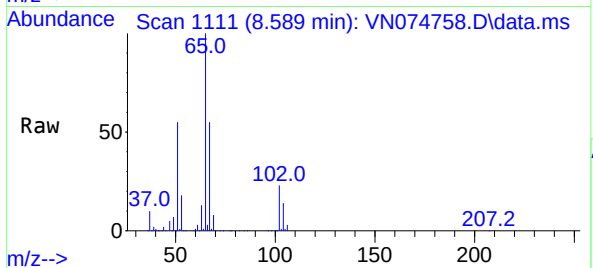

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. -0.000 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion:114 Resp: 513809
Ion Ratio Lower Upper
114 100
63 21.6 0.0 41.2
88 14.7 0.0 30.2


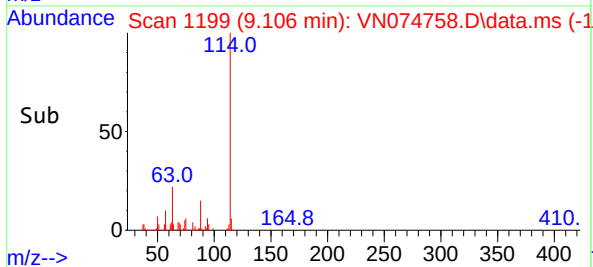
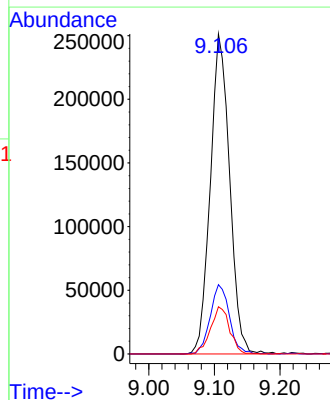
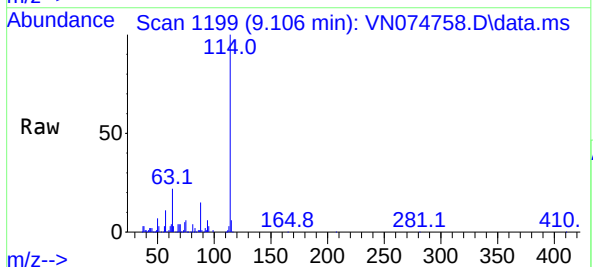


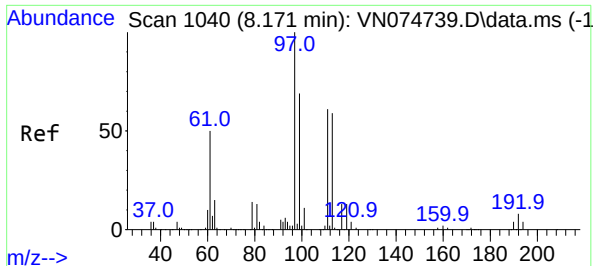

#35
Dibromofluoromethane
Concen: 52.869 ug/l
RT: 8.177 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion:113 Resp: 274460
Ion Ratio Lower Upper
113 100
111 105.0 83.0 124.6
192 15.9 12.6 18.8

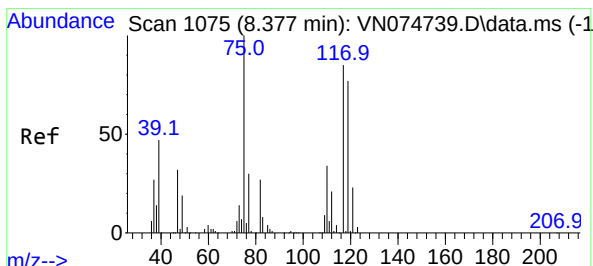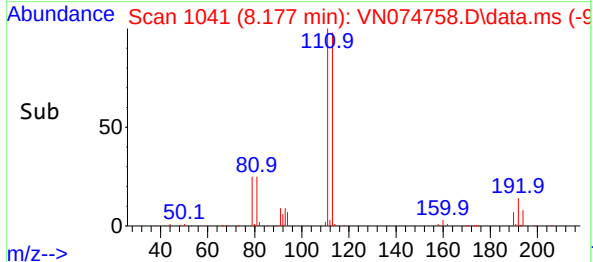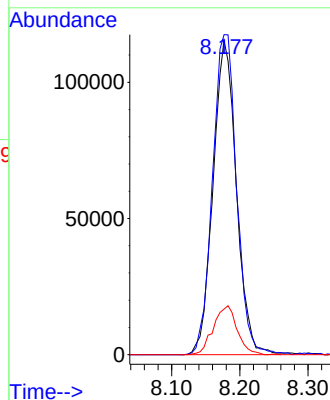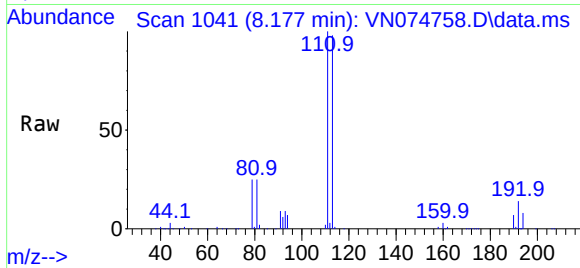

#36
1,1-Dichloropropene
Concen: 3.100 ug/l
RT: 8.236 min Scan# 1051
Delta R.T. -0.141 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 75 Resp: 26044
Ion Ratio Lower Upper
75 100
110 7.2 17.2 51.5#
77 0.0 24.3 36.5#


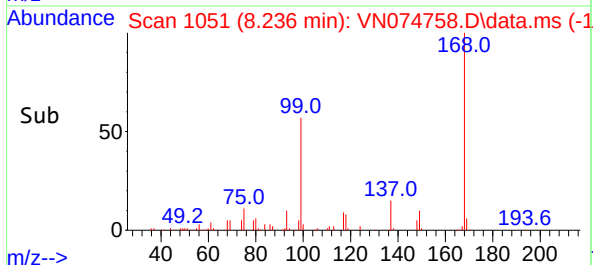
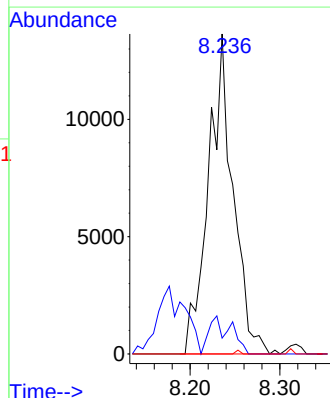
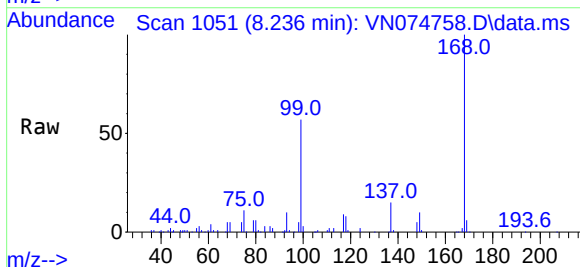




#37
Ethyl Acetate
Concen: 0.406 ug/l
RT: 7.512 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 43 Resp: 13682
Ion Ratio Lower Upper
43 100
61 0.0 4.3 6.5#
70 0.0 3.0 4.4#



#38
Carbon Tetrachloride
Concen: 3.660 ug/l
RT: 8.241 min Scan# 1052
Delta R.T. -0.129 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 117 Resp: 29003
Ion Ratio Lower Upper
117 100
119 2.9 74.3 111.5#
121 0.0 25.0 37.4#



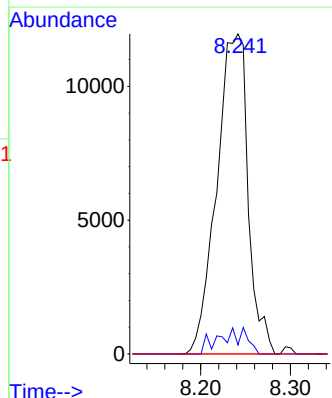



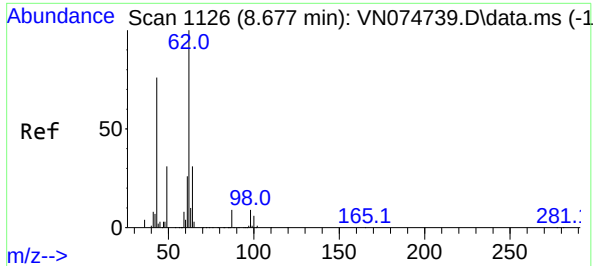

#42
1,2-Dichloroethane
Concen: 0.418 ug/l
RT: 8.689 min Scan# 1126
Delta R.T. 0.012 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 62 Resp: 3567
Ion Ratio Lower Upper
62 100
98 10.3 0.0 19.4

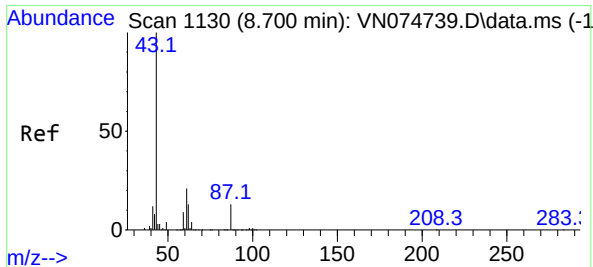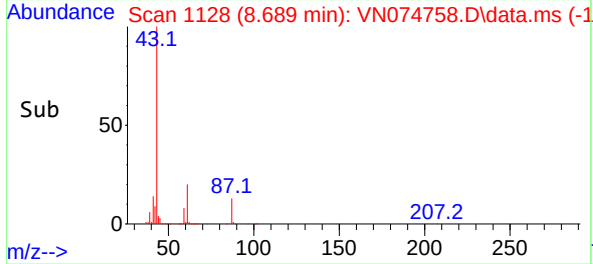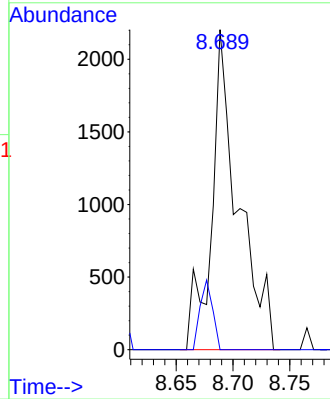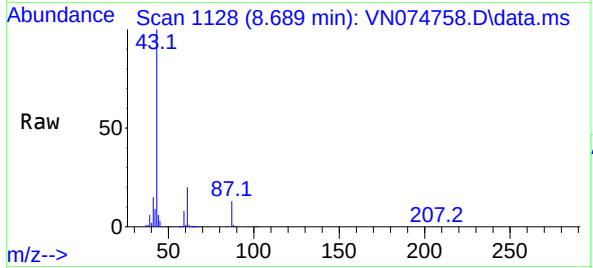

#43
Isopropyl Acetate
Concen: 26.012 ug/l
RT: 8.700 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 43 Resp: 541775
Ion Ratio Lower Upper
43 100
61 18.3 19.4 29.0#
87 12.5 10.1 15.1


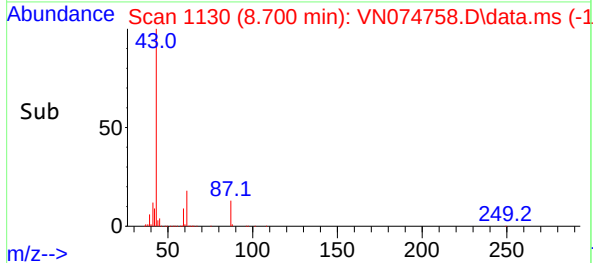
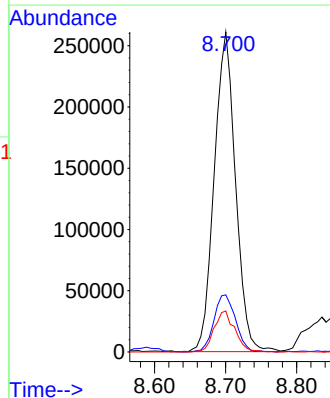
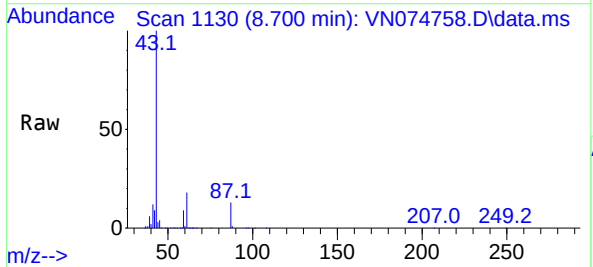


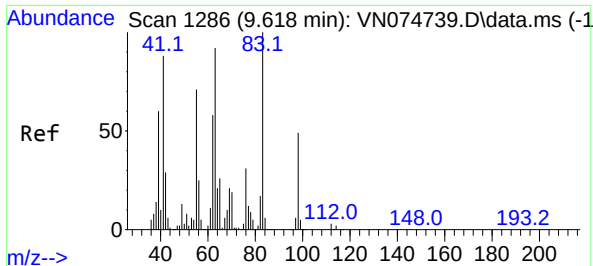

#48
Methyl methacrylate
Concen: 2.062 ug/l
RT: 9.683 min Scan# 11
Delta R.T. 0.065 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 41 Resp: 17631
Ion Ratio Lower Upper
41 100
69 2.9 0.0 0.0#
39 0.0 54.4 81.6#

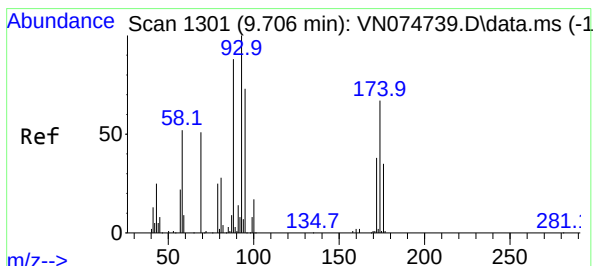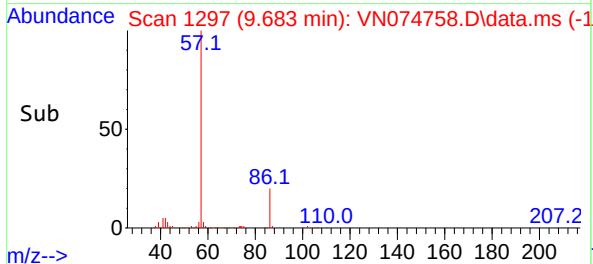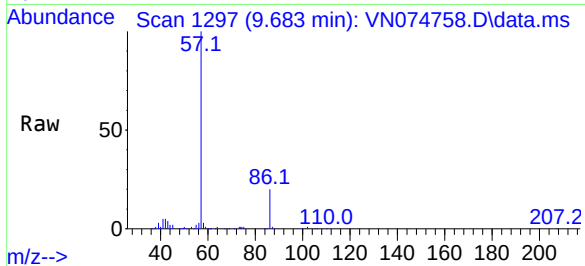

#49
1,4-Dioxane
Concen: 2.234 ug/l
RT: 9.736 min Scan# 1306
Delta R.T. 0.029 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 88 Resp: 414
Ion Ratio Lower Upper
88 100
43 1259280.7 23.4 35.2#
58 4914.3 54.9 82.3#


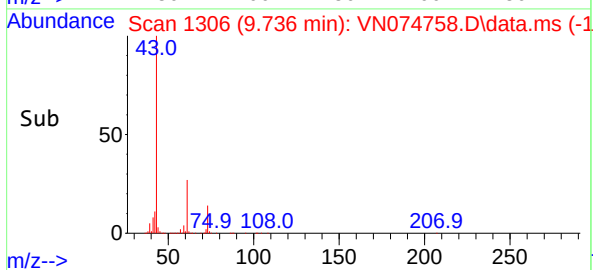

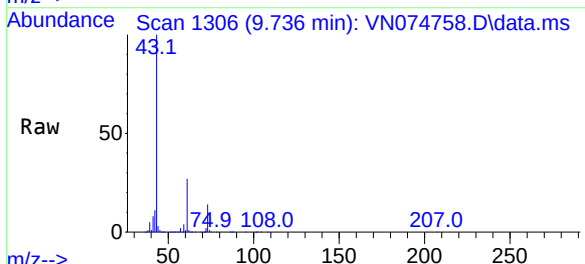




#50
Toluene-d8
Concen: 52.260 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 98 Resp: 1164097
Ion Ratio Lower Upper
98 100
100 62.0 50.7 76.1

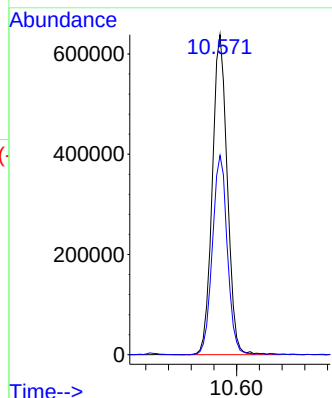

#51
4-Methyl-2-Pentanone
Concen: 2.011 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. -0.000 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 43 Resp: 26978
Ion Ratio Lower Upper
43 100
58 42.7 30.6 45.8









#52
Toluene
Concen: 0.232 ug/l
RT: 10.635 min Scan# 1459
Delta R.T. -0.000 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 92 Resp: 3786
Ion Ratio Lower Upper
92 100
91 183.2 140.2 210.4

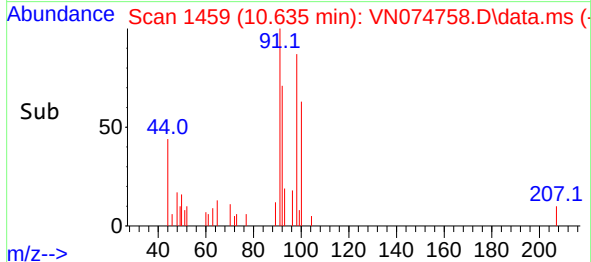

#53
t-1,3-Dichloropropene
Concen: 0.372 ug/l
RT: 10.730 min Scan# 1475
Delta R.T. -0.112 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38


Tgt Ion: 75 Resp: 3913
Ion Ratio Lower Upper
75 100
77 34.1 26.0 39.0

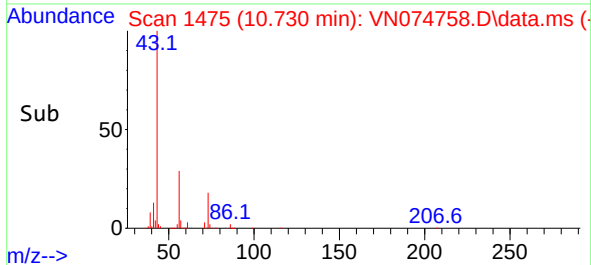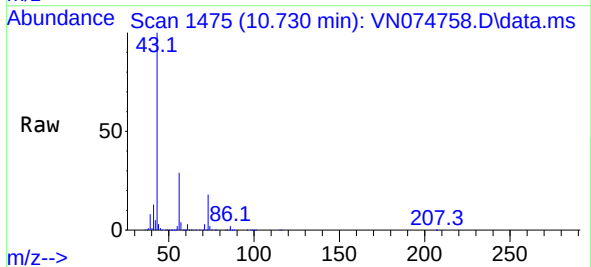






#54
cis-1,3-Dichloropropene
Concen: 15.171 ug/l
RT: 10.359 min Scan# 1412
Delta R.T. 0.047 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Instrument :
MSVOA_N
ClientSampleId :
SB-26



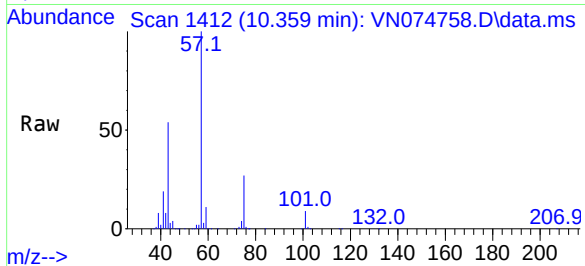



Tgt Ion: 75 Resp: 172325
Ion Ratio Lower Upper
75 100
77 0.3 24.4 36.6#
39 30.2 38.6 57.8#



#57
1,3-Dichloropropane
Concen: 2.072 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.041 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 76 Resp: 24533
Ion Ratio Lower Upper
76 100
78 0.0 26.2 39.2#


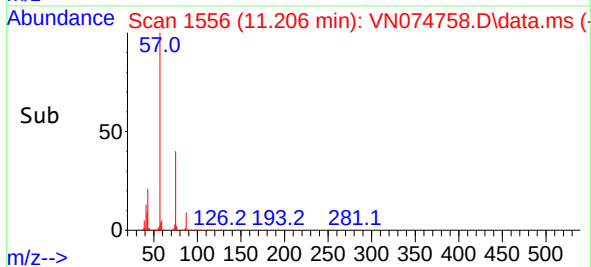

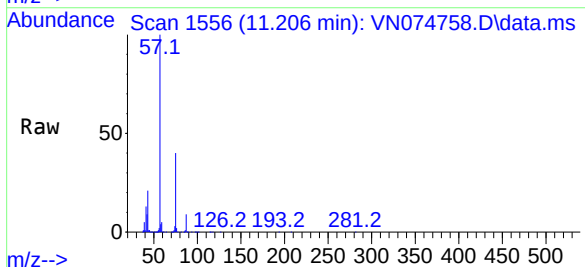




#59
2-Hexanone
Concen: 47.335 ug/l
RT: 11.177 min Scan# 11
Delta R.T. -0.024 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 43 Resp: 480209
Ion Ratio Lower Upper
43 100
58 0.0 27.3 81.9#



#62
4-Bromofluorobenzene
Concen: 45.346 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.006 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 95 Resp: 307053
Ion Ratio Lower Upper
95 100
174 74.8 0.0 149.4
176 72.4 0.0 142.0


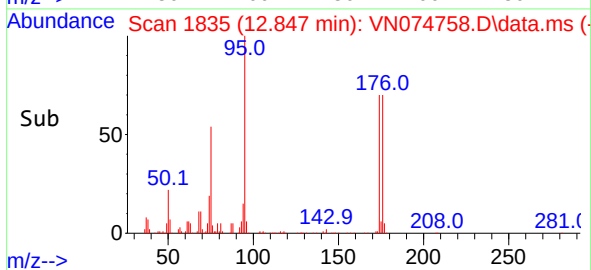






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.006 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion:117 Resp: 540821
Ion Ratio Lower Upper
117 100
82 55.9 45.4 68.2
119 29.6 25.1 37.7

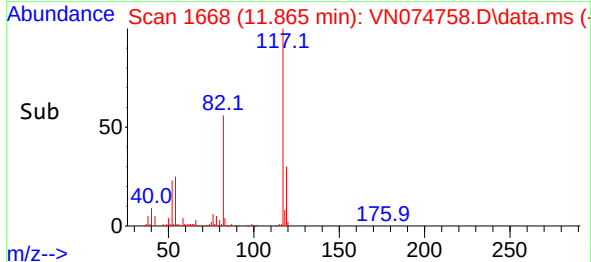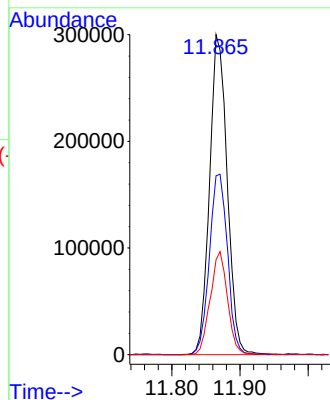

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion:152 Resp: 254995
Ion Ratio Lower Upper
152 100
115 62.2 30.0 90.0
150 162.8 0.0 356.4


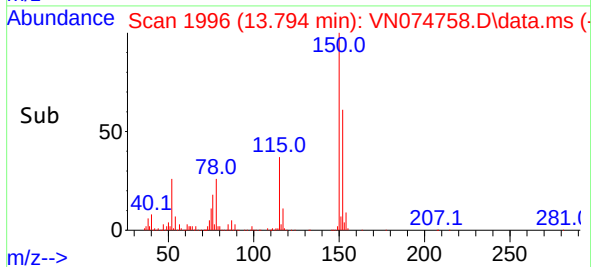
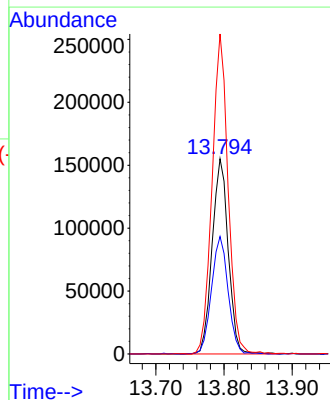
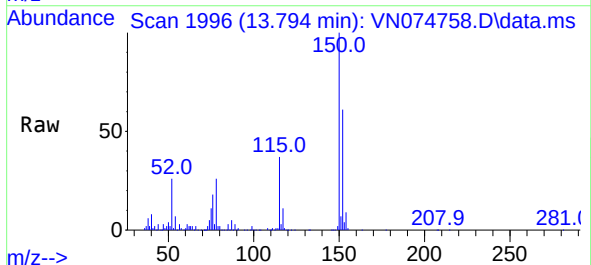




#74
N-amy1 acetate
Concen: 0.482 ug/l
RT: 12.477 min Scan# 11
Delta R.T. -0.018 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 43 Resp: 7148
Ion Ratio Lower Upper
43 100
70 7.8 32.9 49.3#
55 10.5 17.8 26.6#
61 0.0 18.9 28.3#

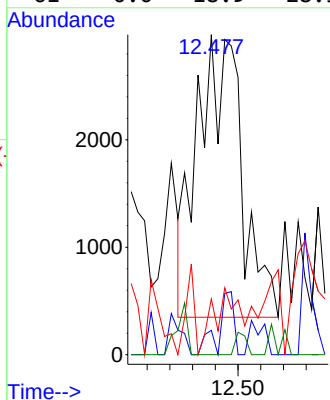

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.859 min Scan# 1837
Delta R.T. -0.082 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 83 Resp: 185
Ion Ratio Lower Upper
83 100
131 33.0 4.3 12.8#
85 0.0 32.9 98.6#


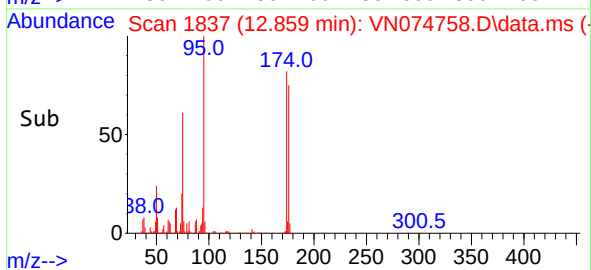
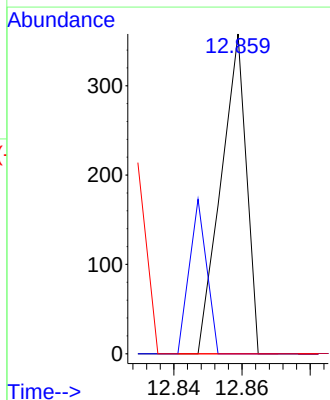





#76
1,2,3-Trichloropropane
Concen: 23.298 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.147 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38




Instrument :
MSVOA_N
ClientSampleId :
SB-26


Tgt Ion: 75 Resp: 177317
Ion Ratio Lower Upper
75 100
77 1.9 76.9 230.7#



#81
trans-1,4-Dichloro-2-butene
Concen: 45.393 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.112 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Tgt Ion: 75 Resp: 177317
Ion Ratio Lower Upper
75 100
53 0.1 71.4 107.0#
89 0.0 32.1 48.1#


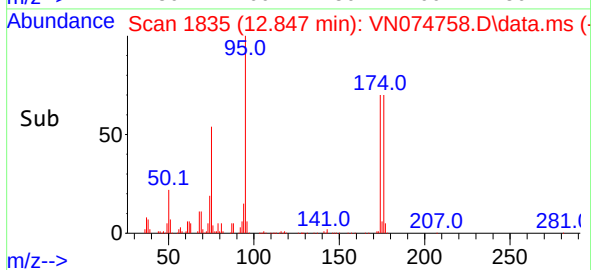






#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.206 ug/l
 RT: 14.723 min Scan# 2154
 Delta R.T. 0.000 min
 Lab File: VN074758.D
 Acq: 05 Oct 2022 23:38




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-26


Tgt Ion: 75 Resp: 419
 Ion Ratio Lower Upper
 75 100
 155 0.0 40.3 120.8#
 157 0.0 51.3 153.9#

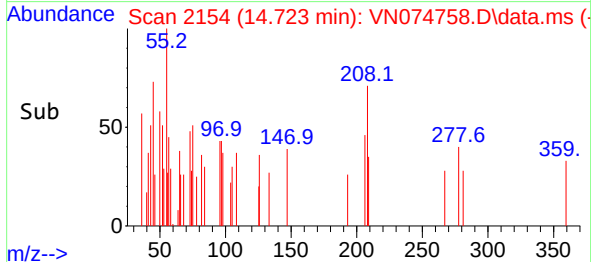

#95
 Naphthalene
 Concen: 0.543 ug/l
 RT: 15.635 min Scan# 2309
 Delta R.T. -0.006 min
 Lab File: VN074758.D
 Acq: 05 Oct 2022 23:38


Tgt Ion: 128 Resp: 9623
 Ion Ratio Lower Upper
 128 100
 127 6.3 10.2 15.2#
 129 0.0 9.0 13.4#

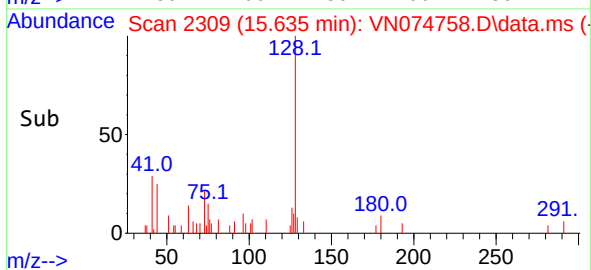



#96
1,2,3-Trichlorobenzene
Concen: Below Cal
RT: 15.859 min Scan# 21
Delta R.T. 0.018 min
Lab File: VN074758.D
Acq: 05 Oct 2022 23:38

Instrument :
MSVOA_N
ClientSampleId :
SB-26



Tgt Ion:180 Resp: 191
Ion Ratio Lower Upper
180 100
182 33.0 47.3 142.0#
145 0.0 17.1 51.2#

