

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100522\
 Data File : VN074762.D
 Acq On : 06 Oct 2022 01:15
 Operator : JC\MD
 Sample : N4957-14
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-30

Quant Time: Oct 06 07:47:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 05:37:50 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.235	168	241503	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	493307	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	515503	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	253092	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	336514	58.808	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 117.620%	
35) Dibromofluoromethane	8.177	113	267832	53.737	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 107.480%	
50) Toluene-d8	10.570	98	1093208	51.117	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.240%	
62) 4-Bromofluorobenzene	12.853	95	296720	45.641	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 91.280%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	1545	0.210	ug/l #	41
5) Bromomethane	2.947	94	1351	0.210	ug/l #	3
11) Tert butyl alcohol	5.547	59	2113	1.103	ug/l #	74
13) Acrolein	4.200	56	475	Below Cal	#	61
16) Acetone	4.459	43	130217	40.156	ug/l	94
18) Methyl Acetate	5.059	43	19713	1.642	ug/l #	82
20) Methylene Chloride	5.300	84	27573	3.269	ug/l #	88
25) 2-Butanone	7.512	43	13308	2.261	ug/l #	88
29) Tetrahydrofuran	7.877	42	4109	1.002	ug/l #	73
31) Cyclohexane	8.235	56	8961	0.906	ug/l #	30
36) 1,1-Dichloropropene	8.229	75	24544	3.042	ug/l #	50
37) Ethyl Acetate	7.512	43	13308	0.411	ug/l #	86
38) Carbon Tetrachloride	8.235	117	26766	3.518	ug/l #	17
40) Benzene	8.606	78	7343	0.281	ug/l	90
42) 1,2-Dichloroethane	8.700	62	2977	0.363	ug/l #	74
43) Isopropyl Acetate	8.700	43	543690	27.189	ug/l #	91
48) Methyl methacrylate	9.676	41	16391	1.997	ug/l #	71
49) 1,4-Dioxane	9.688	88	740	4.159	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	29244	2.271	ug/l	97
52) Toluene	10.635	92	5448	0.347	ug/l #	68
54) cis-1,3-Dichloropropene	10.365	75	171189	15.697	ug/l #	62
57) 1,3-Dichloropropane	11.206	76	22310	1.962	ug/l #	45
59) 2-Hexanone	11.170	43	460415	47.270	ug/l #	24
74) N-amyl acetate	12.494	43	7005	0.476	ug/l #	46
75) 1,1,2,2-Tetrachloroethane	12.941	83	86	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.847	75	174887	23.151	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	174887	45.107	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	14.723	75	974	0.482	ug/l #	3
95) Naphthalene	15.647	128	20896	1.188	ug/l #	74
96) 1,2,3-Trichlorobenzene	15.835	180	102	Below Cal	#	12

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 06 07:47:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 05:37:50 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1
Delta R.T. -0.001 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion:168 Resp: 241503
Ion Ratio Lower Upper
168 100
99 61.8 42.8 64.2

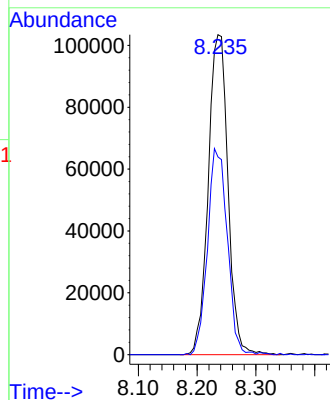

#3
Chloromethane
Concen: 0.210 ug/l
RT: 2.371 min Scan# 54
Delta R.T. -0.006 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 50 Resp: 1545
Ion Ratio Lower Upper
50 100
52 0.0 26.7 40.1#


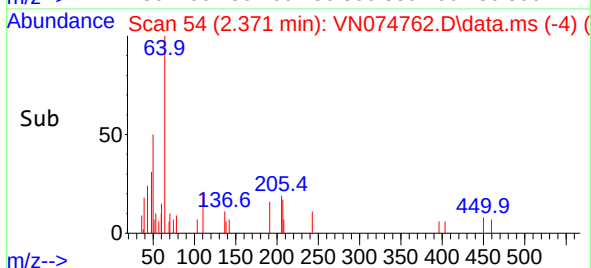
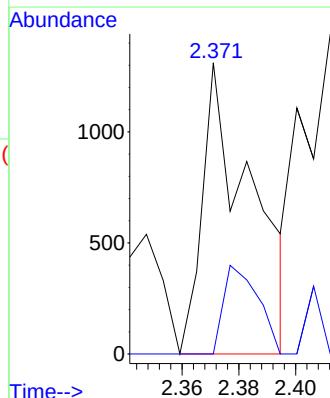





#5
Bromomethane
Concen: 0.210 ug/l
RT: 2.947 min Scan# 11
Delta R.T. 0.017 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 94 Resp: 1351
Ion Ratio Lower Upper
94 100
96 0.0 75.0 112.6#

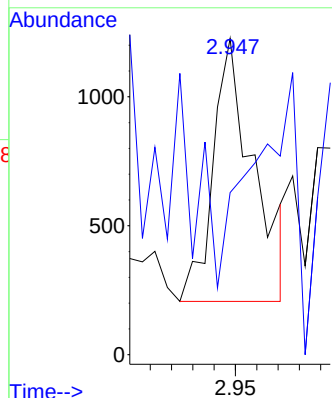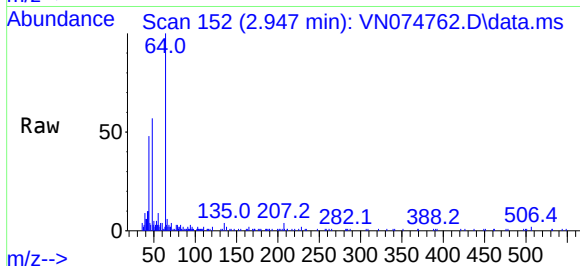

#11
Tert butyl alcohol
Concen: 1.103 ug/l
RT: 5.547 min Scan# 594
Delta R.T. -0.012 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 59 Resp: 2113
Ion Ratio Lower Upper
59 100
57 0.0 7.7 11.5#


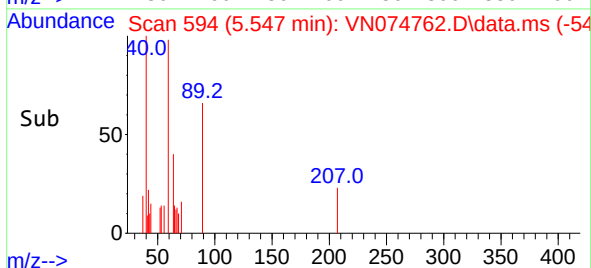

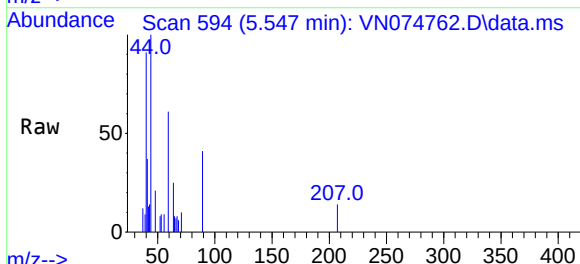




#13
Acrolein
Concen: Below Cal
RT: 4.200 min Scan# 30
Delta R.T. -0.001 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 56 Resp: 475
Ion Ratio Lower Upper
56 100
55 100.0 54.9 82.3#



#16
Acetone
Concen: 40.156 ug/l
RT: 4.459 min Scan# 409
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 43 Resp: 130217
Ion Ratio Lower Upper
43 100
58 27.9 24.9 37.3


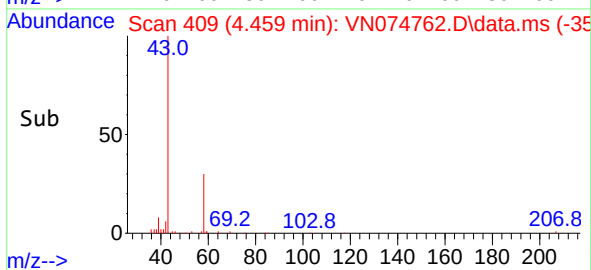






#18
Methyl Acetate
Concen: 1.642 ug/l
RT: 5.059 min Scan# 511
Delta R.T. 0.011 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 43 Resp: 19713
Ion Ratio Lower Upper
43 100
74 31.6 18.5 27.7#

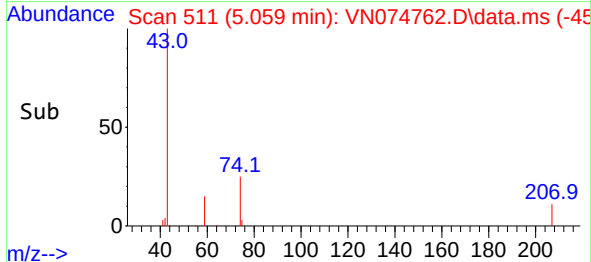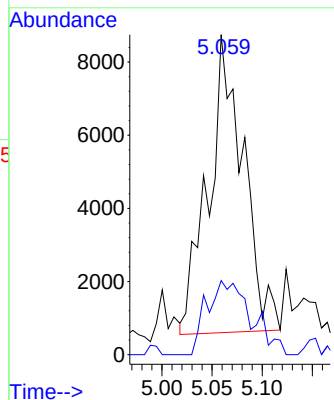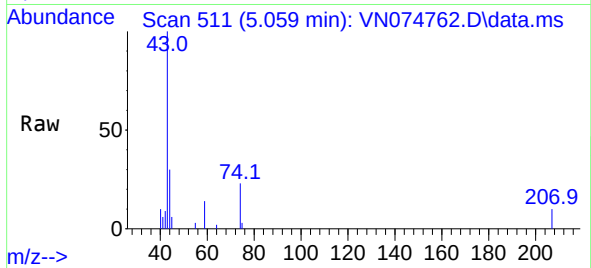

#20
Methylene Chloride
Concen: 3.269 ug/l
RT: 5.300 min Scan# 552
Delta R.T. 0.005 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 84 Resp: 27573
Ion Ratio Lower Upper
84 100
49 121.8 107.4 161.0
51 40.0 35.1 52.7
86 47.6 50.4 75.6#


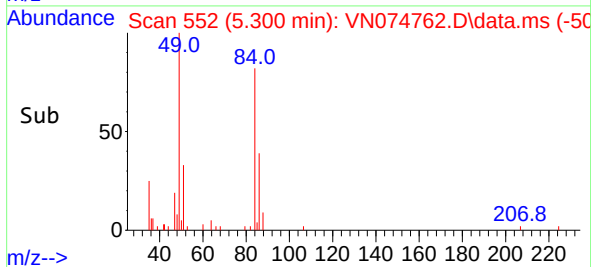
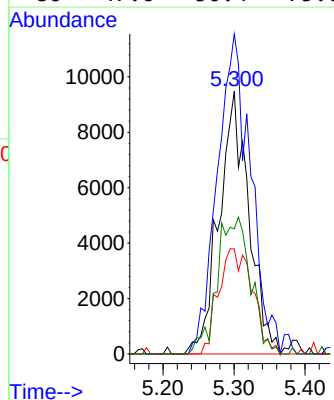
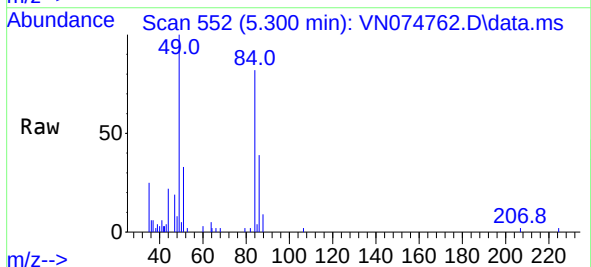




#25
2-Butanone
Concen: 2.261 ug/l
RT: 7.512 min Scan# 91
Delta R.T. 0.011 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 43 Resp: 13308
Ion Ratio Lower Upper
43 100
72 33.0 21.4 32.0#



#29
Tetrahydrofuran
Concen: 1.002 ug/l
RT: 7.877 min Scan# 990
Delta R.T. 0.023 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 42 Resp: 4109
Ion Ratio Lower Upper
42 100
72 61.2 33.0 49.6#
71 51.0 30.4 45.6#


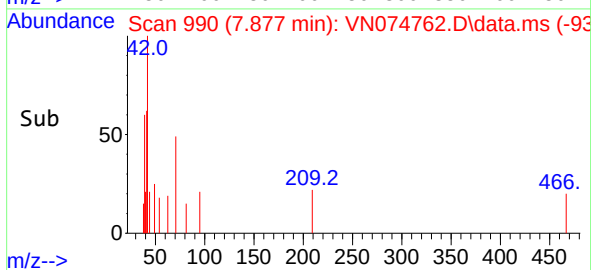






#31
Cyclohexane
Concen: 0.906 ug/l
RT: 8.235 min Scan# 11051
Delta R.T. -0.030 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 56 Resp: 8961
Ion Ratio Lower Upper
56 100
69 102.1 23.1 34.7#
84 125.8 67.1 100.7#

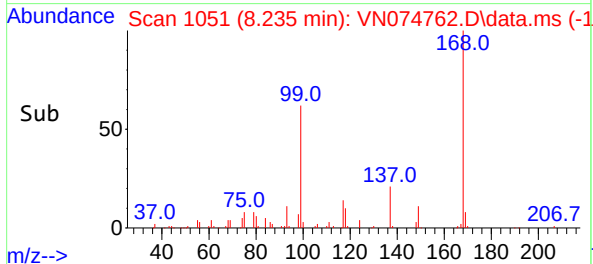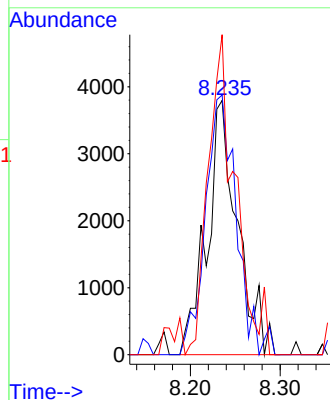

#33
1,2-Dichloroethane-d4
Concen: 58.808 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 65 Resp: 336514
Ion Ratio Lower Upper
65 100
67 56.2 0.0 109.0

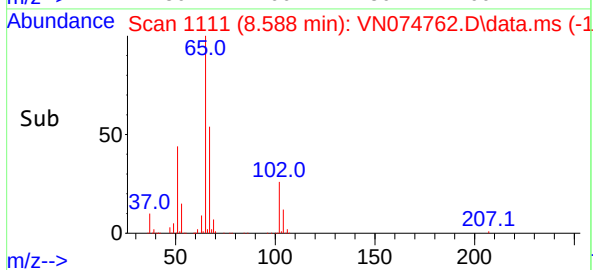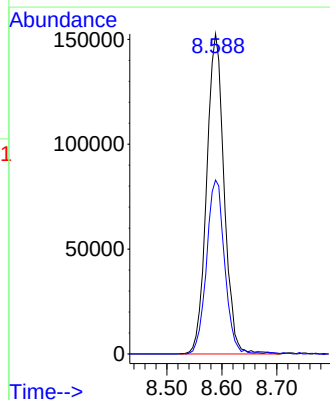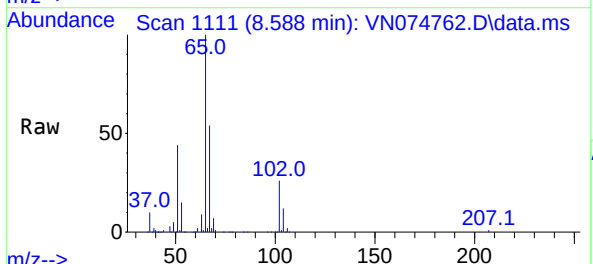



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1199

Delta R.T. 0.006 min

Lab File: VN074762.D

Acq: 06 Oct 2022 01:15

Instrument :

MSVOA_N

ClientSampleId :

SB-30





Tgt Ion:114 Resp: 493307

Ion Ratio Lower Upper

114 100

63 23.6 0.0 41.2

88 14.3 0.0 30.2

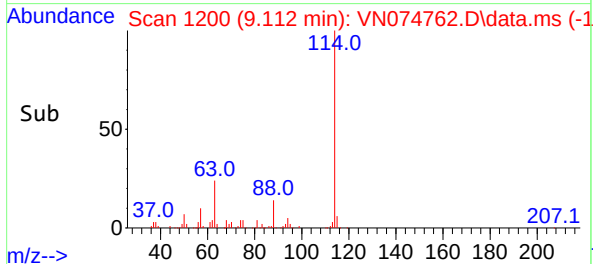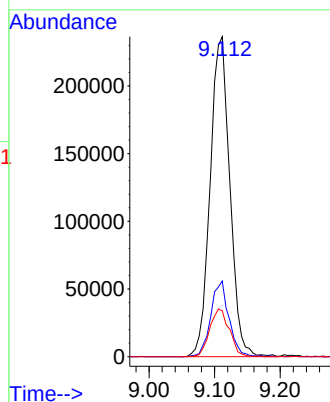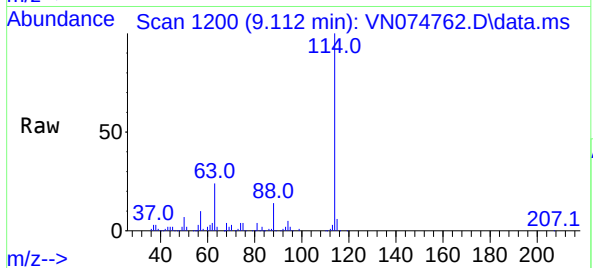

#35

Dibromofluoromethane

Concen: 53.737 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN074762.D

Acq: 06 Oct 2022 01:15




Tgt Ion:113 Resp: 267832


Ion Ratio Lower Upper

113 100

111 102.7 83.0 124.6

192 15.2 12.6 18.8

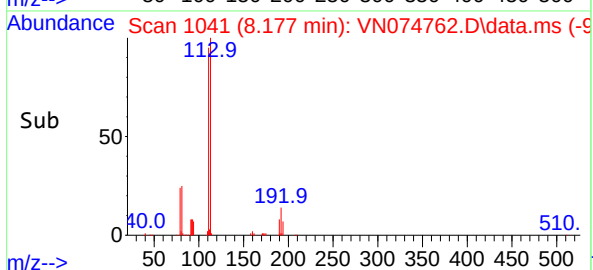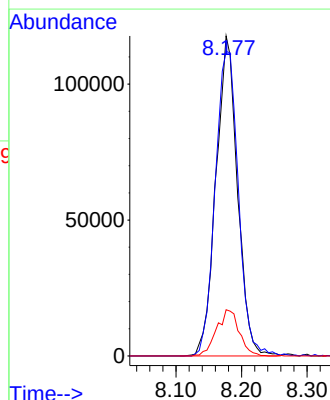

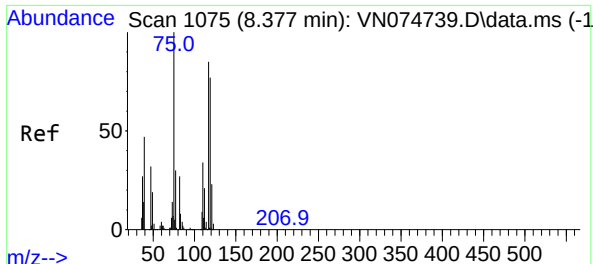

#36

1,1-Dichloropropene

Concen: 3.042 ug/l

RT: 8.229 min Scan# 1050

Delta R.T. -0.147 min

Lab File: VN074762.D

Acq: 06 Oct 2022 01:15

Instrument :

MSVOA_N

ClientSampleId :

SB-30





Tgt Ion: 75 Resp: 24544

Ion Ratio Lower Upper

75 100

110 8.2 17.2 51.5#

77 0.0 24.3 36.5#



#37

Ethyl Acetate

Concen: 0.411 ug/l

RT: 7.512 min Scan# 928

Delta R.T. 0.011 min

Lab File: VN074762.D

Acq: 06 Oct 2022 01:15




Tgt Ion: 43 Resp: 13308


Ion Ratio Lower Upper

43 100

61 0.0 4.3 6.5#

70 0.0 3.0 4.4#


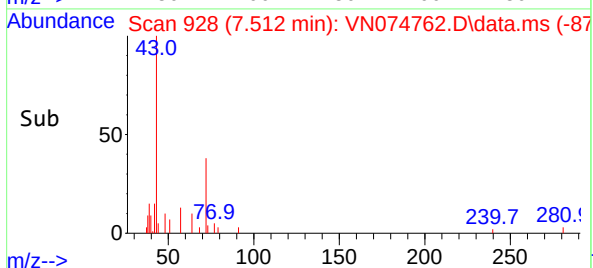

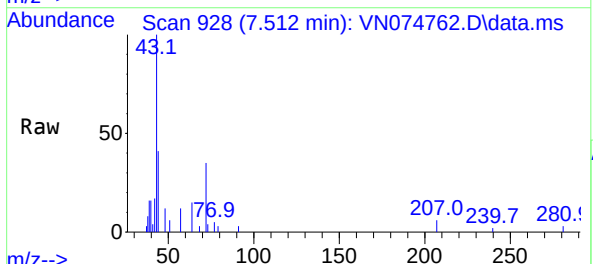




#38
Carbon Tetrachloride
Concen: 3.518 ug/l
RT: 8.235 min Scan# 1105
Delta R.T. -0.136 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion:117 Resp: 26766
Ion Ratio Lower Upper
117 100
119 4.3 74.3 111.5#
121 0.0 25.0 37.4#

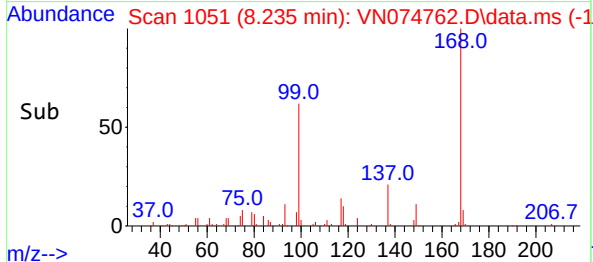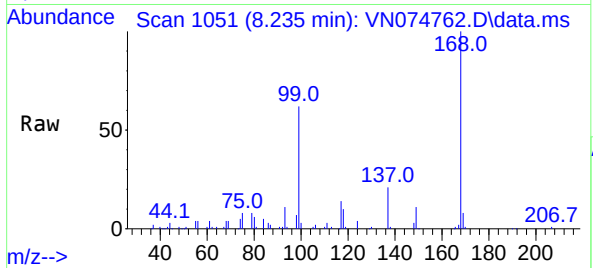

#40
Benzene
Concen: 0.281 ug/l
RT: 8.606 min Scan# 1114
Delta R.T. -0.006 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 78 Resp: 7343
Ion Ratio Lower Upper
78 100
77 30.0 20.1 30.1


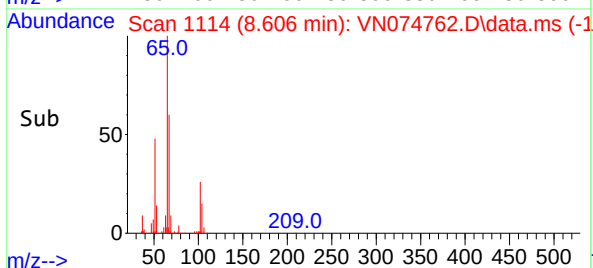
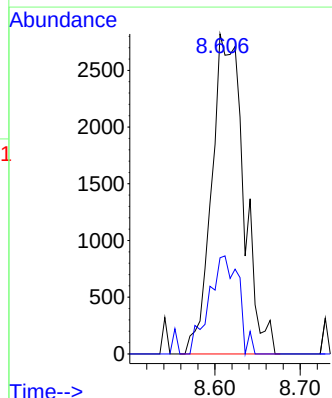
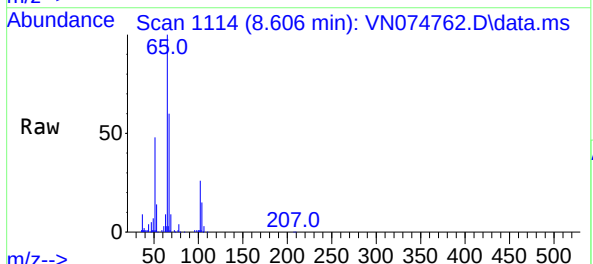




#42
1,2-Dichloroethane
Concen: 0.363 ug/l
RT: 8.700 min Scan# 1126
Delta R.T. 0.023 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 62 Resp: 2977
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.4

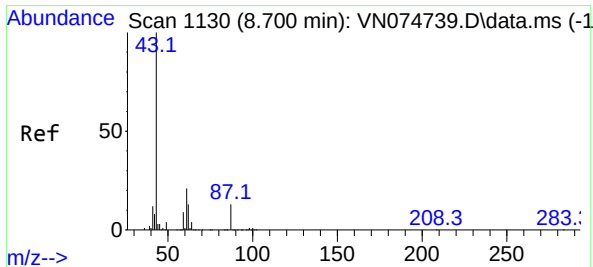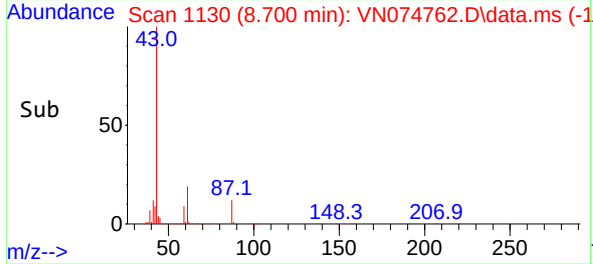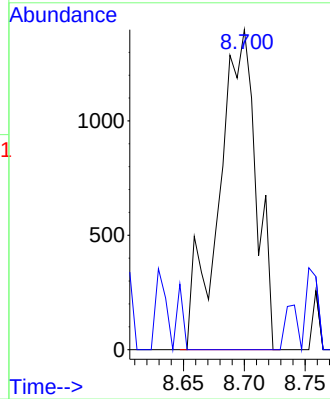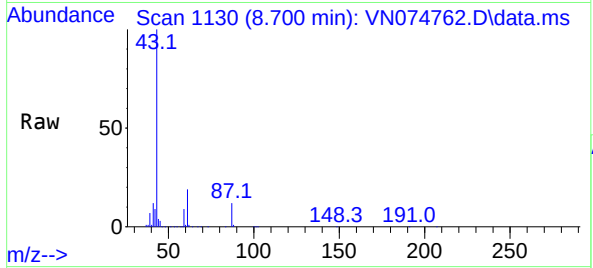

#43
Isopropyl Acetate
Concen: 27.189 ug/l
RT: 8.700 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 43 Resp: 543690
Ion Ratio Lower Upper
43 100
61 18.2 19.4 29.0#
87 11.4 10.1 15.1

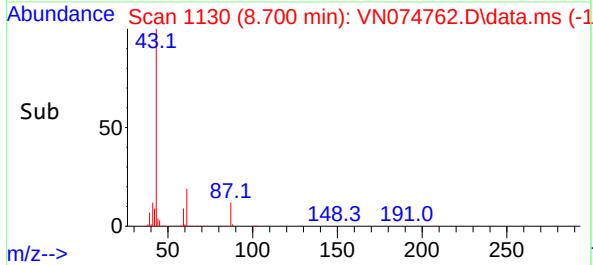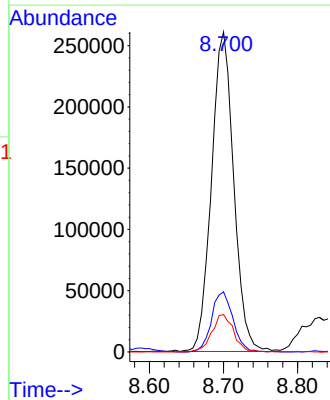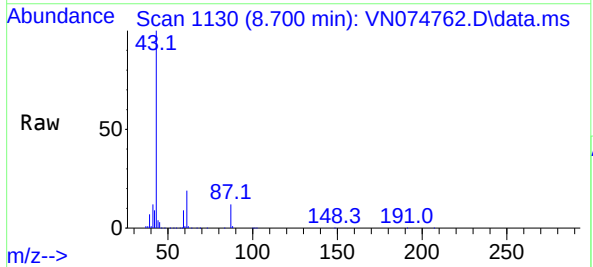



#48

Methyl methacrylate

Concen: 1.997 ug/l

RT: 9.676 min Scan# 1296

Delta R.T. 0.059 min

Lab File: VN074762.D

Acq: 06 Oct 2022 01:15

Instrument :

MSVOA_N

ClientSampleId :

SB-30


Tgt Ion: 41 Resp: 16391

Ion Ratio Lower Upper




41 100

69 0.5 0.0 0.0#

39 44.4 54.4 81.6#

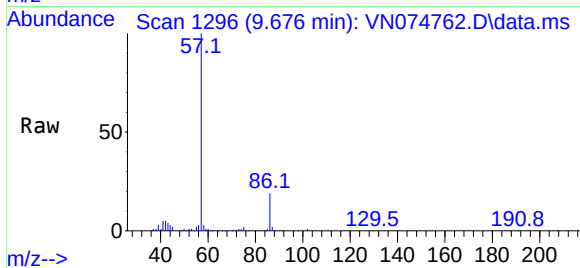

Abundance

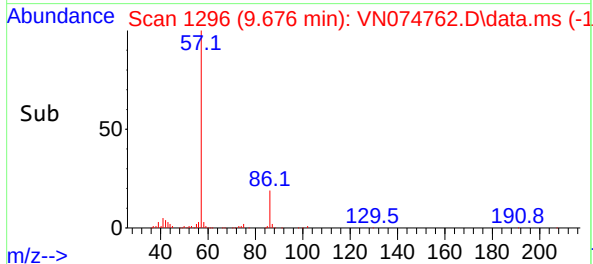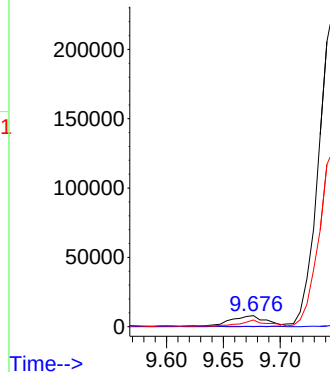

#49

1,4-Dioxane

Concen: 4.159 ug/l

RT: 9.688 min Scan# 1298

Delta R.T. -0.018 min

Lab File: VN074762.D

Acq: 06 Oct 2022 01:15


Tgt Ion: 88 Resp: 740

Ion Ratio Lower Upper



88 100


43 0.0 23.4 35.2#

58 1627.0 54.9 82.3#

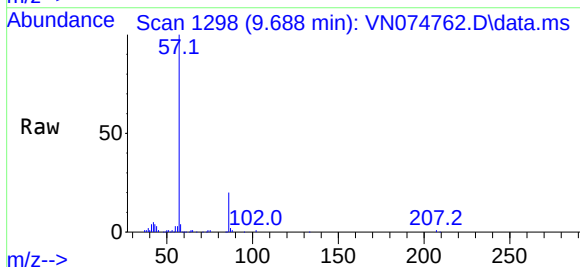

Abundance



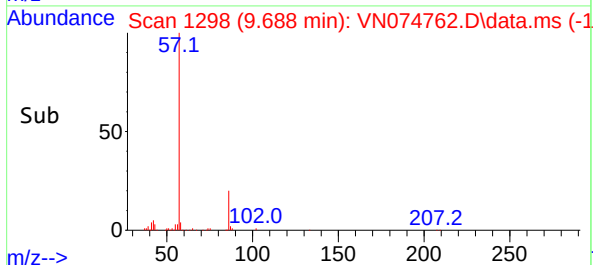
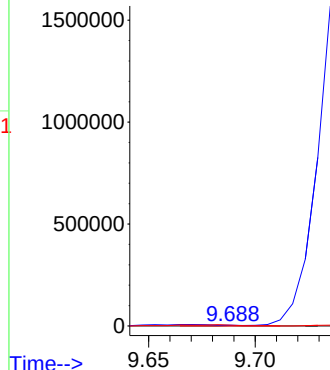




#50
Toluene-d8
Concen: 51.117 ug/l
RT: 10.570 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 98 Resp: 1093208
Ion Ratio Lower Upper
98 100
100 65.9 50.7 76.1

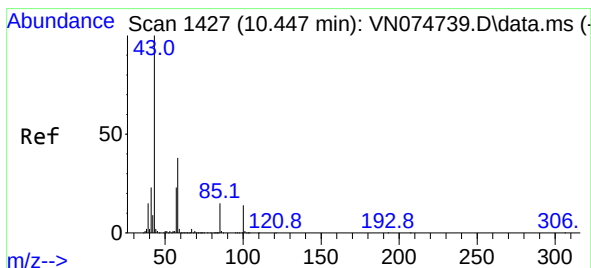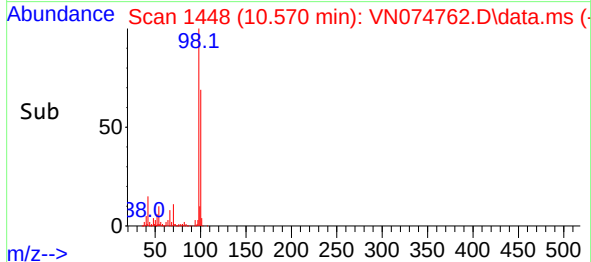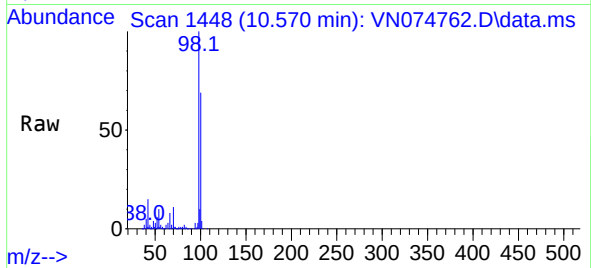

#51
4-Methyl-2-Pentanone
Concen: 2.271 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 43 Resp: 29244
Ion Ratio Lower Upper
43 100
58 40.1 30.6 45.8


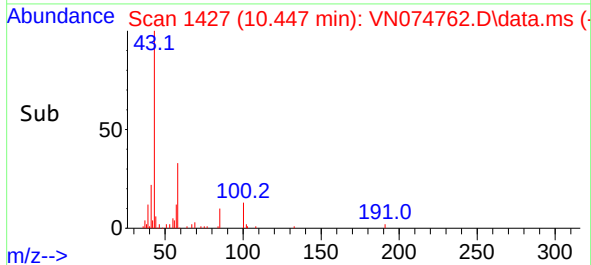

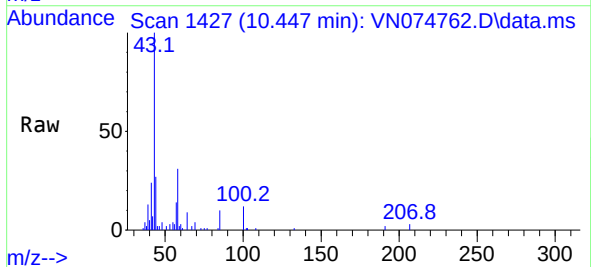




#52
Toluene
Concen: 0.347 ug/l
RT: 10.635 min Scan# 1413
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 92 Resp: 5448
Ion Ratio Lower Upper
92 100
91 220.1 140.2 210.4#

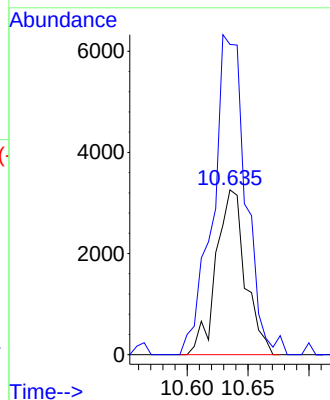

#54
cis-1,3-Dichloropropene
Concen: 15.697 ug/l
RT: 10.365 min Scan# 1413
Delta R.T. 0.053 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 75 Resp: 171189
Ion Ratio Lower Upper
75 100
77 0.4 24.4 36.6#
39 29.3 38.6 57.8#


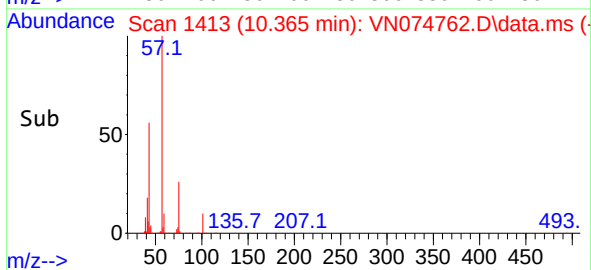
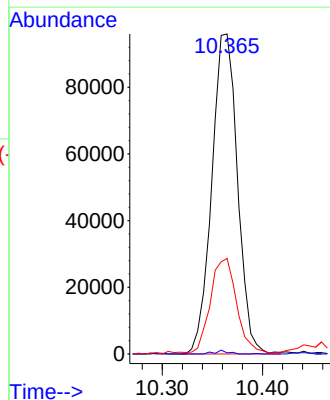





#57
1,3-Dichloropropane
Concen: 1.962 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.041 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 76 Resp: 22310
Ion Ratio Lower Upper
76 100
78 1.5 26.2 39.2#

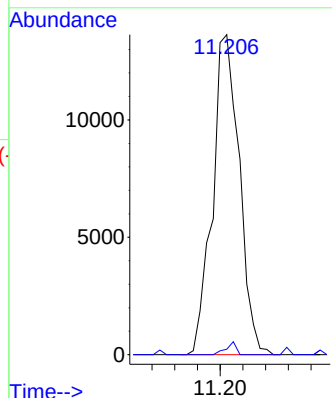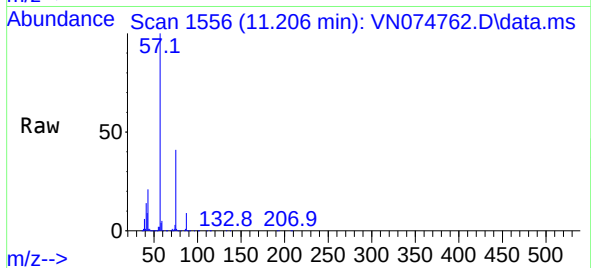

#59
2-Hexanone
Concen: 47.270 ug/l
RT: 11.170 min Scan# 1550
Delta R.T. -0.030 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 43 Resp: 460415
Ion Ratio Lower Upper
43 100
58 0.0 27.3 81.9#


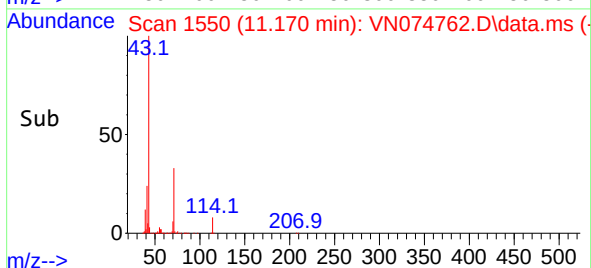

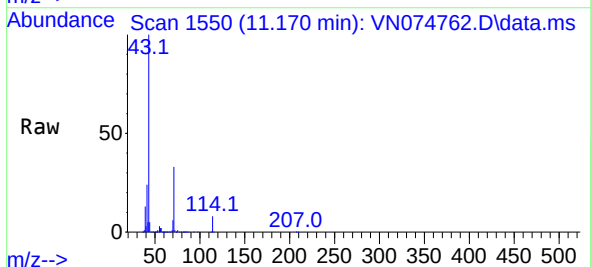


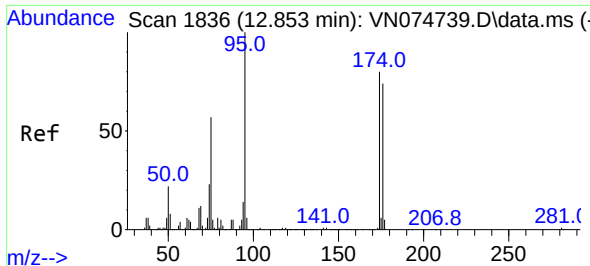

#62
4-Bromofluorobenzene
Concen: 45.641 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 95 Resp: 296720
Ion Ratio Lower Upper
95 100
174 78.1 0.0 149.4
176 74.6 0.0 142.0

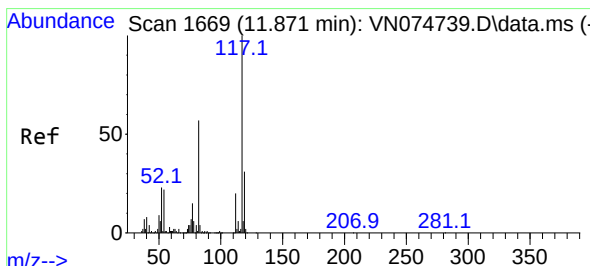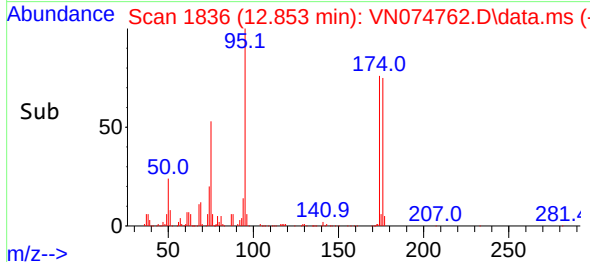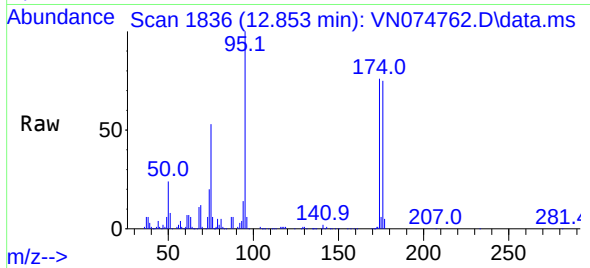

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1669
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 117 Resp: 515503
Ion Ratio Lower Upper
117 100
82 60.2 45.4 68.2
119 30.2 25.1 37.7


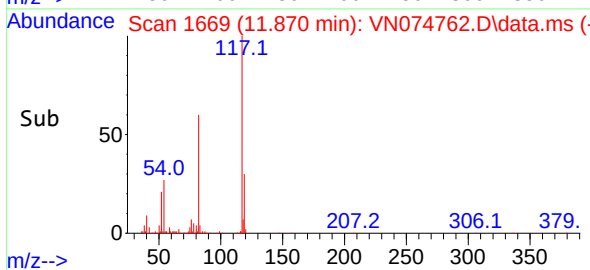

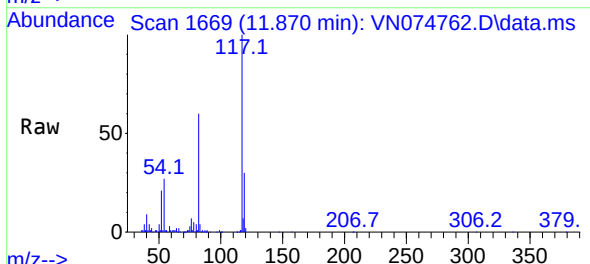


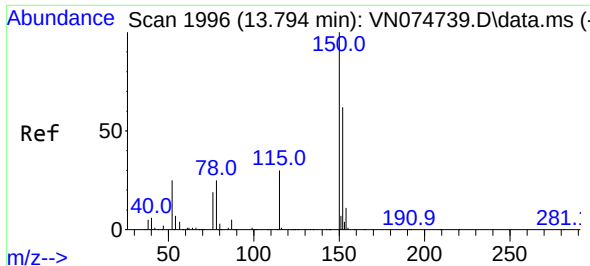

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion:152 Resp: 253092
Ion Ratio Lower Upper
152 100
115 59.8 30.0 90.0
150 160.6 0.0 356.4

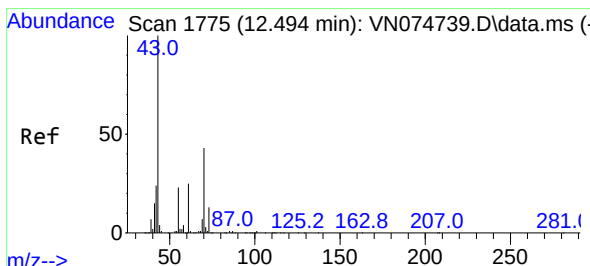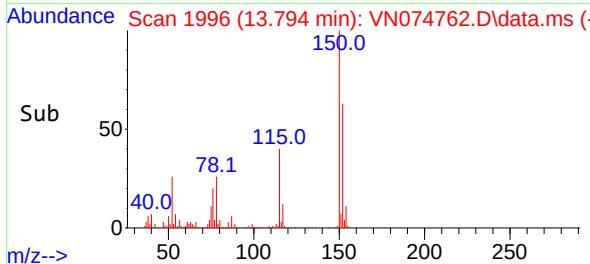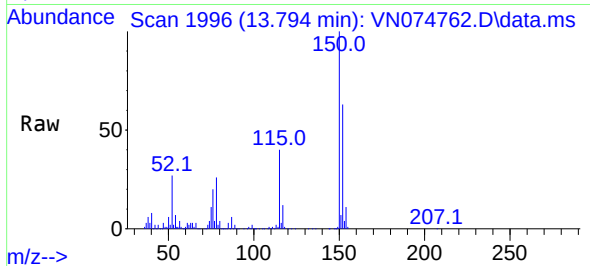

#74
N-ethyl acetate
Concen: 0.476 ug/l
RT: 12.494 min Scan# 1775
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 43 Resp: 7005
Ion Ratio Lower Upper
43 100
70 0.0 32.9 49.3#
55 4.4 17.8 26.6#
61 0.0 18.9 28.3#


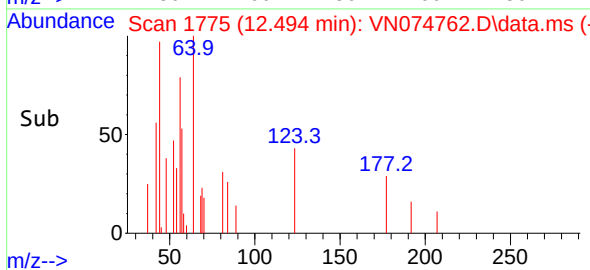

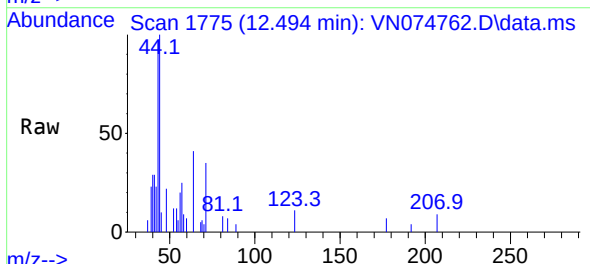




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.941 min Scan# 1851
Delta R.T. -0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 83 Resp: 86
Ion Ratio Lower Upper
83 100
131 76.7 4.3 12.8#
85 337.2 32.9 98.6#



#76
1,2,3-Trichloropropane
Concen: 23.151 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.147 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 75 Resp: 174887
Ion Ratio Lower Upper
75 100
77 1.3 76.9 230.7#


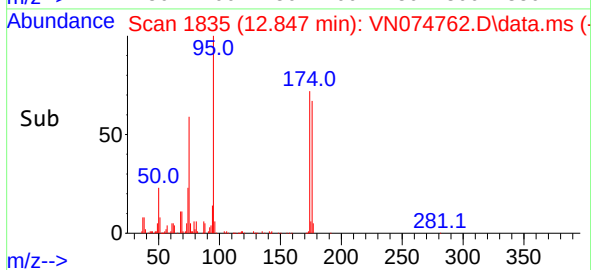






#81
trans-1,4-Dichloro-2-butene
Concen: 45.107 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.111 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15




Instrument :
MSVOA_N
ClientSampleId :
SB-30


Tgt Ion: 75 Resp: 174887
Ion Ratio Lower Upper
75 100
53 0.2 71.4 107.0#
89 0.0 32.1 48.1#

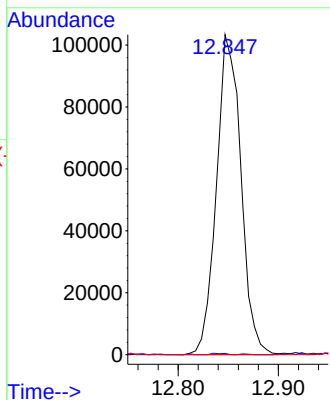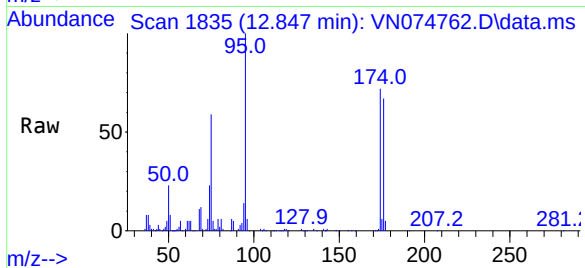

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.482 ug/l
RT: 14.723 min Scan# 2154
Delta R.T. 0.000 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion: 75 Resp: 974
Ion Ratio Lower Upper
75 100
155 0.0 40.3 120.8#
157 0.0 51.3 153.9#


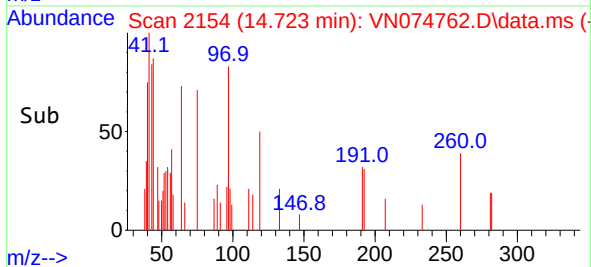
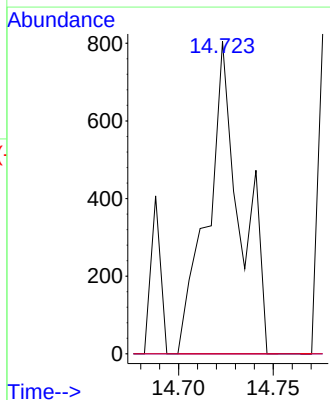
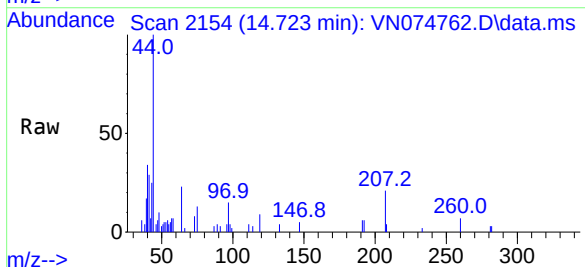




#95
Naphthalene
Concen: 1.188 ug/l
RT: 15.647 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Instrument :
MSVOA_N
ClientSampleId :
SB-30

Tgt Ion:128 Resp: 20896
Ion Ratio Lower Upper
128 100
127 3.4 10.2 15.2#
129 0.0 9.0 13.4#



#96
1,2,3-Trichlorobenzene
Concen: Below Cal
RT: 15.835 min Scan# 2343
Delta R.T. -0.006 min
Lab File: VN074762.D
Acq: 06 Oct 2022 01:15

Tgt Ion:180 Resp: 102
Ion Ratio Lower Upper
180 100
182 0.0 47.3 142.0#
145 0.0 17.1 51.2#

