
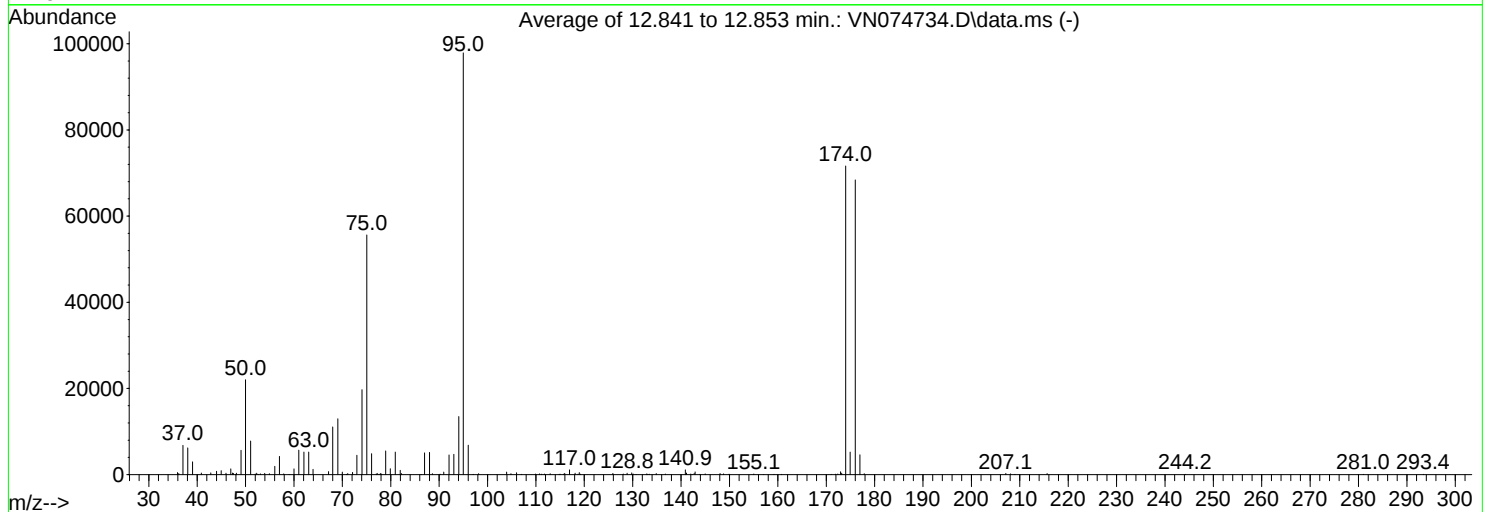


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100522\
Data File : VN074734.D
Acq On : 05 Oct 2022 10:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Title : SW846 8260
Last Update : Thu Oct 06 05:37:50 2022

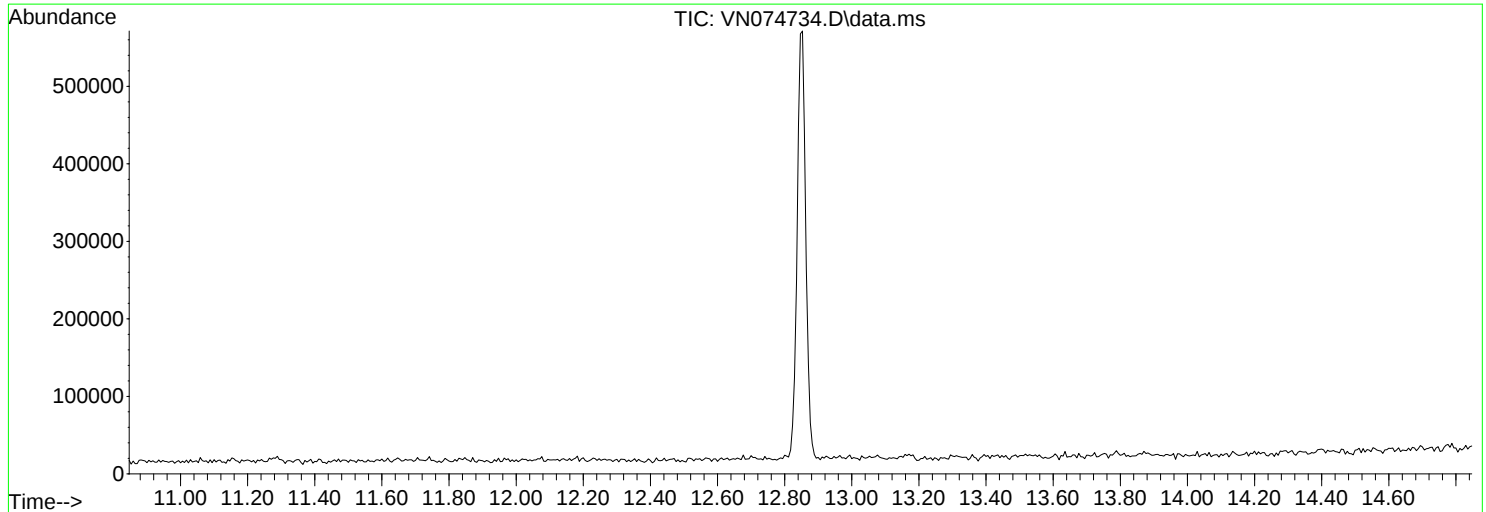

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	22004	PASS
75	95	30	60	56.8	55615	PASS
95	95	100	100	100.0	97891	PASS
96	95	5	9	7.0	6842	PASS
173	174	0.00	2	0.9	672	PASS
174	95	50	100	73.2	71640	PASS
175	174	5	9	7.3	5248	PASS
176	174	95	101	95.5	68419	PASS
177	176	5	9	6.7	4591	PASS