


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100522\
Data File : VN074743.D
Acq On : 05 Oct 2022 16:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Title : SW846 8260
Last Update : Thu Oct 06 05:37:50 2022

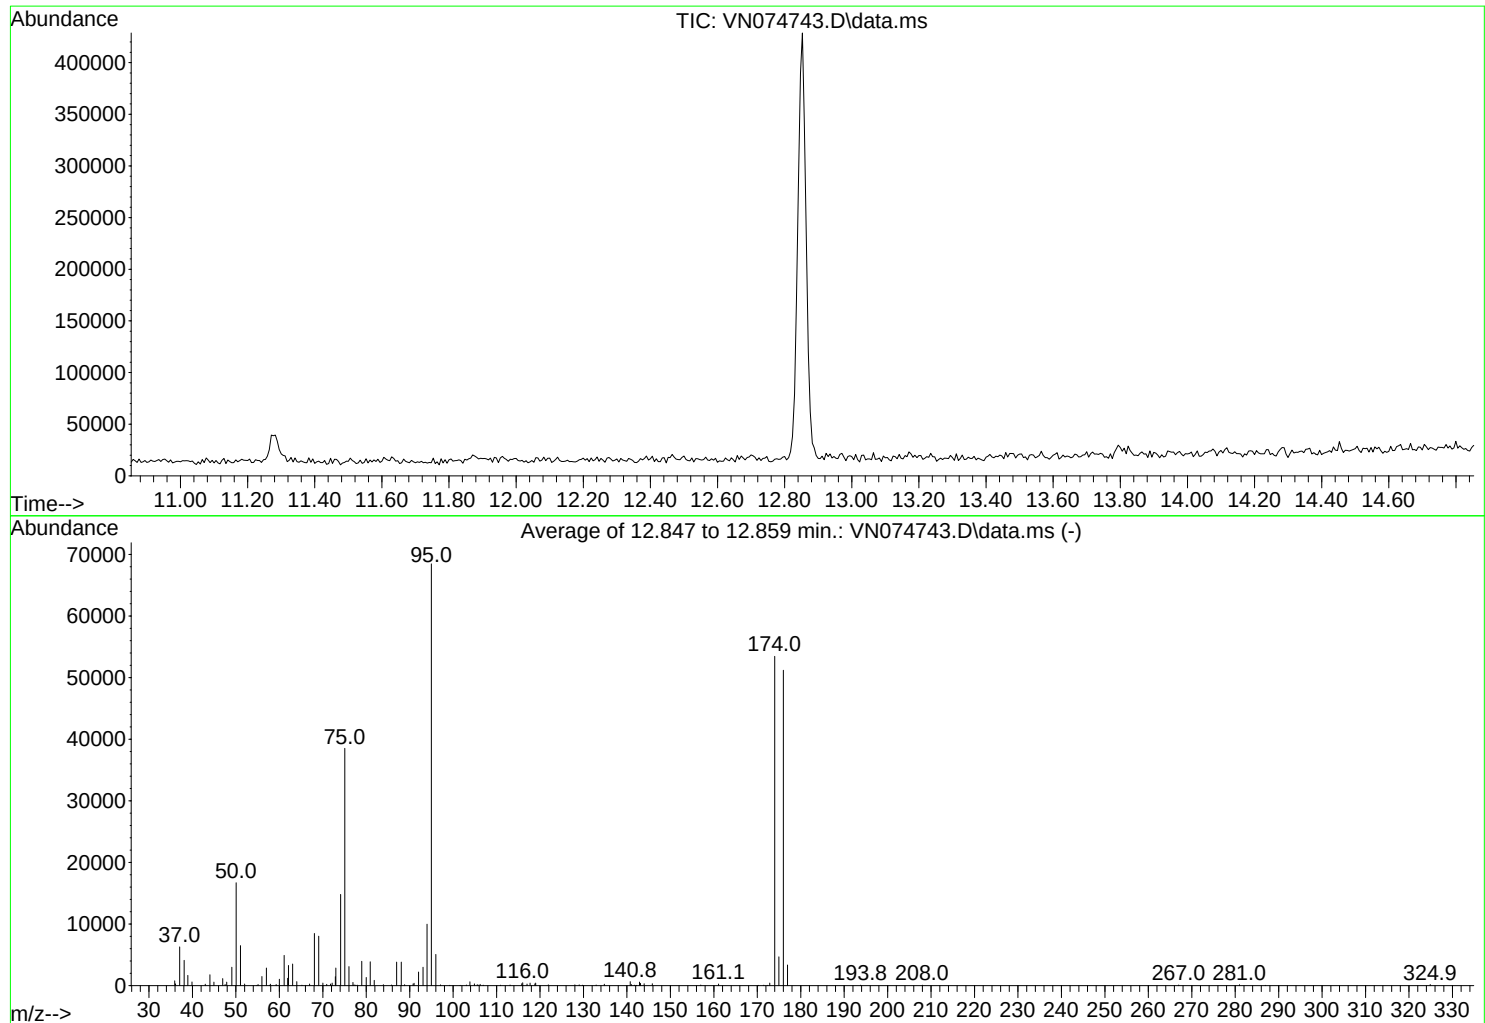

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.4	16708	PASS
75	95	30	60	56.2	38516	PASS
95	95	100	100	100.0	68485	PASS
96	95	5	9	7.4	5059	PASS
173	174	0.00	2	0.8	412	PASS
174	95	50	100	78.1	53469	PASS
175	174	5	9	8.8	4688	PASS
176	174	95	101	95.8	51211	PASS
177	176	5	9	6.6	3358	PASS