
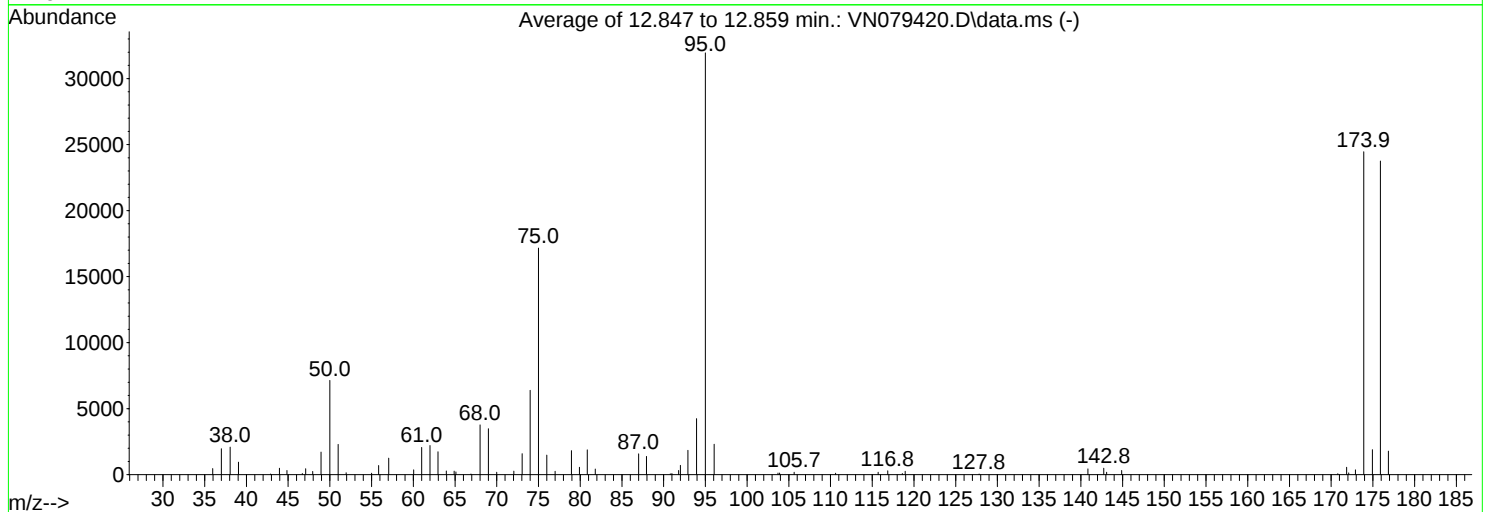


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100523\
Data File : VN079420.D
Acq On : 05 Oct 2023 15:02
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Title : SW846 8260
Last Update : Fri Oct 06 03:34:49 2023

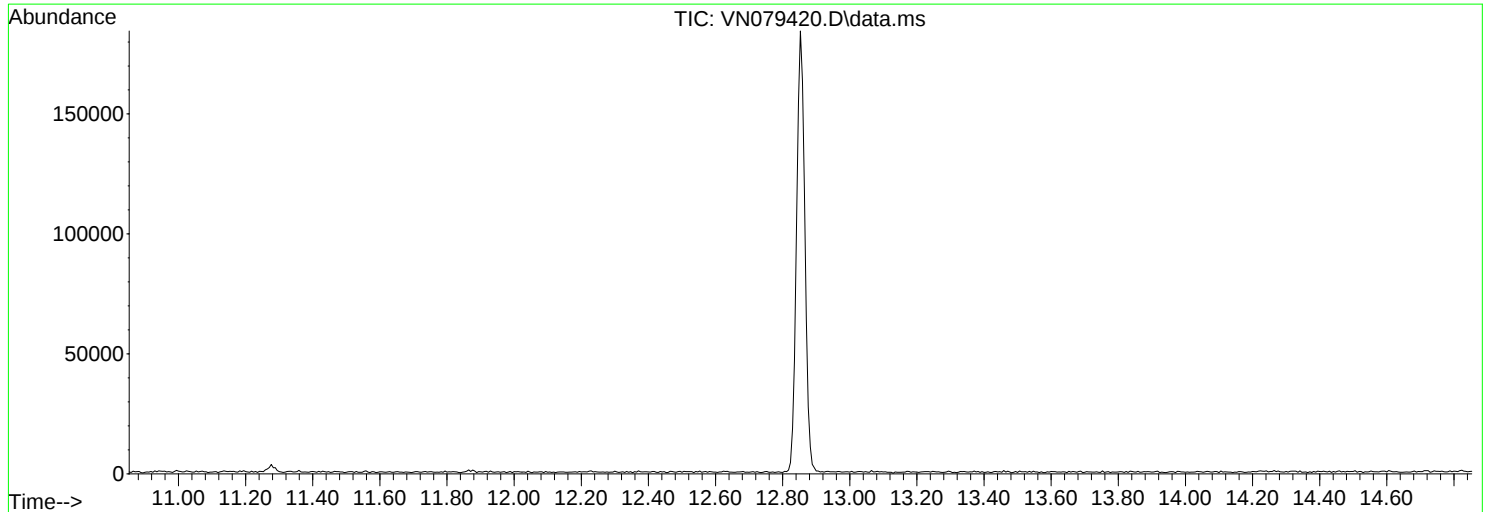

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	7137	PASS
75	95	30	60	53.7	17160	PASS
95	95	100	100	100.0	31952	PASS
96	95	5	9	7.2	2300	PASS
173	174	0.00	2	1.5	369	PASS
174	95	50	100	76.6	24461	PASS
175	174	5	9	7.7	1894	PASS
176	174	95	101	97.1	23763	PASS
177	176	5	9	7.5	1781	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	464	50.00	7137	64.90	265	77.00	251
37.00	1967	51.00	2287	65.10	202	78.95	181
38.05	2080	51.95	144	66.90	50	79.90	56
39.05	942	55.00	105	68.00	3769	80.85	187
42.90	55	55.85	694	69.00	3476	81.80	420
43.95	482	57.05	1247	70.00	186	87.00	1577
44.85	314	60.05	366	72.05	266	87.95	1389
46.70	91	61.00	2063	73.05	1590	90.80	66
47.10	452	62.00	2203	74.00	6387	91.00	83
47.95	239	62.95	1734	75.00	17160	91.80	311
48.95	1709	63.95	281	76.00	1478	92.00	707

Average of 12.847 to 12.859 min.: VN079420.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.90	1839	118.95	260	174.95	1894		
93.95	4246	127.80	52	175.90	23763		
95.00	31952	140.85	432	176.85	1781		
96.05	2300	142.75	482				
103.70	127	143.10	180				
103.90	121	144.90	315				
105.65	179	170.80	70				
110.60	106	171.85	554				
115.70	184	172.10	135				
116.85	293	172.90	369				
118.60	80	173.90	24461				

Instrument :

MSVOA_N

ClientSampleId :

BFB