

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100620\
 Data File : VN063920.D
 Acq On : 7 Oct 2020 3:05
 Operator : JC/MD
 Sample : L4242-08
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B24-100120-17-18

Quant Time: Oct 07 05:40:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	226290	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	413156	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	444401	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	180660	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	201017	53.77	ug/l	0.00
Spiked Amount			Recovery	=	107.54%	
35) Dibromofluoromethane	7.55	113	143440	50.04	ug/l	0.00
Spiked Amount			Recovery	=	100.08%	
50) Toluene-d8	10.06	98	549233	50.54	ug/l	0.00
Spiked Amount			Recovery	=	101.08%	
62) 4-Bromofluorobenzene	12.38	95	212926	52.12	ug/l	0.00
Spiked Amount			Recovery	=	104.24%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acrolein	3.57	56	63	0.249	ug/l #	14
16) Acetone	3.79	43	24501	21.290	ug/l	94
17) Carbon Disulfide	4.01	76	1937	1.011	ug/l #	68
18) Methyl Acetate	4.28	43	1769	0.592	ug/l	95
20) Methylene Chloride	4.50	84	6802	2.673	ug/l	95
25) 2-Butanone	6.80	43	2679	1.642	ug/l	97
29) Tetrahydrofuran	7.18	42	1094	1.000	ug/l #	49
31) Cyclohexane	7.62	56	6094	1.404	ug/l #	18
36) 1,1-Dichloropropene	7.63	75	19999	4.778	ug/l #	51
38) Carbon Tetrachloride	7.62	117	26017	5.543	ug/l #	14
41) Methacrylonitrile	7.15	41	372	0.201	ug/l #	41
43) Isopropyl Acetate	8.13	43	77699	11.328	ug/l	99
45) 1,2-Dichloropropane	9.23	63	1076	0.333	ug/l #	44
48) Methyl methacrylate	9.15	41	4487	1.324	ug/l #	12
51) 4-Methyl-2-Pentanone	9.96	43	8281	2.057	ug/l	95
54) cis-1,3-Dichloropropene	9.87	75	25455	4.946	ug/l #	69
56) Ethyl methacrylate	10.51	69	1857	0.442	ug/l #	1
57) 1,3-Dichloropropane	10.73	76	2582	0.515	ug/l #	43
59) 2-Hexanone	10.74	43	46711	15.621	ug/l #	55
74) N-amyl acetate	12.03	43	311	2.264	ug/l #	46
76) 1,2,3-Trichloropropane	12.38	75	119282	29.952	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	119282	86.266	ug/l #	6
86) p-Isopropyltoluene	13.27	119	43242	4.115	ug/l	97
95) Naphthalene	15.12	128	415	1.965	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100620\
Data File : VN063920.D
Acq On : 7 Oct 2020 3:05
Operator : JC/MD
Sample : L4242-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PAV-B24-100120-17-18

Quant Time: Oct 07 05:40:59 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

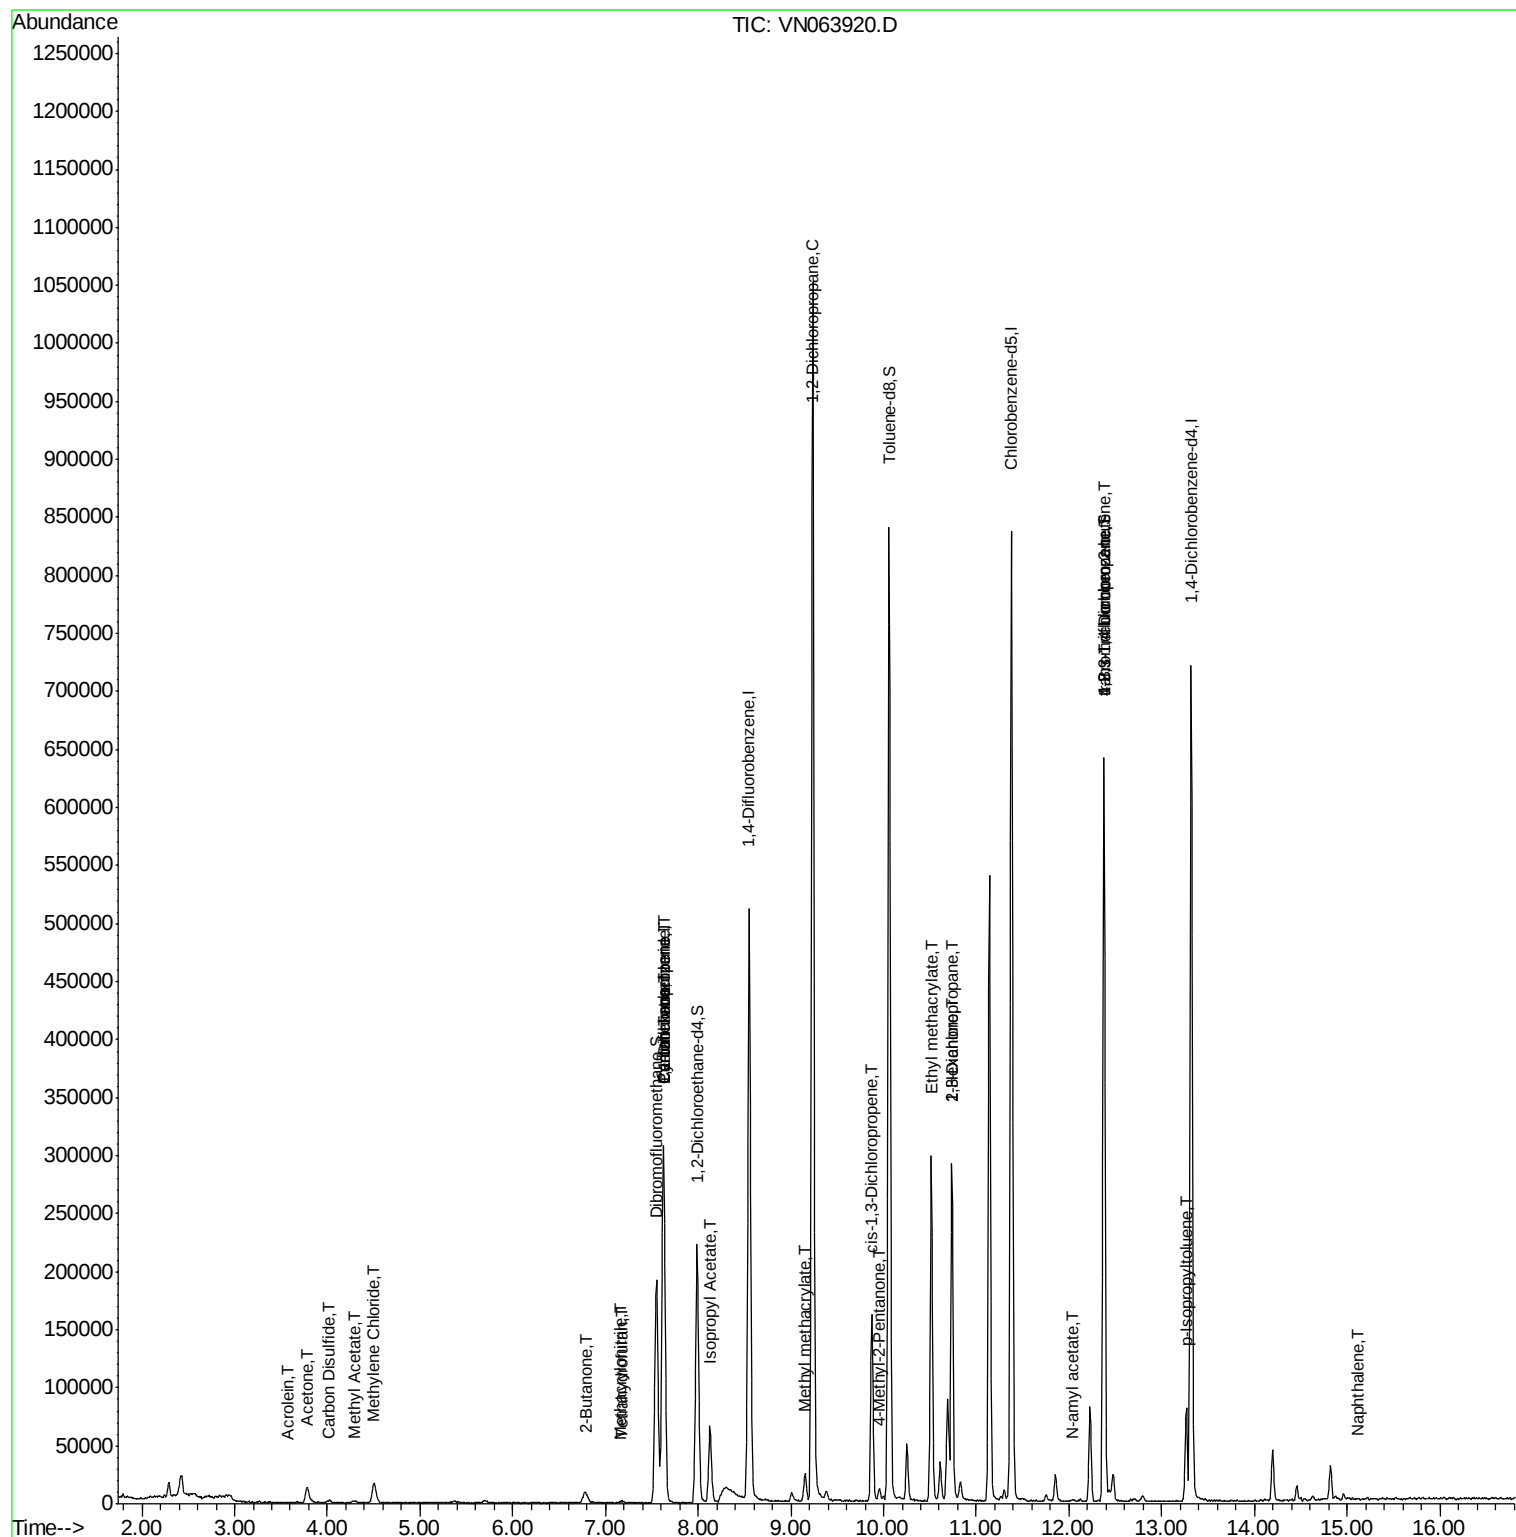



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Instrument :

MSVOA_N

ClientSampleId :


PAV-B24-100120-17-18

Tot Ion:168 Resp: 226290

Ion Ratio Lower Upper

168 100

99 65.7 51.8 77.6

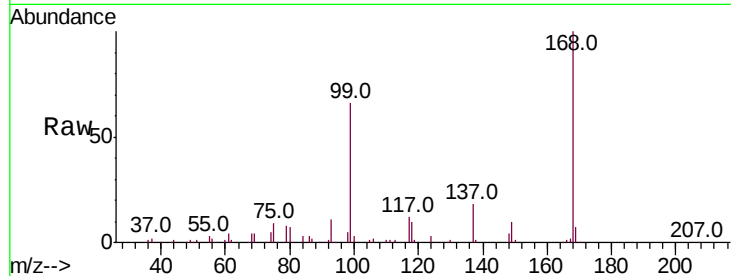

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#13

Acrolein

Concen: 0.249 ug/l

RT: 3.57 min Scan# 569

Delta R.T. 0.00 min

Lab File: VN063920.D


Acq: 7 Oct 2020 3:05

Tgt Ion: 56 Resp: 63

Ion Ratio Lower Upper

56 100

55 0.0 56.9 85.3#



Abundance Ion 56.00 (55.70 to 56.70): VN

Ion 55.00 (54.70 to 55.70): VN

3.57

200


150


100

50

0

Time--> 3.56 3.57 3.58





#16

Acetone

Concen: 21.290 ug/l

RT: 3.79 min Scan# 636

Delta R.T. 0.01 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Instrument :

MSVOA_N

ClientSampleId :





PAV-B24-100120-17-18

Tot Ion: 43 Resp: 24501

Ion Ratio Lower Upper

43 100

58 24.9 22.3 33.5

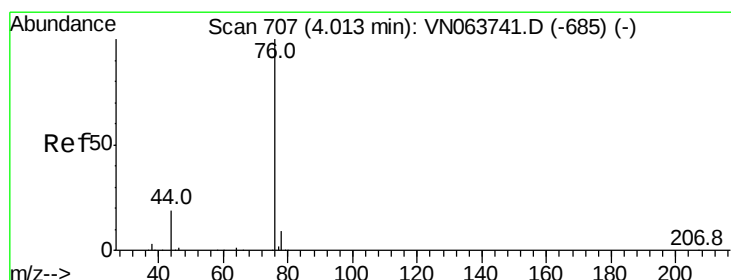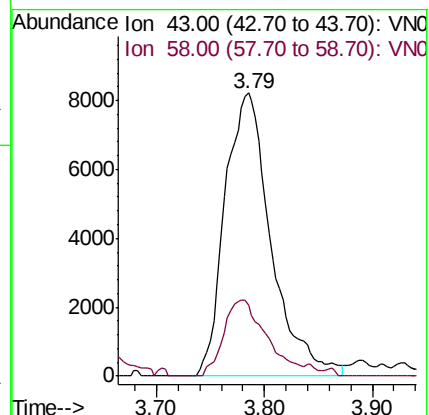

#17

Carbon Disulfide

Concen: 1.011 ug/l

RT: 4.01 min Scan# 707

Delta R.T. 0.00 min

Lab File: VN063920.D




Acq: 7 Oct 2020 3:05


Tgt Ion: 76 Resp: 1937

Ion Ratio Lower Upper

76 100

78 20.3 7.0 10.4#


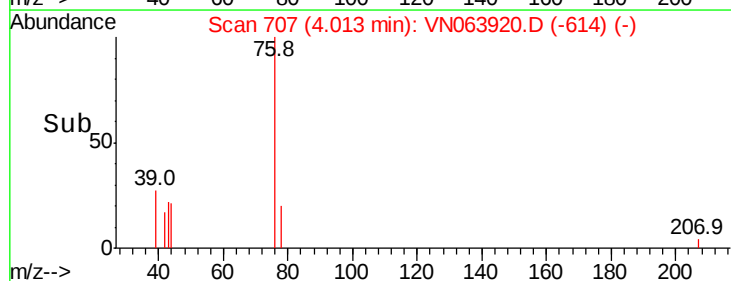
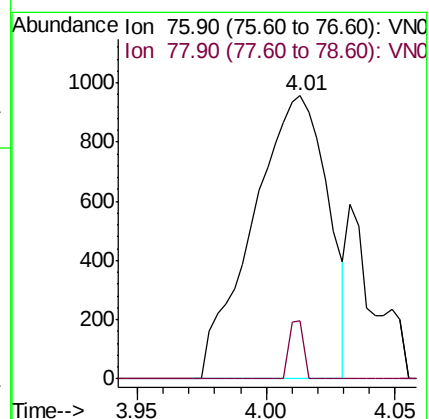
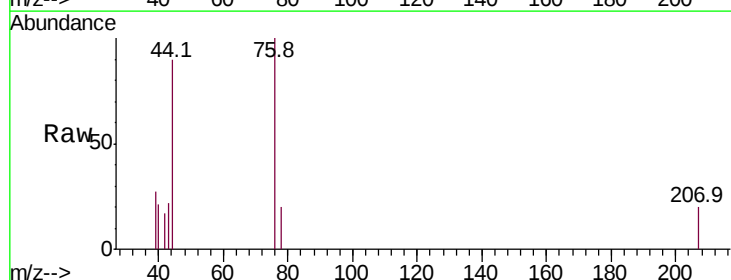




#18
Methvl Acetate
Concen: 0.592 ug/l
RT: 4.28 min Scan# 790
Delta R.T. 0.00 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05




Instrument :
MSVOA_N
ClientSampleId :
PAV-B24-100120-17-18


Tot Ion: 43 Resp: 1769
Ion Ratio Lower Upper
43 100
74 19.3 17.4 26.2

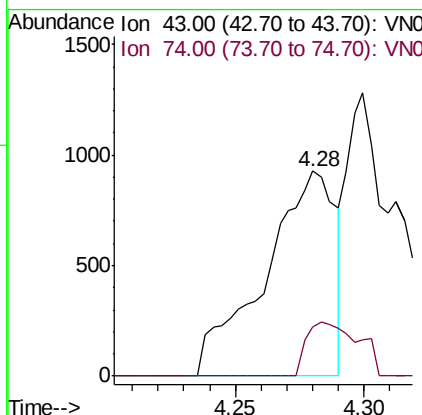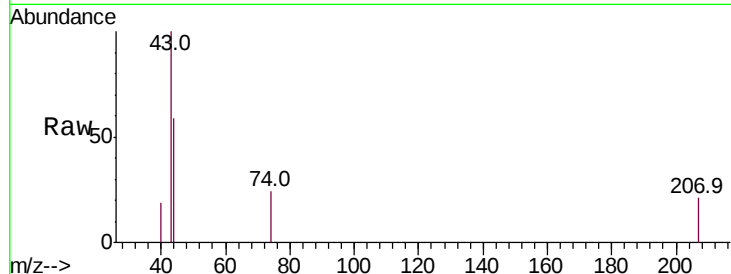

#20
Methylene Chloride
Concen: 2.673 ug/l
RT: 4.50 min Scan# 858
Delta R.T. -0.01 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05

Tgt Ion: 84 Resp: 6802
Ion Ratio Lower Upper
84 100
49 143.1 110.4 165.6
51 49.4 33.3 49.9
86 60.5 50.7 76.1



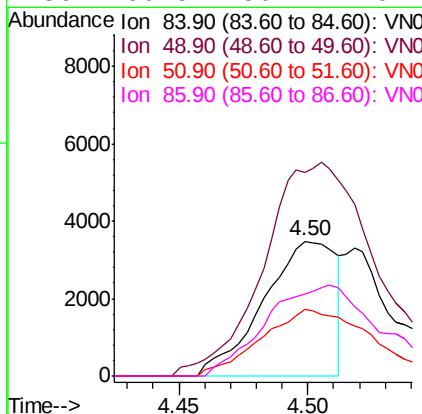





#25
2-Butanone
Concen: 1.642 ug/l
RT: 6.80 min Scan# 1575
Delta R.T. 0.02 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05




Instrument :
MSVOA_N
ClientSampleId :
PAV-B24-100120-17-18


Tot Ion: 43 Resp: 2679
Ion Ratio Lower Upper
43 100
72 22.5 19.3 28.9

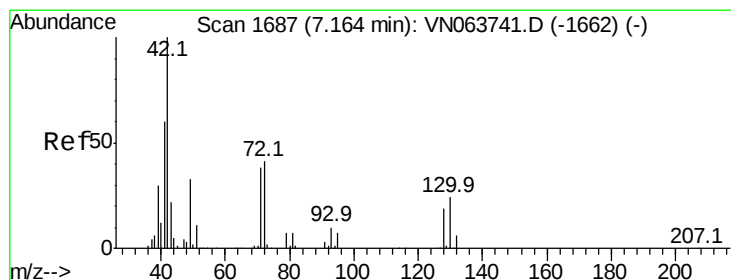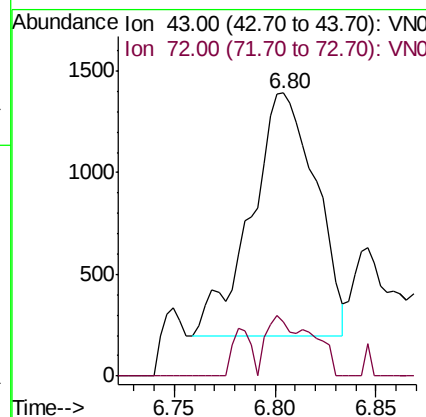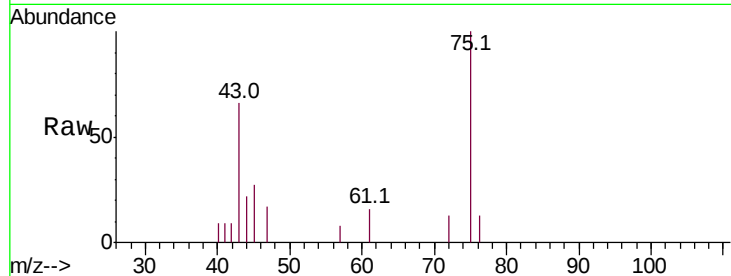

#29
Tetrahydrofuran
Concen: 1.000 ug/l
RT: 7.18 min Scan# 1692
Delta R.T. 0.02 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05

Tgt Ion: 42 Resp: 1094
Ion Ratio Lower Upper
42 100
72 12.9 32.8 49.2#
71 2.9 30.6 45.8#

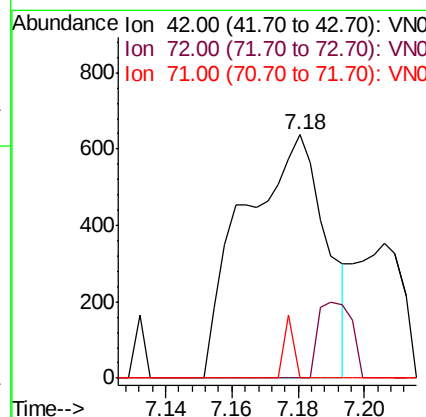


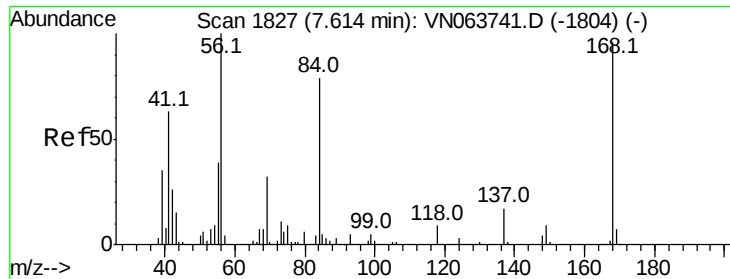




#31
Cyclohexane
Concen: 1.404 ug/l
RT: 7.62 min Scan# 1829
Delta R.T. 0.01 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05

Instrument :
MSVOA_N
ClientSampleId :
PAV-B24-100120-17-18

Tot Ion: 56 Resp: 6094
Ion Ratio Lower Upper
56 100
69 151.7 25.4 38.2#
84 103.8 63.3 94.9#

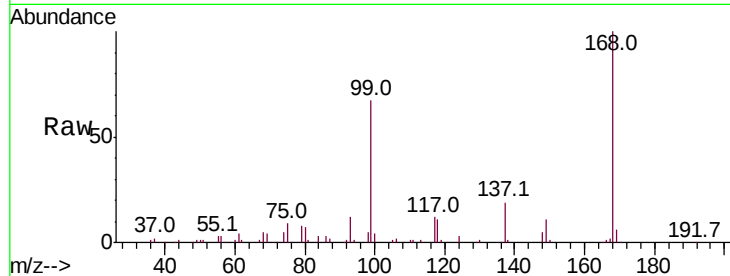


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0

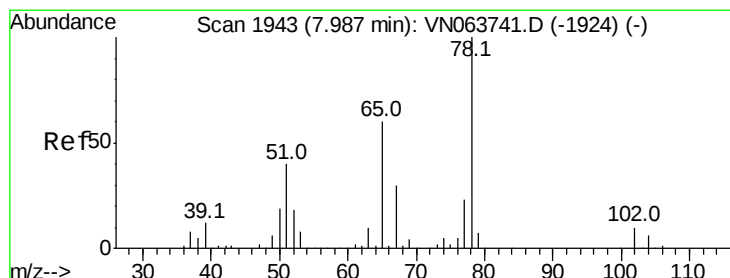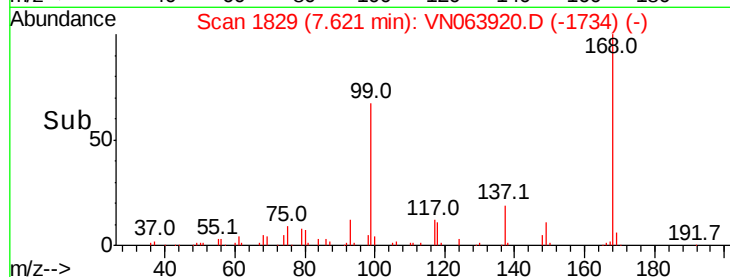
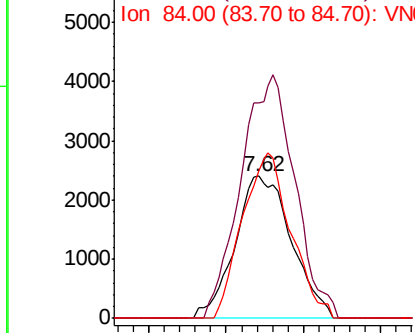



#33
1,2-Dichloroethane-d4
Concen: 53.770 ug/l
RT: 7.99 min Scan# 1943
Delta R.T. 0.00 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05

Tgt Ion: 65 Resp: 201017
Ion Ratio Lower Upper
65 100
67 49.7 0.0 99.6

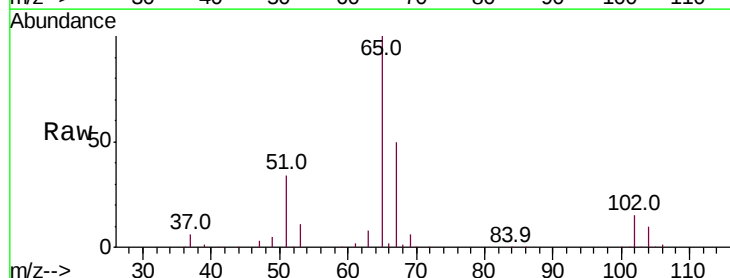

Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

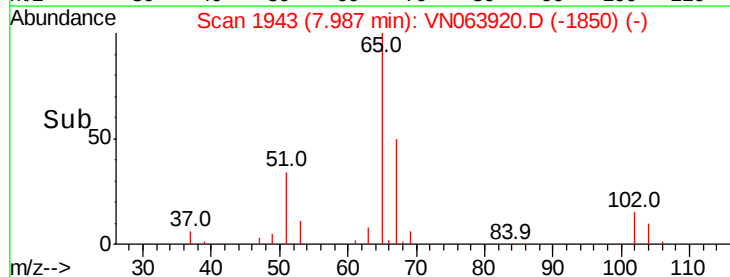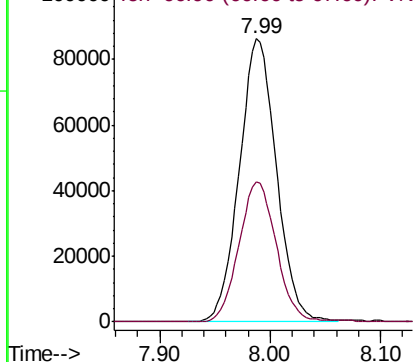

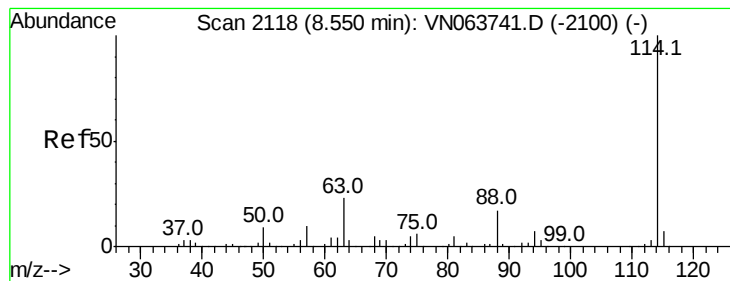

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. 0.00 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Instrument :

MSVOA_N

ClientSampleId :

PAV-B24-100120-17-18


Tot Ion:114 Resp: 413156

Ion Ratio Lower Upper

114 100

63 23.6 0.0 45.0




88 16.9 0.0 34.0

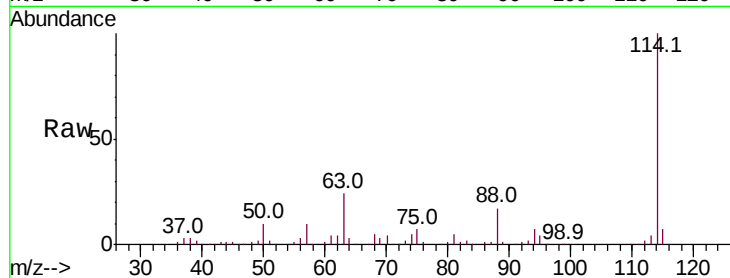

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0

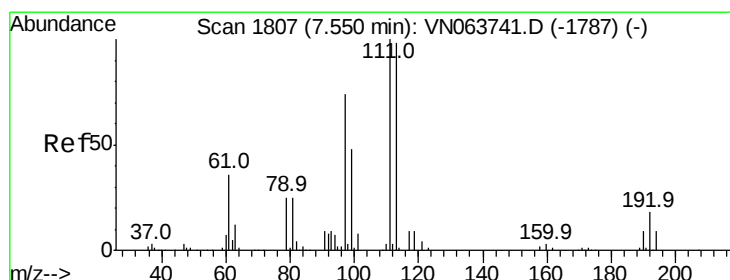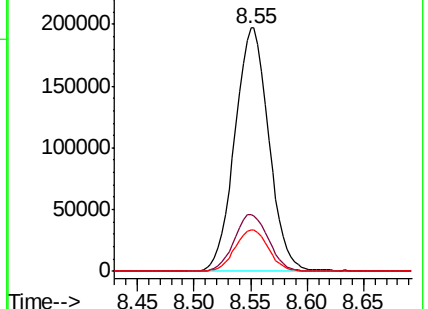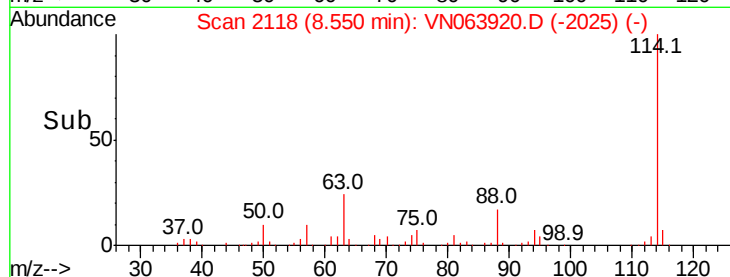

#35

Dibromofluoromethane

Concen: 50.035 ug/l

RT: 7.55 min Scan# 1807

Delta R.T. 0.00 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05


Tgt Ion:113 Resp: 143440

Ion Ratio Lower Upper

113 100

111 104.4 81.8 122.8



192 18.0 14.2 21.2

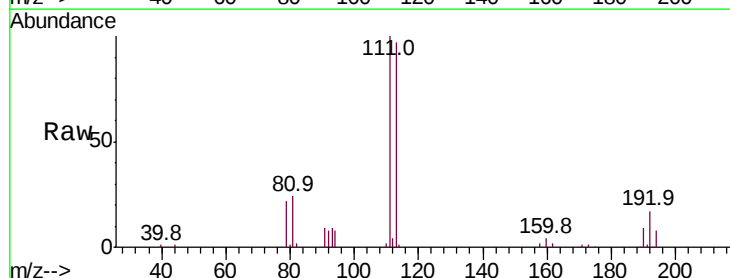


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



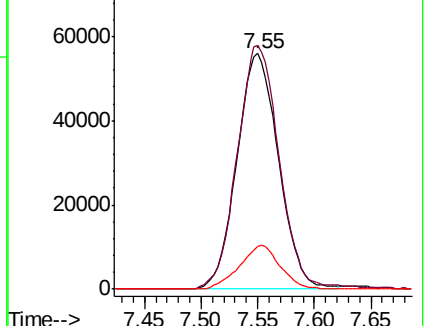
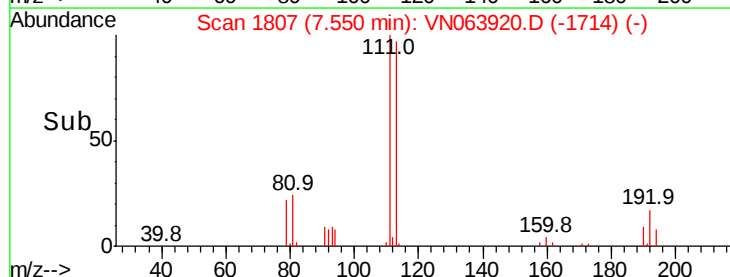




#36
 1,1-Dichloropropene
 Concen: 4.778 ug/l
 RT: 7.63 min Scan# 1831
 Delta R.T. -0.13 min
 Lab File: VN063920.D
 Acq: 7 Oct 2020 3:05




Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B24-100120-17-18


Tot Ion: 75 Resp: 19999
 Ion Ratio Lower Upper
 75 100
 110 9.0 16.9 50.6#
 77 0.0 24.5 36.7#

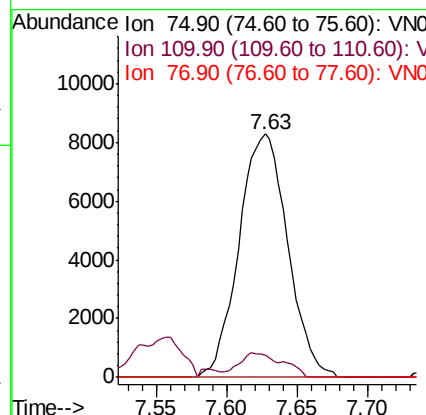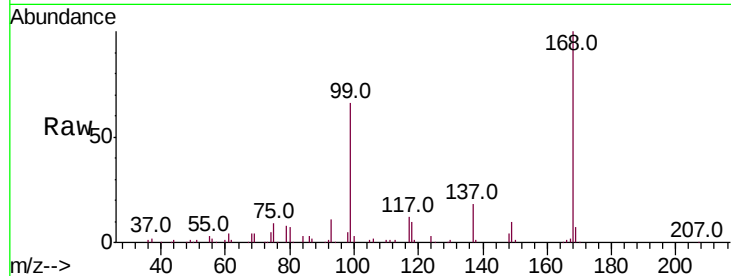

#38
 Carbon Tetrachloride
 Concen: 5.543 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.11 min
 Lab File: VN063920.D
 Acq: 7 Oct 2020 3:05

Tgt Ion: 117 Resp: 26017
 Ion Ratio Lower Upper
 117 100
 119 4.7 80.1 120.1#
 121 0.0 25.7 38.5#


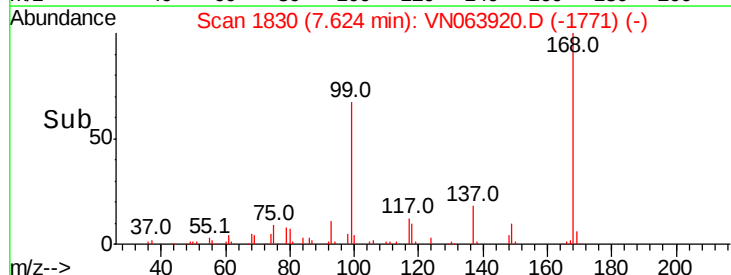
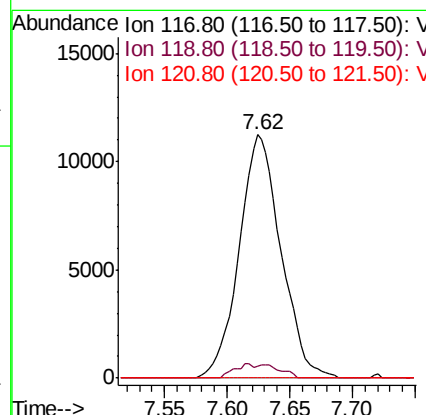



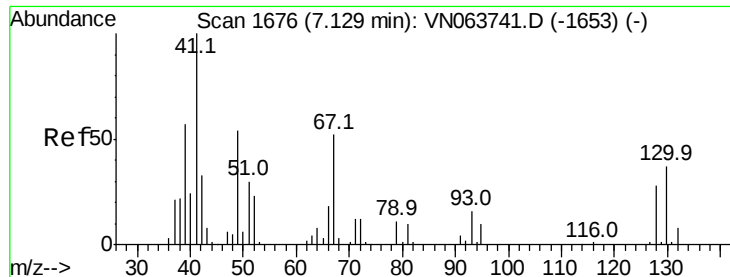

#41
Methacrylonitrile
Concen: 0.201 ug/l
RT: 7.15 min Scan# 1682
Delta R.T. 0.02 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05




Instrument :
MSVOA_N
ClientSampleId :
PAV-B24-100120-17-18


Tot Ion: 41 Resp: 372
Ion Ratio Lower Upper
41 100
39 38.2 42.5 63.7#
67 0.0 57.4 86.2#
52 0.0 26.9 40.3#

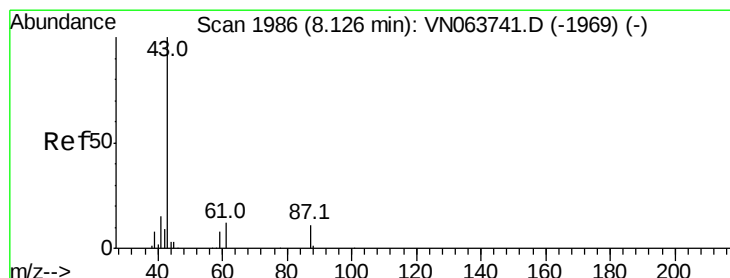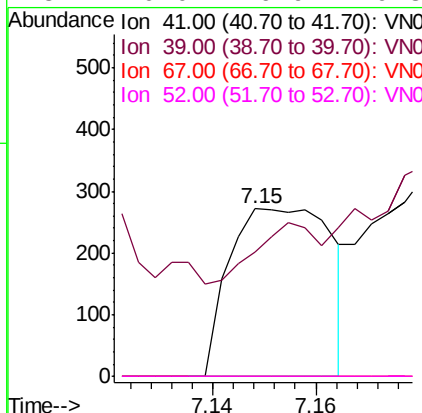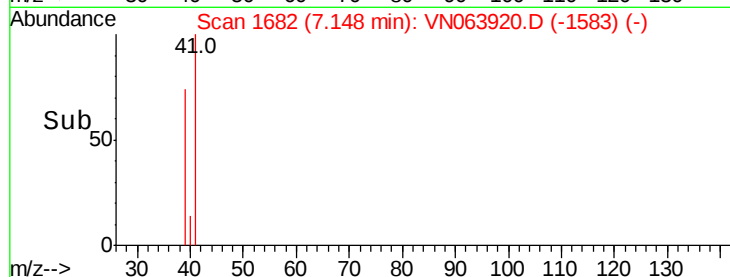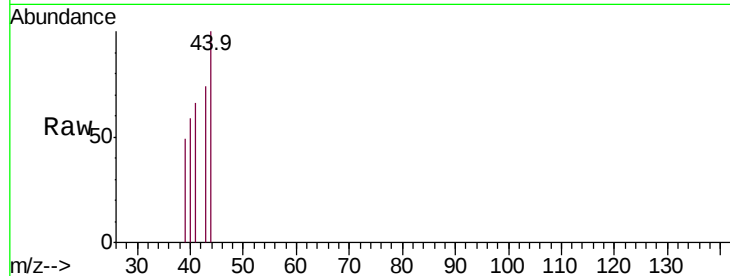

#43
Isopropyl Acetate
Concen: 11.328 ug/l
RT: 8.13 min Scan# 1987
Delta R.T. 0.00 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05

Tgt Ion: 43 Resp: 77699
Ion Ratio Lower Upper
43 100
61 17.5 14.2 21.4
87 11.4 9.0 13.6

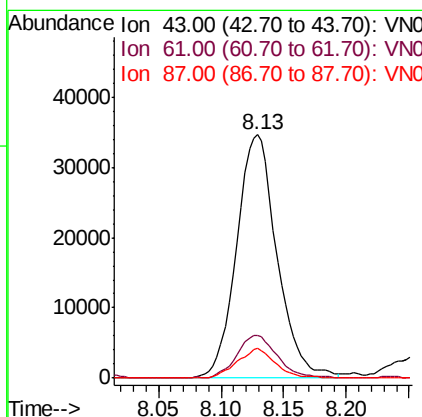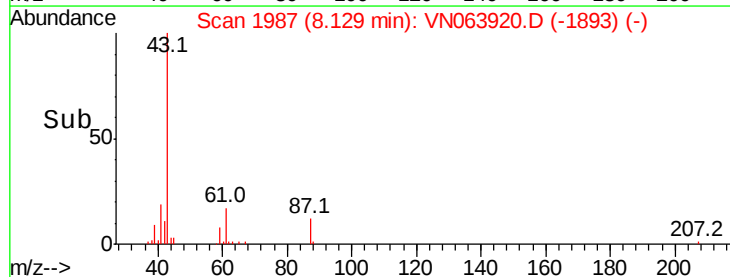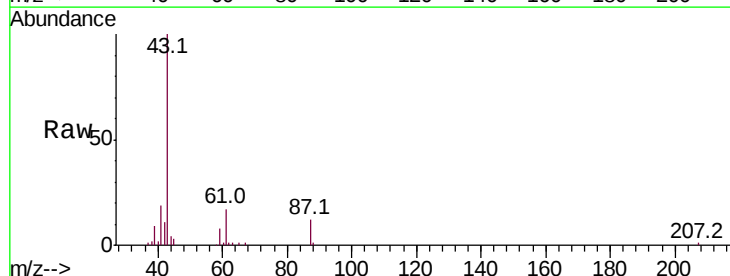



#45

1,2-Dichloropropane

Concen: 0.333 ug/l

RT: 9.23 min Scan# 2331

Delta R.T. 0.15 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Instrument :

MSVOA_N

ClientSampleId :


PAV-B24-100120-17-18

Tot Ion: 63 Resp: 1076

Ion Ratio Lower Upper

63 100

65 0.0 24.7 37.1#

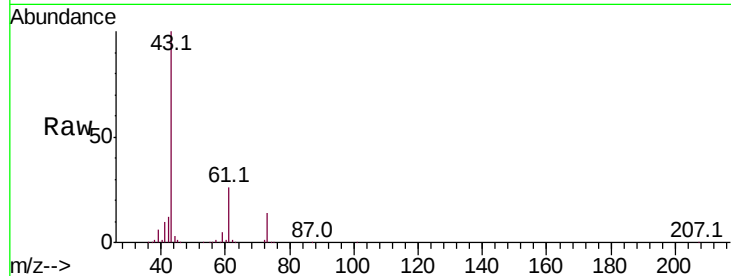

Abundance Ion 62.90 (62.60 to 63.60): VNO

Ion 64.90 (64.60 to 65.60): VNO

9.23



600

400

200

0

Time-->

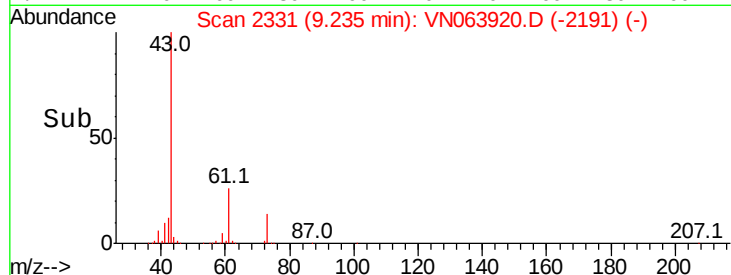

#48

Methyl methacrylate

Concen: 1.324 ug/l

RT: 9.15 min Scan# 2304

Delta R.T. -0.02 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05


Tgt Ion: 41 Resp: 4487

Ion Ratio Lower Upper

41 100

69 0.0 60.9 91.3#

39 0.0 57.5 86.3#



Abundance Ion 41.00 (40.70 to 41.70): VNO

Ion 69.00 (68.70 to 69.70): VNO

Ion 39.00 (38.70 to 39.70): VNO

80000


60000


40000

20000

0

Time-->





#50

Toluene-d8

Concen: 50.538 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Instrument :

MSVOA_N

ClientSampleId :


PAV-B24-100120-17-18

Tot Ion: 98 Resp: 549233

Ion Ratio Lower Upper

98 100

100 63.5 49.8 74.6

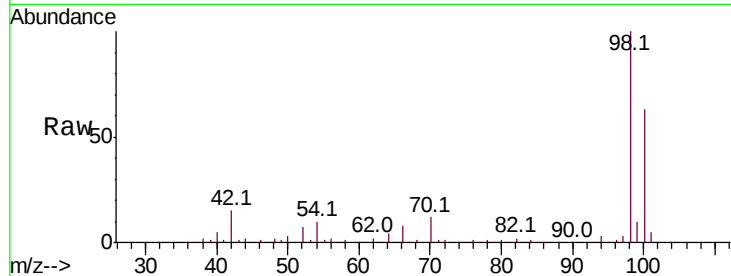

Abundance Ion 98.00 (97.70 to 98.70): VN063741.D (-2571) (-)

Ion 100.00 (99.70 to 100.70): VN063741.D (-2571) (-)

10.06



300000

200000

100000

0

Time-->



#51

4-Methyl-2-Pentanone

Concen: 2.057 ug/l

RT: 9.96 min Scan# 2555

Delta R.T. 0.00 min

Lab File: VN063920.D


Acq: 7 Oct 2020 3:05

Tgt Ion: 43 Resp: 8281

Ion Ratio Lower Upper

43 100

58 32.8 28.4 42.6



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-2537) (-)

Ion 58.00 (57.70 to 58.70): VN063741.D (-2537) (-)

9.96

5000

4000


3000


2000

1000

0

Time-->






#54




cis-1,3-Dichloropropene
Concen: 4.946 ug/l
RT: 9.87 min Scan# 2530
Delta R.T. 0.07 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05

Instrument :
MSVOA_N
ClientSampleId :
PAV-B24-100120-17-18

Tot Ion: 75 Resp: 25455
Ion Ratio Lower Upper
75 100
77 0.0 24.6 36.8#
39 48.3 49.7 74.5#

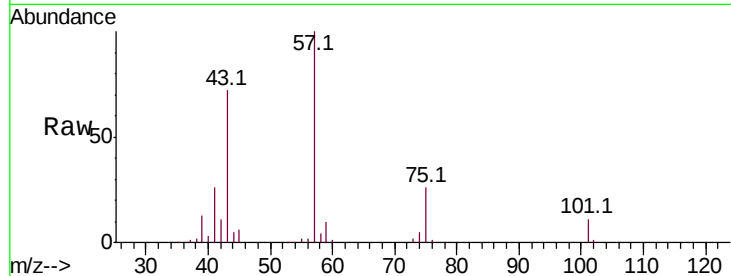


Abundance Ion 74.90 (74.60 to 75.60): VN0
Ion 76.90 (76.60 to 77.60): VN0
Ion 39.00 (38.70 to 39.70): VN0

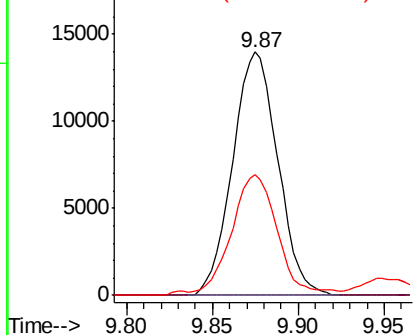



#56


Ethyl methacrylate
Concen: 0.442 ug/l
RT: 10.51 min Scan# 2729
Delta R.T. 0.12 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05

Tgt Ion: 69 Resp: 1857
Ion Ratio Lower Upper
69 100
41 3456.0 61.1 91.7#
39 1655.3 42.2 63.4#

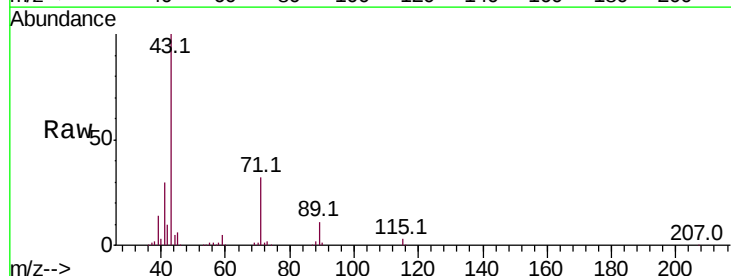

Abundance Ion 69.00 (68.70 to 69.70): VN0
Ion 41.00 (40.70 to 41.70): VN0
Ion 39.00 (38.70 to 39.70): VN0

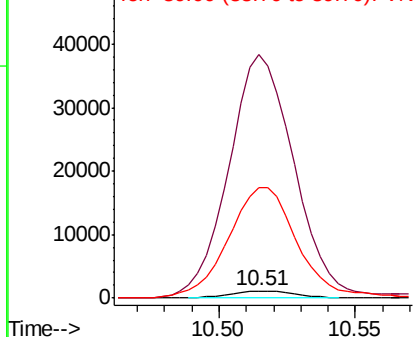



#57

1,3-Dichloropropane

Concen: 0.515 ug/l

RT: 10.73 min Scan# 2797

Delta R.T. 0.05 min





Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Instrument :
MSVOA_N
ClientSampleId :
PAV-B24-100120-17-18

Tot Ion: 76 Resp: 2582

Ion	Ratio	Lower	Upper
76	100		
78	0.0	25.2	37.8#

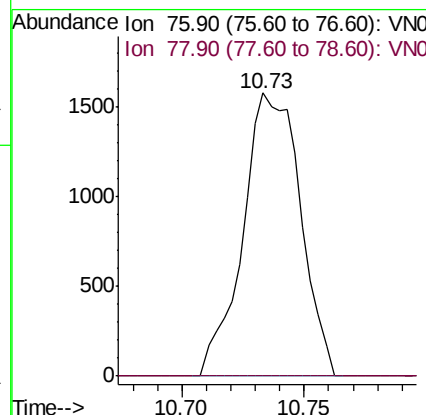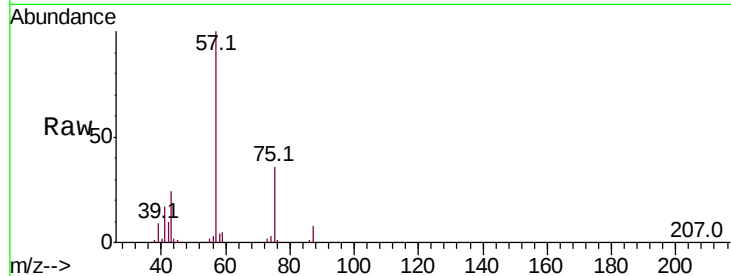

#59

2-Hexanone

Concen: 15.621 ug/l

RT: 10.74 min Scan# 2798




Delta R.T. 0.02 min


Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Tgt Ion: 43 Resp: 46711

Ion	Ratio	Lower	Upper
43	100		
58	18.8	24.6	73.8#



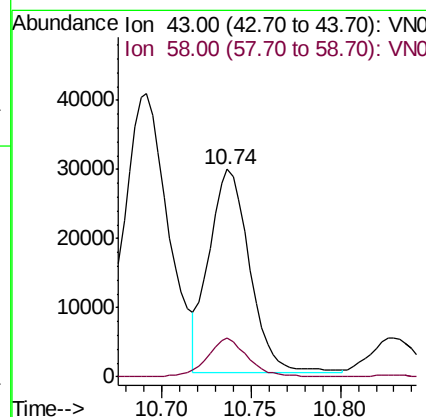



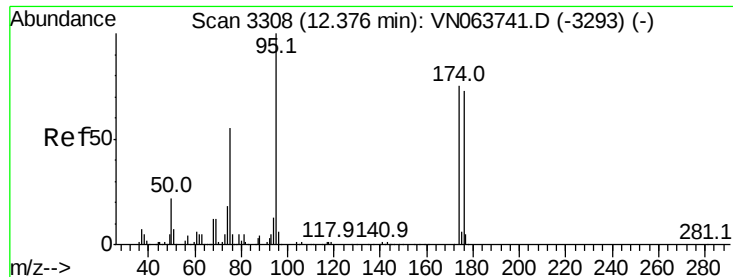

#62
4-Bromofluorobenzene
Concen: 52.120 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05




Instrument :
MSVOA_N
ClientSampleId :
PAV-B24-100120-17-18


Tot Ion	95	Resp	212926
Ion Ratio	100		
Lower		0.0	150.6
Upper		0.0	145.4

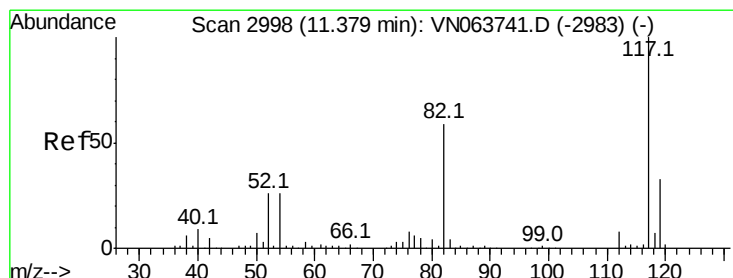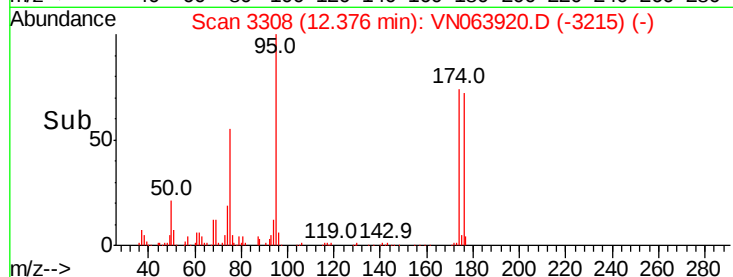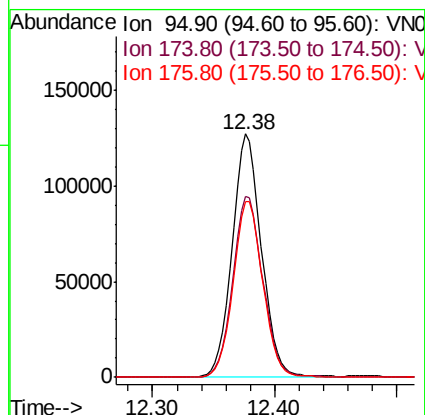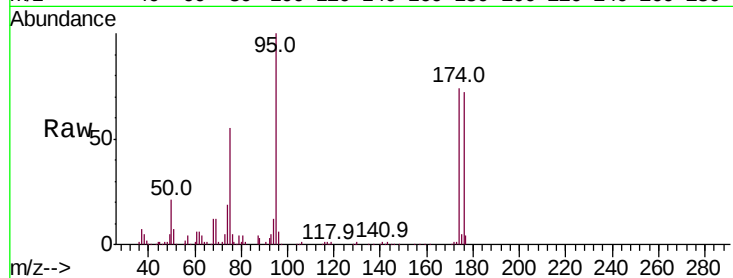

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063920.D
Acq: 7 Oct 2020 3:05

Tgt Ion	117	Resp	444401
Ion Ratio	100		
Lower		47.4	71.2
Upper		26.4	39.6

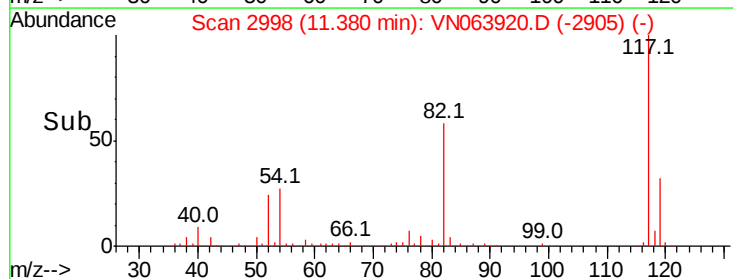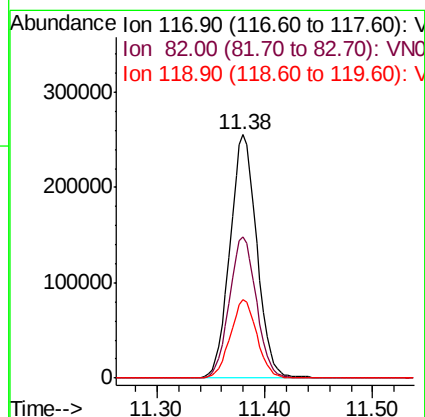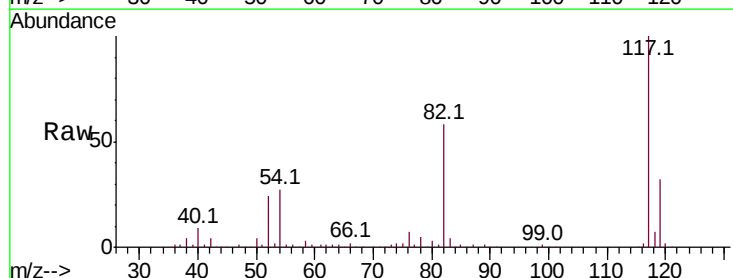



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Instrument :

MSVOA_N

ClientSampleId :

PAV-B24-100120-17-18


Tot Ion:152 Resp: 180660

Ion Ratio Lower Upper

152 100

115 61.6 31.3 93.8




150 154.9 0.0 341.8



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

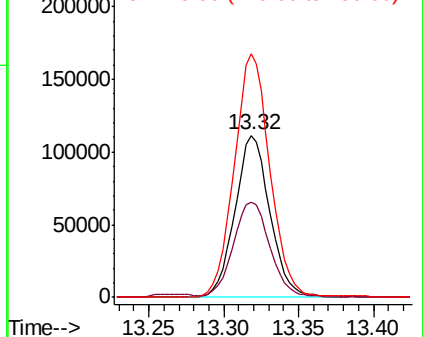

#74

N-ethyl acetate

Concen: 2.264 ug/l

RT: 12.03 min Scan# 3199

Delta R.T. -0.02 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Tgt Ion: 43 Resp: 311


Ion Ratio Lower Upper

43 100

70 0.0 29.8 44.8#

55 0.0 17.9 26.9#

61 0.0 17.0 25.4#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V

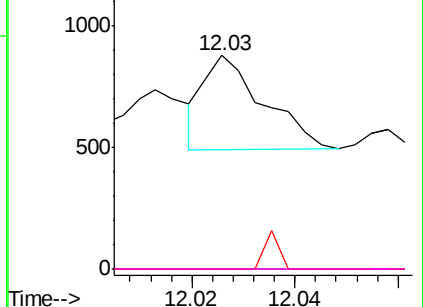



#76

1,2,3-Trichloropropane

Concen: 29.952 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05

Instrument :

MSVOA_N

ClientSampleId :


PAV-B24-100120-17-18

Tot Ion: 75 Resp: 119282

Ion Ratio Lower Upper




75 100

77 1.0 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

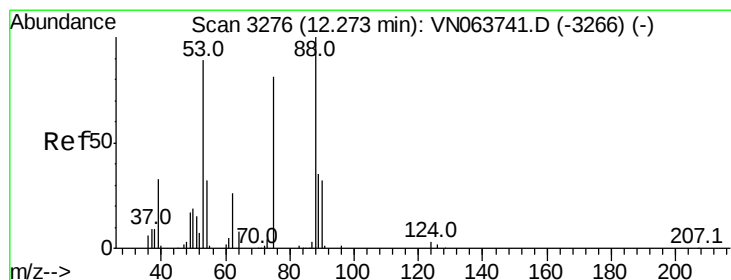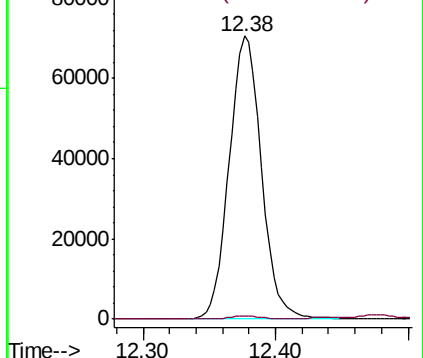

#81

trans-1,4-Dichloro-2-butene

Concen: 86.266 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN063920.D

Acq: 7 Oct 2020 3:05


Tgt Ion: 75 Resp: 119282

Ion Ratio Lower Upper

75 100

53 0.0 88.2 132.2#



89 0.0 36.0 54.0#




Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0

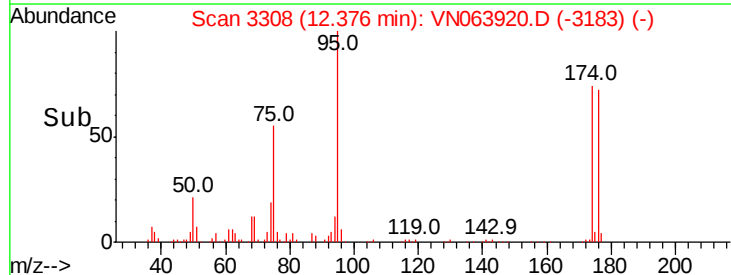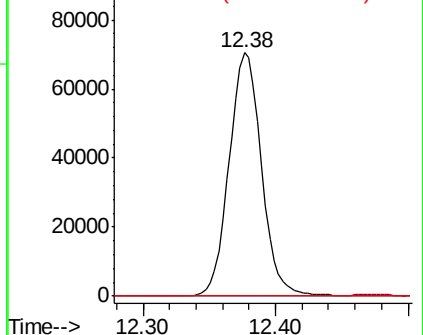







#86
 p-Isopropyltoluene
 Concen: 4.115 ug/l
 RT: 13.27 min Scan# 3585
 Delta R.T. 0.00 min
 Lab File: VN063920.D
 Acq: 7 Oct 2020 3:05

Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B24-100120-17-18

Tot Ion:119 Resp: 43242
 Ion Ratio Lower Upper
 119 100
 134 24.2 12.6 37.8
 91 28.4 13.4 40.2

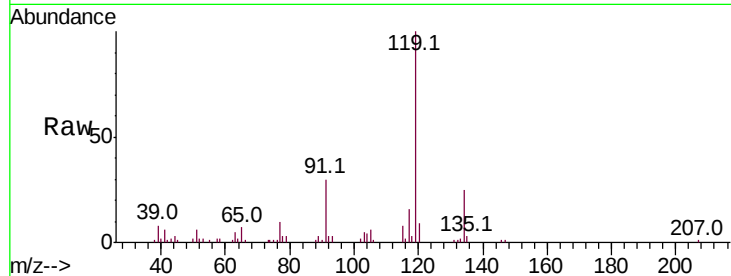


Abundance Ion 119.00 (118.70 to 119.70): V
 Ion 134.00 (133.70 to 134.70): V
 Ion 91.00 (90.70 to 91.70): V

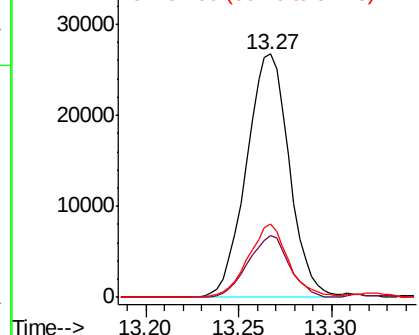

#95
 Naphthalene
 Concen: 1.965 ug/l
 RT: 15.12 min Scan# 4161
 Delta R.T. 0.02 min
 Lab File: VN063920.D
 Acq: 7 Oct 2020 3:05

Tgt Ion:128 Resp: 415
 Ion Ratio Lower Upper
 128 100
 127 0.0 10.5 15.7#
 129 0.0 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 127.00 (126.70 to 127.70): V
 Ion 129.00 (128.70 to 129.70): V

