


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100620\
 Data File : VN063887.D
 Acq On : 6 Oct 2020 8:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N100620W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Oct 06 16:42:38 2020

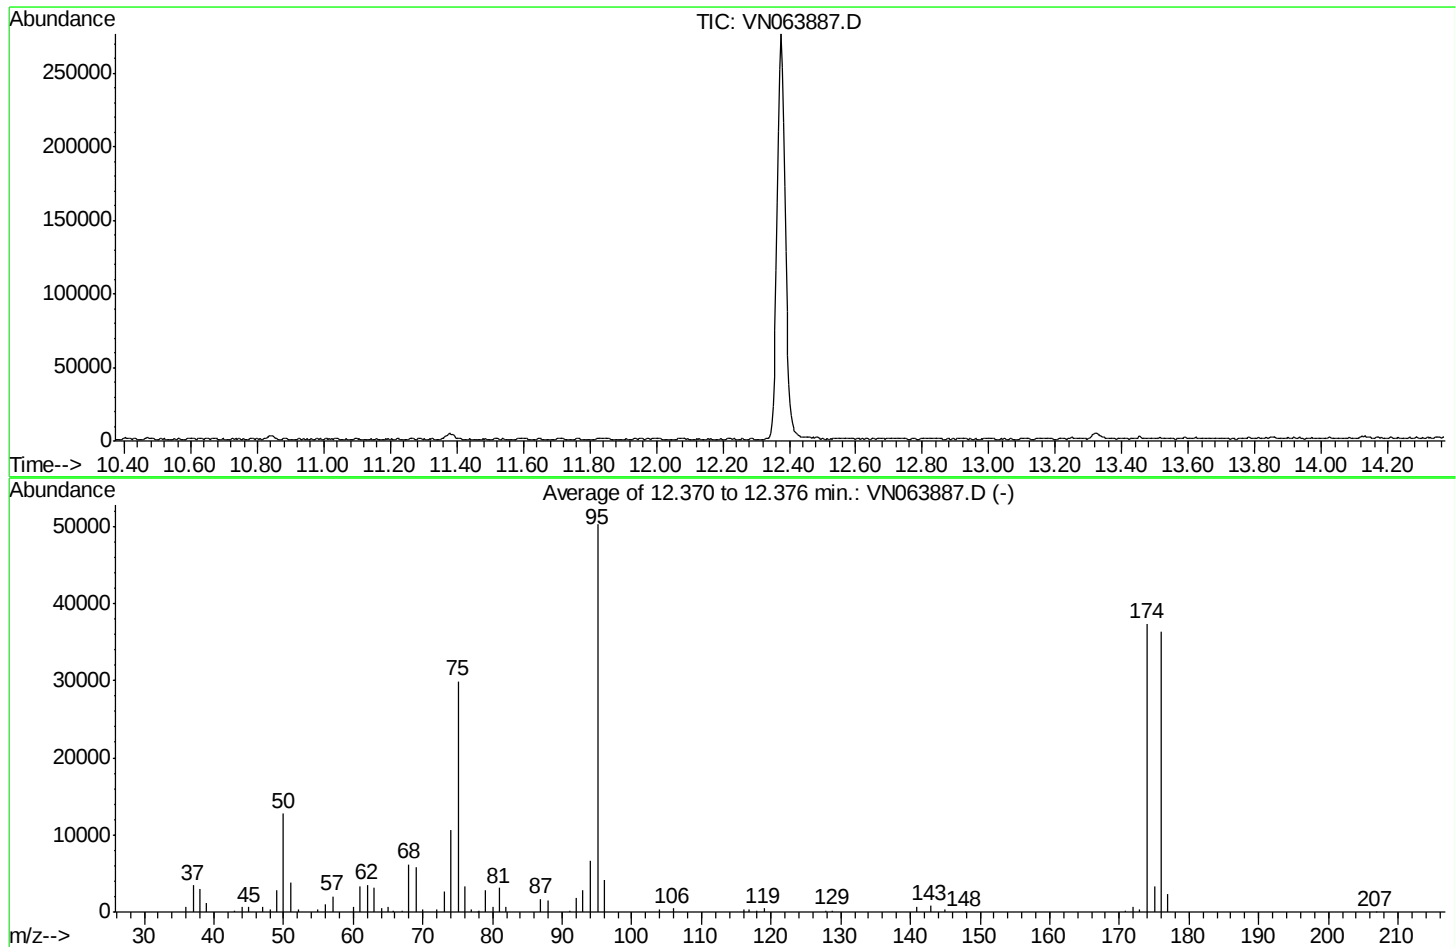

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.3	12733	PASS
75	95	30	60	59.5	29909	PASS
95	95	100	100	100.0	50261	PASS
96	95	5	9	8.2	4135	PASS
173	174	0.00	2	1.1	394	PASS
174	95	50	100	74.4	37373	PASS
175	174	5	9	8.8	3285	PASS
176	174	95	101	97.4	36394	PASS
177	176	5	9	6.2	2257	PASS