


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100620\
 Data File : VN063909.D
 Acq On : 6 Oct 2020 21:54
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Title : SW846 8260
 Last Update : Thu Oct 01 01:46:38 2020

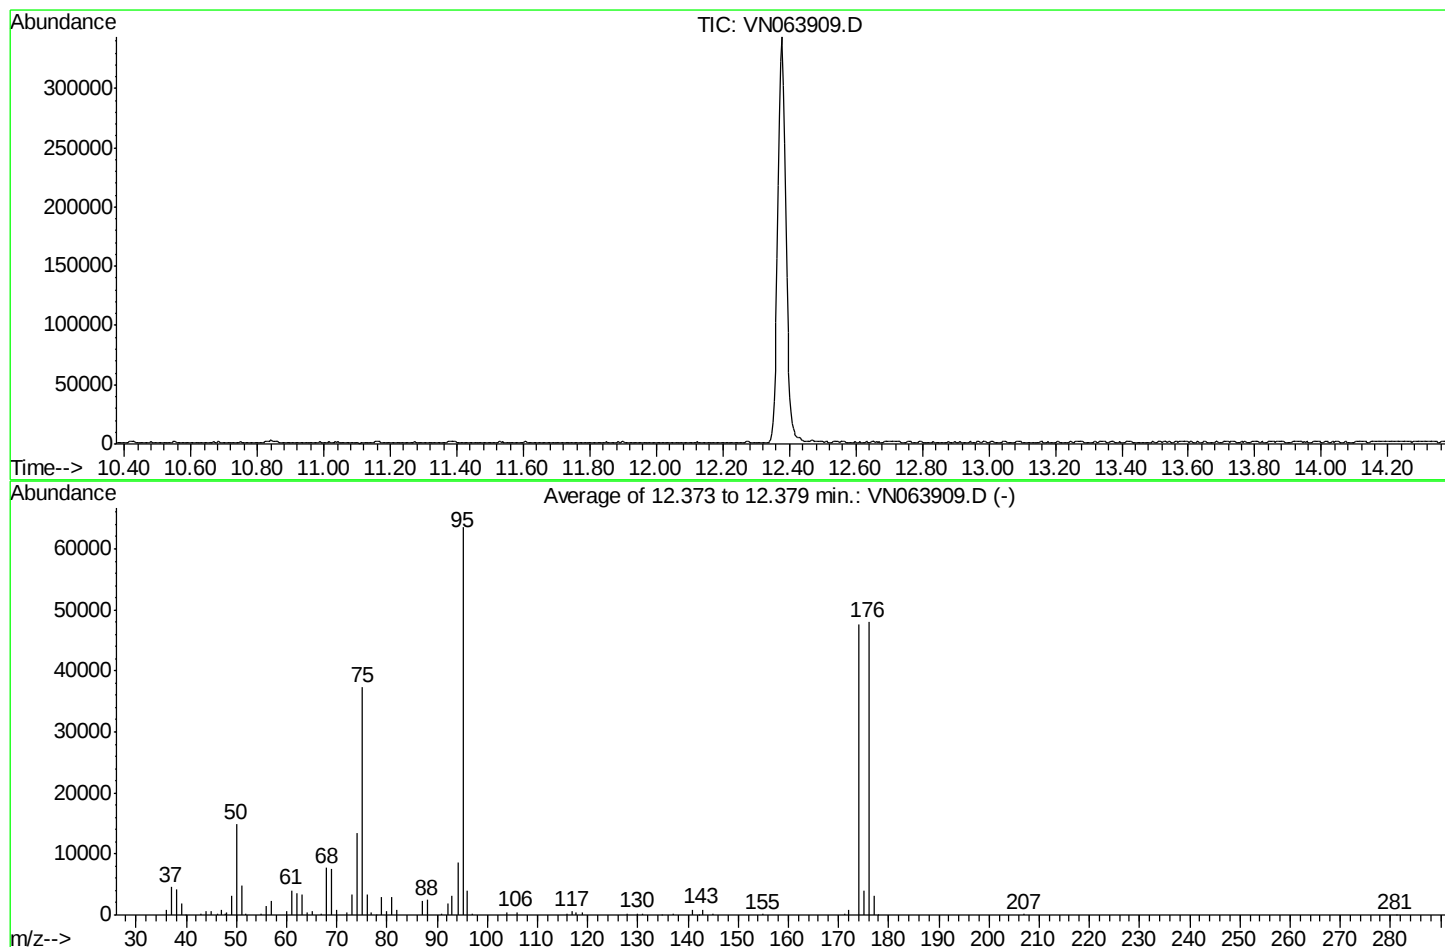

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	14843	PASS
75	95	30	60	58.7	37298	PASS
95	95	100	100	100.0	63533	PASS
96	95	5	9	6.3	3973	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.9	47562	PASS
175	174	5	9	8.3	3944	PASS
176	174	95	101	100.8	47957	PASS
177	176	5	9	6.8	3256	PASS