


Chloromethane

Response Ratio

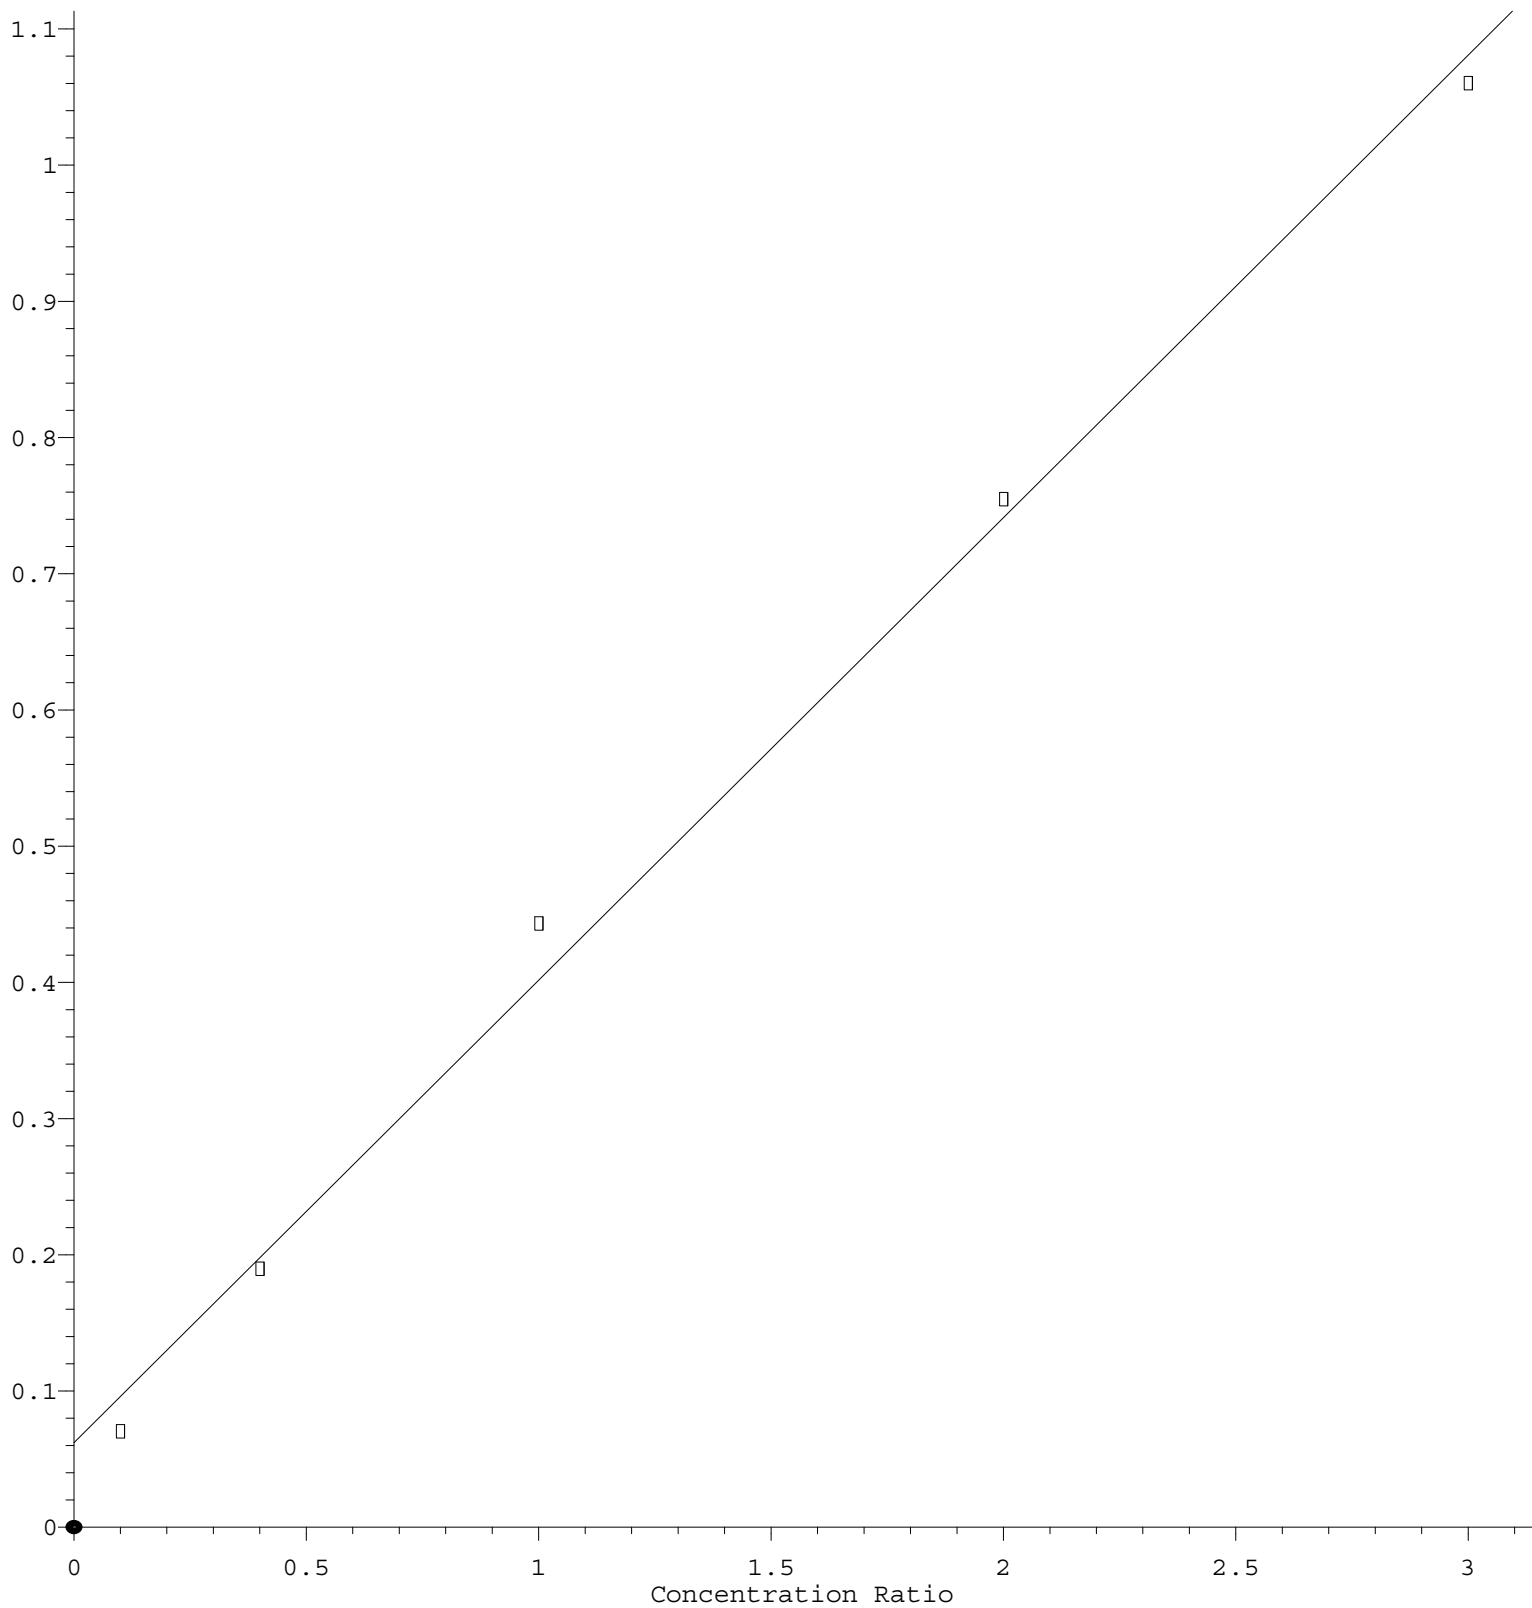

$$\text{Response} = 3.396\text{e-}001 * \text{Amt} + 6.217\text{e-}002$$


Coef of Det (r^2) = 0.995379 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

Vinyl Chloride


Response Ratio

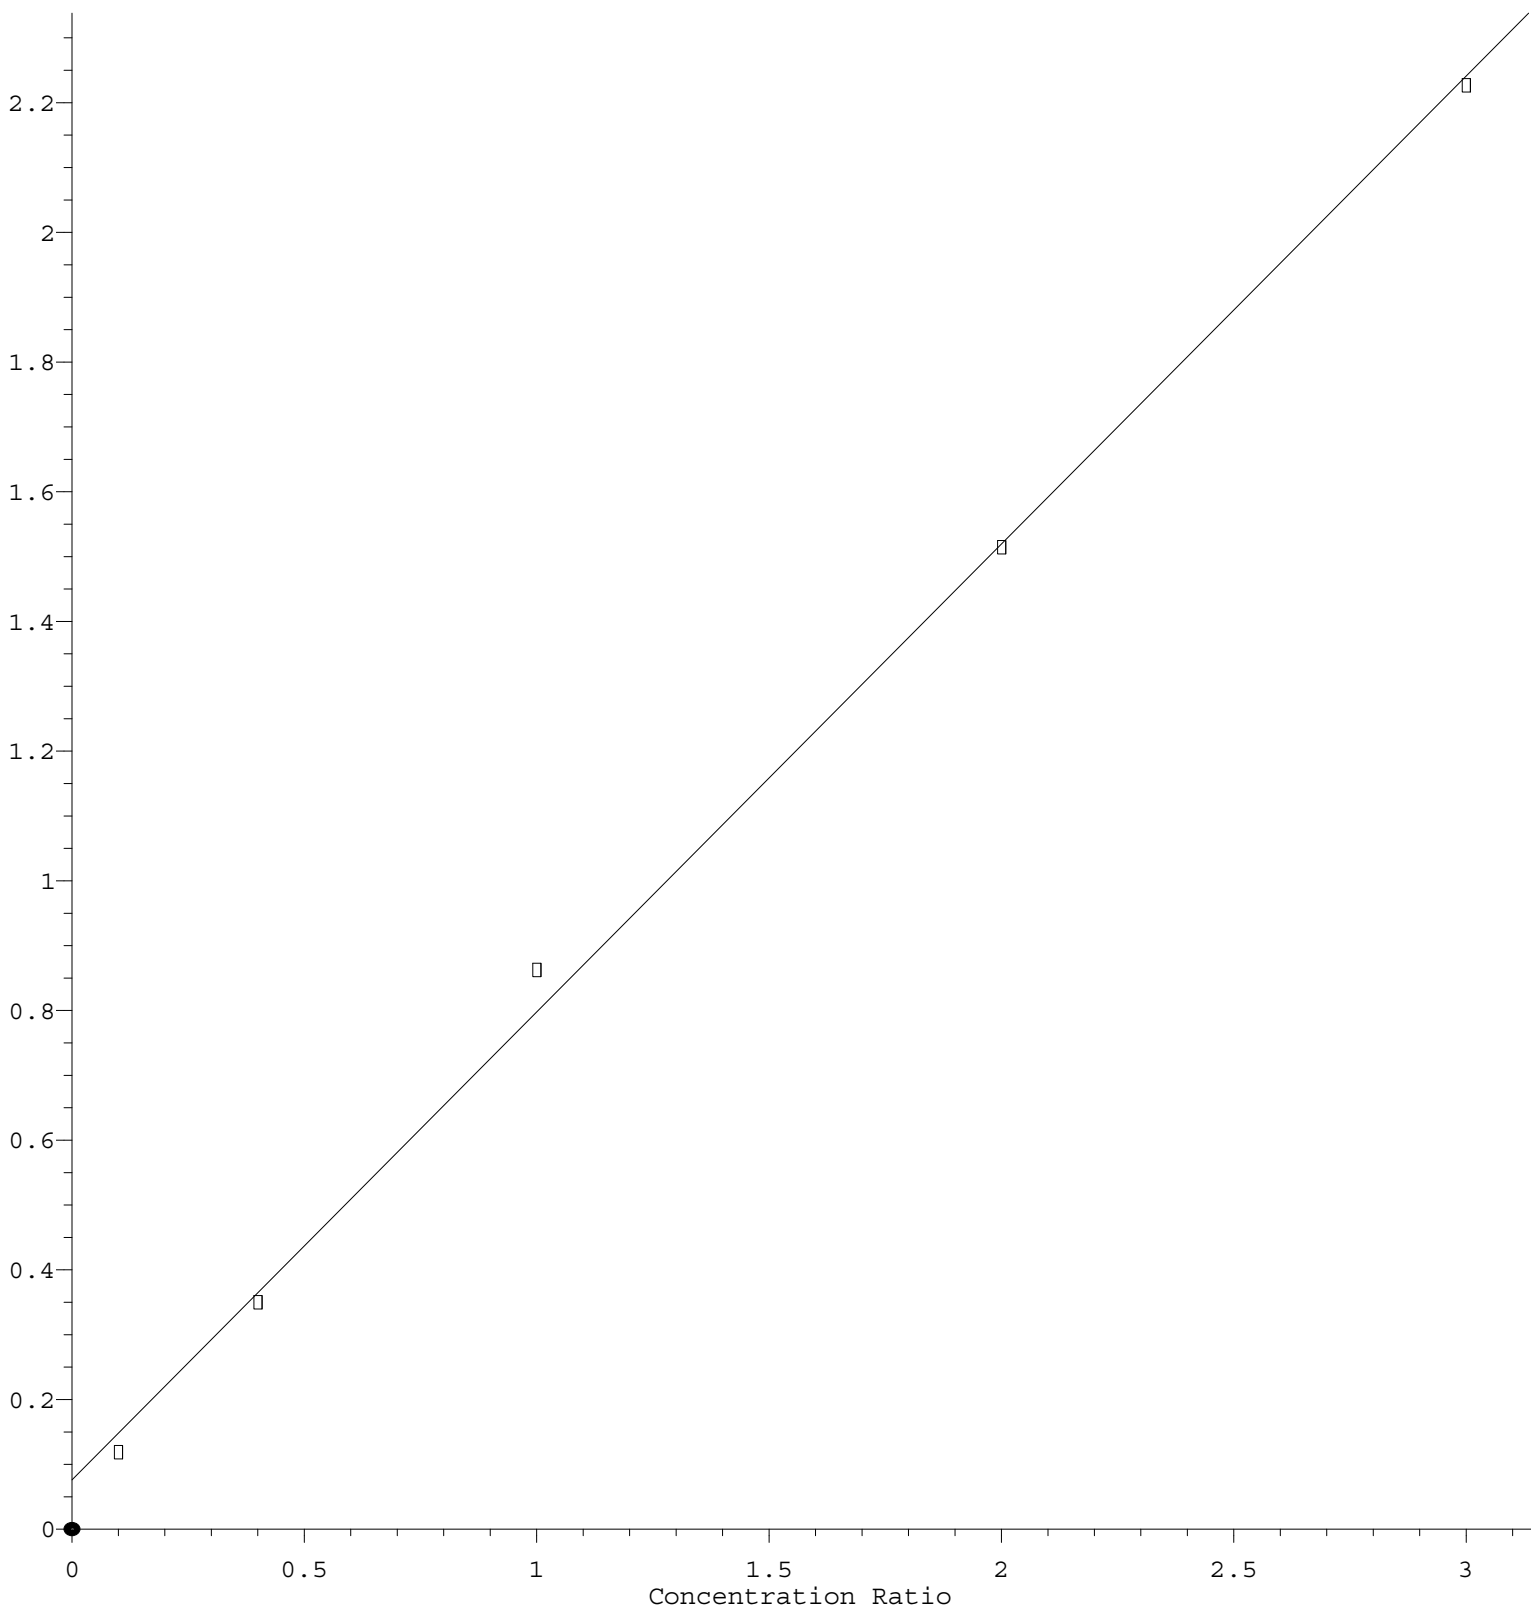

$\text{Response} = 7.220\text{e-}001 * \text{Amt} + 7.585\text{e-}002$
 Coef of Det (r^2) = 0.998159 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M
 Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

Chloroethane

Response Ratio

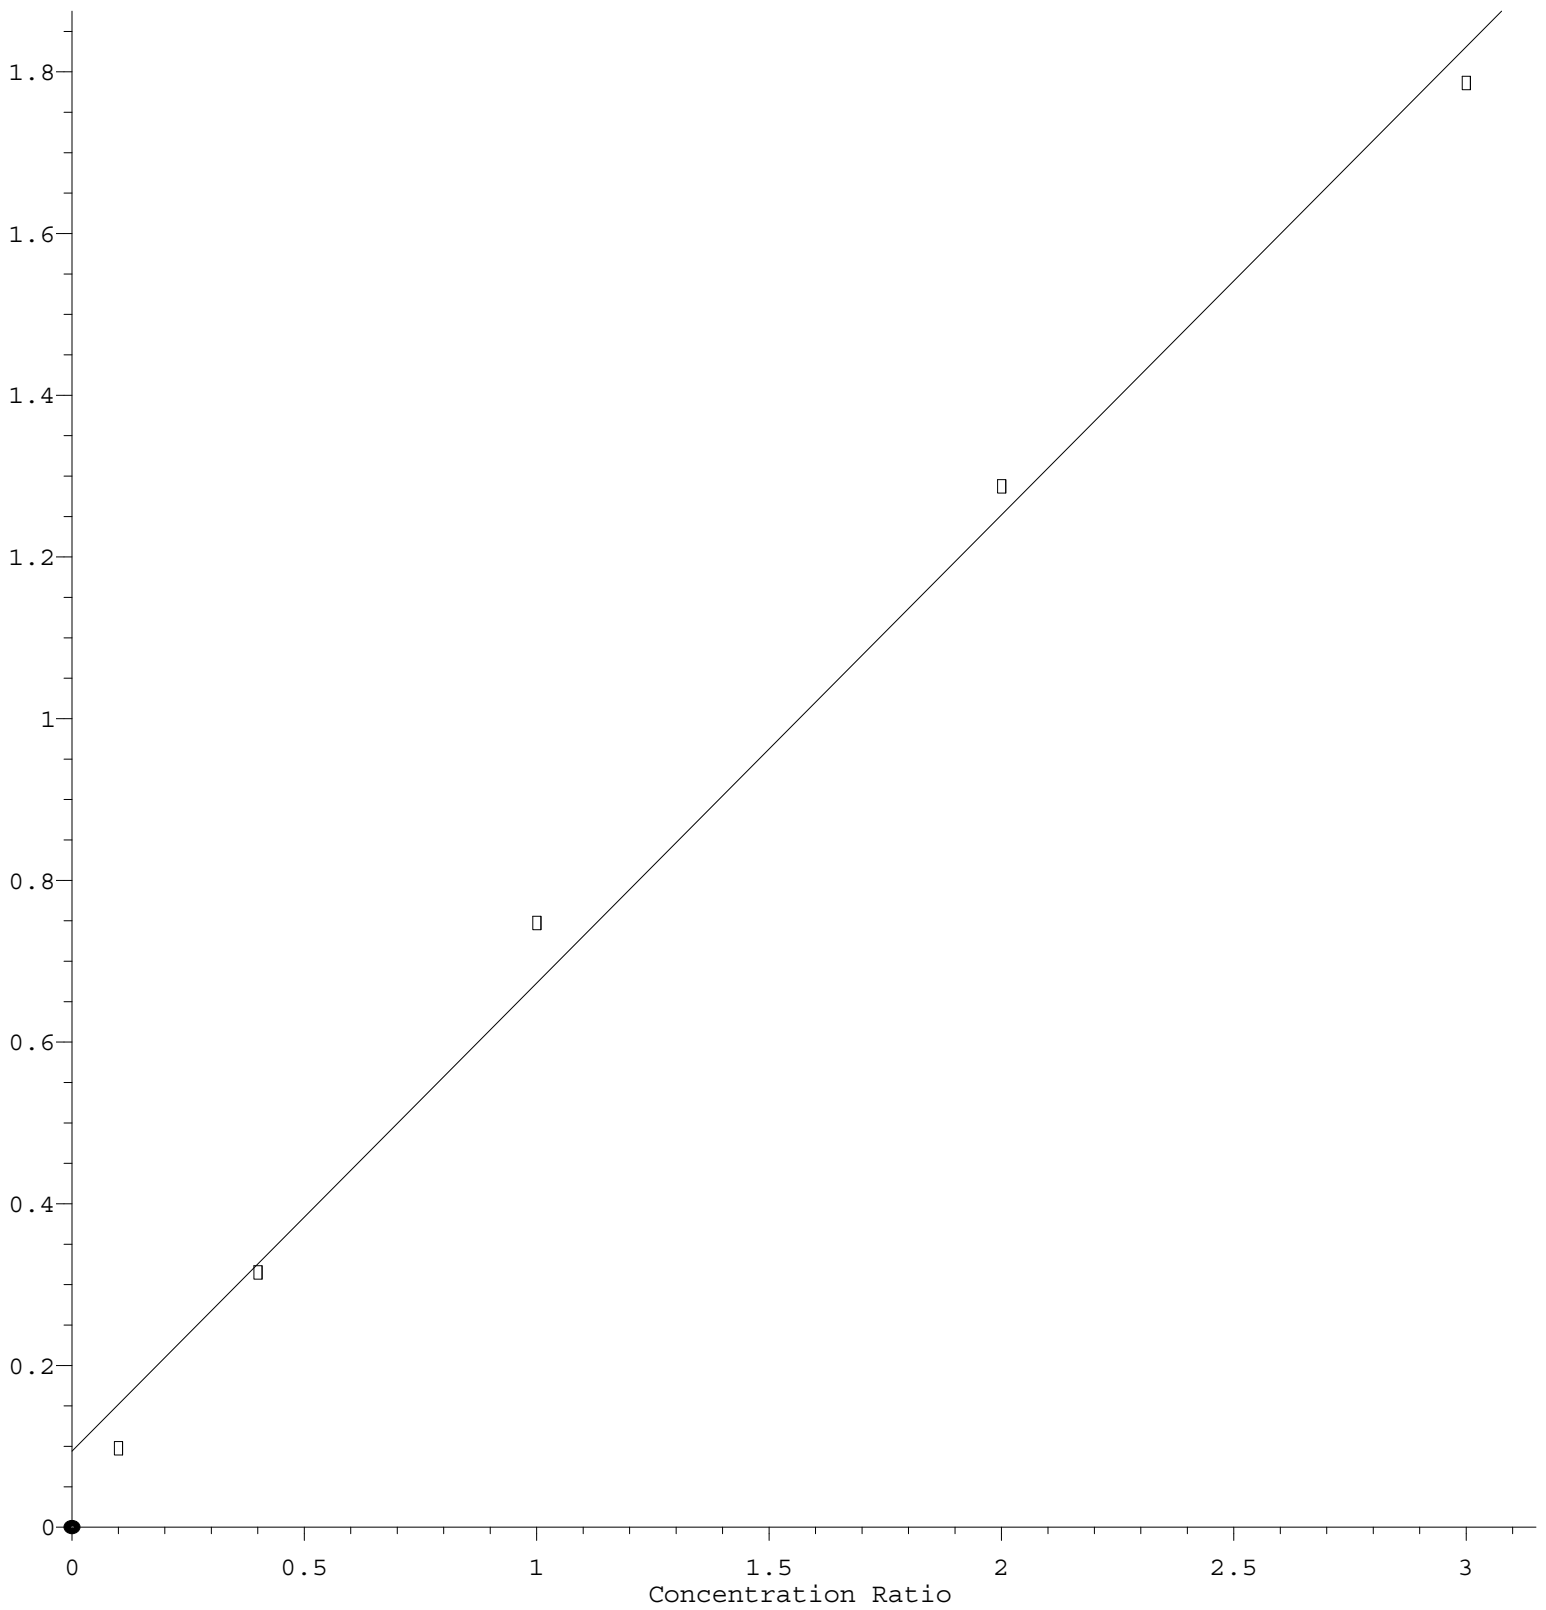

$$\text{Response} = 5.792\text{e-}001 * \text{Amt} + 9.370\text{e-}002$$


Coef of Det (r^2) = 0.993856 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

Trichlorofluoromethane

Response Ratio

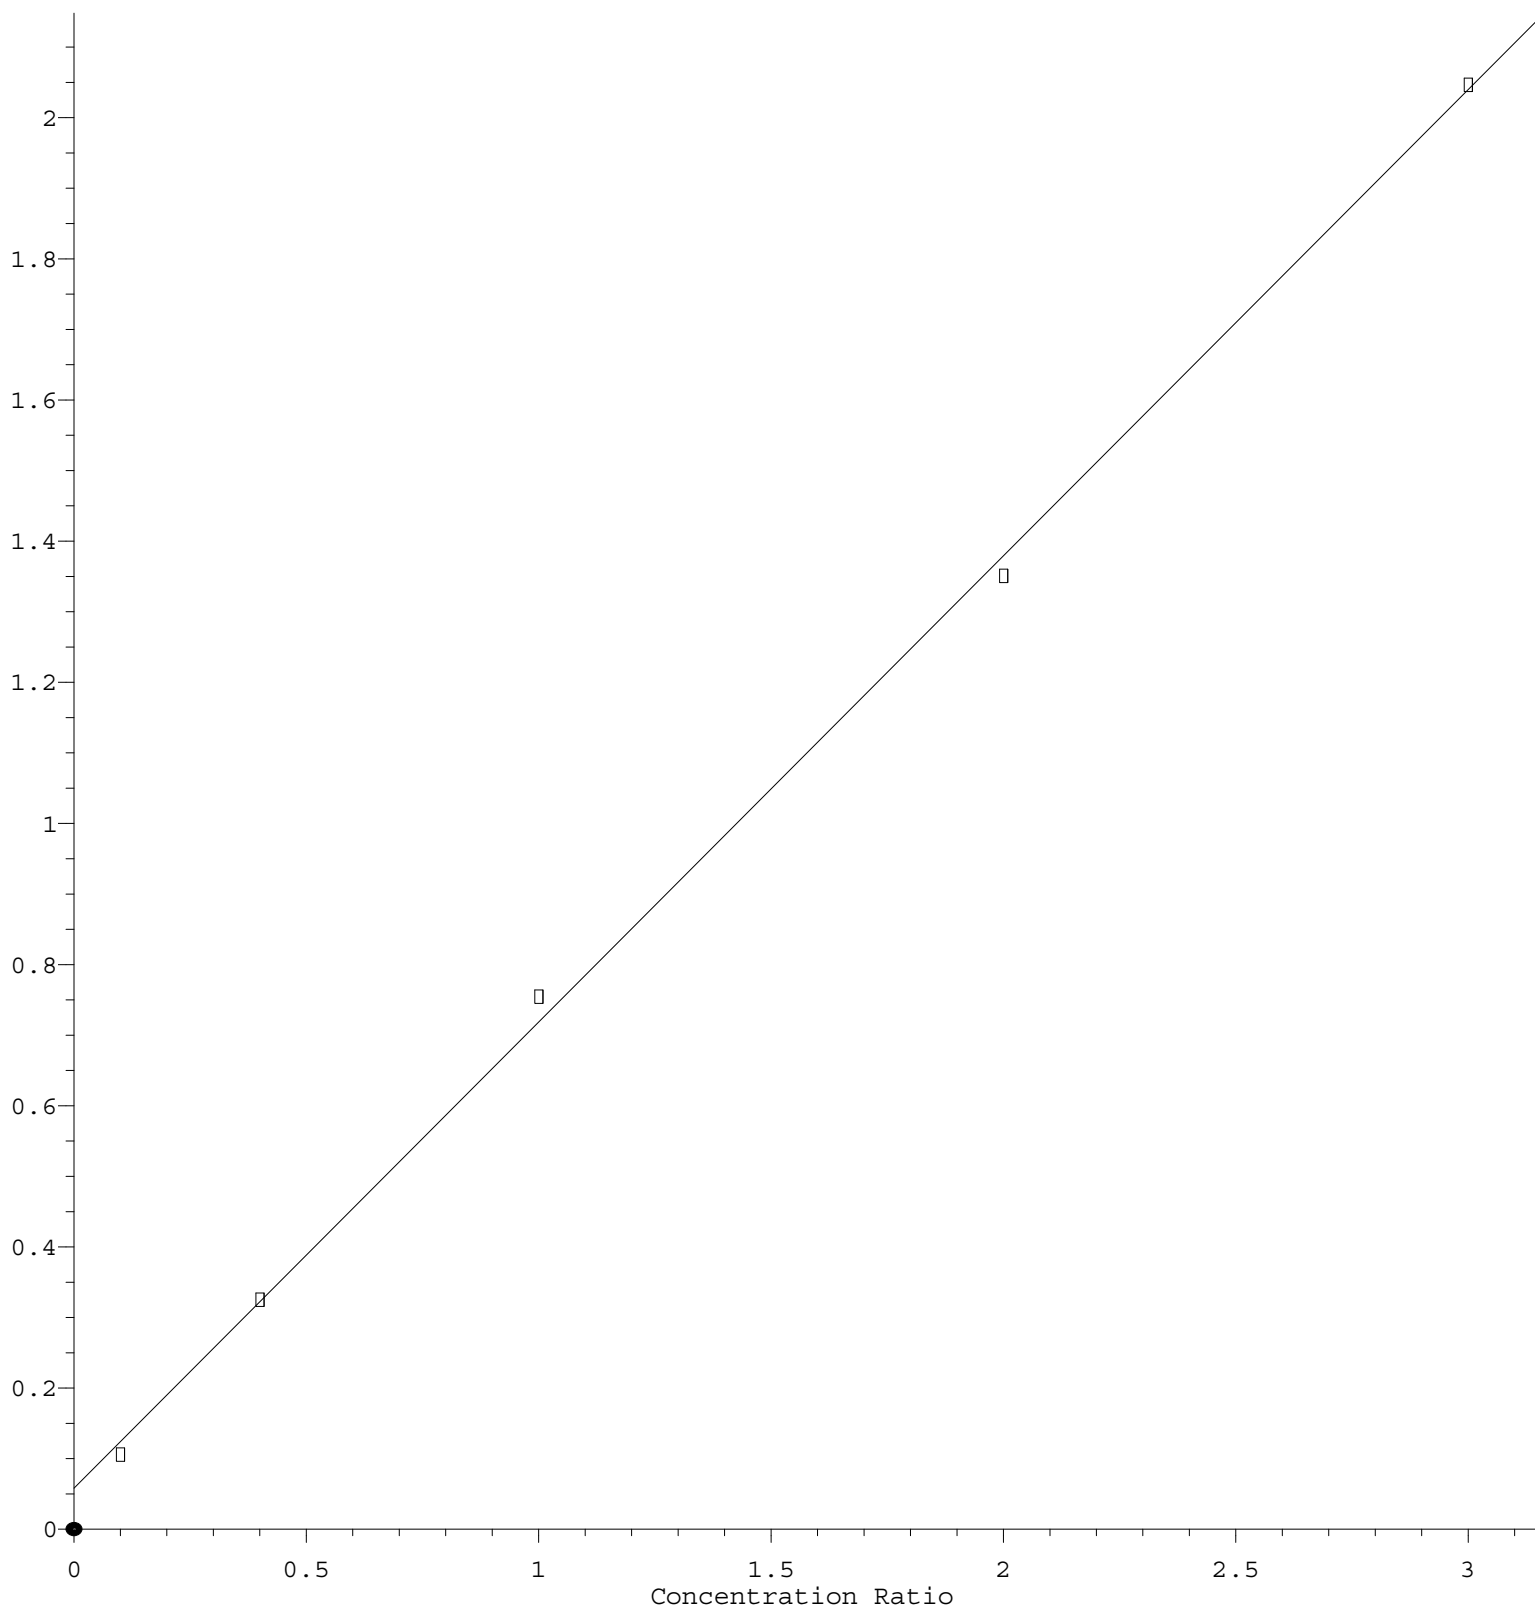

$$\text{Response} = 6.606\text{e-}001 * \text{Amt} + 5.772\text{e-}002$$


Coef of Det (r^2) = 0.999001 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

1,1-Dichloroethene

Response Ratio

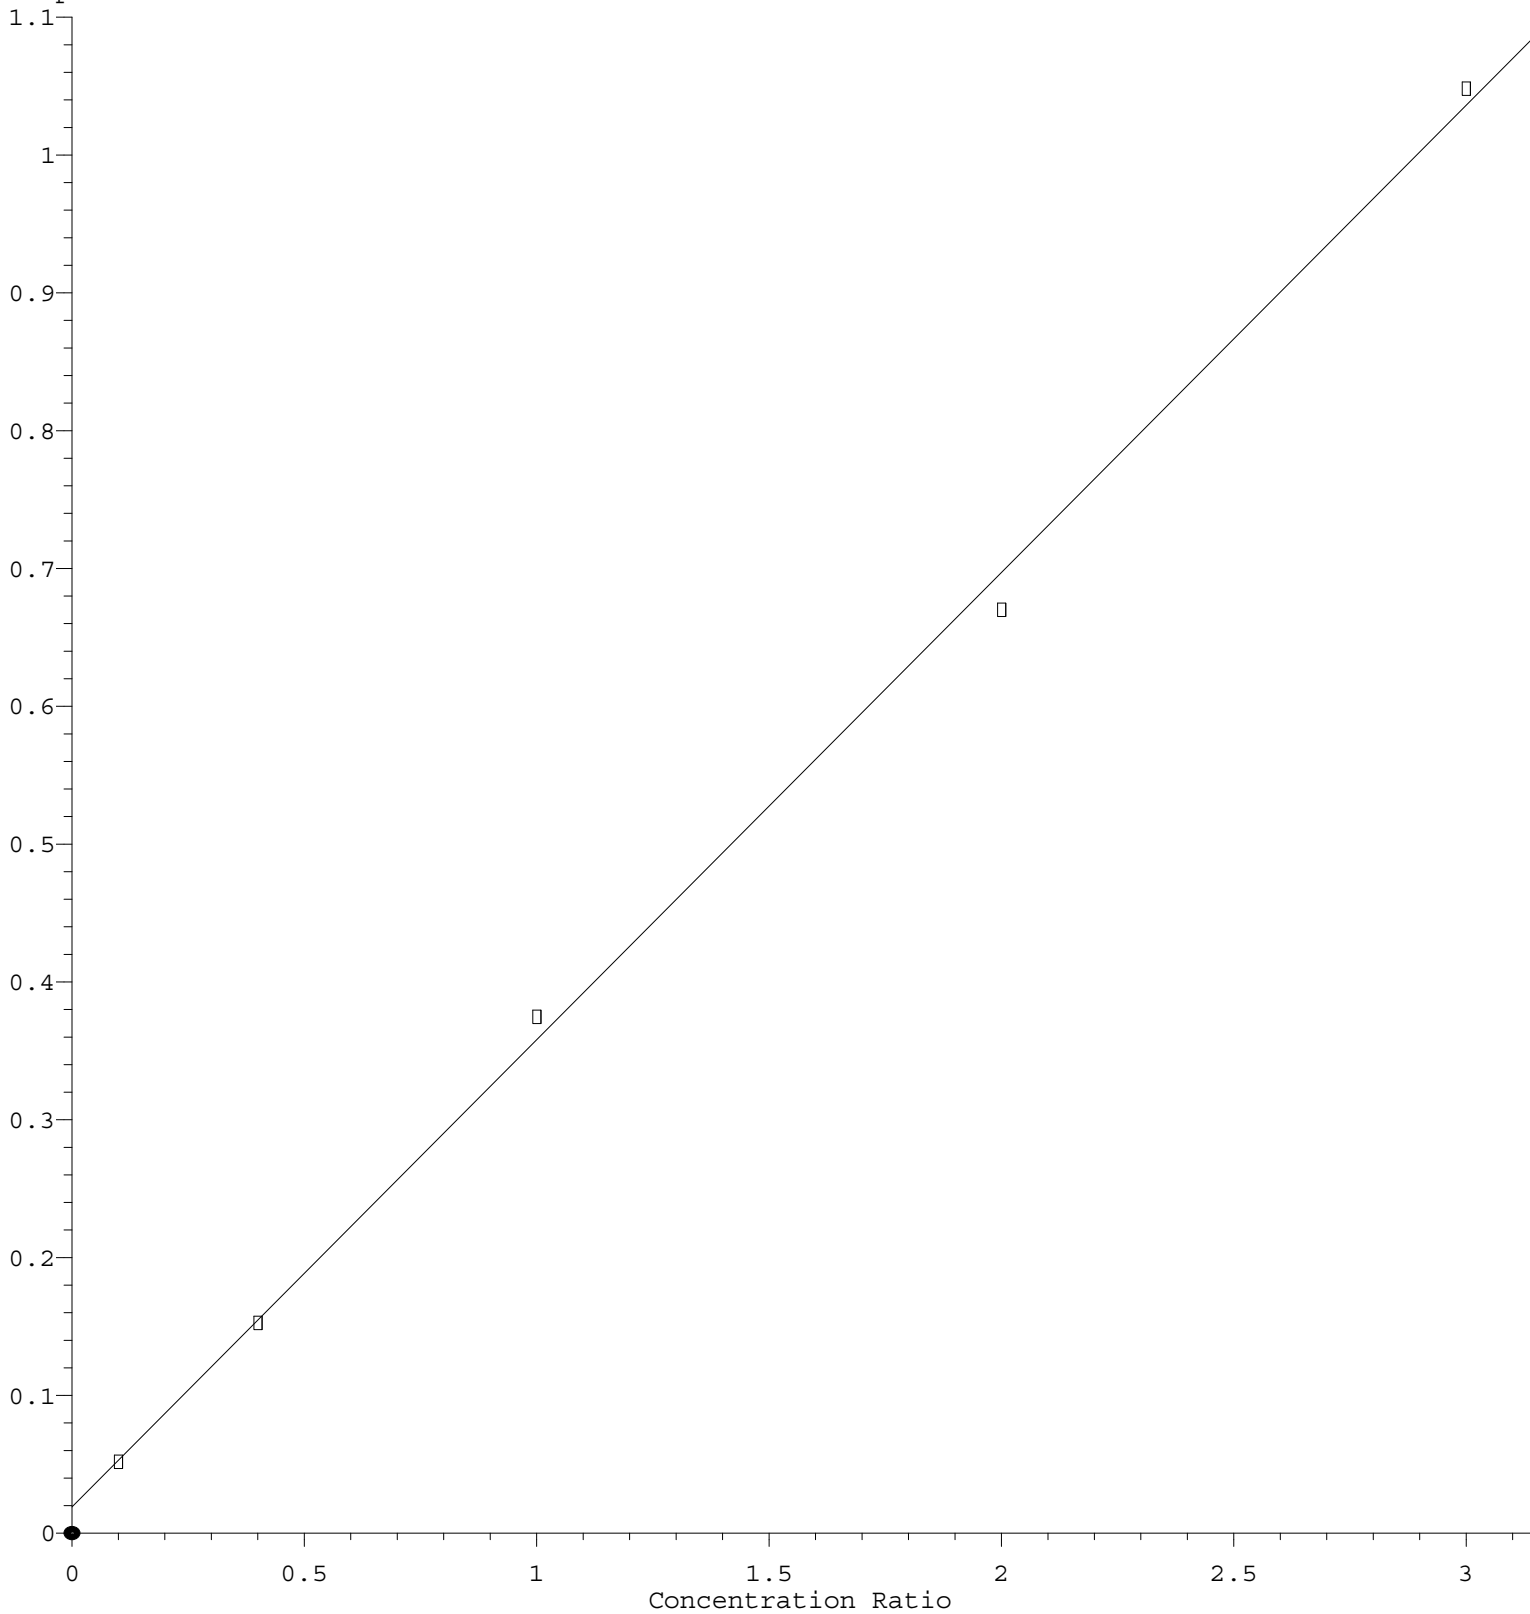

$$\text{Response} = 3.390\text{e-}001 * \text{Amt} + 1.870\text{e-}002$$


Coef of Det (r^2) = 0.998241 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

Acetone


Response Ratio

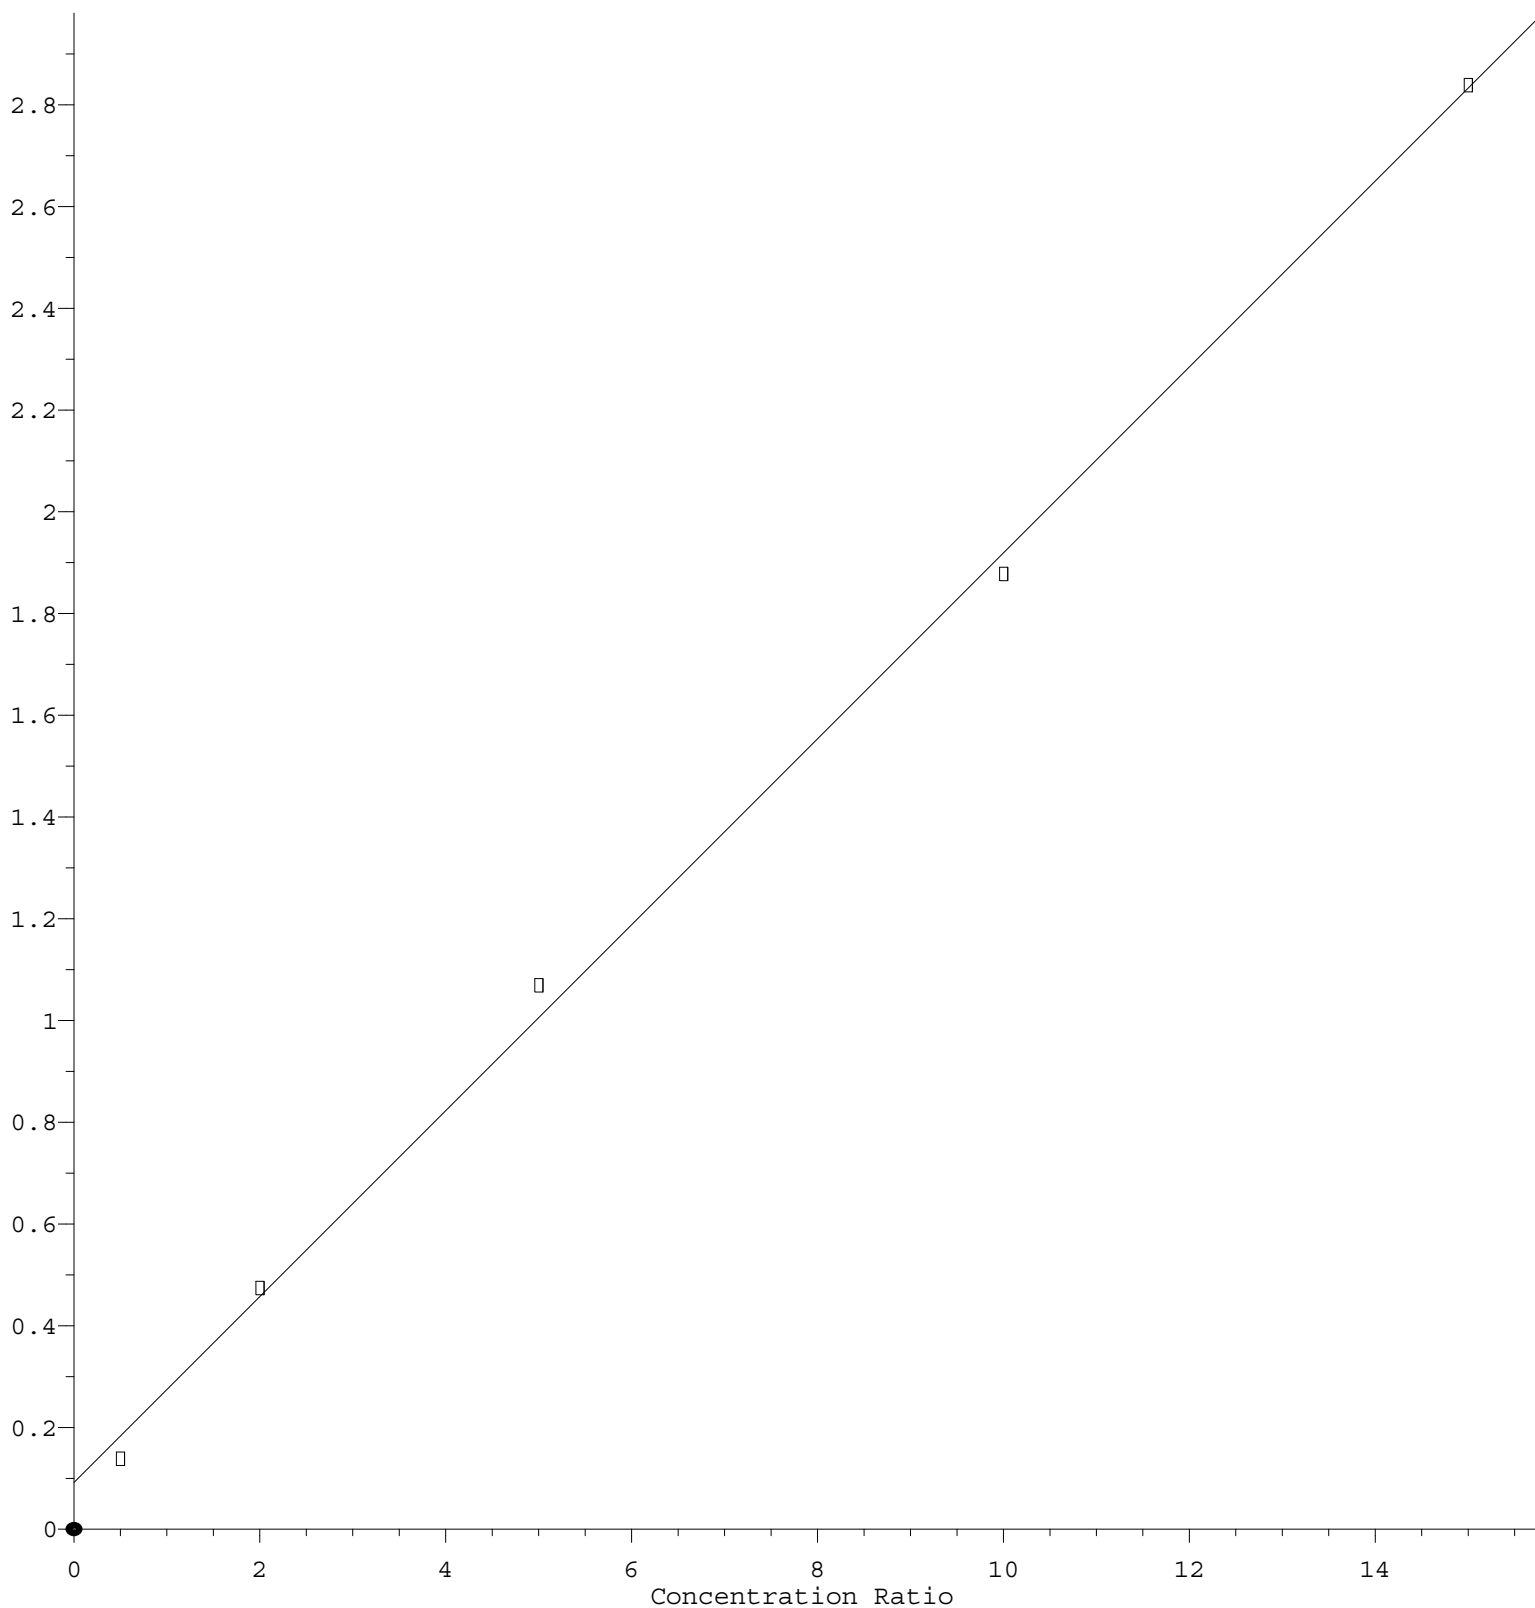

$\text{Response} = 1.828\text{e-}001 * \text{Amt} + 9.153\text{e-}002$
 Coef of Det (r^2) = 0.998315 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M
 Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

Carbon Disulfide

Response Ratio

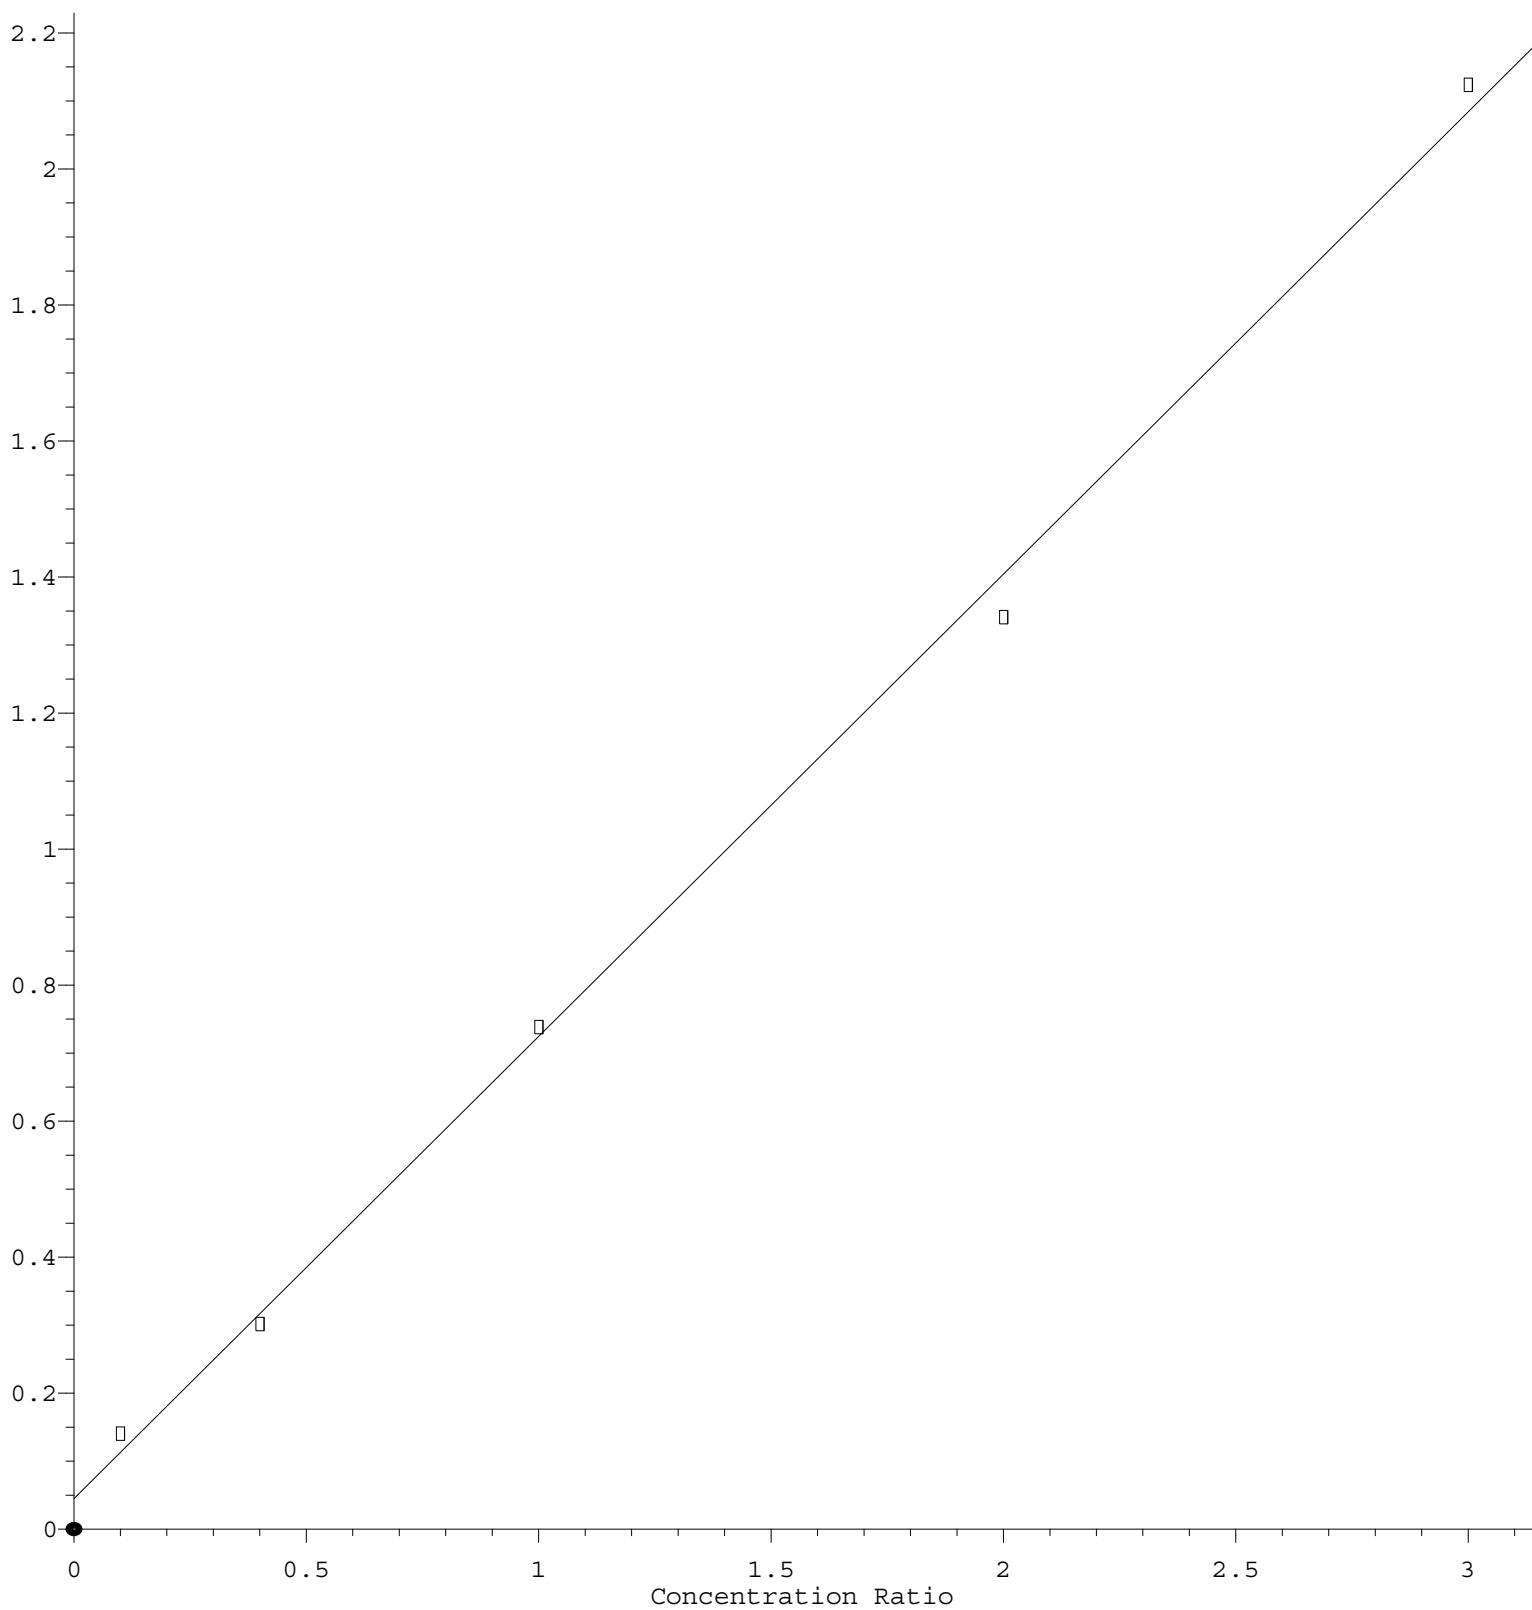

$$\text{Response} = 6.796\text{e-}001 * \text{Amt} + 4.546\text{e-}002$$


Coef of Det (r^2) = 0.997445 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

Methylene Chloride

Response Ratio

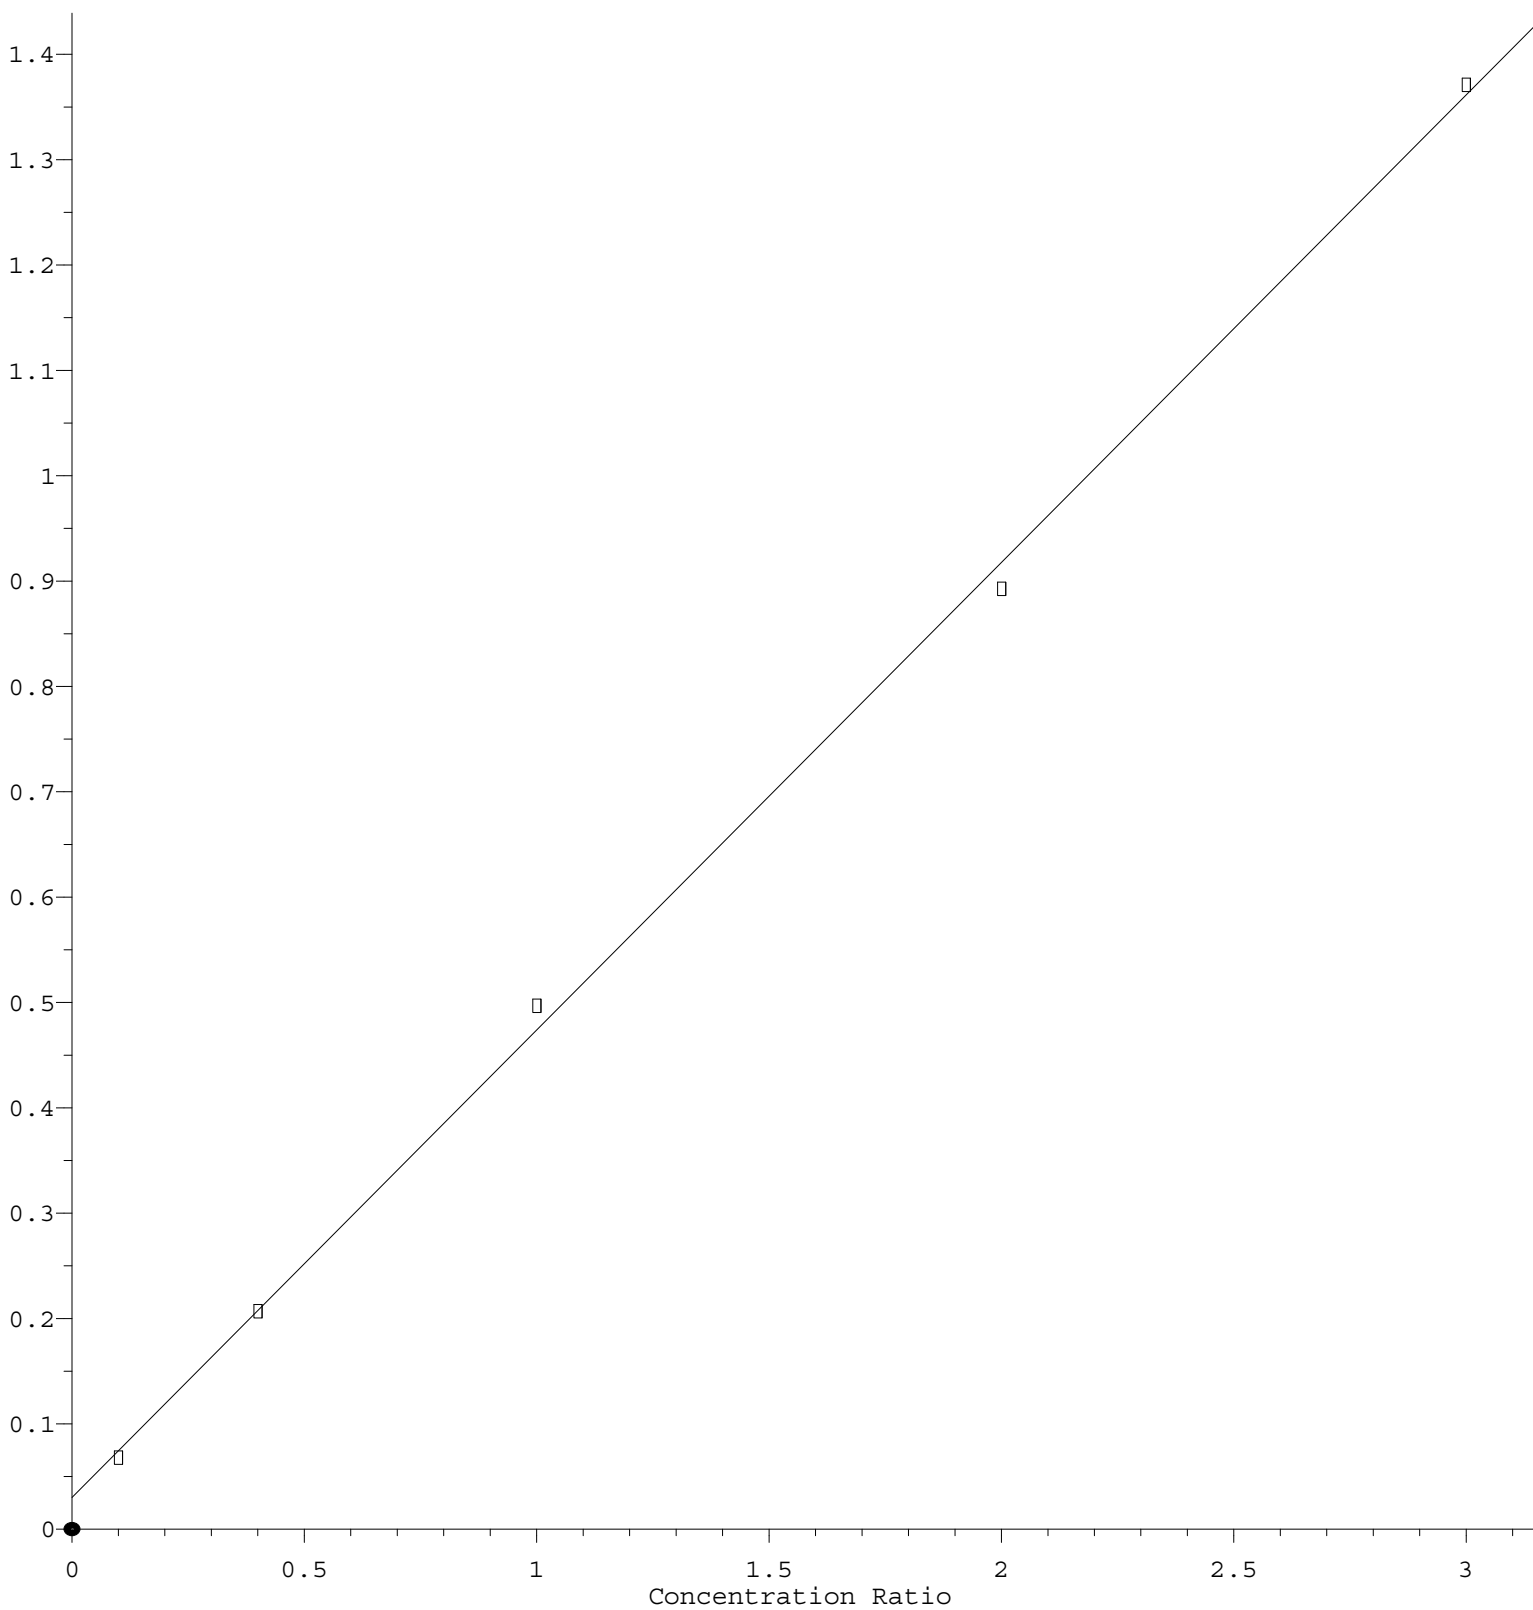

$$\text{Response} = 4.438\text{e-}001 * \text{Amt} + 3.000\text{e-}002$$


Coef of Det (r^2) = 0.998858 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

trans-1,2-Dichloroethene

Response Ratio

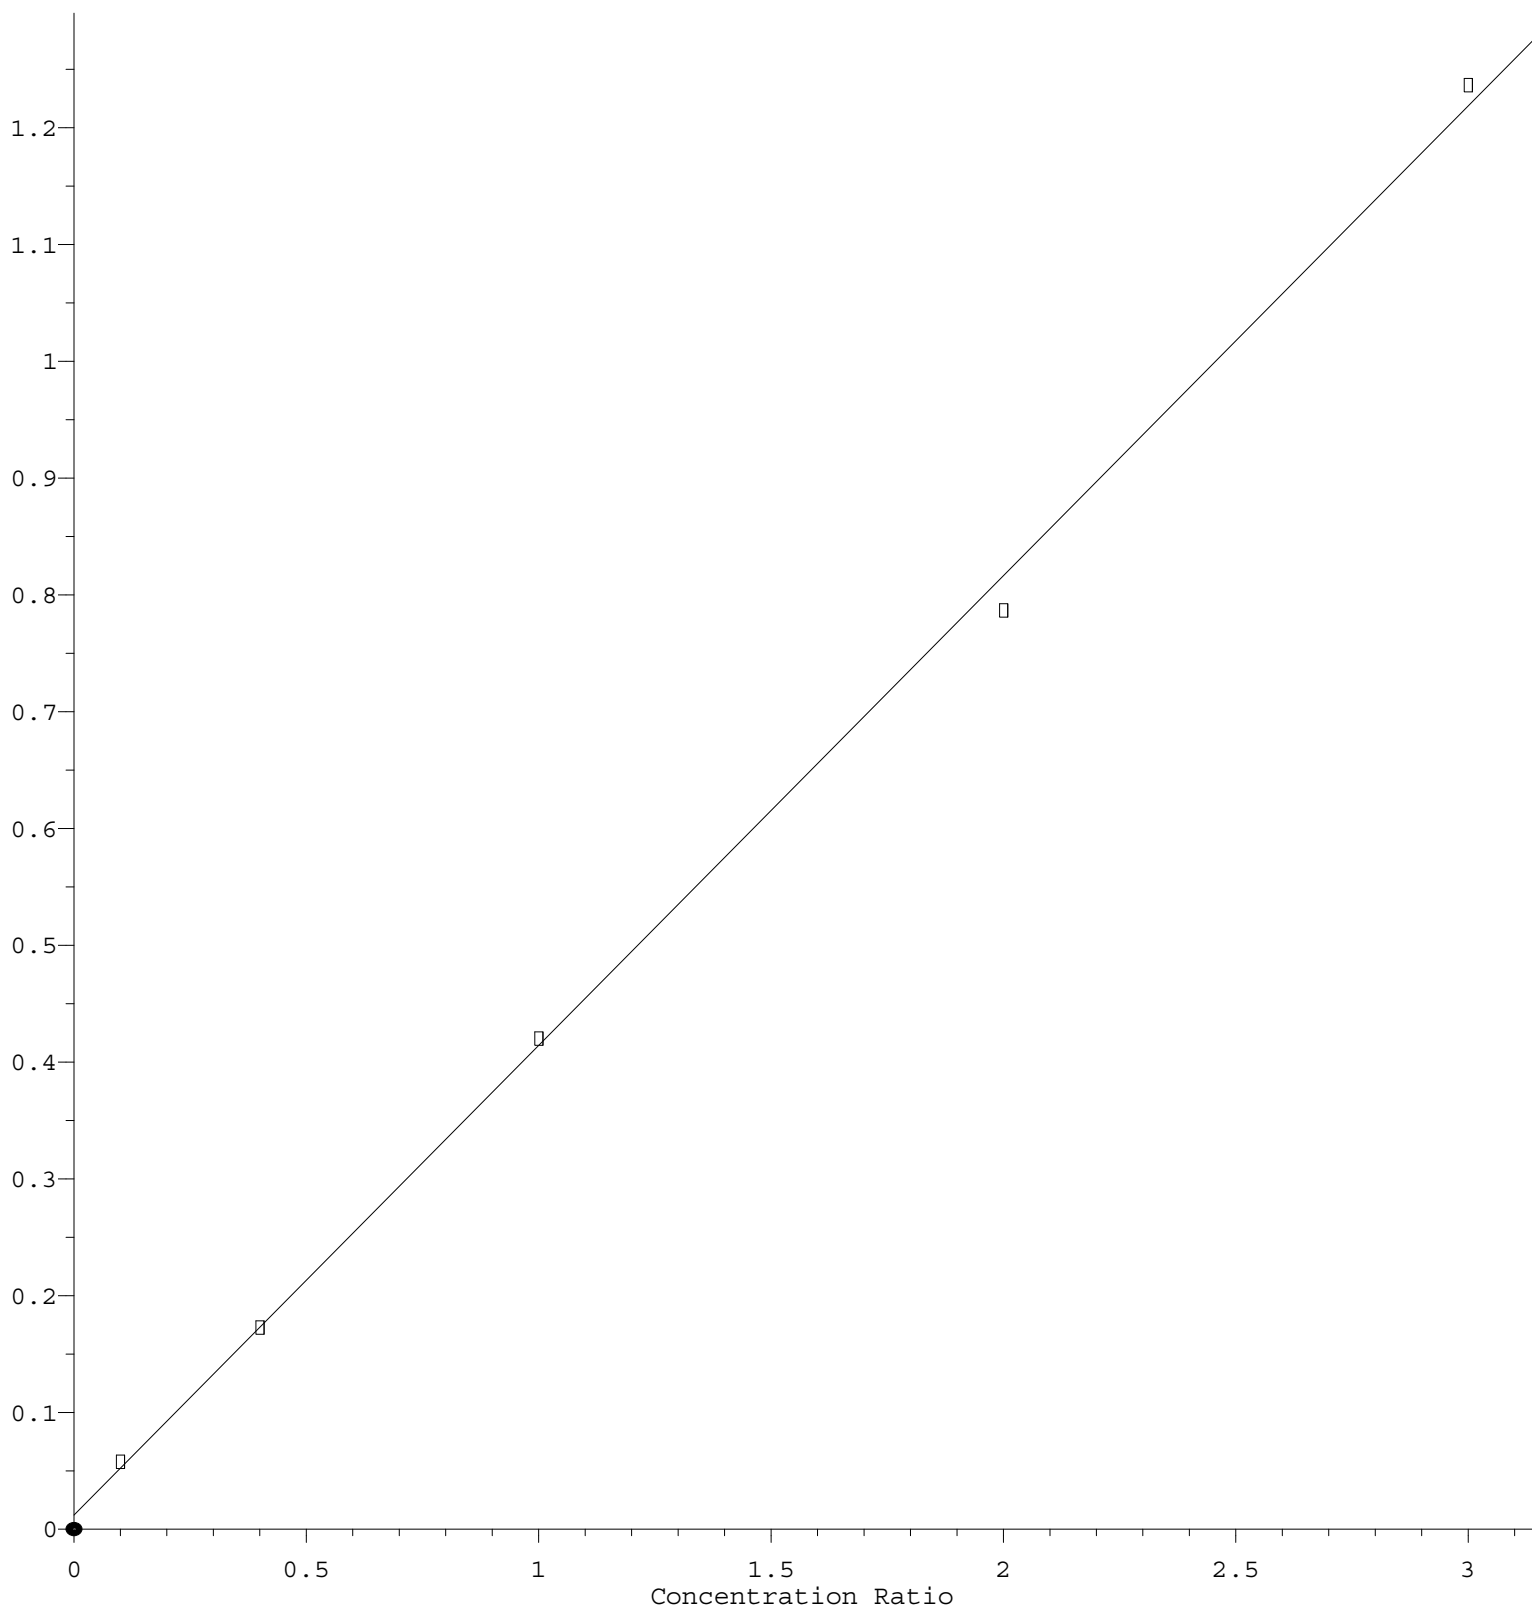

$$\text{Response} = 4.024\text{e-}001 * \text{Amt} + 1.151\text{e-}002$$


Coef of Det (r^2) = 0.998638 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

Cyclohexane

Response Ratio

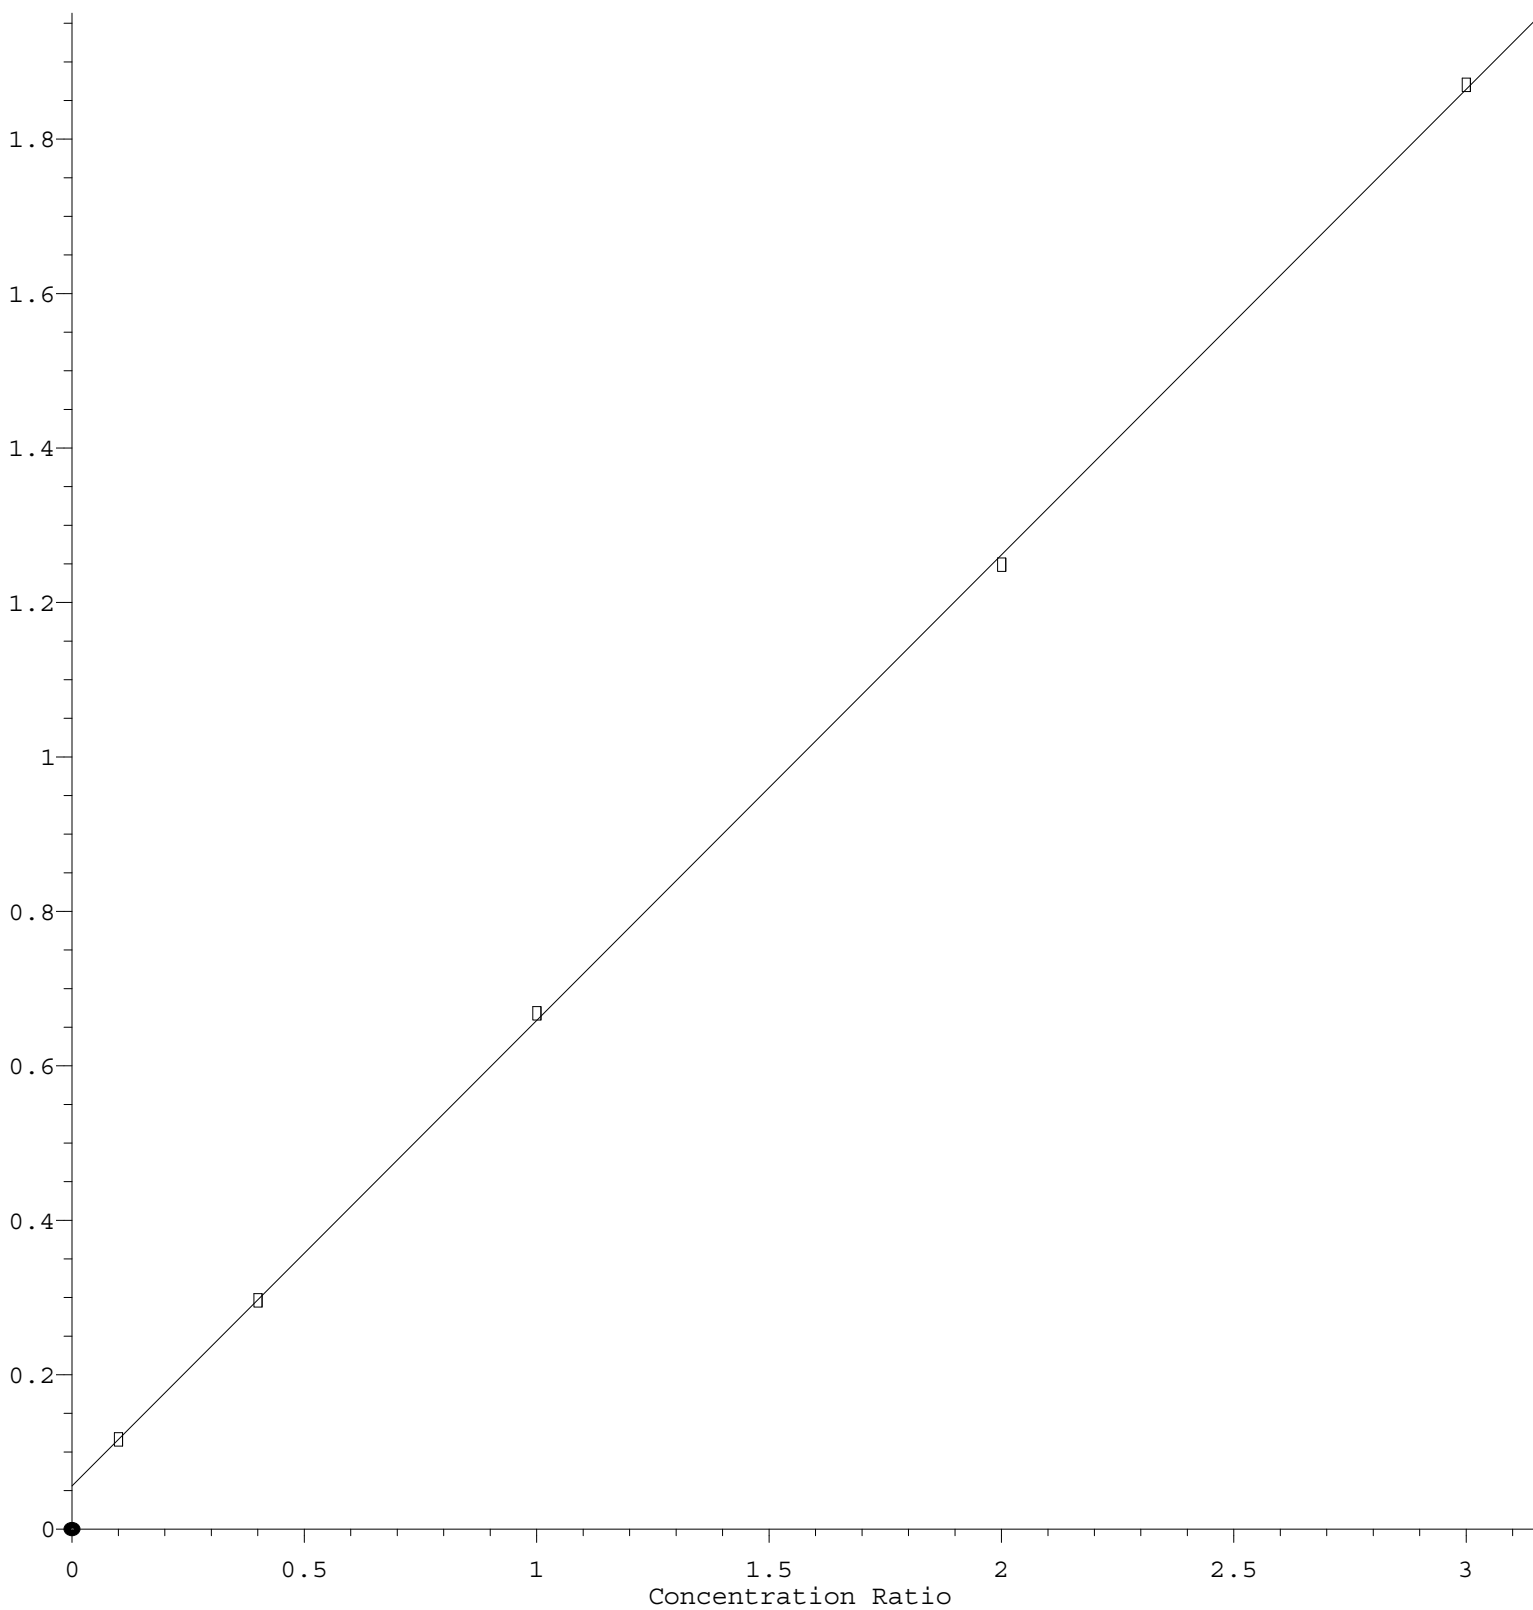

$$\text{Response} = 6.026\text{e-}001 * \text{Amt} + 5.650\text{e-}002$$


Coef of Det (r^2) = 0.999866 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

2-Chloroethyl Vinyl ether

Response Ratio

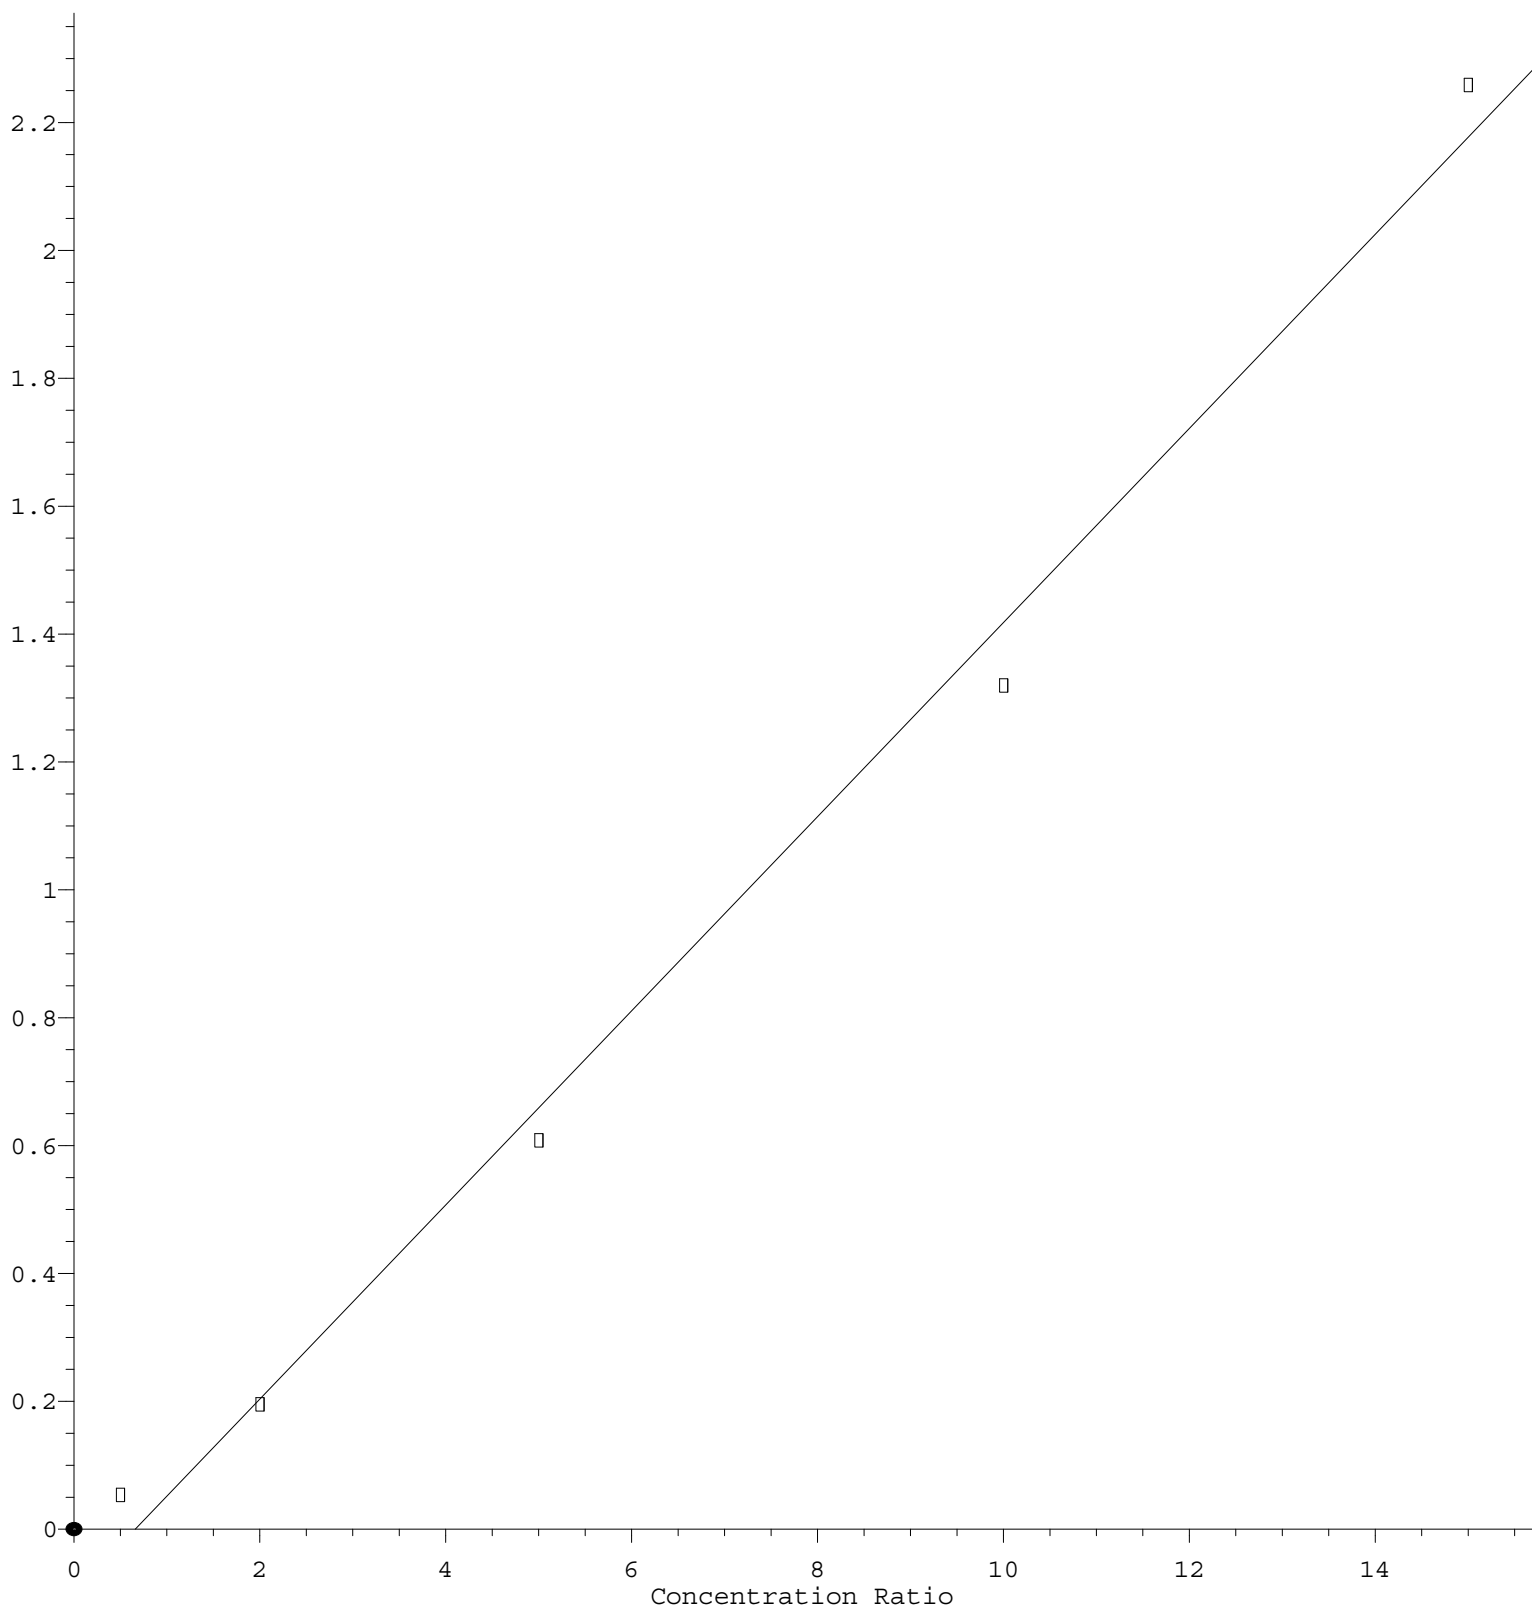

$$\text{Response} = 1.518\text{e-}001 * \text{Amt} - 9.965\text{e-}002$$


Coef of Det (r^2) = 0.992455 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021

4-Bromofluorobenzene

Response Ratio

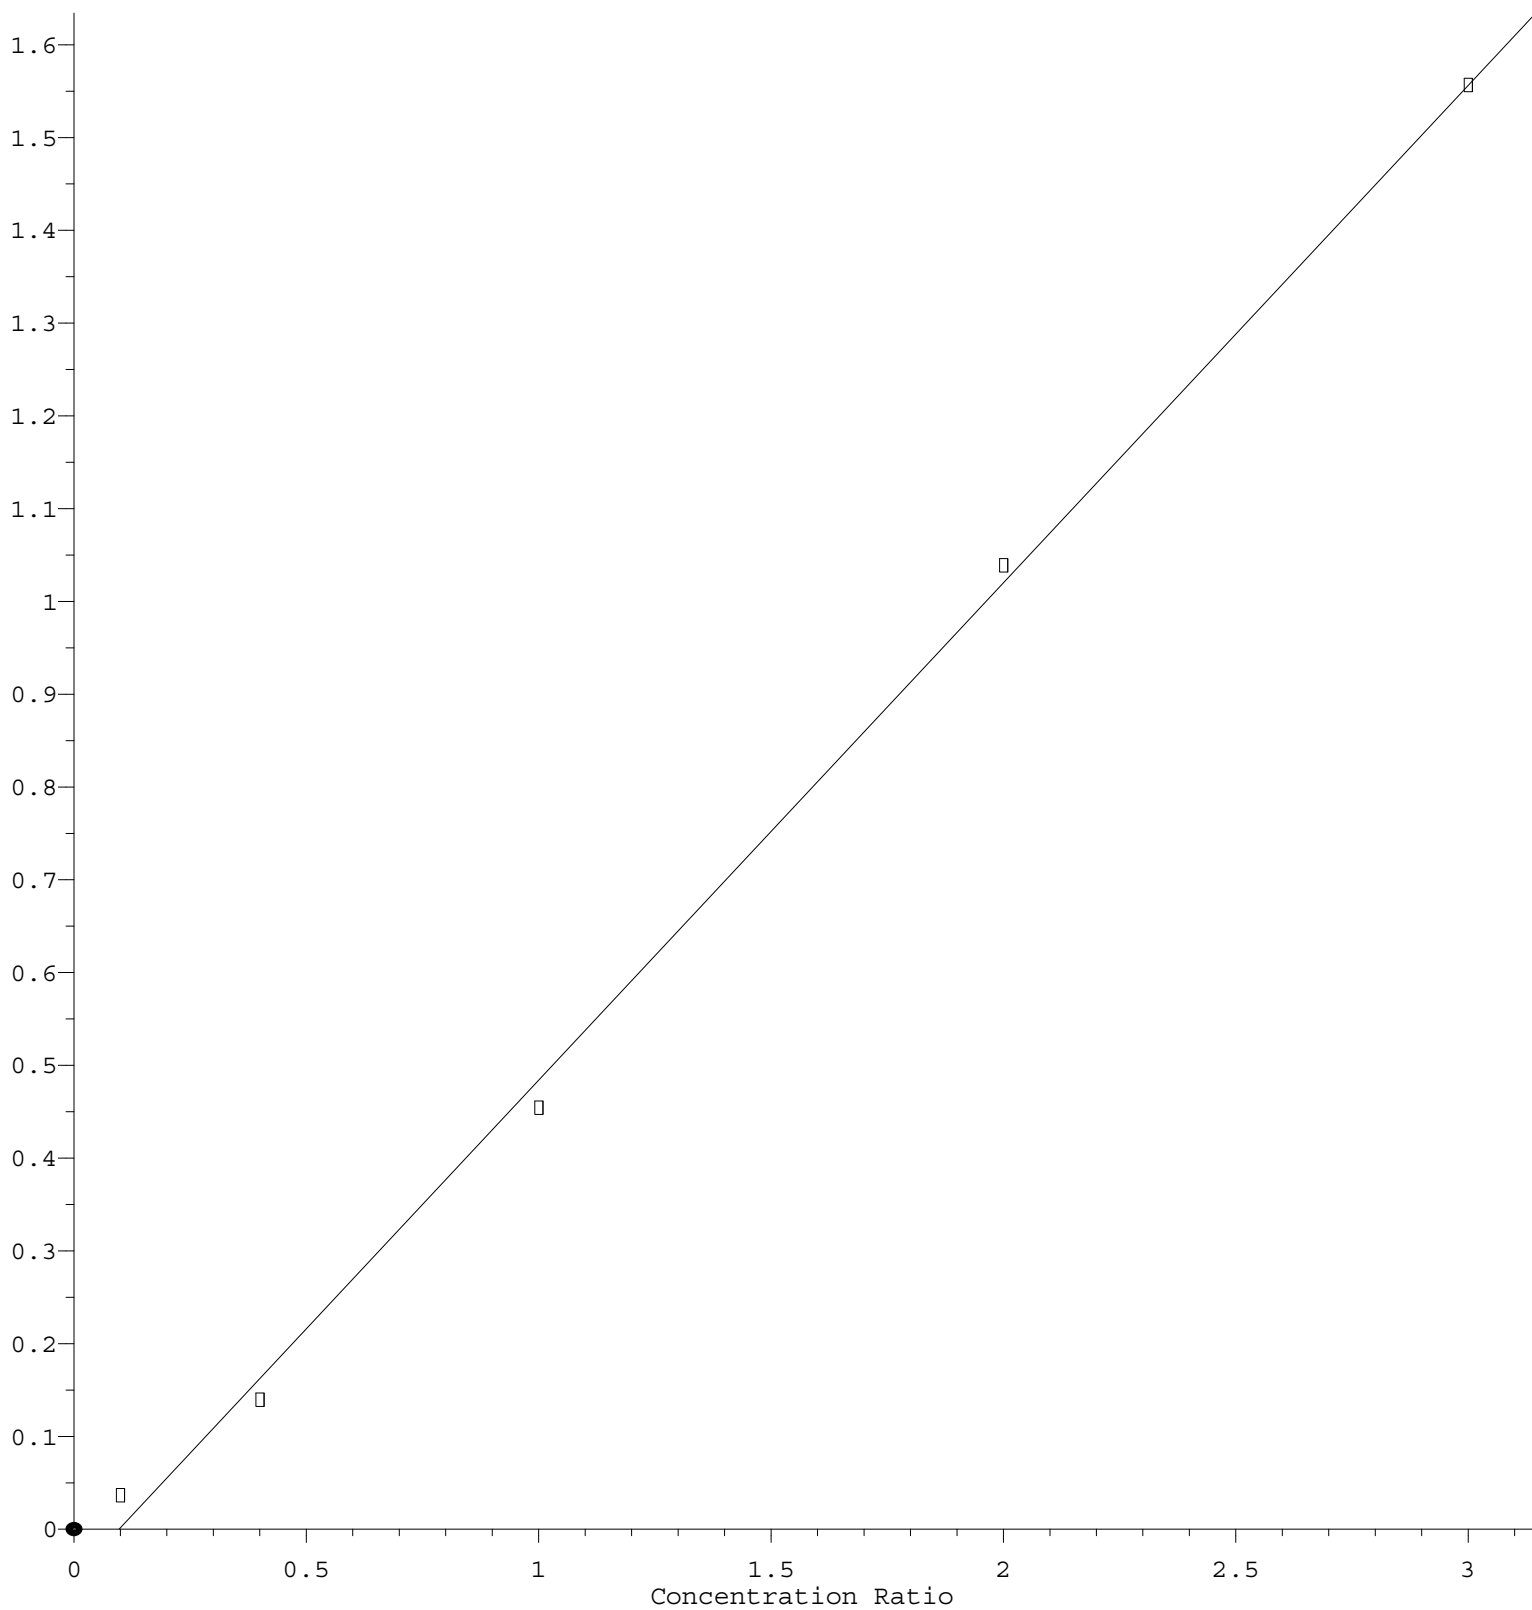

$$\text{Response} = 5.363\text{e-}001 * \text{Amt} - 5.207\text{e-}002$$

Coef of Det (r^2) = 0.998188 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N100621W.M

Calibration Table Last Updated: Wed Oct 06 14:41:09 2021