


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100622\
Data File : VN074769.D
Acq On : 06 Oct 2022 08:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Title : SW846 8260
Last Update : Thu Oct 06 05:37:50 2022

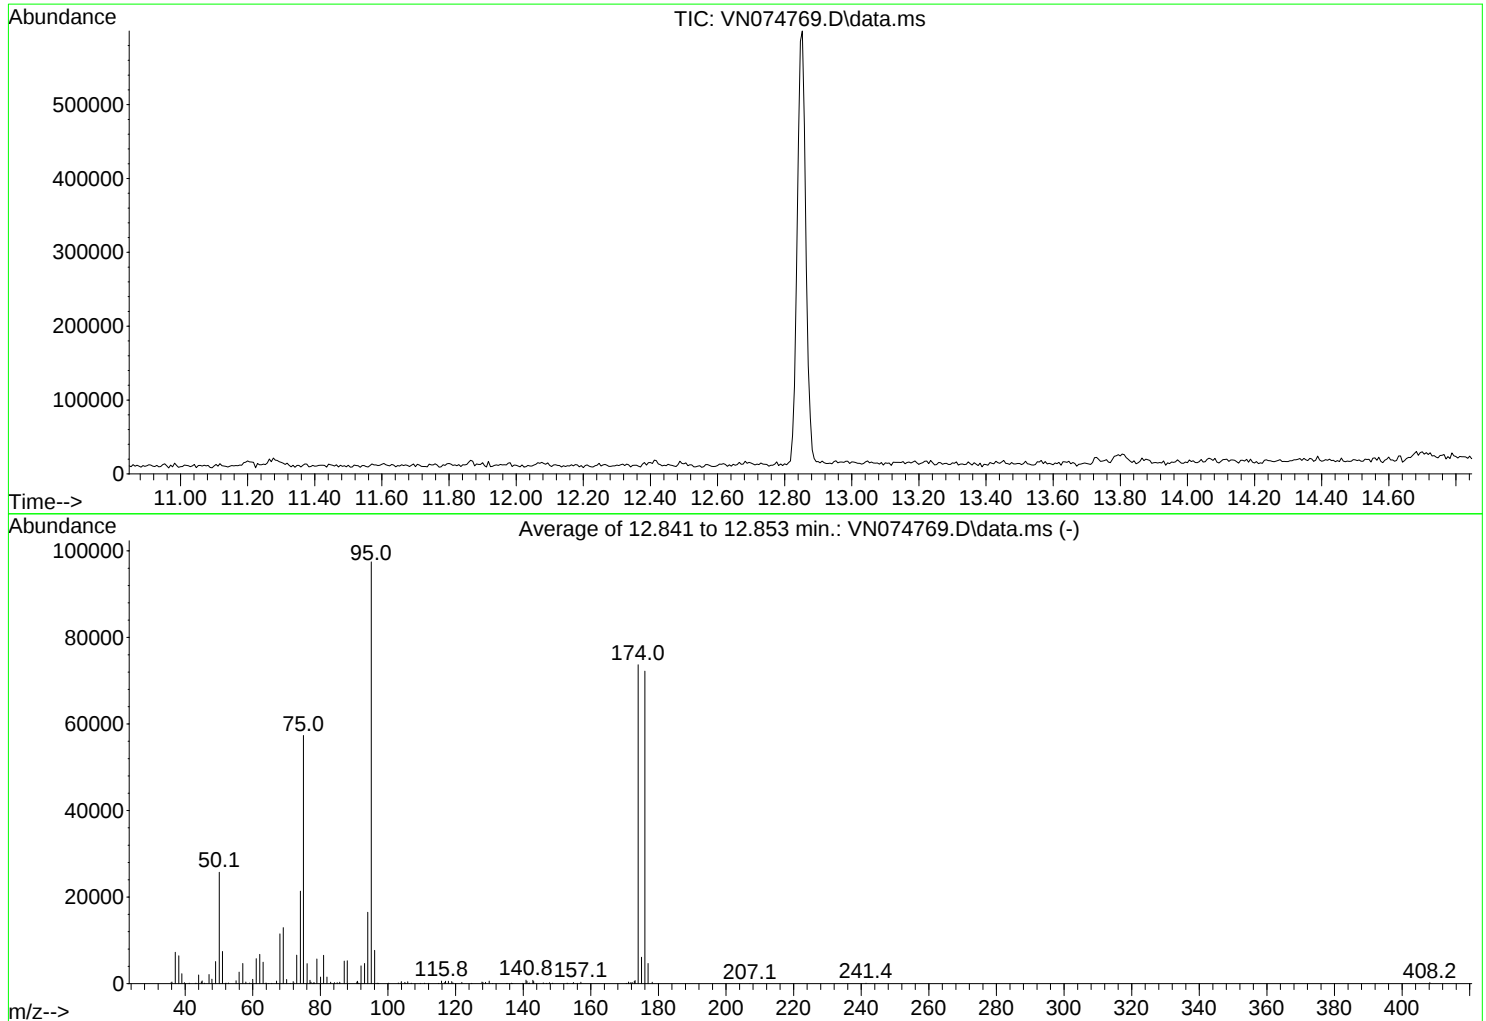

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1826

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	26.4	25755	PASS
75	95	30	60	58.9	57364	PASS
95	95	100	100	100.0	97472	PASS
96	95	5	9	7.9	7691	PASS
173	174	0.00	2	0.9	689	PASS
174	95	50	100	75.6	73704	PASS
175	174	5	9	8.3	6108	PASS
176	174	95	101	98.0	72205	PASS
177	176	5	9	6.4	4652	PASS