

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100623\
 Data File : VN079435.D
 Acq On : 06 Oct 2023 09:57
 Operator : JC\MD
 Sample : VN1006MBL01
 Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1006MBL01

Quant Time: Oct 06 22:59:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 06 03:34:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	164894	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	289407	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	273401	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	96622	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	129782	48.542	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.080%
35) Dibromofluoromethane	8.171	113	120560	57.968	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	115.940%
50) Toluene-d8	10.571	98	285127	37.889	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	75.780%#
62) 4-Bromofluorobenzene	12.853	95	119685	49.559	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100623\
Data File : VN079435.D
Acq On : 06 Oct 2023 09:57
Operator : JC\MD
Sample : VN1006MBL01
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1006MBL01

Quant Time: Oct 06 22:59:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 06 03:34:49 2023
Response via : Initial Calibration




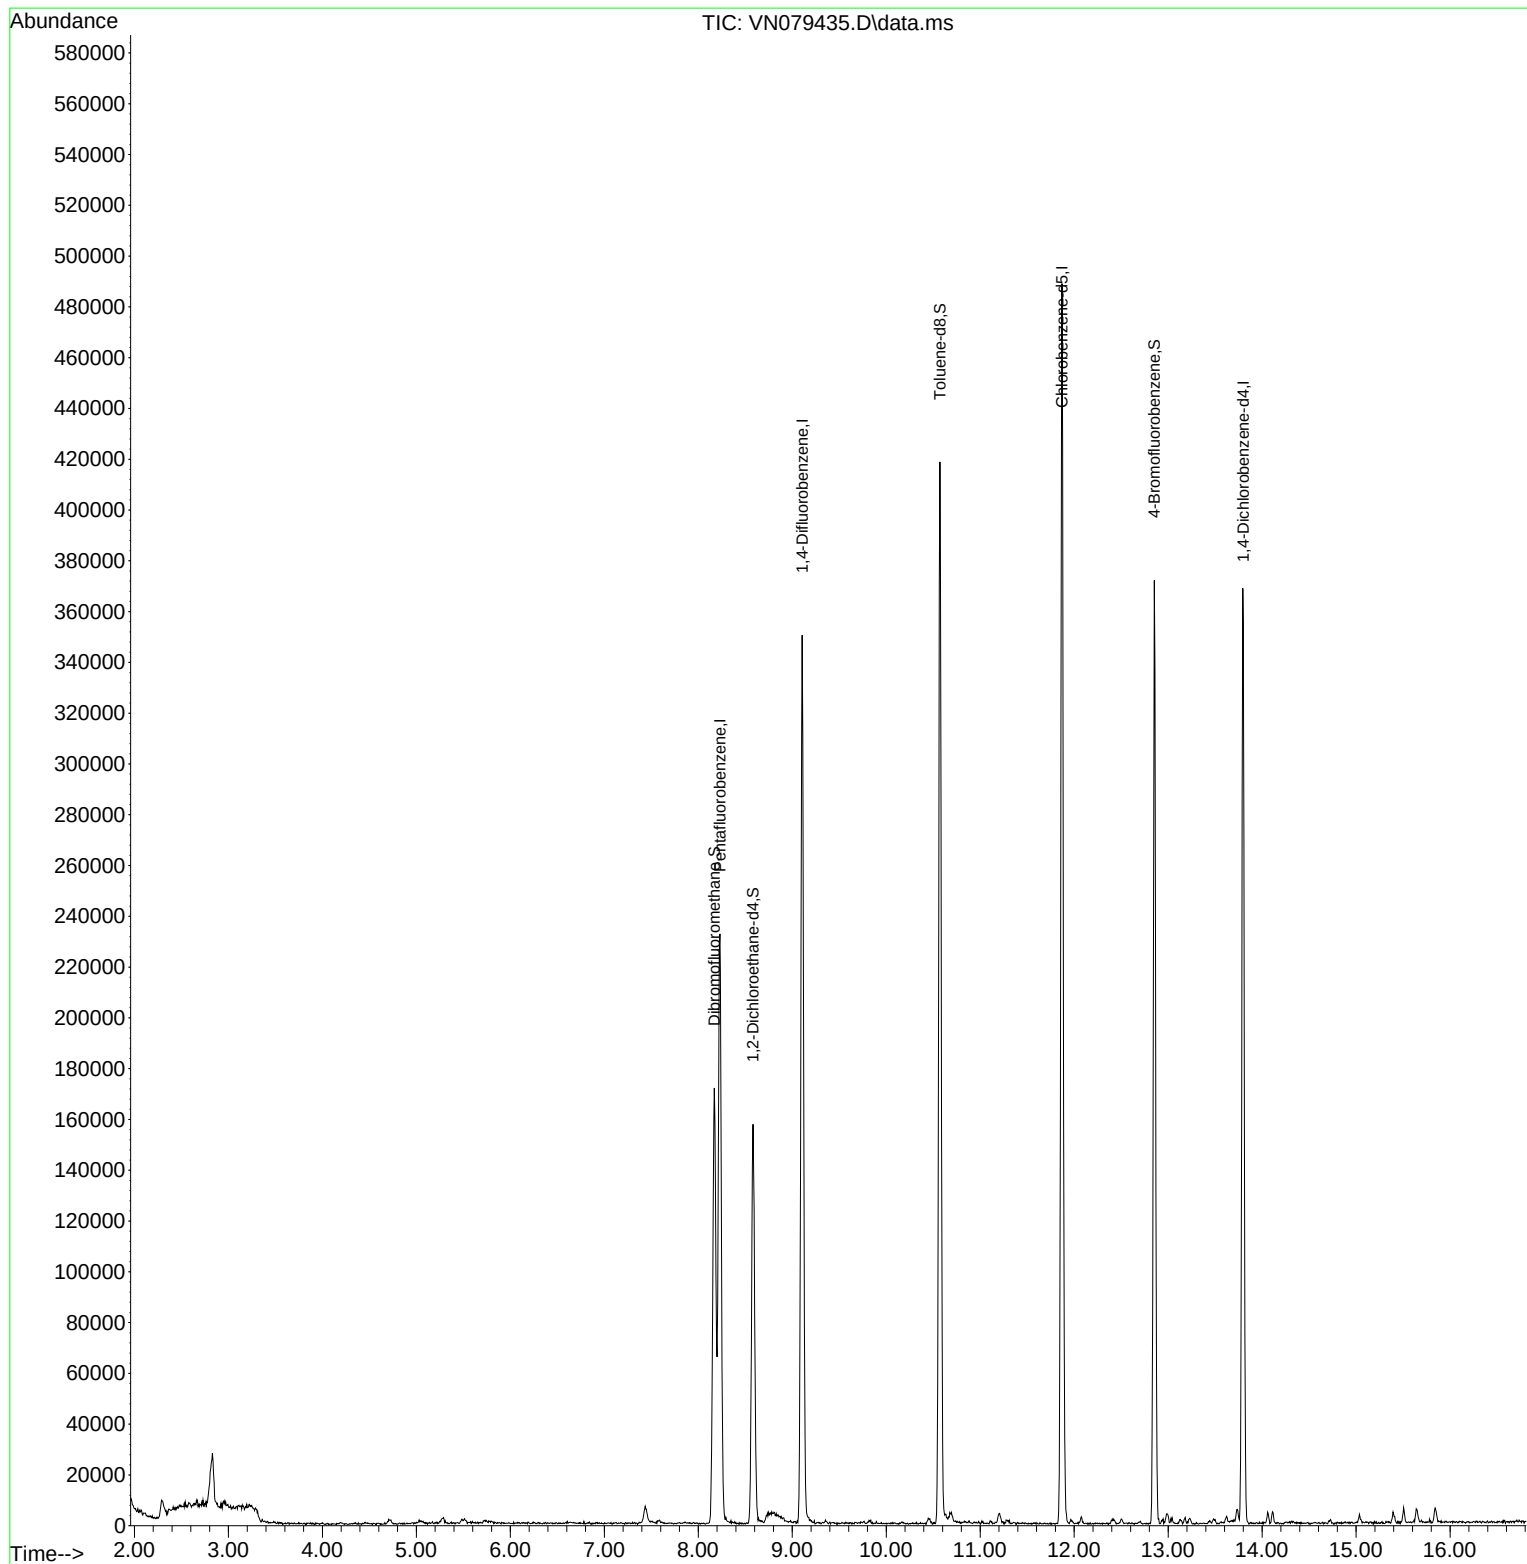


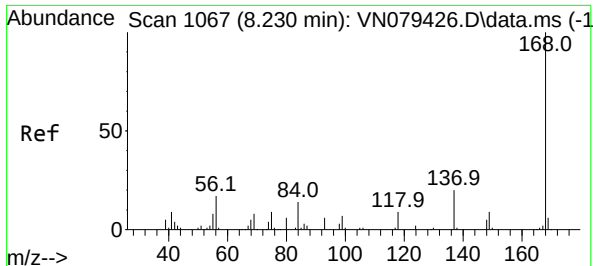

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.000 min
Lab File: VN079435.D
Acq: 06 Oct 2023 09:57




Instrument :
MSVOA_N
ClientSampleId :
VN1006MBL01


Tgt Ion:168 Resp: 164894
Ion Ratio Lower Upper
168 100
99 61.8 53.0 79.6

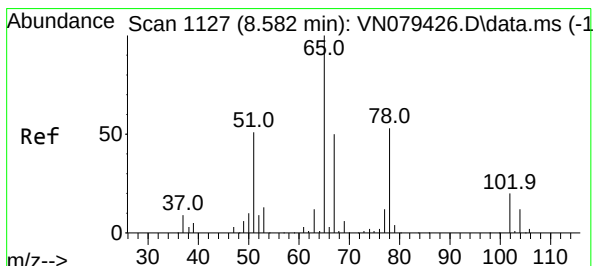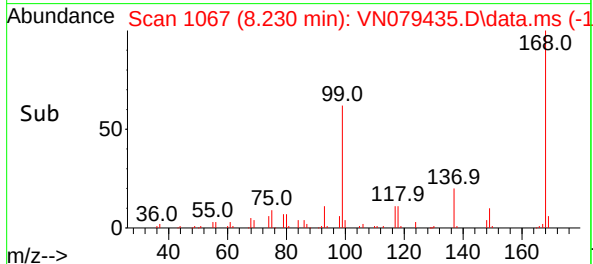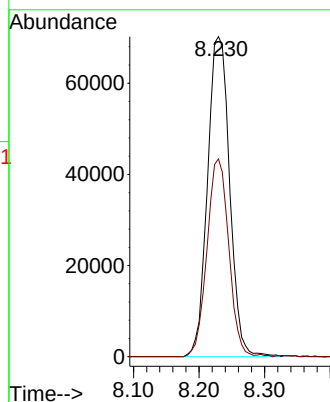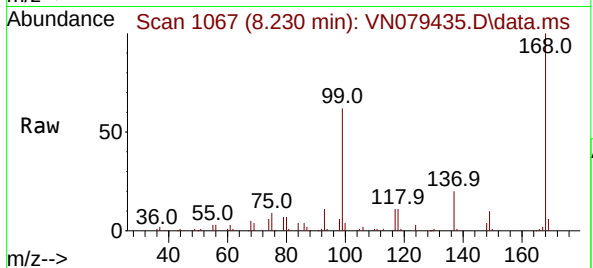

#33
1,2-Dichloroethane-d4
Concen: 48.542 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN079435.D
Acq: 06 Oct 2023 09:57

Tgt Ion: 65 Resp: 129782
Ion Ratio Lower Upper
65 100
67 50.5 0.0 106.6

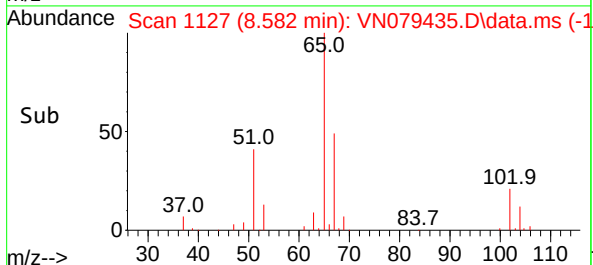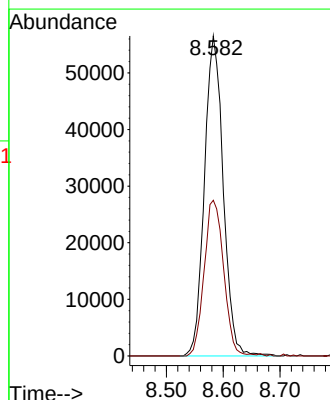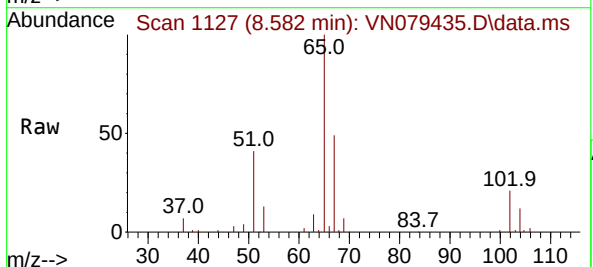

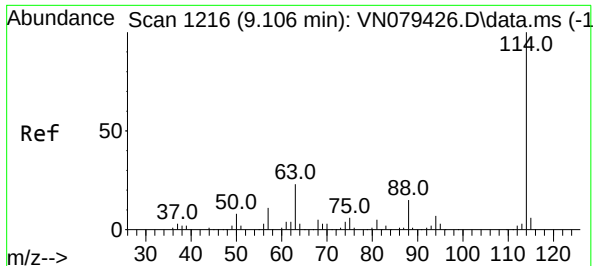

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN079435.D

Acq: 06 Oct 2023 09:57

Instrument :

MSVOA_N

ClientSampleId :

VN1006MBL01





Tgt Ion:114 Resp: 289407

Ion Ratio Lower Upper

114 100

63 22.0 0.0 36.4

88 14.3 0.0 30.6

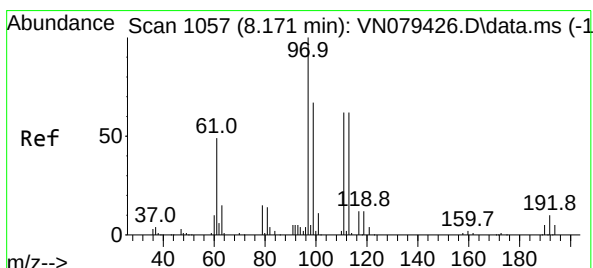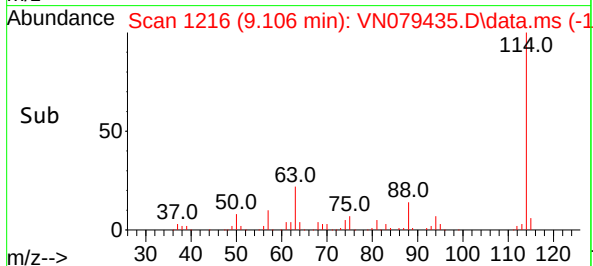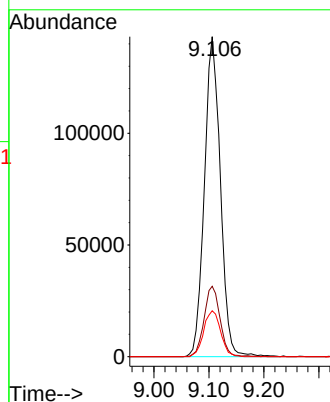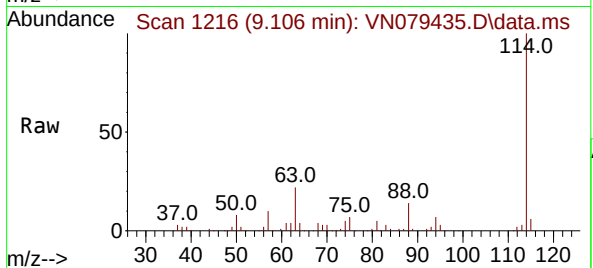

#35

Dibromofluoromethane

Concen: 57.968 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN079435.D

Acq: 06 Oct 2023 09:57




Tgt Ion:113 Resp: 120560


Ion Ratio Lower Upper

113 100

111 104.1 82.6 123.8

192 17.7 12.7 19.1


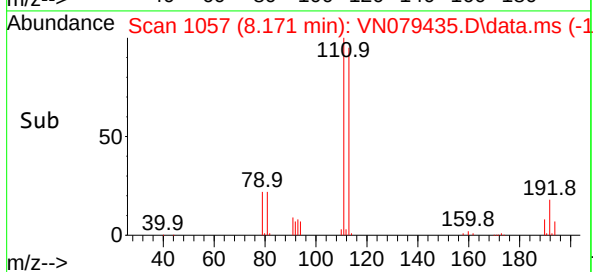
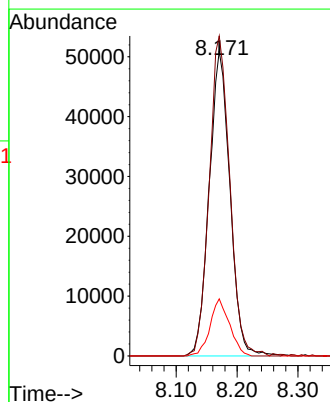
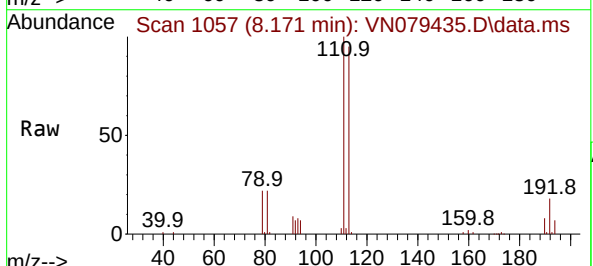


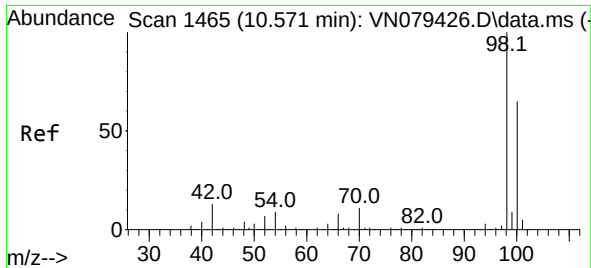

#50
Toluene-d8
Concen: 37.889 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN079435.D
Acq: 06 Oct 2023 09:57




Instrument :
MSVOA_N
ClientSampleId :
VN1006MBL01


Tgt Ion: 98 Resp: 285127
Ion Ratio Lower Upper
98 100
100 63.5 52.0 78.0

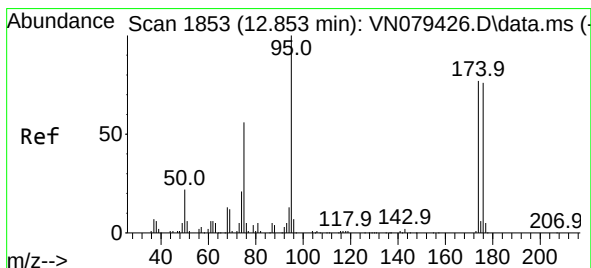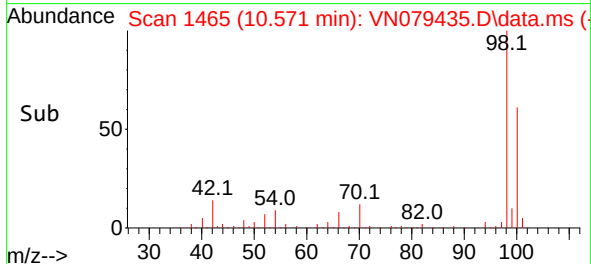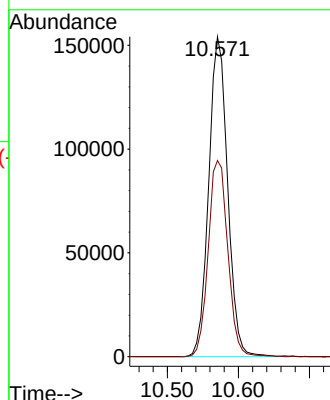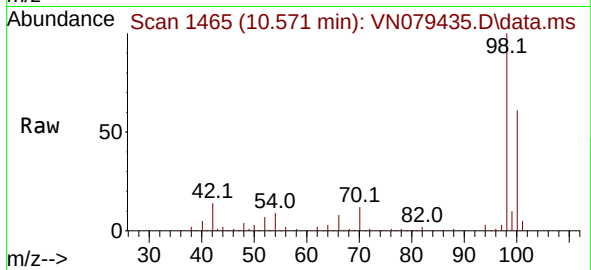

#62
4-Bromofluorobenzene
Concen: 49.559 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079435.D
Acq: 06 Oct 2023 09:57

Tgt Ion: 95 Resp: 119685
Ion Ratio Lower Upper
95 100
174 77.1 0.0 143.8
176 73.5 0.0 135.8


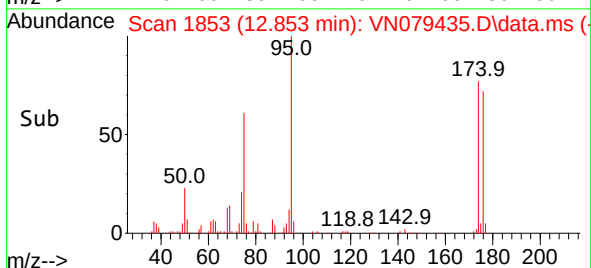
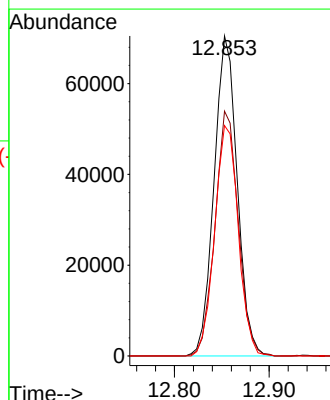
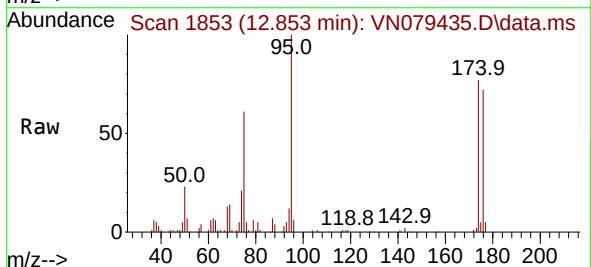


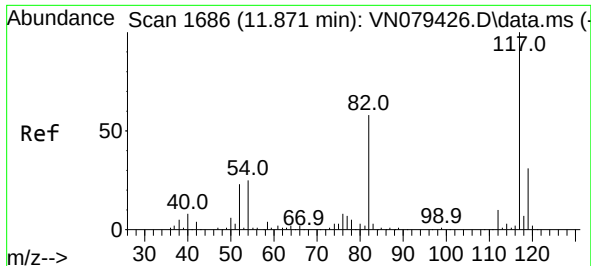

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN079435.D
Acq: 06 Oct 2023 09:57

Instrument :
MSVOA_N
ClientSampleId :
VN1006MBL01

Tgt Ion:117 Resp: 273401
Ion Ratio Lower Upper
117 100
82 59.7 44.0 66.0
119 34.0 25.6 38.4

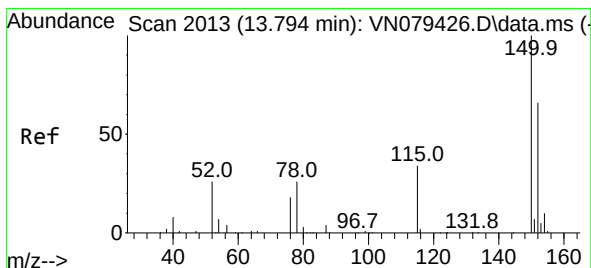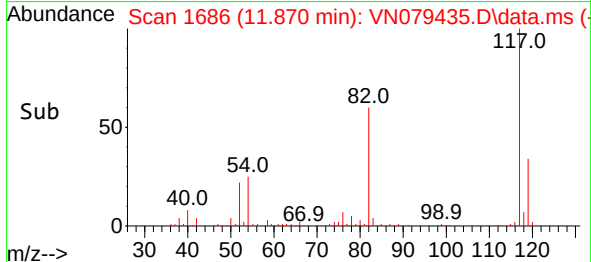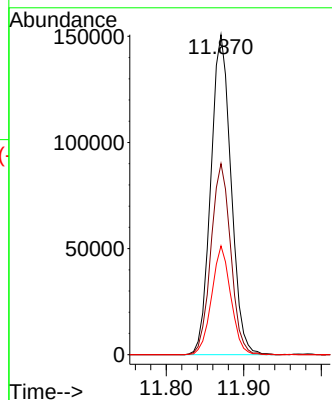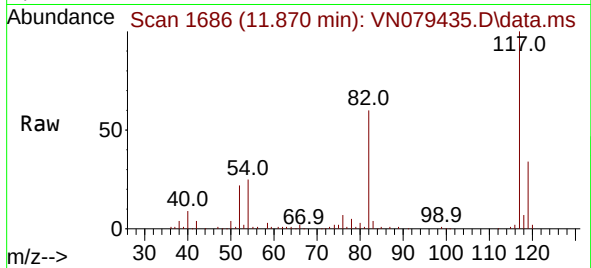

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. 0.006 min
Lab File: VN079435.D
Acq: 06 Oct 2023 09:57

Tgt Ion:152 Resp: 96622
Ion Ratio Lower Upper
152 100
115 60.7 32.3 96.8
150 161.6 0.0 355.8

