
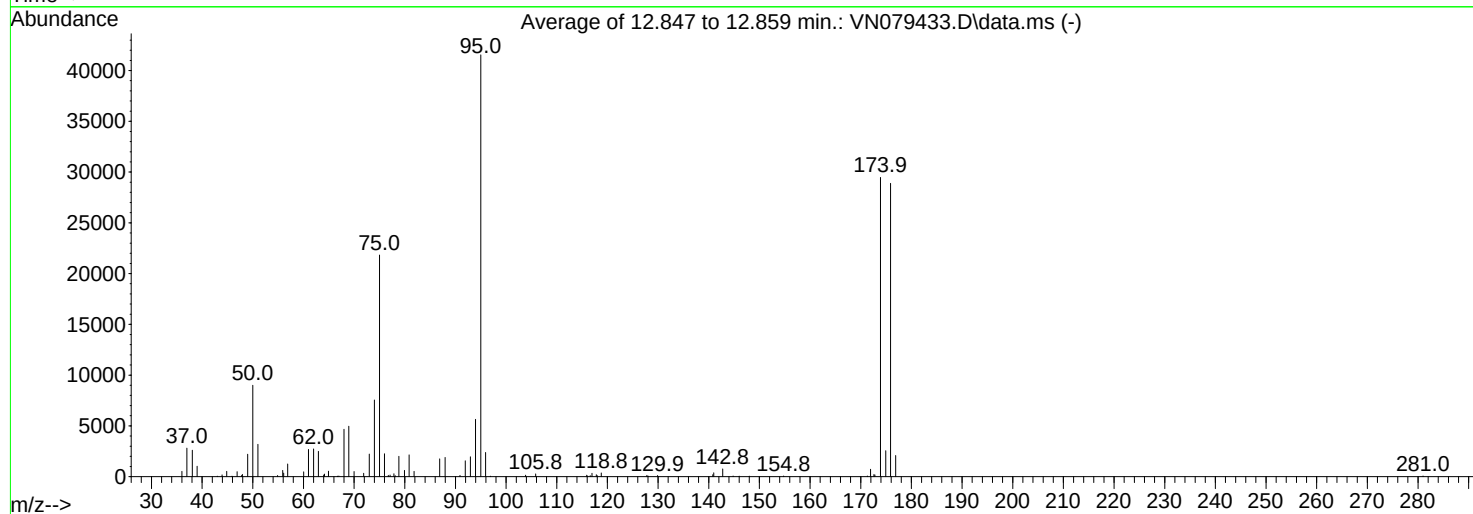


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100623\
Data File : VN079433.D
Acq On : 06 Oct 2023 08:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Title : SW846 8260
Last Update : Fri Oct 06 03:34:49 2023

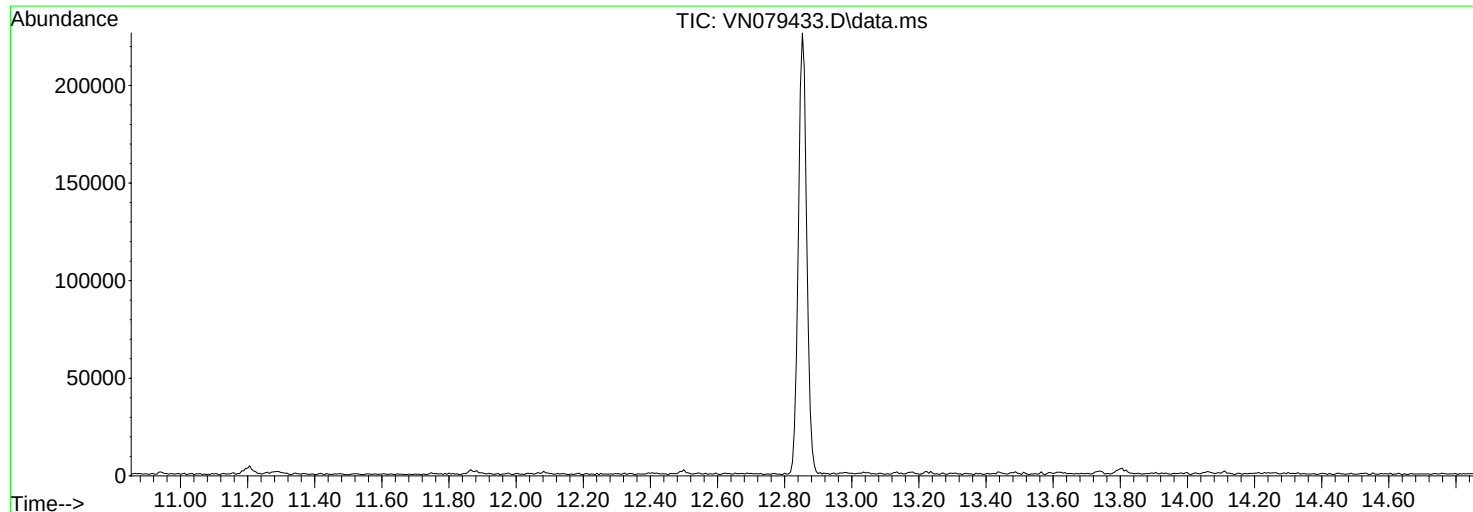

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	8997	PASS
75	95	30	60	52.6	21837	PASS
95	95	100	100	100.0	41547	PASS
96	95	5	9	5.7	2378	PASS
173	174	0.00	2	0.6	181	PASS
174	95	50	100	70.9	29472	PASS
175	174	5	9	8.7	2550	PASS
176	174	95	101	98.0	28883	PASS
177	176	5	9	7.2	2079	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	514	49.00	2212	64.00	162	75.00	2183
37.00	2812	50.00	8997	64.15	257	76.00	2251
38.05	2597	51.00	3182	64.95	541	76.75	1215
39.00	1019	54.90	119	66.70	55	77.10	151
43.00	51	55.90	615	67.00	57	77.85	280
43.95	179	56.10	353	68.00	4669	78.10	101
44.85	529	56.90	1250	68.95	4959	78.85	1996
45.90	52	60.05	473	70.00	500	79.95	615
46.90	496	61.00	2677	71.90	337	80.85	2148
47.80	118	62.00	2728	73.00	2228	81.85	526
47.95	214	62.95	2496	74.00	7546	86.90	1749

Average of 12.847 to 12.859 min.: VN079433.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	1898	116.10	58	142.75	756	175.90	28883
90.90	130	116.60	88	144.80	70	176.90	2079
91.95	1568	116.95	331	146.00	52	281.00	71
92.95	1960	117.80	188	148.00	54		
93.95	5649	118.00	98	154.80	57		
95.00	41547	118.80	371	171.30	71		
95.95	2378	127.80	125	171.95	723		
96.90	54	128.00	62	172.60	198		
103.85	142	129.90	113	172.80	181		
105.85	262	140.80	191	173.90	29472		
115.90	137	141.00	374	174.95	2550		

Instrument :

MSVOA_N

ClientSampleId :

BFB