


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100719\
Data File : VN058557.D
Acq On : 7 Oct 2019 10:55
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N092419W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Sep 25 01:36:25 2019

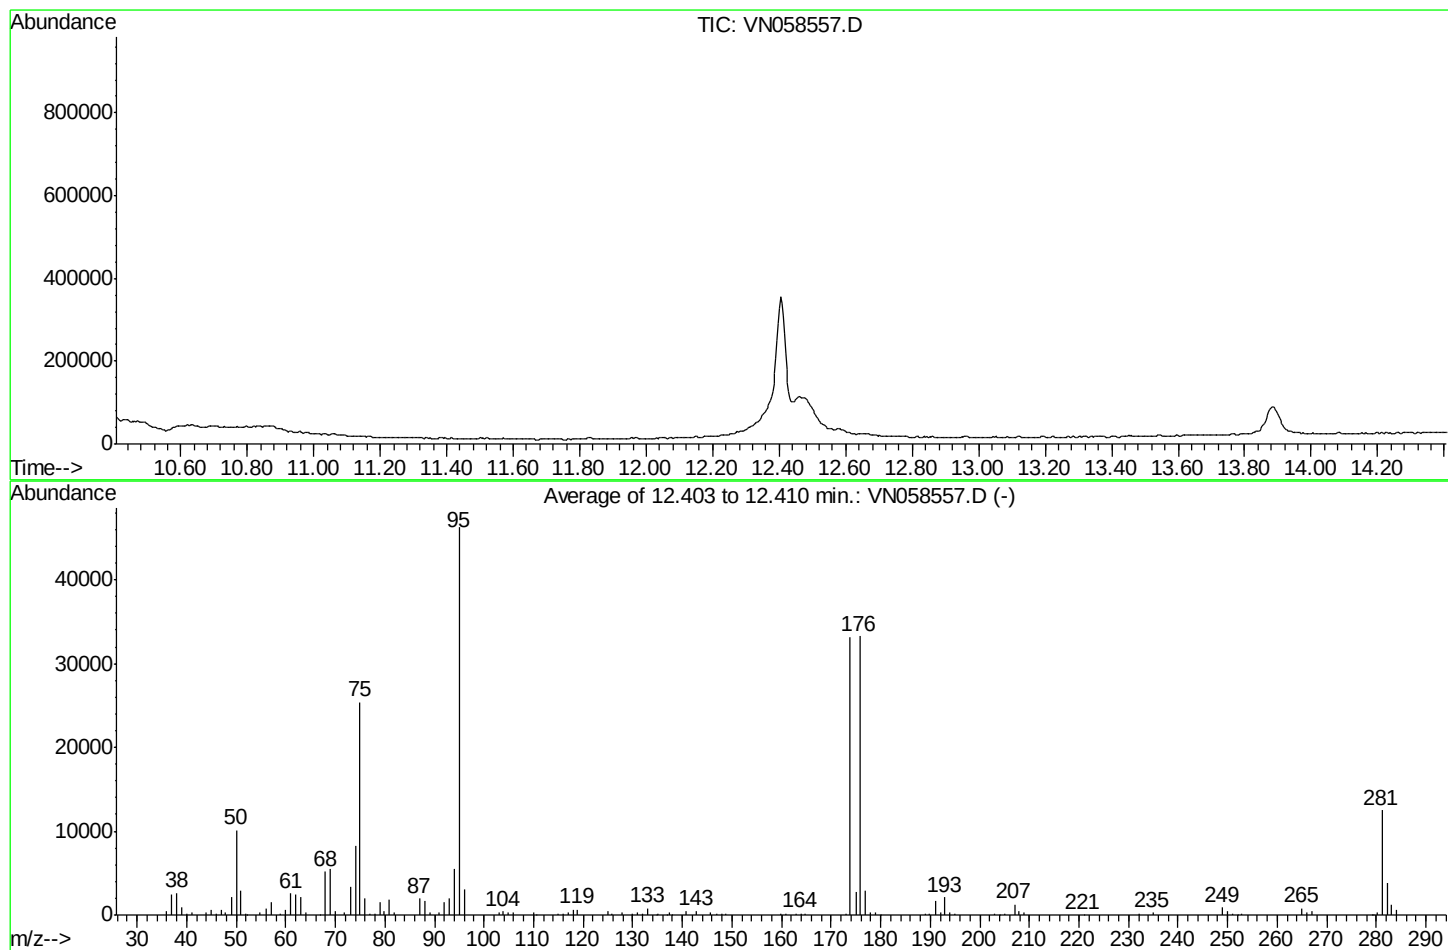

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	10095	PASS
75	95	30	60	54.9	25402	PASS
95	95	100	100	100.0	46258	PASS
96	95	5	9	6.6	3042	PASS
173	174	0.00	2	0.5	154	PASS
174	95	50	100	71.6	33098	PASS
175	174	5	9	8.2	2730	PASS
176	174	95	101	100.4	33237	PASS
177	176	5	9	8.6	2868	PASS