


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100719\
Data File : VN058565.D
Acq On : 7 Oct 2019 14:24
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092719W.M
Title : SW846 8260
Last Update : Mon Sep 30 08:07:38 2019

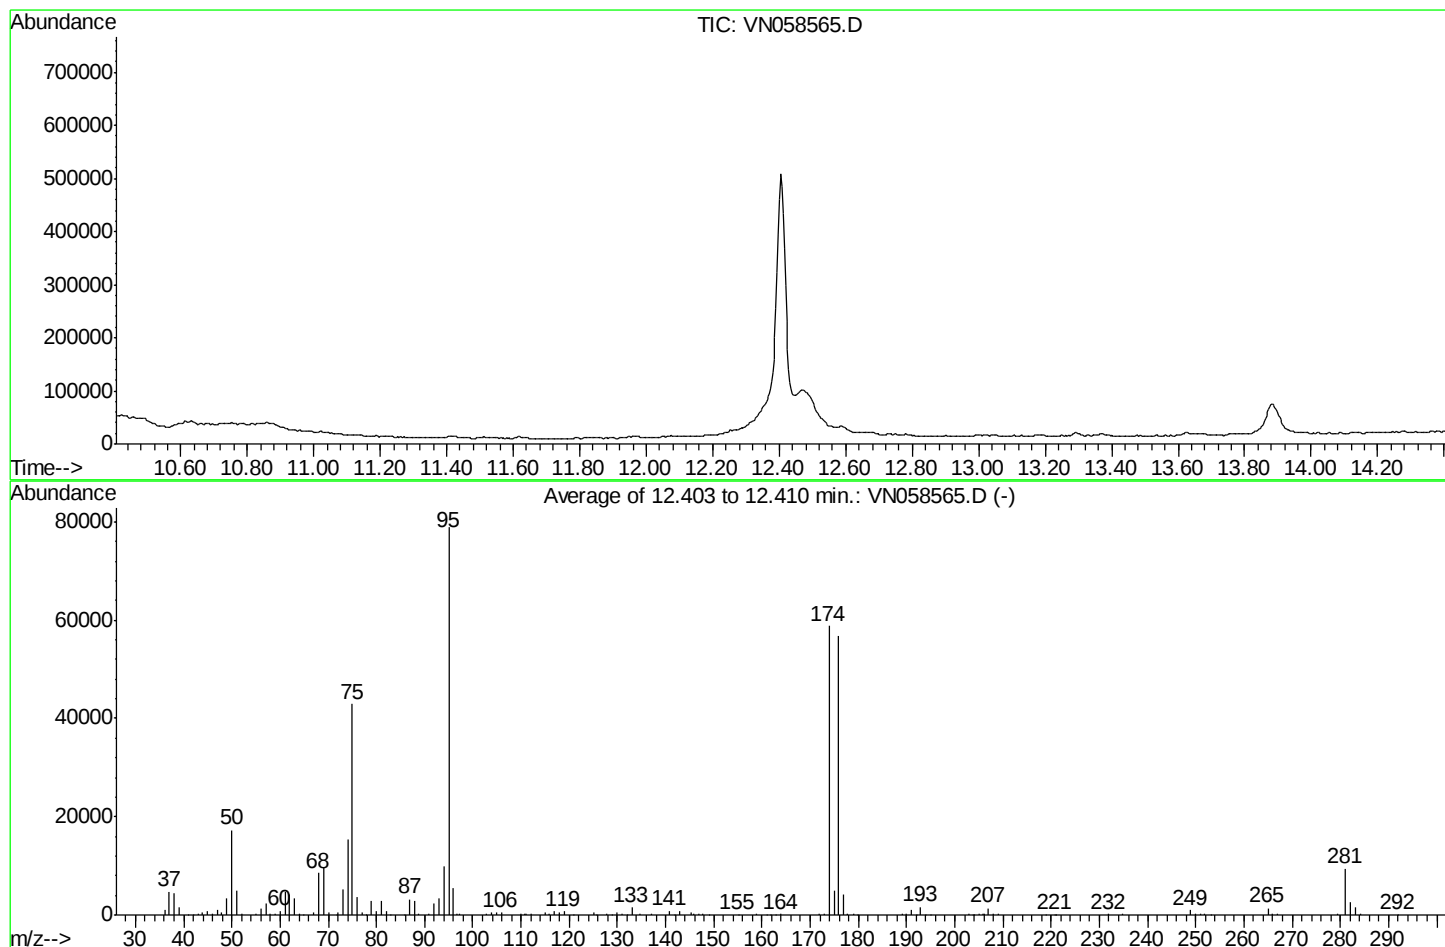

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	17293	PASS
75	95	30	60	54.3	42864	PASS
95	95	100	100	100.0	78885	PASS
96	95	5	9	7.0	5553	PASS
173	174	0.00	2	0.4	210	PASS
174	95	50	100	74.5	58778	PASS
175	174	5	9	8.4	4948	PASS
176	174	95	101	96.5	56746	PASS
177	176	5	9	7.6	4304	PASS