

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100720\
 Data File : VN063968.D
 Acq On : 8 Oct 2020 2:53
 Operator : JC/MD
 Sample : PB132153ZHE#04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132153ZHE#04

Quant Time: Oct 08 05:10:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.62	168	236895	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	443755	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	461399	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	187221	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	201158	51.40	ug/l	0.00
Spiked Amount			Recovery	=	102.80%	
35) Dibromofluoromethane	7.55	113	148267	48.15	ug/l	0.00
Spiked Amount			Recovery	=	96.30%	
50) Toluene-d8	10.06	98	573655	49.15	ug/l	0.00
Spiked Amount			Recovery	=	98.30%	
62) 4-Bromofluorobenzene	12.38	95	223753	50.99	ug/l	0.00
Spiked Amount			Recovery	=	101.98%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.74	59	341	0.789	ug/l #	71
16) Acetone	3.78	43	11970	9.936	ug/l	96
17) Carbon Disulfide	4.01	76	552	0.785	ug/l #	76
18) Methyl Acetate	4.30	43	3674	1.175	ug/l #	70
20) Methylene Chloride	4.51	84	11222	4.157	ug/l	89
25) 2-Butanone	6.79	43	2578	1.509	ug/l #	82
29) Tetrahydrofuran	7.15	42	251	0.219	ug/l #	36
31) Cyclohexane	7.63	56	6379	1.404	ug/l #	49
36) 1,1-Dichloropropene	7.63	75	21070	4.687	ug/l #	47
38) Carbon Tetrachloride	7.62	117	24966	4.952	ug/l #	15
41) Methacrylonitrile	7.17	41	417	0.210	ug/l #	44
43) Isopropyl Acetate	8.13	43	92204	12.515	ug/l	99
45) 1,2-Dichloropropane	9.23	63	2075	0.598	ug/l #	44
48) Methyl methacrylate	9.23	41	169853	46.664	ug/l #	45
49) 1,4-Dioxane	9.17	88	33	0.638	ug/l #	20
51) 4-Methyl-2-Pentanone	9.95	43	9310	2.153	ug/l	96
54) cis-1,3-Dichloropropene	9.87	75	35704	6.460	ug/l #	66
56) Ethyl methacrylate	10.51	69	2484	0.550	ug/l #	1
57) 1,3-Dichloropropane	10.73	76	5520	1.024	ug/l #	43
59) 2-Hexanone	10.74	43	110280	34.336	ug/l #	53
74) N-amyl acetate	12.00	43	5023	2.972	ug/l #	48
76) 1,2,3-Trichloropropane	12.38	75	121115	29.346	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.70	105	3454	0.301	ug/l	91
81) trans-1,4-Dichloro-2-buten	12.38	75	121115	84.522	ug/l #	6
95) Naphthalene	15.11	128	324	1.955	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN100720\
Data File : VN063968.D
Acq On : 8 Oct 2020 2:53
Operator : JC/MD
Sample : PB132153ZHE#04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB132153ZHE#04

Quant Time: Oct 08 05:10:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration





#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. -0.00 min

Lab File: VN063968.D

Acq: 8 Oct 2020 2:53

Instrument :

MSVOA_N

ClientSampleId :


PB132153ZHE#04

Tot Ion:168 Resp: 236895

Ion Ratio Lower Upper

168 100

99 63.4 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.62

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#11

Tert butyl alcohol

Concen: 0.789 ug/l

RT: 4.74 min Scan# 934

Delta R.T. 0.02 min

Lab File: VN063968.D


Acq: 8 Oct 2020 2:53

Tgt Ion: 59 Resp: 341

Ion Ratio Lower Upper

59 100

57 0.0 8.7 13.1#



Abundance Ion 59.00 (58.70 to 59.70): VN

Ion 57.00 (56.70 to 57.70): VN

4.74

300

250

200


150


100

50

0

Time--> 4.72 4.74 4.76





#16

Acetone

Concen: 9.936 ug/l

RT: 3.78 min Scan# 635

Delta R.T. 0.01 min

Lab File: VN063968.D

Acq: 8 Oct 2020 2:53

Instrument :

MSVOA_N

ClientSampleId :


PB132153ZHE#04

Tot Ion: 43 Resp: 11970




Ion Ratio Lower Upper

43 100

58 30.0 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-599) (-)



#17

Carbon Disulfide

Concen: 0.785 ug/l

RT: 4.01 min Scan# 706

Delta R.T. -0.00 min

Lab File: VN063968.D


Acq: 8 Oct 2020 2:53

Tgt Ion: 76 Resp: 552



Ion Ratio Lower Upper


76 100

78 0.0 7.0 10.4#



Abundance Ion 75.90 (75.60 to 76.60): VN063741.D (-685) (-)







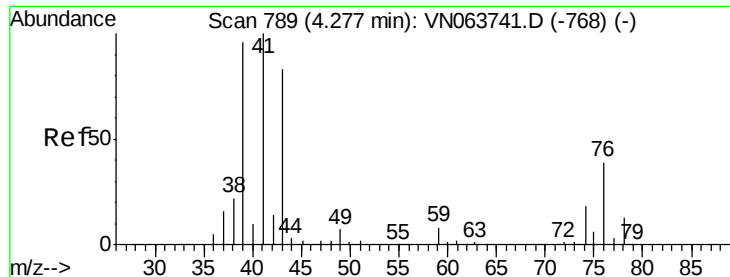

#18
Methyl Acetate
Concen: 1.175 ug/l
RT: 4.30 min Scan# 795
Delta R.T. 0.02 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53




Instrument :
MSVOA_N
ClientSampleId :
PB132153ZHE#04


Tot Ion: 43 Resp: 3674
Ion Ratio Lower Upper
43 100
74 7.8 17.4 26.2#



#20
Methylene Chloride
Concen: 4.157 ug/l
RT: 4.51 min Scan# 860
Delta R.T. 0.00 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Tgt Ion: 84 Resp: 11222
Ion Ratio Lower Upper
84 100
49 123.0 110.4 165.6
51 35.0 33.3 49.9
86 58.0 50.7 76.1







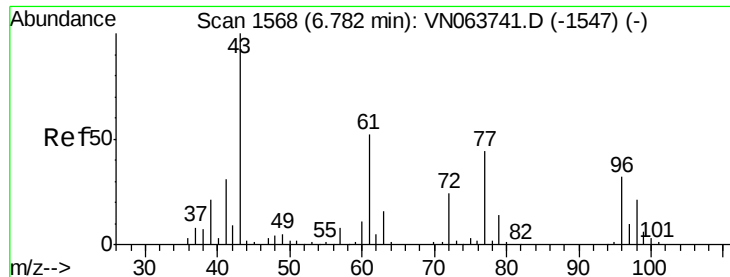

#25
2-Butanone
Concen: 1.509 ug/l
RT: 6.79 min Scan# 1570
Delta R.T. 0.01 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53




Instrument :
MSVOA_N
ClientSampleId :
PB132153ZHE#04


Tot Ion: 43 Resp: 2578
Ion Ratio Lower Upper
43 100
72 15.3 19.3 28.9#



#29
Tetrahydrofuran
Concen: 0.219 ug/l
RT: 7.15 min Scan# 1683
Delta R.T. -0.01 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Tgt Ion: 42 Resp: 251
Ion Ratio Lower Upper
42 100
72 0.0 32.8 49.2#
71 0.0 30.6 45.8#




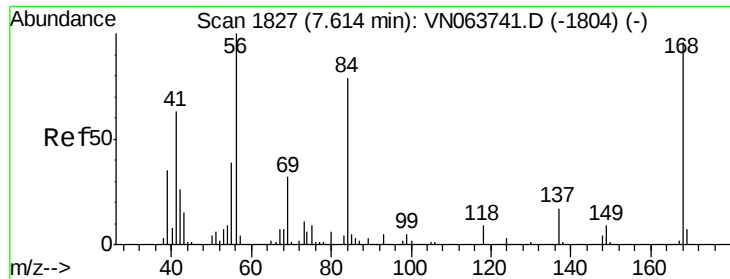




#31
Cyclohexane
Concen: 1.404 ug/l
RT: 7.63 min Scan# 1831
Delta R.T. 0.01 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Instrument :
MSVOA_N
ClientSampleId :
PB132153ZHE#04

Tot Ion: 56 Resp: 6379
Ion Ratio Lower Upper
56 100
69 126.6 25.4 38.2#
84 76.6 63.3 94.9




Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0






#33
1,2-Dichloroethane-d4
Concen: 51.399 ug/l
RT: 7.99 min Scan# 1943
Delta R.T. 0.00 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Tgt Ion: 65 Resp: 201158
Ion Ratio Lower Upper
65 100
67 49.0 0.0 99.6



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0









#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.55 min Scan# 2118
Delta R.T. 0.00 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Instrument :
MSVOA_N
ClientSampleId :
PB132153ZHE#04

Tot Ion:114 Resp: 443755
Ion Ratio Lower Upper
114 100
63 22.7 0.0 45.0
88 17.1 0.0 34.0




Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN






#35
Dibromofluoromethane
Concen: 48.153 ug/l
RT: 7.55 min Scan# 1807
Delta R.T. 0.00 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Tgt Ion:113 Resp: 148267
Ion Ratio Lower Upper
113 100
111 101.4 81.8 122.8
192 19.3 14.2 21.2



Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V









#36
 1,1-Dichloropropene
 Concen: 4.687 ug/l
 RT: 7.63 min Scan# 1831
 Delta R.T. -0.13 min
 Lab File: VN063968.D
 Acq: 8 Oct 2020 2:53

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132153ZHE#04

Tot Ion: 75 Resp: 21070
 Ion Ratio Lower Upper
 75 100
 110 4.9 16.9 50.6#
 77 0.0 24.5 36.7#




Abundance Ion 74.90 (74.60 to 75.60): VN0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VN0






#38
 Carbon Tetrachloride
 Concen: 4.952 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.11 min
 Lab File: VN063968.D
 Acq: 8 Oct 2020 2:53

Tgt Ion: 117 Resp: 24966
 Ion Ratio Lower Upper
 117 100
 119 6.3 80.1 120.1#
 121 0.0 25.7 38.5#



Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V





#41

Methacrylonitrile

Concen: 0.210 ug/l

RT: 7.17 min Scan# 1690

Delta R.T. 0.05 min

Lab File: VN063968.D

Acq: 8 Oct 2020 2:53

Instrument :

MSVOA_N

ClientSampleId :

PB132153ZHE#04

Tot Ion: 41 Resp: 417





Ion Ratio Lower Upper

41 100

39 43.2 42.5 63.7

67 0.0 57.4 86.2#

52 0.0 26.9 40.3#



#43

Isopropyl Acetate

Concen: 12.515 ug/l

RT: 8.13 min Scan# 1986

Delta R.T. 0.00 min

Lab File: VN063968.D

Acq: 8 Oct 2020 2:53




Tgt Ion: 43 Resp: 92204


Ion Ratio Lower Upper

43 100

61 17.1 14.2 21.4

87 11.5 9.0 13.6









#45
 1,2-Dichloropropane
 Concen: 0.598 ug/l
 RT: 9.23 min Scan# 2330
 Delta R.T. 0.15 min
 Lab File: VN063968.D
 Acq: 8 Oct 2020 2:53




Instrument :
 MSVOA_N
 ClientSampleId :
 PB132153ZHE#04


Tot Ion: 63 Resp: 2075
 Ion Ratio Lower Upper
 63 100
 65 0.0 24.7 37.1#



#48
 Methyl methacrylate
 Concen: 46.664 ug/l
 RT: 9.23 min Scan# 2331
 Delta R.T. 0.07 min
 Lab File: VN063968.D
 Acq: 8 Oct 2020 2:53

Tgt Ion: 41 Resp: 169853
 Ion Ratio Lower Upper
 41 100
 69 0.0 60.9 91.3#
 39 56.1 57.5 86.3#









#49
1,4-Dioxane
Concen: 0.638 ug/l
RT: 9.17 min Scan# 2312
Delta R.T. 0.01 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Instrument :
MSVOA_N
ClientSampleId :
PB132153ZHE#04

Tot Ion: 88 Resp: 33
Ion Ratio Lower Upper
88 100
43 0.0 33.1 49.7#
58 0.0 58.9 88.3#




Abundance Ion 88.00 (87.70 to 88.70): VN0
Ion 43.00 (42.70 to 43.70): VN0
Ion 58.00 (57.70 to 58.70): VN0






#50
Toluene-d8
Concen: 49.146 ug/l
RT: 10.06 min Scan# 2588
Delta R.T. 0.00 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Tgt Ion: 98 Resp: 573655
Ion Ratio Lower Upper
98 100
100 63.9 49.8 74.6



Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0





#51

4-Methyl-2-Pentanone

Concen: 2.153 ug/l

RT: 9.95 min Scan# 2554

Delta R.T. 0.00 min

Lab File: VN063968.D

Acq: 8 Oct 2020 2:53

Instrument :

MSVOA_N

ClientSampleId :


PB132153ZHE#04

Tot Ion: 43 Resp: 9310

Ion Ratio Lower Upper

43 100

58 33.1 28.4 42.6



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-2537) (-)

Ion 58.00 (57.70 to 58.70): VN063741.D (-2537) (-)

20000



15000

10000

5000

0

Time--> 9.90 9.95



#54

cis-1,3-Dichloropropene

Concen: 6.460 ug/l

RT: 9.87 min Scan# 2529

Delta R.T. 0.06 min

Lab File: VN063968.D

Acq: 8 Oct 2020 2:53


Tgt Ion: 75 Resp: 35704

Ion Ratio Lower Upper

75 100

77 0.0 24.6 36.8#

39 44.3 49.7 74.5#



Abundance Ion 74.90 (74.60 to 75.60): VN063741.D (-2493) (-)

Ion 76.90 (76.60 to 77.60): VN063741.D (-2493) (-)

Ion 39.00 (38.70 to 39.70): VN063741.D (-2493) (-)

25000

20000


15000


10000

5000

0

Time--> 9.80 9.85 9.90 9.95





#56

Ethyl methacrylate

Concen: 0.550 ug/l

RT: 10.51 min Scan# 2729

Delta R.T. 0.12 min

Lab File: VN063968.D

Acq: 8 Oct 2020 2:53

Instrument :

MSVOA_N

ClientSampleId :

PB132153ZHE#04





Tot Ion: 69 Resp: 2484

Ion Ratio Lower Upper

69 100

41 4011.8 61.1 91.7#

39 1724.0 42.2 63.4#



#57

1,3-Dichloropropane

Concen: 1.024 ug/l

RT: 10.73 min Scan# 2797

Delta R.T. 0.05 min

Lab File: VN063968.D




Acq: 8 Oct 2020 2:53


Tgt Ion: 76 Resp: 5520

Ion Ratio Lower Upper

76 100

78 0.0 25.2 37.8#









#59
2-Hexanone
Concen: 34.336 ug/l
RT: 10.74 min Scan# 2798
Delta R.T. 0.02 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53




Instrument :
MSVOA_N
ClientSampleId :
PB132153ZHE#04


Tot Ion: 43 Resp: 110280
Ion Ratio Lower Upper
43 100
58 17.3 24.6 73.8#



#62
4-Bromofluorobenzene
Concen: 50.994 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Tgt Ion: 95 Resp: 223753
Ion Ratio Lower Upper
95 100
174 76.4 0.0 150.6
176 73.2 0.0 145.4









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Instrument :
MSVOA_N
ClientSampleId :
PB132153ZHE#04

Tot Ion:117 Resp: 461399
Ion Ratio Lower Upper
117 100
82 60.0 47.4 71.2
119 32.8 26.4 39.6




Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN063968.D
Acq: 8 Oct 2020 2:53

Tgt Ion:152 Resp: 187221
Ion Ratio Lower Upper
152 100
115 61.8 31.3 93.8
150 155.1 0.0 341.8



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V





#74

N-amvl acetate

Concen: 2.972 ug/l

RT: 12.00 min Scan# 3191

Delta R.T. -0.04 min

Lab File: VN063968.D

Acq: 8 Oct 2020 2:53

Instrument :

MSVOA_N

ClientSampleId :

PB132153ZHE#04

Tot Ion: 43 Resp: 5023



Ion Ratio Lower Upper

43 100

70 0.0 29.8 44.8#

55 2.6 17.9 26.9#

61 0.0 17.0 25.4#





Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0



#76

1,2,3-Trichloropropane

Concen: 29.346 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN063968.D



Acq: 8 Oct 2020 2:53

Tgt Ion: 75 Resp: 121115

Ion Ratio Lower Upper


75 100


77 1.2 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0









#80
 1,3,5-Trimethylbenzene
 Concen: 0.301 ug/l
 RT: 12.70 min Scan# 3410
 Delta R.T. -0.00 min
 Lab File: VN063968.D
 Acq: 8 Oct 2020 2:53




Instrument :
 MSVOA_N
 ClientSampleId :
 PB132153ZHE#04


Tot Ion:105 Resp: 3454
 Ion Ratio Lower Upper
 105 100
 120 40.8 23.3 69.9



#81
 trans-1,4-Dichloro-2-butene
 Concen: 84.522 ug/l
 RT: 12.38 min Scan# 3308
 Delta R.T. 0.10 min
 Lab File: VN063968.D
 Acq: 8 Oct 2020 2:53

Tgt Ion: 75 Resp: 121115
 Ion Ratio Lower Upper
 75 100
 53 0.3 88.2 132.2#
 89 0.0 36.0 54.0#





#95

Naphthalene

Concen: 1.955 ug/l

RT: 15.11 min Scan# 4159

Delta R.T. 0.01 min

Lab File: VN063968.D


Acq: 8 Oct 2020 2:53

Instrument :

MSVOA_N

ClientSampleId :

PB132153ZHE#04




Tot Ion:128 Resp: 324

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#


129 0.0 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V



Time-->