


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100720\
 Data File : VN063933.D
 Acq On : 7 Oct 2020 9:53
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N0100217W.M
 Title : SW846 8260
 Last Update : Mon Oct 02 13:46:34 2017

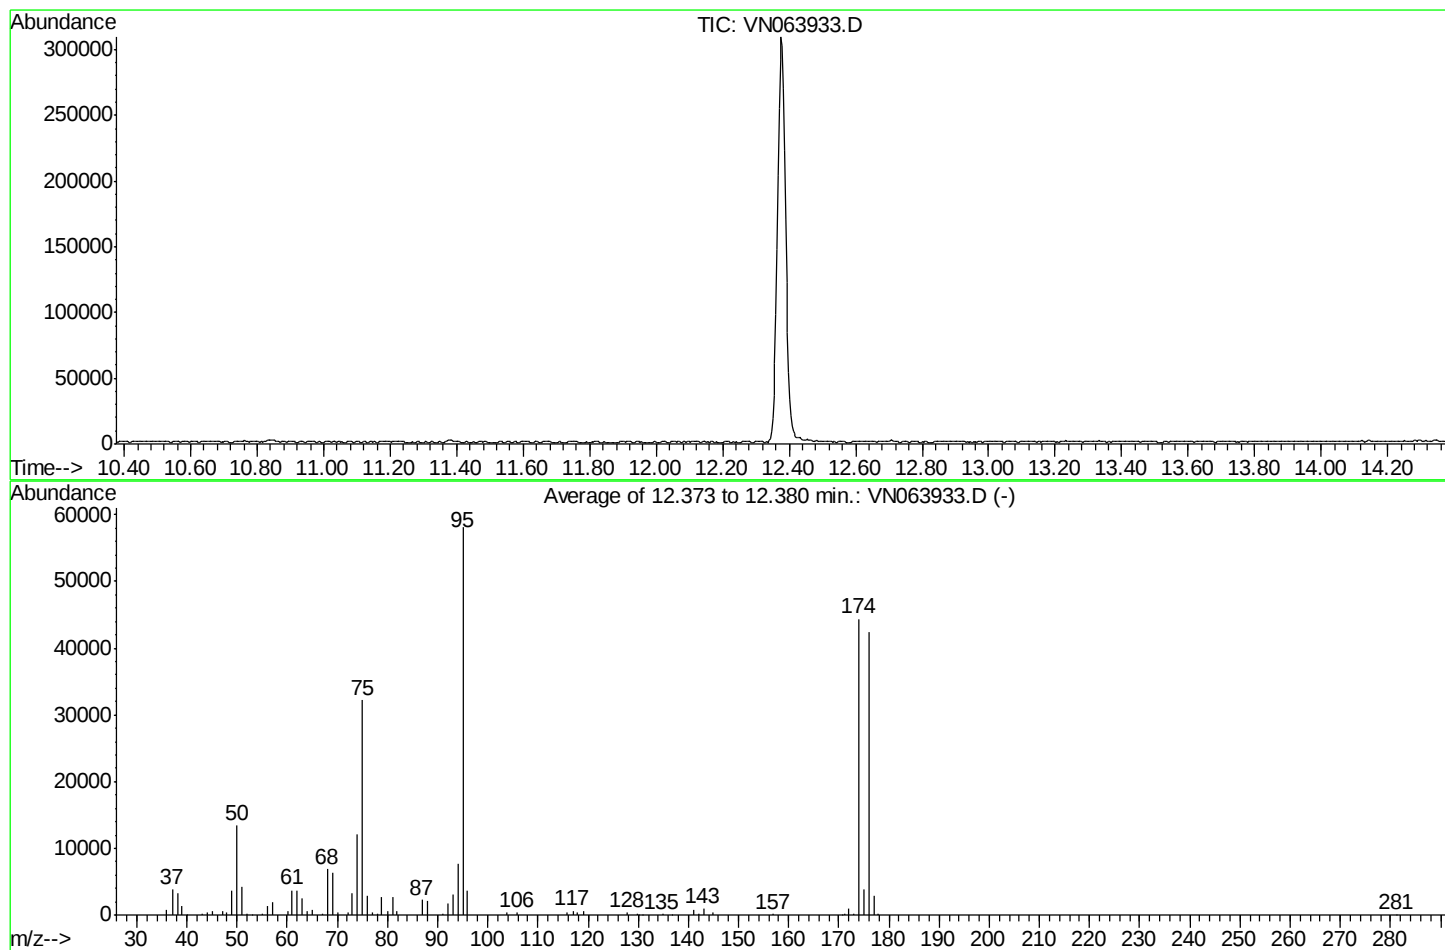

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	13378	PASS
75	95	30	60	55.4	32200	PASS
95	95	100	100	100.0	58122	PASS
96	95	5	9	6.2	3590	PASS
173	174	0.00	2	0.6	280	PASS
174	95	50	100	76.4	44392	PASS
175	174	5	9	8.5	3754	PASS
176	174	95	101	95.7	42488	PASS
177	176	5	9	6.6	2824	PASS