


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100720\  
Data File : VN063959.D  
Acq On : 7 Oct 2020 22:30  
Operator : JC/MD  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 32 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N0100217W.M  
Title : SW846 8260  
Last Update : Mon Oct 02 13:46:34 2017

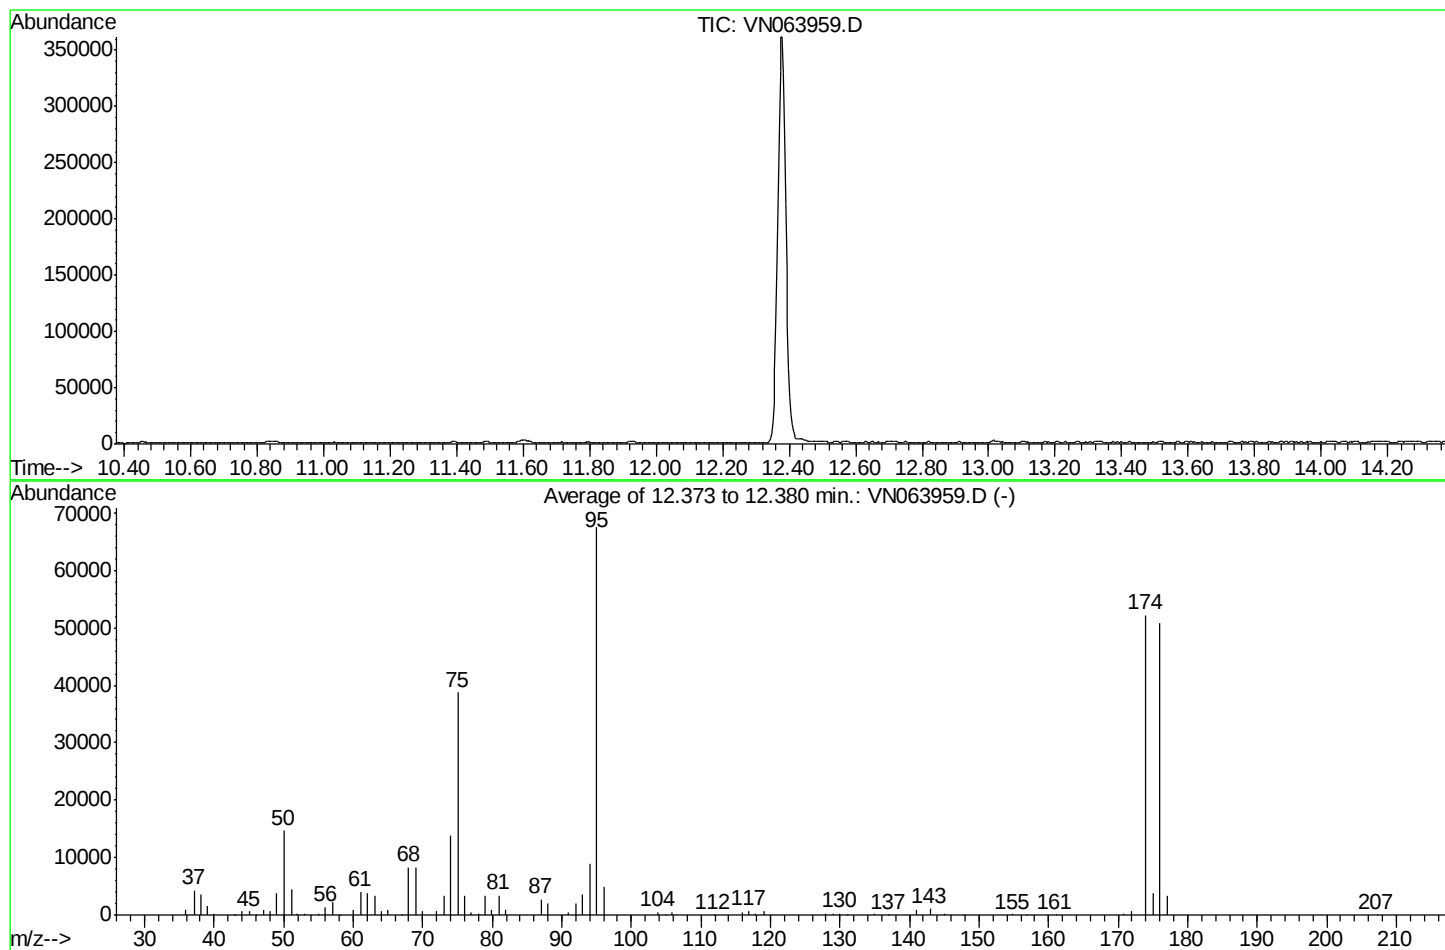

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 21.7      | 14643   | PASS             |
| 75          | 95           | 30           | 60           | 57.4      | 38728   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 67504   | PASS             |
| 96          | 95           | 5            | 9            | 7.2       | 4865    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 77.4      | 52224   | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 3904    | PASS             |
| 176         | 174          | 95           | 101          | 97.4      | 50864   | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 3387    | PASS             |