

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100721\
 Data File : VN068841.D
 Acq On : 7 Oct 2021 15:07
 Operator : JC/MD
 Sample : M4057-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SHAFT-17B-SP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100621W.M

Title : SW846 8260

Signal : TIC: VN068841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.103	1138	1161	1190	rVB2	30667	100815	1.85%	0.340%
2	8.024	2226	2250	2261	rBV2	363067	876028	16.04%	2.958%
3	8.088	2262	2274	2302	rVB	647190	1491862	27.32%	5.037%
4	8.440	2383	2405	2431	rBV2	411233	947294	17.35%	3.198%
5	8.566	2437	2452	2464	rBV4	46938	124065	2.27%	0.419%
6	8.971	2583	2603	2636	rBV	962426	2005527	36.73%	6.771%
7	9.550	2803	2819	2831	rBV3	38278	86638	1.59%	0.293%
8	9.625	2831	2847	2887	rVV	1852429	3451640	63.21%	11.654%
9	10.245	3062	3078	3099	rBV	385219	680681	12.47%	2.298%
10	10.443	3134	3152	3175	rBV	1552963	2894994	53.02%	9.774%
11	10.875	3299	3313	3329	rBV2	108175	189173	3.46%	0.639%
12	10.969	3333	3348	3366	rVV2	212749	371621	6.81%	1.255%
13	11.092	3370	3394	3416	rVV	3301147	5460465	100.00%	18.436%
14	11.181	3416	3427	3456	rVB	219548	392747	7.19%	1.326%
15	11.494	3526	3544	3578	rBV	2579525	4202451	76.96%	14.188%
16	11.746	3621	3638	3670	rVB	1433283	2553419	46.76%	8.621%
17	12.197	3794	3806	3824	rBV2	41582	72099	1.32%	0.243%
18	12.733	3990	4006	4027	rBV	1080691	1844065	33.77%	6.226%
19	13.677	4341	4358	4378	rBV	1106530	1873192	34.30%	6.324%


Sum of corrected areas: 29618776

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100721\
Data File : VN068841.D
Acq On : 7 Oct 2021 15:07
Operator : JC/MD
Sample : M4057-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SHAFT-17B-SP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100621W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

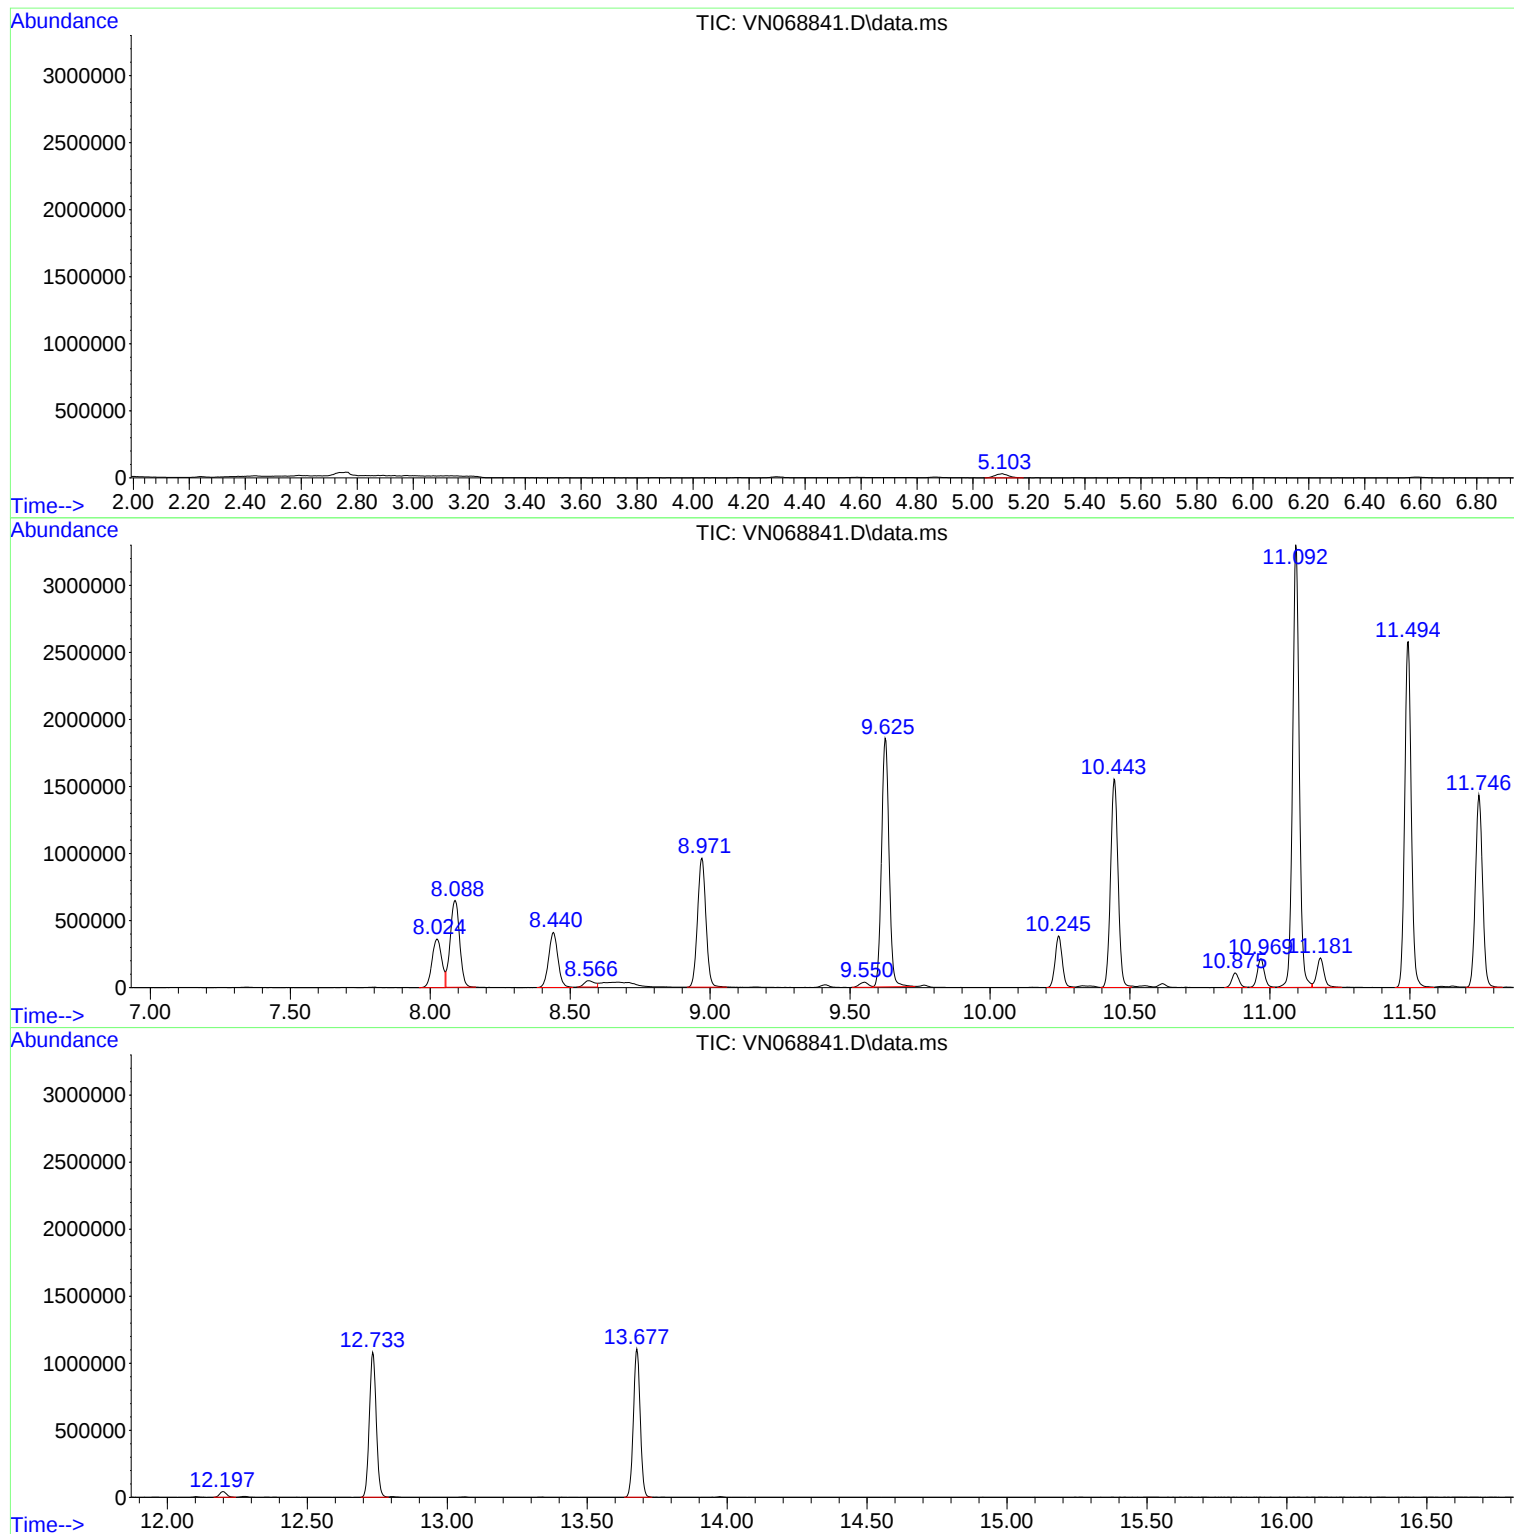

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100721\
Data File : VN068841.D
Acq On : 7 Oct 2021 15:07
Operator : JC/MD
Sample : M4057-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SHAFT-17B-SP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100621W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100721\
Data File : VN068841.D
Acq On : 7 Oct 2021 15:07
Operator : JC/MD
Sample : M4057-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SHAFT-17B-SP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100621W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
