
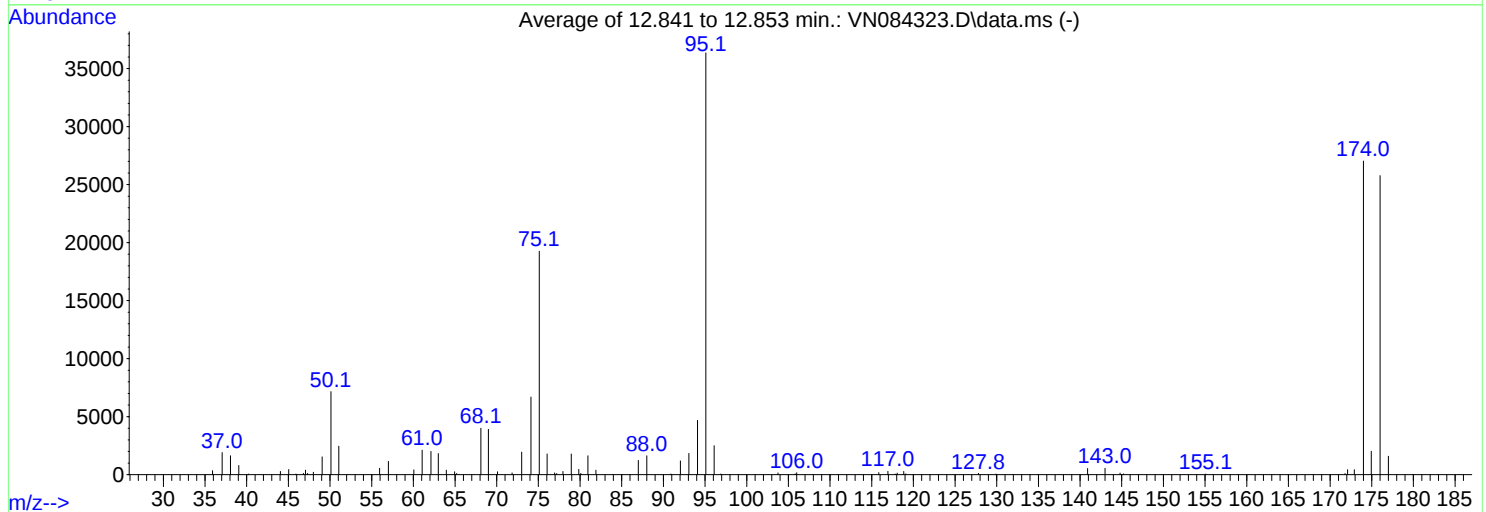


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100724\
Data File : VN084323.D
Acq On : 07 Oct 2024 09:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

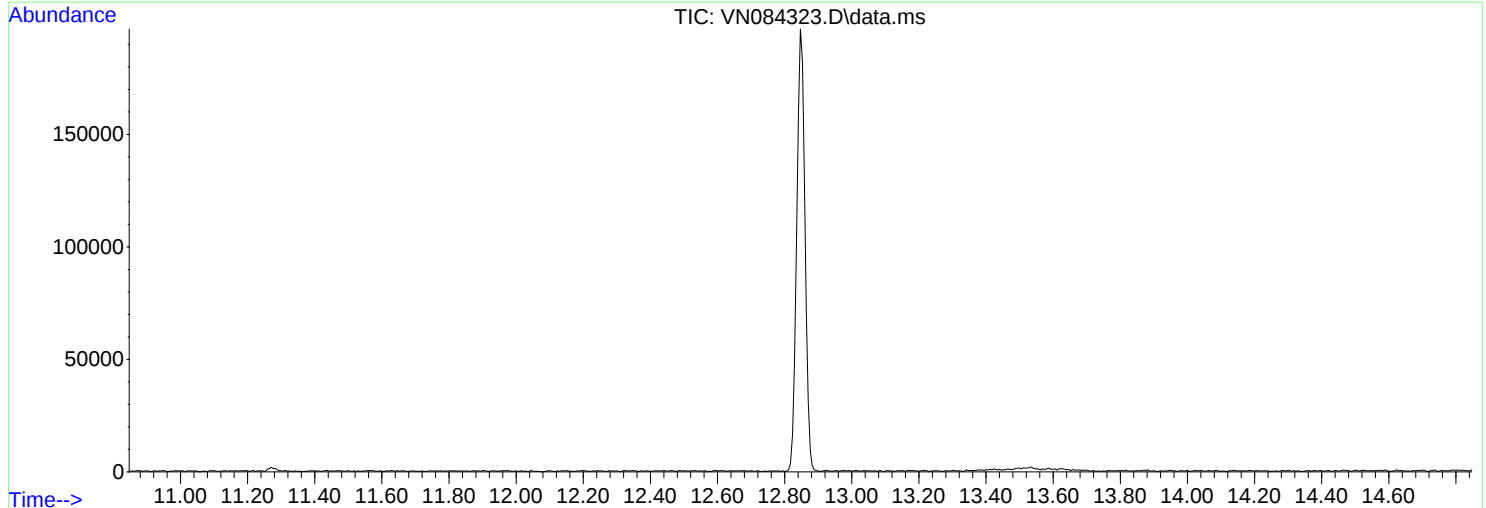

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	7162	PASS
75	95	30	60	53.0	19259	PASS
95	95	100	100	100.0	36360	PASS
96	95	5	9	6.9	2502	PASS
173	174	0.00	2	1.6	425	PASS
174	95	50	100	74.4	27037	PASS
175	174	5	9	7.5	2020	PASS
176	174	95	101	95.3	25779	PASS
177	176	5	9	6.2	1592	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	343	48.00	209	64.95	245	77.20	9
37.05	1900	49.05	1534	65.20	95	77.95	27
38.05	1634	50.10	7162	68.10	3998	78.95	178
39.05	789	51.05	2457	69.00	3906	79.85	45
40.20	60	55.95	559	70.10	255	80.10	111
44.05	283	57.00	1152	71.85	158	80.95	1622
45.05	439	60.05	415	73.00	1947	81.90	380
45.90	54	61.05	2115	74.10	6693	87.00	1234
46.80	111	62.10	2002	75.10	19259	88.00	1623
47.05	392	63.00	1818	76.05	1778	90.90	58
47.30	108	63.95	382	76.95	155	92.05	1183

Average of 12.841 to 12.853 min.: VN084323.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.05	1841	118.05	141	172.10	431		
94.10	4680	118.85	281	172.90	425		
95.10	36360	119.10	73	174.00	27037		
96.10	2502	127.80	109	174.95	2020		
96.90	51	129.90	58	176.00	25779		
103.75	157	140.90	528	177.00	1592		
105.80	77	143.00	551				
106.00	169	144.80	141				
115.85	187	145.20	66				
116.95	292	155.10	52				
117.80	60	171.80	102				

Instrument :

MSVOA_N

ClientSampleId :

BFB