

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100820\
 Data File : VN064022.D
 Acq On : 9 Oct 2020 5:40
 Operator : JC/MD
 Sample : L4291-10
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Oct 09 07:07:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	238768	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	461948	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	478567	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	182808	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	204190	51.76	ug/l	0.00
Spiked Amount			Recovery	=	103.52%	
35) Dibromofluoromethane	7.55	113	153440	47.87	ug/l	0.00
Spiked Amount			Recovery	=	95.74%	
50) Toluene-d8	10.06	98	594877	48.96	ug/l	0.00
Spiked Amount			Recovery	=	97.92%	
62) 4-Bromofluorobenzene	12.38	95	221221	48.43	ug/l	0.00
Spiked Amount			Recovery	=	96.86%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.79	43	15186	12.506	ug/l	99
17) Carbon Disulfide	4.02	76	533	0.781	ug/l #	76
18) Methyl Acetate	4.29	43	4252	1.349	ug/l #	66
20) Methylene Chloride	4.51	84	10371	3.820	ug/l	91
25) 2-Butanone	6.79	43	758	0.440	ug/l #	51
29) Tetrahydrofuran	7.17	42	460	0.398	ug/l #	36
31) Cyclohexane	7.63	56	6803	1.486	ug/l #	30
36) 1,1-Dichloropropene	7.62	75	21321	4.556	ug/l #	51
38) Carbon Tetrachloride	7.63	117	25806	4.917	ug/l #	16
41) Methacrylonitrile	7.18	41	454	0.220	ug/l #	42
43) Isopropyl Acetate	8.13	43	90371	11.783	ug/l	99
45) 1,2-Dichloropropane	9.23	63	1628	0.451	ug/l #	44
48) Methyl methacrylate	9.15	41	5518	1.456	ug/l #	12
49) 1,4-Dioxane	9.23	88	161	2.990	ug/l #	1
51) 4-Methyl-2-Pentanone	9.95	43	9432	2.096	ug/l	91
54) cis-1,3-Dichloropropene	9.87	75	33184	5.767	ug/l #	66
56) Ethyl methacrylate	10.51	69	2387	0.508	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	5892	1.050	ug/l #	43
59) 2-Hexanone	10.74	43	93776	28.048	ug/l #	55
71) Bromoform	12.37	173	1002	0.348	ug/l #	1
74) N-amyl acetate	12.01	43	3116	2.696	ug/l #	48
76) 1,2,3-Trichloropropane	12.38	75	120018	29.783	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	120018	85.778	ug/l #	6
95) Naphthalene	15.12	128	73	1.932	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100820\
Data File : VN064022.D
Acq On : 9 Oct 2020 5:40
Operator : JC/MD
Sample : L4291-10
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Oct 09 07:07:16 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

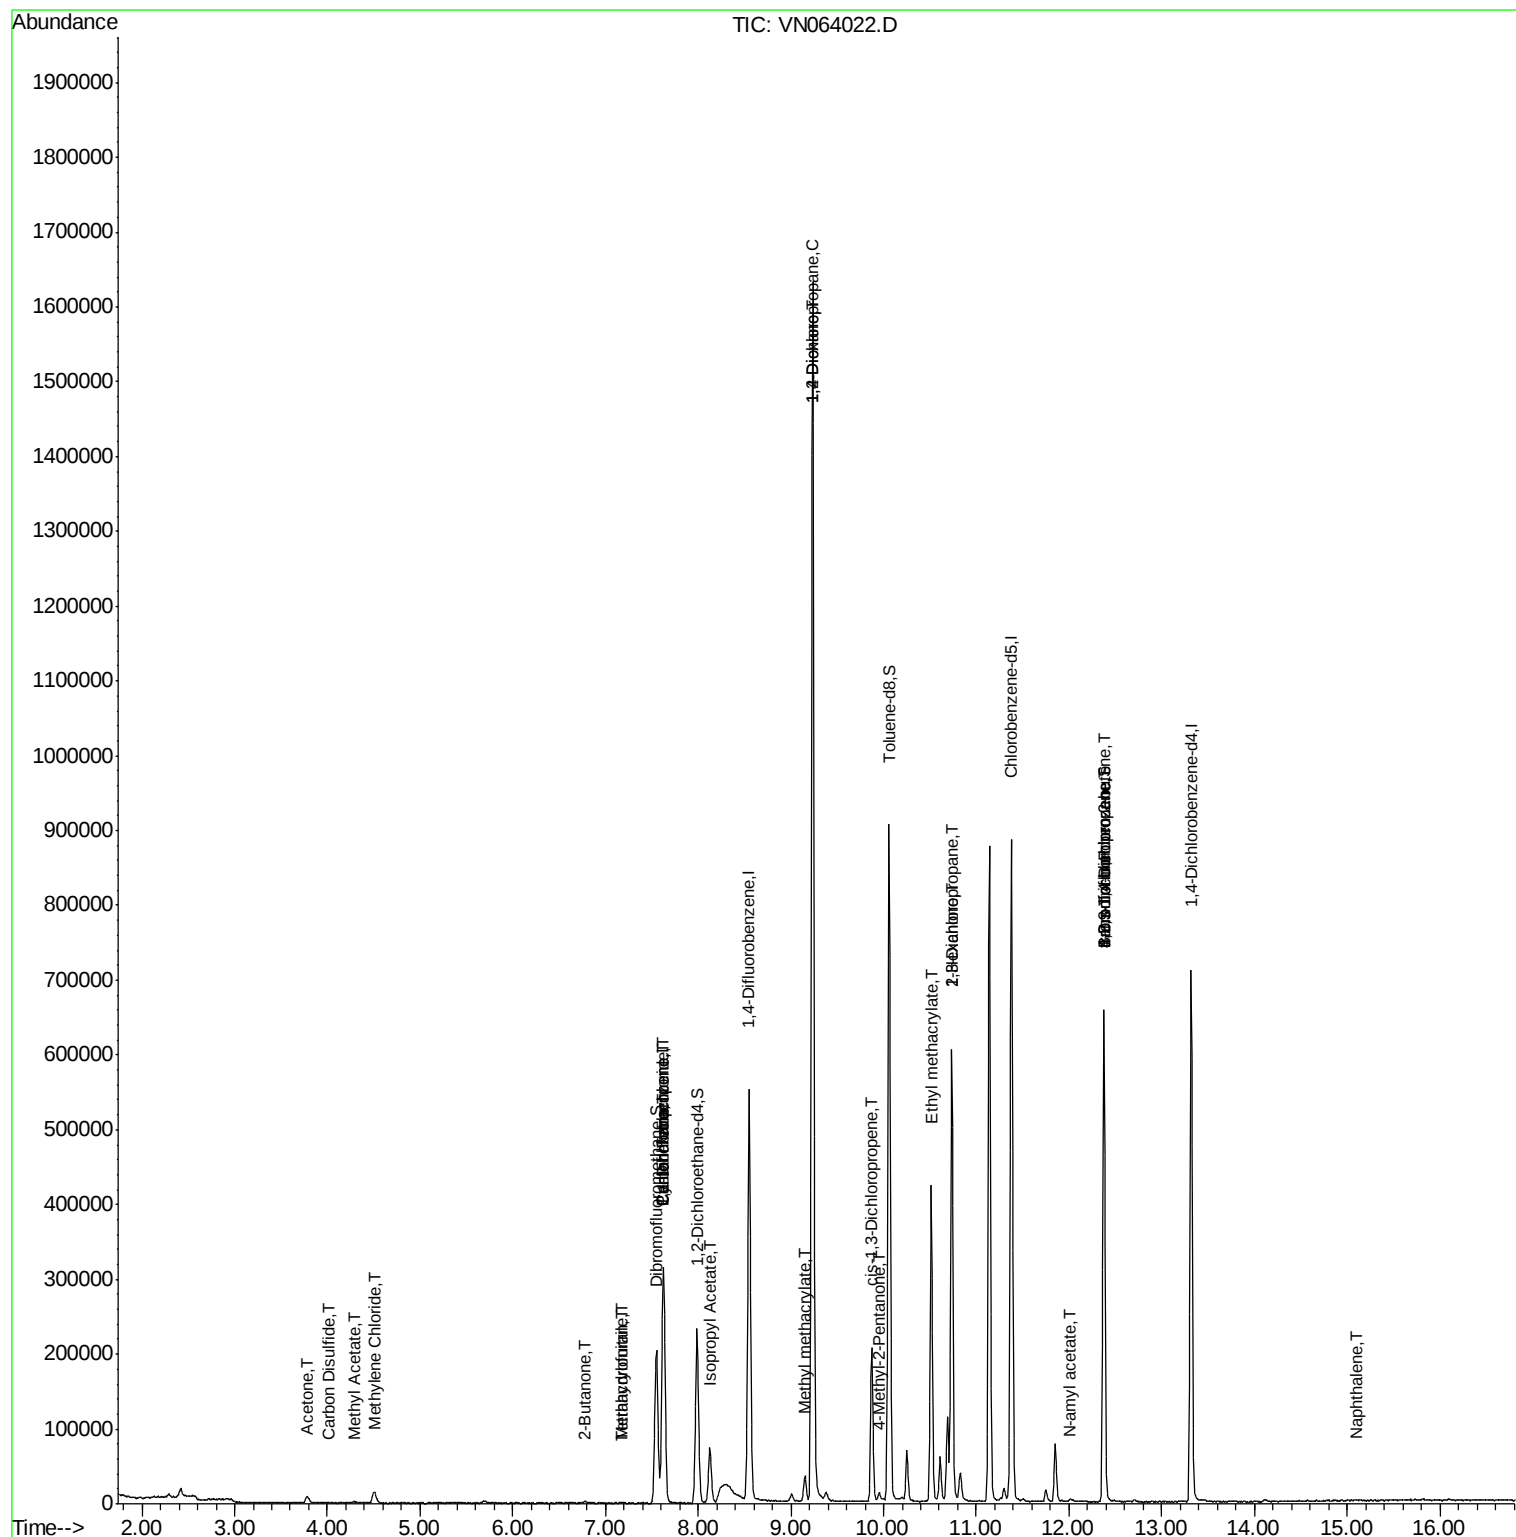

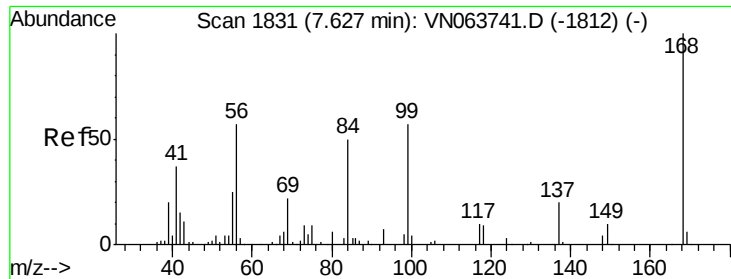

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion:168 Resp: 238768

Ion Ratio Lower Upper

168 100

99 61.9 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): VN063741.D (-1812) (-)

Ion 98.90 (98.60 to 99.60): VN063741.D (-1812) (-)

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#16

Acetone

Concen: 12.506 ug/l

RT: 3.79 min Scan# 636

Delta R.T. 0.01 min

Lab File: VN064022.D


Acq: 9 Oct 2020 5:40

Tgt Ion: 43 Resp: 15186

Ion Ratio Lower Upper

43 100

58 27.6 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-599) (-)

Ion 58.00 (57.70 to 58.70): VN063741.D (-599) (-)

3.79

6000

5000

4000


3000


2000

1000

0

Time--> 3.70 3.75 3.80 3.85



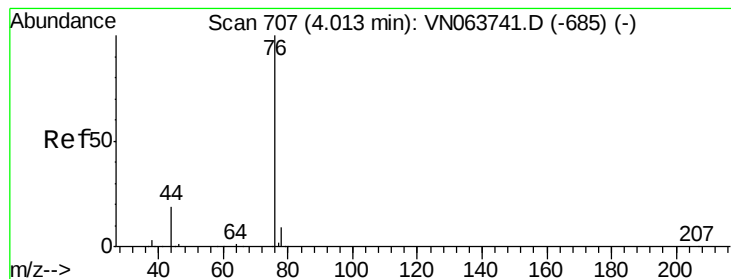

#17

Carbon Disulfide

Concen: 0.781 ug/l

RT: 4.02 min Scan# 708

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N





ClientSampled :

Tot Ion: 76 Resp: 533

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.4#

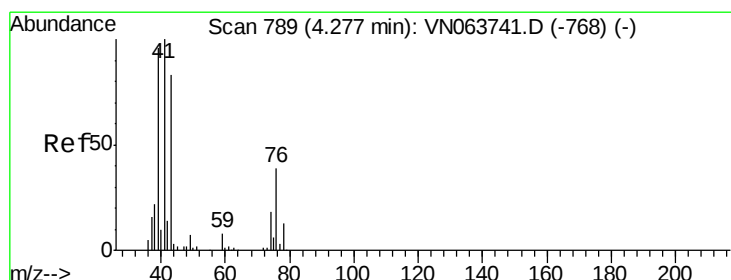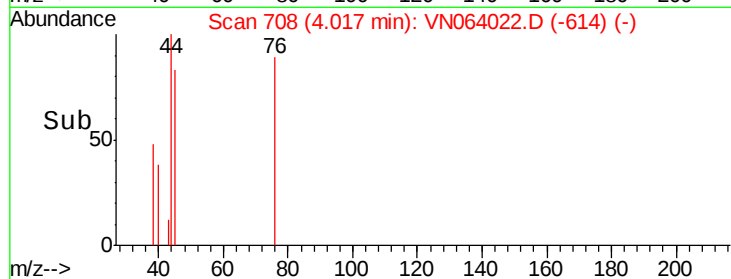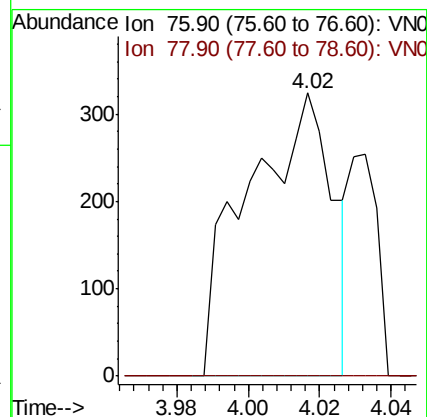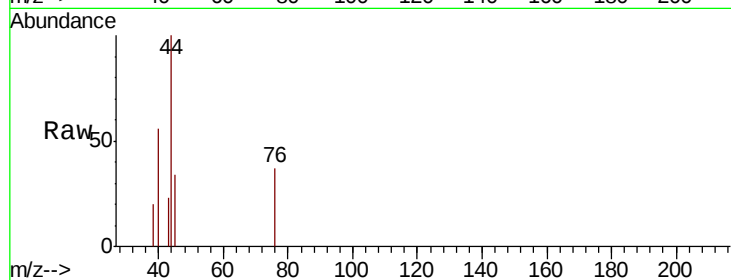

#18

Methyl Acetate

Concen: 1.349 ug/l

RT: 4.29 min Scan# 794

Delta R.T. 0.02 min

Lab File: VN064022.D




Acq: 9 Oct 2020 5:40


Tgt Ion: 43 Resp: 4252

Ion Ratio Lower Upper

43 100

74 5.7 17.4 26.2#


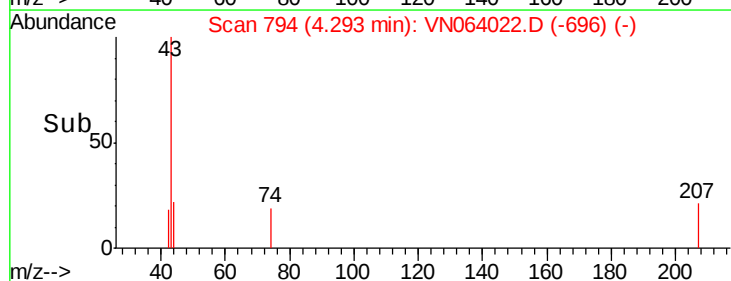
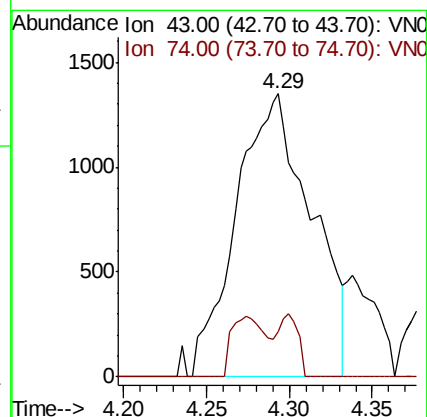
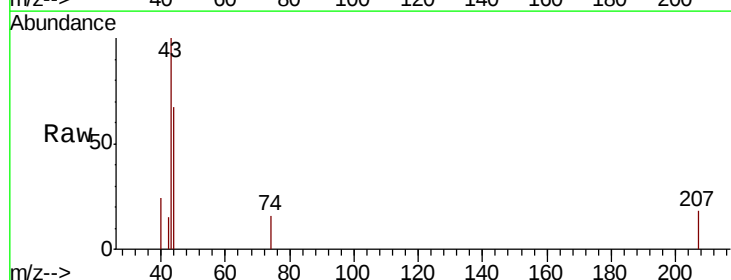


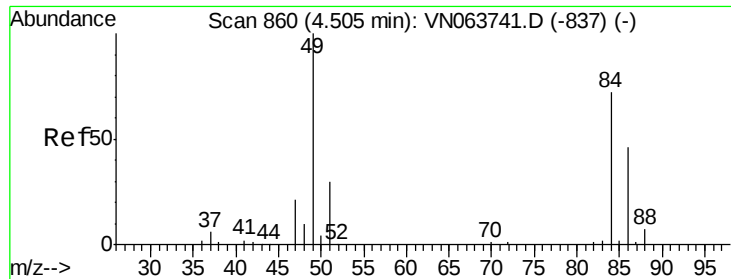

#20
Methvlene Chloride
Concen: 3.820 ug/l
RT: 4.51 min Scan# 861
Delta R.T. 0.00 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 84 Resp: 10371
Ion Ratio Lower Upper
84 100
49 124.2 110.4 165.6
51 39.9 33.3 49.9
86 58.3 50.7 76.1

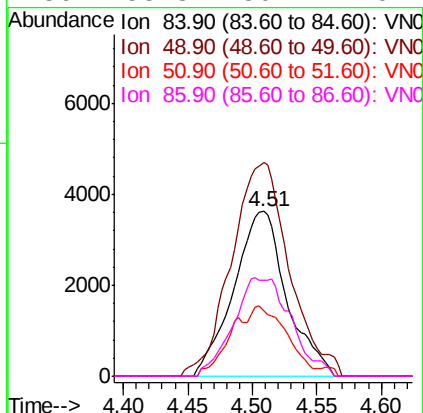

#25
2-Butanone
Concen: 0.440 ug/l
RT: 6.79 min Scan# 1570
Delta R.T. 0.01 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Tgt Ion: 43 Resp: 758
Ion Ratio Lower Upper
43 100
72 0.0 19.3 28.9#

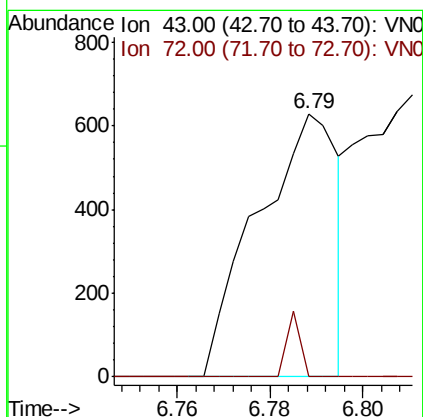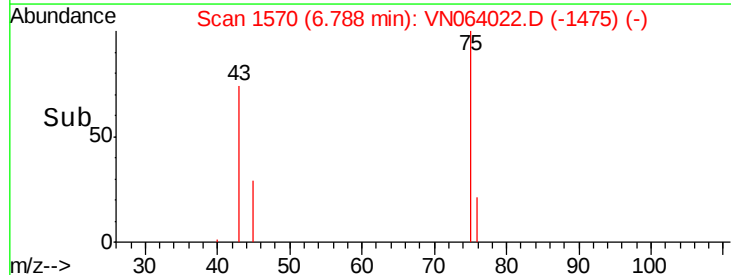



#29

Tetrahydrofuran

Concen: 0.398 ug/l

RT: 7.17 min Scan# 1688

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 42 Resp: 460

Ion Ratio Lower Upper

42 100

72 0.0 32.8 49.2#

71 0.0 30.6 45.8#



Abundance Ion 42.00 (41.70 to 42.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

Ion 71.00 (70.70 to 71.70): VN0

800

600



400

200

0

7.15 7.16 7.17 7.18 7.19

Time-->



#31

Cyclohexane

Concen: 1.486 ug/l

RT: 7.63 min Scan# 1833

Delta R.T. 0.02 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40


Tgt Ion: 56 Resp: 6803

Ion Ratio Lower Upper

56 100

69 156.8 25.4 38.2#

84 86.5 63.3 94.9



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

6000

5000

4000

3000


2000


1000

0

7.55 7.60 7.65 7.70

Time-->







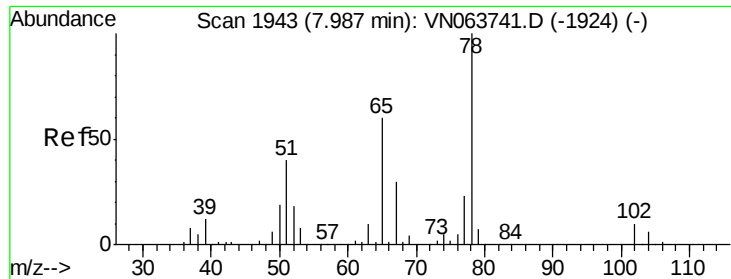

#33
 1,2-Dichloroethane-d4
 Concen: 51.764 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion: 65 Resp: 204190
 Ion Ratio Lower Upper
 65 100
 67 51.3 0.0 99.6

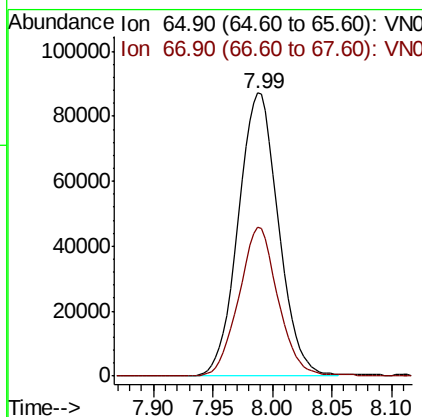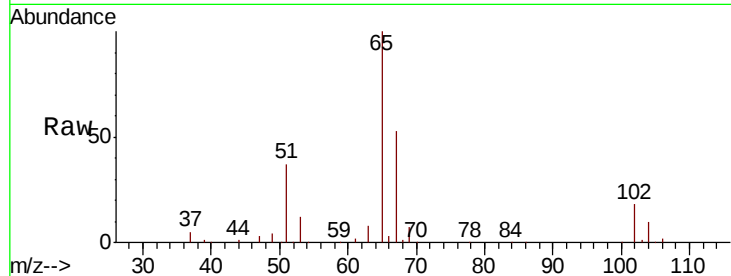

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40

Tgt Ion: 114 Resp: 461948
 Ion Ratio Lower Upper
 114 100
 63 22.7 0.0 45.0
 88 16.5 0.0 34.0

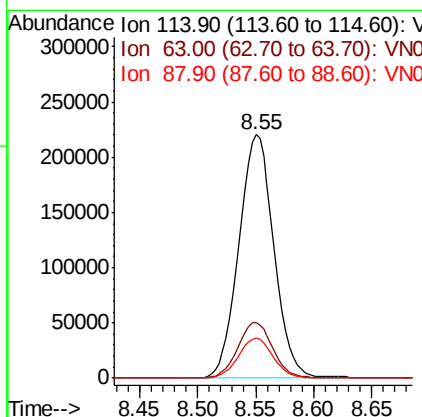







#35
 Dibromofluoromethane
 Concen: 47.870 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40

Instrument :
 MSVOA_N
 ClientSampleId :

Tot Ion:113 Resp: 153440
 Ion Ratio Lower Upper
 113 100
 111 103.3 81.8 122.8
 192 18.3 14.2 21.2

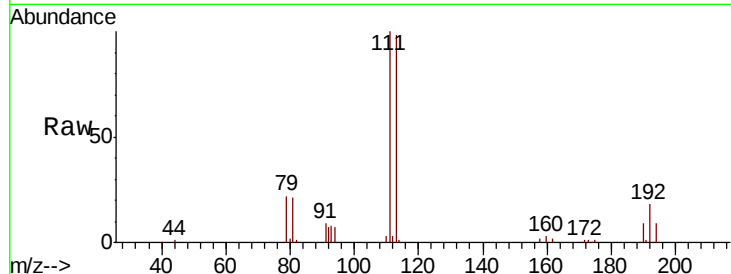


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V


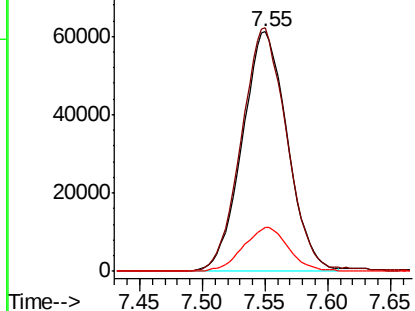



#36
 1,1-Dichloropropene
 Concen: 4.556 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.13 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40

Tgt Ion: 75 Resp: 21321
 Ion Ratio Lower Upper
 75 100
 110 8.8 16.9 50.6#
 77 0.0 24.5 36.7#

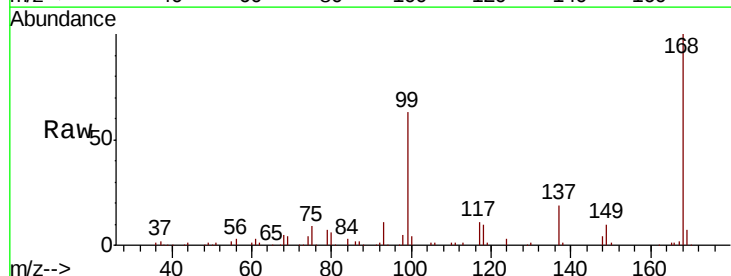

Abundance Ion 74.90 (74.60 to 75.60): V
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): V

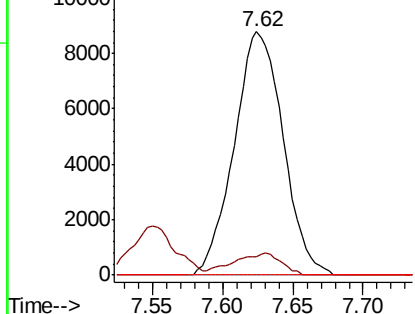



#38

Carbon Tetrachloride

Concen: 4.917 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. -0.11 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampled :


Tot Ion:117 Resp: 25806

Ion Ratio Lower Upper

117 100

119 7.0 80.1 120.1#




121 0.0 25.7 38.5#

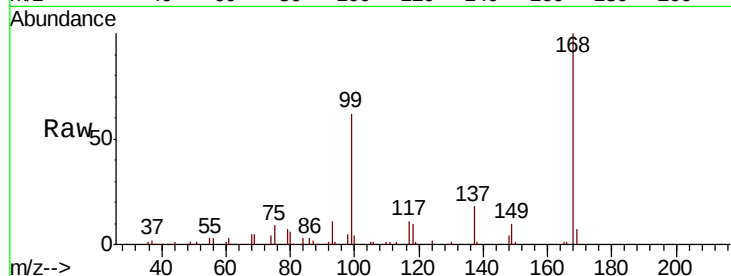

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

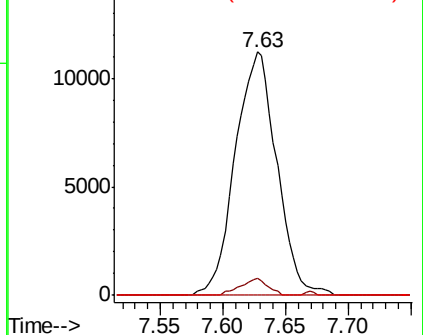

#41

Methacrylonitrile

Concen: 0.220 ug/l

RT: 7.18 min Scan# 1693

Delta R.T. 0.05 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Tgt Ion: 41 Resp: 454


Ion Ratio Lower Upper

41 100

39 39.4 42.5 63.7#

67 0.0 57.4 86.2#

52 0.0 26.9 40.3#






Abundance Ion 41.00 (40.70 to 41.70): V

Ion 39.00 (38.70 to 39.70): V

Ion 67.00 (66.70 to 67.70): V

Ion 52.00 (51.70 to 52.70): V

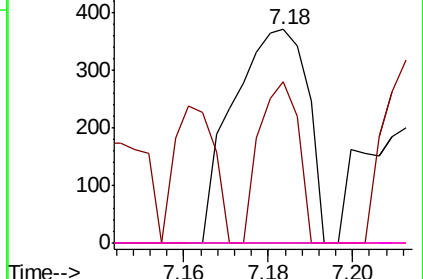



#43

Isopropyl Acetate

Concen: 11.783 ug/l

RT: 8.13 min Scan# 1986

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampled :


Tot Ion: 43 Resp: 90371

Ion Ratio Lower Upper

43 100

61 17.4 14.2 21.4




87 10.8 9.0 13.6

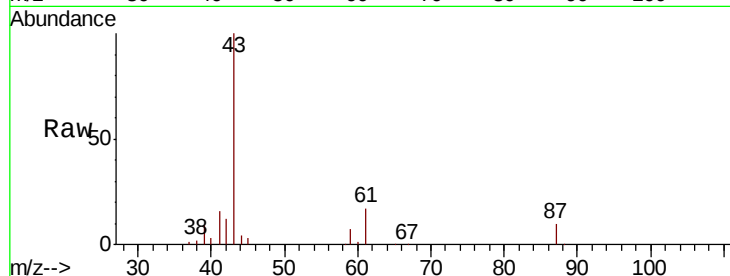

Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-1969) (-)

Ion 61.00 (60.70 to 61.70): VN063741.D (-1969) (-)

Ion 87.00 (86.70 to 87.70): VN063741.D (-1969) (-)

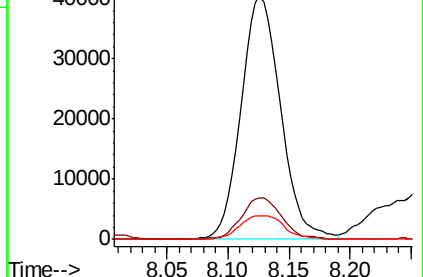

#45

1,2-Dichloropropane

Concen: 0.451 ug/l

RT: 9.23 min Scan# 2329

Delta R.T. 0.14 min

Lab File: VN064022.D


Acq: 9 Oct 2020 5:40

Tgt Ion: 63 Resp: 1628

Ion Ratio Lower Upper



63 100


65 0.0 24.7 37.1#



Abundance Ion 62.90 (62.60 to 63.60): VN063741.D (-2262) (-)

Ion 64.90 (64.60 to 65.60): VN063741.D (-2262) (-)

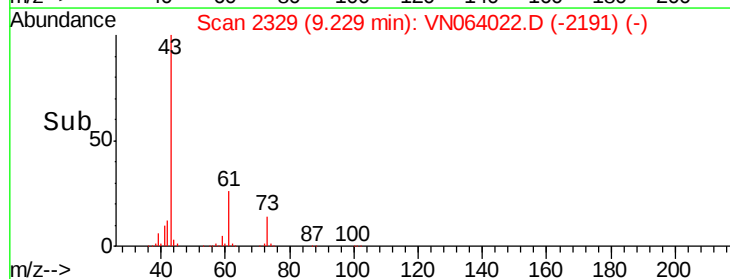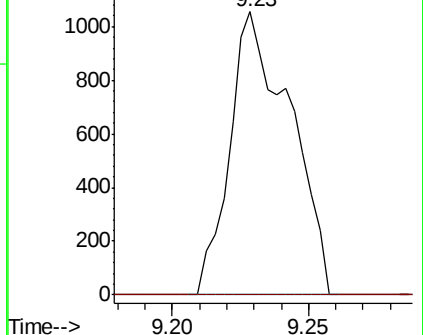


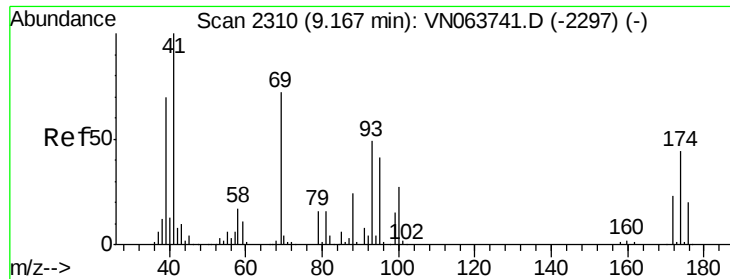




#48
Methyl methacrylate
Concen: 1.456 ug/l
RT: 9.15 min Scan# 2303
Delta R.T. -0.02 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Instrument :
MSVOA_N
ClientSampleId :

Tot Ion: 41 Resp: 5518
Ion Ratio Lower Upper
41 100
69 0.0 60.9 91.3#
39 0.0 57.5 86.3#




Abundance Ion 41.00 (40.70 to 41.70): VNO
Ion 69.00 (68.70 to 69.70): VNO
Ion 39.00 (38.70 to 39.70): VNO


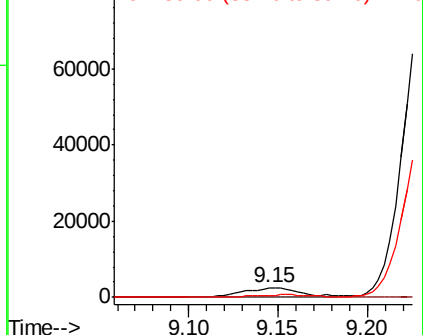



#49
1,4-Dioxane
Concen: 2.990 ug/l
RT: 9.23 min Scan# 2330
Delta R.T. 0.07 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Tgt Ion: 88 Resp: 161
Ion Ratio Lower Upper
88 100
43 1018220.5 33.1 49.7#
58 4874.5 58.9 88.3#



Abundance Ion 88.00 (87.70 to 88.70): VNO
Ion 43.00 (42.70 to 43.70): VNO
Ion 58.00 (57.70 to 58.70): VNO

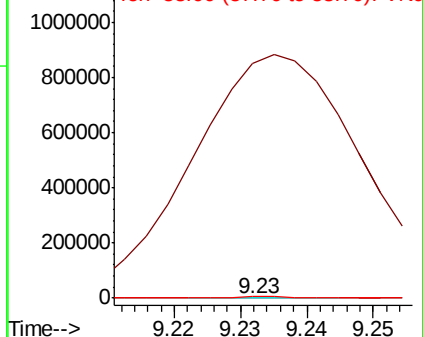

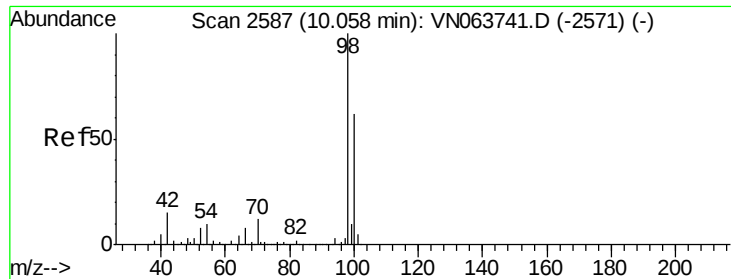

#50

Toluene-d8

Concen: 48.957 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N





ClientSampled :

Tot Ion: 98 Resp: 594877

Ion Ratio Lower Upper

98 100

100 63.4 49.8 74.6

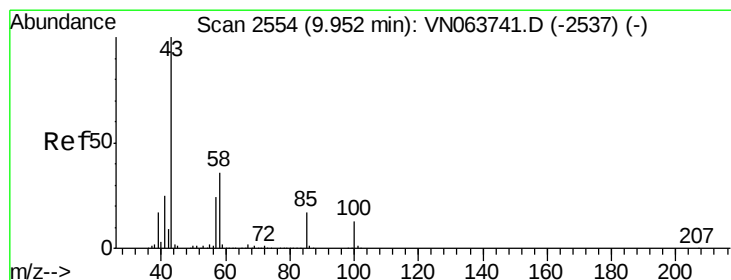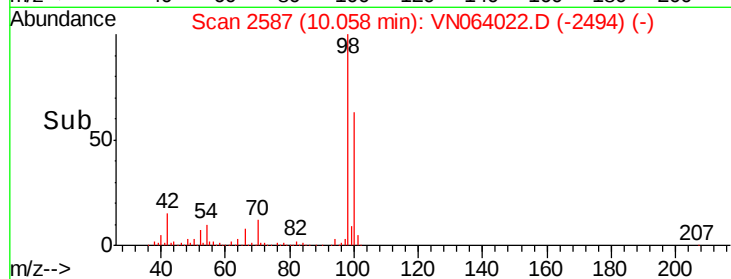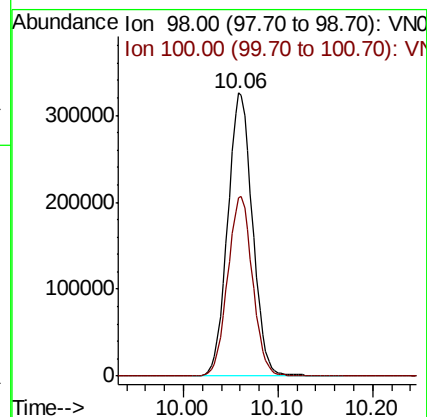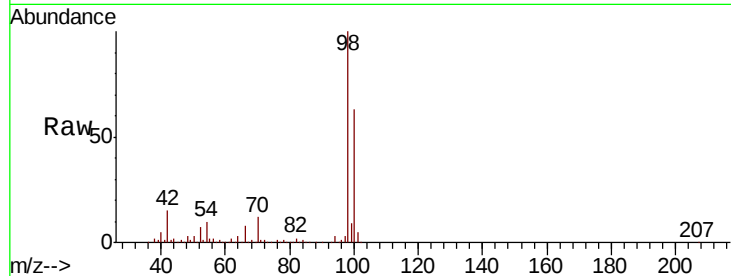

#51

4-Methyl-2-Pentanone

Concen: 2.096 ug/l

RT: 9.95 min Scan# 2554

Delta R.T. 0.00 min

Lab File: VN064022.D




Acq: 9 Oct 2020 5:40


Tgt Ion: 43 Resp: 9432

Ion Ratio Lower Upper

43 100

58 30.4 28.4 42.6

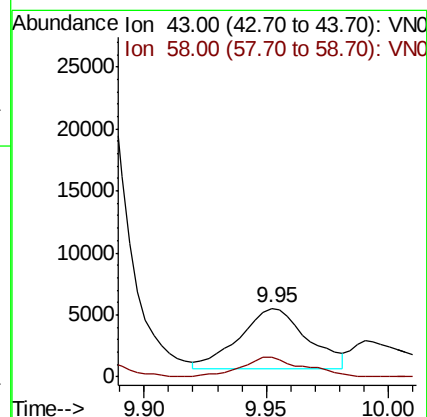




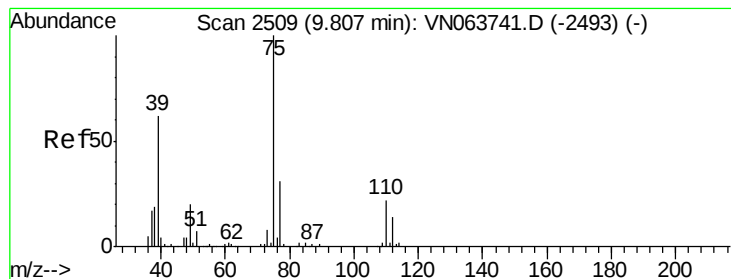


#54

cis-1,3-Dichloropropene
 Concen: 5.767 ug/l
 RT: 9.87 min Scan# 2530
 Delta R.T. 0.07 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40

Instrument :
 MSVOA_N
 ClientSampled :




Tot Ion	Ratio	Lower	Upper
75	100		
77	0.0	24.6	36.8#
39	44.3	49.7	74.5#

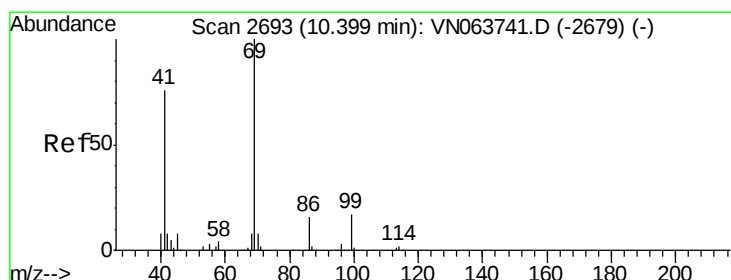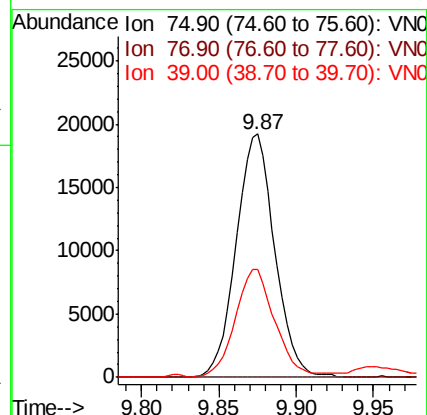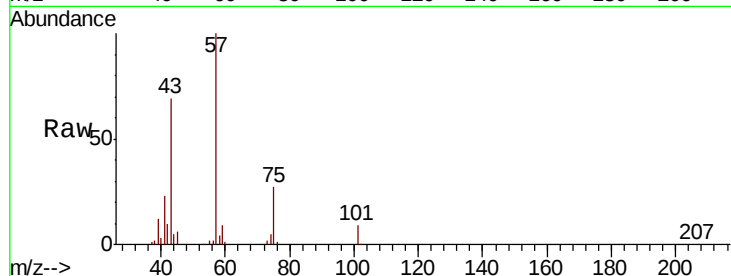


#56

Ethyl methacrylate
 Concen: 0.508 ug/l
 RT: 10.51 min Scan# 2729
 Delta R.T. 0.12 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40

Tgt Ion	Ratio	Lower	Upper
69	100		
41	3677.0	61.1	91.7#
39	1653.8	42.2	63.4#



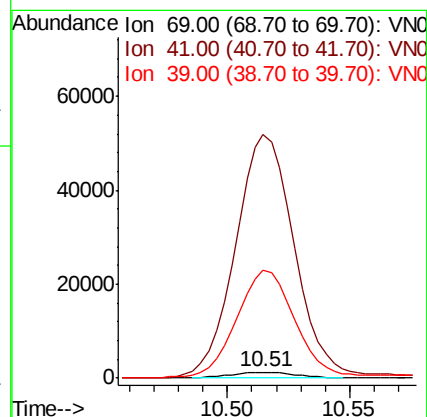



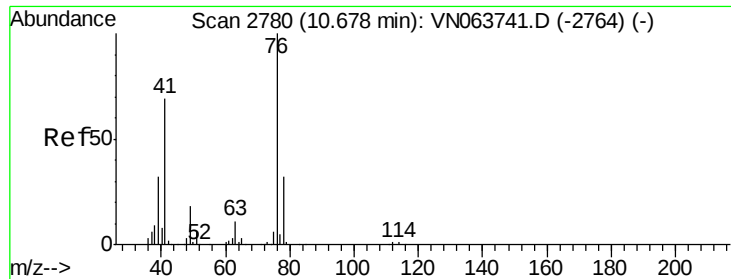

#57
 1,3-Dichloropropane
 Concen: 1.050 ug/l
 RT: 10.74 min Scan# 2798
 Delta R.T. 0.06 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion: 76 Resp: 5892
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.2 37.8#

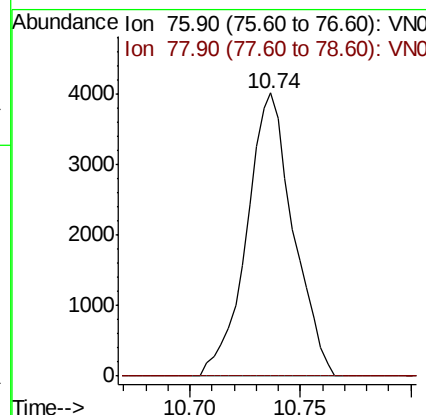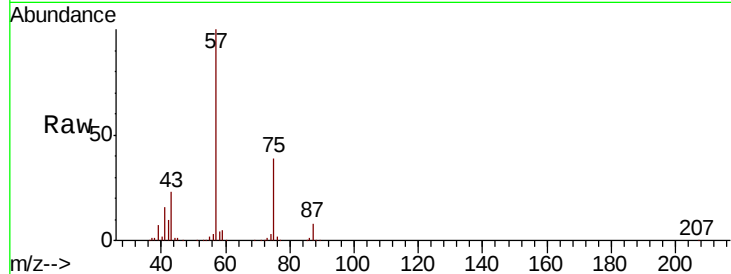

#59
 2-Hexanone
 Concen: 28.048 ug/l
 RT: 10.74 min Scan# 2798
 Delta R.T. 0.02 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40

Tgt Ion: 43 Resp: 93776
 Ion Ratio Lower Upper
 43 100
 58 18.5 24.6 73.8#

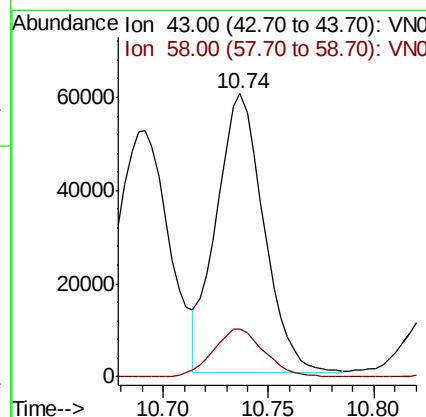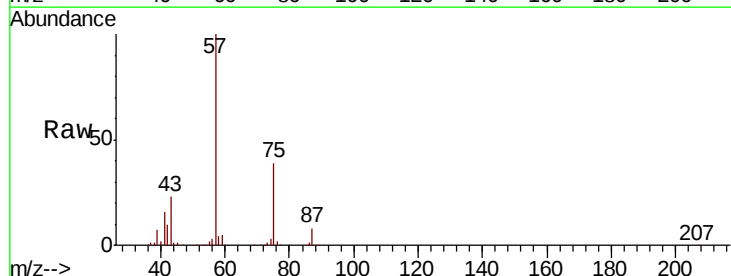



#62

4-Bromofluorobenzene

Concen: 48.431 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 95 Resp: 221221

Ion Ratio Lower Upper

95 100

174 76.8 0.0 150.6




176 74.4 0.0 145.4



Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): VN0

Ion 175.80 (175.50 to 176.50): VN0

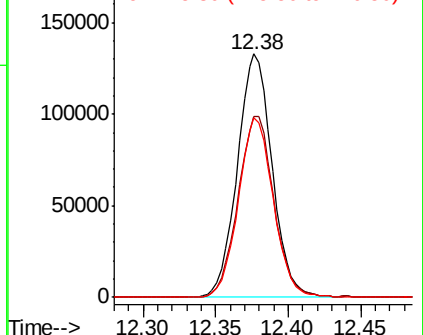

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2998

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40


Tgt Ion: 117 Resp: 478567

Ion Ratio Lower Upper

117 100

82 58.1 47.4 71.2



119 32.7 26.4 39.6




Abundance Ion 116.90 (116.60 to 117.60): VN0

Ion 82.00 (81.70 to 82.70): VN0

Ion 118.90 (118.60 to 119.60): VN0

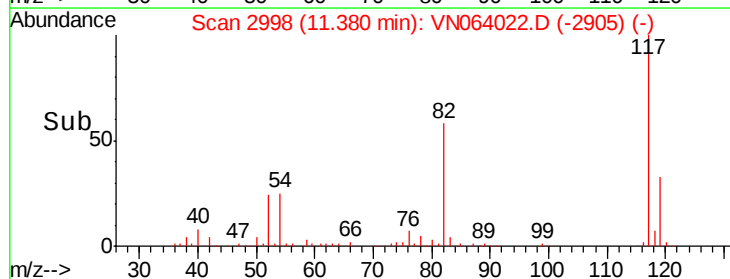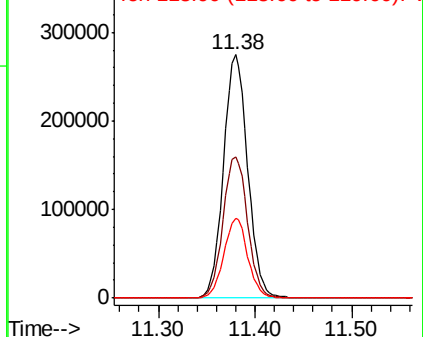



#71

Bromoform

Concen: 0.348 ug/l

RT: 12.37 min Scan# 3306

Delta R.T. 0.27 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampled :


Tot Ion:173 Resp: 1002

Ion Ratio Lower Upper

173 100

175 1087.5 23.5 70.5#




254 0.0 0.0 0.0

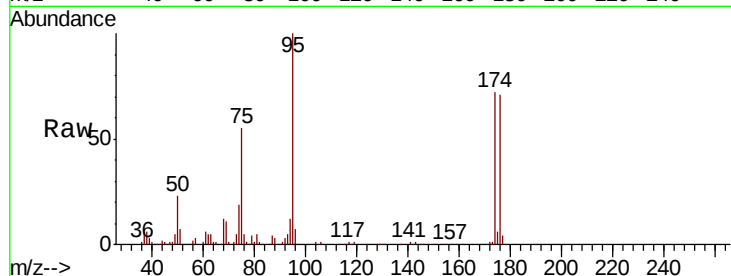

Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

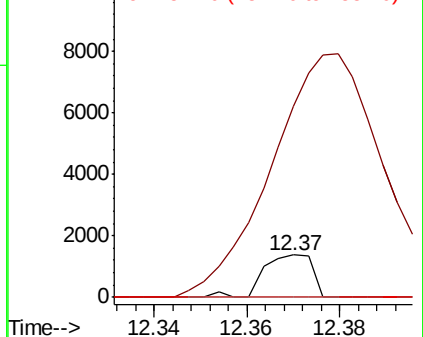

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40


Tgt Ion:152 Resp: 182808

Ion Ratio Lower Upper

152 100

115 62.3 31.3 93.8



150 156.2 0.0 341.8




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

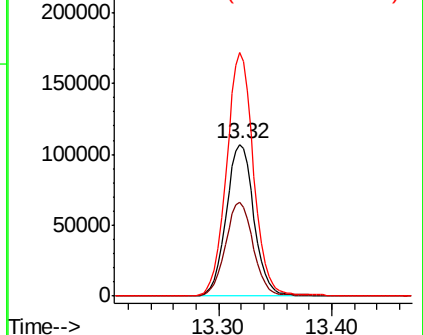

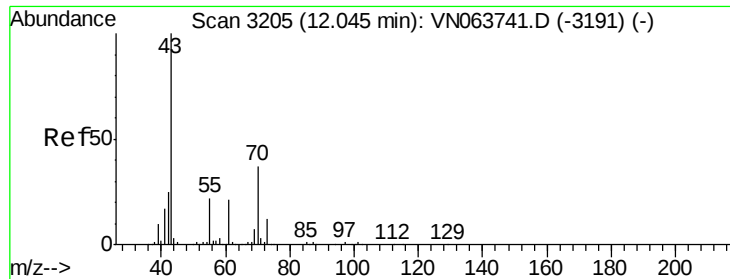

#74

N-amvl acetate

Concen: 2.696 ug/l

RT: 12.01 min Scan# 3193

Delta R.T. -0.04 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :

Tot Ion: 43 Resp: 3116


Ion Ratio Lower Upper

43 100

70 0.0 29.8 44.8#

55 3.4 17.9 26.9#

61 0.0 17.0 25.4#






Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

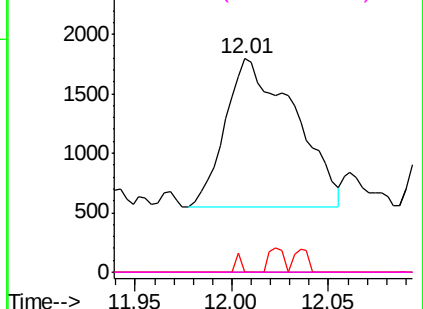

#76

1,2,3-Trichloropropane

Concen: 29.783 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064022.D


Acq: 9 Oct 2020 5:40

Tgt Ion: 75 Resp: 120018

Ion Ratio Lower Upper



75 100


77 1.2 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

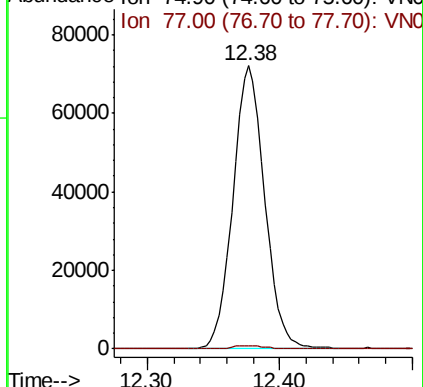







#81
trans-1,4-Dichloro-2-butene
Concen: 85.778 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.10 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Instrument :
MSVOA_N
ClientSampled :

Tot Ion: 75 Resp: 120018
Ion Ratio Lower Upper
75 100
53 0.1 88.2 132.2#
89 0.0 36.0 54.0#

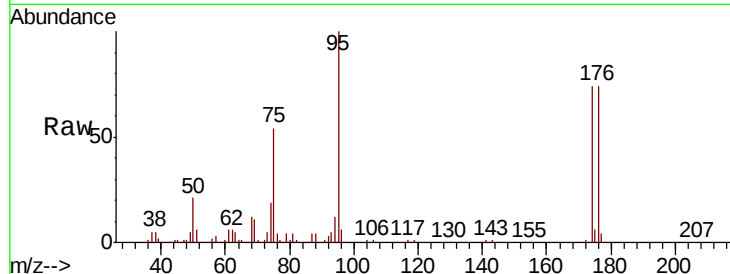


Abundance Ion 74.90 (74.60 to 75.60): VN0
Ion 53.00 (52.70 to 53.70): VN0
Ion 88.90 (88.60 to 89.60): VN0

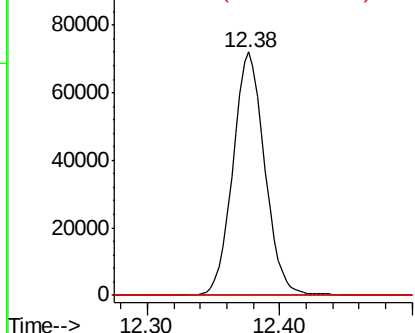

#95
Naphthalene
Concen: 1.932 ug/l
RT: 15.12 min Scan# 4160
Delta R.T. 0.01 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Tgt Ion: 128 Resp: 73
Ion Ratio Lower Upper
128 100
127 0.0 10.5 15.7#
129 0.0 8.7 13.1#

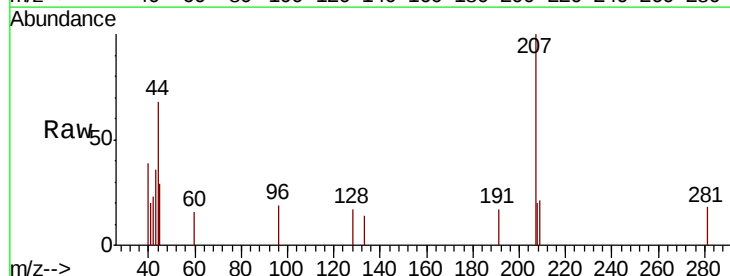

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

