

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN100820\
 Data File : VN064022.D
 Acq On : 9 Oct 2020 5:40
 Operator : JC/MD
 Sample : L4291-10
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B4-100620-DP

Quant Time: Oct 09 12:06:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	238768	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	461948	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	478567	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	182808	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	204190	51.76	ug/l	0.00
Spiked Amount			Recovery	=	103.52%	
35) Dibromofluoromethane	7.55	113	153440	47.87	ug/l	0.00
Spiked Amount			Recovery	=	95.74%	
50) Toluene-d8	10.06	98	594877	48.96	ug/l	0.00
Spiked Amount			Recovery	=	97.92%	
62) 4-Bromofluorobenzene	12.38	95	221221	48.43	ug/l	0.00
Spiked Amount			Recovery	=	96.86%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.79	43	15186	12.506	ug/l	99
17) Carbon Disulfide	4.02	76	533	0.781	ug/l #	76
18) Methyl Acetate	4.29	43	4252	1.349	ug/l #	66
20) Methylene Chloride	4.51	84	10371	3.820	ug/l	91
25) 2-Butanone	6.79	43	758	0.440	ug/l #	51
29) Tetrahydrofuran	7.17	42	460	0.398	ug/l #	36
31) Cyclohexane	7.63	56	6803	1.486	ug/l #	30
36) 1,1-Dichloropropene	7.62	75	21321	4.556	ug/l #	51
38) Carbon Tetrachloride	7.63	117	25806	4.917	ug/l #	16
41) Methacrylonitrile	7.18	41	454	0.220	ug/l #	42
43) Isopropyl Acetate	8.13	43	90371	11.783	ug/l	99
45) 1,2-Dichloropropane	9.23	63	1628	0.451	ug/l #	44
48) Methyl methacrylate	9.15	41	5518	1.456	ug/l #	12
49) 1,4-Dioxane	9.23	88	161	2.990	ug/l #	1
51) 4-Methyl-2-Pentanone	9.95	43	9432	2.096	ug/l	91
54) cis-1,3-Dichloropropene	9.87	75	33184	5.767	ug/l #	66
56) Ethyl methacrylate	10.51	69	2387	0.508	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	5892	1.050	ug/l #	43
59) 2-Hexanone	10.74	43	93776	28.048	ug/l #	55
71) Bromoform	12.37	173	1002	0.348	ug/l #	1
74) N-amyl acetate	12.01	43	3116	2.696	ug/l #	48
76) 1,2,3-Trichloropropane	12.38	75	120018	29.783	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	120018	85.778	ug/l #	6
95) Naphthalene	15.12	128	73	1.932	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN100820\
Data File : VN064022.D
Acq On : 9 Oct 2020 5:40
Operator : JC/MD
Sample : L4291-10
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PAV-B4-100620-DP

Quant Time: Oct 09 12:06:39 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

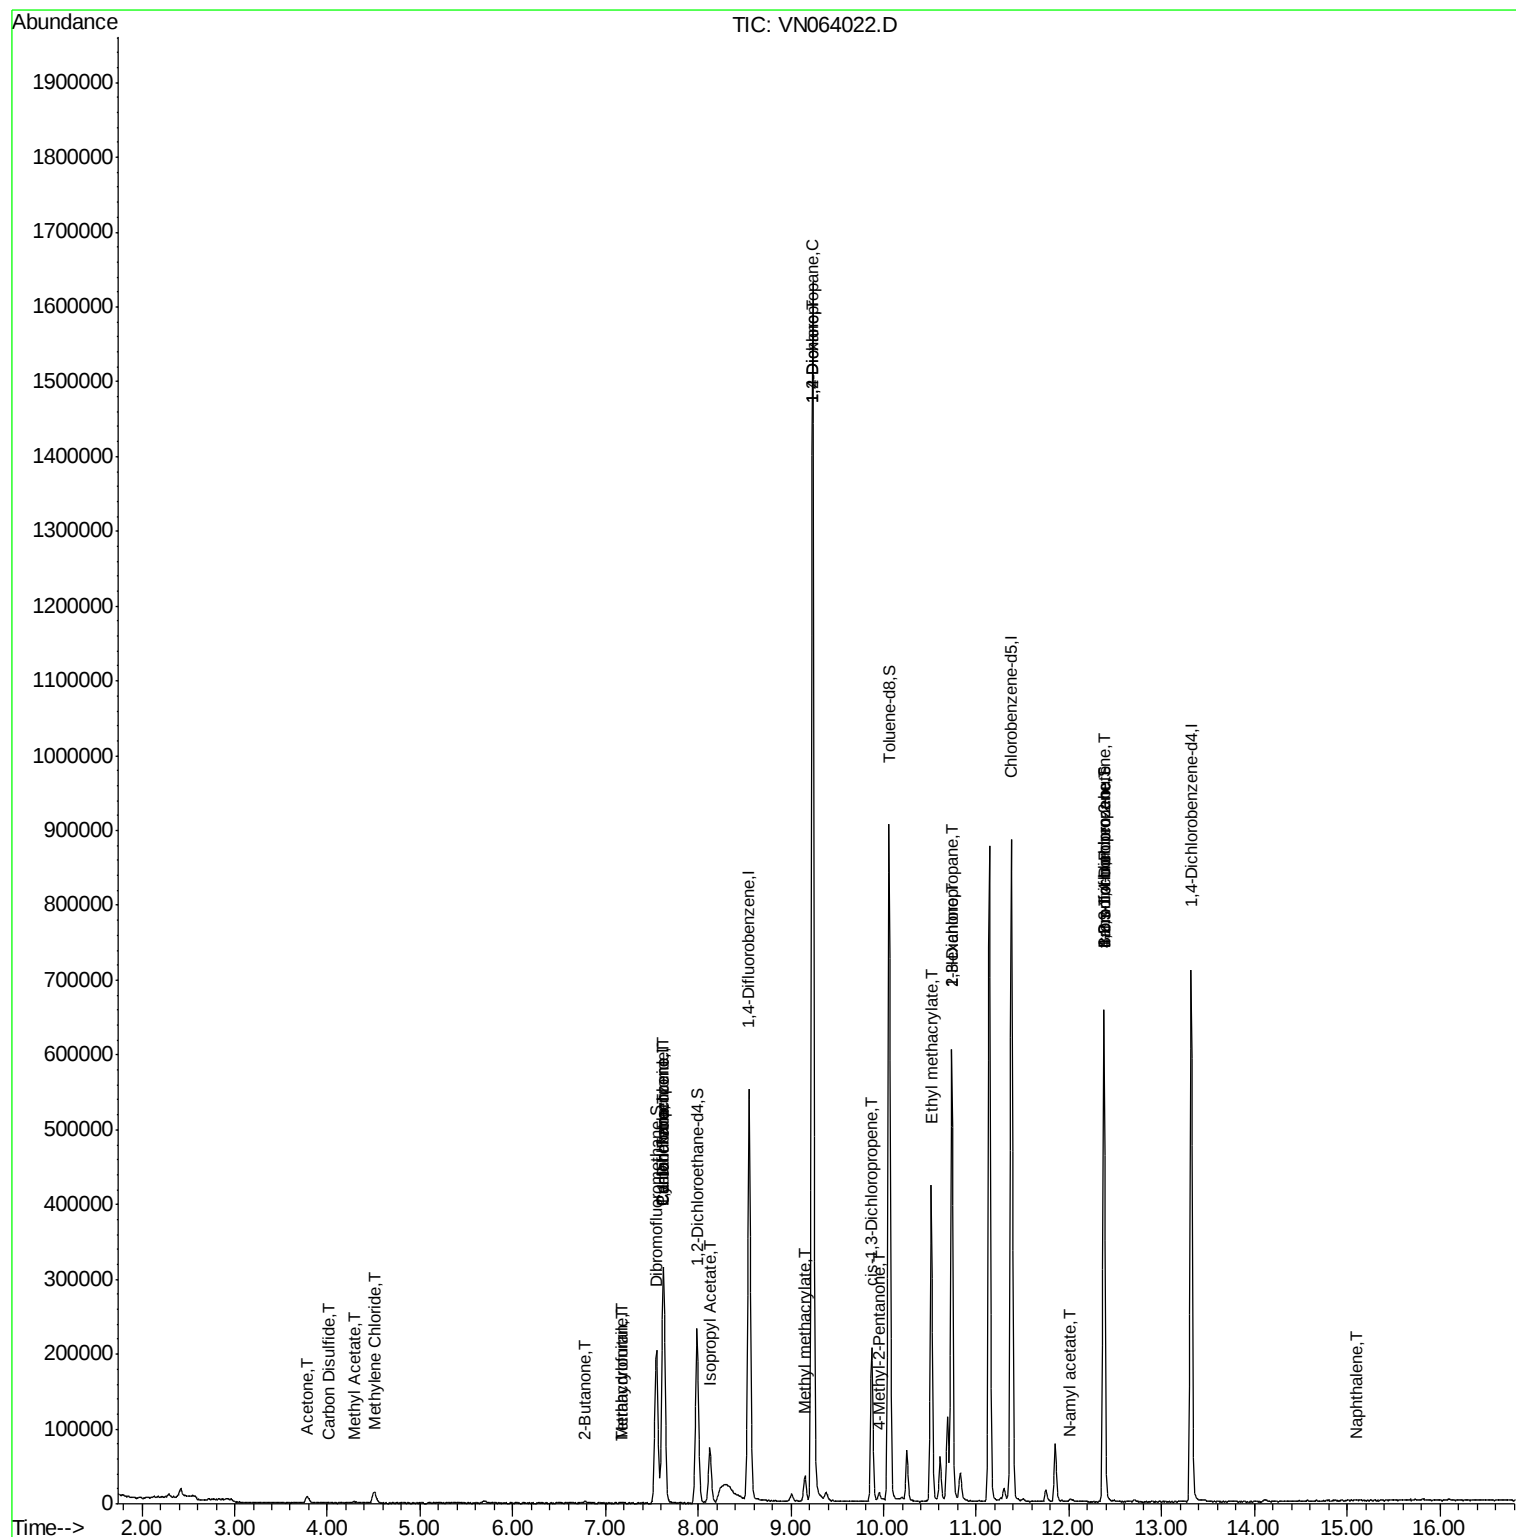



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :


PAV-B4-100620-DP

Tgt Ion:168 Resp: 238768

Ion Ratio Lower Upper




168 100

99 61.9 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

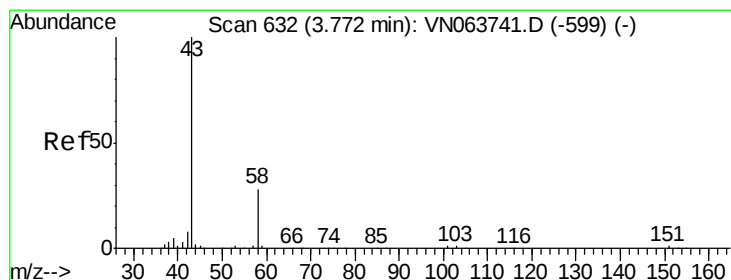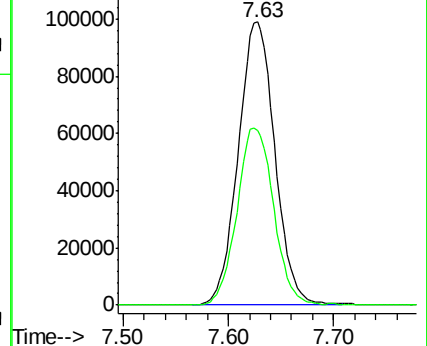

#16

Acetone

Concen: 12.506 ug/l

RT: 3.79 min Scan# 636

Delta R.T. 0.01 min

Lab File: VN064022.D


Acq: 9 Oct 2020 5:40

Tgt Ion: 43 Resp: 15186

Ion Ratio Lower Upper



43 100


58 27.6 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO

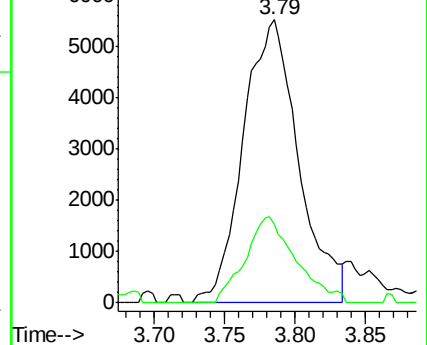



#17

Carbon Disulfide

Concen: 0.781 ug/l

RT: 4.02 min Scan# 708

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :





PAV-B4-100620-DP

Tgt Ion: 76 Resp: 533

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.4#

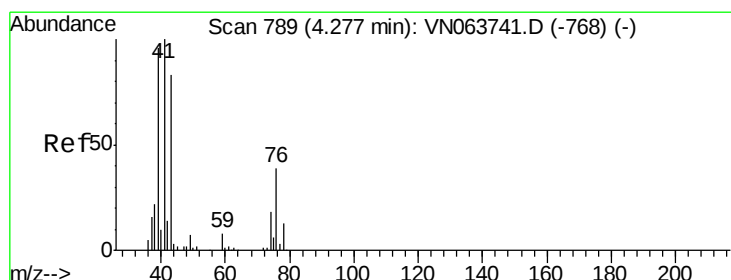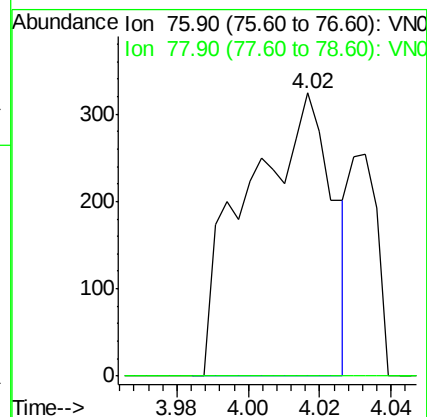

#18

Methyl Acetate

Concen: 1.349 ug/l

RT: 4.29 min Scan# 794

Delta R.T. 0.02 min

Lab File: VN064022.D




Acq: 9 Oct 2020 5:40


Tgt Ion: 43 Resp: 4252

Ion Ratio Lower Upper

43 100

74 5.7 17.4 26.2#

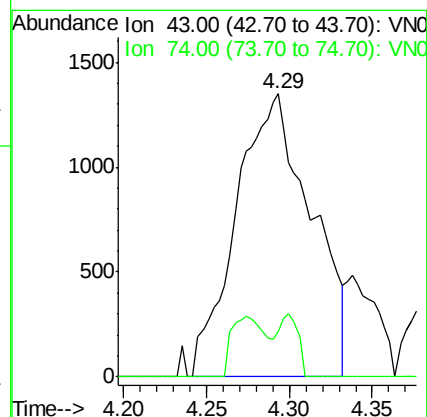







#20
Methylene Chloride
Concen: 3.820 ug/l
RT: 4.51 min Scan# 861
Delta R.T. 0.00 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Instrument :
MSVOA_N
ClientSampleId :
PAV-B4-100620-DP

Tgt Ion: 84 Resp: 10371
Ion Ratio Lower Upper
84 100
49 124.2 110.4 165.6
51 39.9 33.3 49.9
86 58.3 50.7 76.1




Abundance Ion 83.90 (83.60 to 84.60): VN0
Ion 48.90 (48.60 to 49.60): VN0
Ion 50.90 (50.60 to 51.60): VN0
Ion 85.90 (85.60 to 86.60): VN0

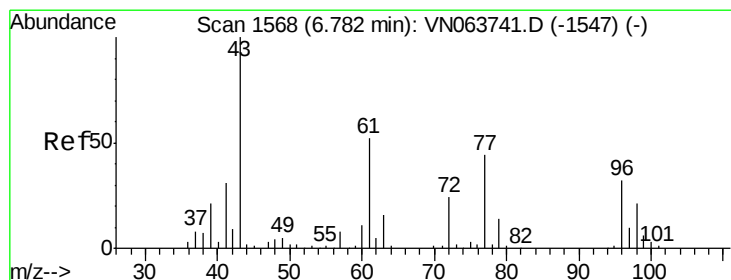
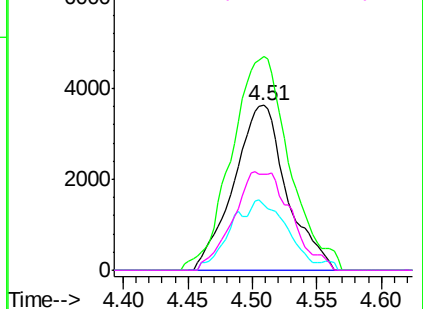



#25
2-Butanone
Concen: 0.440 ug/l
RT: 6.79 min Scan# 1570
Delta R.T. 0.01 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Tgt Ion: 43 Resp: 758
Ion Ratio Lower Upper
43 100
72 0.0 19.3 28.9#



Abundance Ion 43.00 (42.70 to 43.70): VN0
Ion 72.00 (71.70 to 72.70): VN0



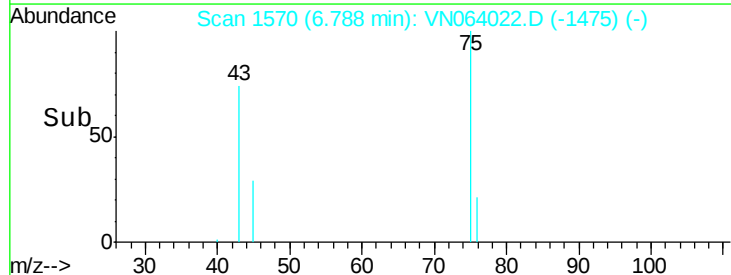
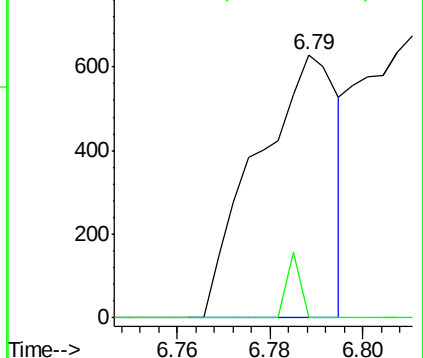




#29
Tetrahydrofuran
Concen: 0.398 ug/l
RT: 7.17 min Scan# 1688
Delta R.T. 0.00 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40




Instrument :
MSVOA_N
ClientSampleId :
PAV-B4-100620-DP


Tgt Ion: 42 Resp: 460
Ion Ratio Lower Upper
42 100
72 0.0 32.8 49.2#
71 0.0 30.6 45.8#

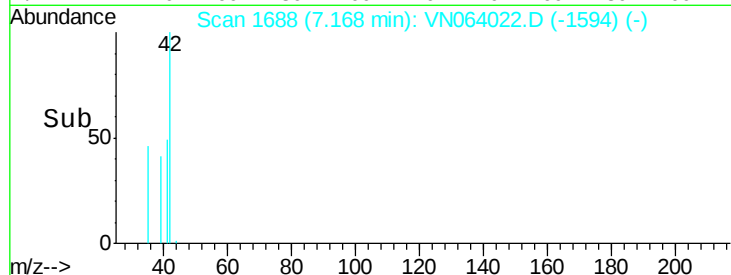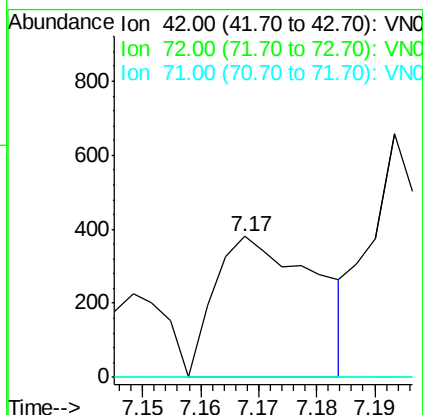

#31
Cyclohexane
Concen: 1.486 ug/l
RT: 7.63 min Scan# 1833
Delta R.T. 0.02 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Tgt Ion: 56 Resp: 6803
Ion Ratio Lower Upper
56 100
69 156.8 25.4 38.2#
84 86.5 63.3 94.9



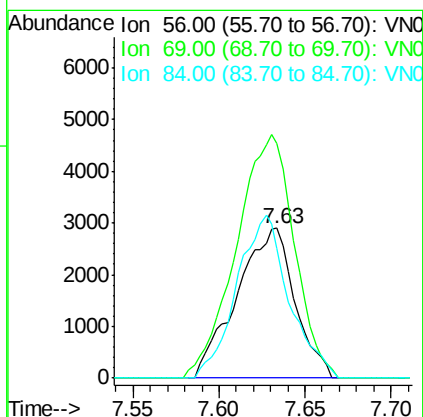



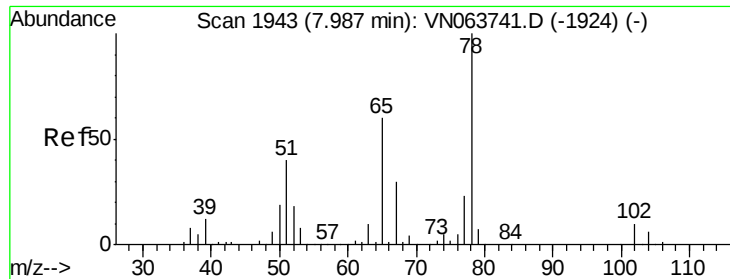

#33
 1,2-Dichloroethane-d4
 Concen: 51.764 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40




Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B4-100620-DP


Tgt Ion: 65 Resp: 204190
 Ion Ratio Lower Upper
 65 100
 67 51.3 0.0 99.6

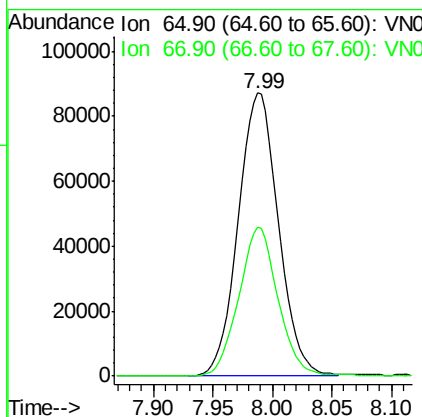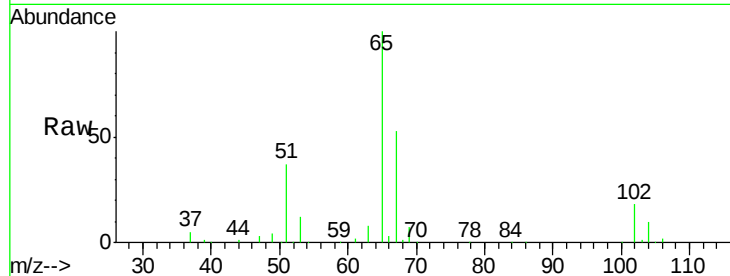

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40

Tgt Ion: 114 Resp: 461948
 Ion Ratio Lower Upper
 114 100
 63 22.7 0.0 45.0
 88 16.5 0.0 34.0



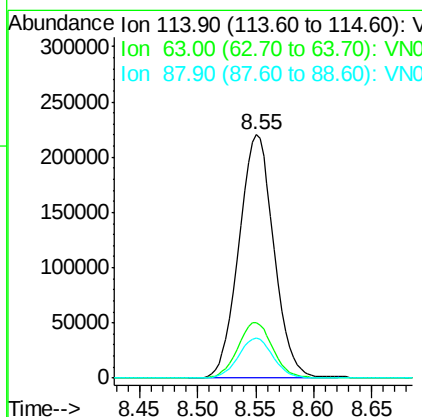





#35
Dibromofluoromethane
Concen: 47.870 ug/l
RT: 7.55 min Scan# 1807
Delta R.T. 0.00 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40




Instrument :
MSVOA_N
ClientSampleId :
PAV-B4-100620-DP


Tgt Ion: 113 Resp: 153440
Ion Ratio Lower Upper
113 100
111 103.3 81.8 122.8
192 18.3 14.2 21.2

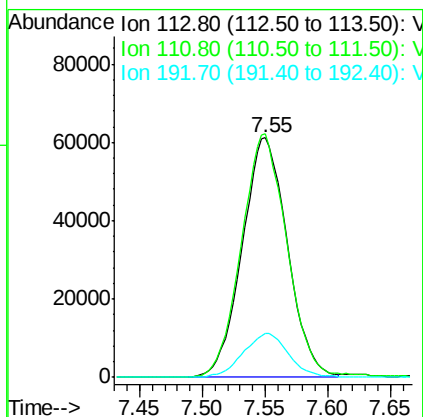

#36
1,1-Dichloropropene
Concen: 4.556 ug/l
RT: 7.62 min Scan# 1830
Delta R.T. -0.13 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Tgt Ion: 75 Resp: 21321
Ion Ratio Lower Upper
75 100
110 8.8 16.9 50.6#
77 0.0 24.5 36.7#

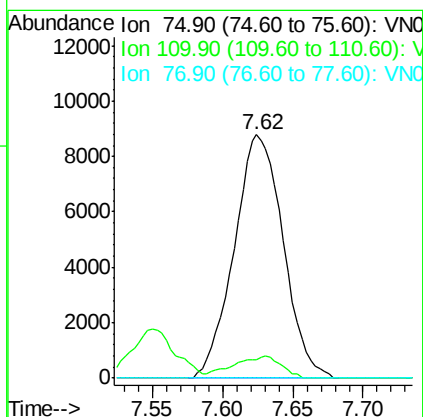



#38

Carbon Tetrachloride

Concen: 4.917 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. -0.11 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :

PAV-B4-100620-DP


Tgt Ion:117 Resp: 25806

Ion Ratio Lower Upper

117 100

119 7.0 80.1 120.1#




121 0.0 25.7 38.5#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

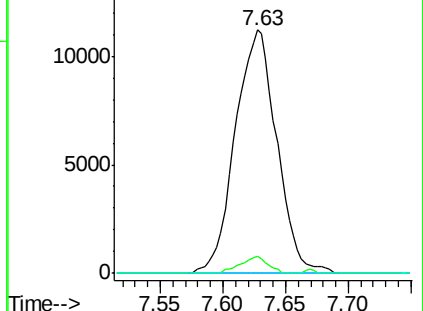

#41

Methacrylonitrile

Concen: 0.220 ug/l

RT: 7.18 min Scan# 1693

Delta R.T. 0.05 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Tgt Ion: 41 Resp: 454


Ion Ratio Lower Upper

41 100

39 39.4 42.5 63.7#

67 0.0 57.4 86.2#

52 0.0 26.9 40.3#






Abundance Ion 41.00 (40.70 to 41.70): VN0

Ion 39.00 (38.70 to 39.70): VN0

Ion 67.00 (66.70 to 67.70): VN0

Ion 52.00 (51.70 to 52.70): VN0



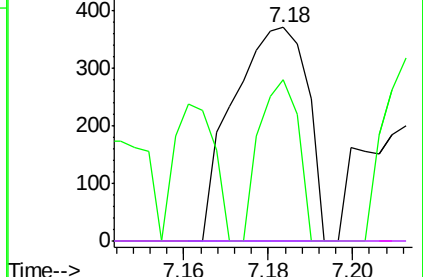





#43
Isopropyl Acetate
Concen: 11.783 ug/l
RT: 8.13 min Scan# 1986
Delta R.T. 0.00 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40




Instrument :
MSVOA_N
ClientSampleId :
PAV-B4-100620-DP


Tgt Ion: 43 Resp: 90371
Ion Ratio Lower Upper
43 100
61 17.4 14.2 21.4
87 10.8 9.0 13.6

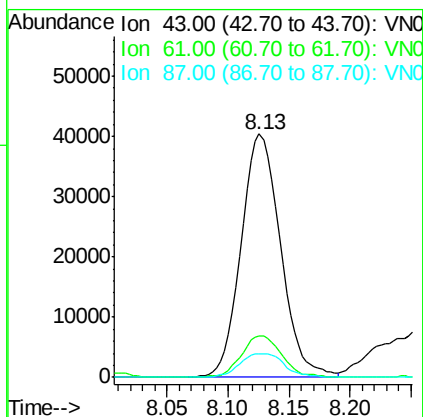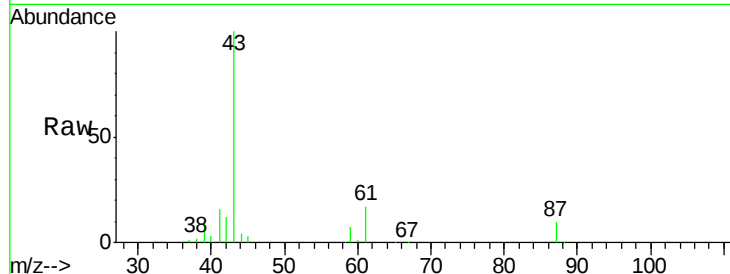

#45
1,2-Dichloropropane
Concen: 0.451 ug/l
RT: 9.23 min Scan# 2329
Delta R.T. 0.14 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Tgt Ion: 63 Resp: 1628
Ion Ratio Lower Upper
63 100
65 0.0 24.7 37.1#



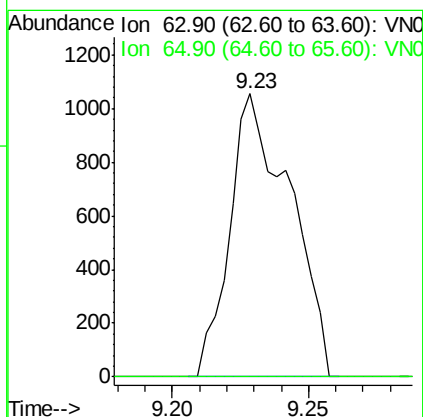
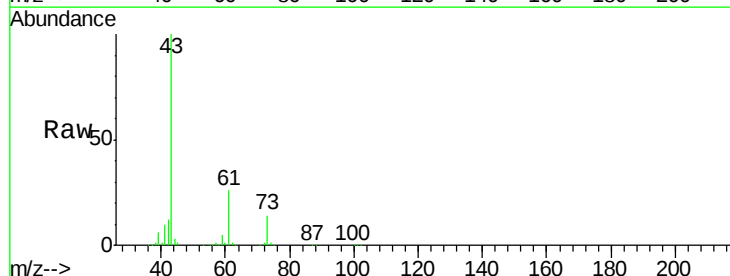


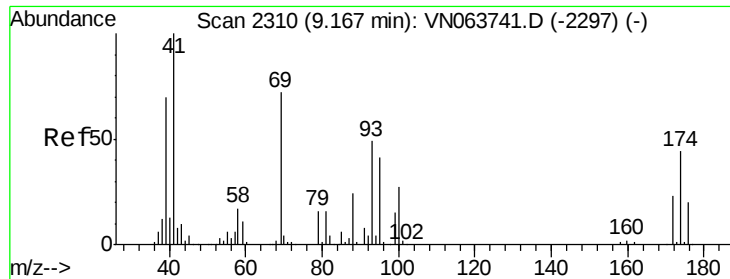

#48
Methyl methacrylate
Concen: 1.456 ug/l
RT: 9.15 min Scan# 2303
Delta R.T. -0.02 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40




Instrument :
MSVOA_N
ClientSampleId :
PAV-B4-100620-DP


Tgt Ion: 41 Resp: 5518
Ion Ratio Lower Upper
41 100
69 0.0 60.9 91.3#
39 0.0 57.5 86.3#

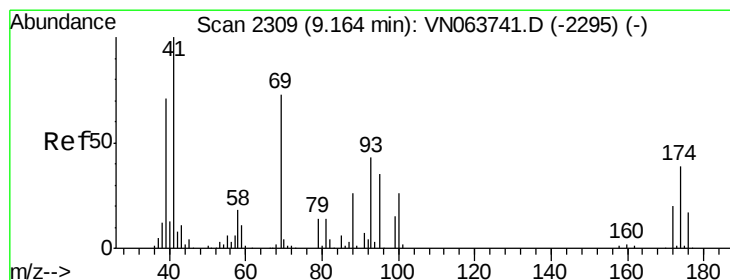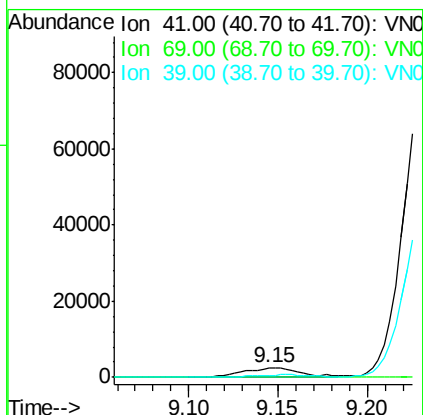

#49
1,4-Dioxane
Concen: 2.990 ug/l
RT: 9.23 min Scan# 2330
Delta R.T. 0.07 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Tgt Ion: 88 Resp: 161
Ion Ratio Lower Upper
88 100
43 1018220.5 33.1 49.7#
58 4874.5 58.9 88.3#

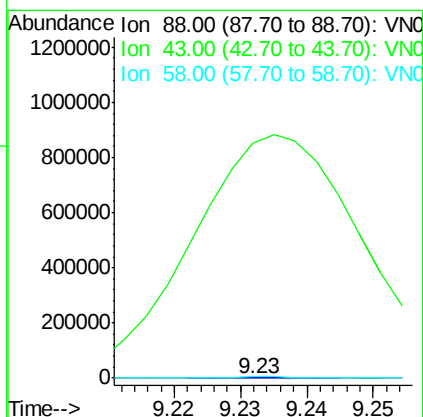



#50

Toluene-d8

Concen: 48.957 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :





PAV-B4-100620-DP

Tgt Ion: 98 Resp: 594877

Ion Ratio Lower Upper

98 100

100 63.4 49.8 74.6

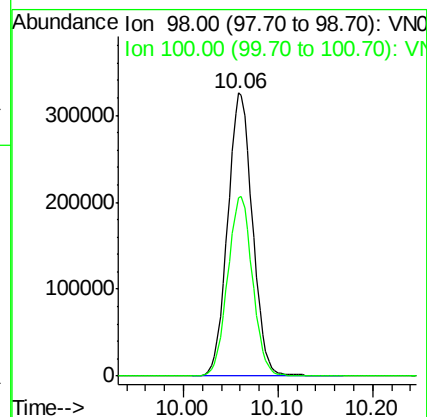

#51

4-Methyl-2-Pentanone

Concen: 2.096 ug/l

RT: 9.95 min Scan# 2554

Delta R.T. 0.00 min

Lab File: VN064022.D




Acq: 9 Oct 2020 5:40


Tgt Ion: 43 Resp: 9432

Ion Ratio Lower Upper

43 100

58 30.4 28.4 42.6

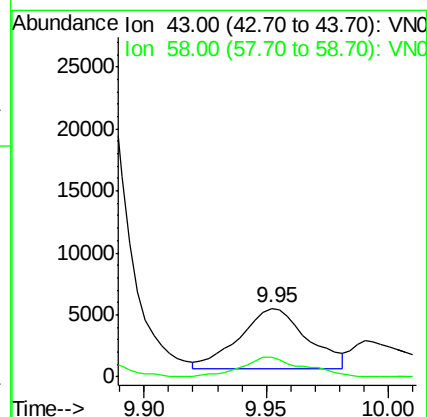







#54

cis-1,3-Dichloropropene
 Concen: 5.767 ug/l
 RT: 9.87 min Scan# 2530
 Delta R.T. 0.07 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40

Instrument :
 MSVOA_N
 ClientSampleId :
 PAV-B4-100620-DP




Tgt Ion	Ratio	Lower	Upper
75	100		
77	0.0	24.6	36.8#
39	44.3	49.7	74.5#

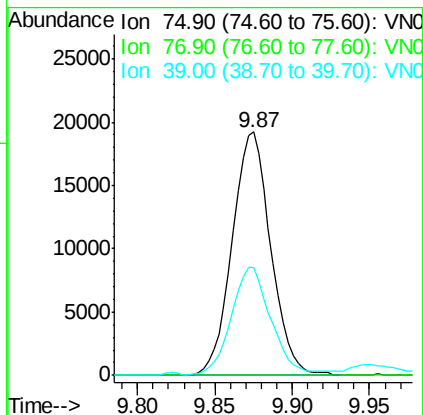


#56

Ethyl methacrylate
 Concen: 0.508 ug/l
 RT: 10.51 min Scan# 2729
 Delta R.T. 0.12 min
 Lab File: VN064022.D
 Acq: 9 Oct 2020 5:40

Tgt Ion	Ratio	Lower	Upper
69	100		
41	3677.0	61.1	91.7#
39	1653.8	42.2	63.4#

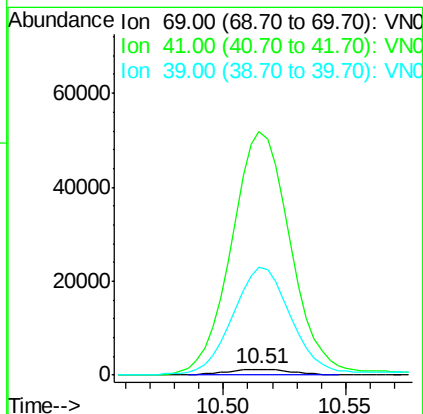

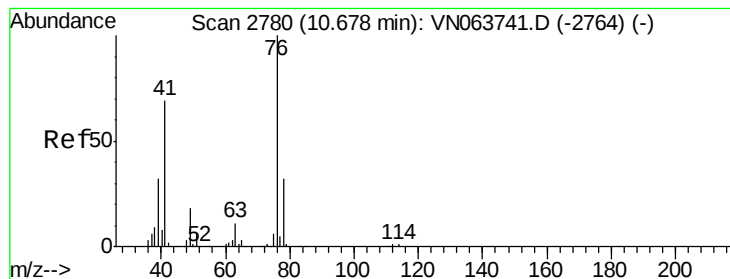

#57

1,3-Dichloropropane

Concen: 1.050 ug/l

RT: 10.74 min Scan# 2798

Delta R.T. 0.06 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :


PAV-B4-100620-DP

Tgt Ion: 76 Resp: 5892

Ion Ratio Lower Upper




76 100

78 0.0 25.2 37.8#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

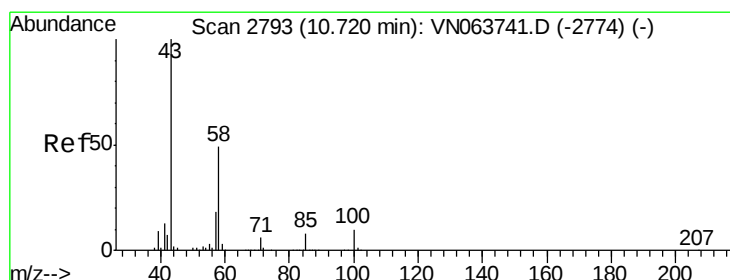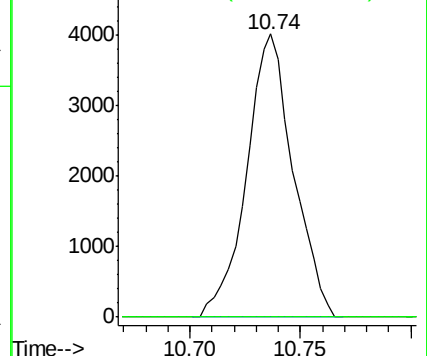

#59

2-Hexanone

Concen: 28.048 ug/l

RT: 10.74 min Scan# 2798

Delta R.T. 0.02 min

Lab File: VN064022.D


Acq: 9 Oct 2020 5:40

Tgt Ion: 43 Resp: 93776

Ion Ratio Lower Upper



43 100


58 18.5 24.6 73.8#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

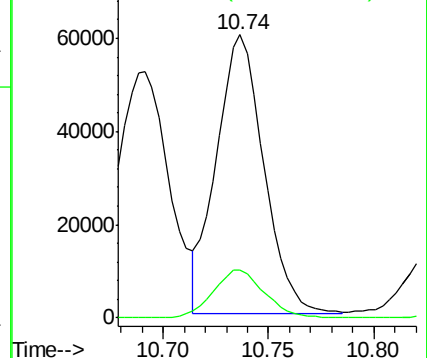



#62

4-Bromofluorobenzene

Concen: 48.431 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :

PAV-B4-100620-DP


Tgt Ion: 95 Resp: 221221

Ion Ratio Lower Upper

95 100

174 76.8 0.0 150.6

176 74.4 0.0 145.4



Abundance Ion 94.90 (94.60 to 95.60): VN063741.D (-3293) (-)

Ion 173.80 (173.50 to 174.50): VN063741.D (-3293) (-)

Ion 175.80 (175.50 to 176.50): VN063741.D (-3293) (-)

12.38



150000

100000

50000

0

Time-->



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2998

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40


Tgt Ion: 117 Resp: 478567

Ion Ratio Lower Upper

117 100

82 58.1 47.4 71.2

119 32.7 26.4 39.6



Abundance Ion 116.90 (116.60 to 117.60): VN063741.D (-2983) (-)

Ion 82.00 (81.70 to 82.70): VN063741.D (-2983) (-)

Ion 118.90 (118.60 to 119.60): VN063741.D (-2983) (-)

11.38


300000


200000

100000

0

Time-->





#71

Bromoform

Concen: 0.348 ug/l

RT: 12.37 min Scan# 3306

Delta R.T. 0.27 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :

PAV-B4-100620-DP


Tgt Ion:173 Resp: 1002

Ion Ratio Lower Upper




173 100

175 1087.5 23.5 70.5#

254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

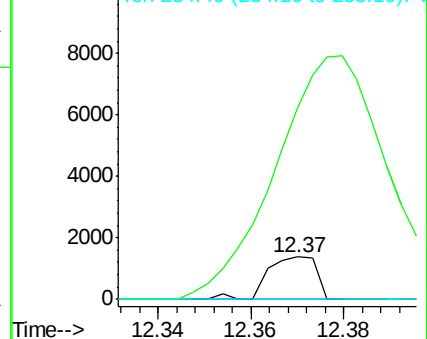

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40


Tgt Ion:152 Resp: 182808

Ion Ratio Lower Upper



152 100


115 62.3 31.3 93.8

150 156.2 0.0 341.8



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V




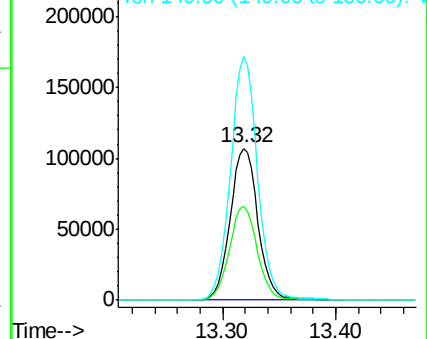


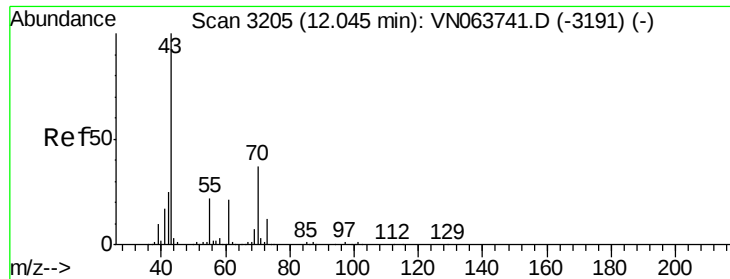

#74
N-ethyl acetate
Concen: 2.696 ug/l
RT: 12.01 min Scan# 3193
Delta R.T. -0.04 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40




Instrument :
MSVOA_N
ClientSampleId :
PAV-B4-100620-DP


Tgt Ion: 43 Resp: 3116
Ion Ratio Lower Upper
43 100
70 0.0 29.8 44.8#
55 3.4 17.9 26.9#
61 0.0 17.0 25.4#

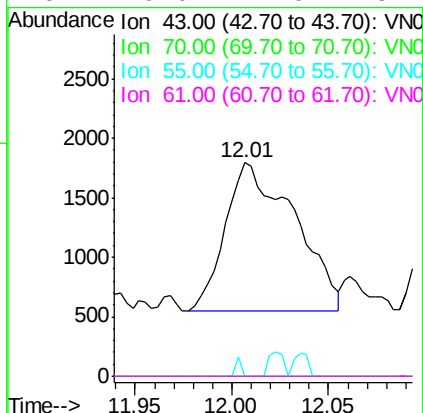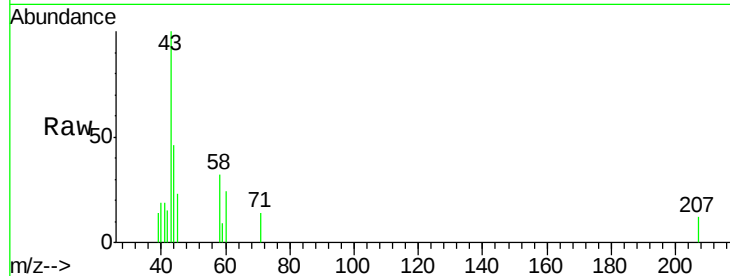

#76
1,2,3-Trichloropropane
Concen: 29.783 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. -0.15 min
Lab File: VN064022.D
Acq: 9 Oct 2020 5:40

Tgt Ion: 75 Resp: 120018
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

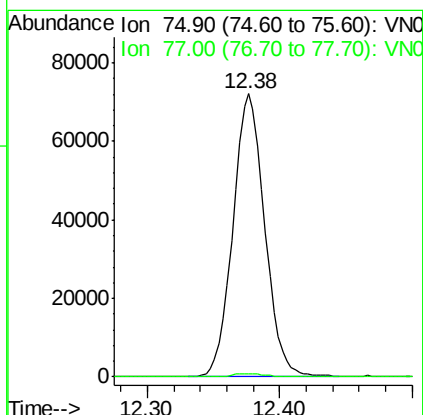

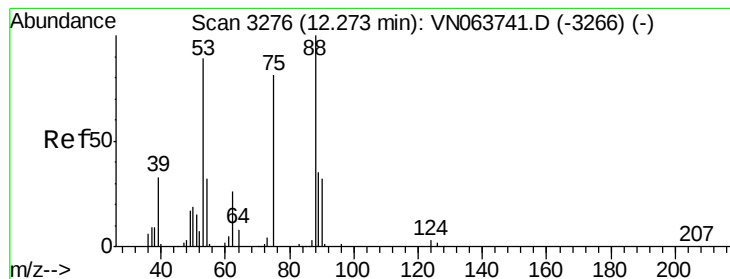

#81

trans-1,4-Dichloro-2-butene

Concen: 85.778 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40

Instrument :

MSVOA_N

ClientSampleId :

PAV-B4-100620-DP


Tgt Ion: 75 Resp: 120018

Ion Ratio Lower Upper

75 100

53 0.1 88.2 132.2#




89 0.0 36.0 54.0#



Abundance Ion 74.90 (74.60 to 75.60): VN063741.D (-3266) (-)

Ion 53.00 (52.70 to 53.70): VN063741.D (-3266) (-)

Ion 88.90 (88.60 to 89.60): VN063741.D (-3266) (-)

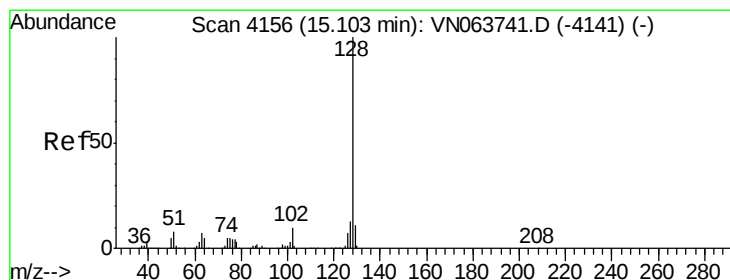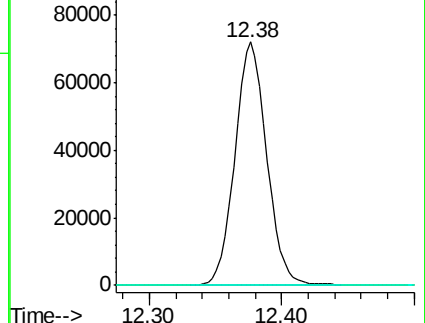

#95

Naphthalene

Concen: 1.932 ug/l

RT: 15.12 min Scan# 4160

Delta R.T. 0.01 min

Lab File: VN064022.D

Acq: 9 Oct 2020 5:40


Tgt Ion: 128 Resp: 73

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): VN063741.D (-4141) (-)

Ion 127.00 (126.70 to 127.70): VN063741.D (-4141) (-)

Ion 129.00 (128.70 to 129.70): VN063741.D (-4141) (-)

