

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_N\DATA\VN100820\  
 Data File : VN064024.D  
 Acq On : 9 Oct 2020 6:28  
 Operator : JC/MD  
 Sample : L4292-06  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PAV-B13-100620-15-16

Quant Time: Oct 09 12:06:57 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N093020W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Oct 01 01:46:38 2020  
 Response via : Initial Calibration


| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 7.63  | 168  | 244653   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.55  | 114  | 454905   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.38 | 117  | 478248   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.32 | 152  | 182489   | 50.00 | ug/l  | 0.00     |

|                             |        |     |          |       |         |      |
|-----------------------------|--------|-----|----------|-------|---------|------|
| System Monitoring Compounds |        |     |          |       |         |      |
| 33) 1,2-Dichloroethane-d4   | 7.98   | 65  | 203077   | 50.24 | ug/l    | 0.00 |
| Spiked Amount               | 50.000 |     | Recovery | =     | 100.48% |      |
| 35) Dibromofluoromethane    | 7.55   | 113 | 154123   | 48.83 | ug/l    | 0.00 |
| Spiked Amount               | 50.000 |     | Recovery | =     | 97.66%  |      |
| 50) Toluene-d8              | 10.06  | 98  | 591254   | 49.41 | ug/l    | 0.00 |
| Spiked Amount               | 50.000 |     | Recovery | =     | 98.82%  |      |
| 62) 4-Bromofluorobenzene    | 12.38  | 95  | 216225   | 48.07 | ug/l    | 0.00 |
| Spiked Amount               | 50.000 |     | Recovery | =     | 96.14%  |      |

| Target Compounds               | R.T.  | QIon | Response | Conc   | Units  | Qvalue |
|--------------------------------|-------|------|----------|--------|--------|--------|
| 16) Acetone                    | 3.78  | 43   | 17513    | 14.076 | ug/l   | 97     |
| 17) Carbon Disulfide           | 4.01  | 76   | 821      | 0.822  | ug/l # | 76     |
| 18) Methyl Acetate             | 4.28  | 43   | 1771     | 0.548  | ug/l # | 75     |
| 20) Methylene Chloride         | 4.51  | 84   | 9510     | 3.428  | ug/l   | 96     |
| 29) Tetrahydrofuran            | 7.17  | 42   | 765      | 0.647  | ug/l # | 36     |
| 31) Cyclohexane                | 7.62  | 56   | 7114     | 1.516  | ug/l # | 42     |
| 36) 1,1-Dichloropropene        | 7.62  | 75   | 21020    | 4.561  | ug/l # | 46     |
| 37) Ethyl Acetate              | 6.81  | 43   | 2489     | 0.544  | ug/l # | 70     |
| 38) Carbon Tetrachloride       | 7.62  | 117  | 25151    | 4.867  | ug/l # | 16     |
| 43) Isopropyl Acetate          | 8.13  | 43   | 85204    | 11.282 | ug/l   | 99     |
| 45) 1,2-Dichloropropane        | 9.23  | 63   | 1529     | 0.430  | ug/l # | 44     |
| 48) Methyl methacrylate        | 9.14  | 41   | 4380     | 1.174  | ug/l # | 12     |
| 49) 1,4-Dioxane                | 9.24  | 88   | 61       | 1.150  | ug/l # | 1      |
| 51) 4-Methyl-2-Pentanone       | 9.96  | 43   | 7430     | 1.676  | ug/l   | 99     |
| 54) cis-1,3-Dichloropropene    | 9.87  | 75   | 25958    | 4.581  | ug/l # | 65     |
| 56) Ethyl methacrylate         | 10.51 | 69   | 2214     | 0.478  | ug/l # | 1      |
| 57) 1,3-Dichloropropane        | 10.73 | 76   | 1945     | 0.352  | ug/l # | 43     |
| 59) 2-Hexanone                 | 10.74 | 43   | 32416    | 9.846  | ug/l # | 57     |
| 74) N-amyl acetate             | 12.03 | 43   | 751      | 2.332  | ug/l # | 46     |
| 76) 1,2,3-Trichloropropane     | 12.38 | 75   | 116633   | 28.993 | ug/l # | 100    |
| 81) trans-1,4-Dichloro-2-buten | 12.38 | 75   | 116633   | 83.505 | ug/l # | 6      |
| 95) Naphthalene                | 15.10 | 128  | 72       | 1.931  | ug/l # | 69     |

(#) = qualifier out of range (m) = manual integration (+) = signals summed



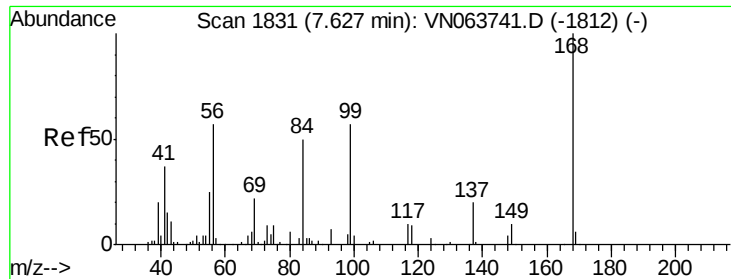

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28

Instrument :

MSVOA\_N

ClientSampleId :


PAV-B13-100620-15-16

Tgt Ion:168 Resp: 244653

Ion Ratio Lower Upper

168 100

99 61.1 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#16

Acetone

Concen: 14.076 ug/l

RT: 3.78 min Scan# 635

Delta R.T. 0.01 min

Lab File: VN064024.D


Acq: 9 Oct 2020 6:28

Tgt Ion: 43 Resp: 17513

Ion Ratio Lower Upper

43 100

58 26.4 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

3.78


6000


4000

2000

0

Time--> 3.70 3.75 3.80 3.85 3.90





#17

Carbon Disulfide

Concen: 0.822 ug/l

RT: 4.01 min Scan# 705

Delta R.T. -0.01 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28

Instrument :

MSVOA\_N

ClientSampleId :


PAV-B13-100620-15-16

Tgt Ion: 76 Resp: 821

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.4#



Abundance Ion 75.90 (75.60 to 76.60): VN063741.D (-685) (-)

Ion 77.90 (77.60 to 78.60): VN063741.D (-685) (-)

4.01



600

400

200

0

Time-->



#18

Methyl Acetate

Concen: 0.548 ug/l

RT: 4.28 min Scan# 790

Delta R.T. 0.00 min

Lab File: VN064024.D


Acq: 9 Oct 2020 6:28

Tgt Ion: 43 Resp: 1771

Ion Ratio Lower Upper

43 100

74 33.9 17.4 26.2#



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-768) (-)

Ion 74.00 (73.70 to 74.70): VN063741.D (-768) (-)

4.28


1500


1000

500

0

Time-->









#20  
Methylene Chloride  
Concen: 3.428 ug/l  
RT: 4.51 min Scan# 860  
Delta R.T. 0.00 min  
Lab File: VN064024.D  
Acq: 9 Oct 2020 6:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
PAV-B13-100620-15-16


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 84    | Resp: | 9510  |
| Ion      | Ratio | Lower | Upper |
| 84       | 100   |       |       |
| 49       | 136.7 | 110.4 | 165.6 |
| 51       | 38.4  | 33.3  | 49.9  |
| 86       | 54.9  | 50.7  | 76.1  |



#29  
Tetrahydrofuran  
Concen: 0.647 ug/l  
RT: 7.17 min Scan# 1689  
Delta R.T. 0.01 min  
Lab File: VN064024.D  
Acq: 9 Oct 2020 6:28

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 42    | Resp: | 765   |
| Ion      | Ratio | Lower | Upper |
| 42       | 100   |       |       |
| 72       | 0.0   | 32.8  | 49.2# |
| 71       | 0.0   | 30.6  | 45.8# |





#31

Cyclohexane

Concen: 1.516 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. 0.01 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28

Instrument :

MSVOA\_N

ClientSampleId :

PAV-B13-100620-15-16


Tgt Ion: 56 Resp: 7114

Ion Ratio Lower Upper

56 100

69 128.1 25.4 38.2#




84 89.0 63.3 94.9



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0



#33

1,2-Dichloroethane-d4

Concen: 50.244 ug/l

RT: 7.98 min Scan# 1942

Delta R.T. -0.00 min

Lab File: VN064024.D


Acq: 9 Oct 2020 6:28

Tgt Ion: 65 Resp: 203077

Ion Ratio Lower Upper



65 100


67 51.6 0.0 99.6



Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0





#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. 0.00 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28

Instrument :

MSVOA\_N

ClientSampleId :

PAV-B13-100620-15-16


Tgt Ion:114 Resp: 454905

Ion Ratio Lower Upper

114 100

63 23.0 0.0 45.0




88 16.7 0.0 34.0



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0



#35

Dibromofluoromethane

Concen: 48.828 ug/l

RT: 7.55 min Scan# 1807

Delta R.T. 0.00 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28


Tgt Ion:113 Resp: 154123

Ion Ratio Lower Upper

113 100

111 102.1 81.8 122.8



192 17.8 14.2 21.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V









#36  
 1,1-Dichloropropene  
 Concen: 4.561 ug/l  
 RT: 7.62 min Scan# 1830  
 Delta R.T. -0.13 min  
 Lab File: VN064024.D  
 Acq: 9 Oct 2020 6:28




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PAV-B13-100620-15-16


Tgt Ion: 75 Resp: 21020  
 Ion Ratio Lower Upper  
 75 100  
 110 3.5 16.9 50.6#  
 77 0.0 24.5 36.7#



#37  
 Ethyl Acetate  
 Concen: 0.544 ug/l  
 RT: 6.81 min Scan# 1576  
 Delta R.T. -0.07 min  
 Lab File: VN064024.D  
 Acq: 9 Oct 2020 6:28

Tgt Ion: 43 Resp: 2489  
 Ion Ratio Lower Upper  
 43 100  
 61 0.0 10.4 15.6#  
 70 0.0 7.3 10.9#





#38

Carbon Tetrachloride

Concen: 4.867 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. -0.11 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28

Instrument :

MSVOA\_N

ClientSampleId :

PAV-B13-100620-15-16


Tgt Ion:117 Resp: 25151

Ion Ratio Lower Upper

117 100

119 6.9 80.1 120.1#




121 0.0 25.7 38.5#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V



#43

Isopropyl Acetate

Concen: 11.282 ug/l

RT: 8.13 min Scan# 1986

Delta R.T. 0.00 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28


Tgt Ion: 43 Resp: 85204

Ion Ratio Lower Upper

43 100

61 17.8 14.2 21.4



87 12.0 9.0 13.6




Abundance Ion 43.00 (42.70 to 43.70): V

Ion 61.00 (60.70 to 61.70): V

Ion 87.00 (86.70 to 87.70): V





#45

1,2-Dichloropropane

Concen: 0.430 ug/l

RT: 9.23 min Scan# 2331

Delta R.T. 0.15 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28

Instrument :

MSVOA\_N

ClientSampleId :


PAV-B13-100620-15-16

Tgt Ion: 63 Resp: 1529

Ion Ratio Lower Upper




63 100

65 0.0 24.7 37.1#



Abundance Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0



#48

Methyl methacrylate

Concen: 1.174 ug/l

RT: 9.14 min Scan# 2302

Delta R.T. -0.03 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28


Tgt Ion: 41 Resp: 4380

Ion Ratio Lower Upper

41 100

69 0.0 60.9 91.3#



39 0.0 57.5 86.3#




Abundance Ion 41.00 (40.70 to 41.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 39.00 (38.70 to 39.70): VN0





#49

1,4-Dioxane

Concen: 1.150 ug/l

RT: 9.24 min Scan# 2332

Delta R.T. 0.07 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28

Instrument :

MSVOA\_N

ClientSampleId :

PAV-B13-100620-15-16


Tgt Ion: 88 Resp: 61

Ion Ratio Lower Upper

88 100

43 2048495.1 33.1 49.7#




58 10660.7 58.9 88.3#



Abundance Ion 88.00 (87.70 to 88.70): VN0

Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0



#50

Toluene-d8

Concen: 49.412 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN064024.D


Acq: 9 Oct 2020 6:28

Tgt Ion: 98 Resp: 591254

Ion Ratio Lower Upper



98 100


100 63.7 49.8 74.6



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0









#51  
 4-Methyl-2-Pentanone  
 Concen: 1.676 ug/l  
 RT: 9.96 min Scan# 2555  
 Delta R.T. 0.00 min  
 Lab File: VN064024.D  
 Acq: 9 Oct 2020 6:28




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PAV-B13-100620-15-16


Tgt Ion: 43 Resp: 7430  
 Ion Ratio Lower Upper  
 43 100  
 58 34.7 28.4 42.6



#54  
 cis-1,3-Dichloropropene  
 Concen: 4.581 ug/l  
 RT: 9.87 min Scan# 2530  
 Delta R.T. 0.07 min  
 Lab File: VN064024.D  
 Acq: 9 Oct 2020 6:28

Tgt Ion: 75 Resp: 25958  
 Ion Ratio Lower Upper  
 75 100  
 77 0.0 24.6 36.8#  
 39 43.0 49.7 74.5#





#56

Ethyl methacrylate

Concen: 0.478 ug/l

RT: 10.51 min Scan# 2729

Delta R.T. 0.12 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28

Instrument :

MSVOA\_N

ClientSampleId :

PAV-B13-100620-15-16





Tgt Ion: 69 Resp: 2214

Ion Ratio Lower Upper

69 100

41 2945.4 61.1 91.7#

39 1286.2 42.2 63.4#



#57

1,3-Dichloropropane

Concen: 0.352 ug/l

RT: 10.73 min Scan# 2797

Delta R.T. 0.05 min

Lab File: VN064024.D




Acq: 9 Oct 2020 6:28


Tgt Ion: 76 Resp: 1945

Ion Ratio Lower Upper

76 100

78 0.0 25.2 37.8#









#59  
2-Hexanone  
Concen: 9.846 ug/l  
RT: 10.74 min Scan# 2798  
Delta R.T. 0.02 min  
Lab File: VN064024.D  
Acq: 9 Oct 2020 6:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
PAV-B13-100620-15-16


Tgt Ion: 43 Resp: 32416  
Ion Ratio Lower Upper  
43 100  
58 19.5 24.6 73.8#



#62  
4-Bromofluorobenzene  
Concen: 48.070 ug/l  
RT: 12.38 min Scan# 3308  
Delta R.T. 0.00 min  
Lab File: VN064024.D  
Acq: 9 Oct 2020 6:28

Tgt Ion: 95 Resp: 216225  
Ion Ratio Lower Upper  
95 100  
174 78.3 0.0 150.6  
176 74.9 0.0 145.4









#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.38 min Scan# 2998  
Delta R.T. 0.00 min  
Lab File: VN064024.D  
Acq: 9 Oct 2020 6:28

Instrument :  
MSVOA\_N  
ClientSampleId :  
PAV-B13-100620-15-16

Tgt Ion:117 Resp: 478248  
Ion Ratio Lower Upper  
117 100  
82 59.2 47.4 71.2  
119 32.1 26.4 39.6




Abundance Ion 116.90 (116.60 to 117.60): V  
Ion 82.00 (81.70 to 82.70): V  
Ion 118.90 (118.60 to 119.60): V






#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.32 min Scan# 3601  
Delta R.T. 0.00 min  
Lab File: VN064024.D  
Acq: 9 Oct 2020 6:28

Tgt Ion:152 Resp: 182489  
Ion Ratio Lower Upper  
152 100  
115 62.4 31.3 93.8  
150 157.3 0.0 341.8



Abundance Ion 151.90 (151.60 to 152.60): V  
Ion 114.90 (114.60 to 115.60): V  
Ion 149.90 (149.60 to 150.60): V









#74  
N-ethyl acetate  
Concen: 2.332 ug/l  
RT: 12.03 min Scan# 3199  
Delta R.T. -0.02 min  
Lab File: VN064024.D  
Acq: 9 Oct 2020 6:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
PAV-B13-100620-15-16


Tgt Ion: 43 Resp: 751  
Ion Ratio Lower Upper  
43 100  
70 0.0 29.8 44.8#  
55 0.0 17.9 26.9#  
61 0.0 17.0 25.4#



#76  
1,2,3-Trichloropropane  
Concen: 28.993 ug/l  
RT: 12.38 min Scan# 3308  
Delta R.T. -0.15 min  
Lab File: VN064024.D  
Acq: 9 Oct 2020 6:28

Tgt Ion: 75 Resp: 116633  
Ion Ratio Lower Upper  
75 100  
77 1.0 0.0 0.0#





#81

trans-1,4-Dichloro-2-butene

Concen: 83.505 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28

Instrument :

MSVOA\_N

ClientSampleId :

PAV-B13-100620-15-16


Tgt Ion: 75 Resp: 116633

Ion Ratio Lower Upper

75 100

53 0.2 88.2 132.2#




89 0.0 36.0 54.0#



Abundance Ion 74.90 (74.60 to 75.60): VN064024.D (-3308) (-)

Ion 53.00 (52.70 to 53.70): VN064024.D (-3308) (-)

Ion 88.90 (88.60 to 89.60): VN064024.D (-3308) (-)



#95

Naphthalene

Concen: 1.931 ug/l

RT: 15.10 min Scan# 4155

Delta R.T. -0.00 min

Lab File: VN064024.D

Acq: 9 Oct 2020 6:28


Tgt Ion: 128 Resp: 72

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): VN064024.D (-4156) (-)

Ion 127.00 (126.70 to 127.70): VN064024.D (-4156) (-)

Ion 129.00 (128.70 to 129.70): VN064024.D (-4156) (-)

