


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100820\
Data File : VN063980.D
Acq On : 8 Oct 2020 8:55
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Title : SW846 8260
Last Update : Thu Oct 01 01:46:38 2020

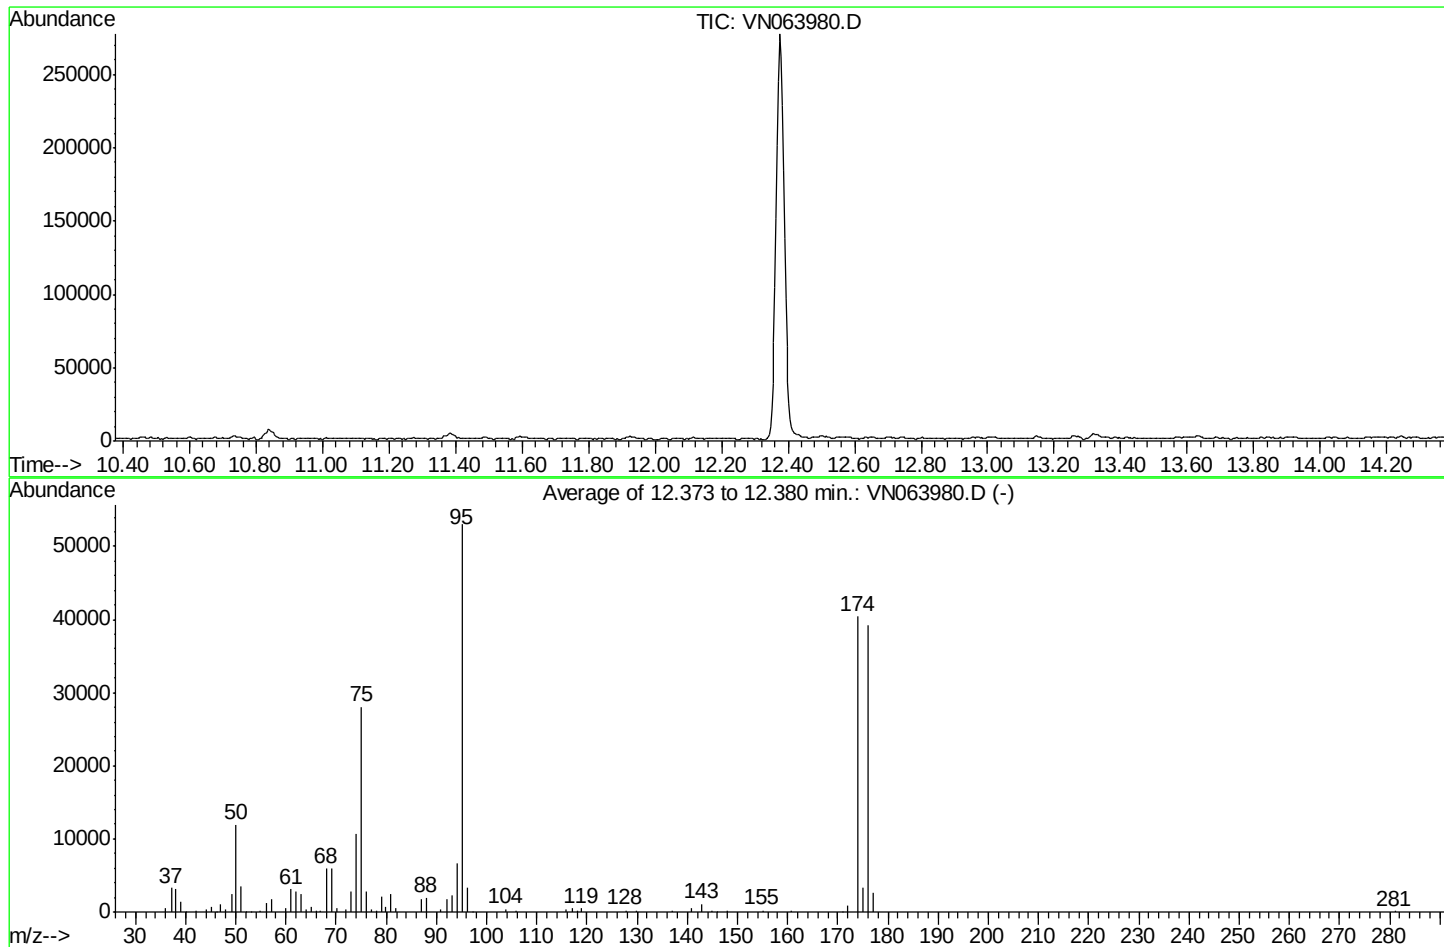

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	11978	PASS
75	95	30	60	53.0	28096	PASS
95	95	100	100	100.0	53018	PASS
96	95	5	9	6.2	3312	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.3	40432	PASS
175	174	5	9	8.5	3417	PASS
176	174	95	101	96.9	39186	PASS
177	176	5	9	6.9	2701	PASS