

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100824\
 Data File : VN084346.D
 Acq On : 08 Oct 2024 13:45
 Operator : JC\MD
 Sample : VN1008WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1008WBL01

Quant Time: Oct 09 02:30:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N100824W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Oct 09 02:21:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.812	128	30307	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.100	114	164744	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.865	117	147299	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.577	65	77450	31.742	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	105.800%
60) 4-Bromofluorobenzene	12.847	95	61537	25.313	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	84.367%
63) Toluene-d8	10.565	98	200328	29.357	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	97.867%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100824\
Data File : VN084346.D
Acq On : 08 Oct 2024 13:45
Operator : JC\MD
Sample : VN1008WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1008WBL01

Quant Time: Oct 09 02:30:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N100824W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Oct 09 02:21:08 2024
Response via : Initial Calibration




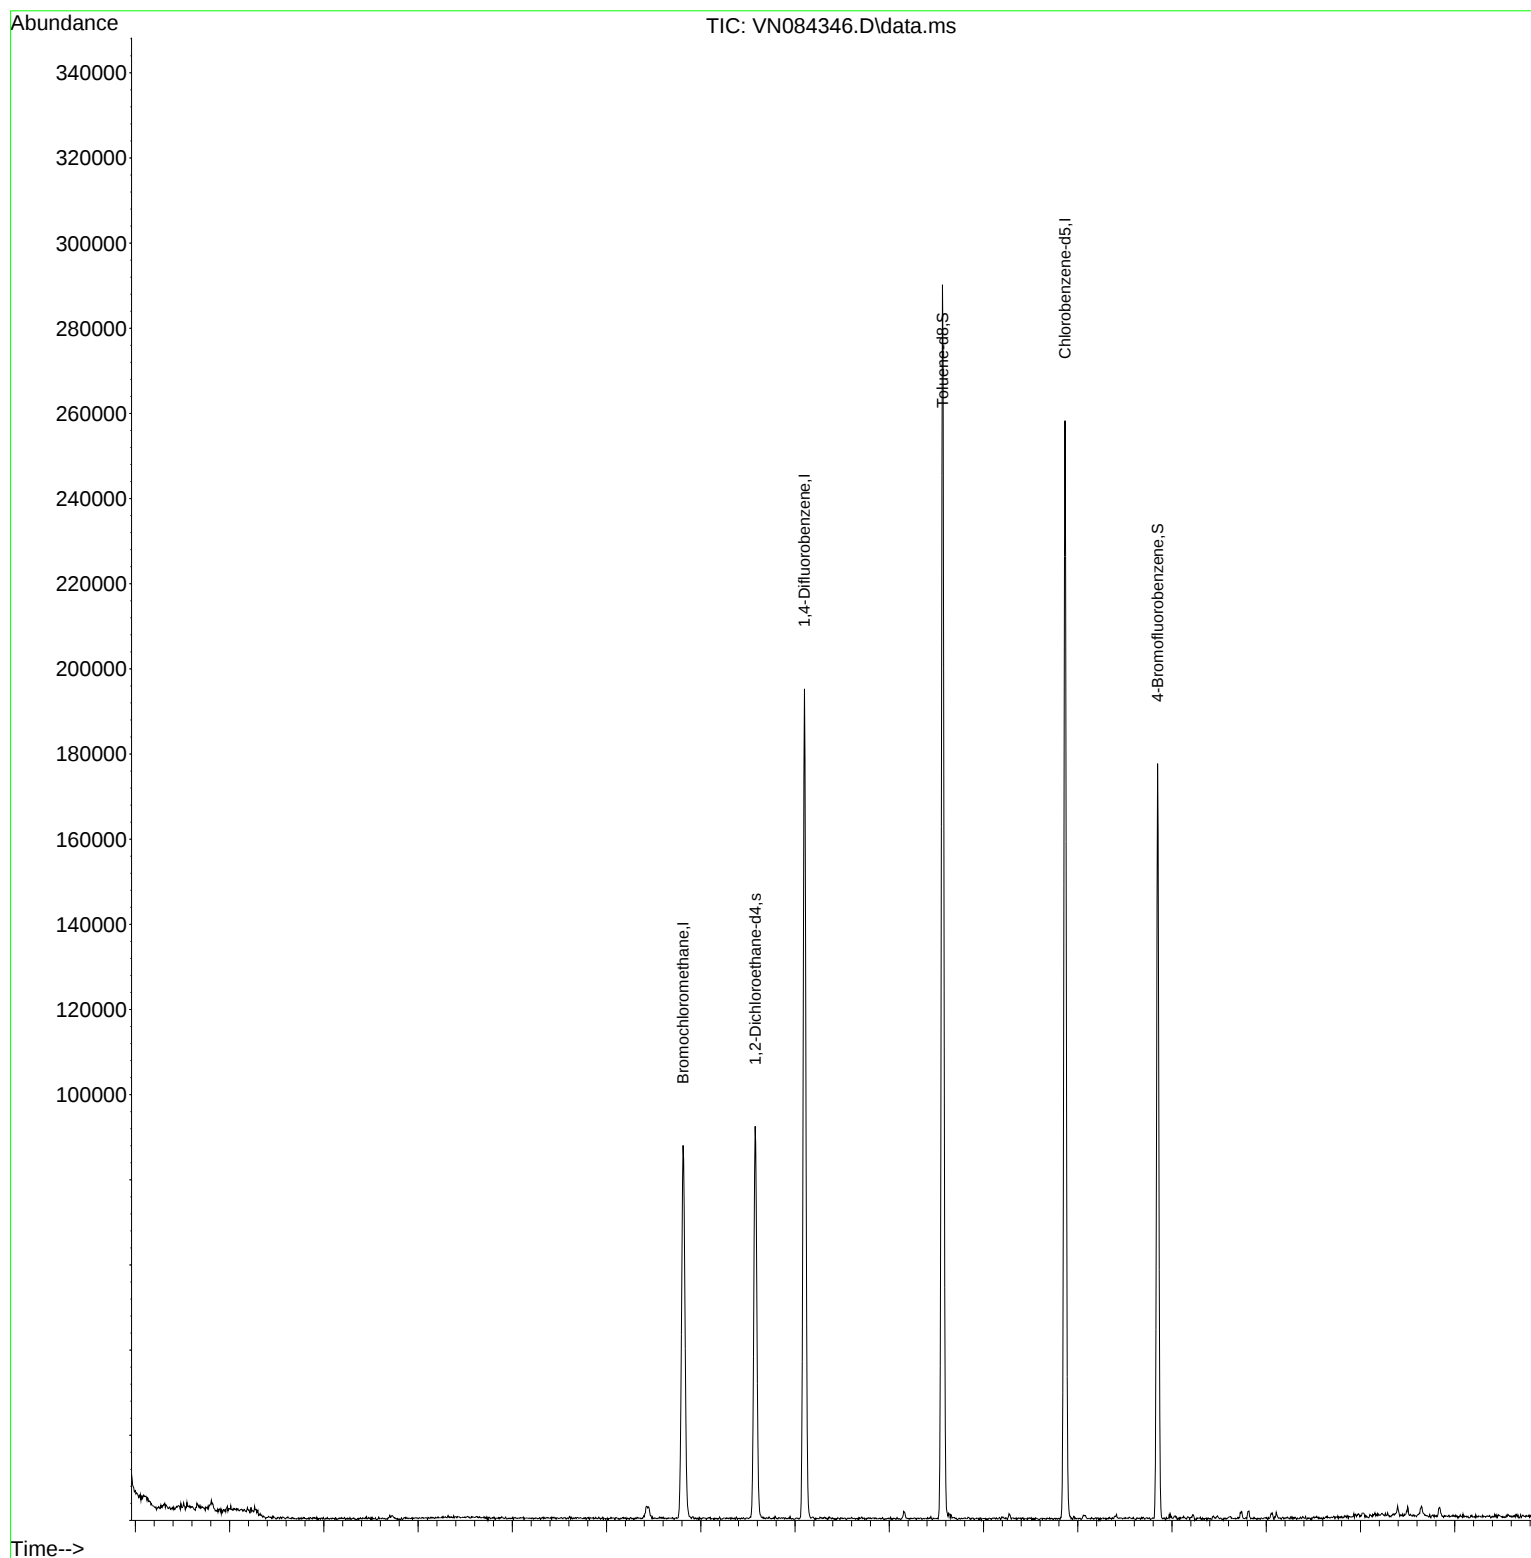


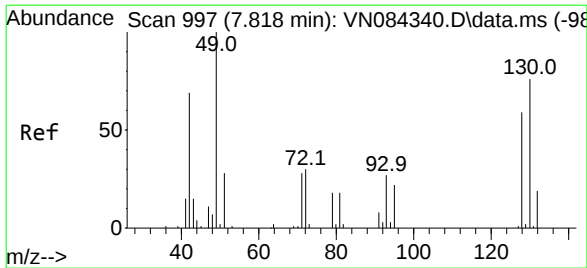

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.812 min Scan# 997
Delta R.T. -0.006 min
Lab File: VN084346.D
Acq: 08 Oct 2024 13:45




Instrument :
MSVOA_N
ClientSampleId :
VN1008WBL01


Tgt Ion:128 Resp: 30307
Ion Ratio Lower Upper
128 100
49 176.6 0.0 430.0
130 131.2 0.0 329.8

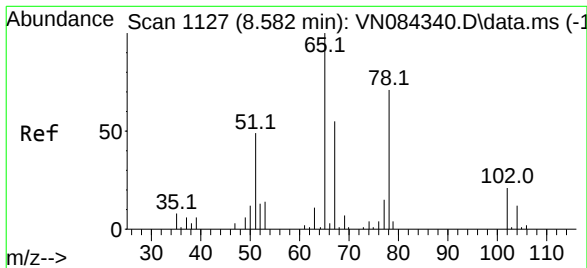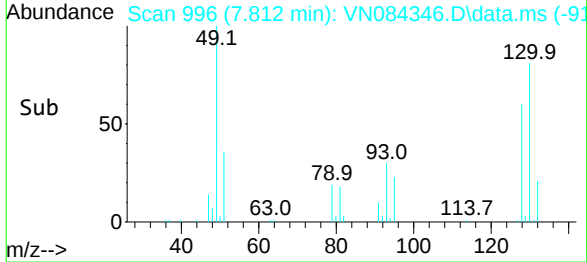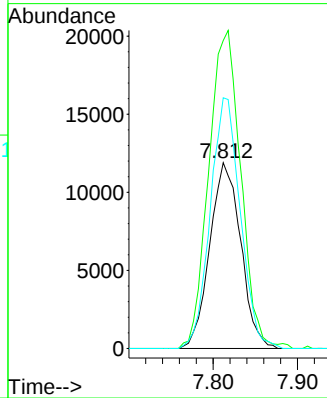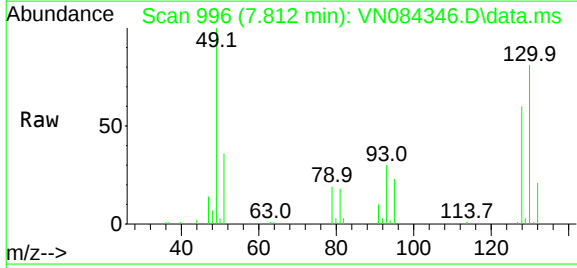

#27
1,2-Dichloroethane-d4
Concen: 31.742 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.006 min
Lab File: VN084346.D
Acq: 08 Oct 2024 13:45

Tgt Ion: 65 Resp: 77450
Ion Ratio Lower Upper
65 100
67 52.4 41.5 62.3


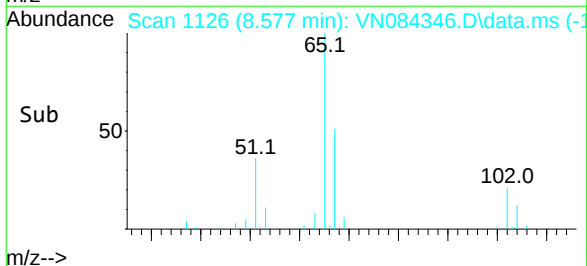
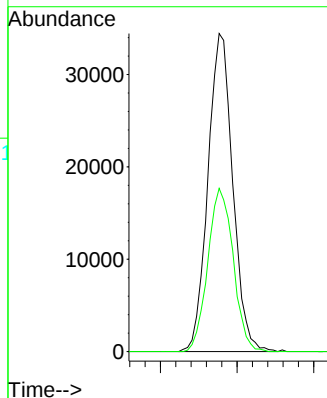
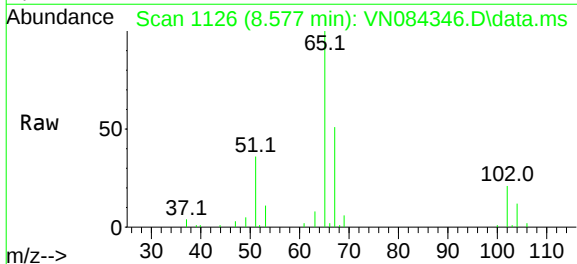


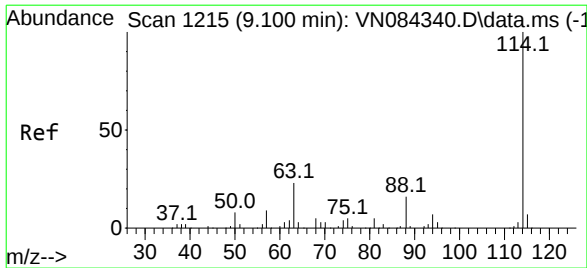

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 9.100 min Scan# 1215
Delta R.T. 0.000 min
Lab File: VN084346.D
Acq: 08 Oct 2024 13:45




Instrument :
MSVOA_N
ClientSampleId :
VN1008WBL01


Tgt Ion:	114	Resp:	164744
Ion	Ratio	Lower	Upper
114	100		
63	21.4	17.4	26.0
88	16.1	13.2	19.8

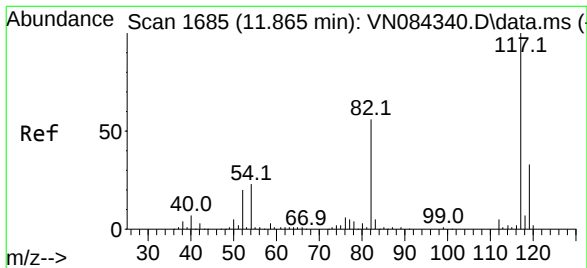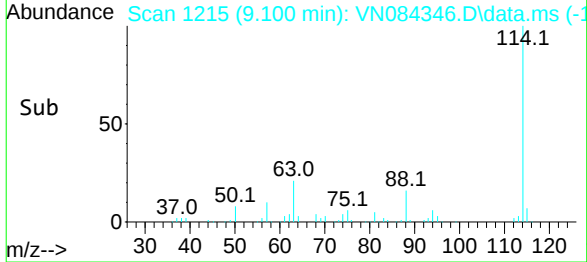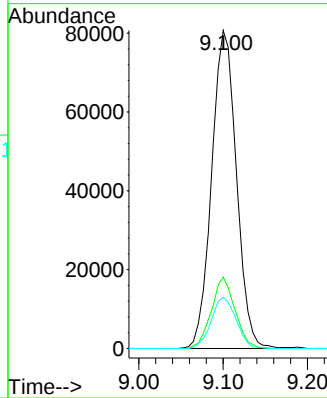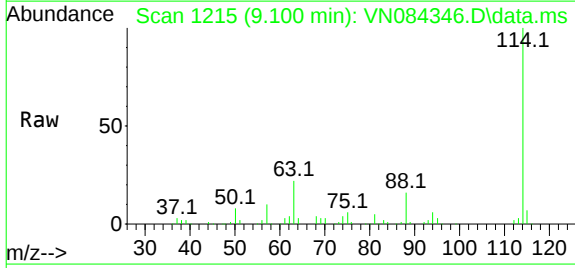

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VN084346.D
Acq: 08 Oct 2024 13:45


Tgt Ion:	117	Resp:	147299
Ion	Ratio	Lower	Upper
117	100		
82	56.7	46.2	69.4
119	32.3	25.4	38.2

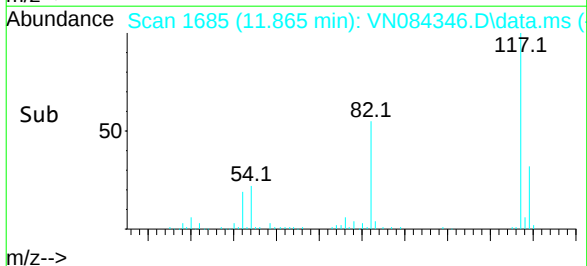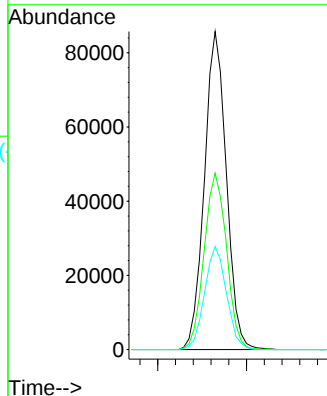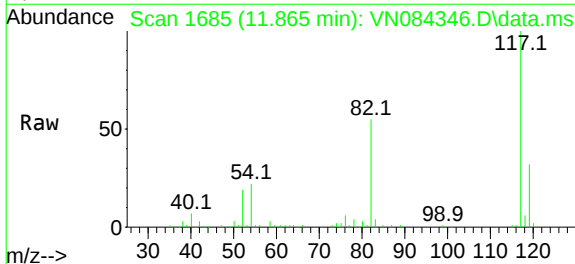



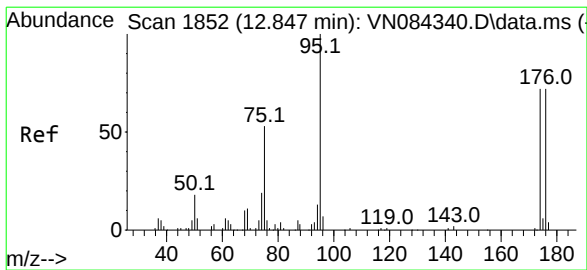


#60
4-Bromofluorobenzene
Concen: 25.313 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN084346.D
Acq: 08 Oct 2024 13:45

Instrument :
MSVOA_N
ClientSampleId :
VN1008WBL01

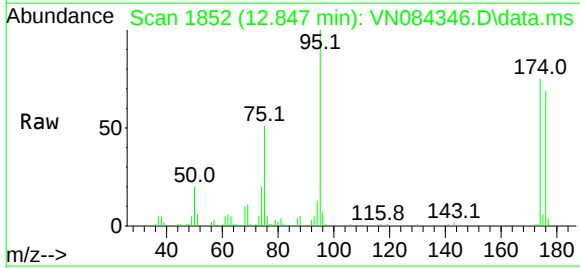

Tgt Ion:	95	Resp:	61537
Ion Ratio	Lower	Upper	
95	100		
174	73.7	58.2	87.2
176	70.3	56.4	84.6

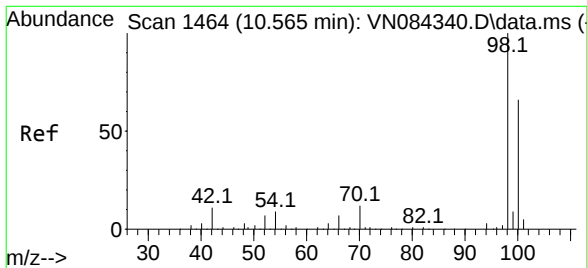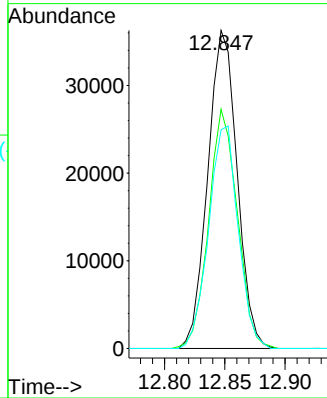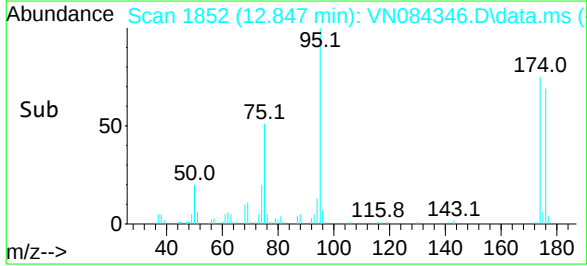

#63
Toluene-d8
Concen: 29.357 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN084346.D
Acq: 08 Oct 2024 13:45

Tgt Ion:	98	Resp:	200328
Ion Ratio	Lower	Upper	
98	100		
100	65.2	52.5	78.7

