


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100918\
 Data File : VN051742.D
 Acq On : 9 Oct 2018 7:48
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N100518W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Oct 05 11:11:26 2018

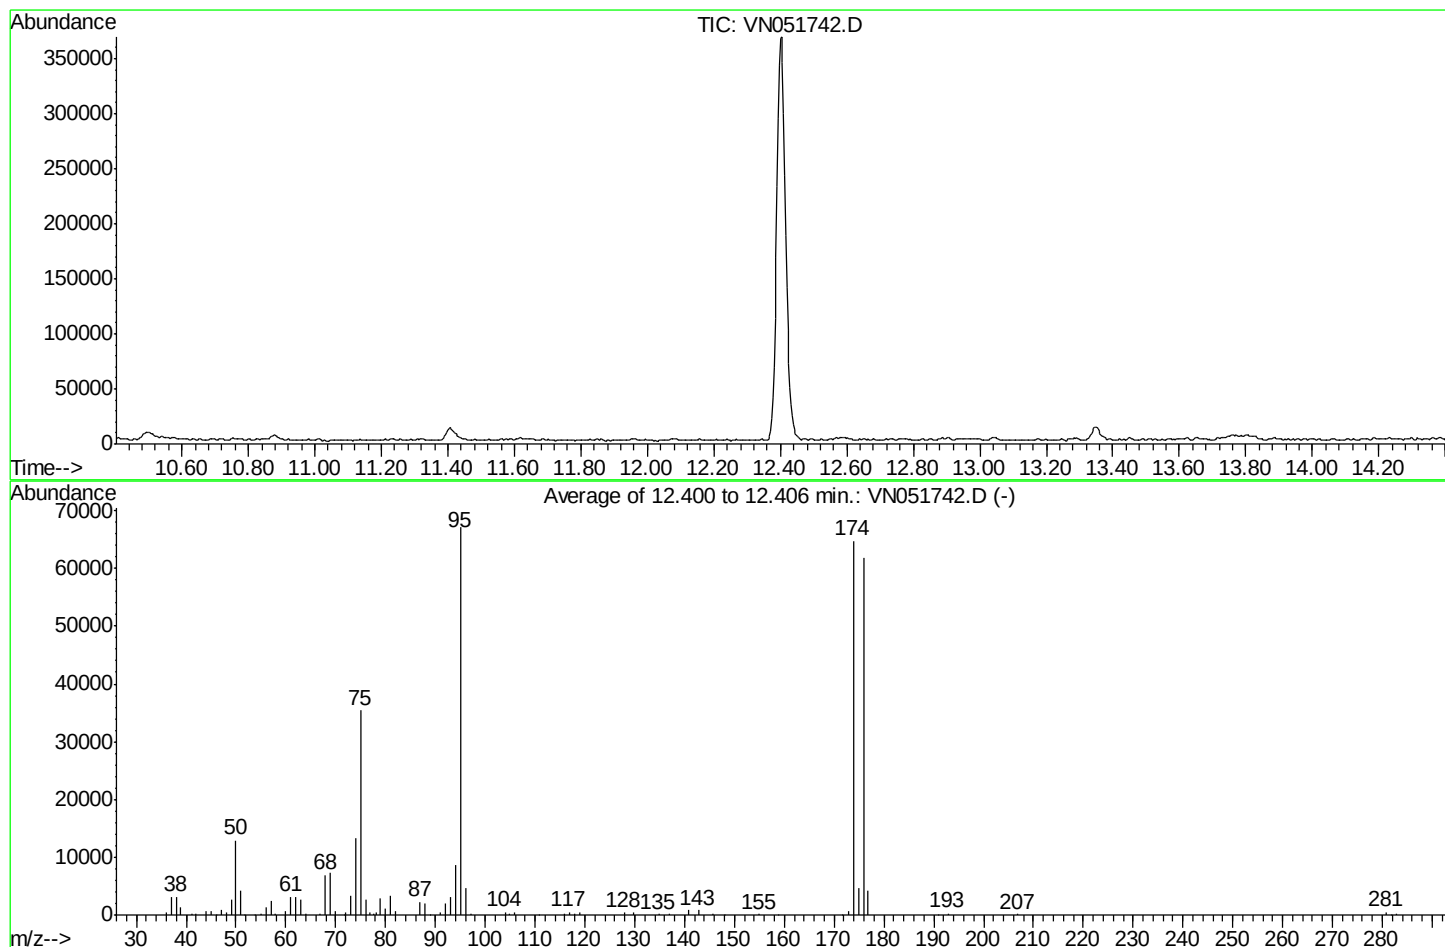

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	12935	PASS
75	95	30	60	52.8	35440	PASS
95	95	100	100	100.0	67112	PASS
96	95	5	9	7.0	4673	PASS
173	174	0.00	2	1.0	634	PASS
174	95	50	100	96.5	64770	PASS
175	174	5	9	7.1	4626	PASS
176	174	95	101	95.5	61877	PASS
177	176	5	9	7.0	4331	PASS