


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100918\
Data File : VN051751.D
Acq On : 9 Oct 2018 14:59
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Title : SW846 8260
Last Update : Tue Oct 09 06:03:49 2018

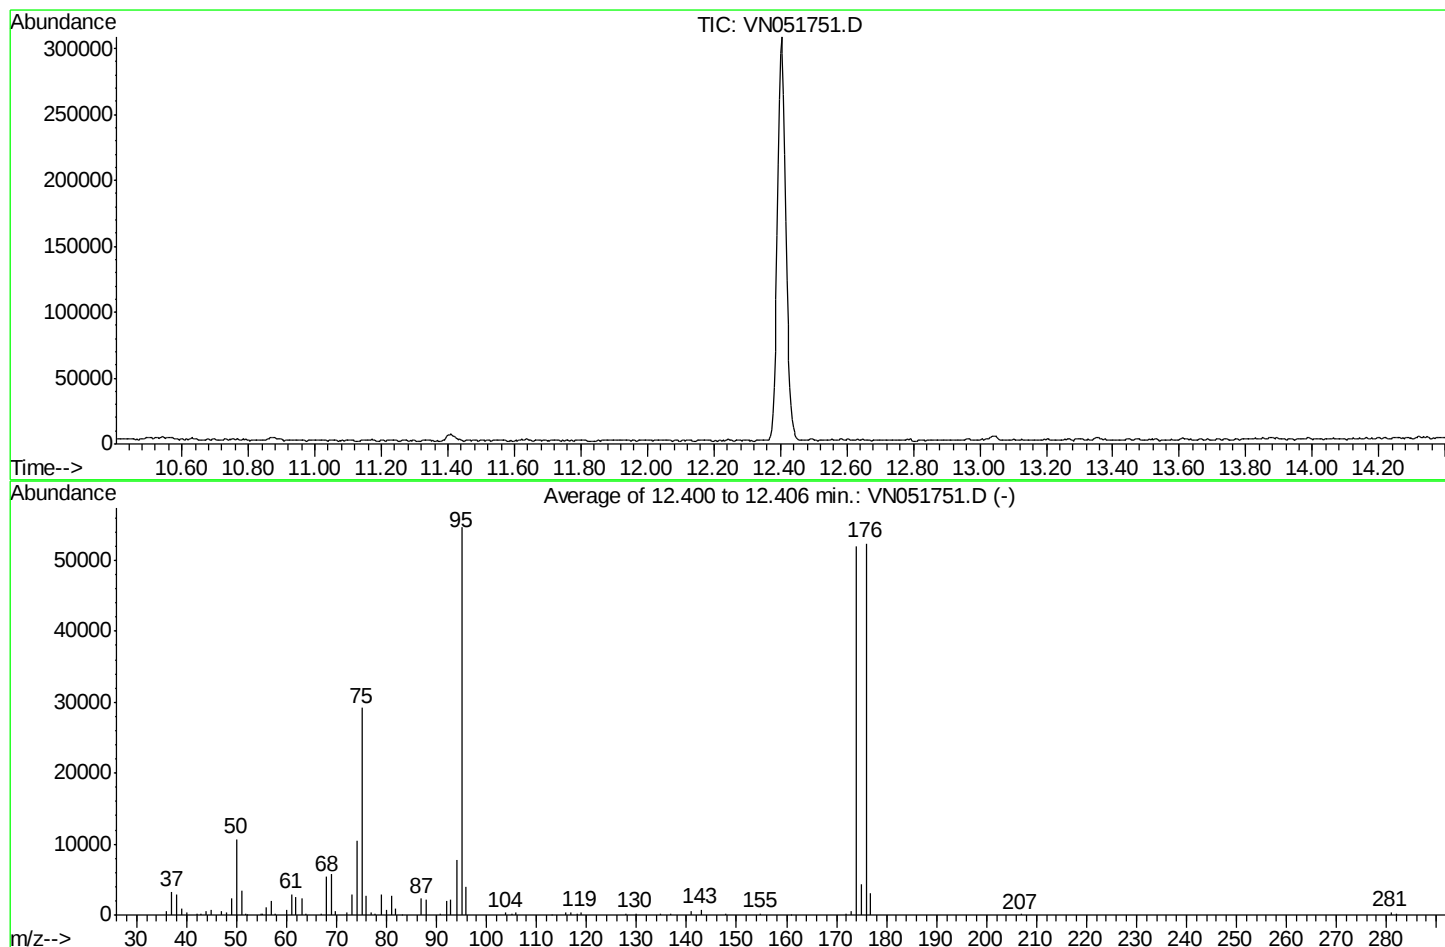

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	10714	PASS
75	95	30	60	53.5	29232	PASS
95	95	100	100	100.0	54656	PASS
96	95	5	9	7.2	3929	PASS
173	174	0.00	2	1.0	515	PASS
174	95	50	100	95.2	52053	PASS
175	174	5	9	8.4	4347	PASS
176	174	95	101	100.7	52418	PASS
177	176	5	9	6.0	3131	PASS