


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100919\
Data File : VN058627.D
Acq On : 9 Oct 2019 8:51
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100819SIM-VINYL.M
Title : SW846 8260
Last Update : Wed Oct 09 04:07:23 2019

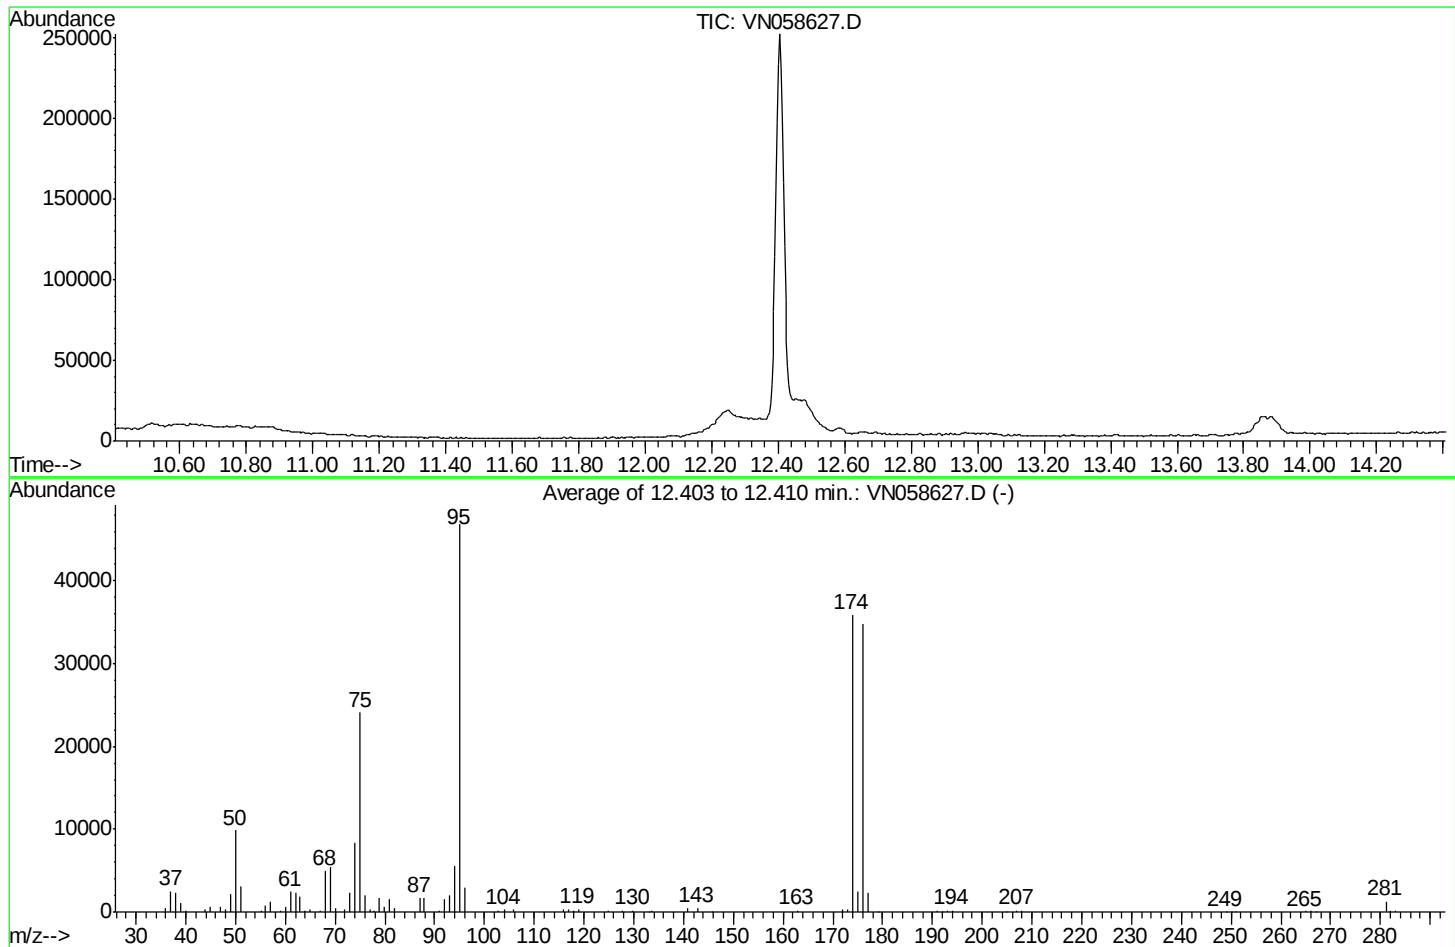

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	9859	PASS
75	95	30	60	51.4	24069	PASS
95	95	100	100	100.0	46834	PASS
96	95	5	9	6.2	2925	PASS
173	174	0.00	2	0.9	311	PASS
174	95	50	100	76.6	35890	PASS
175	174	5	9	7.0	2497	PASS
176	174	95	101	96.8	34738	PASS
177	176	5	9	6.7	2329	PASS