

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100920\
 Data File : VN064069.D
 Acq On : 10 Oct 2020 5:13
 Operator : JC/MD
 Sample : L4319-04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 12018

Quant Time: Oct 10 05:50:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	201505	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	407503	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	420559	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	160647	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	182438	54.80	ug/l	0.00
Spiked Amount			Recovery	=	109.60%	
35) Dibromofluoromethane	7.55	113	133061	47.06	ug/l	0.00
Spiked Amount			Recovery	=	94.12%	
50) Toluene-d8	10.06	98	513270	47.88	ug/l	0.00
Spiked Amount			Recovery	=	95.76%	
62) 4-Bromofluorobenzene	12.38	95	193979	48.14	ug/l	0.00
Spiked Amount			Recovery	=	96.28%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acrolein	3.67	56	66	0.293	ug/l #	14
16) Acetone	3.78	43	45215	44.122	ug/l	95
17) Carbon Disulfide	4.01	76	413	0.775	ug/l #	76
18) Methyl Acetate	4.29	43	4259	1.601	ug/l #	84
20) Methylene Chloride	4.50	84	10808	4.694	ug/l #	85
25) 2-Butanone	6.78	43	1020	0.702	ug/l #	51
29) Tetrahydrofuran	7.15	42	321	0.329	ug/l #	53
31) Cyclohexane	7.63	56	6020	1.558	ug/l #	24
36) 1,1-Dichloropropene	7.62	75	18666	4.521	ug/l #	51
38) Carbon Tetrachloride	7.62	117	22875	4.941	ug/l #	15
43) Isopropyl Acetate	8.13	43	73302	10.835	ug/l	99
45) 1,2-Dichloropropane	9.23	63	964	0.303	ug/l #	44
48) Methyl methacrylate	9.14	41	6037	1.806	ug/l #	30
51) 4-Methyl-2-Pentanone	9.95	43	7483	1.885	ug/l	96
54) cis-1,3-Dichloropropene	9.87	75	29659	5.843	ug/l #	65
56) Ethyl methacrylate	10.51	69	2607	0.629	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	3208	0.648	ug/l #	43
59) 2-Hexanone	10.74	43	54324	18.419	ug/l #	56
71) Bromoform	12.37	173	785	0.310	ug/l #	1
74) N-amyl acetate	12.01	43	3761	2.876	ug/l #	49
76) 1,2,3-Trichloropropane	12.38	75	106246	30.002	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	106246	86.411	ug/l #	6
95) Naphthalene	15.11	128	30	1.928	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100920\
Data File : VN064069.D
Acq On : 10 Oct 2020 5:13
Operator : JC/MD
Sample : L4319-04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
12018

Quant Time: Oct 10 05:50:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

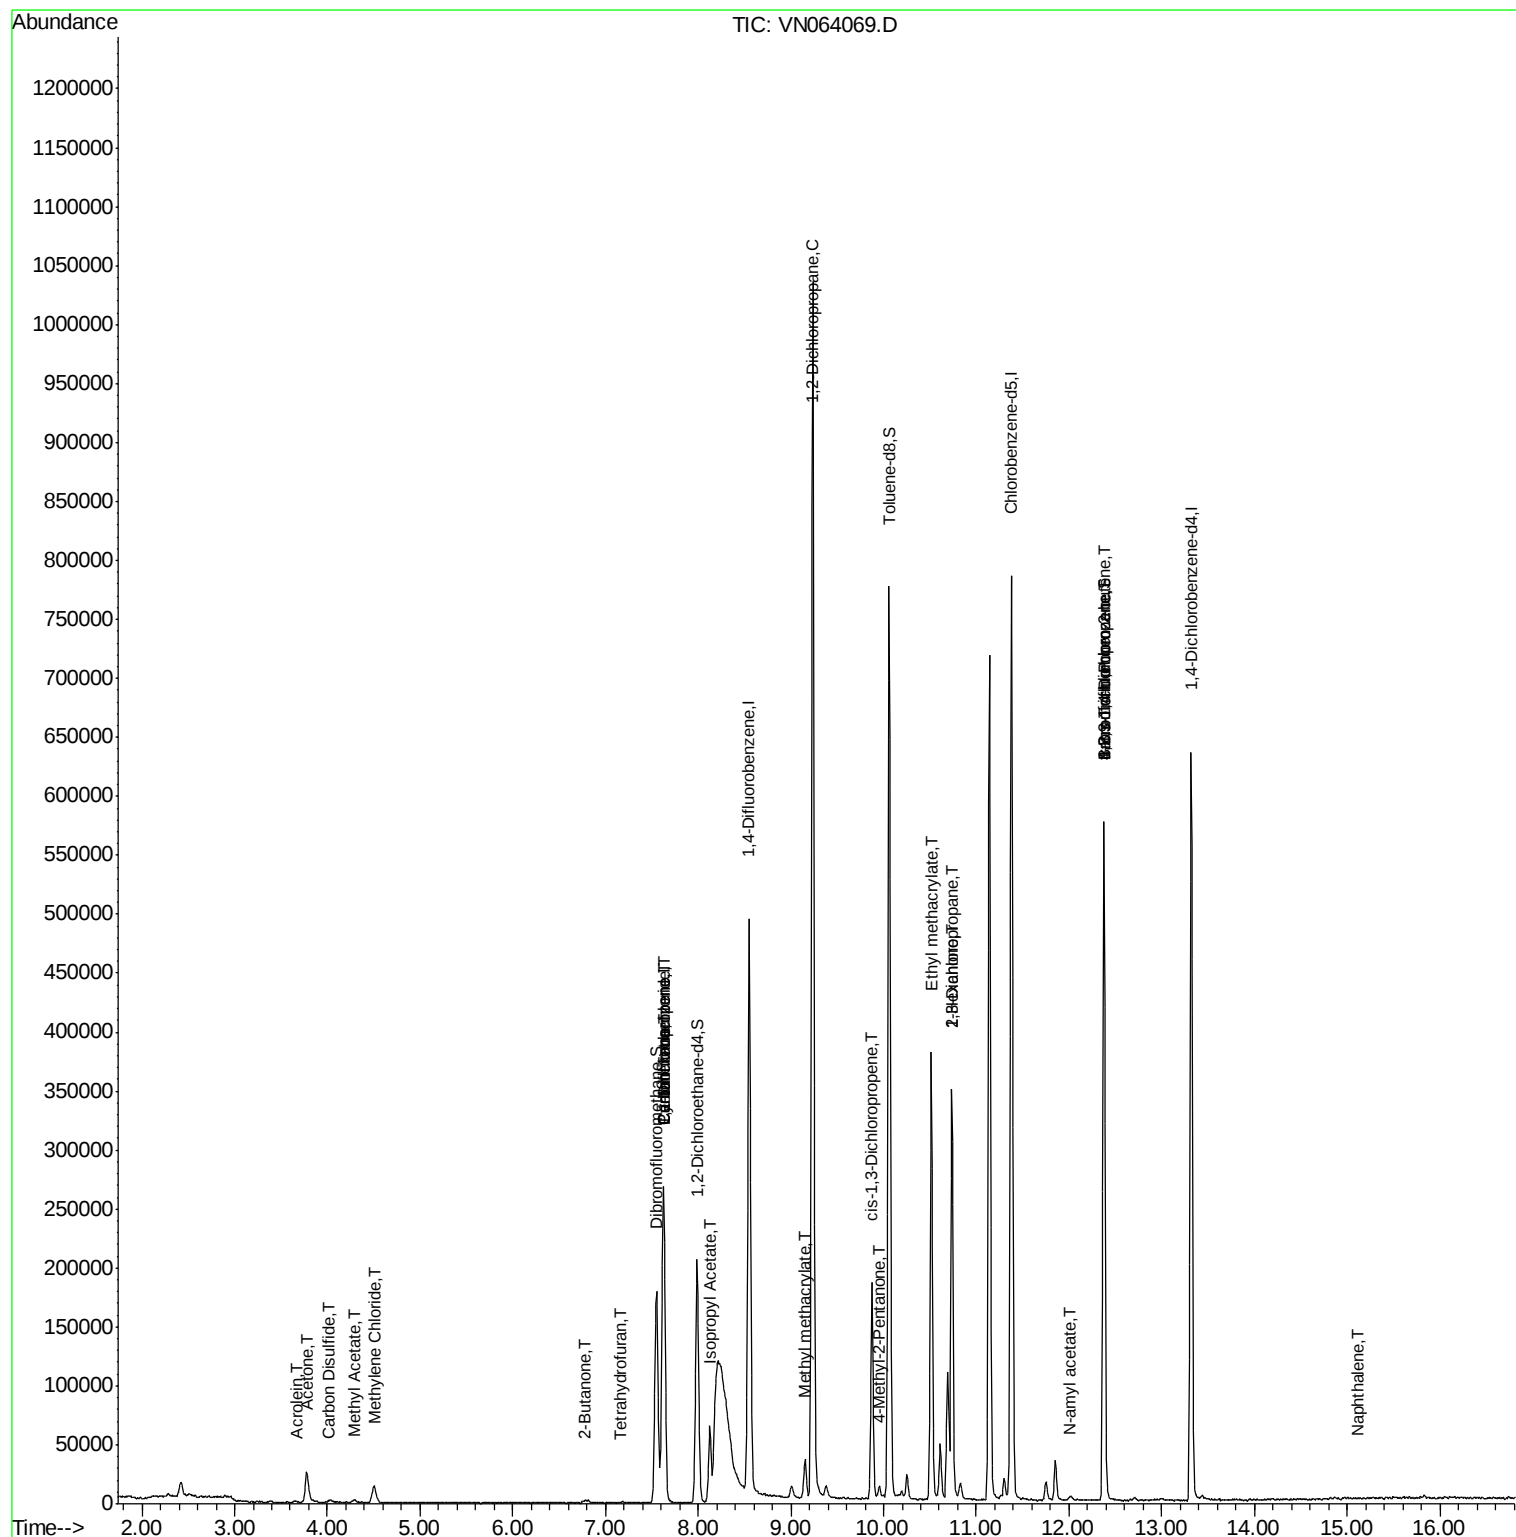

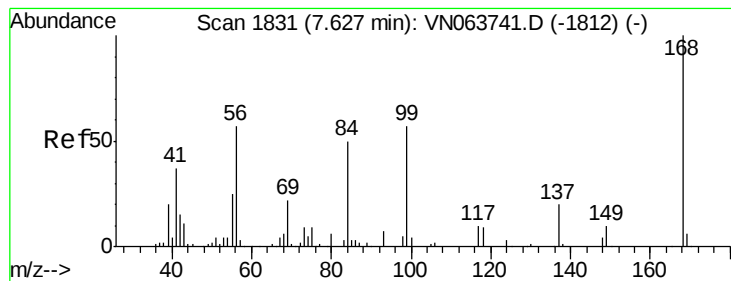

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13


Instrument :
MSVOA_N
ClientSampled :
12018

Tot Ion:168 Resp: 201505

Ion Ratio Lower Upper




168 100

99 62.8 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

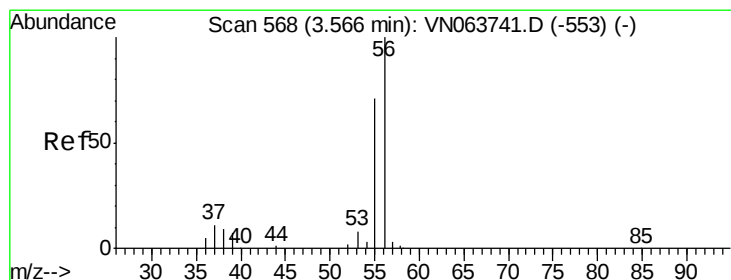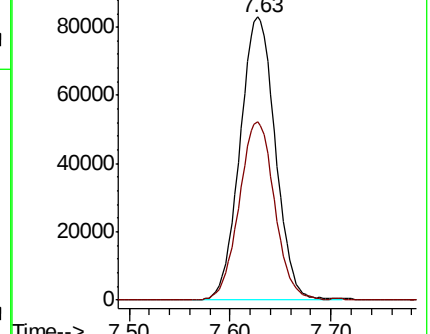

#13

Acrolein

Concen: 0.293 ug/l

RT: 3.67 min Scan# 599

Delta R.T. 0.10 min

Lab File: VN064069.D


Acq: 10 Oct 2020 5:13

Tgt Ion: 56 Resp: 66

Ion Ratio Lower Upper



56 100


55 0.0 56.9 85.3#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

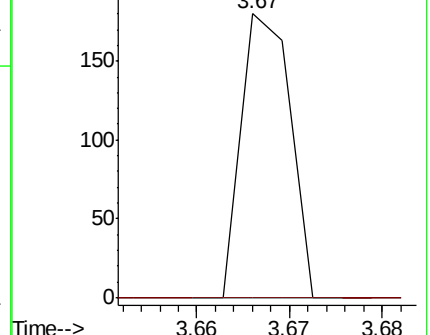



#16

Acetone

Concen: 44.122 ug/l

RT: 3.78 min Scan# 634

Delta R.T. 0.01 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Instrument :

MSVOA_N

ClientSampleId :


12018

Tot Ion: 43 Resp: 45215

Ion Ratio Lower Upper

43 100

58 25.3 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-599) (-)

Ion 58.00 (57.70 to 58.70): VN063741.D (-599) (-)

20000

15000



10000

5000

0

3.70 3.80 3.90

Time-->



#17

Carbon Disulfide

Concen: 0.775 ug/l

RT: 4.01 min Scan# 707

Delta R.T. 0.00 min

Lab File: VN064069.D


Acq: 10 Oct 2020 5:13

Tgt Ion: 76 Resp: 413

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.4#



Abundance Ion 75.90 (75.60 to 76.60): VN063741.D (-685) (-)

Ion 77.90 (77.60 to 78.60): VN063741.D (-685) (-)

400

300


200


100

0

4.00 4.02 4.04

Time-->



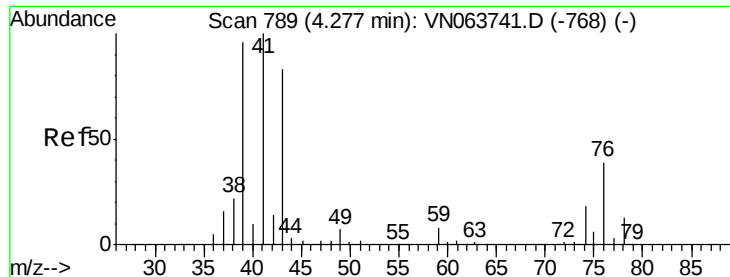

#18

Methvl Acetate

Concen: 1.601 ug/l

RT: 4.29 min Scan# 793

Delta R.T. 0.01 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Instrument :

MSVOA_N


ClientSampleId :
12018

Tot Ion: 43 Resp: 4259

Ion Ratio Lower Upper


43 100

74 14.2 17.4 26.2#


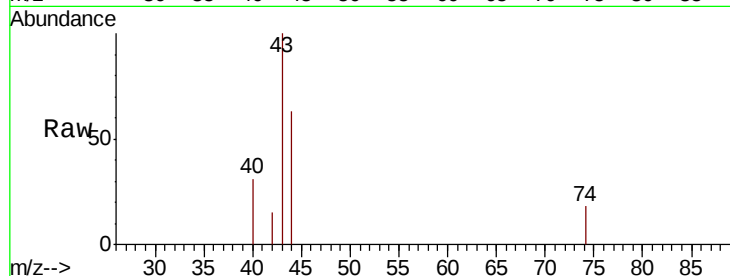


Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-768) (-)

Ion 74.00 (73.70 to 74.70): VN063741.D (-768) (-)

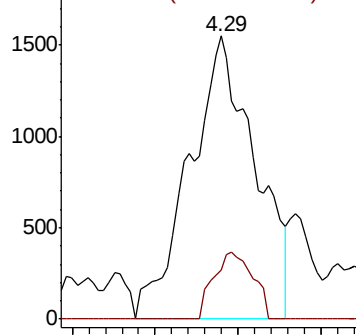

Time-->

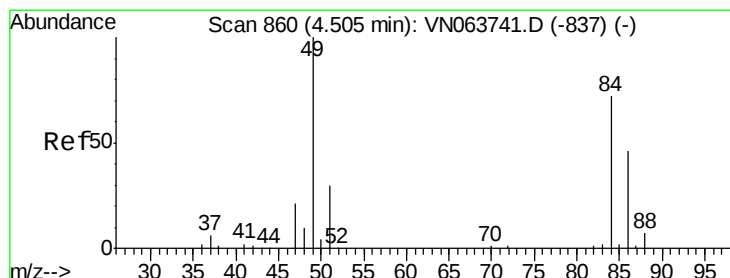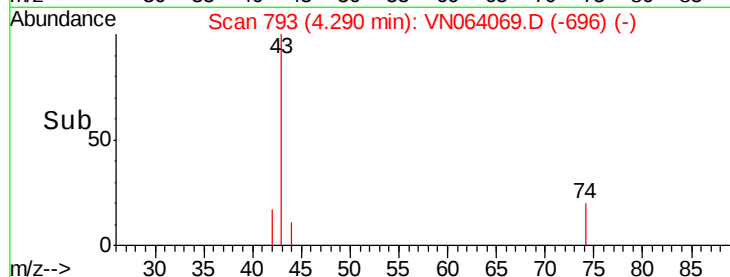

#20

Methylene Chloride

Concen: 4.694 ug/l

RT: 4.50 min Scan# 858

Delta R.T. -0.01 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Tgt Ion: 84 Resp: 10808


Ion Ratio Lower Upper

84 100

49 122.7 110.4 165.6

51 31.1 33.3 49.9#

86 50.0 50.7 76.1#

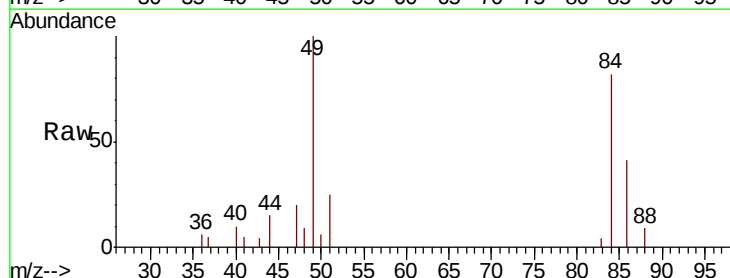


Abundance Ion 83.90 (83.60 to 84.60): VN063741.D (-837) (-)


Ion 48.90 (48.60 to 49.60): VN063741.D (-837) (-)


Ion 50.90 (50.60 to 51.60): VN063741.D (-837) (-)

Ion 85.90 (85.60 to 86.60): VN063741.D (-837) (-)

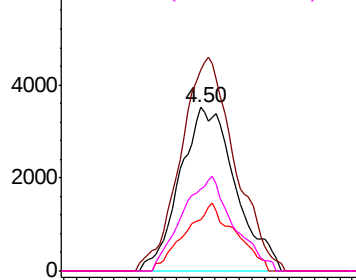

Time-->

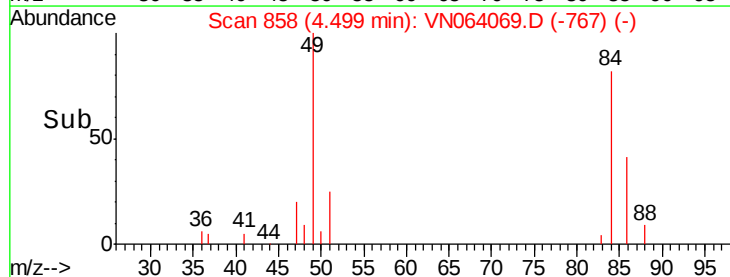

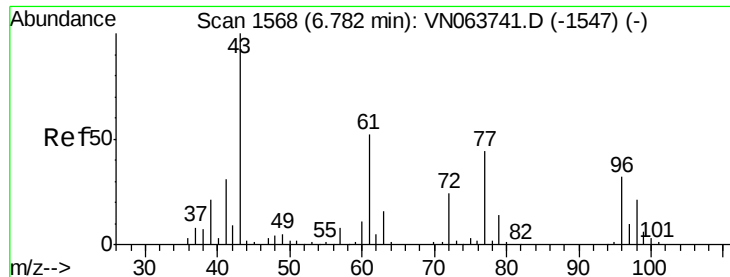

#25

2-Butanone

Concen: 0.702 ug/l

RT: 6.78 min Scan# 1568

Delta R.T. 0.00 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Instrument :

MSVOA_N


ClientSampled :
12018

Tot Ion: 43 Resp: 1020

Ion Ratio Lower Upper




43 100

72 0.0 19.3 28.9#

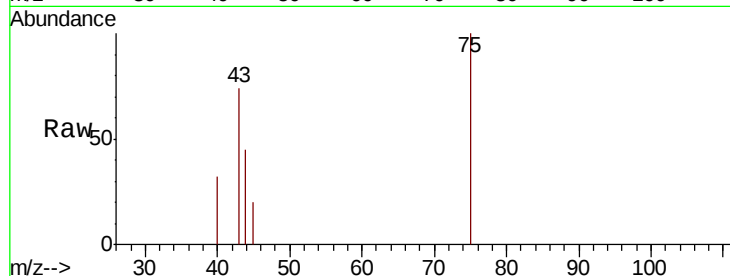

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

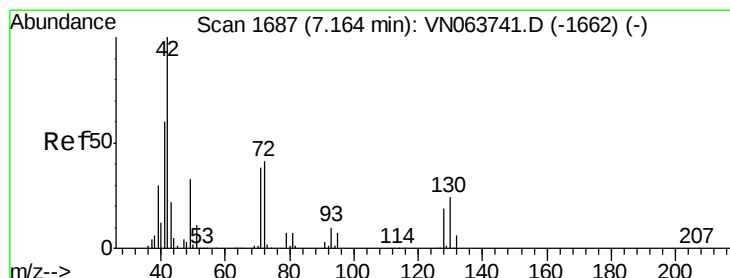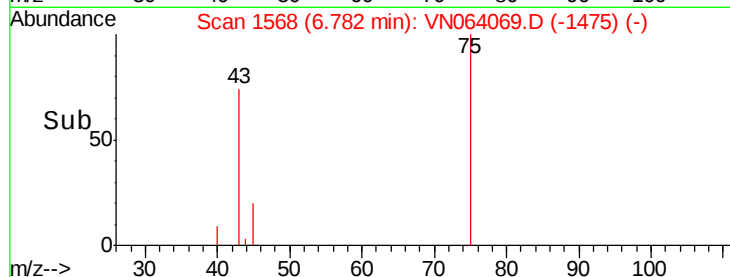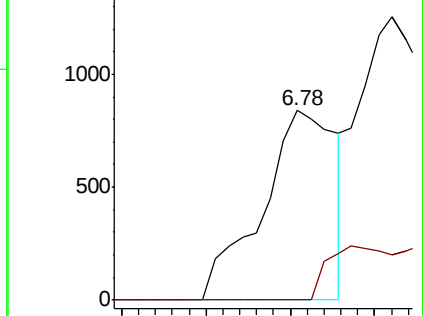

#29

Tetrahydrofuran

Concen: 0.329 ug/l

RT: 7.15 min Scan# 1684

Delta R.T. -0.01 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13


Tgt Ion: 42 Resp: 321

Ion Ratio Lower Upper

42 100

72 21.5 32.8 49.2#



71 0.0 30.6 45.8#

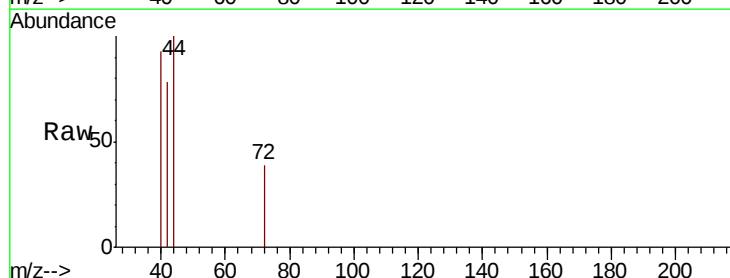


Abundance Ion 42.00 (41.70 to 42.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

Ion 71.00 (70.70 to 71.70): VN0

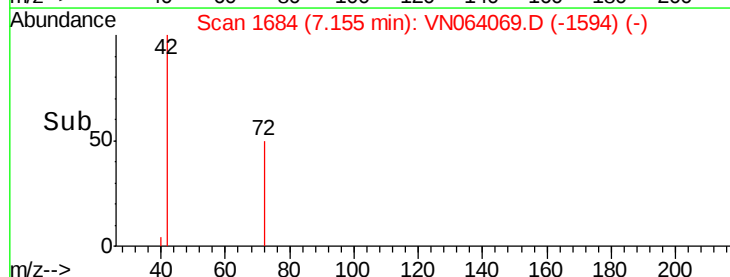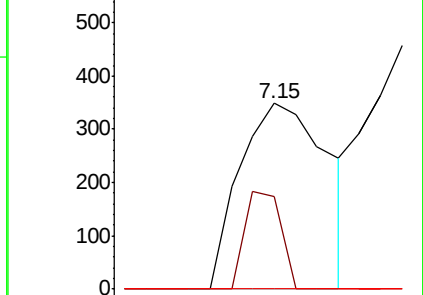


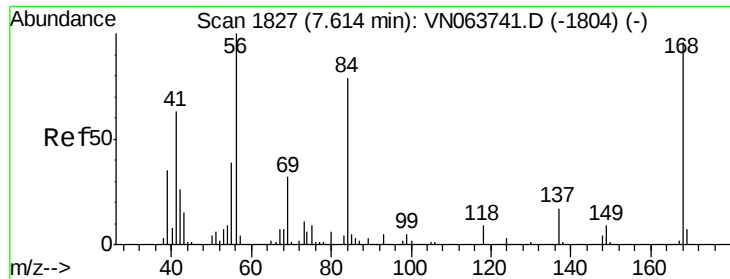




#31
Cyclohexane
Concen: 1.558 ug/l
RT: 7.63 min Scan# 1832
Delta R.T. 0.02 min
Lab File: VN064069.D
Acq: 10 Oct 2020 5:13

Instrument :
MSVOA_N
ClientSampled :
12018

Tot Ion: 56 Resp: 6020
Ion Ratio Lower Upper
56 100
69 160.6 25.4 38.2#
84 91.2 63.3 94.9

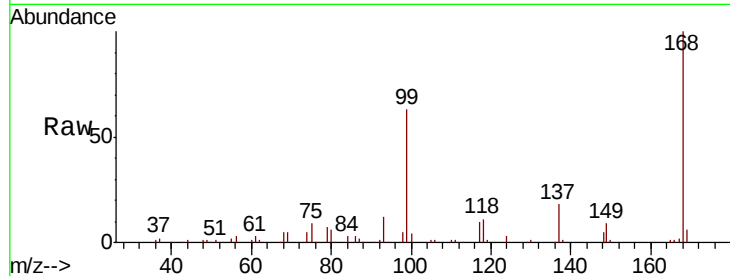


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0

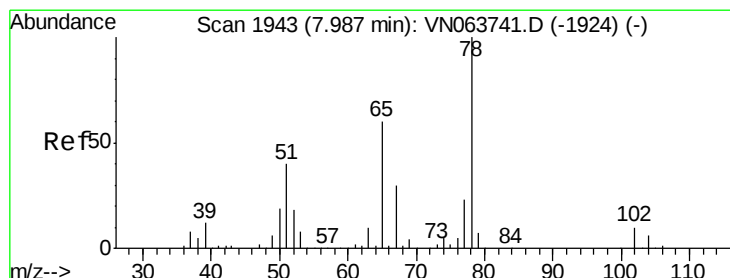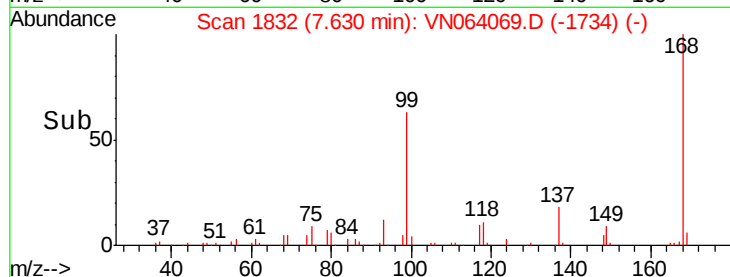
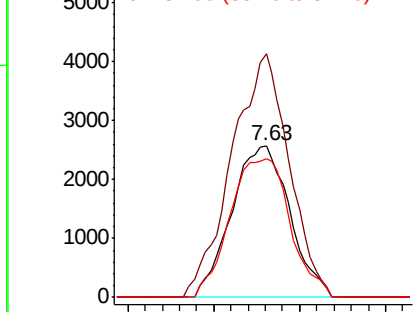



#33
1,2-Dichloroethane-d4
Concen: 54.803 ug/l
RT: 7.99 min Scan# 1943
Delta R.T. 0.00 min
Lab File: VN064069.D
Acq: 10 Oct 2020 5:13

Tgt Ion: 65 Resp: 182438
Ion Ratio Lower Upper
65 100
67 50.6 0.0 99.6

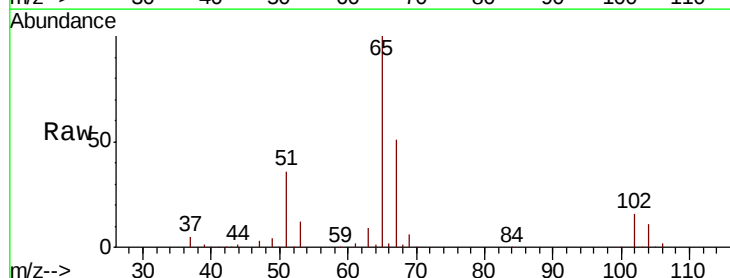

Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

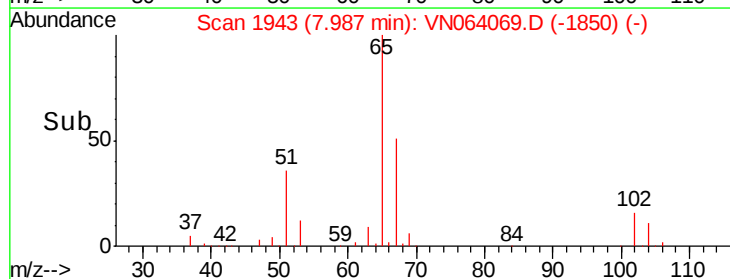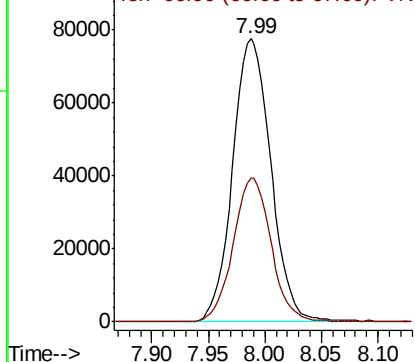



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. 0.00 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Instrument :

MSVOA_N

ClientSampleId :
12018


Tot Ion:114 Resp: 407503

Ion Ratio Lower Upper




114 100

63 23.2 0.0 45.0

88 16.2 0.0 34.0



Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN

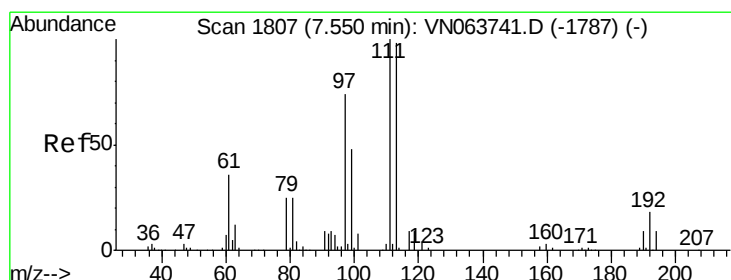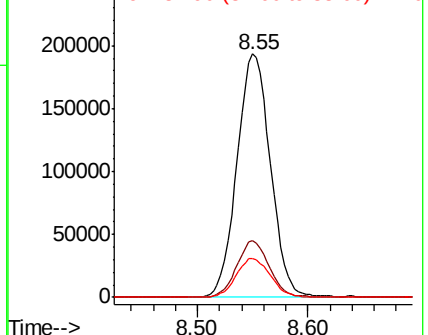

#35

Dibromofluoromethane

Concen: 47.058 ug/l

RT: 7.55 min Scan# 1807

Delta R.T. 0.00 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13


Tgt Ion:113 Resp: 133061

Ion Ratio Lower Upper



113 100


111 104.1 81.8 122.8

192 18.5 14.2 21.2



Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

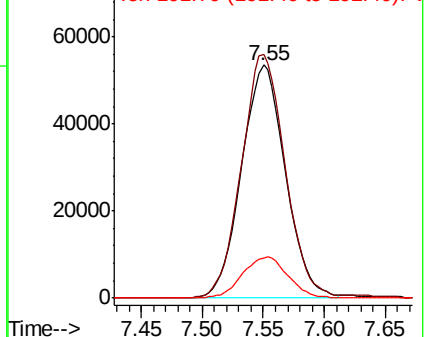







#36
 1,1-Dichloropropene
 Concen: 4.521 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.13 min
 Lab File: VN064069.D
 Acq: 10 Oct 2020 5:13

Instrument :
 MSVOA_N
 ClientSampled :
 12018

Tot Ion	Ratio	Lower	Upper
75	100		
110	8.9	16.9	50.6#
77	0.0	24.5	36.7#

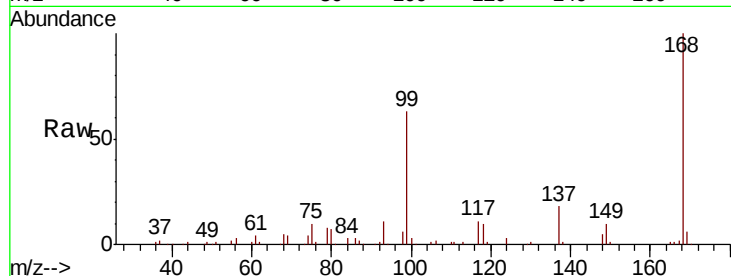


Abundance Ion 74.90 (74.60 to 75.60): VN0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VN0


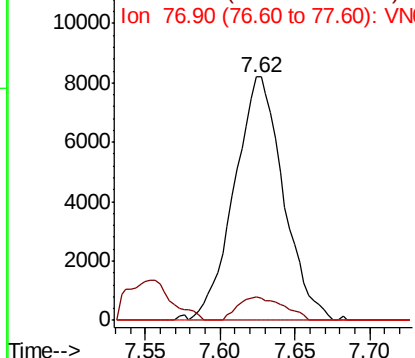



#38
 Carbon Tetrachloride
 Concen: 4.941 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.11 min
 Lab File: VN064069.D
 Acq: 10 Oct 2020 5:13

Tgt Ion	Ratio	Lower	Upper
117	100		
119	6.7	80.1	120.1#
121	0.0	25.7	38.5#



Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V

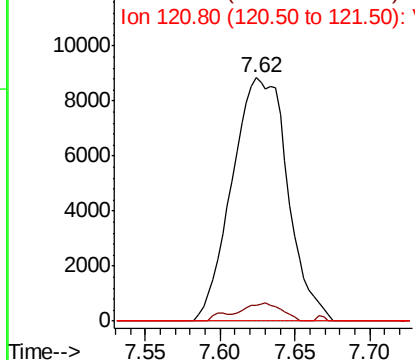







#43

Isopropyl Acetate
 Concen: 10.835 ug/l
 RT: 8.13 min Scan# 1986
 Delta R.T. 0.00 min
 Lab File: VN064069.D
 Acq: 10 Oct 2020 5:13

Instrument :
 MSVOA_N
 ClientSampleId :
 12018




Tot Ion	43	61	87
Resp:	73302		
Ion Ratio	100	18.1	11.8
Lower		14.2	9.0
Upper		21.4	13.6

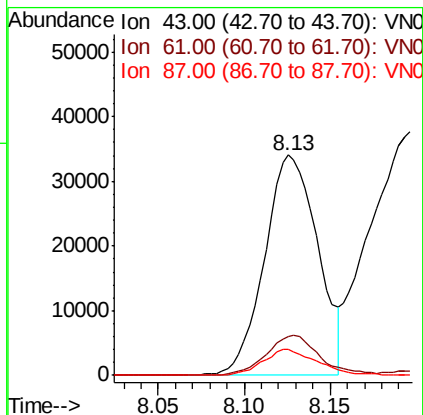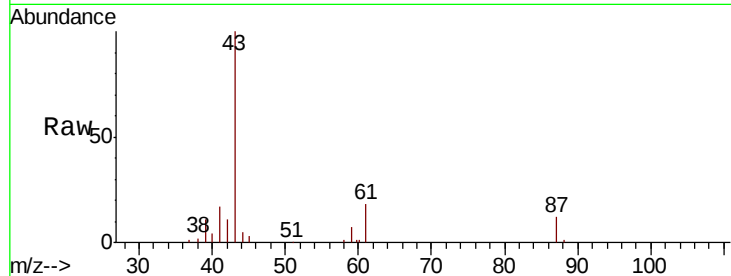


#45

1,2-Dichloropropane
 Concen: 0.303 ug/l
 RT: 9.23 min Scan# 2330
 Delta R.T. 0.15 min
 Lab File: VN064069.D
 Acq: 10 Oct 2020 5:13

Tgt Ion	63	65
Resp:	964	
Ion Ratio	100	0.0
Lower		24.7
Upper		37.1#

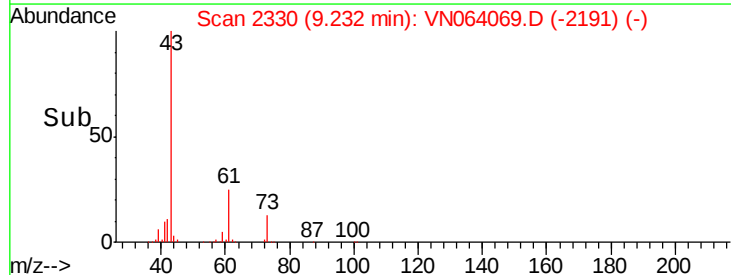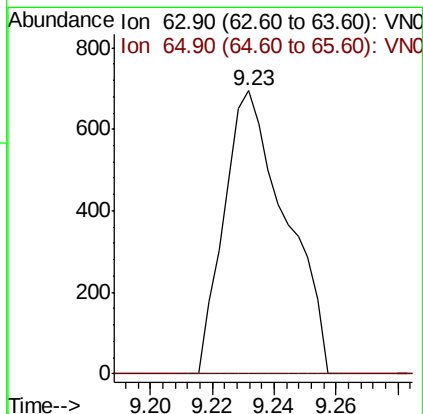







#48
Methvl methacrylate
Concen: 1.806 ug/l
RT: 9.14 min Scan# 2302
Delta R.T. -0.03 min
Lab File: VN064069.D
Acq: 10 Oct 2020 5:13

Instrument :
MSVOA_N
ClientSampleId :
12018

Tot Ion: 41 Resp: 6037
Ion Ratio Lower Upper
41 100
69 0.0 60.9 91.3#
39 29.7 57.5 86.3#




Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0

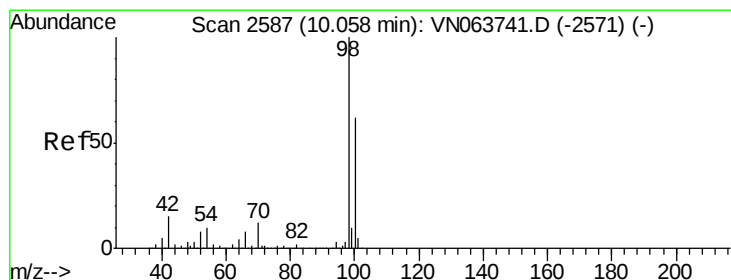
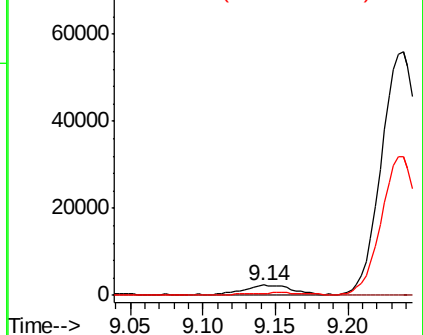



#50
Toluene-d8
Concen: 47.884 ug/l
RT: 10.06 min Scan# 2588
Delta R.T. 0.00 min
Lab File: VN064069.D
Acq: 10 Oct 2020 5:13

Tgt Ion: 98 Resp: 513270
Ion Ratio Lower Upper
98 100
100 63.6 49.8 74.6

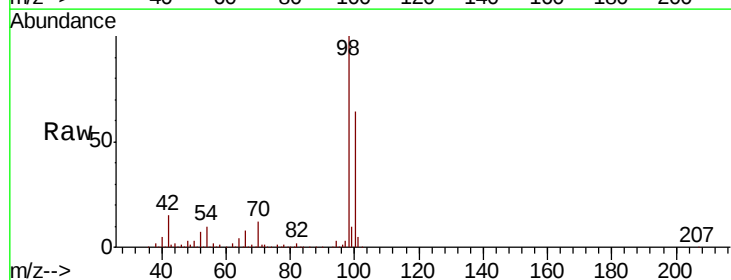

Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0

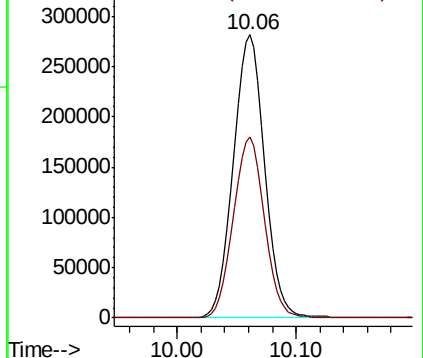



#51

4-Methyl-2-Pentanone

Concen: 1.885 ug/l

RT: 9.95 min Scan# 2553

Delta R.T. -0.00 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Instrument :

MSVOA_N


ClientSampled :
12018

Tot Ion: 43 Resp: 7483

Ion Ratio Lower Upper




43 100

58 37.7 28.4 42.6



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-2537) (-)

Ion 58.00 (57.70 to 58.70): VN063741.D (-2537) (-)

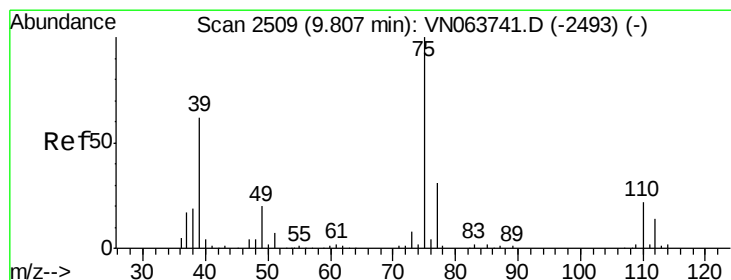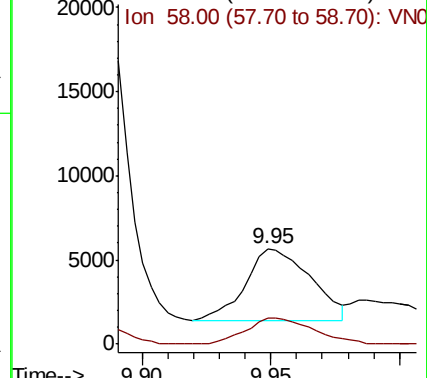

#54

cis-1,3-Dichloropropene

Concen: 5.843 ug/l

RT: 9.87 min Scan# 2530

Delta R.T. 0.07 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13


Tgt Ion: 75 Resp: 29659

Ion Ratio Lower Upper

75 100

77 0.0 24.6 36.8#



39 43.3 49.7 74.5#




Abundance Ion 74.90 (74.60 to 75.60): VN063741.D (-2493) (-)

Ion 76.90 (76.60 to 77.60): VN063741.D (-2493) (-)

Ion 39.00 (38.70 to 39.70): VN063741.D (-2493) (-)

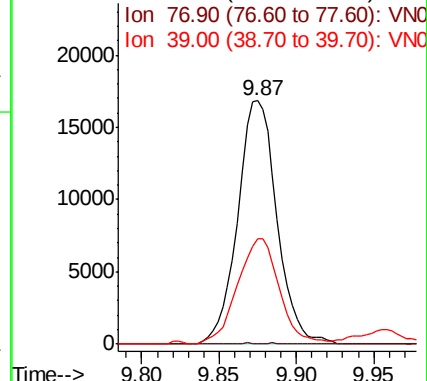



#56

Ethyl methacrylate

Concen: 0.629 ug/l

RT: 10.51 min Scan# 2729

Delta R.T. 0.12 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Instrument :

MSVOA_N

ClientSampled :
12018


Tot Ion: 69 Resp: 2607

Ion Ratio Lower Upper




69 100

41 3060.6 61.1 91.7#

39 1347.3 42.2 63.4#

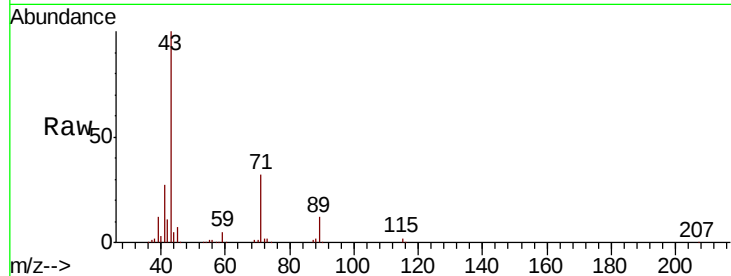

Abundance Ion 69.00 (68.70 to 69.70): VN0
Ion 41.00 (40.70 to 41.70): VN0
Ion 39.00 (38.70 to 39.70): VN0

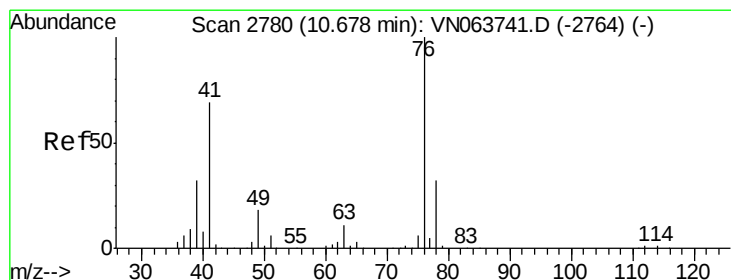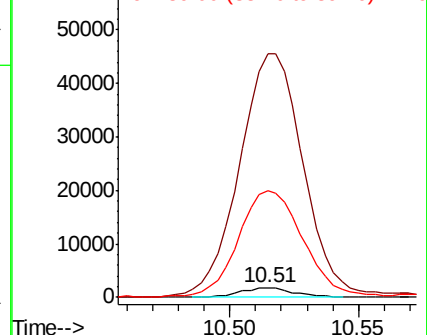

#57

1,3-Dichloropropane

Concen: 0.648 ug/l

RT: 10.74 min Scan# 2799

Delta R.T. 0.06 min

Lab File: VN064069.D


Acq: 10 Oct 2020 5:13

Tgt Ion: 76 Resp: 3208



Ion Ratio Lower Upper


76 100

78 0.0 25.2 37.8#



Abundance Ion 75.90 (75.60 to 76.60): VN0
Ion 77.90 (77.60 to 78.60): VN0




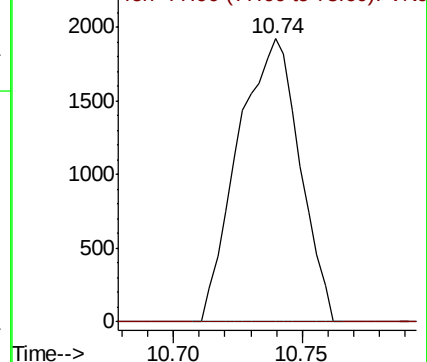




#59
2-Hexanone
Concen: 18.419 ug/l
RT: 10.74 min Scan# 2798
Delta R.T. 0.02 min
Lab File: VN064069.D
Acq: 10 Oct 2020 5:13




Instrument :
MSVOA_N
ClientSampled :
12018


Tot Ion: 43 Resp: 54324
Ion Ratio Lower Upper
43 100
58 19.2 24.6 73.8#

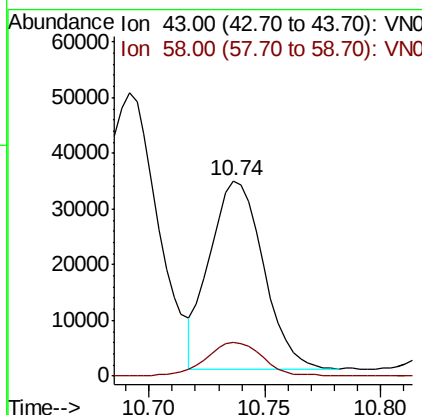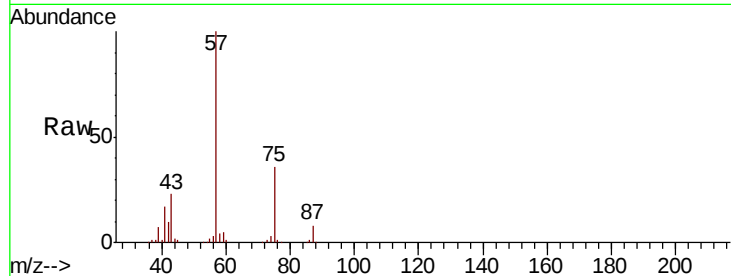

#62
4-Bromofluorobenzene
Concen: 48.141 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN064069.D
Acq: 10 Oct 2020 5:13

Tgt Ion: 95 Resp: 193979
Ion Ratio Lower Upper
95 100
174 74.9 0.0 150.6
176 71.2 0.0 145.4

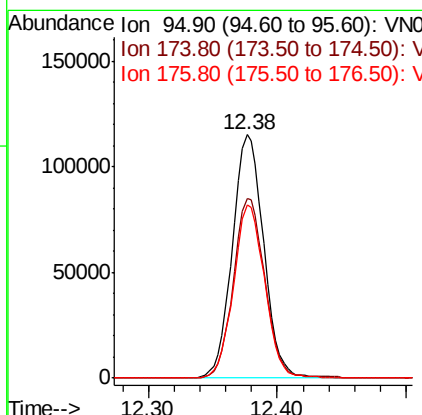







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN064069.D
Acq: 10 Oct 2020 5:13

Instrument :
MSVOA_N
ClientSampled :
12018

Tot Ion:117 Resp: 420559
Ion Ratio Lower Upper
117 100
82 60.7 47.4 71.2
119 31.6 26.4 39.6

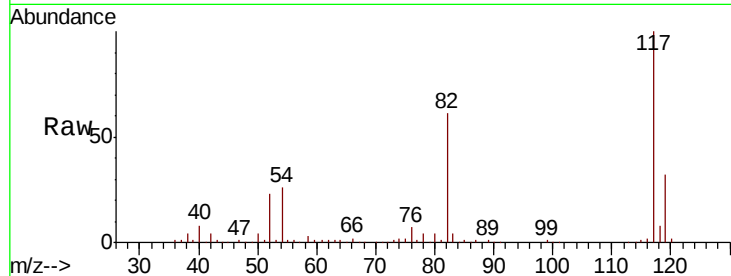


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V


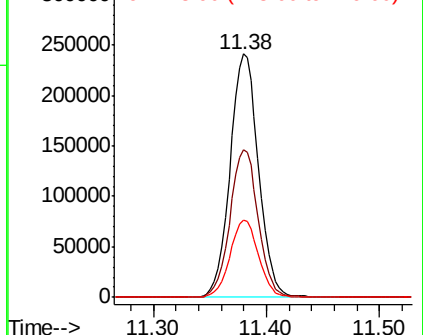



#71
Bromoform
Concen: 0.310 ug/l
RT: 12.37 min Scan# 3307
Delta R.T. 0.27 min
Lab File: VN064069.D
Acq: 10 Oct 2020 5:13

Tgt Ion:173 Resp: 785
Ion Ratio Lower Upper
173 100
175 1180.8 23.5 70.5#
254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

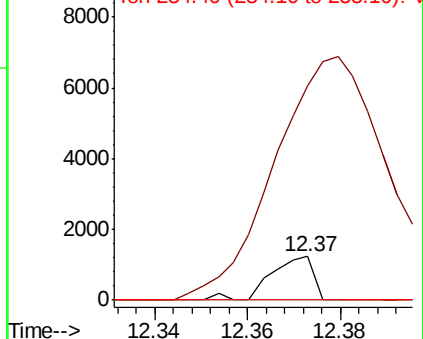



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Instrument :

MSVOA_N

ClientSampleId :
12018


Tot Ion:152 Resp: 160647

Ion Ratio Lower Upper




152 100

115 62.6 31.3 93.8

150 156.8 0.0 341.8

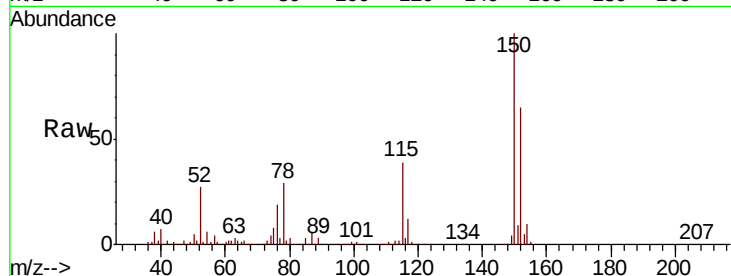

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

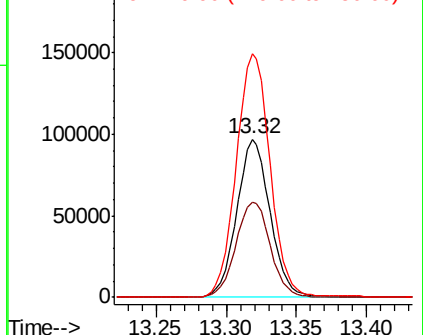

#74

N-ethyl acetate

Concen: 2.876 ug/l

RT: 12.01 min Scan# 3193

Delta R.T. -0.04 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Tgt Ion: 43 Resp: 3761


Ion Ratio Lower Upper

43 100



70 0.0 29.8 44.8#


55 4.9 17.9 26.9#

61 0.0 17.0 25.4#



Abundance Ion 43.00 (42.70 to 43.70): V
Ion 70.00 (69.70 to 70.70): V
Ion 55.00 (54.70 to 55.70): V
Ion 61.00 (60.70 to 61.70): V

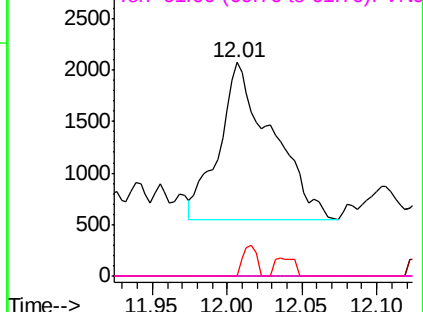



#76

1,2,3-Trichloropropane

Concen: 30.002 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Instrument :

MSVOA_N





ClientSampled :
12018

Tot Ion: 75 Resp: 106246

Ion Ratio Lower Upper

75 100

77 1.0 0.0 0.0#

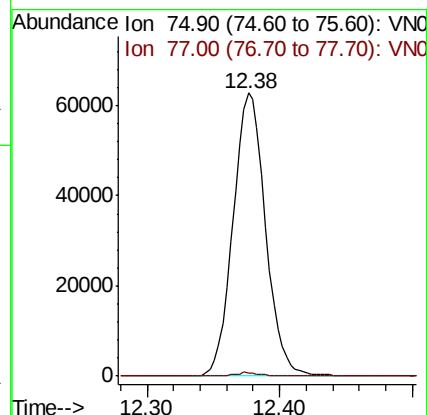

#81

trans-1,4-Dichloro-2-butene

Concen: 86.411 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064069.D

Acq: 10 Oct 2020 5:13




Tgt Ion: 75 Resp: 106246


Ion Ratio Lower Upper

75 100

53 0.0 88.2 132.2#

89 0.0 36.0 54.0#

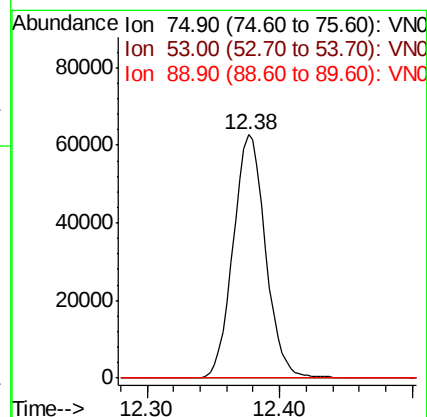

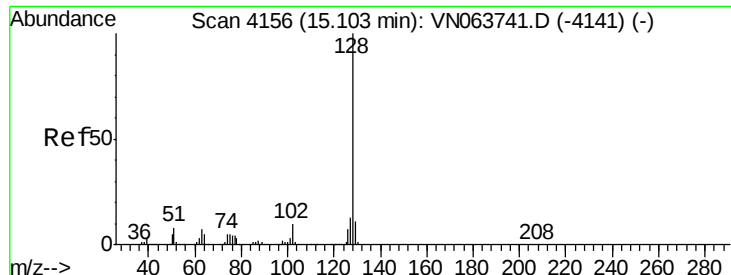

#95

Naphthalene

Concen: 1.928 ug/l

RT: 15.11 min Scan# 4158

Delta R.T. 0.01 min


Lab File: VN064069.D

Acq: 10 Oct 2020 5:13

Instrument :

MSVOA_N

ClientSampleId :
12018




Tot Ion:128 Resp: 30

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

