

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100920\
 Data File : VN064039.D
 Acq On : 9 Oct 2020 15:39
 Operator : JC/MD
 Sample : L4301-03
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WGGM-20-WW-TSF-034

Quant Time: Oct 10 01:56:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N100620W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Tue Oct 06 16:42:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.15	128	43353	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.55	114	217907	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.38	117	205537	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	7.99	65	118476	30.43	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	101.43%
60) 4-Bromofluorobenzene	12.38	95	81580	23.21	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	77.37%
63) Toluene-d8	10.06	98	273621	29.38	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	97.93%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100920\
Data File : VN064039.D
Acq On : 9 Oct 2020 15:39
Operator : JC/MD
Sample : L4301-03
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WGGM-20-WW-TSF-034

Quant Time: Oct 10 01:56:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N100620W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Tue Oct 06 16:42:38 2020
Response via : Initial Calibration

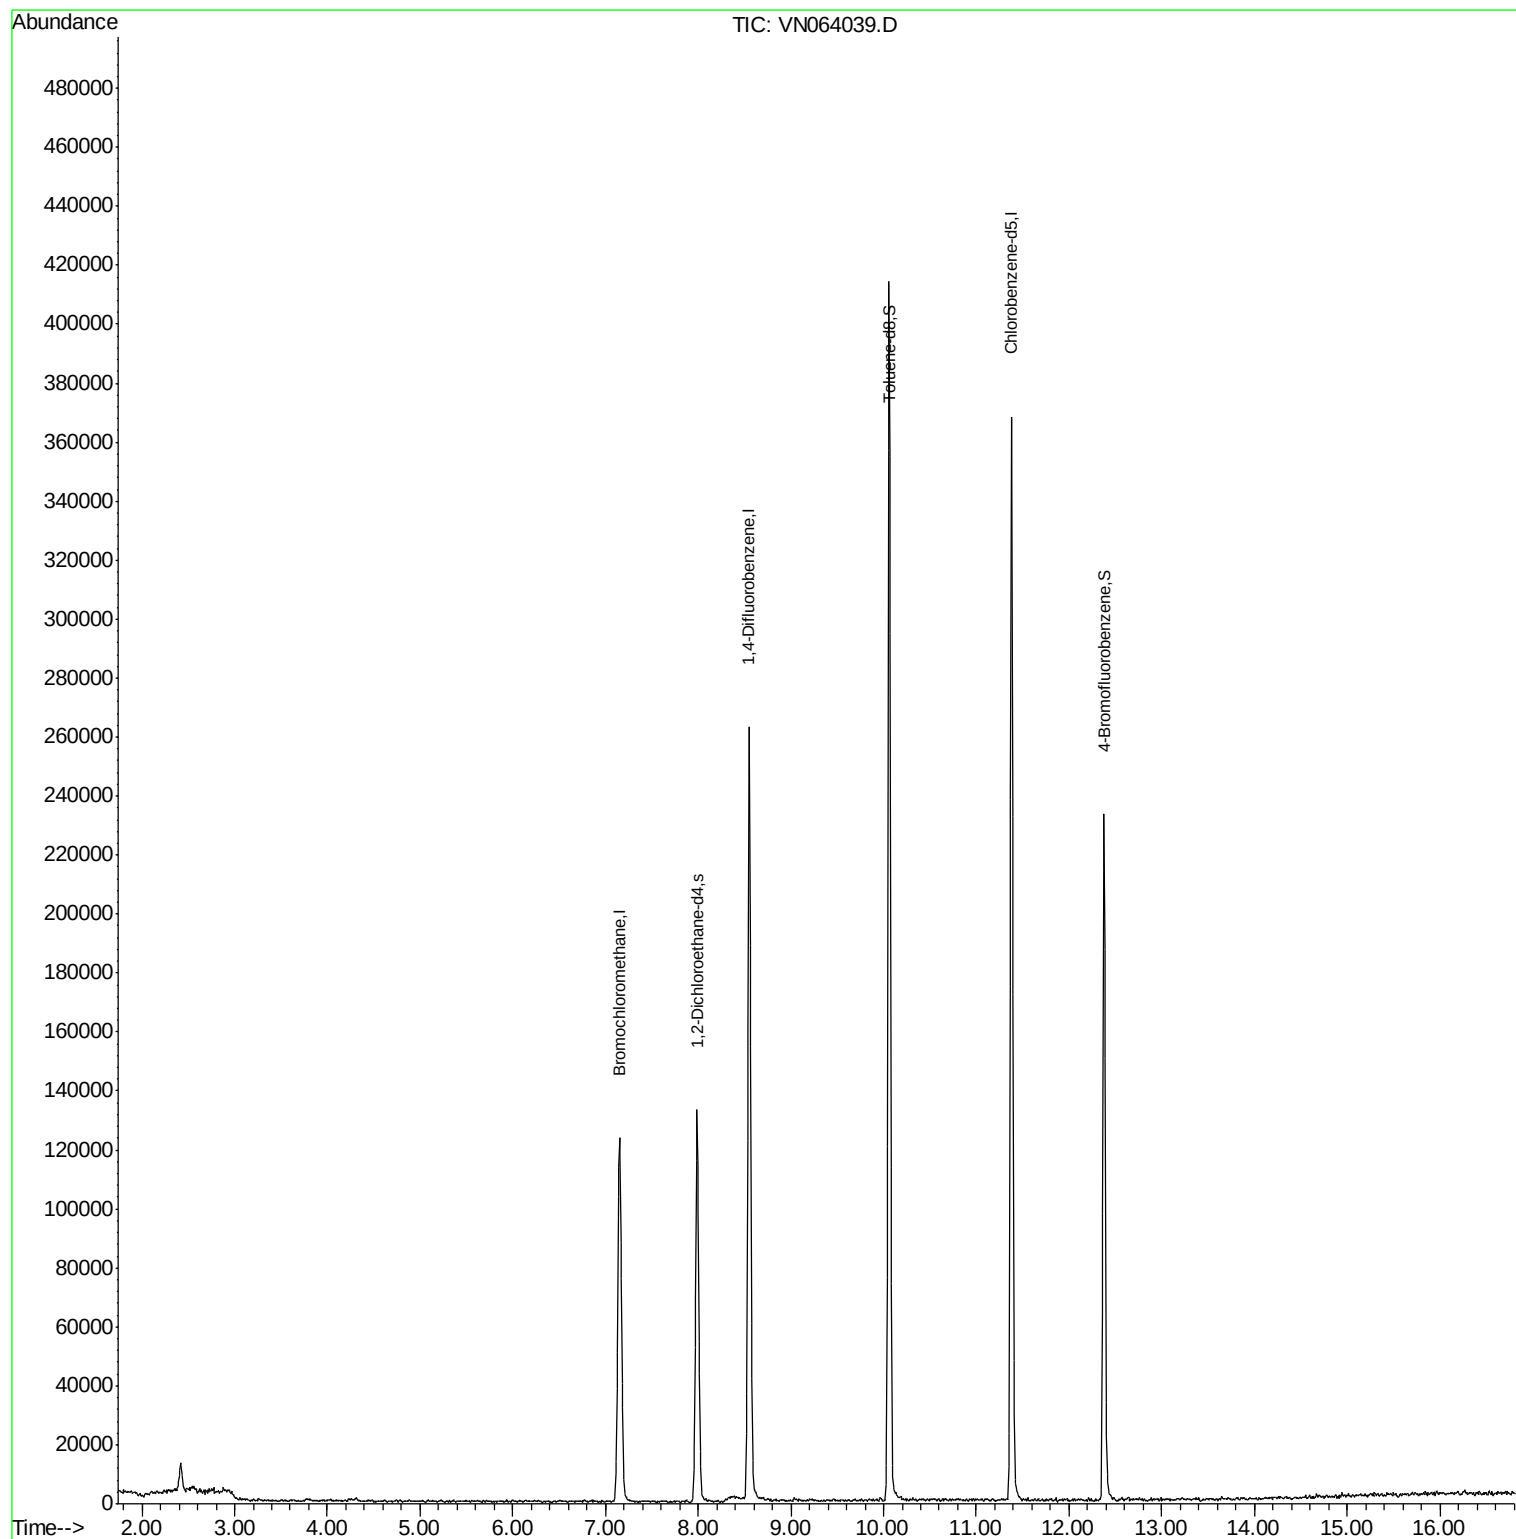

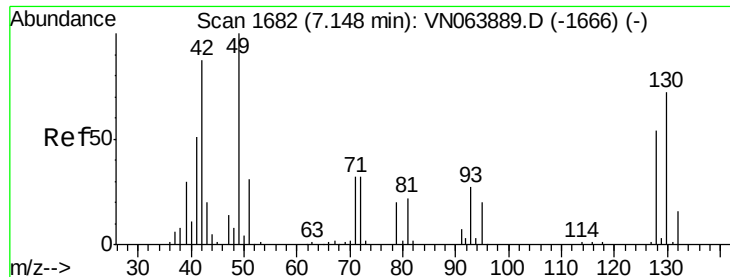

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 7.15 min Scan# 1684

Delta R.T. 0.00 min

Lab File: VN064039.D

Acq: 9 Oct 2020 15:39

Instrument :

MSVOA_N

ClientSampleId :

WGGM-20-WW-TSF-034


Tot Ion:128 Resp: 43353

Ion Ratio Lower Upper

128 100

49 196.6 0.0 437.5


130 130.9 0.0 327.3

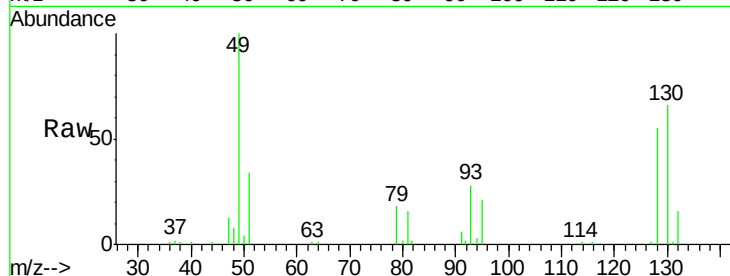



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VN0

Ion 130.00 (129.70 to 130.70): V

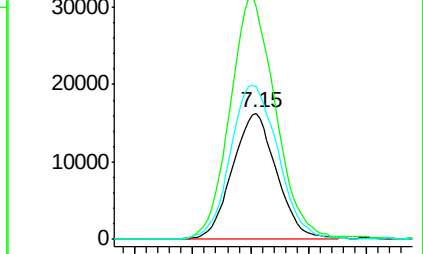

Time-->

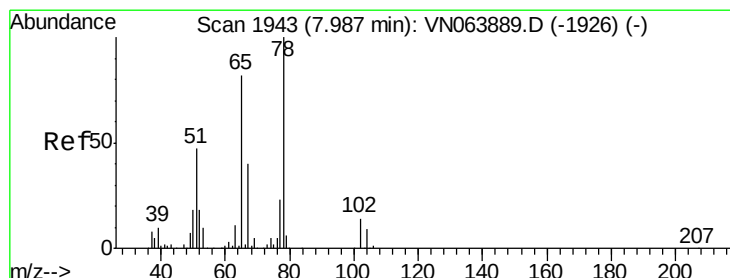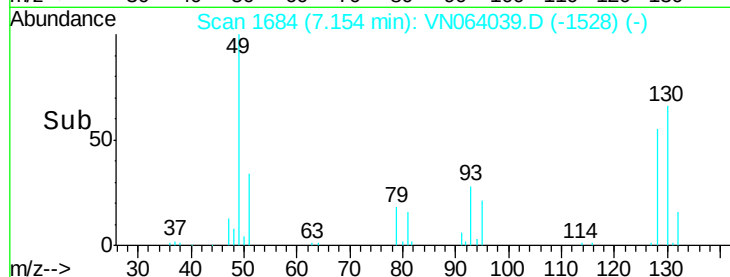

#27

1,2-Dichloroethane-d4

Concen: 30.429 ug/l

RT: 7.99 min Scan# 1943

Delta R.T. -0.00 min

Lab File: VN064039.D


Acq: 9 Oct 2020 15:39

Tgt Ion: 65 Resp: 118476

Ion Ratio Lower Upper


65 100

67 50.9 43.8 65.6

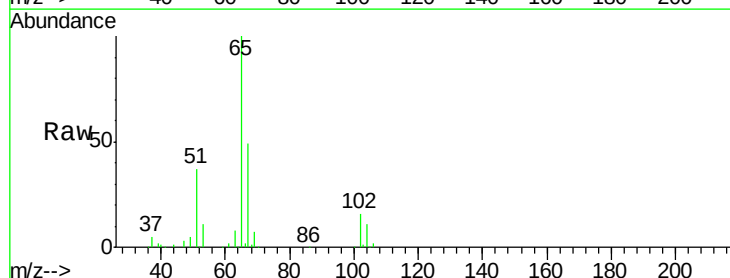



Abundance Ion 65.00 (64.70 to 65.70): VN0

Ion 67.00 (66.70 to 67.70): VN0

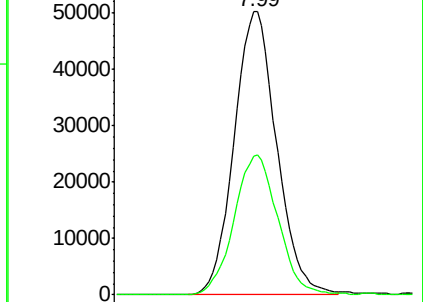

Time-->




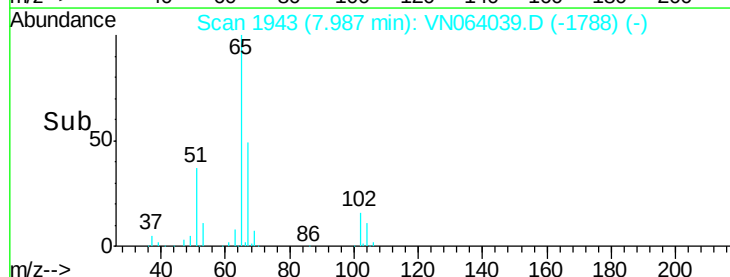


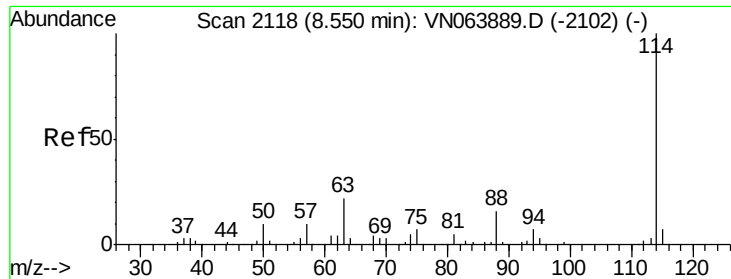

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 8.55 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN064039.D
 Acq: 9 Oct 2020 15:39




Instrument :
 MSVOA_N
 ClientSampleId :
 WGM-20-WW-TSF-034


Tot Ion:114 Resp: 217907
 Ion Ratio Lower Upper
 114 100
 63 23.5 17.0 25.6
 88 16.7 12.6 18.8

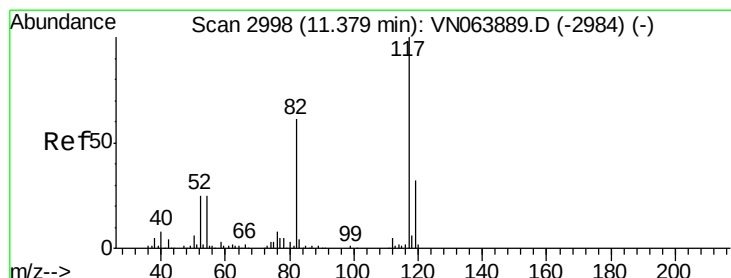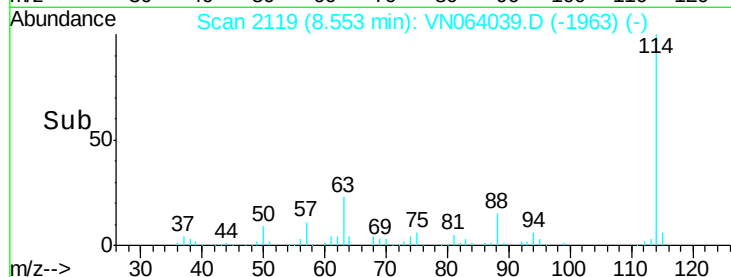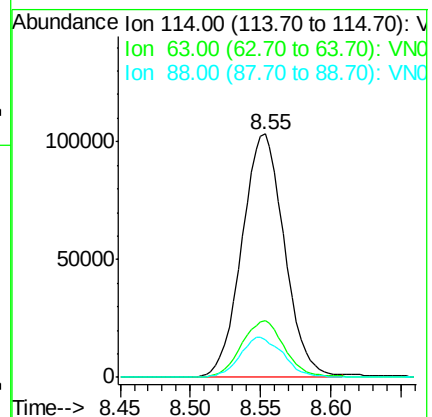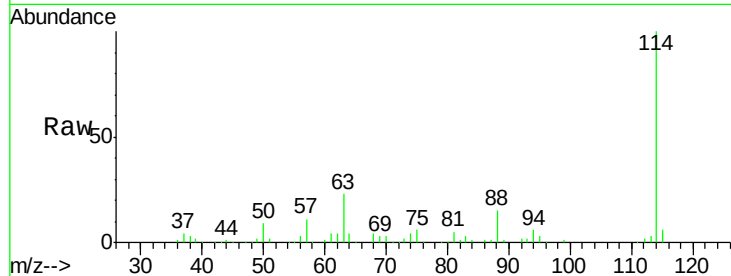

#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 11.38 min Scan# 2999
 Delta R.T. 0.00 min
 Lab File: VN064039.D
 Acq: 9 Oct 2020 15:39

Tgt Ion:117 Resp: 205537
 Ion Ratio Lower Upper
 117 100
 82 59.5 44.9 67.3
 119 31.3 26.0 39.0


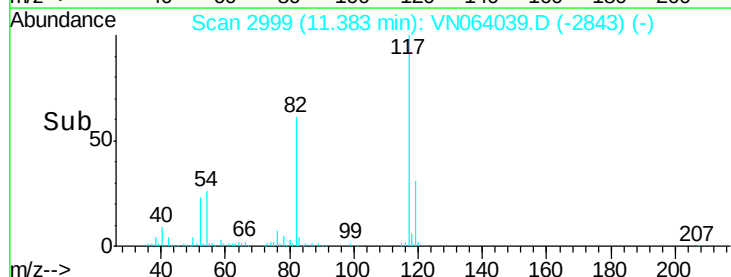
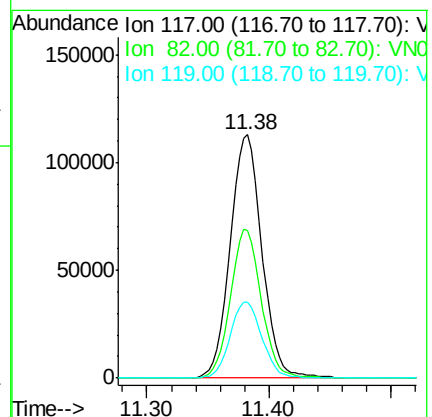
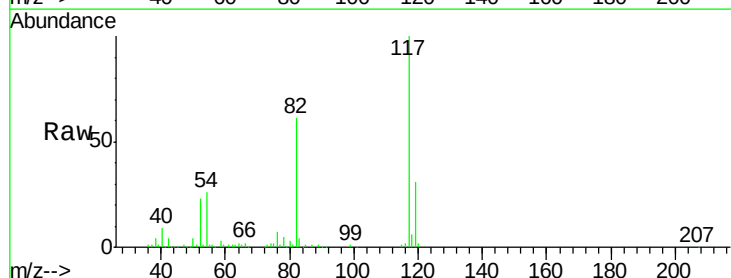


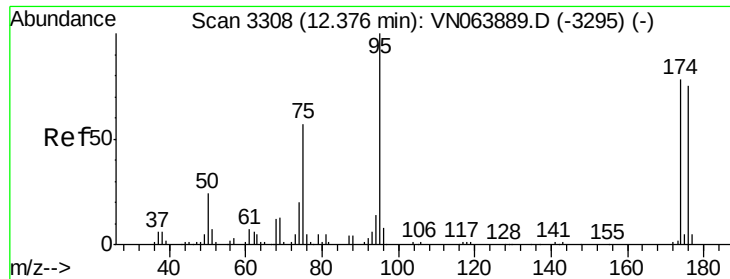

#60
4-Bromofluorobenzene
Concen: 23.210 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. -0.00 min
Lab File: VN064039.D
Acq: 9 Oct 2020 15:39

Instrument :
MSVOA_N
ClientSampleId :
WGGM-20-WW-TSF-034

Tot Ion: 95 Resp: 81580
Ion Ratio Lower Upper
95 100
174 76.0 70.1 105.1
176 71.1 66.8 100.2

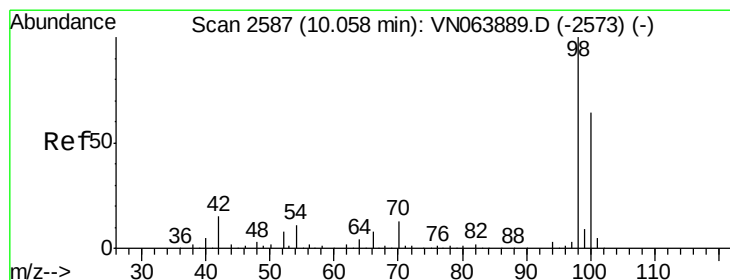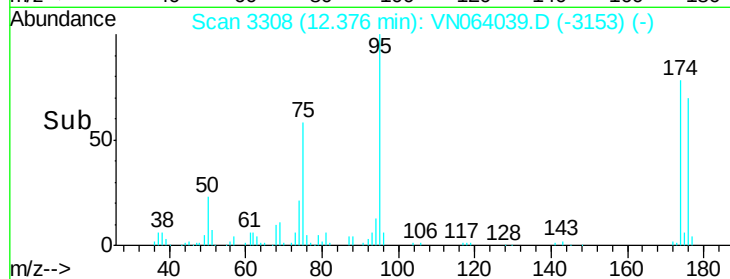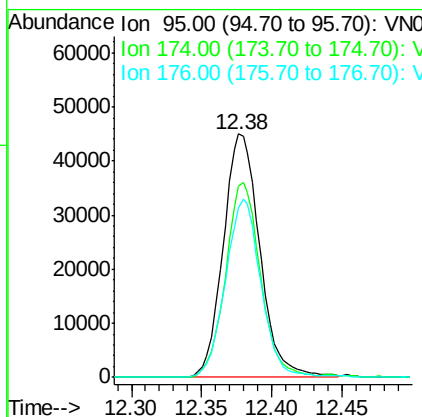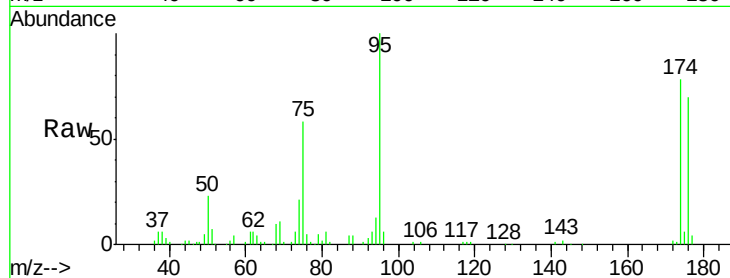

#63
Toluene-d8
Concen: 29.375 ug/l
RT: 10.06 min Scan# 2588
Delta R.T. 0.00 min
Lab File: VN064039.D
Acq: 9 Oct 2020 15:39

Tgt Ion: 98 Resp: 273621
Ion Ratio Lower Upper
98 100
100 63.0 51.4 77.2

