

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100920\
 Data File : VN064065.D
 Acq On : 10 Oct 2020 3:37
 Operator : JC/MD
 Sample : L4317-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 11991

Quant Time: Oct 10 04:48:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	197007	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	397426	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	411258	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	154062	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	173184	53.21	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.42%	
35) Dibromofluoromethane	7.55	113	131365	47.64	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.28%	
50) Toluene-d8	10.06	98	509729	48.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.52%	
62) 4-Bromofluorobenzene	12.38	95	191596	48.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.52%	
Target Compounds						
16) Acetone	3.78	43	30406	30.348	ug/l	99
18) Methyl Acetate	4.29	43	4596	1.767	ug/l #	68
20) Methylene Chloride	4.51	84	9976	4.437	ug/l	92
43) Isopropyl Acetate	8.13	43	83649	12.678	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100920\
Data File : VN064065.D
Acq On : 10 Oct 2020 3:37
Operator : JC/MD
Sample : L4317-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
11991

Quant Time: Oct 10 04:48:03 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

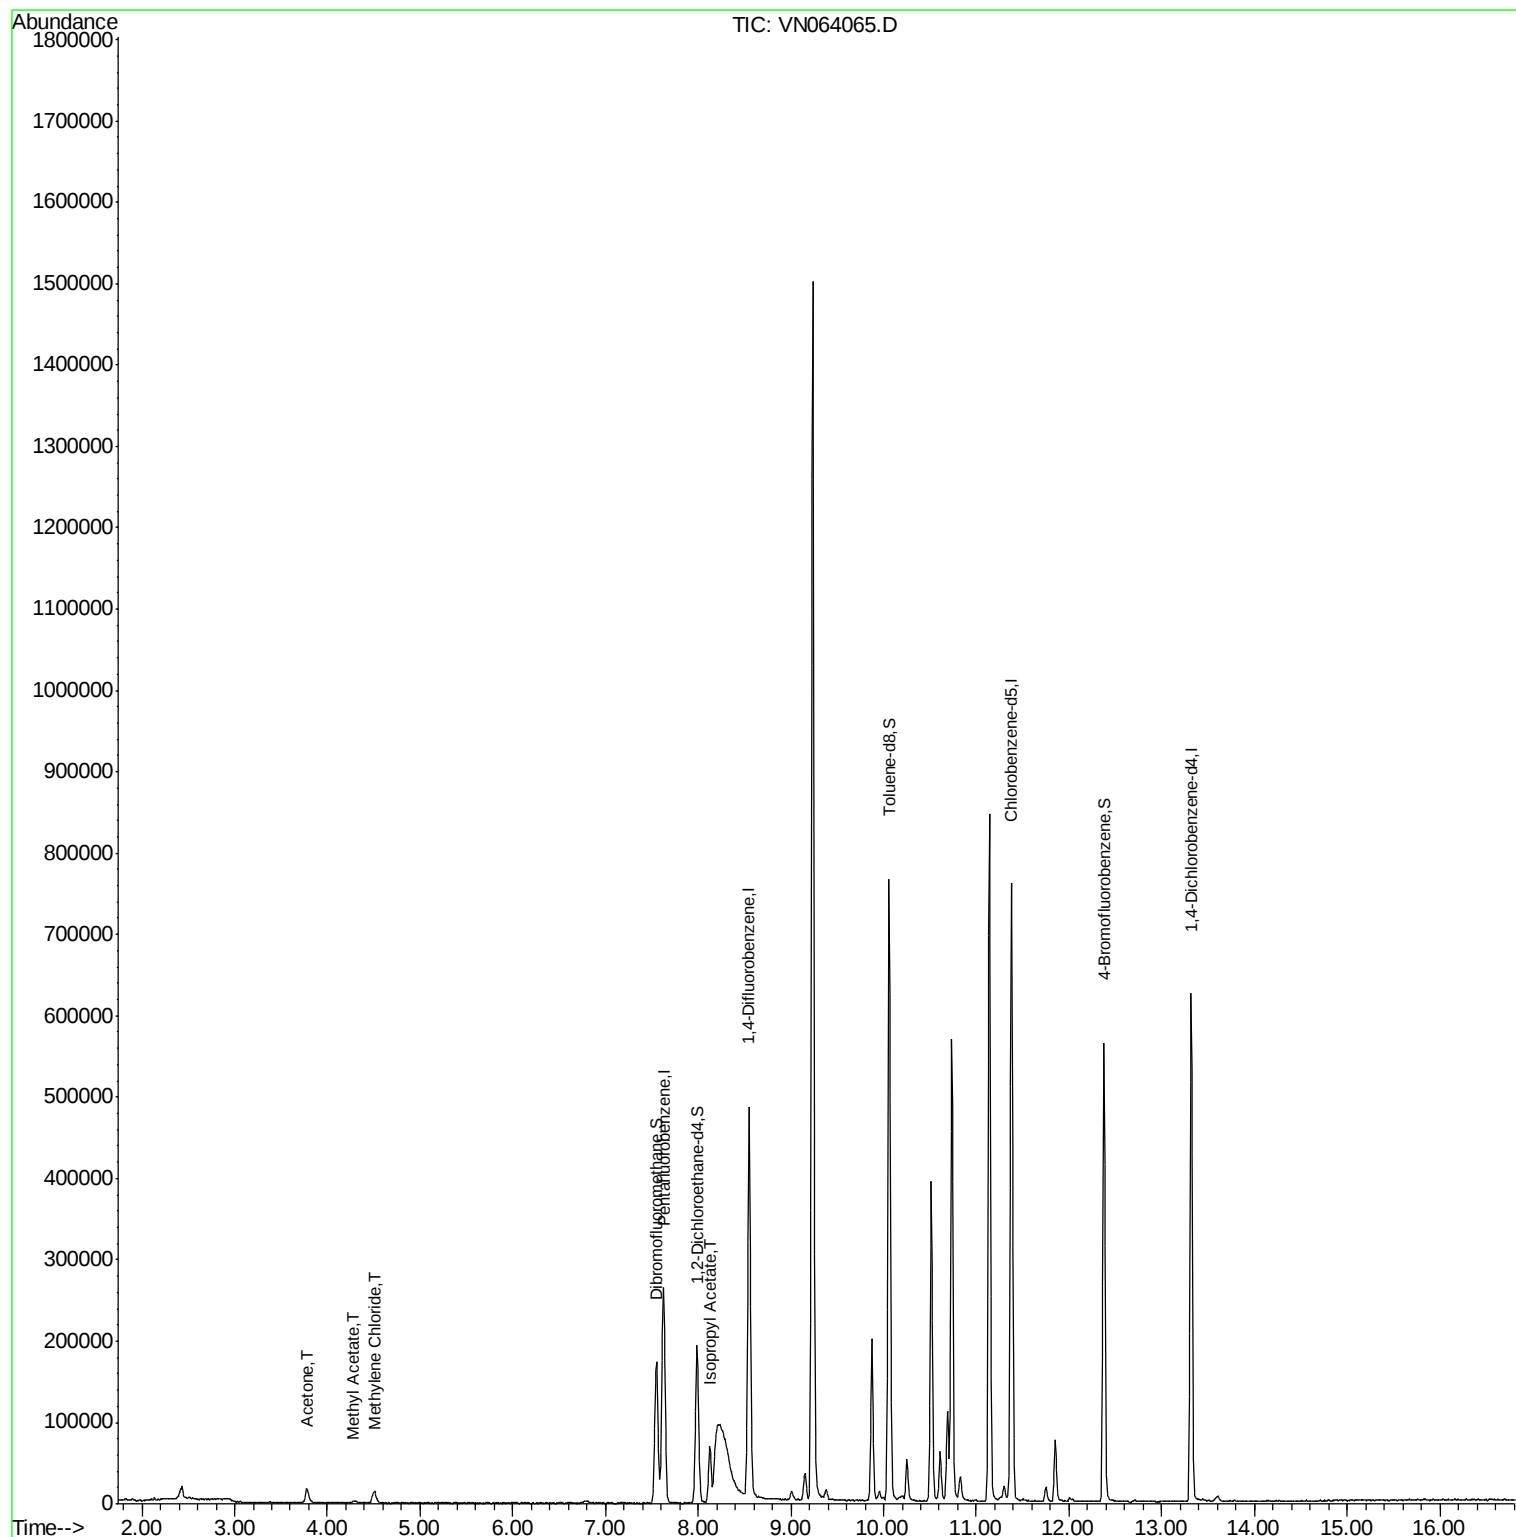

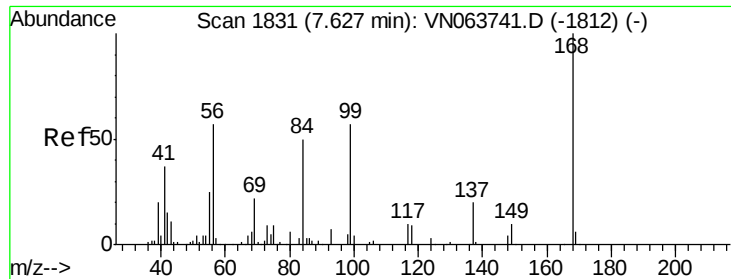

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064065.D

Acq: 10 Oct 2020 3:37


Instrument :
MSVOA_N
ClientSampleId :
11991

Tot Ion:168 Resp: 197007

Ion Ratio Lower Upper

168 100

99 64.9 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.63

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70

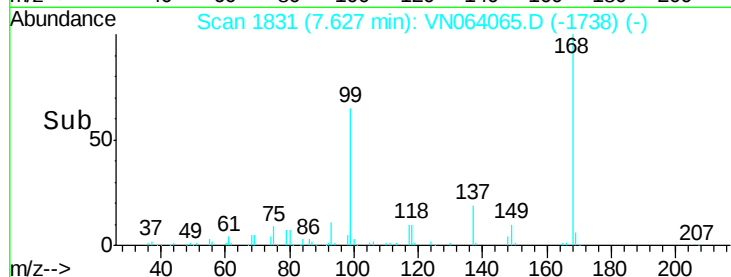

#16

Acetone

Concen: 30.348 ug/l

RT: 3.78 min Scan# 634

Delta R.T. 0.01 min

Lab File: VN064065.D


Acq: 10 Oct 2020 3:37

Tgt Ion: 43 Resp: 30406

Ion Ratio Lower Upper

43 100

58 27.4 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO

3.78

12000

10000

8000


6000


4000

2000

0

Time--> 3.70 3.80 3.90




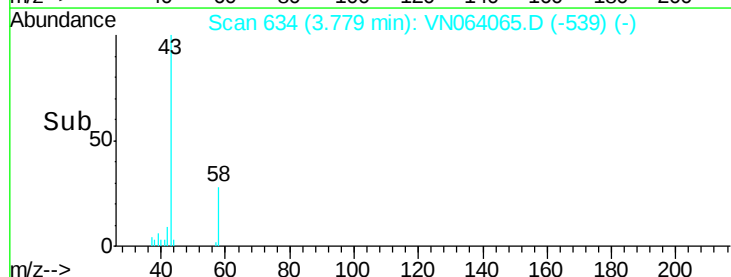


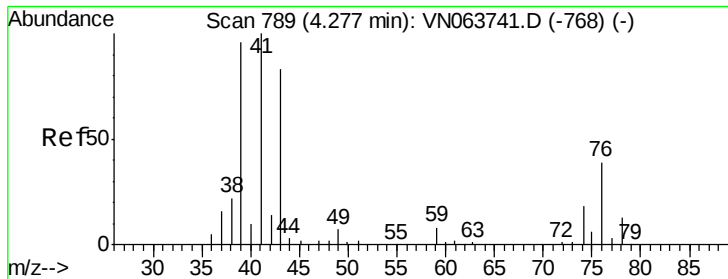

#18
Methvl Acetate
Concen: 1.767 ug/l
RT: 4.29 min Scan# 793
Delta R.T. 0.01 min
Lab File: VN064065.D
Acq: 10 Oct 2020 3:37




Instrument :
MSVOA_N
ClientSampled :
11991


Tot Ion: 43 Resp: 4596
Ion Ratio Lower Upper
43 100
74 6.6 17.4 26.2#

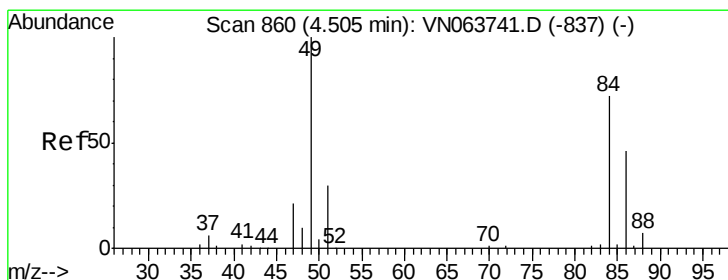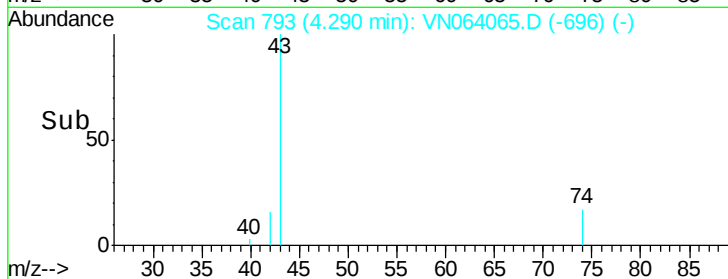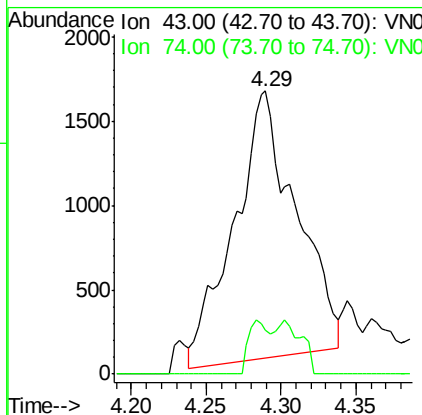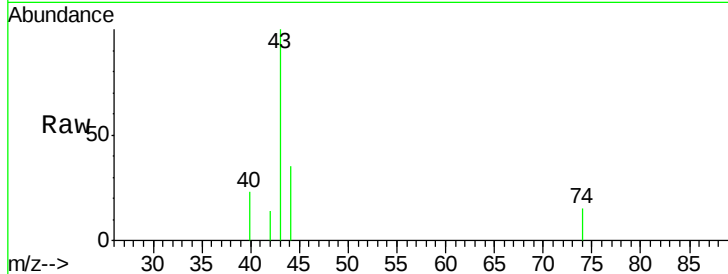

#20
Methylene Chloride
Concen: 4.437 ug/l
RT: 4.51 min Scan# 862
Delta R.T. 0.01 min
Lab File: VN064065.D
Acq: 10 Oct 2020 3:37

Tgt Ion: 84 Resp: 9976
Ion Ratio Lower Upper
84 100
49 121.6 110.4 165.6
51 42.4 33.3 49.9
86 62.3 50.7 76.1


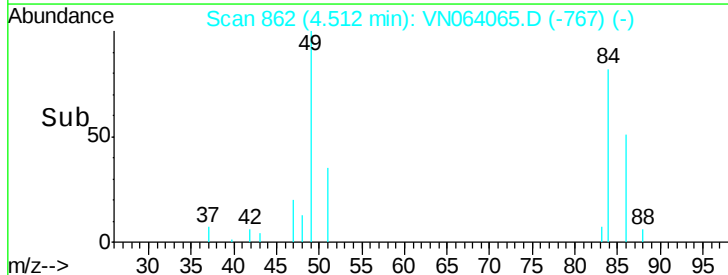
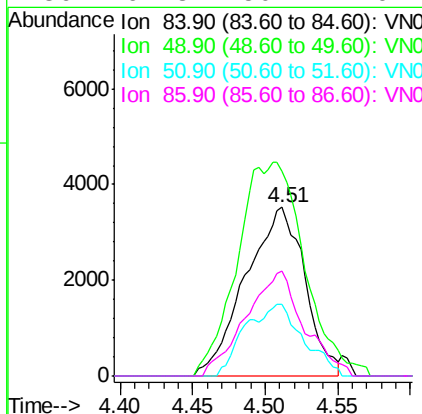
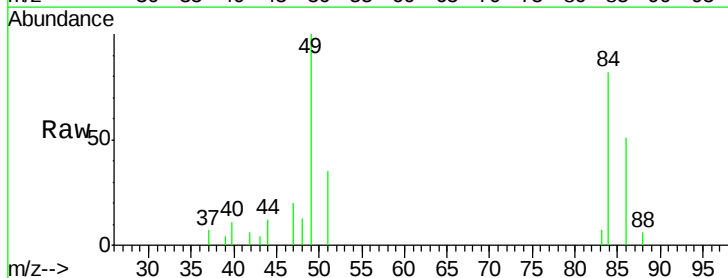


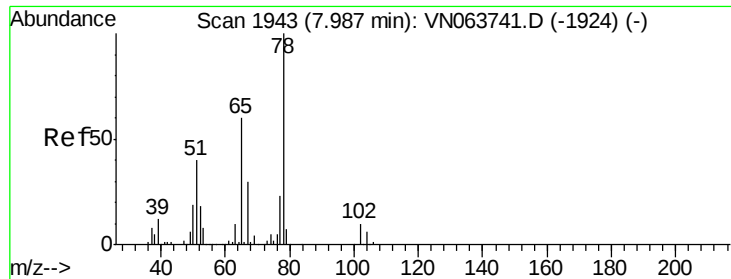

#33
 1,2-Dichloroethane-d4
 Concen: 53.211 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN064065.D
 Acq: 10 Oct 2020 3:37




Instrument :
 MSVOA_N
 ClientSampled :
 11991

Tot Ion: 65 Resp: 173184
 Ion Ratio Lower Upper
 65 100
 67 52.1 0.0 99.6

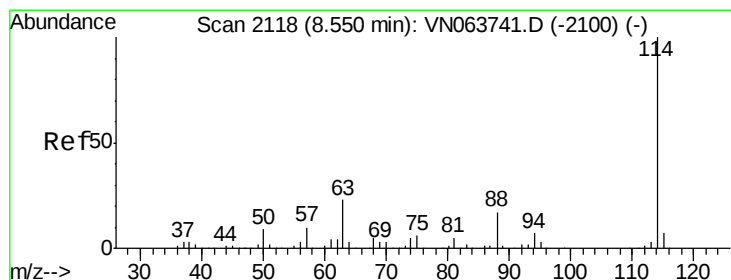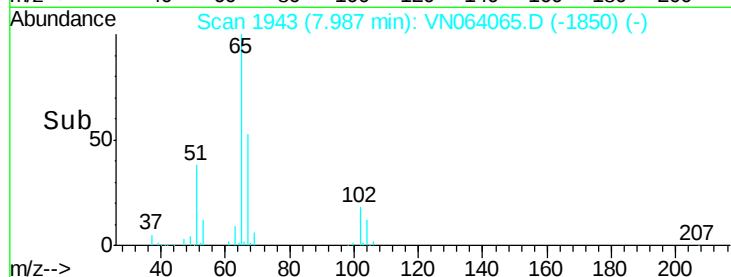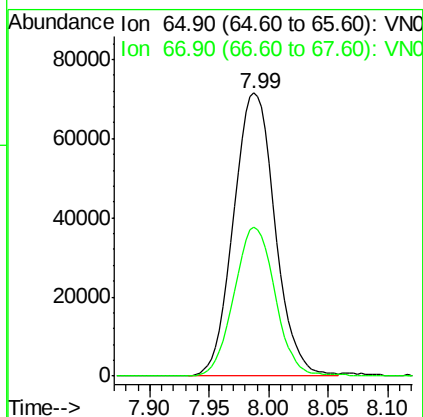

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN064065.D
 Acq: 10 Oct 2020 3:37

Tgt Ion: 114 Resp: 397426
 Ion Ratio Lower Upper
 114 100
 63 22.8 0.0 45.0
 88 16.3 0.0 34.0

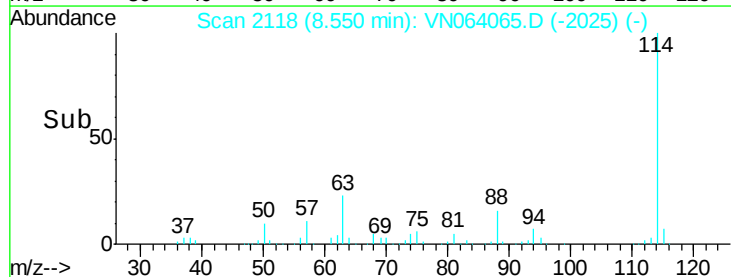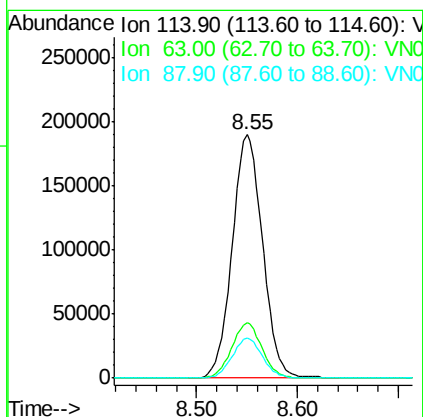







#35
 Dibromofluoromethane
 Concen: 47.637 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN064065.D
 Acq: 10 Oct 2020 3:37

Instrument :
 MSVOA_N
 ClientSampled :
 11991

Tot Ion:113 Resp: 131365
 Ion Ratio Lower Upper
 113 100
 111 102.5 81.8 122.8
 192 18.3 14.2 21.2

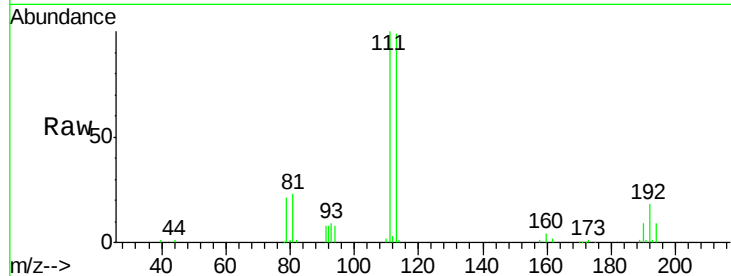


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

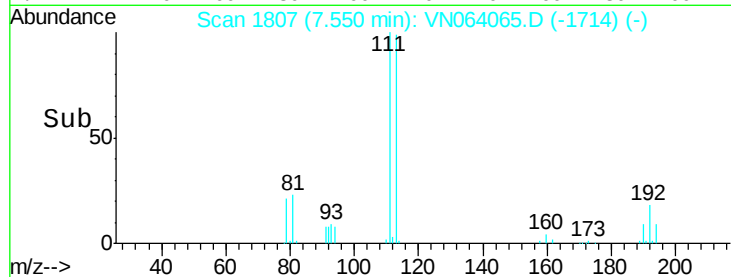
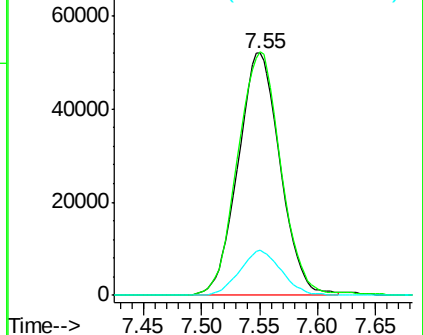



#43
 Isopropyl Acetate
 Concen: 12.678 ug/l
 RT: 8.13 min Scan# 1986
 Delta R.T. 0.00 min
 Lab File: VN064065.D
 Acq: 10 Oct 2020 3:37

Tgt Ion: 43 Resp: 83649
 Ion Ratio Lower Upper
 43 100
 61 17.9 14.2 21.4
 87 11.3 9.0 13.6

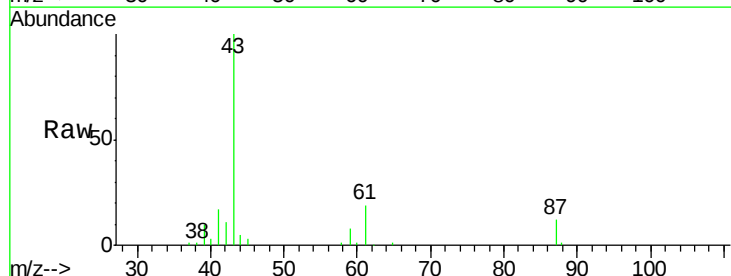

Abundance Ion 43.00 (42.70 to 43.70): V
 Ion 61.00 (60.70 to 61.70): V
 Ion 87.00 (86.70 to 87.70): V

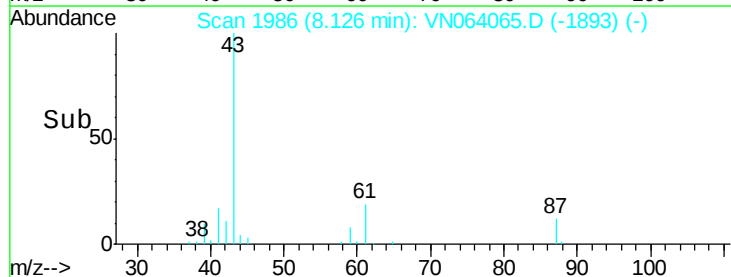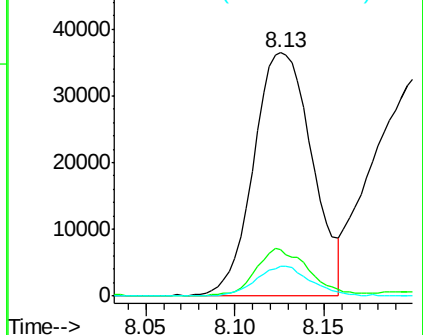

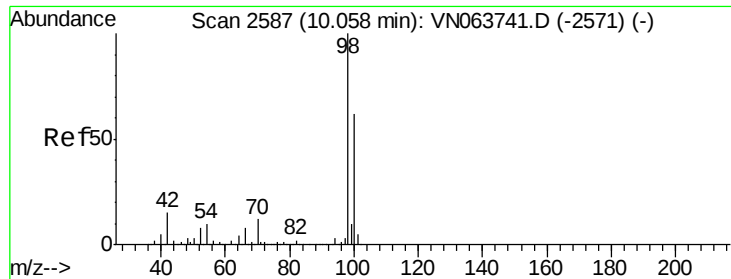

#50

Toluene-d8

Concen: 48.760 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064065.D

Acq: 10 Oct 2020 3:37

Instrument :

MSVOA_N

ClientSampleId :





11991

Tot Ion: 98 Resp: 509729

Ion Ratio Lower Upper

98 100

100 62.8 49.8 74.6

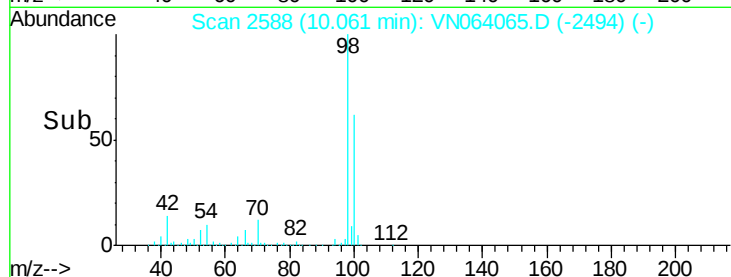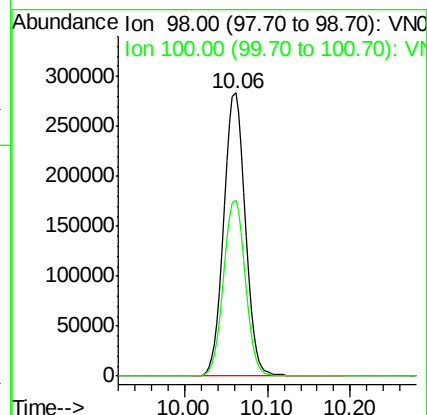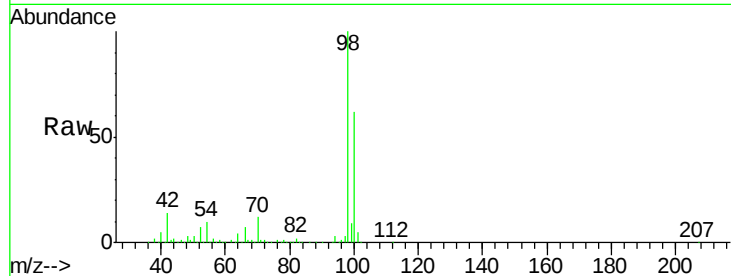

#62

4-Bromofluorobenzene

Concen: 48.755 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN064065.D

Acq: 10 Oct 2020 3:37




Tgt Ion: 95 Resp: 191596


Ion Ratio Lower Upper

95 100

174 75.0 0.0 150.6

176 71.3 0.0 145.4

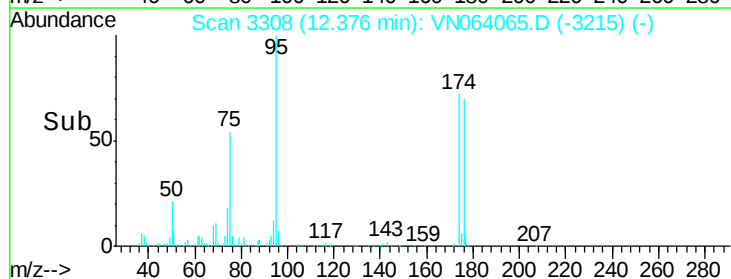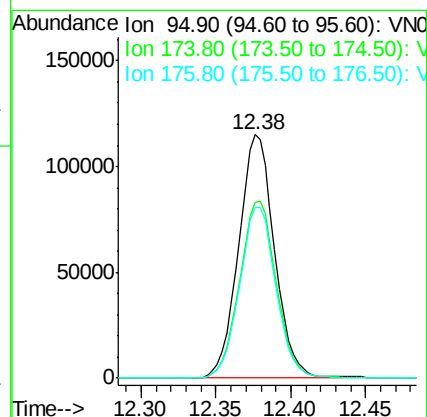


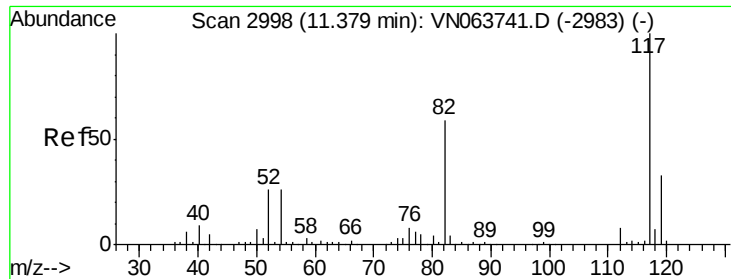




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN064065.D
Acq: 10 Oct 2020 3:37

Instrument :
MSVOA_N
ClientSampleId :
11991

Tot Ion:117 Resp: 411258
Ion Ratio Lower Upper
117 100
82 58.9 47.4 71.2
119 31.8 26.4 39.6

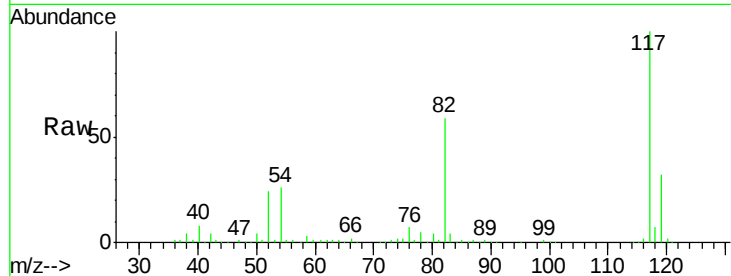


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

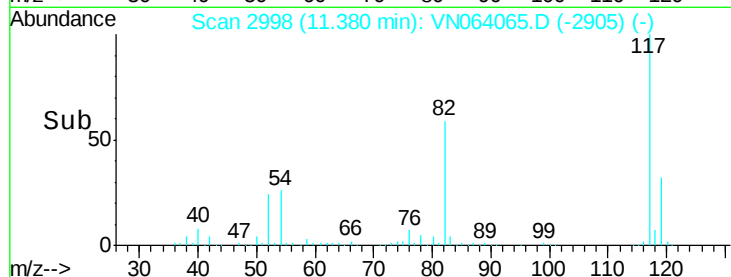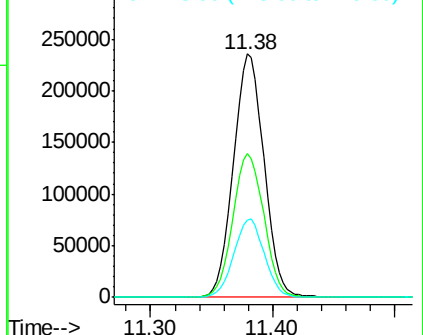

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN064065.D
Acq: 10 Oct 2020 3:37

Tgt Ion:152 Resp: 154062
Ion Ratio Lower Upper
152 100
115 64.2 31.3 93.8
150 158.8 0.0 341.8



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

