


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100920\
 Data File : VN064031.D
 Acq On : 9 Oct 2020 10:34
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N100620W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Oct 06 16:42:38 2020

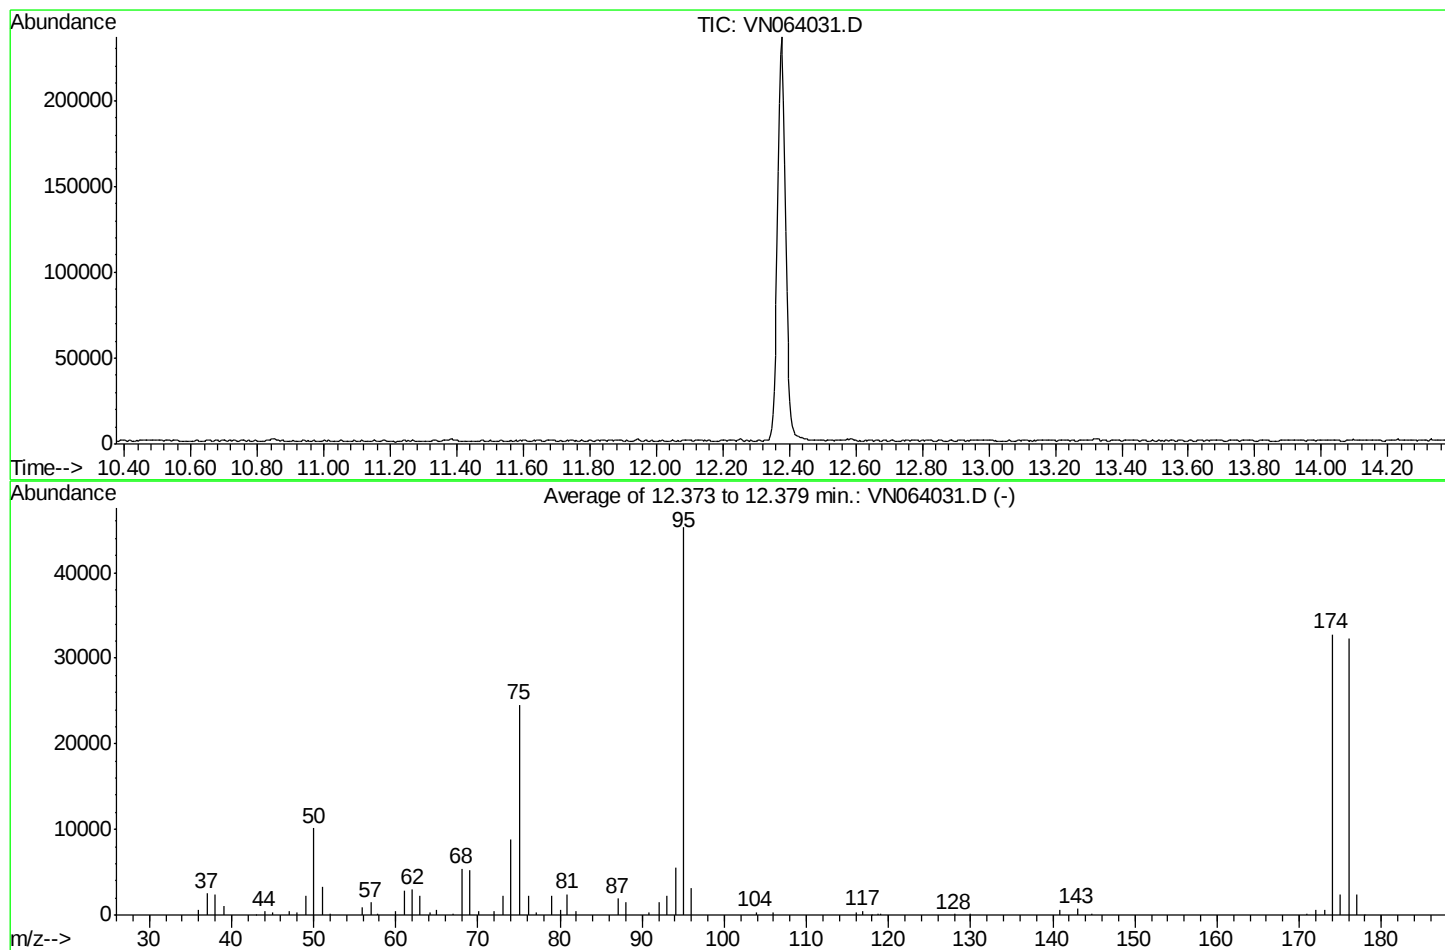

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3295

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	10129	PASS
75	95	30	60	54.3	24600	PASS
95	95	100	100	100.0	45298	PASS
96	95	5	9	7.0	3149	PASS
173	174	0.00	2	1.8	595	PASS
174	95	50	100	72.4	32800	PASS
175	174	5	9	7.5	2454	PASS
176	174	95	101	98.6	32328	PASS
177	176	5	9	7.5	2434	PASS