


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100920\
Data File : VN064049.D
Acq On : 9 Oct 2020 20:25
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Title : SW846 8260
Last Update : Thu Oct 01 01:46:38 2020

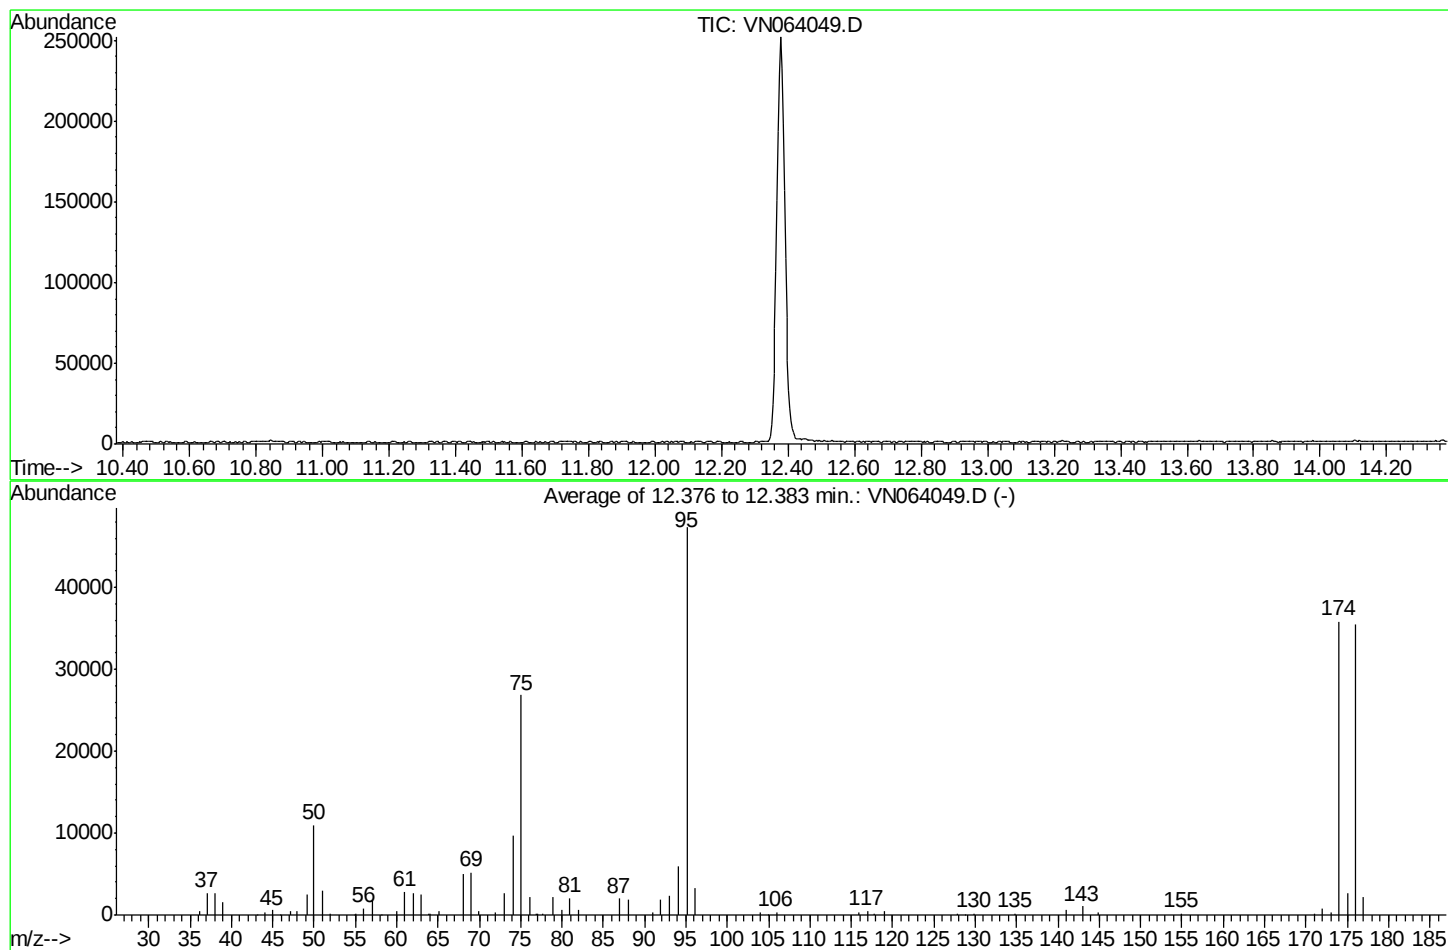

AutoFind: Scans 3308, 3309, 3310; Background Corrected with Scan 3295

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	10997	PASS
75	95	30	60	56.7	26810	PASS
95	95	100	100	100.0	47312	PASS
96	95	5	9	7.1	3340	PASS
173	174	0.00	2	0.7	255	PASS
174	95	50	100	75.7	35816	PASS
175	174	5	9	7.2	2590	PASS
176	174	95	101	99.2	35530	PASS
177	176	5	9	6.3	2248	PASS