
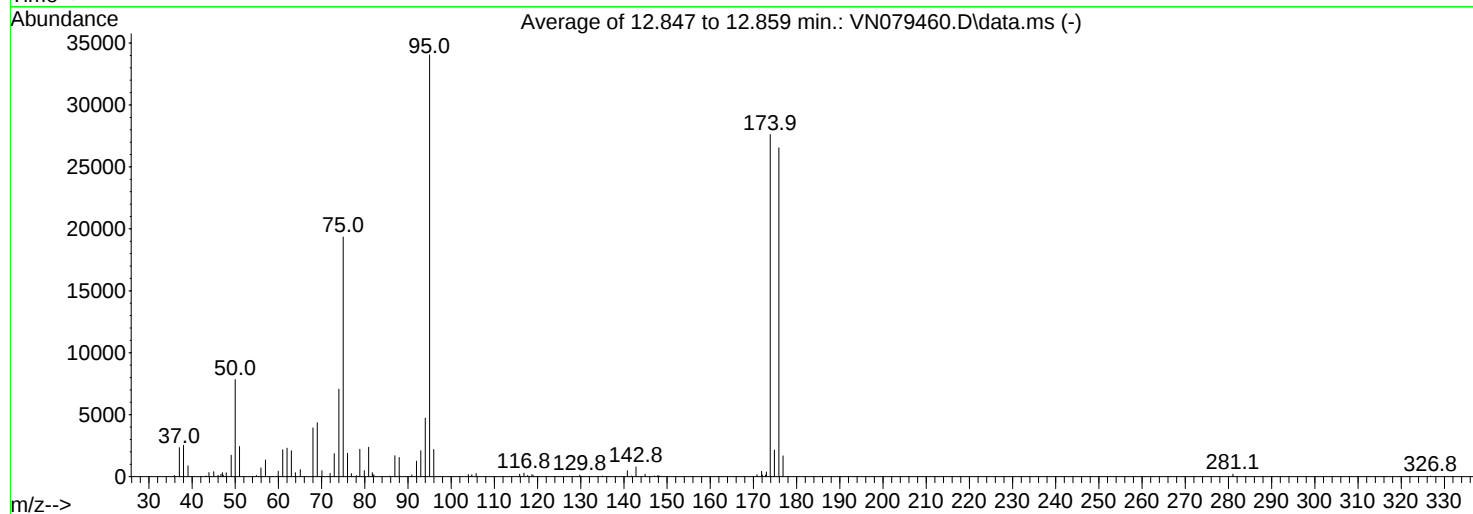


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100923\
 Data File : VN079460.D
 Acq On : 09 Oct 2023 09:03
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
 Title : SW846 8260
 Last Update : Fri Oct 06 03:34:49 2023

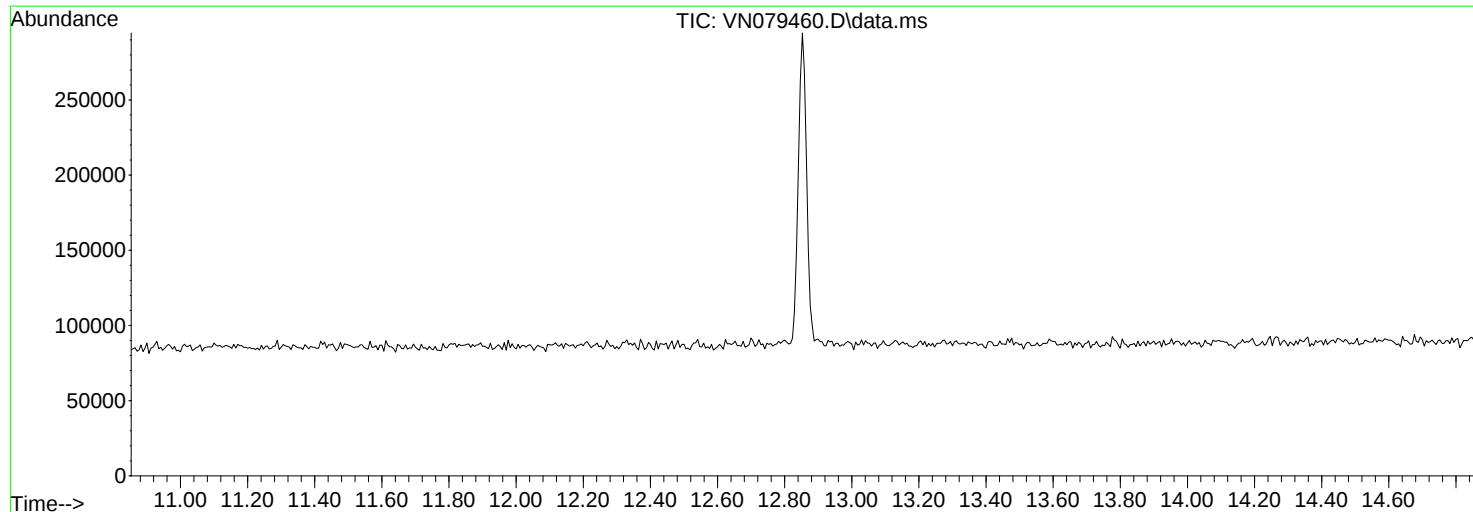

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	7839	PASS
75	95	30	60	56.8	19352	PASS
95	95	100	100	100.0	34048	PASS
96	95	5	9	6.5	2203	PASS
173	174	0.00	2	1.4	376	PASS
174	95	50	100	81.1	27608	PASS
175	174	5	9	7.8	2147	PASS
176	174	95	101	96.1	26544	PASS
177	176	5	9	6.3	1680	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	94	47.90	305	63.90	327	78.10	81
37.05	2332	49.05	1730	65.05	567	78.85	220
38.00	2530	50.00	7839	68.00	3943	79.90	49
39.05	879	51.00	2426	69.00	4351	80.90	237
43.20	52	54.90	91	70.05	481	81.75	328
43.90	332	55.95	715	71.95	272	81.90	175
45.00	403	57.00	1338	72.90	1860	82.10	131
46.00	107	59.95	441	74.00	7066	85.80	52
46.70	188	61.00	2175	75.00	19352	86.95	1693
47.00	318	62.00	2300	76.00	1882	87.95	1546
47.20	120	63.00	2088	76.90	244	90.90	138

Average of 12.847 to 12.859 min.: VN079460.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.95	1253	118.70	183	170.80	159		
92.95	2098	119.00	79	171.90	422		
94.00	4731	129.80	126	172.10	129		
95.00	34048	135.00	54	172.80	137		
95.95	2203	140.80	483	173.00	376		
103.95	162	141.80	53	173.90	27608		
104.80	153	142.80	785	174.85	2147		
105.80	248	144.90	200	175.90	26544		
115.85	191	147.10	68	176.85	1680		
116.85	286	147.80	66	281.05	209		
117.70	110	148.10	72	326.80	53		

Instrument :

MSVOA_N

ClientSampleId :

BFB