
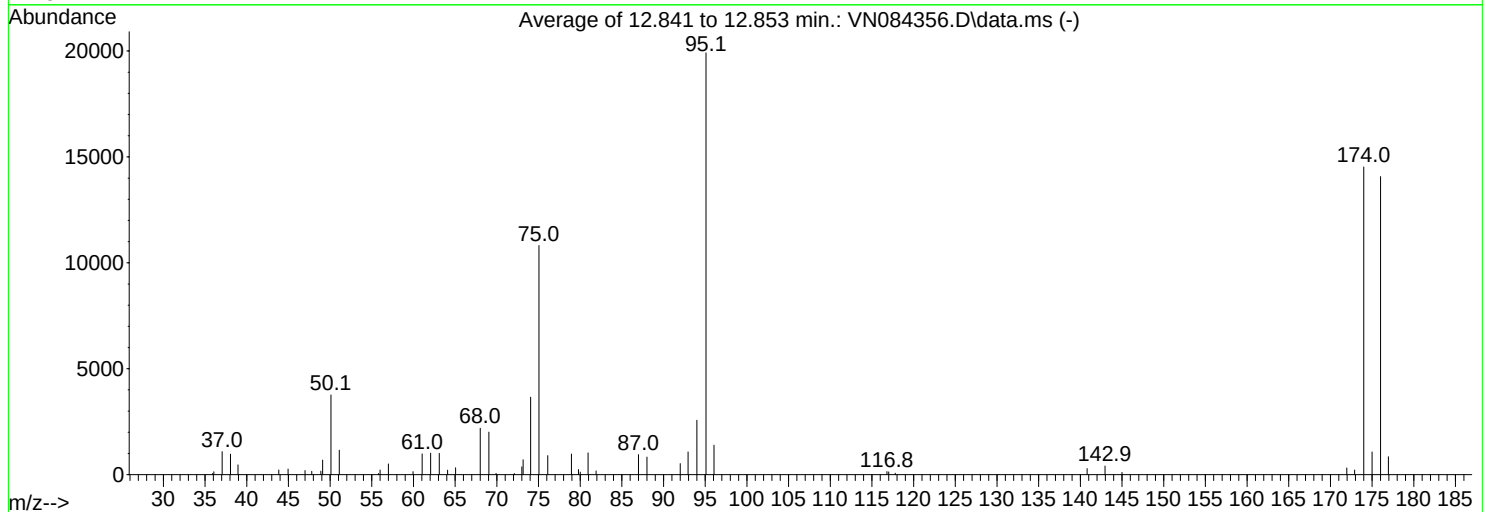


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100924\
Data File : VN084356.D
Acq On : 09 Oct 2024 09:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

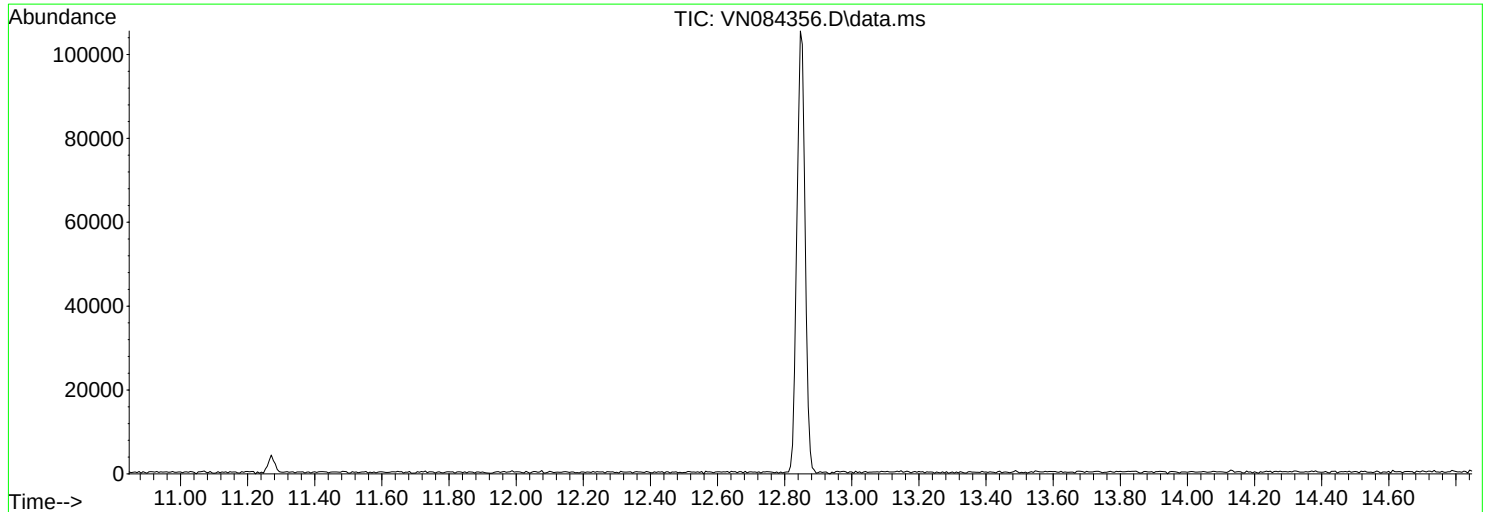

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	3765	PASS
75	95	30	60	54.3	10817	PASS
95	95	100	100	100.0	19912	PASS
96	95	5	9	7.0	1391	PASS
173	174	0.00	2	1.5	221	PASS
174	95	50	100	73.0	14527	PASS
175	174	5	9	7.4	1072	PASS
176	174	95	101	96.9	14074	PASS
177	176	5	9	6.0	844	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	53	49.10	688	65.05	326	79.80	241
36.05	135	50.10	3765	68.00	2188	80.00	121
37.05	1085	51.10	1158	69.05	2012	80.95	102
38.05	969	55.80	56	69.90	61	81.90	17
38.95	461	56.00	217	72.10	52	87.00	942
39.95	14	57.00	510	73.00	369	88.00	831
43.85	217	59.95	140	73.15	702	92.00	525
44.95	263	61.05	980	74.05	3656	92.95	1070
47.00	200	62.05	1015	75.05	10817	94.00	2567
47.80	156	63.10	1007	76.10	898	95.10	19912
48.90	167	64.10	211	78.95	971	96.05	1391

Average of 12.841 to 12.853 min.: VN084356.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.80	143	176.95	844				
117.00	130						
117.80	65						
140.80	288						
142.95	410						
145.00	108						
171.95	317						
172.90	221						
174.00	14527						
175.00	1072						
176.00	14074						

Instrument :

MSVOA_N

ClientSampleId :

BFB