


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN101018\
Data File : VN051776.D
Acq On : 10 Oct 2018 7:38
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Title : SW846 8260
Last Update : Tue Oct 09 06:03:49 2018

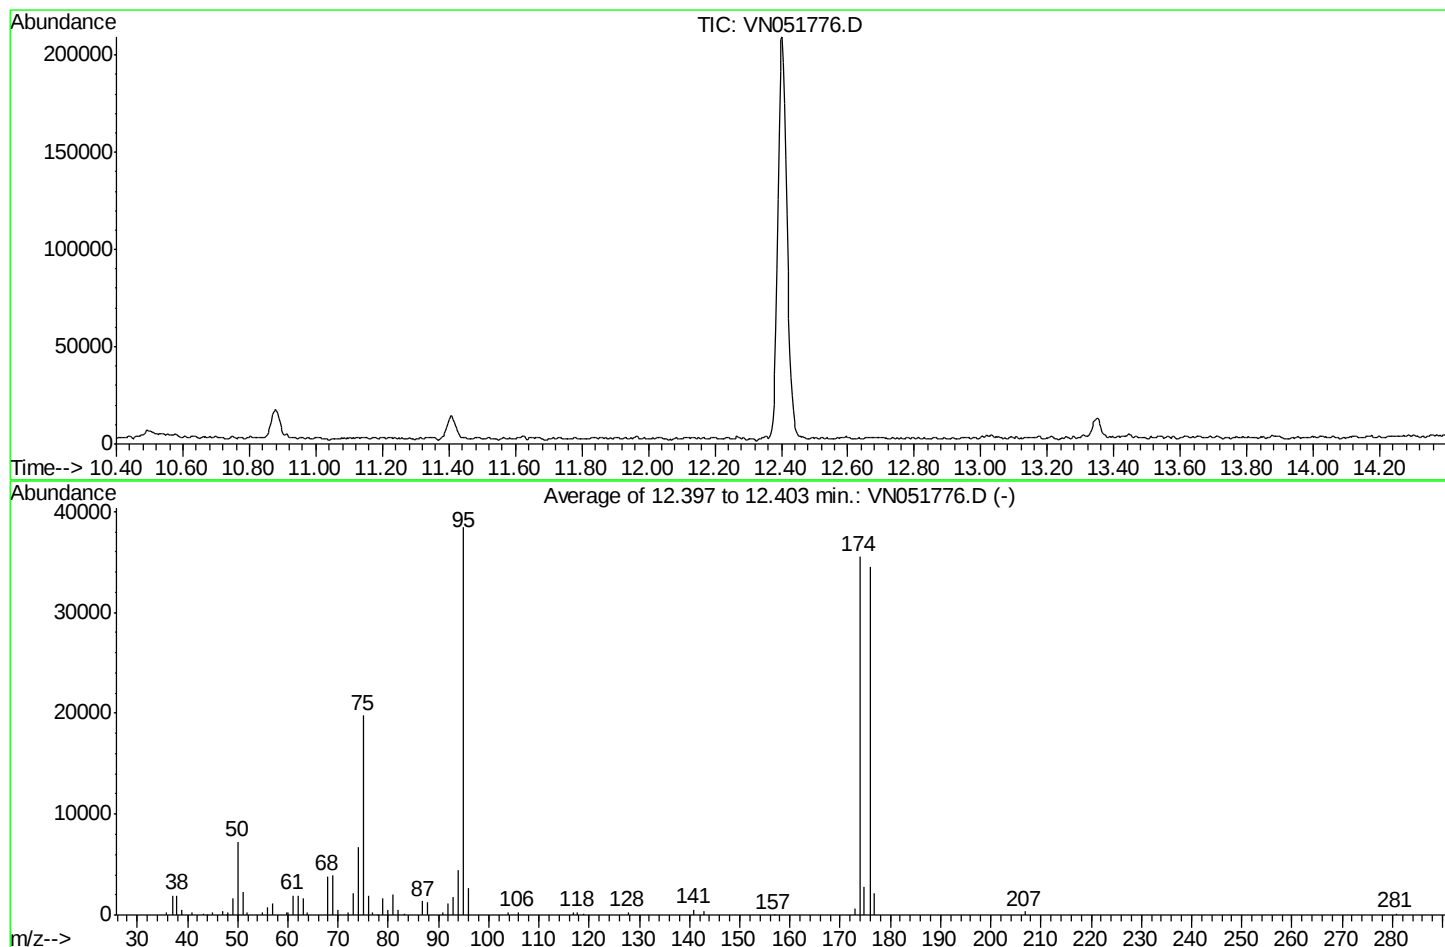

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	7291	PASS
75	95	30	60	51.4	19736	PASS
95	95	100	100	100.0	38426	PASS
96	95	5	9	6.9	2642	PASS
173	174	0.00	2	1.7	612	PASS
174	95	50	100	92.4	35512	PASS
175	174	5	9	7.8	2771	PASS
176	174	95	101	97.2	34528	PASS
177	176	5	9	6.4	2200	PASS