

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101023\
 Data File : VN079499.D
 Acq On : 10 Oct 2023 17:37
 Operator : JC\MD
 Sample : 04817-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Oct 11 06:21:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 06 03:34:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	316662	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	607861	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	584388	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	226176	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	240593	46.859	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	93.720%		
35) Dibromofluoromethane	8.171	113	212904	48.738	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.480%		
50) Toluene-d8	10.571	98	716851	45.354	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	90.700%		
62) 4-Bromofluorobenzene	12.853	95	269079	53.048	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	106.100%		
Target Compounds					Qvalue	
10) Methyl Iodide	4.595	142	876	0.248	ug/l #	11
11) Tert butyl alcohol	5.524	59	295	0.382	ug/l #	72
16) Acetone	4.436	43	51427	25.253	ug/l #	79
18) Methyl Acetate	5.053	43	6134	0.615	ug/l #	77
20) Methylene Chloride	5.283	84	23505	4.725	ug/l #	88
25) 2-Butanone	7.494	43	5464	1.808	ug/l #	67
29) Tetrahydrofuran	7.877	42	468	0.239	ug/l #	20
31) Cyclohexane	8.224	56	8100	1.112	ug/l #	56
36) 1,1-Dichloropropene	8.230	75	28115	4.288	ug/l #	47
37) Ethyl Acetate	7.565	43	5353	0.821	ug/l #	81
38) Carbon Tetrachloride	8.230	117	34279	5.223	ug/l #	15
40) Benzene	8.612	78	7088	0.364	ug/l	91
42) 1,2-Dichloroethane	8.688	62	1722	0.243	ug/l #	73
43) Isopropyl Acetate	8.694	43	333953	29.219	ug/l #	71
45) 1,2-Dichloropropane	9.741	63	2336	0.455	ug/l #	45
48) Methyl methacrylate	9.665	41	5815	1.187	ug/l #	33
49) 1,4-Dioxane	9.735	88	118	1.308	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	19804	3.070	ug/l #	65
52) Toluene	10.629	92	7429	0.648	ug/l	89
54) cis-1,3-Dichloropropene	10.359	75	80298	10.650	ug/l #	71
57) 1,3-Dichloropropane	11.206	76	9368	1.179	ug/l #	42
59) 2-Hexanone	11.176	43	207397	44.547	ug/l #	19
68) m/p-Xylenes	12.070	106	5295	0.644	ug/l	93
69) o-Xylene	12.406	106	2051	0.254	ug/l	70
75) 1,1,2,2-Tetrachloroethane	13.153	83	540	Below Cal		92
76) 1,2,3-Trichloropropane	12.853	75	146258	22.428	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	146258	65.075	ug/l #	15
84) 1,2,4-Trimethylbenzene	13.482	105	9873	0.624	ug/l	93
90) Hexachloroethane	14.335	117	505	Below Cal	#	21
95) Naphthalene	15.641	128	124463	16.487	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101023\
Data File : VN079499.D
Acq On : 10 Oct 2023 17:37
Operator : JC\MD
Sample : 04817-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Oct 11 06:21:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 06 03:34:49 2023
Response via : Initial Calibration




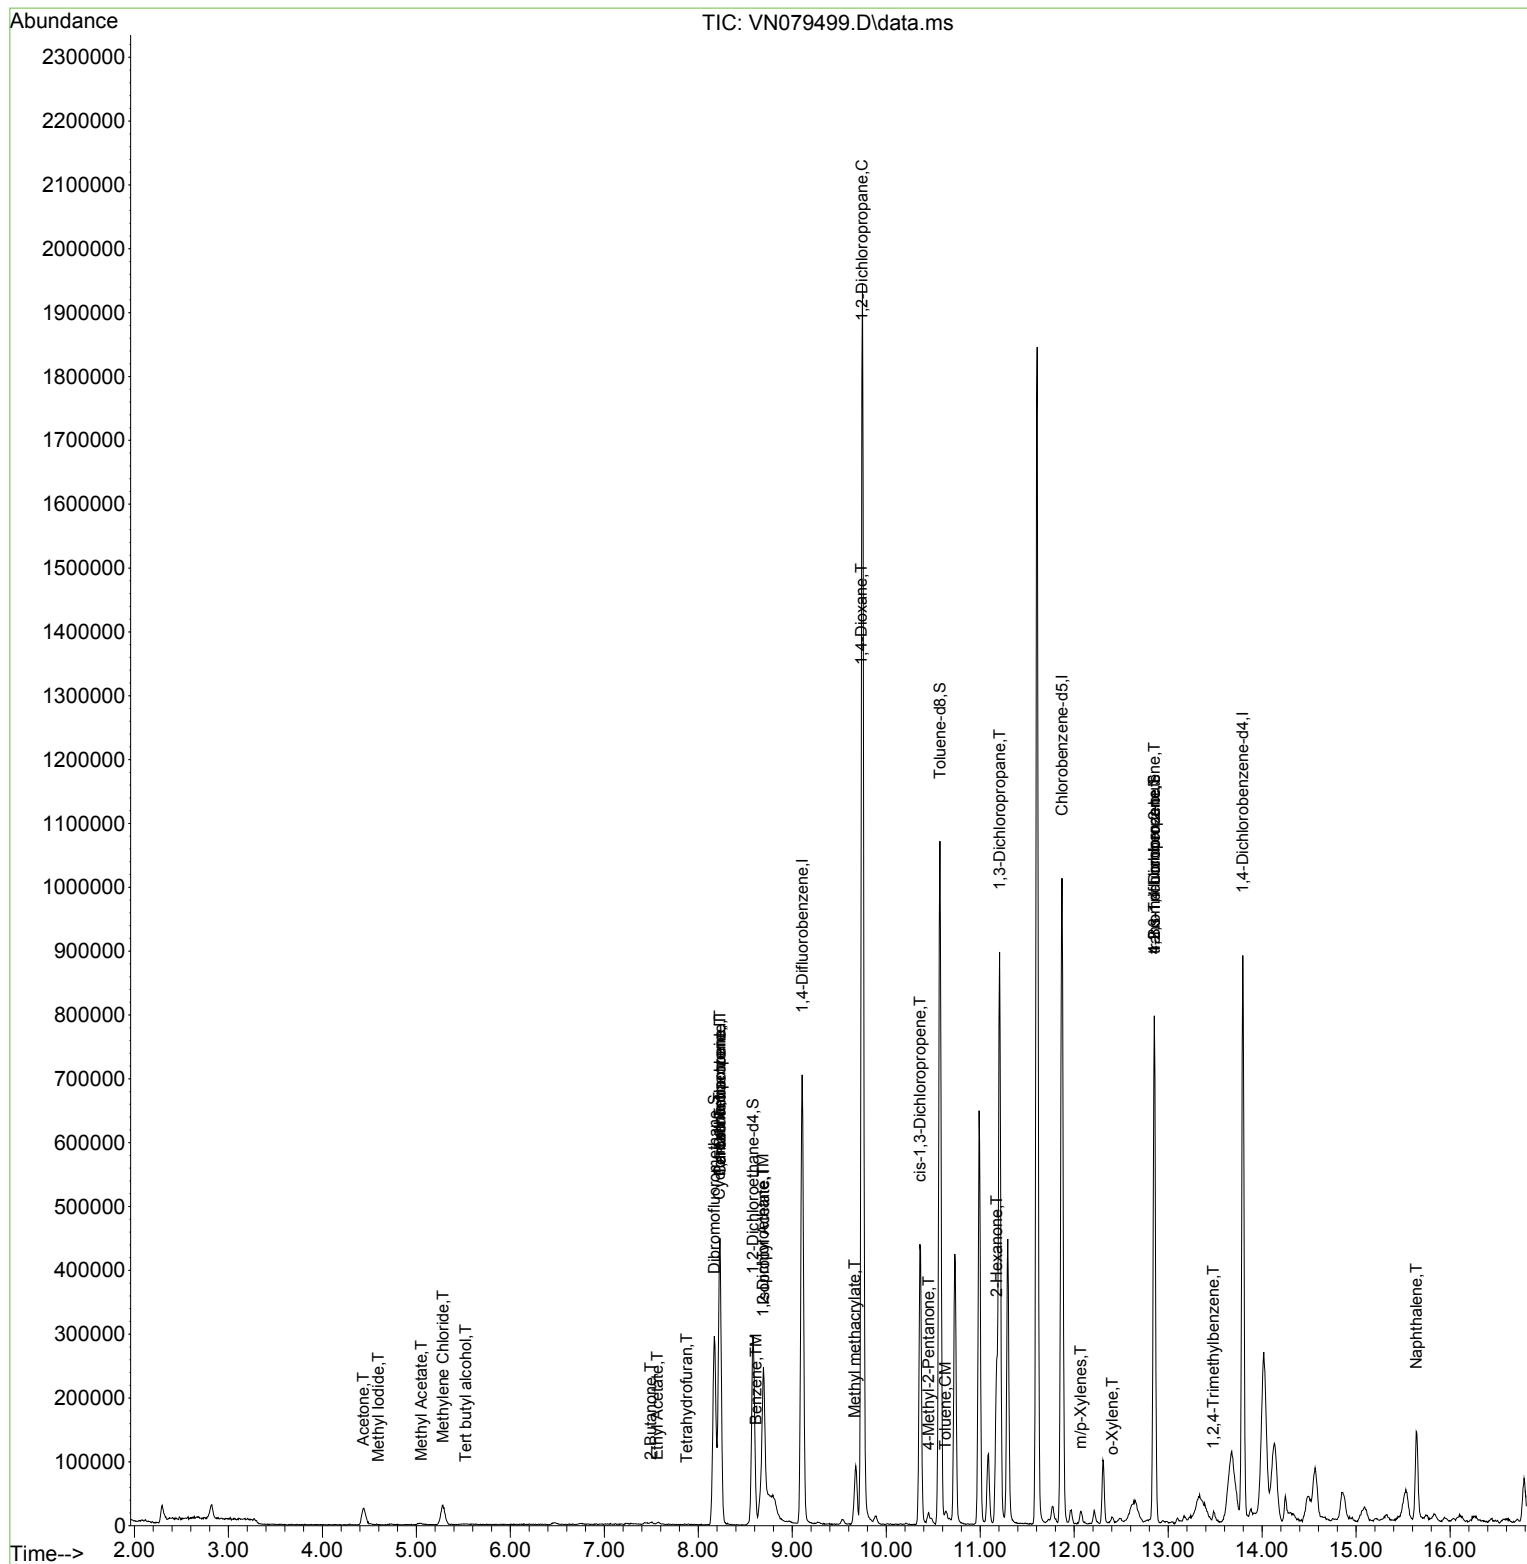




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.000 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 316662
Ion Ratio Lower Upper
168 100
99 62.5 53.0 79.6

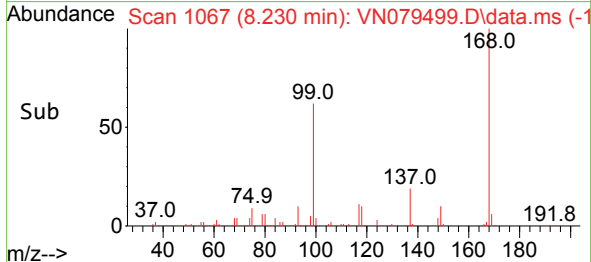

#10
Methyl Iodide
Concen: 0.248 ug/l
RT: 4.595 min Scan# 449
Delta R.T. 0.005 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37

Tgt Ion:142 Resp: 876
Ion Ratio Lower Upper
142 100
127 0.0 37.6 56.4#
141 75.2 11.4 17.0#


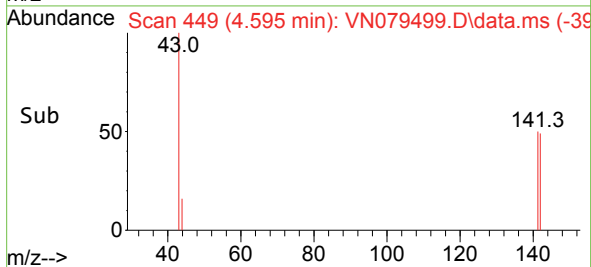

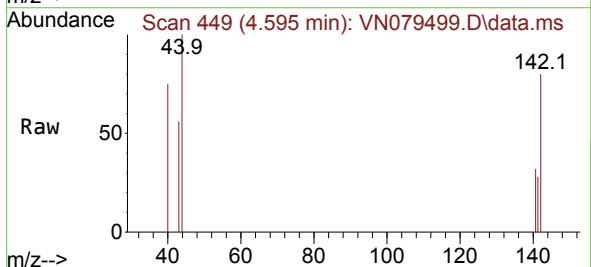




#11
Tert butyl alcohol
Concen: 0.382 ug/l
RT: 5.524 min Scan# 608
Delta R.T. -0.006 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 295
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

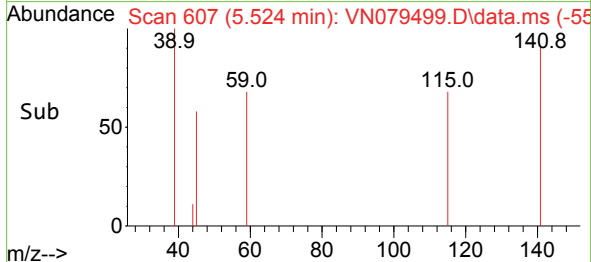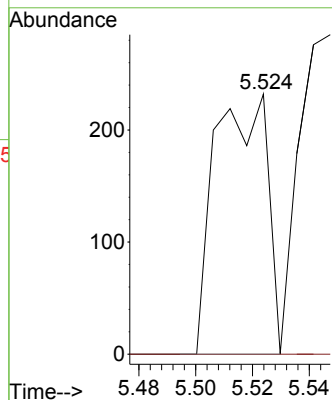

#16
Acetone
Concen: 25.253 ug/l
RT: 4.436 min Scan# 422
Delta R.T. 0.006 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37

Tgt Ion: 43 Resp: 51427
Ion Ratio Lower Upper
43 100
58 22.8 28.0 42.0#


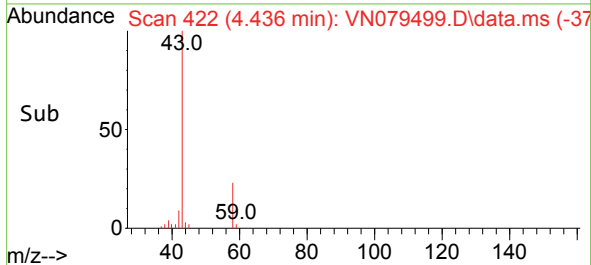
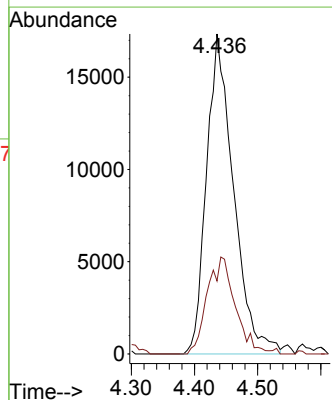
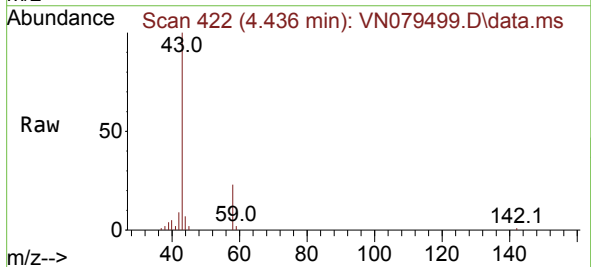




#18
Methyl Acetate
Concen: 0.615 ug/l
RT: 5.053 min Scan# 51
Delta R.T. 0.023 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 6134
Ion Ratio Lower Upper
43 100
74 19.7 26.2 39.4#

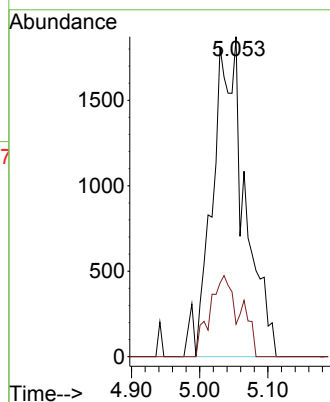

#20
Methylene Chloride
Concen: 4.725 ug/l
RT: 5.283 min Scan# 566
Delta R.T. -0.000 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37


Tgt Ion: 84 Resp: 23505
Ion Ratio Lower Upper
84 100
49 110.4 79.7 119.5
51 38.8 25.2 37.8#
86 57.1 53.3 79.9

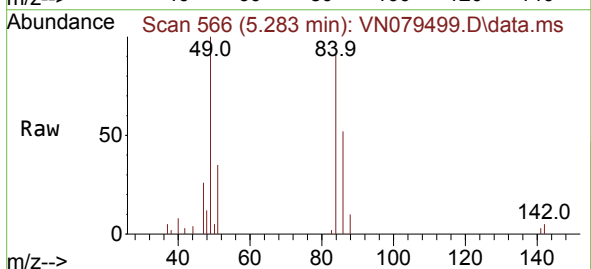



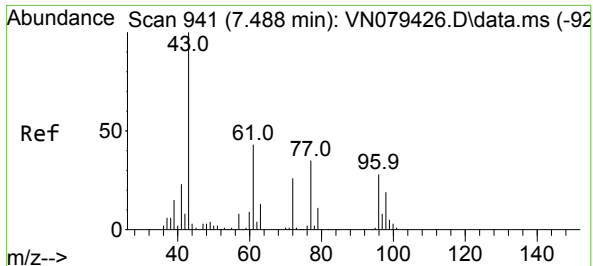


#25
2-Butanone
Concen: 1.808 ug/l
RT: 7.494 min Scan# 941
Delta R.T. 0.006 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37


Instrument :
MSVOA_N
ClientSampleId :

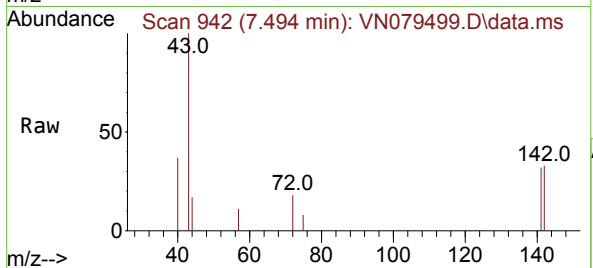



Tgt Ion: 43 Resp: 5464
Ion Ratio Lower Upper
43 100
72 17.9 30.2 45.2#

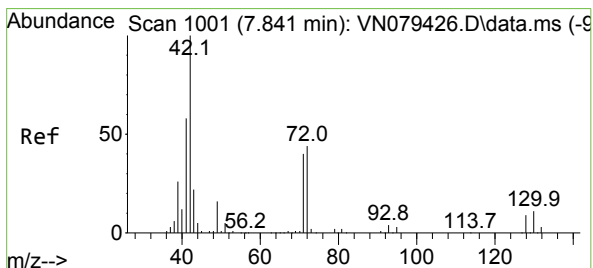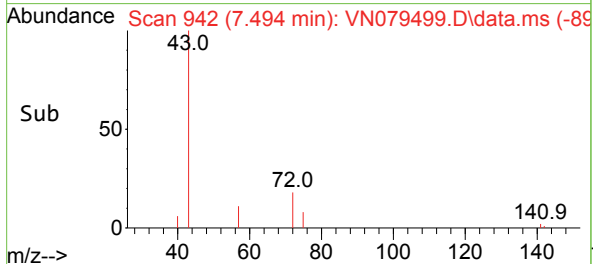


#29
Tetrahydrofuran
Concen: 0.239 ug/l
RT: 7.877 min Scan# 1007
Delta R.T. 0.036 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37

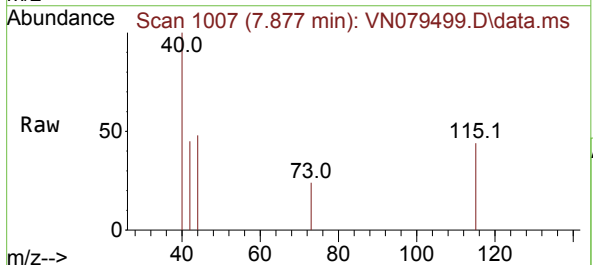


Tgt Ion: 42 Resp: 468
Ion Ratio Lower Upper
42 100
72 0.0 49.8 74.6#
71 0.0 47.4 71.2#

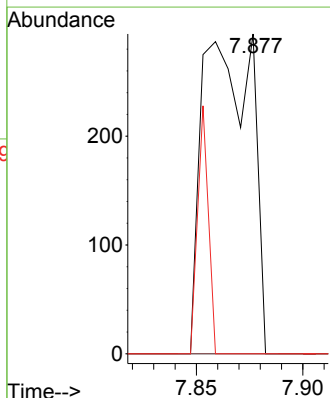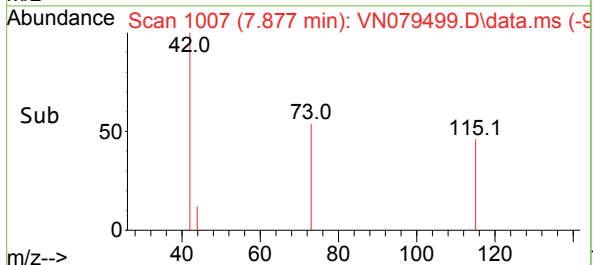






#31
Cyclohexane
Concen: 1.112 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.041 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 8100
Ion Ratio Lower Upper
56 100
69 131.6 26.8 40.2#
84 99.8 81.8 122.6

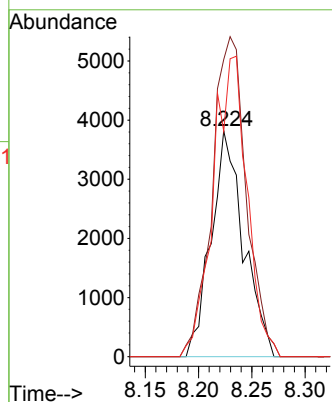

#33
1,2-Dichloroethane-d4
Concen: 46.859 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37

Tgt Ion: 65 Resp: 240593
Ion Ratio Lower Upper
65 100
67 51.6 0.0 106.6

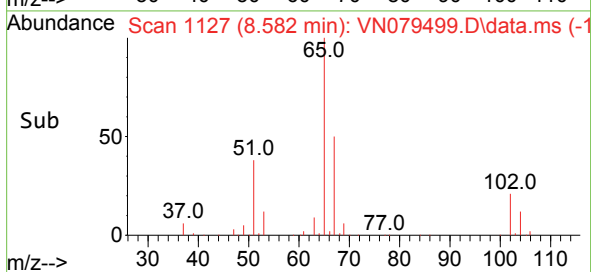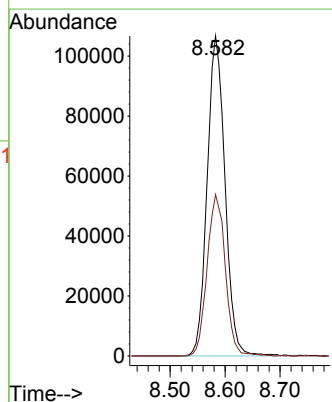



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 607861

Ion Ratio Lower Upper

114 100

63 20.2 0.0 36.4

88 14.9 0.0 30.6

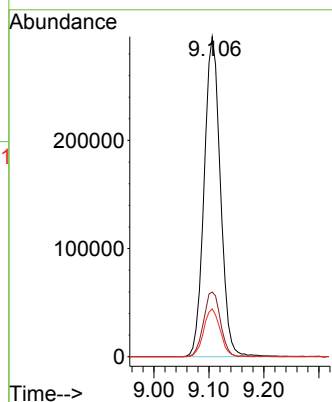

#35

Dibromofluoromethane

Concen: 48.738 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37




Tgt Ion:113 Resp: 212904


Ion Ratio Lower Upper

113 100

111 102.1 82.6 123.8

192 17.8 12.7 19.1

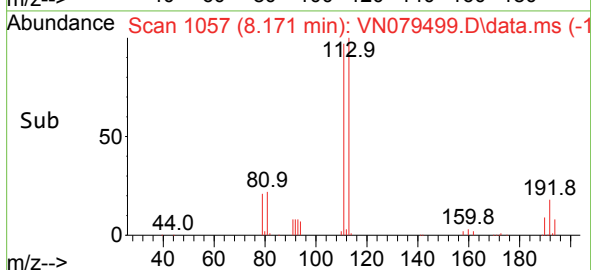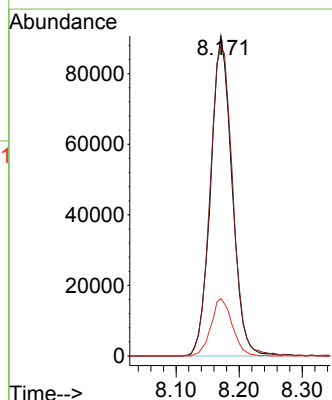



#36

1,1-Dichloropropene

Concen: 4.288 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.147 min


Lab File: VN079499.D

Acq: 10 Oct 2023 17:37

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 75 Resp: 28115

Ion Ratio Lower Upper

75 100

110 8.2 19.1 57.3#

77 0.0 25.0 37.4#

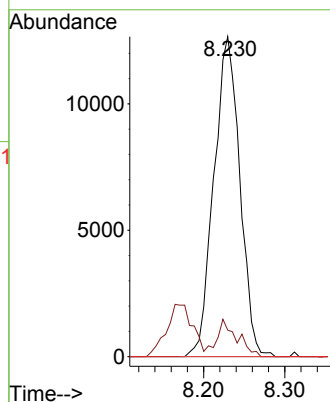

#37

Ethyl Acetate

Concen: 0.821 ug/l

RT: 7.565 min Scan# 954

Delta R.T. -0.006 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37




Tgt Ion: 43 Resp: 5353


Ion Ratio Lower Upper

43 100

61 8.8 13.2 19.8#

70 5.5 11.3 16.9#

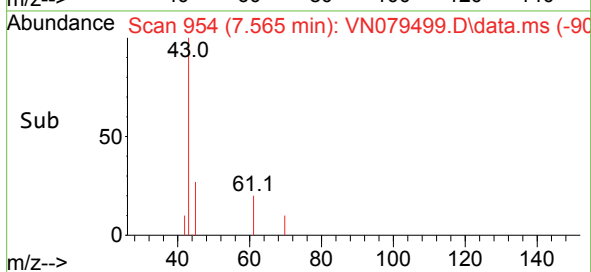



#38

Carbon Tetrachloride

Concen: 5.223 ug/l

RT: 8.230 min Scan# 1090

Delta R.T. -0.135 min


Lab File: VN079499.D

Acq: 10 Oct 2023 17:37

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:117 Resp: 34279

Ion Ratio Lower Upper

117 100

119 4.4 77.3 115.9#

121 0.0 23.3 34.9#

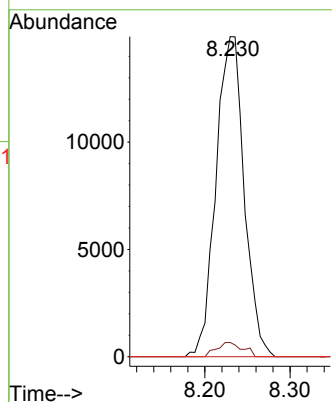

#40

Benzene

Concen: 0.364 ug/l

RT: 8.612 min Scan# 1132

Delta R.T. -0.000 min

Lab File: VN079499.D




Acq: 10 Oct 2023 17:37


Tgt Ion: 78 Resp: 7088

Ion Ratio Lower Upper

78 100

77 19.5 19.0 28.6

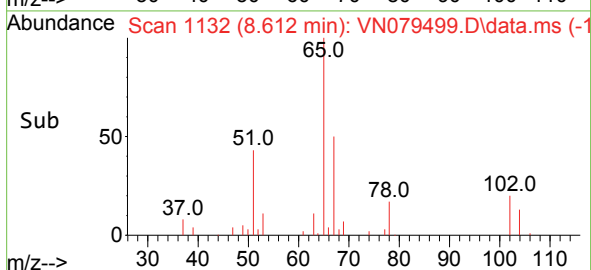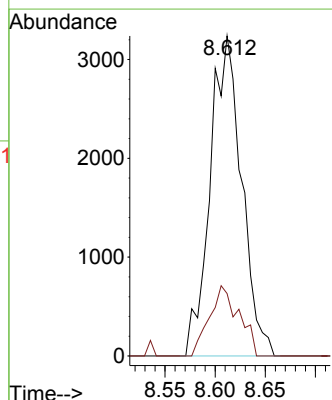



#42

1,2-Dichloroethane

Concen: 0.243 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.012 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 1722

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.8

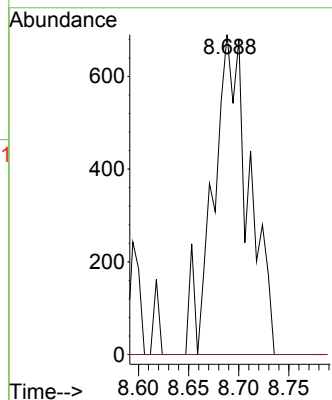

#43

Isopropyl Acetate

Concen: 29.219 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. -0.000 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37




Tgt Ion: 43 Resp: 333953


Ion Ratio Lower Upper

43 100

61 12.7 24.7 37.1#

87 8.6 14.6 21.8#

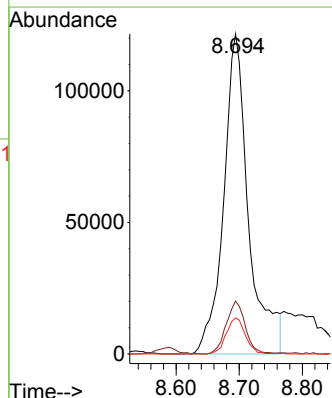



#45

1,2-Dichloropropane

Concen: 0.455 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.118 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 63 Resp: 2336

Ion Ratio Lower Upper

63 100

65 0.0 23.9 35.9#



#48

Methyl methacrylate

Concen: 1.187 ug/l

RT: 9.665 min Scan# 1311

Delta R.T. -0.024 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37




Tgt Ion: 41 Resp: 5815


Ion Ratio Lower Upper

41 100

69 0.0 90.4 135.6#

39 64.8 54.6 81.8


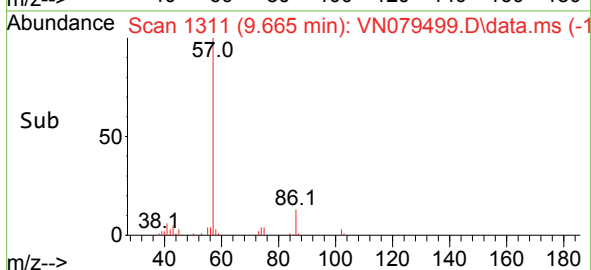






#49
1,4-Dioxane
Concen: 1.308 ug/l
RT: 9.735 min Scan# 11
Delta R.T. 0.035 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 88 Resp: 118
Ion Ratio Lower Upper
88 100
43 1577262.7 17.0 25.6#
58 7208.5 47.0 70.4#

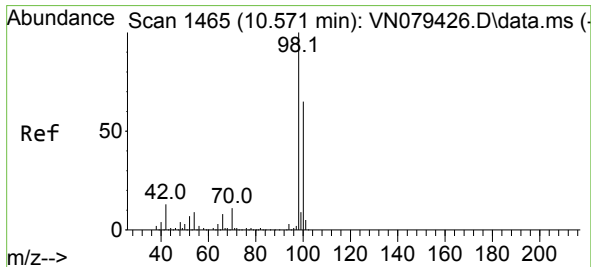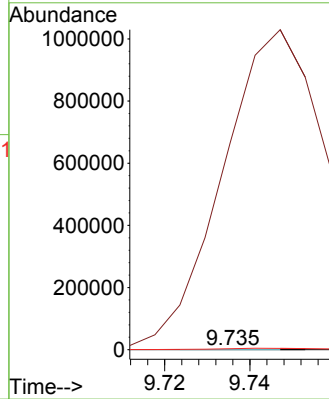

#50
Toluene-d8
Concen: 45.354 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37

Tgt Ion: 98 Resp: 716851
Ion Ratio Lower Upper
98 100
100 65.5 52.0 78.0


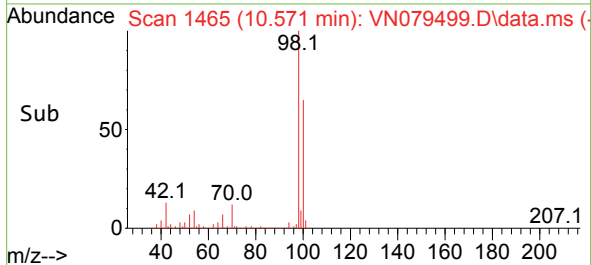
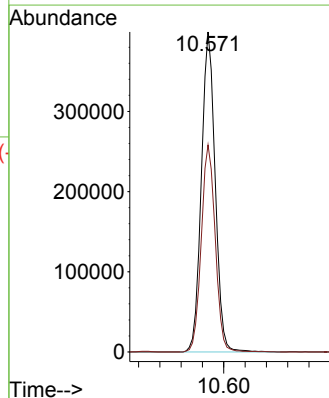
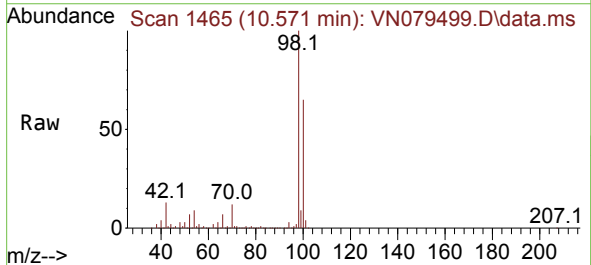


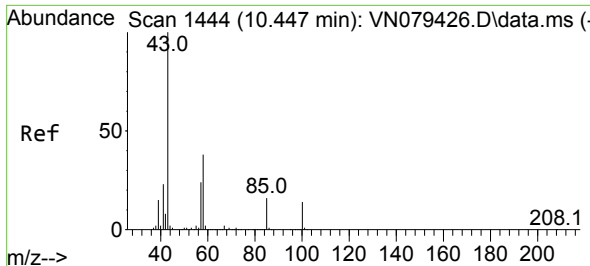

#51
4-Methyl-2-Pentanone
Concen: 3.070 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. 0.006 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 19804
Ion Ratio Lower Upper
43 100
58 22.9 36.6 54.8#

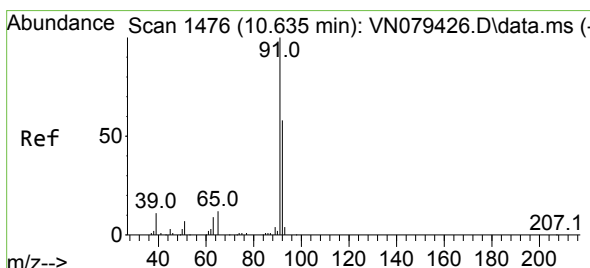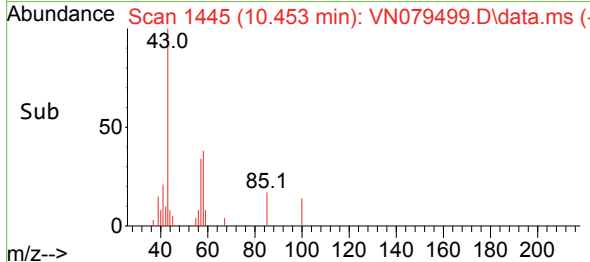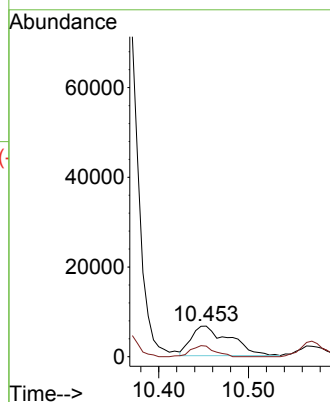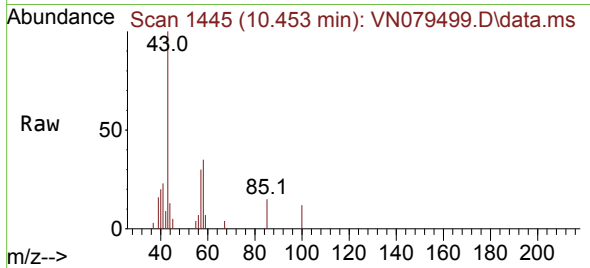

#52
Toluene
Concen: 0.648 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.006 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37


Tgt Ion: 92 Resp: 7429
Ion Ratio Lower Upper
92 100
91 157.0 137.4 206.0

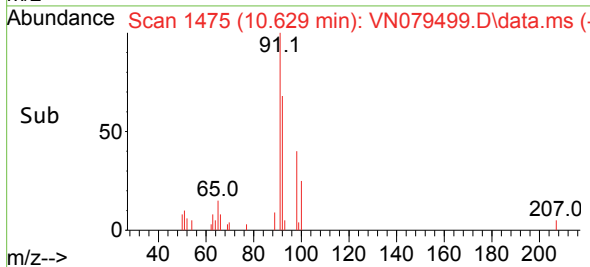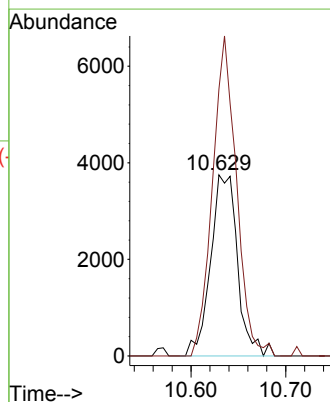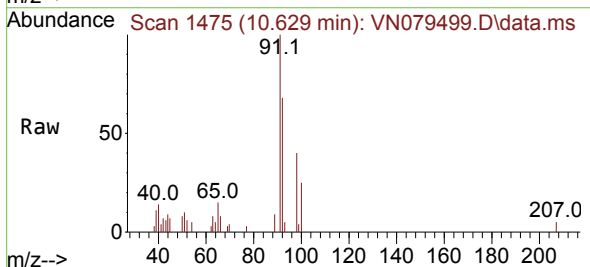






#54
 cis-1,3-Dichloropropene
 Concen: 10.650 ug/l
 RT: 10.359 min Scan# 1429
 Delta R.T. 0.041 min
 Lab File: VN079499.D
 Acq: 10 Oct 2023 17:37


Instrument :
 MSVOA_N
 ClientSampleId :





Tgt Ion	Ratio	Lower	Upper
75	100		
77	1.2	26.1	39.1#
39	35.3	31.6	47.4




#57
 1,3-Dichloropropane
 Concen: 1.179 ug/l
 RT: 11.206 min Scan# 1573
 Delta R.T. 0.035 min
 Lab File: VN079499.D
 Acq: 10 Oct 2023 17:37



Tgt Ion	Ratio	Lower	Upper
76	100		
78	0.0	26.1	39.1#



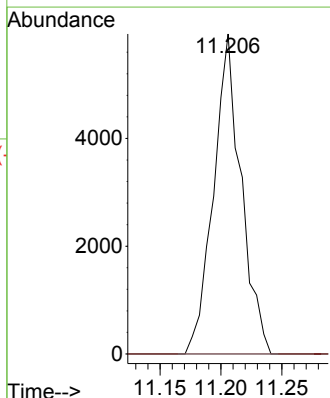



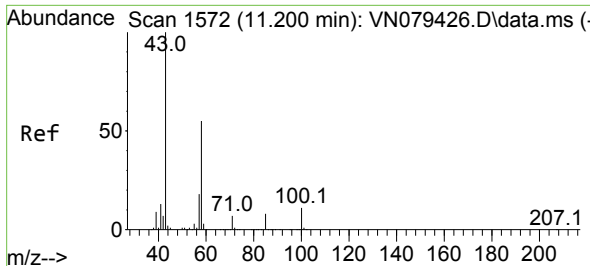

#59
2-Hexanone
Concen: 44.547 ug/l
RT: 11.176 min Scan# 1568
Delta R.T. -0.024 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 207397
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#

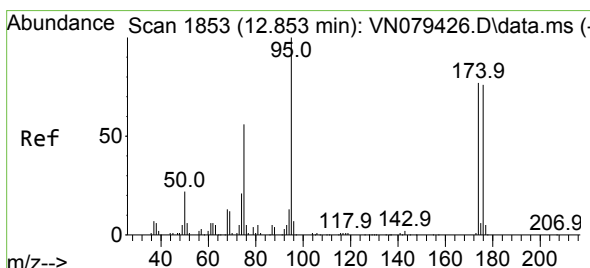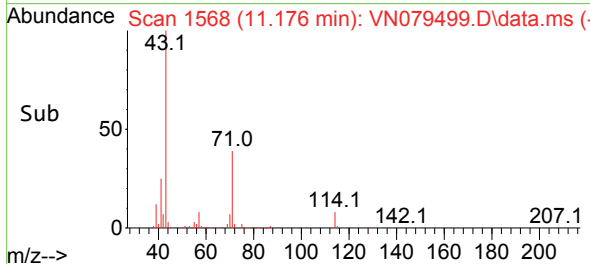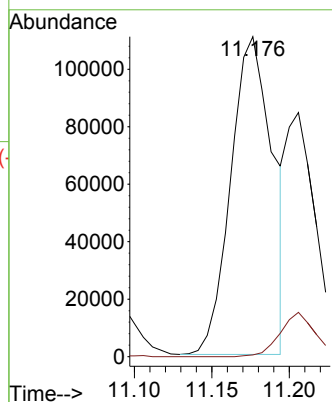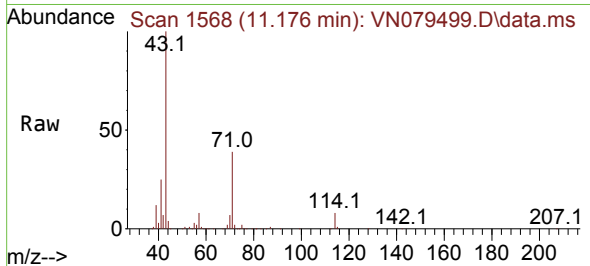

#62
4-Bromofluorobenzene
Concen: 53.048 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37

Tgt Ion: 95 Resp: 269079
Ion Ratio Lower Upper
95 100
174 75.1 0.0 143.8
176 71.7 0.0 135.8


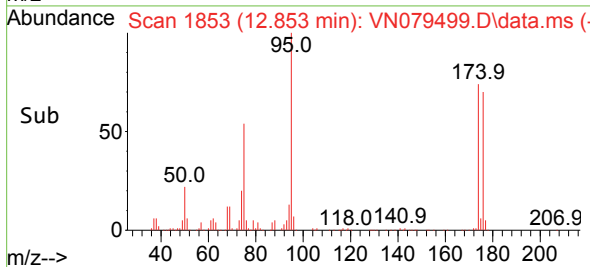
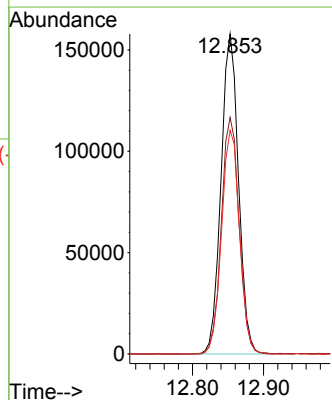
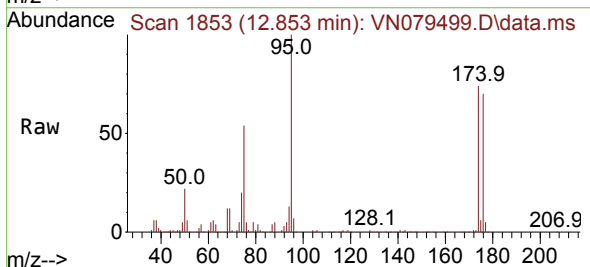




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 584388
Ion Ratio Lower Upper
117 100
82 56.9 44.0 66.0
119 32.6 25.6 38.4

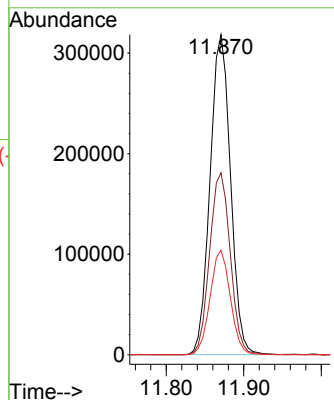

#68
m/p-Xylenes
Concen: 0.644 ug/l
RT: 12.070 min Scan# 1720
Delta R.T. -0.006 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37

Tgt Ion:106 Resp: 5295
Ion Ratio Lower Upper
106 100
91 210.5 159.6 239.4

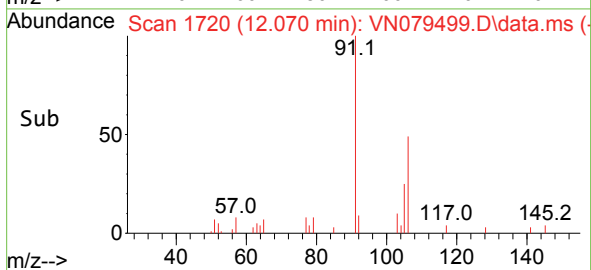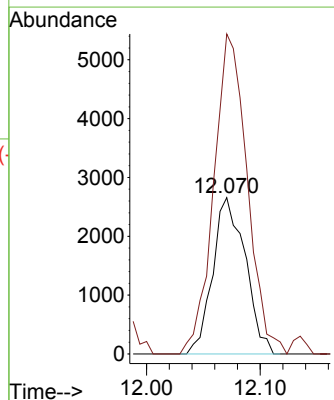

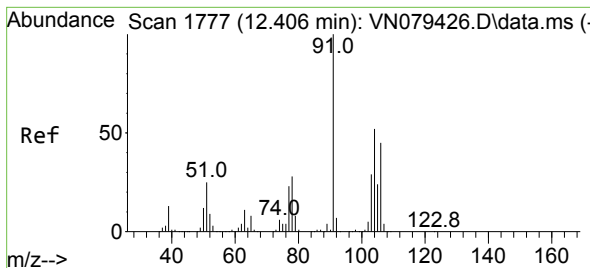

#69

o-Xylene

Concen: 0.254 ug/l

RT: 12.406 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:106 Resp: 2051

Ion Ratio Lower Upper

106 100

91 256.8 105.2 315.5

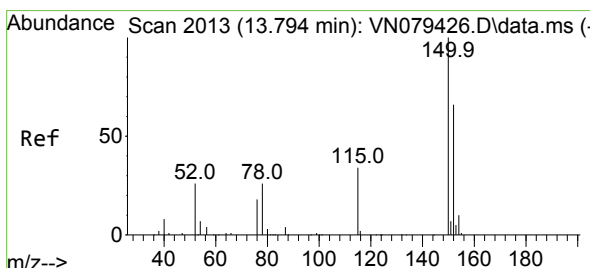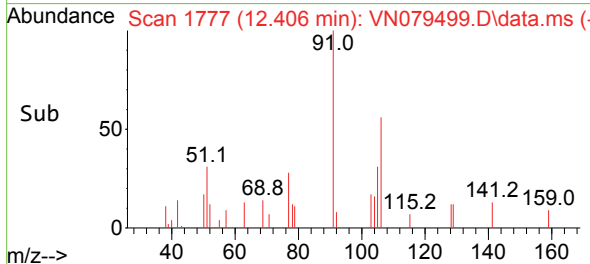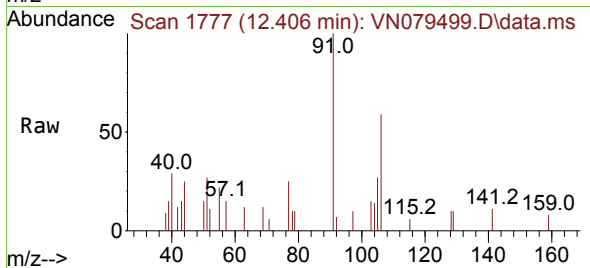

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37




Tgt Ion:152 Resp: 226176


Ion Ratio Lower Upper

152 100

115 62.2 32.3 96.8

150 157.7 0.0 355.8

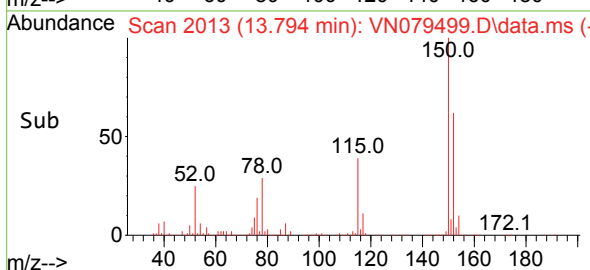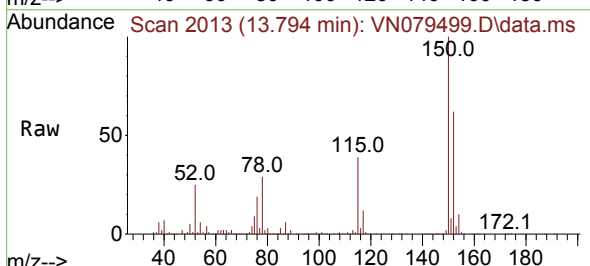



#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 13.153 min Scan# 1904

Delta R.T. 0.212 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 83 Resp: 540

Ion Ratio Lower Upper

83 100

131 12.8 5.0 15.0

85 69.8 31.9 95.7



#76

1,2,3-Trichloropropane

Concen: 22.428 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN079499.D




Acq: 10 Oct 2023 17:37


Tgt Ion: 75 Resp: 146258

Ion Ratio Lower Upper

75 100


77 1.7 84.5 253.5#

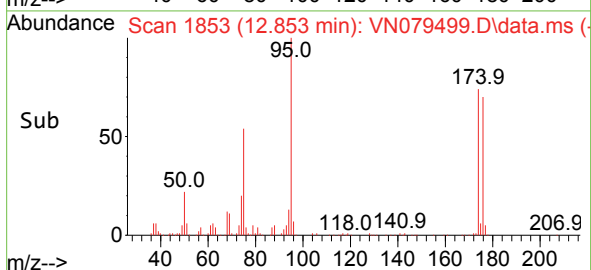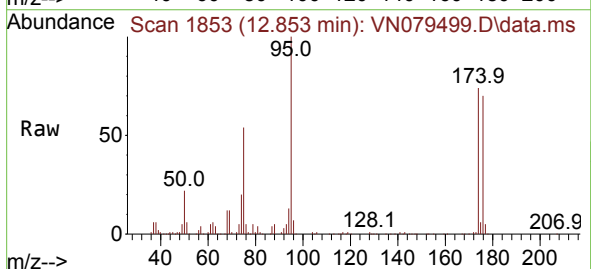



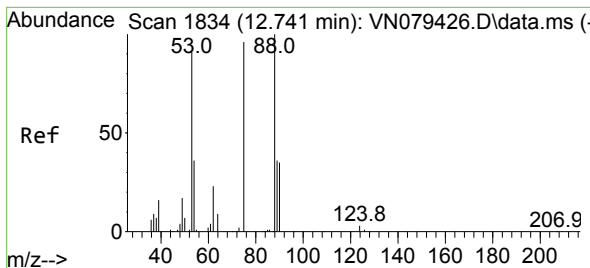


#81
trans-1,4-Dichloro-2-butene
Concen: 65.075 ug/l
RT: 12.853 min Scan# 1834
Delta R.T. 0.112 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37


Instrument :
MSVOA_N
ClientSampleId :

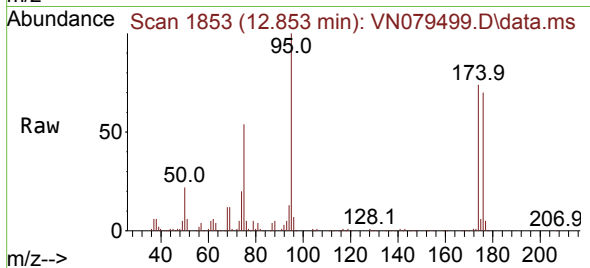



Tgt Ion: 75 Resp: 146258
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 38.8 58.2#

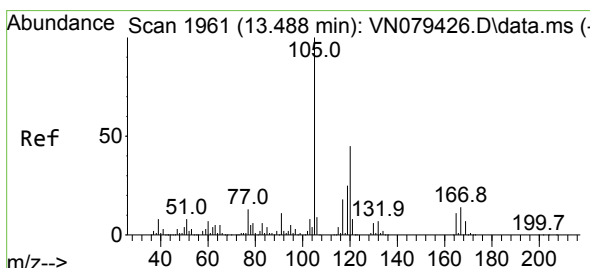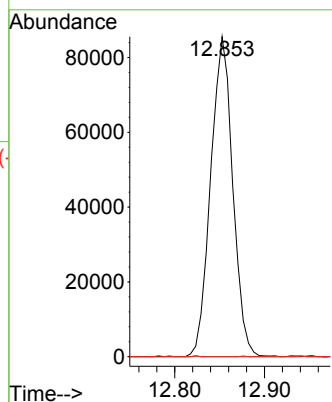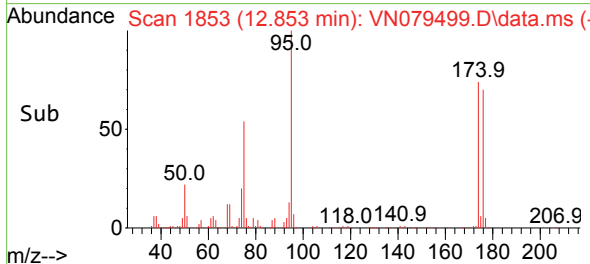


#84
1,2,4-Trimethylbenzene
Concen: 0.624 ug/l
RT: 13.482 min Scan# 1960
Delta R.T. -0.006 min
Lab File: VN079499.D
Acq: 10 Oct 2023 17:37

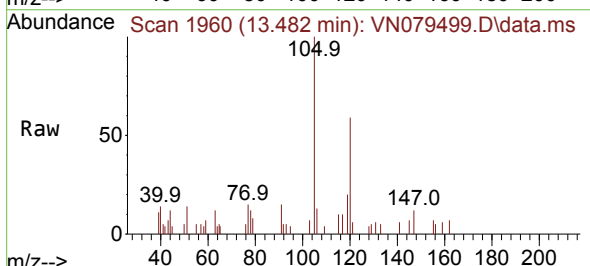

Tgt Ion: 105 Resp: 9873
Ion Ratio Lower Upper
105 100
120 39.6 22.0 66.0

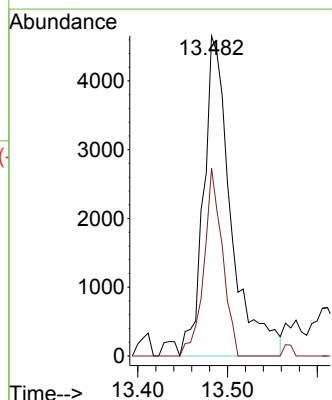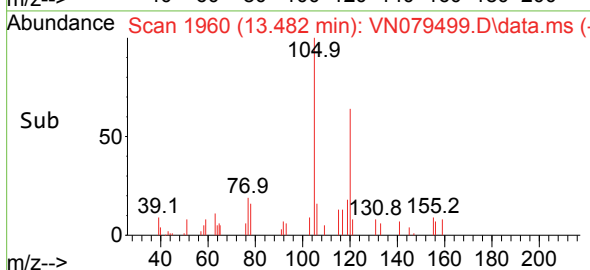



#90

Hexachloroethane

Concen: Below Cal

RT: 14.335 min Scan# 2105

Delta R.T. 0.000 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:117 Resp: 505

Ion Ratio Lower Upper

117 100

201 0.0 29.3 88.0#

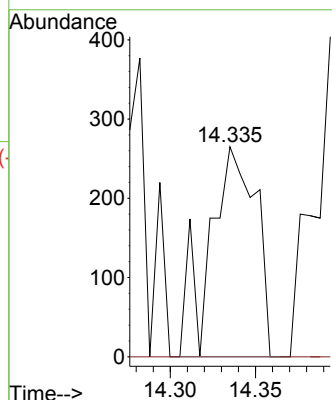

#95

Naphthalene

Concen: 16.487 ug/l

RT: 15.641 min Scan# 2327

Delta R.T. -0.006 min

Lab File: VN079499.D

Acq: 10 Oct 2023 17:37

Tgt Ion:128 Resp: 124463

Ion Ratio Lower Upper

128 100

127 14.0 10.0 15.0

129 11.6 8.7 13.1

