

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101023\
 Data File : VN079501.D
 Acq On : 10 Oct 2023 18:25
 Operator : JC\MD
 Sample : PB156250TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Oct 11 06:22:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 06 03:34:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	310841	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	614276	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	595770	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	206915	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	239543	47.528	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	95.060%
35) Dibromofluoromethane	8.171	113	214402	48.569	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.140%
50) Toluene-d8	10.571	98	733530	45.924	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	91.840%
62) 4-Bromofluorobenzene	12.853	95	264638	51.627	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	103.260%
Target Compounds						
					Qvalue	
6) Chloroethane	3.095	64	1332	0.306	ug/l #	43
11) Tert butyl alcohol	5.542	59	228	0.301	ug/l #	72
16) Acetone	4.448	43	27432	13.723	ug/l	93
18) Methyl Acetate	5.036	43	7147	0.730	ug/l #	73
20) Methylene Chloride	5.289	84	22000	4.477	ug/l #	83
25) 2-Butanone	7.506	43	3347	1.128	ug/l #	77
31) Cyclohexane	8.230	56	8507	1.190	ug/l #	17
36) 1,1-Dichloropropene	8.230	75	27465	4.145	ug/l #	48
37) Ethyl Acetate	7.571	43	5722	0.868	ug/l #	77
38) Carbon Tetrachloride	8.230	117	33788	5.094	ug/l #	16
42) 1,2-Dichloroethane	8.700	62	2220	0.311	ug/l #	73
43) Isopropyl Acetate	8.694	43	387434	33.545	ug/l #	70
45) 1,2-Dichloropropane	9.741	63	2620	0.505	ug/l #	45
48) Methyl methacrylate	9.747	41	192168	38.827	ug/l #	28
49) 1,4-Dioxane	9.741	88	91	0.998	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	17906	2.746	ug/l #	65
52) Toluene	10.629	92	2771	0.239	ug/l	88
53) t-1,3-Dichloropropene	10.729	75	1460	0.210	ug/l	95
54) cis-1,3-Dichloropropene	10.365	75	84299	11.064	ug/l #	64
57) 1,3-Dichloropropane	11.206	76	10845	1.351	ug/l #	42
58) 2-Chloroethyl Vinyl ether	10.165	63	1880	0.768	ug/l #	78
59) 2-Hexanone	11.206	43	122196	25.973	ug/l #	48
68) m/p-Xylenes	12.071	106	2504	0.299	ug/l	85
71) Bromoform	12.853	173	1779	0.500	ug/l #	1
74) N-amyl acetate	12.482	43	2208	0.280	ug/l #	41
75) 1,1,2,2-Tetrachloroethane	12.859	83	150	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.853	75	147585	24.738	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	147585	71.778	ug/l #	15
84) 1,2,4-Trimethylbenzene	13.488	105	3113	0.215	ug/l	91
90) Hexachloroethane	14.335	117	142	Below Cal	#	21
95) Naphthalene	15.641	128	9015	1.305	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101023\
Data File : VN079501.D
Acq On : 10 Oct 2023 18:25
Operator : JC\MD
Sample : PB156250TB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Oct 11 06:22:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 06 03:34:49 2023
Response via : Initial Calibration




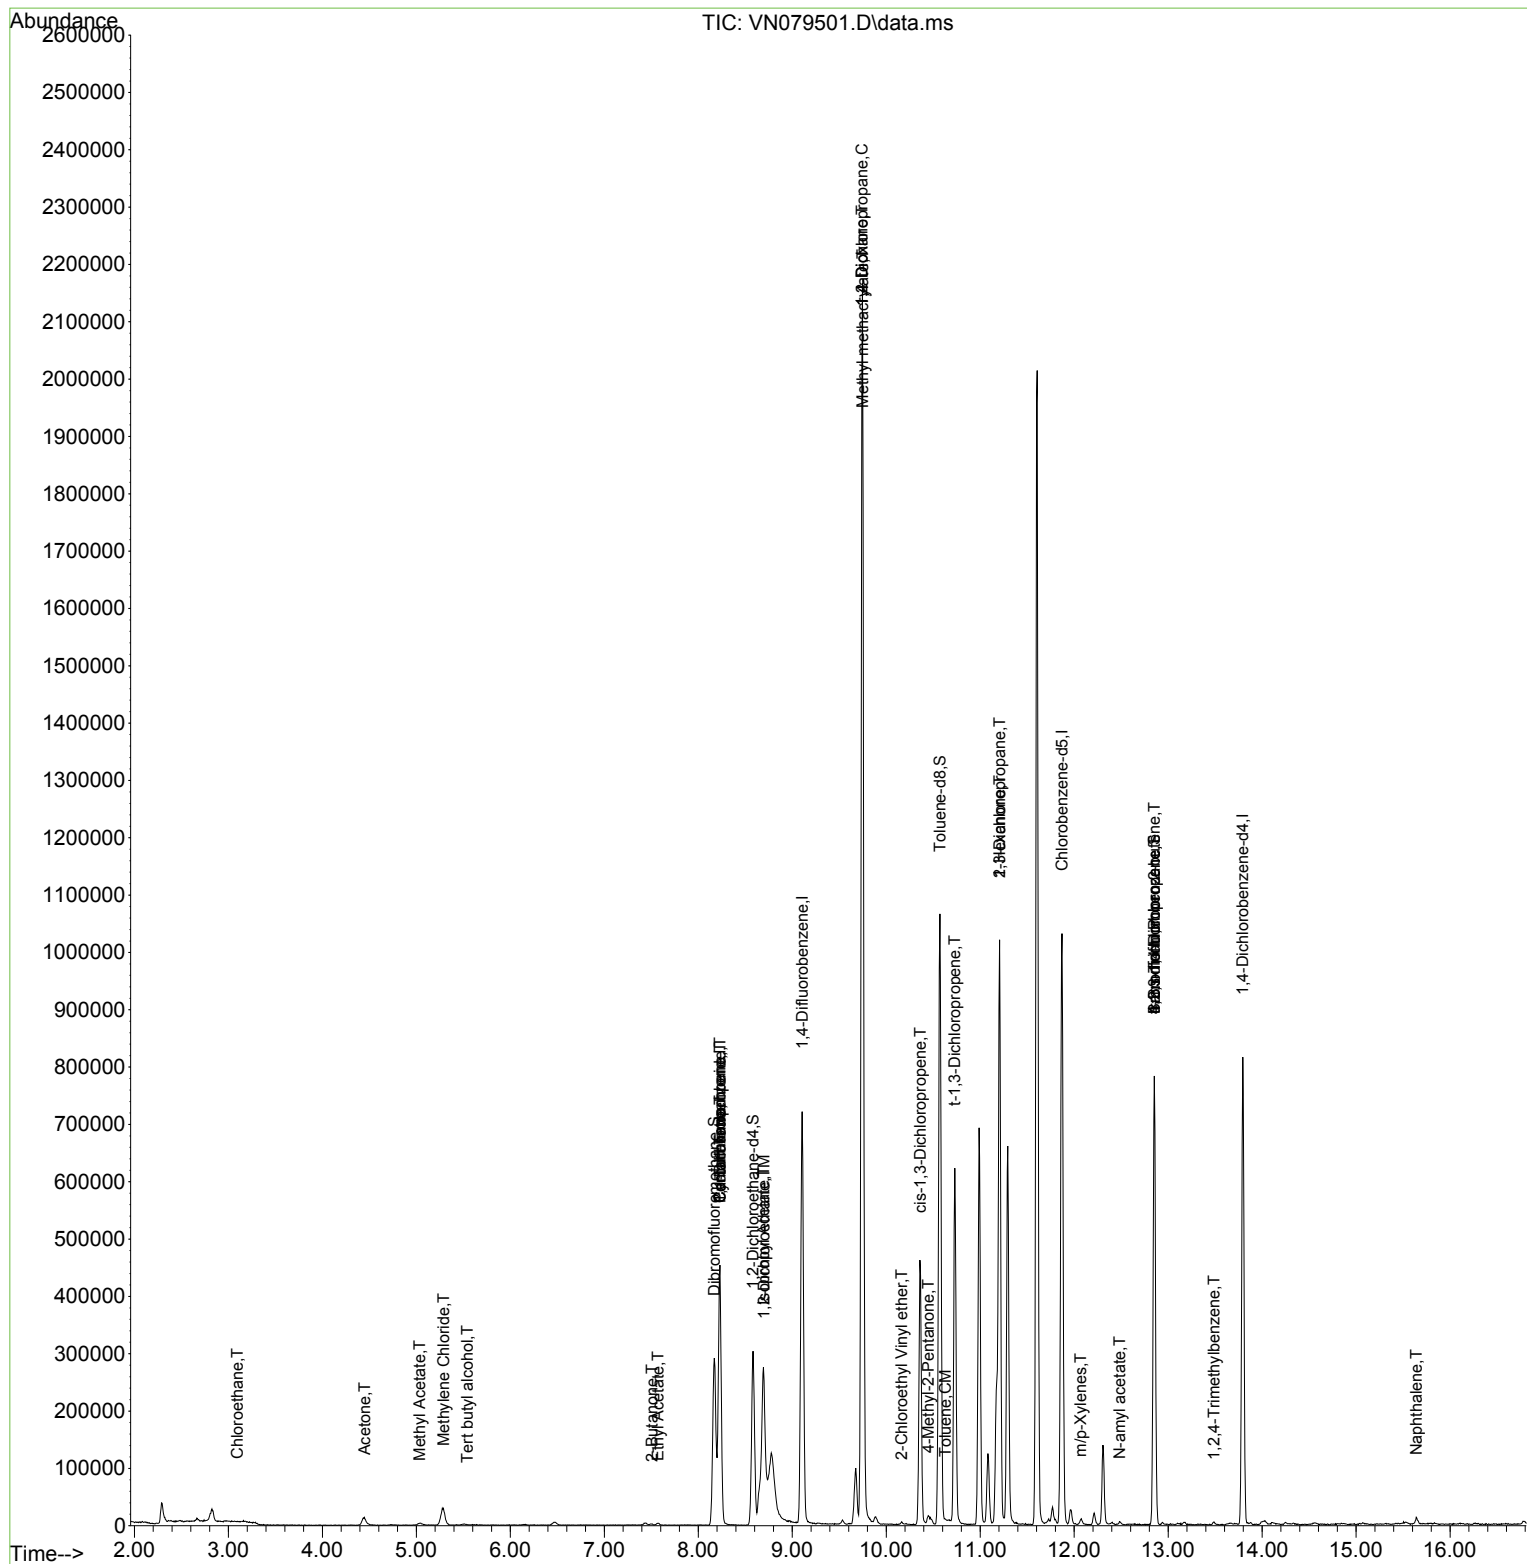




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.000 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 310841
Ion Ratio Lower Upper
168 100
99 62.9 53.0 79.6

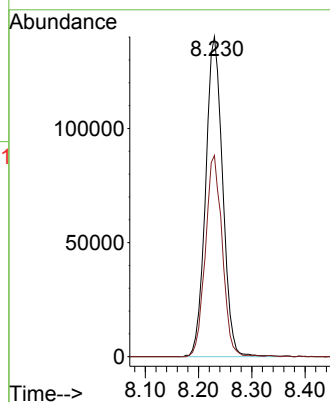

#6
Chloroethane
Concen: 0.306 ug/l
RT: 3.095 min Scan# 194
Delta R.T. -0.018 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Tgt Ion: 64 Resp: 1332
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#


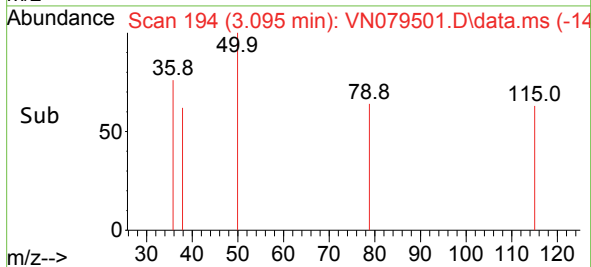
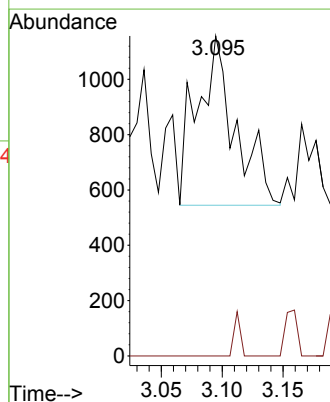
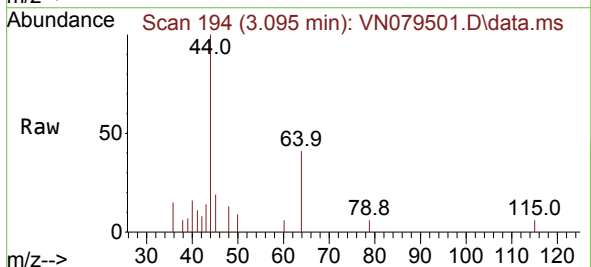




#11
Tert butyl alcohol
Concen: 0.301 ug/l
RT: 5.542 min Scan# 610
Delta R.T. 0.012 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 228
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

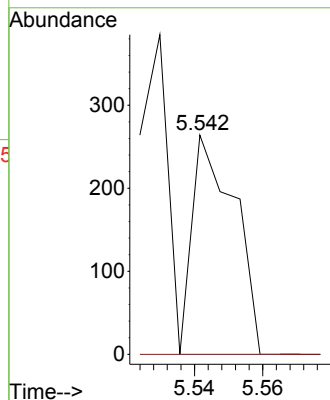

#16
Acetone
Concen: 13.723 ug/l
RT: 4.448 min Scan# 424
Delta R.T. 0.018 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Tgt Ion: 43 Resp: 27432
Ion Ratio Lower Upper
43 100
58 30.8 28.0 42.0


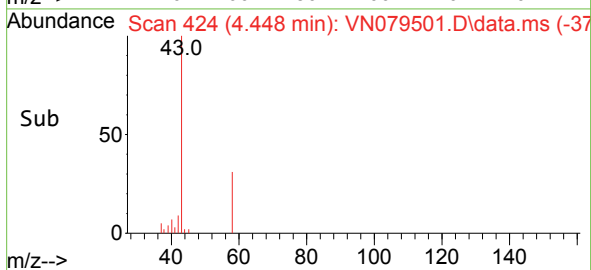
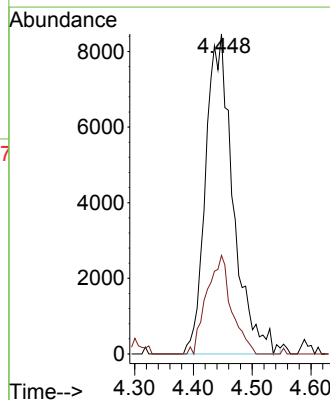





#18
Methyl Acetate
Concen: 0.730 ug/l
RT: 5.036 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 7147
Ion Ratio Lower Upper
43 100
74 17.3 26.2 39.4#



#20
Methylene Chloride
Concen: 4.477 ug/l
RT: 5.289 min Scan# 567
Delta R.T. 0.006 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Tgt Ion: 84 Resp: 22000
Ion Ratio Lower Upper
84 100
49 126.2 79.7 119.5#
51 36.7 25.2 37.8
86 72.2 53.3 79.9


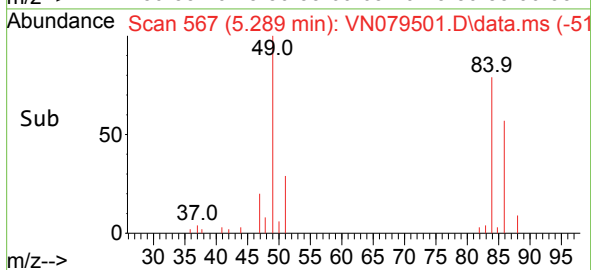






#25
2-Butanone
Concen: 1.128 ug/l
RT: 7.506 min Scan# 941
Delta R.T. 0.018 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 3347
Ion Ratio Lower Upper
43 100
72 23.7 30.2 45.2#



#31
Cyclohexane
Concen: 1.190 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.035 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Tgt Ion: 56 Resp: 8507
Ion Ratio Lower Upper
56 100
69 147.6 26.8 40.2#
84 146.9 81.8 122.6#

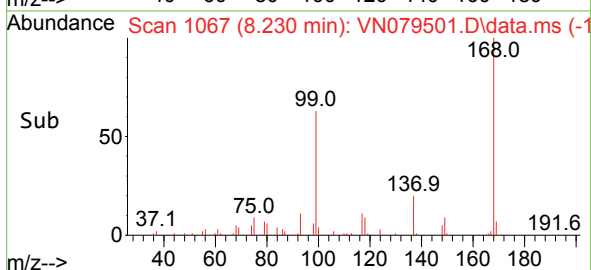



#33

1,2-Dichloroethane-d4

Concen: 47.528 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VN079501.D

Acq: 10 Oct 2023 18:25

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 239543

Ion Ratio Lower Upper

65 100

67 51.8 0.0 106.6

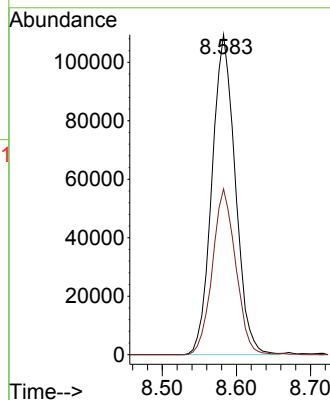

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.000 min

Lab File: VN079501.D

Acq: 10 Oct 2023 18:25




Tgt Ion: 114 Resp: 614276


Ion Ratio Lower Upper

114 100

63 20.9 0.0 36.4

88 14.4 0.0 30.6

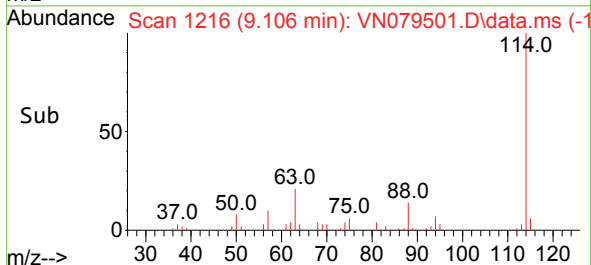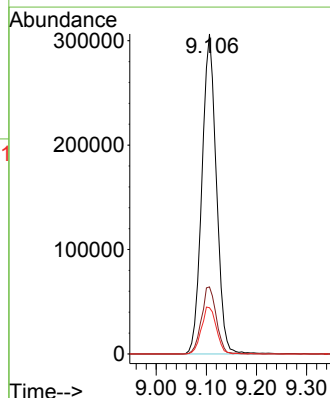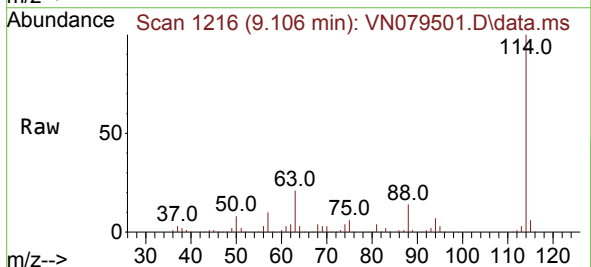



#35

Dibromofluoromethane

Concen: 48.569 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.000 min


Lab File: VN079501.D

Acq: 10 Oct 2023 18:25

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:113 Resp: 214402

Ion Ratio Lower Upper

113 100

111 101.2 82.6 123.8

192 17.1 12.7 19.1

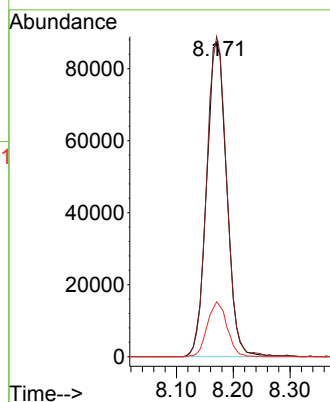

#36

1,1-Dichloropropene

Concen: 4.145 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.147 min

Lab File: VN079501.D

Acq: 10 Oct 2023 18:25




Tgt Ion: 75 Resp: 27465


Ion Ratio Lower Upper

75 100

110 8.5 19.1 57.3#


77 0.0 25.0 37.4#

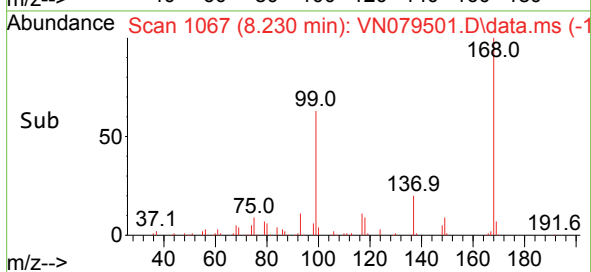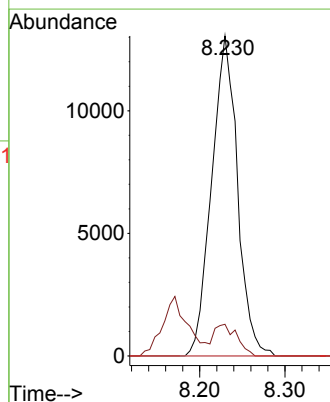






#37
Ethyl Acetate
Concen: 0.868 ug/l
RT: 7.571 min Scan# 91
Delta R.T. 0.000 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 5722
Ion Ratio Lower Upper
43 100
61 6.0 13.2 19.8#
70 5.7 11.3 16.9#

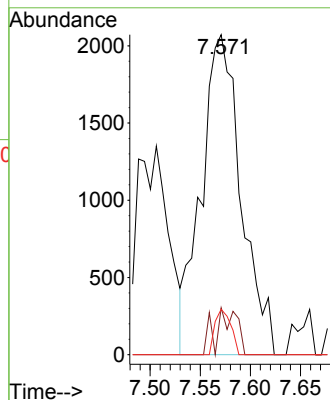

#38
Carbon Tetrachloride
Concen: 5.094 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.135 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Tgt Ion: 117 Resp: 33788
Ion Ratio Lower Upper
117 100
119 5.7 77.3 115.9#
121 0.0 23.3 34.9#

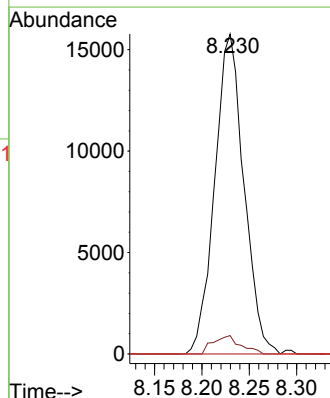



#42

1,2-Dichloroethane

Concen: 0.311 ug/l

RT: 8.700 min Scan# 1147

Delta R.T. 0.024 min

Lab File: VN079501.D

Acq: 10 Oct 2023 18:25

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 2220

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.8



#43

Isopropyl Acetate

Concen: 33.545 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.000 min

Lab File: VN079501.D

Acq: 10 Oct 2023 18:25




Tgt Ion: 43 Resp: 387434


Ion Ratio Lower Upper

43 100

61 11.9 24.7 37.1#

87 7.8 14.6 21.8#


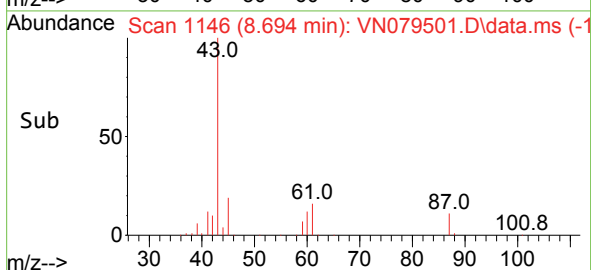






#45
1,2-Dichloropropane
Concen: 0.505 ug/l
RT: 9.741 min Scan# 11
Delta R.T. 0.118 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 2620
Ion Ratio Lower Upper
63 100
65 0.0 23.9 35.9#

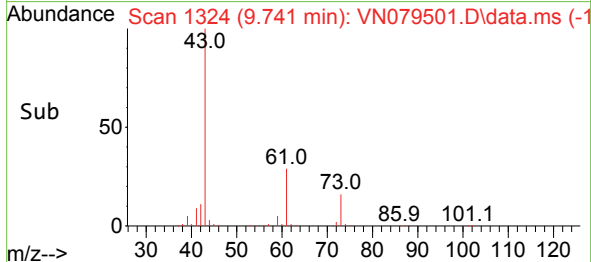

#48
Methyl methacrylate
Concen: 38.827 ug/l
RT: 9.747 min Scan# 1325
Delta R.T. 0.059 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Tgt Ion: 41 Resp: 192168
Ion Ratio Lower Upper
41 100
69 0.1 90.4 135.6#
39 54.3 54.6 81.8#

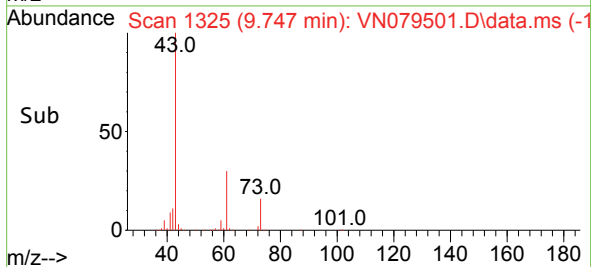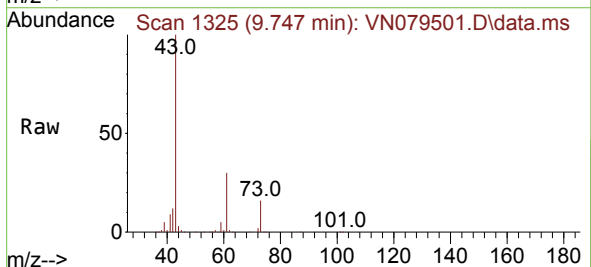



#49

1,4-Dioxane

Concen: 0.998 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.041 min


Lab File: VN079501.D

Acq: 10 Oct 2023 18:25

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 88 Resp: 91

Ion Ratio Lower Upper

88 100

43 2284428.6 17.0 25.6#

58 10119.8 47.0 70.4#

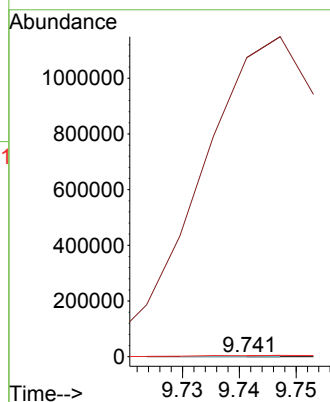

#50

Toluene-d8

Concen: 45.924 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. 0.000 min

Lab File: VN079501.D




Acq: 10 Oct 2023 18:25


Tgt Ion: 98 Resp: 733530

Ion Ratio Lower Upper

98 100

100 64.4 52.0 78.0


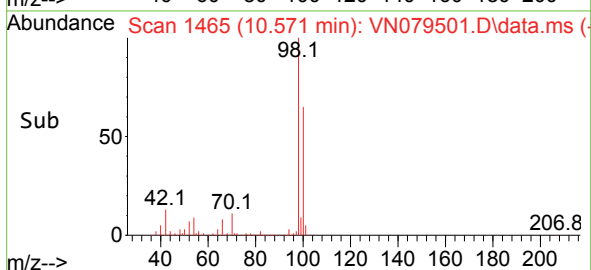
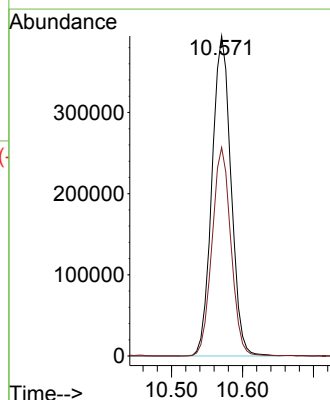



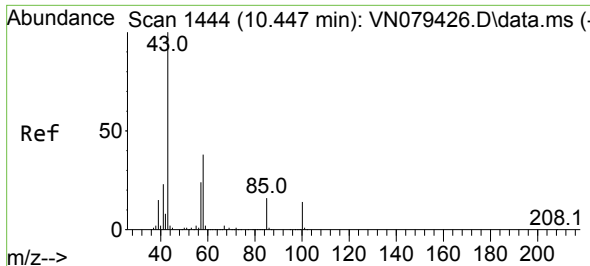

#51
4-Methyl-2-Pentanone
Concen: 2.746 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 17906
Ion Ratio Lower Upper
43 100
58 22.5 36.6 54.8#

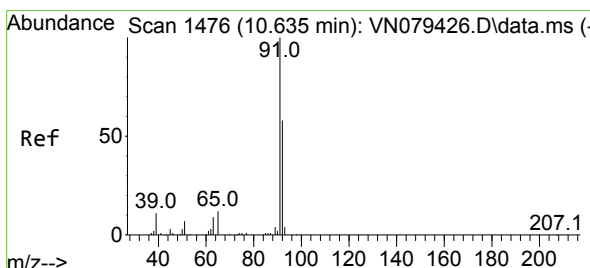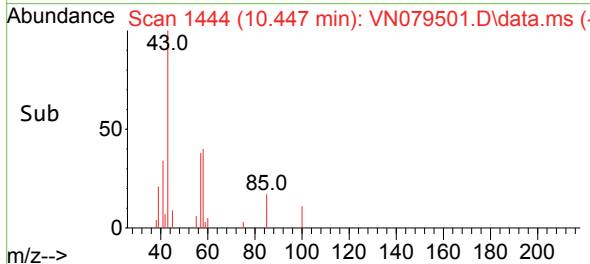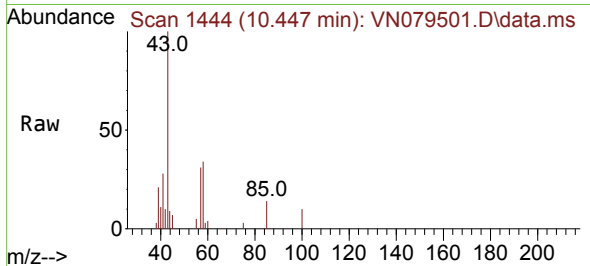

#52
Toluene
Concen: 0.239 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.006 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25


Tgt Ion: 92 Resp: 2771
Ion Ratio Lower Upper
92 100
91 155.5 137.4 206.0

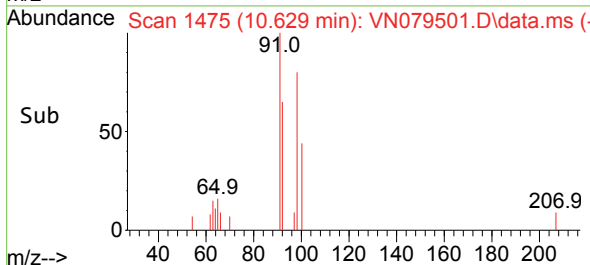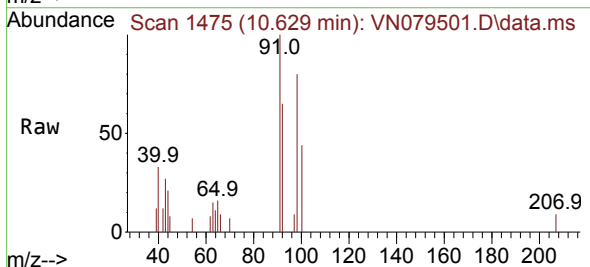



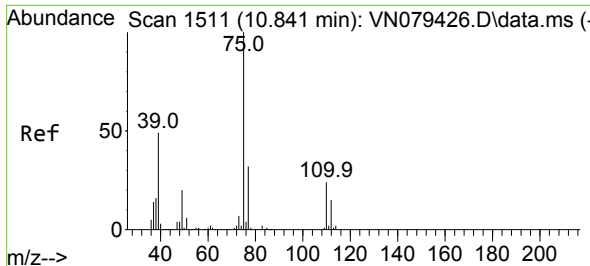


#53
t-1,3-Dichloropropene
Concen: 0.210 ug/l
RT: 10.729 min Scan# 1430
Delta R.T. -0.112 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Instrument :
MSVOA_N
ClientSampleId :



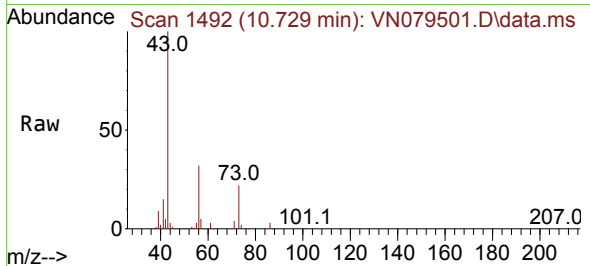



Tgt Ion: 75 Resp: 1460
Ion Ratio Lower Upper
75 100
77 34.7 25.4 38.0

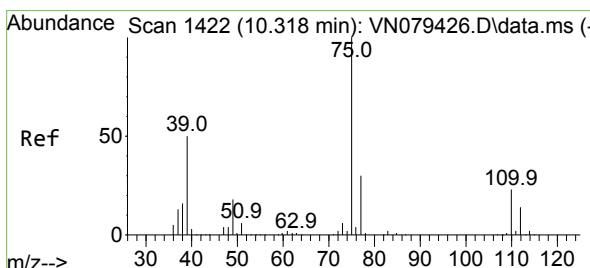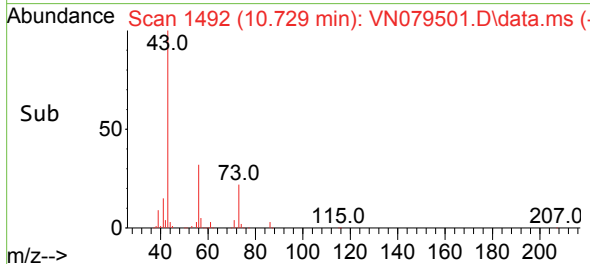

#54
cis-1,3-Dichloropropene
Concen: 11.064 ug/l
RT: 10.365 min Scan# 1430
Delta R.T. 0.047 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Tgt Ion: 75 Resp: 84299
Ion Ratio Lower Upper
75 100
77 0.4 26.1 39.1#
39 28.5 31.6 47.4#

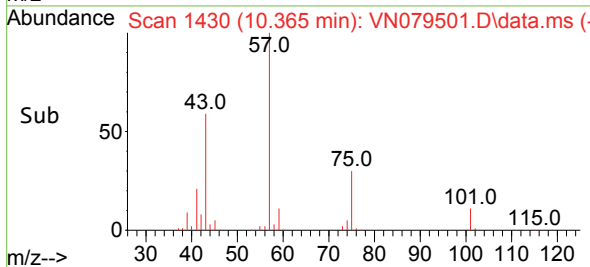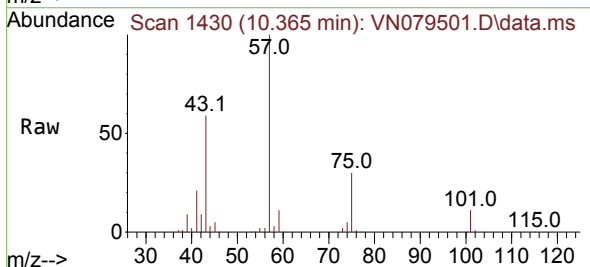



#57

1,3-Dichloropropane

Concen: 1.351 ug/l

RT: 11.206 min Scan# 1573

Delta R.T. 0.035 min


Lab File: VN079501.D

Acq: 10 Oct 2023 18:25

Instrument :

MSVOA_N

ClientSampleId :



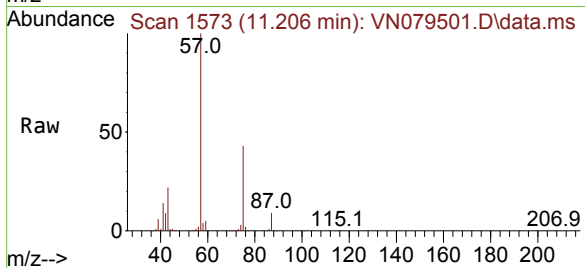


Tgt Ion: 76 Resp: 10845

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

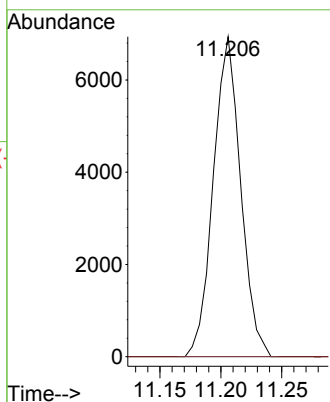

#58

2-Chloroethyl Vinyl ether

Concen: 0.768 ug/l

RT: 10.165 min Scan# 1396

Delta R.T. -0.000 min

Lab File: VN079501.D




Acq: 10 Oct 2023 18:25


Tgt Ion: 63 Resp: 1880

Ion Ratio Lower Upper

63 100

106 20.6 26.2 39.4#


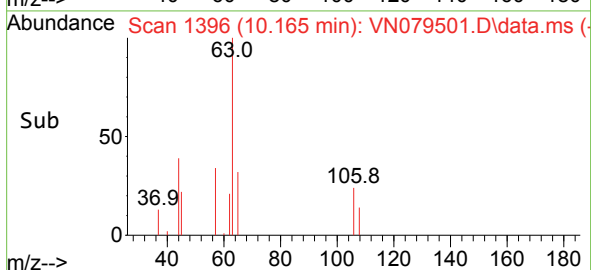
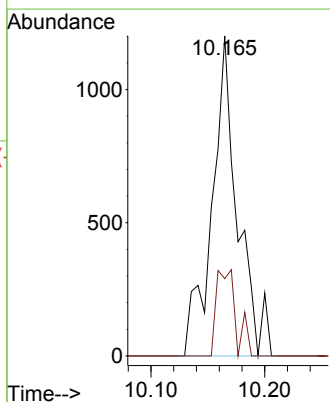
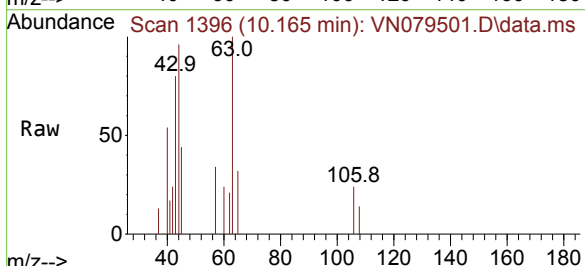


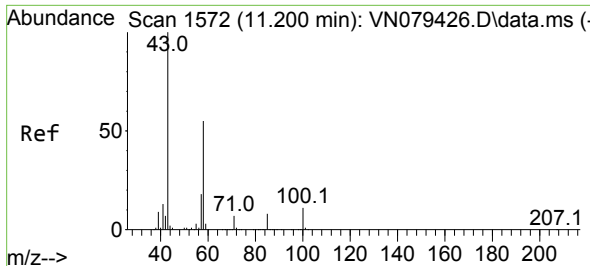

#59
2-Hexanone
Concen: 25.973 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 122196
Ion Ratio Lower Upper
43 100
58 23.0 31.7 95.1#

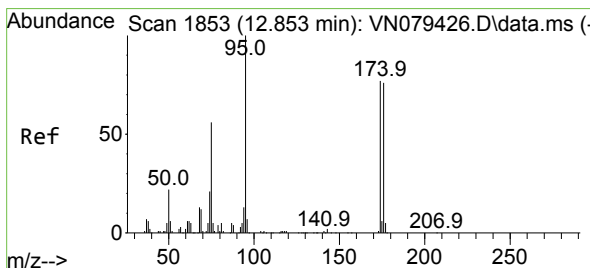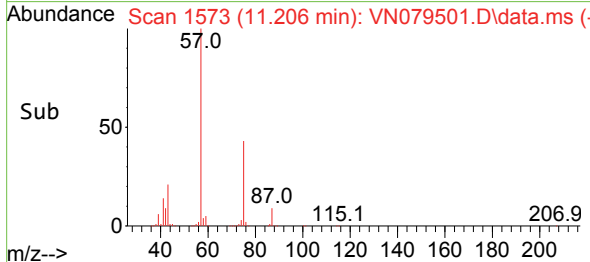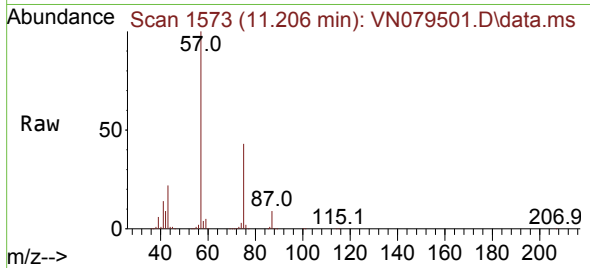

#62
4-Bromofluorobenzene
Concen: 51.627 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Tgt Ion: 95 Resp: 264638
Ion Ratio Lower Upper
95 100
174 74.6 0.0 143.8
176 72.2 0.0 135.8


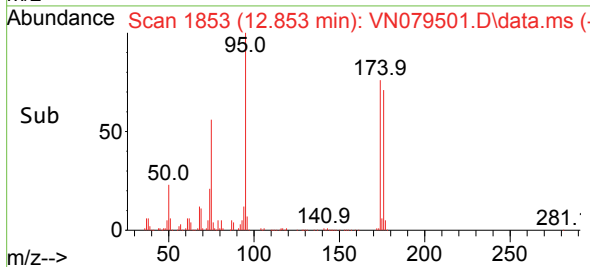

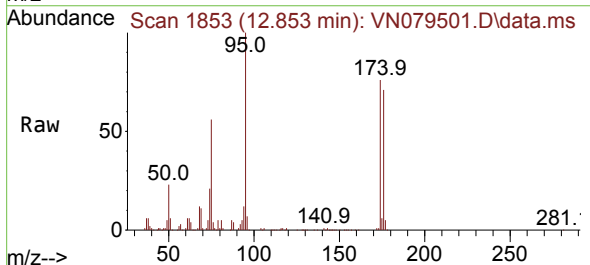




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 595770
Ion Ratio Lower Upper
117 100
82 57.1 44.0 66.0
119 32.4 25.6 38.4



#68
m/p-Xylenes
Concen: 0.299 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. -0.005 min
Lab File: VN079501.D
Acq: 10 Oct 2023 18:25

Tgt Ion:106 Resp: 2504
Ion Ratio Lower Upper
106 100
91 222.9 159.6 239.4

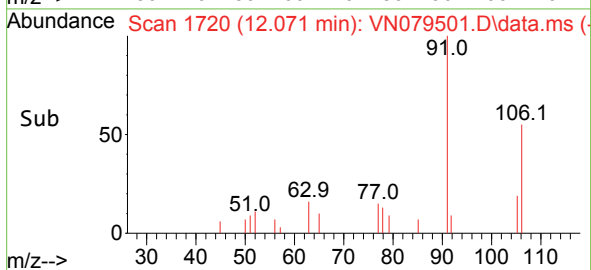

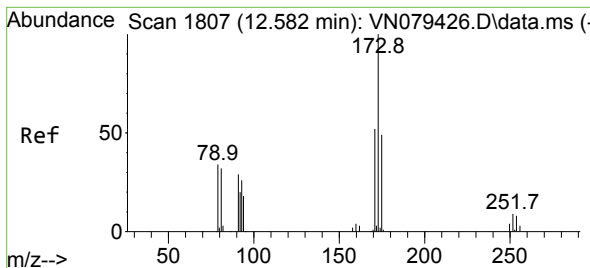

#71

Bromoform

Concen: 0.500 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.271 min


Lab File: VN079501.D

Acq: 10 Oct 2023 18:25

Instrument :

MSVOA_N

ClientSampleId :

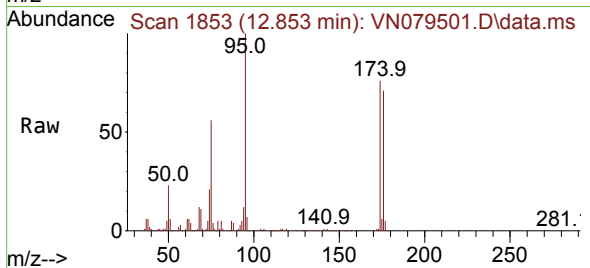




Tgt Ion:173 Resp: 1779

Ion Ratio Lower Upper

173 100

175 684.0 24.3 73.0#

254 0.0 0.0 0.0

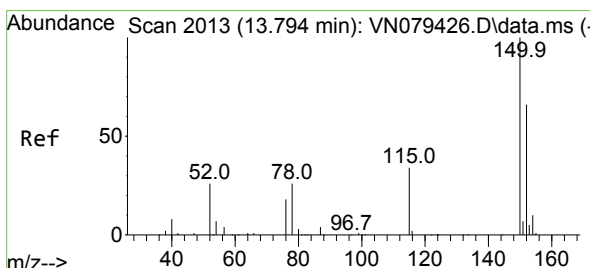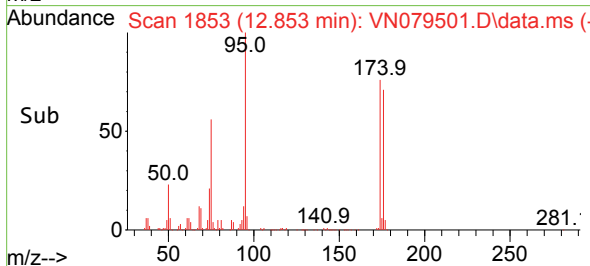

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. 0.000 min

Lab File: VN079501.D

Acq: 10 Oct 2023 18:25




Tgt Ion:152 Resp: 206915


Ion Ratio Lower Upper

152 100

115 64.6 32.3 96.8

150 161.5 0.0 355.8

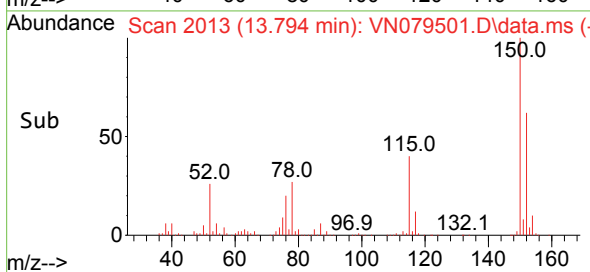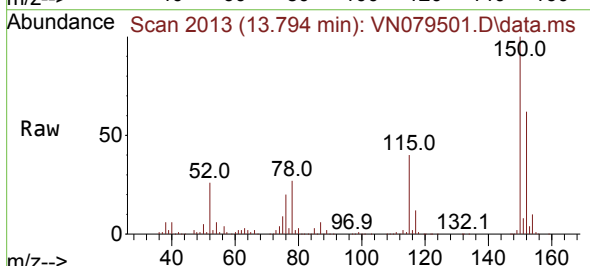



#74

N-amy1 acetate

Concen: 0.280 ug/l

RT: 12.482 min Scan# 1

Delta R.T. -0.018 min


Lab File: VN079501.D

Acq: 10 Oct 2023 18:25

Instrument :

MSVOA_N

ClientSampleId :

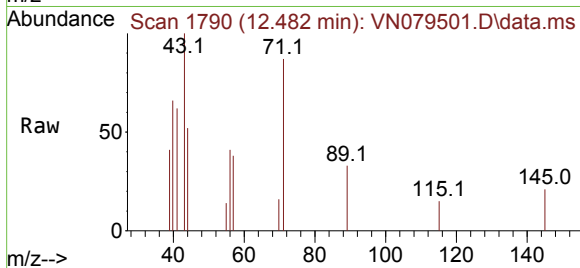

Tgt Ion: 43 Resp: 2208




Ion Ratio Lower Upper

43 100

70 3.2 43.4 65.2#

55 6.7 21.4 32.0#

61 0.0 22.8 34.2#

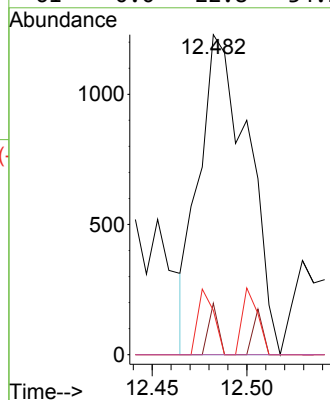

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.859 min Scan# 1854

Delta R.T. -0.082 min

Lab File: VN079501.D

Acq: 10 Oct 2023 18:25




Tgt Ion: 83 Resp: 150


Ion Ratio Lower Upper

83 100

131 266.7 5.0 15.0#

85 0.0 31.9 95.7#


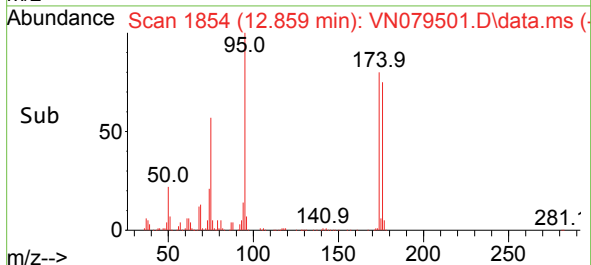
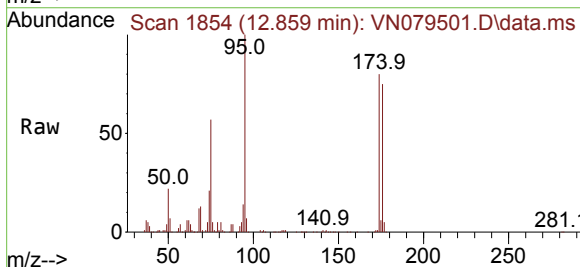
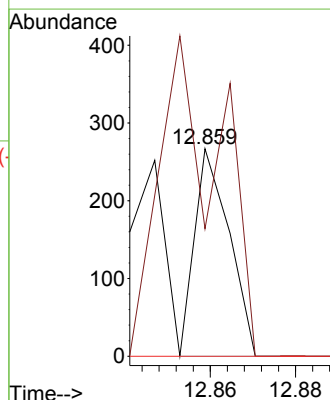




#76
 1,2,3-Trichloropropane
 Concen: 24.738 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.147 min
 Lab File: VN079501.D
 Acq: 10 Oct 2023 18:25




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 147585
 Ion Ratio Lower Upper
 75 100
 77 1.4 84.5 253.5#



#81
 trans-1,4-Dichloro-2-butene
 Concen: 71.778 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. 0.112 min
 Lab File: VN079501.D
 Acq: 10 Oct 2023 18:25

Tgt Ion: 75 Resp: 147585
 Ion Ratio Lower Upper
 75 100
 53 0.0 67.4 101.2#
 89 0.0 38.8 58.2#

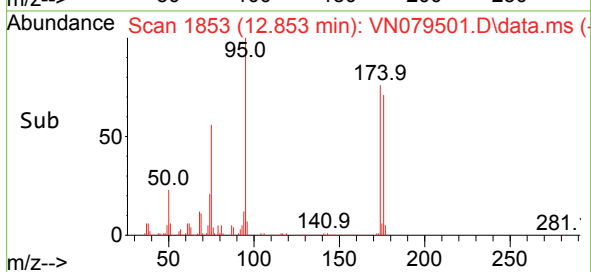



#84

1,2,4-Trimethylbenzene

Concen: 0.215 ug/l

RT: 13.488 min Scan# 1961

Delta R.T. 0.000 min

Lab File: VN079501.D

Acq: 10 Oct 2023 18:25

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 3113

Ion Ratio Lower Upper

105 100

120 50.1 22.0 66.0

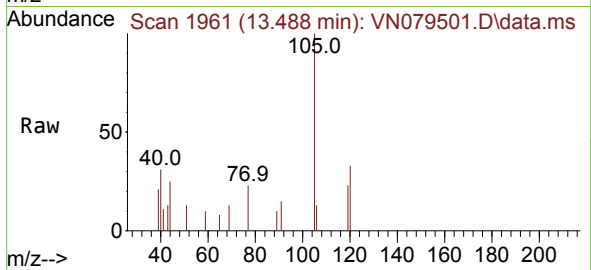

#90

Hexachloroethane

Concen: Below Cal

RT: 14.335 min Scan# 2105

Delta R.T. 0.000 min

Lab File: VN079501.D




Acq: 10 Oct 2023 18:25


Tgt Ion:117 Resp: 142

Ion Ratio Lower Upper

117 100

201 0.0 29.3 88.0#

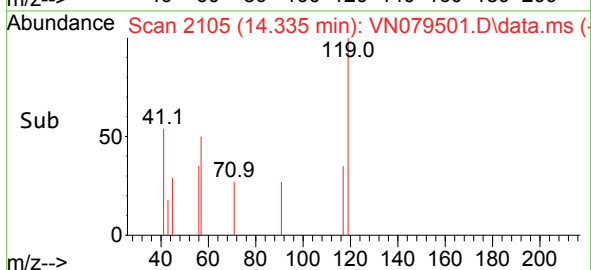



#95

Naphthalene

Concen: 1.305 ug/l

RT: 15.641 min Scan# 21

Delta R.T. -0.006 min


Lab File: VN079501.D

Acq: 10 Oct 2023 18:25

Instrument :

MSVOA_N

ClientSampleId :

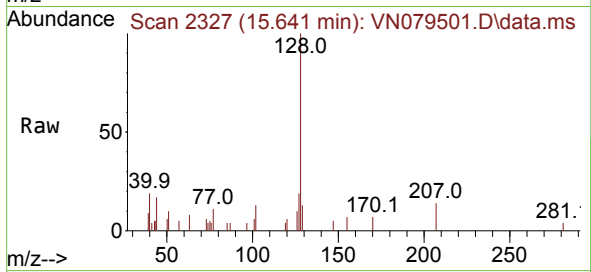

Tgt Ion:128 Resp: 9015

Ion Ratio Lower Upper

128 100

127 14.9 10.0 15.0

129 9.0 8.7 13.1

