
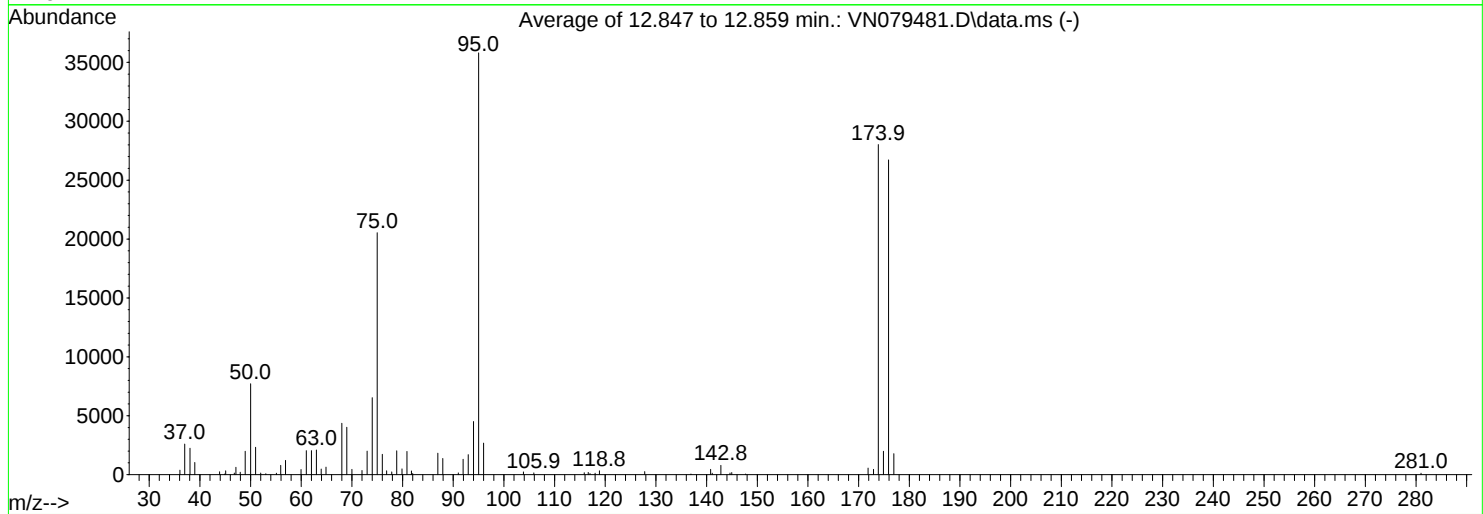


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101023\
Data File : VN079481.D
Acq On : 10 Oct 2023 08:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Title : SW846 8260
Last Update : Fri Oct 06 03:34:49 2023

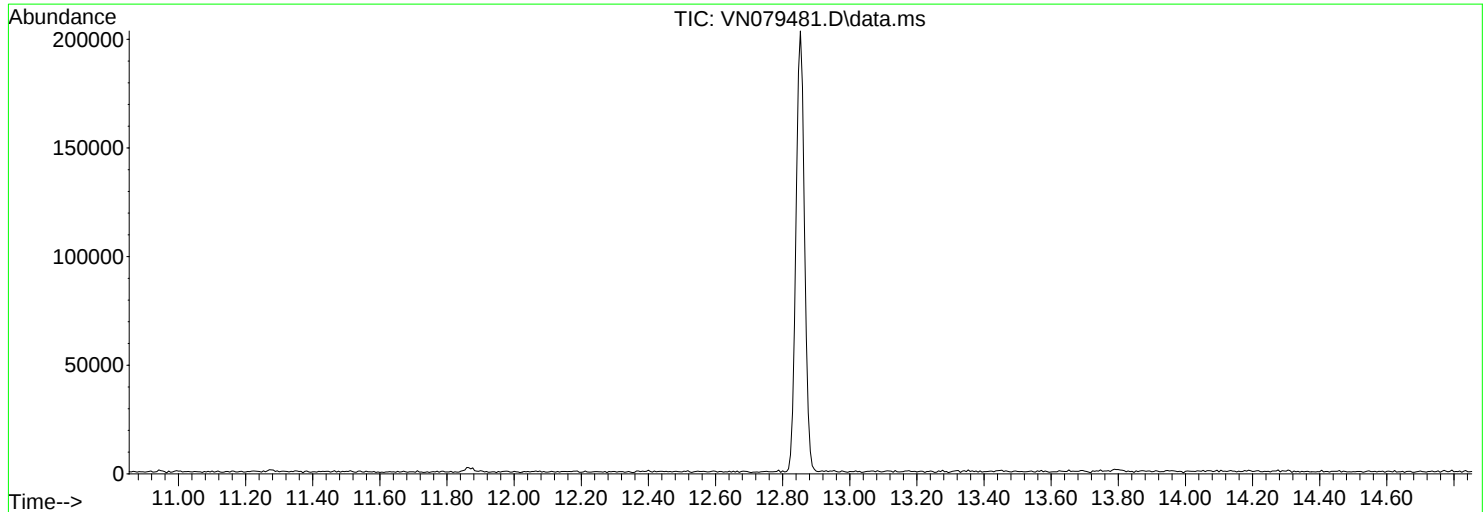

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	7713	PASS
75	95	30	60	57.4	20536	PASS
95	95	100	100	100.0	35808	PASS
96	95	5	9	7.5	2672	PASS
173	174	0.00	2	1.6	450	PASS
174	95	50	100	78.2	28019	PASS
175	174	5	9	7.1	1978	PASS
176	174	95	101	95.3	26712	PASS
177	176	5	9	6.7	1781	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	386	50.00	7713	63.95	480	77.85	23
37.00	2593	51.00	2324	64.90	645	78.85	202
38.05	2242	52.00	135	68.00	4355	79.90	49
39.00	1028	53.00	89	69.00	4027	80.85	196
43.90	242	55.10	124	70.00	449	81.75	317
44.90	56	55.95	792	72.00	348	82.00	94
45.10	328	56.90	1204	73.00	1998	86.95	1821
46.80	141	59.95	433	74.00	6533	87.95	1371
47.10	622	61.00	2043	75.00	20536	91.00	155
47.95	198	62.00	2039	76.00	1722	91.95	1299
48.95	1984	63.00	2097	76.85	330	92.95	1705

Average of 12.847 to 12.859 min.: VN079481.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	4507	136.90	52	175.90	26712		
95.00	35808	140.80	445	176.95	1781		
96.00	2672	141.10	120	281.00	122		
103.85	229	142.80	788				
105.90	150	144.60	132				
115.85	170	144.95	177				
116.65	186	147.70	52				
117.00	100	171.85	561				
118.00	120	172.95	450				
118.85	320	173.90	28019				
127.80	264	174.90	1978				

Instrument :

MSVOA_N

ClientSampleId :

BFB