
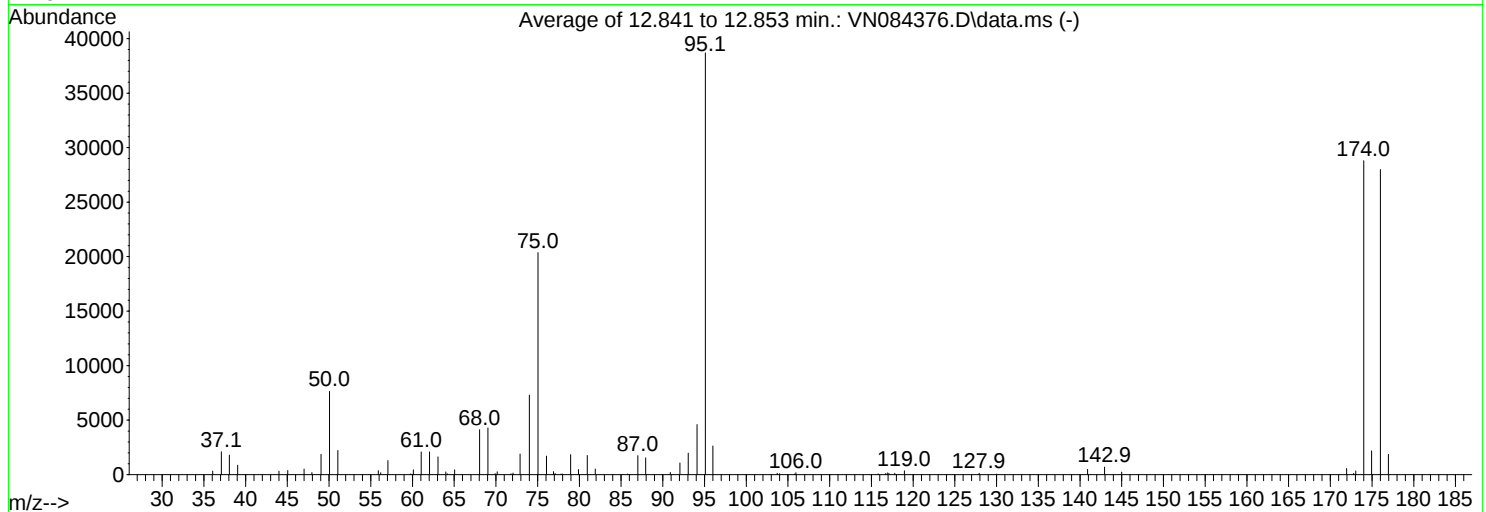


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101024\
Data File : VN084376.D
Acq On : 10 Oct 2024 09:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

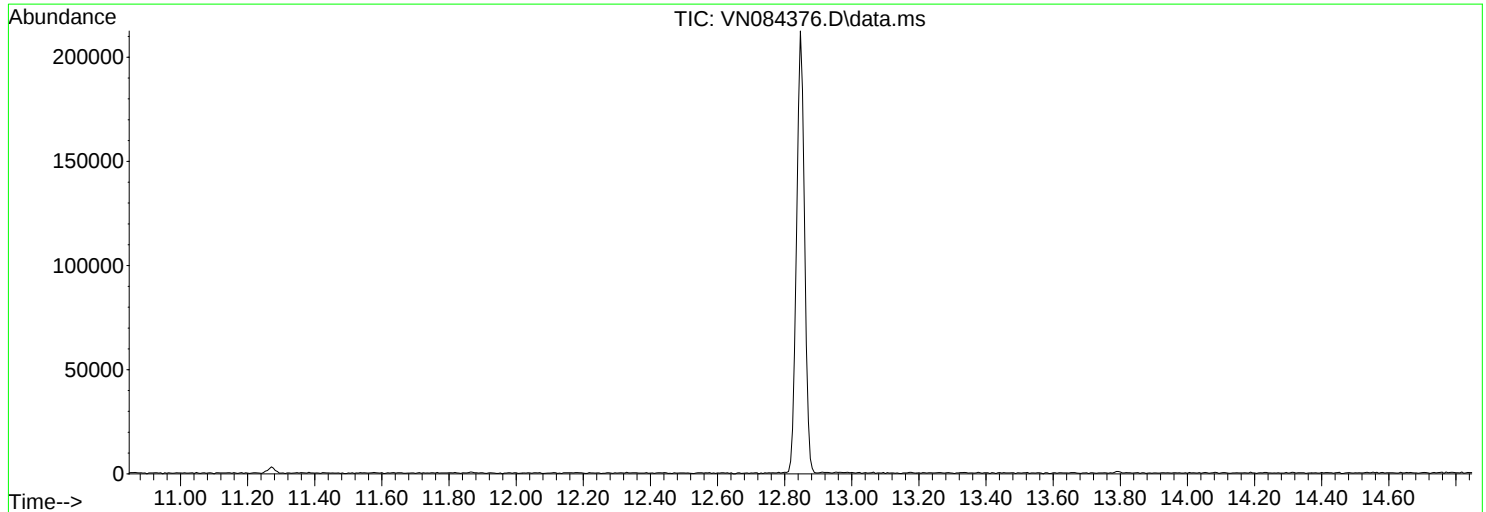

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	7640	PASS
75	95	30	60	52.6	20373	PASS
95	95	100	100	100.0	38696	PASS
96	95	5	9	6.8	2626	PASS
173	174	0.00	2	1.2	344	PASS
174	95	50	100	74.4	28795	PASS
175	174	5	9	7.6	2189	PASS
176	174	95	101	97.2	27992	PASS
177	176	5	9	6.7	1866	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	327	51.05	2219	65.05	447	76.90	281
37.10	2102	55.90	371	68.05	4125	77.10	111
38.05	1792	56.20	180	69.05	4287	77.80	5
39.05	871	57.05	1288	69.90	82	78.00	5
39.95	31	59.80	75	70.15	266	78.95	1843
44.00	328	60.10	448	71.80	77	79.90	471
45.05	386	61.05	2086	72.05	153	80.95	1760
47.00	510	62.05	2091	72.90	1899	81.90	520
47.95	193	63.05	1634	74.00	7298	85.80	61
49.05	1865	64.00	245	75.05	20373	87.00	1753
50.05	7640	64.20	71	76.05	1699	87.95	1543

Average of 12.841 to 12.853 min.: VN084376.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	205	116.70	94	172.80	114		
92.05	1072	116.90	156	173.05	344		
93.05	1971	117.10	133	174.00	28795		
94.10	4592	117.80	128	174.95	2189		
95.10	38696	118.95	348	176.00	27992		
96.00	2626	127.90	137	176.95	1866		
103.70	134	130.00	54				
104.00	83	140.90	485				
105.80	60	142.95	684				
105.95	182	145.00	240				
115.80	78	171.95	552				